

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090524\
 Data File : P0106243.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2024 10:48
 Operator : YP/AJ
 Sample : P3838-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-01-0902424

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/06/2024
 Supervised By :Ankita Jodhani 09/06/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 13:26:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 27 06:50:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.451	3.716	167.8E6	60268971	18.397m	22.307m
2) SA Decachlor...	10.192	8.746	109.0E6	38796188	20.084	17.772

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090524\
Data File : PO106243.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2024 10:48
Operator : YP/AJ
Sample : P3838-01
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OK-01-0902424


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/06/2024
Supervised By :Ankita Jodhani 09/06/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 13:26:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 27 06:50:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

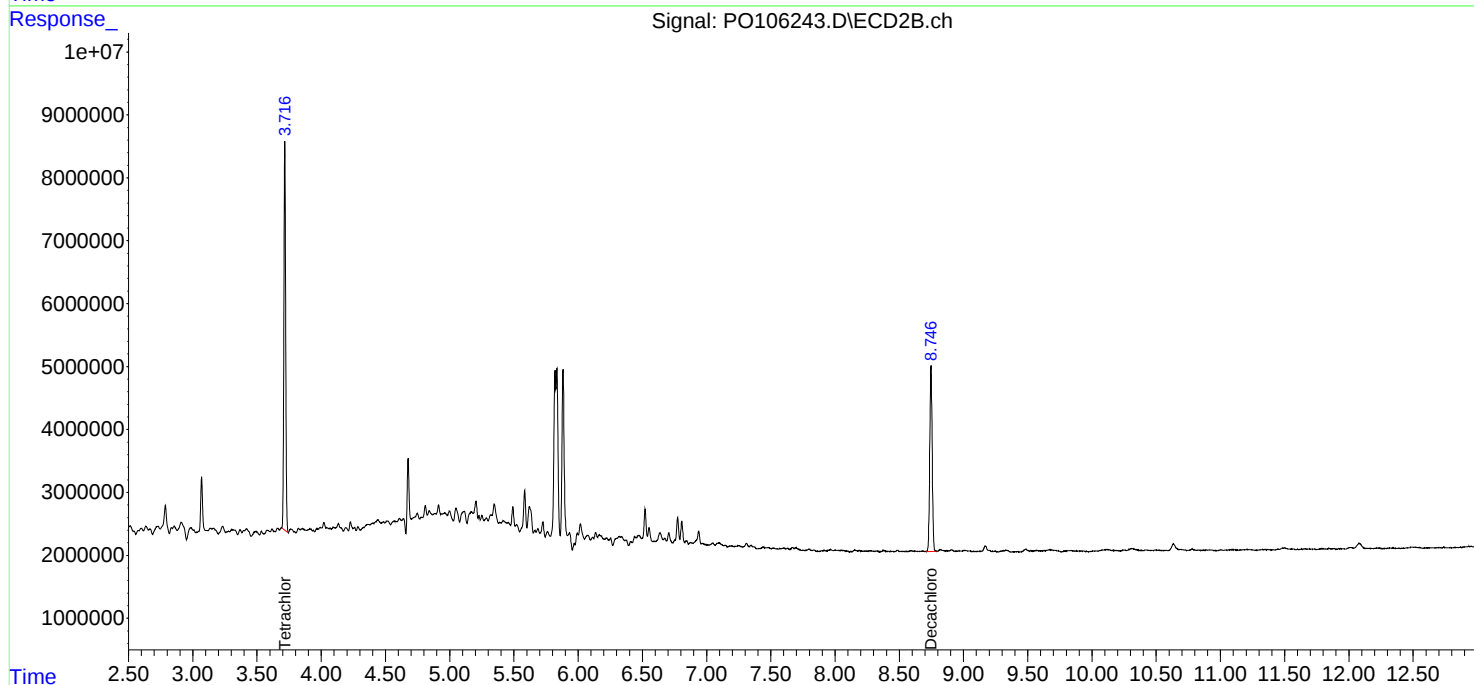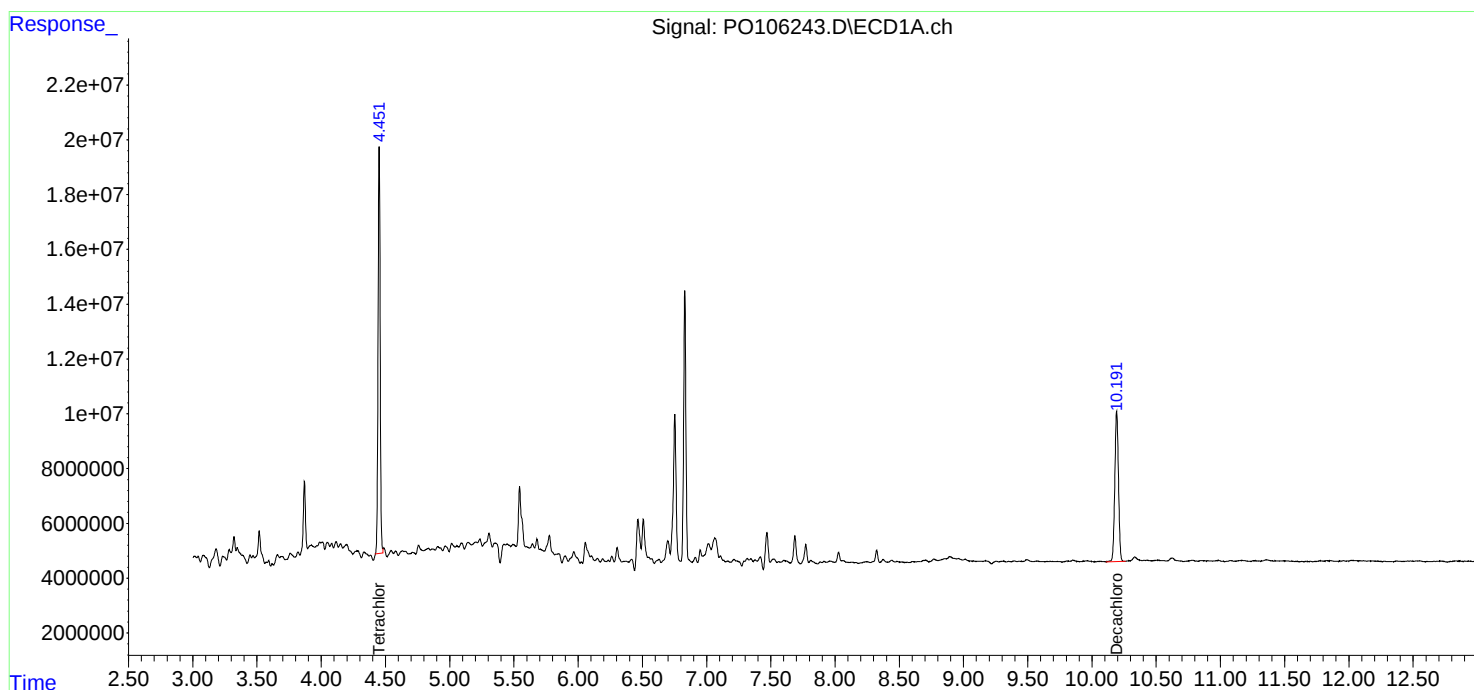

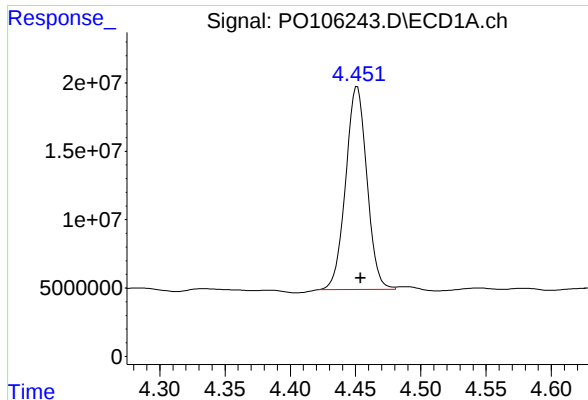


#1 Tetrachloro-m-xylene

R.T.: 4.451 min
Delta R.T.: -0.003 min
Response: 167838074
Conc: 18.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-01-0902424


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/06/2024
Supervised By :Ankita Jodhani 09/06/2024

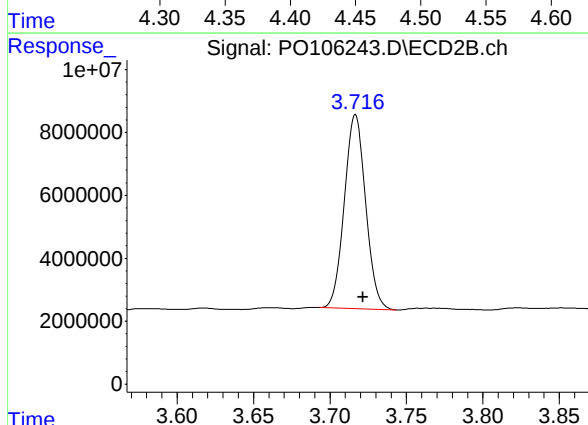


#1 Tetrachloro-m-xylene

R.T.: 3.716 min
Delta R.T.: -0.005 min
Response: 60268971
Conc: 22.31 ng/ml

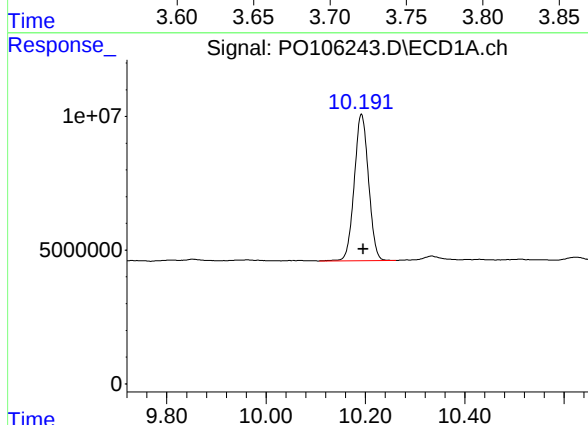

#2 Decachlorobiphenyl

R.T.: 10.192 min
Delta R.T.: -0.003 min
Response: 108994768
Conc: 20.08 ng/ml

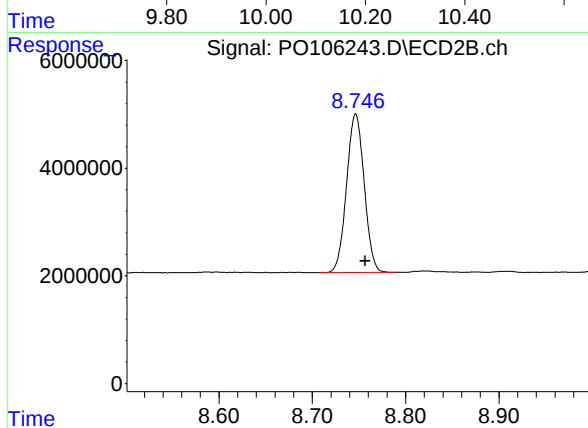

#2 Decachlorobiphenyl

R.T.: 8.746 min
Delta R.T.: -0.010 min
Response: 38796188
Conc: 17.77 ng/ml