

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090525\
 Data File : P0113516.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 18:17
 Operator : YP/AJ
 Sample : Q2893-09
 Misc : AR1660 WATER LOD 25PPB
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:34:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.659	3.653	155.0E6	92834892	18.934	18.344
2)	SA Decachlor...	8.675	8.620	91699101	30899920	13.229	16.307
Target Compounds							
3)	L1 AR-1016-1	4.742	4.725	5763227	4297785	21.586	25.196
4)	L1 AR-1016-2	4.760	4.743	9141528	6036296	22.772	23.428
5)	L1 AR-1016-3	4.817	4.916	5789065	3058782	22.700	21.909
6)	L1 AR-1016-4	4.936	4.960	3464345	3794926	15.887	32.519 #
7)	L1 AR-1016-5	5.192	5.171	6683333	5224125	30.156	36.653
8)	L2 AR-1221-1	3.880	3.868	1646696	1438834	17.598	22.795 #
9)	L2 AR-1221-2	3.959	3.948	2312416	3652005	34.232	78.246 #
10)	L2 AR-1221-3	4.032	4.020	2607110	2563462	11.778	17.265 #
11)	L3 AR-1232-1	4.032	4.020	2607110	2563462	14.983	21.835 #
12)	L3 AR-1232-2	4.521	4.743	7993691	6036296	80.055	49.258 #
13)	L3 AR-1232-3	4.760	4.916	9141528	3058782	48.246	48.287
14)	L3 AR-1232-4	4.936	5.002	3464345	3610958	36.788	64.228 #
15)	L3 AR-1232-5	4.980	5.171	4710305	5224125	76.043	87.267
16)	L4 AR-1242-1	4.742	4.725	5763227	4297785	25.065	29.742
17)	L4 AR-1242-2	4.760	4.743	9141528	6036296	26.603	27.828
18)	L4 AR-1242-3	4.817	4.916	5789065	3058782	26.090	26.151
19)	L4 AR-1242-4	4.936	5.002	3464345	3610958	19.972	30.696 #
20)	L4 AR-1242-5	5.589	5.521	13679199	5737882	68.341	38.475 #
21)	L5 AR-1248-1	4.742	4.725	5763227	4297785	33.033	38.541
22)	L5 AR-1248-2	4.980	4.960	4710305	3794926	19.475	23.615
23)	L5 AR-1248-3	5.192	5.002	6683333	3610958	20.960	21.283
24)	L5 AR-1248-4	5.546	5.171	24396868	5224125	48.832	26.223 #
25)	L5 AR-1248-5	5.589	5.563	13679199	3231342	40.057	15.221 #
26)	L6 AR-1254-1	5.546	5.521	24396868	5737882	45.181	18.195 #
27)	L6 AR-1254-2	5.694	5.669	15495390	4823293	31.402	17.205 #
28)	L6 AR-1254-3	6.114	6.084	21279268	7595413	28.799	18.218 #
29)	L6 AR-1254-4	6.323	6.296	4143861	1603007	7.440	5.833
30)	L6 AR-1254-5	6.745	6.710	17229178	5954666	24.579	16.657 #
31)	L7 AR-1260-1	6.228	6.198	17979431	7975846	40.314	31.269
32)	L7 AR-1260-2	6.418	6.386	12841117	7239107	18.699	20.940
33)	L7 AR-1260-3	6.784	6.539	15717089	5909009	25.454	19.867
34)	L7 AR-1260-4	7.043	7.007	12338590	3969081	27.549	19.151 #
35)	L7 AR-1260-5	7.287	7.249	29400717	11299387	24.284	24.122
36)	L8 AR-1262-1	6.784	6.749	15717089	5918996	17.163	14.276
37)	L8 AR-1262-2	7.287	7.249	29400717	11299387	19.443	21.827
38)	L8 AR-1262-3	7.570	7.528	3246157	1693072	5.858	9.427 #
39)	L8 AR-1262-4	7.633	7.592	10740130	4825245	10.982	16.644 #
40)	L8 AR-1262-5	8.130	8.086	8463006	2131951	20.301	19.680
41)	L9 AR-1268-1	7.570	7.528	3246157	1693072	1.886	3.323 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090525\
 Data File : P0113516.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 18:17
 Operator : YP/AJ
 Sample : Q2893-09
 Misc : AR1660 WATER LOD 25PPB
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:34:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	7.633	7.592	10740130	4825245	7.416	11.616 #
43) L9	AR-1268-3	7.834	7.791	336736	135378	0.279	0.415 #
44) L9	AR-1268-4	8.130	8.086	8463006	2131951	18.371	17.702
45) L9	AR-1268-5	8.418	8.372	1180959	238372	0.370	0.305



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090525\
Data File : PO113516.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2025 18:17
Operator : YP/AJ
Sample : Q2893-09
Misc : AR1660 WATER LOD 25PPB
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 23:34:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

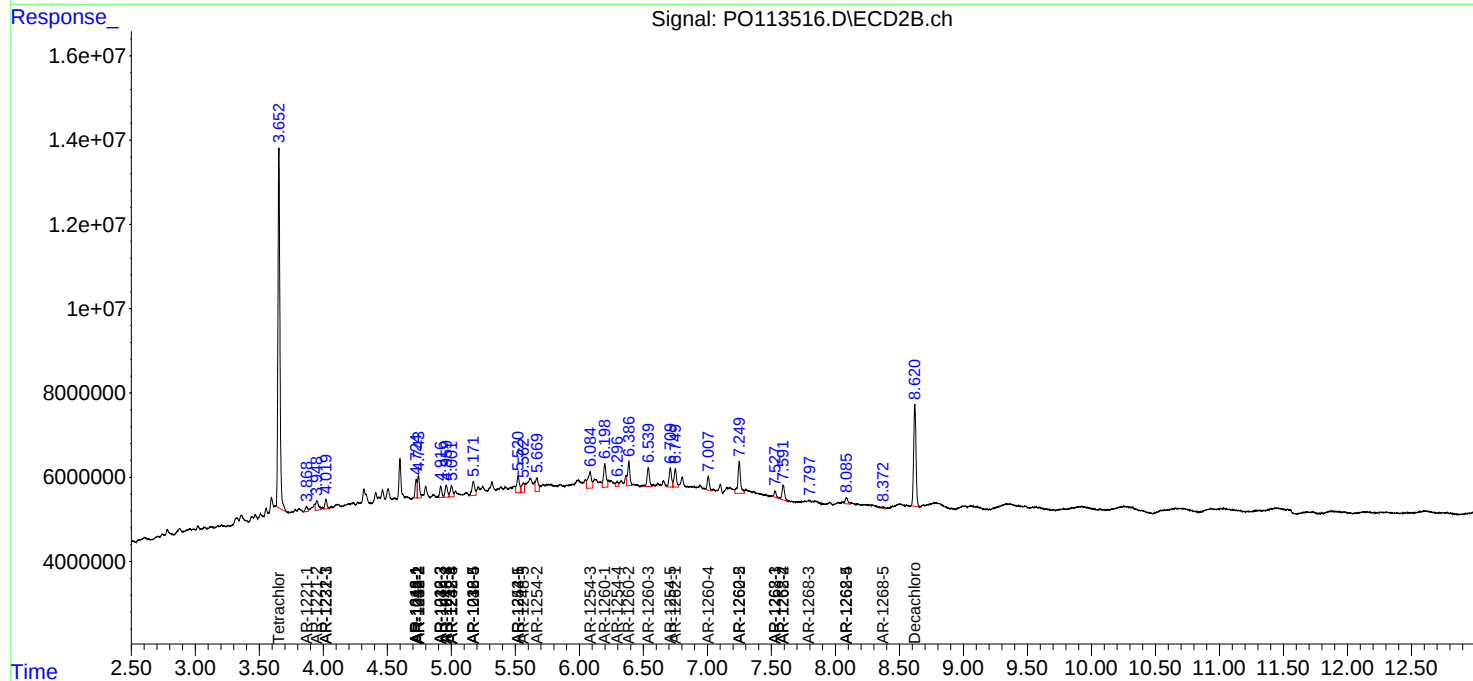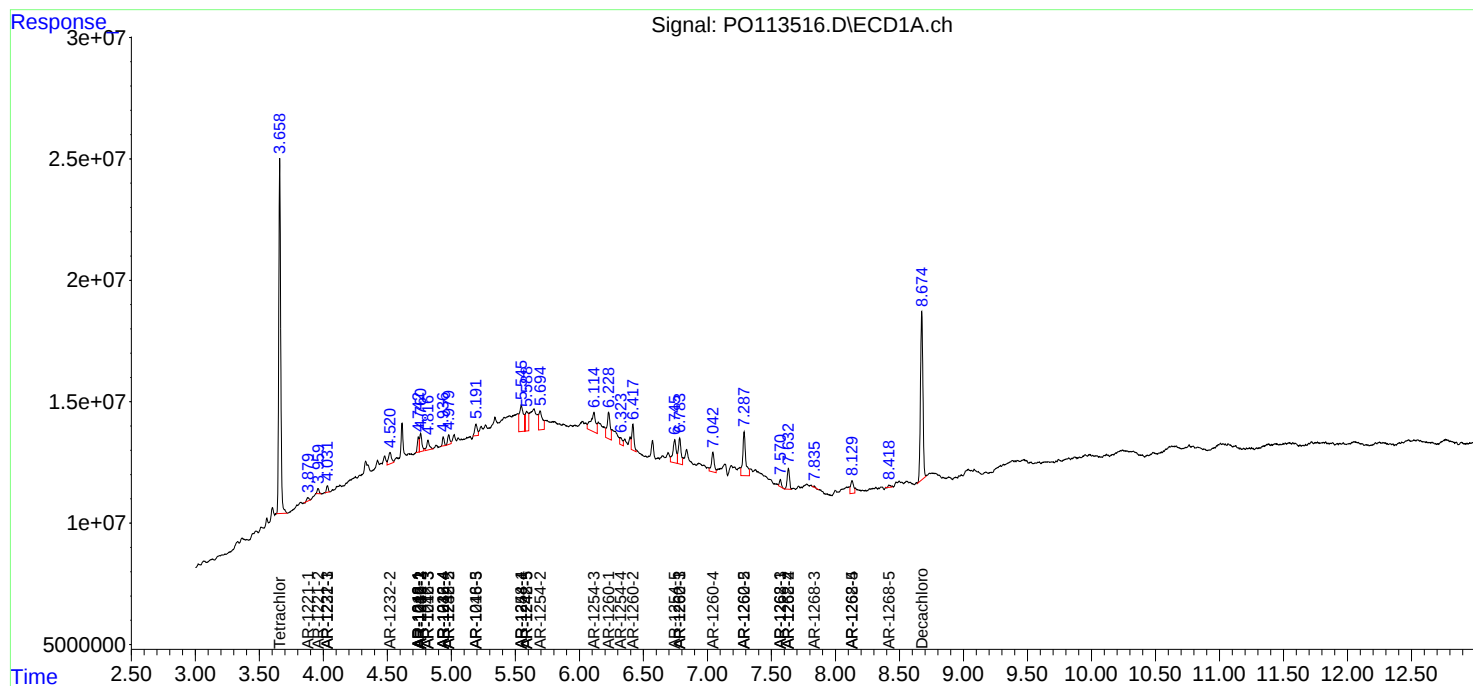


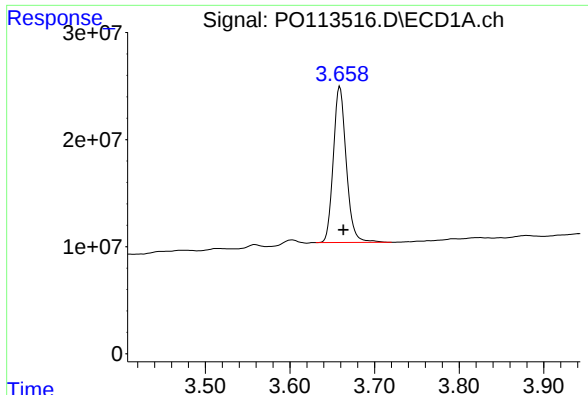

#1 Tetrachloro-m-xylene


R.T.: 3.659 min
Delta R.T.: -0.004 min
Response: 155002981
Conc: 18.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

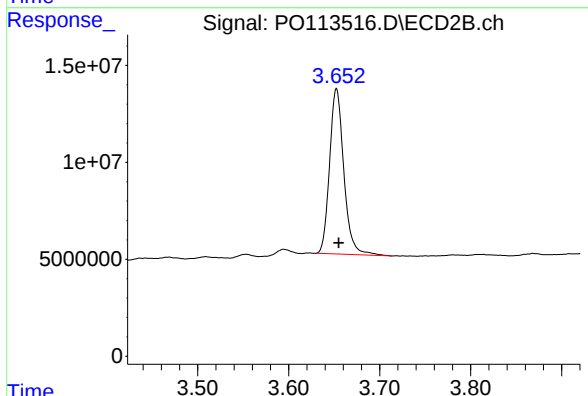


#1 Tetrachloro-m-xylene

R.T.: 3.653 min
Delta R.T.: -0.002 min
Response: 92834892
Conc: 18.34 ng/ml

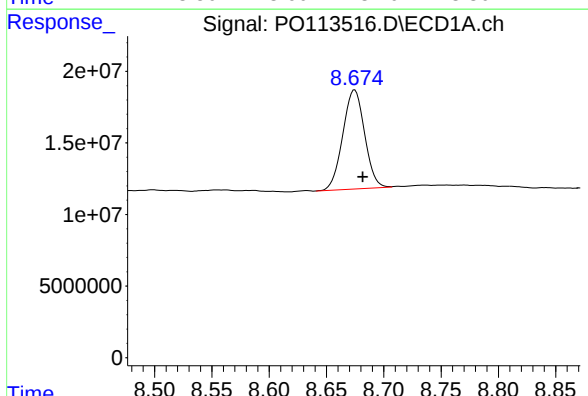


#2 Decachlorobiphenyl

R.T.: 8.675 min
Delta R.T.: -0.007 min
Response: 91699101
Conc: 13.23 ng/ml

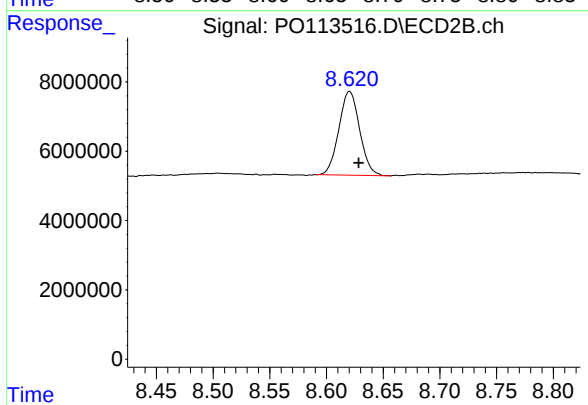

#2 Decachlorobiphenyl


R.T.: 8.620 min
Delta R.T.: -0.008 min
Response: 30899920
Conc: 16.31 ng/ml

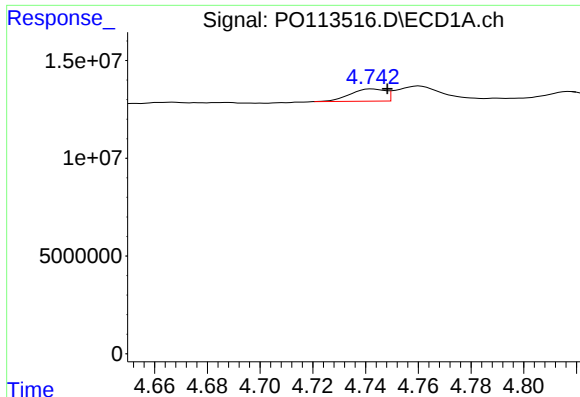

#3 AR-1016-1


R.T.: 4.742 min
Delta R.T.: -0.006 min
Response: 5763227
Conc: 21.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

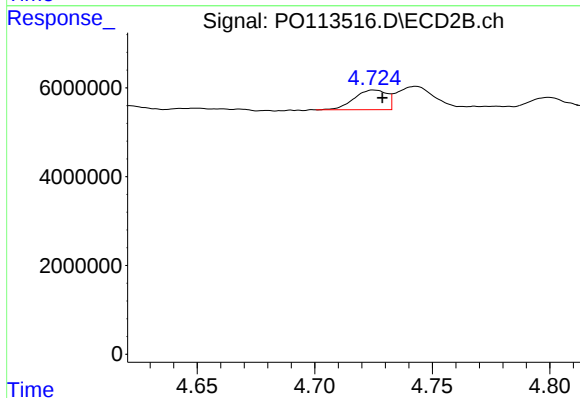


#3 AR-1016-1

R.T.: 4.725 min
Delta R.T.: -0.004 min
Response: 4297785
Conc: 25.20 ng/ml

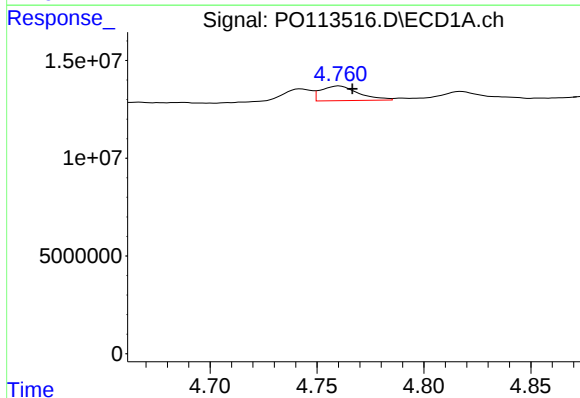


#4 AR-1016-2

R.T.: 4.760 min
Delta R.T.: -0.006 min
Response: 9141528
Conc: 22.77 ng/ml

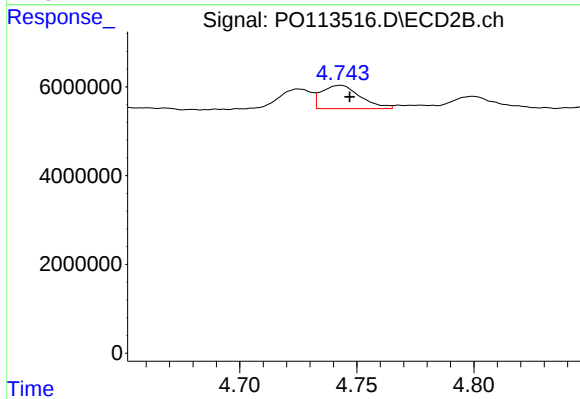

#4 AR-1016-2


R.T.: 4.743 min
Delta R.T.: -0.004 min
Response: 6036296
Conc: 23.43 ng/ml

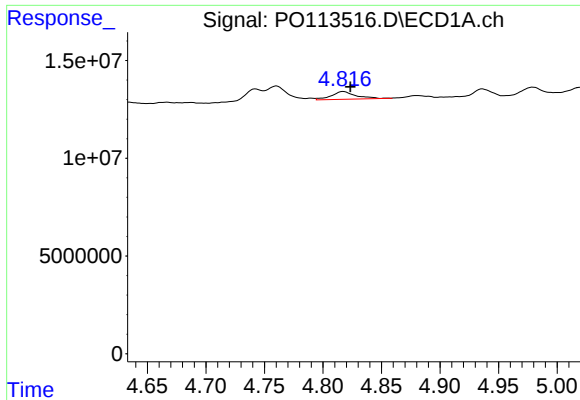

#5 AR-1016-3


R.T.: 4.817 min
Delta R.T.: -0.006 min
Response: 5789065
Conc: 22.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

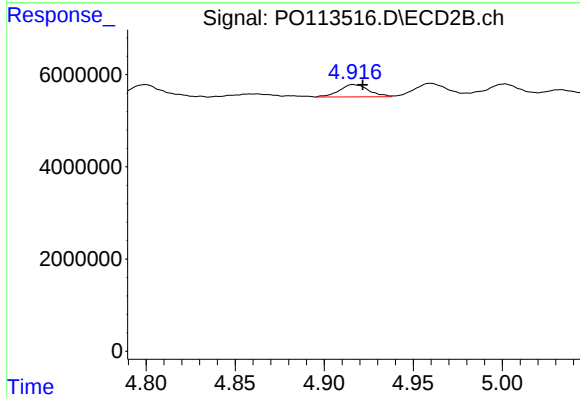


#5 AR-1016-3

R.T.: 4.916 min
Delta R.T.: -0.005 min
Response: 3058782
Conc: 21.91 ng/ml

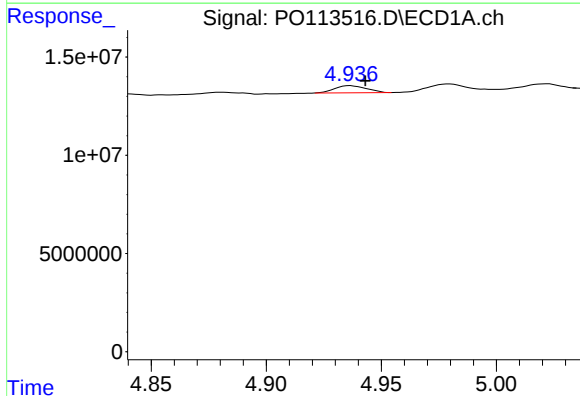


#6 AR-1016-4

R.T.: 4.936 min
Delta R.T.: -0.007 min
Response: 3464345
Conc: 15.89 ng/ml

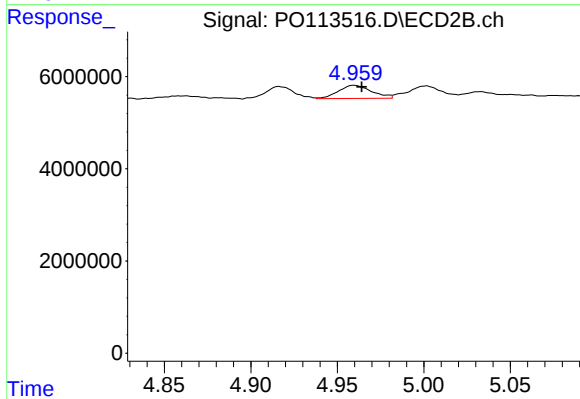

#6 AR-1016-4


R.T.: 4.960 min
Delta R.T.: -0.005 min
Response: 3794926
Conc: 32.52 ng/ml

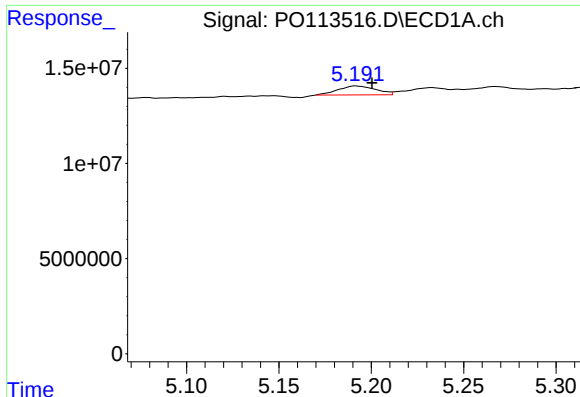

#7 AR-1016-5


R.T.: 5.192 min
Delta R.T.: -0.008 min
Response: 6683333
Conc: 30.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

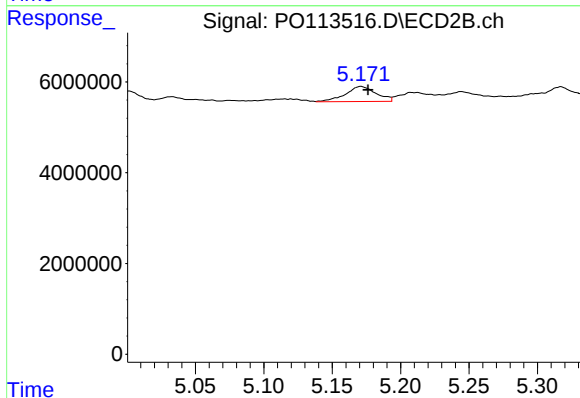


#7 AR-1016-5

R.T.: 5.171 min
Delta R.T.: -0.005 min
Response: 5224125
Conc: 36.65 ng/ml

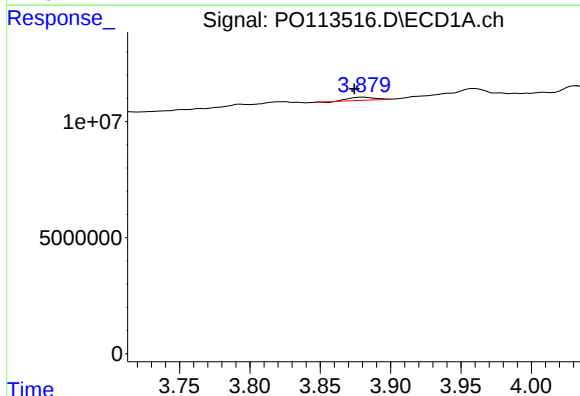


#8 AR-1221-1

R.T.: 3.880 min
Delta R.T.: 0.006 min
Response: 1646696
Conc: 17.60 ng/ml

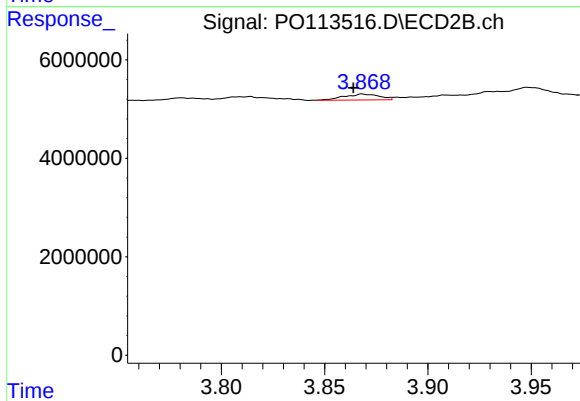

#8 AR-1221-1


R.T.: 3.868 min
Delta R.T.: 0.004 min
Response: 1438834
Conc: 22.79 ng/ml

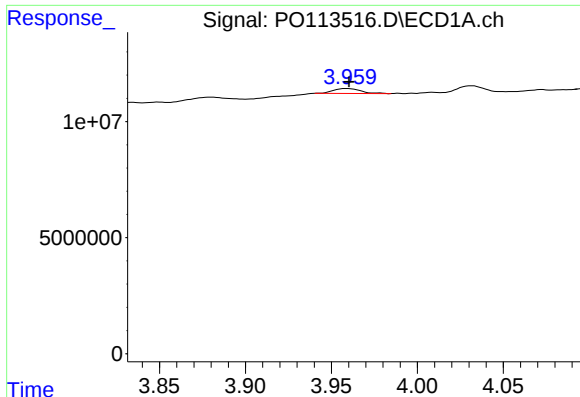

#9 AR-1221-2


R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 2312416
Conc: 34.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

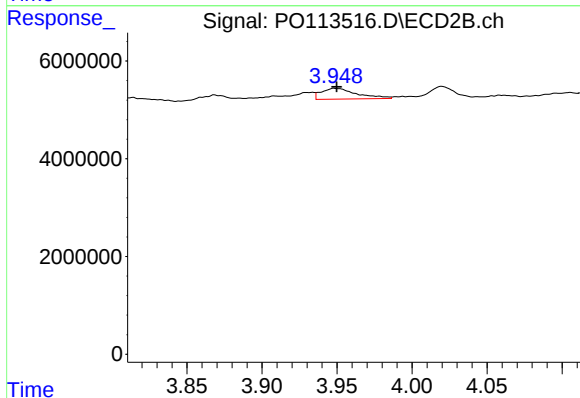


#9 AR-1221-2

R.T.: 3.948 min
Delta R.T.: -0.002 min
Response: 3652005
Conc: 78.25 ng/ml

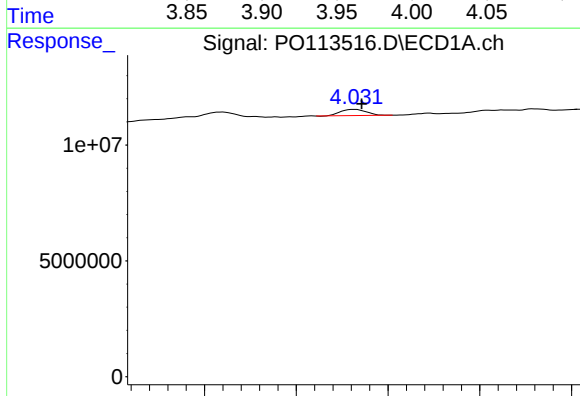


#10 AR-1221-3

R.T.: 4.032 min
Delta R.T.: -0.004 min
Response: 2607110
Conc: 11.78 ng/ml

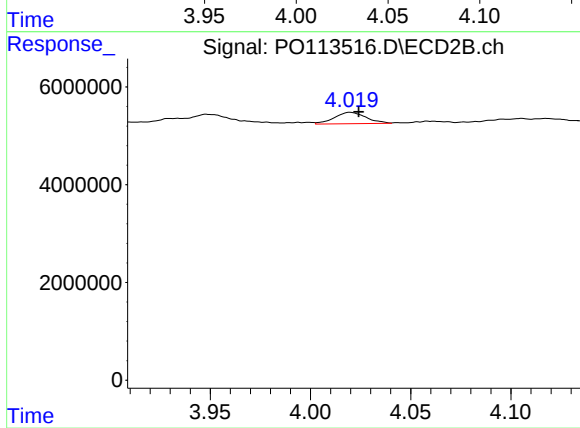

#10 AR-1221-3


R.T.: 4.020 min
Delta R.T.: -0.004 min
Response: 2563462
Conc: 17.27 ng/ml

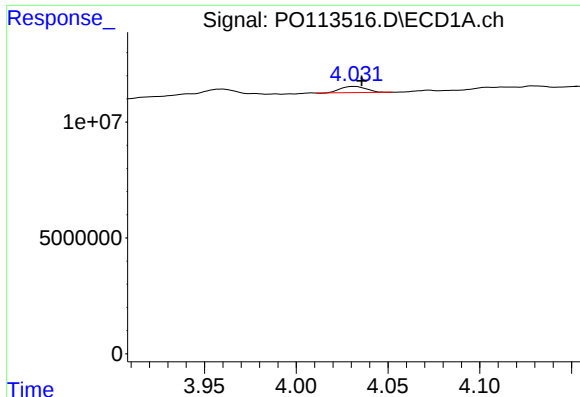

#11 AR-1232-1


R.T.: 4.032 min
Delta R.T.: -0.004 min
Response: 2607110
Conc: 14.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

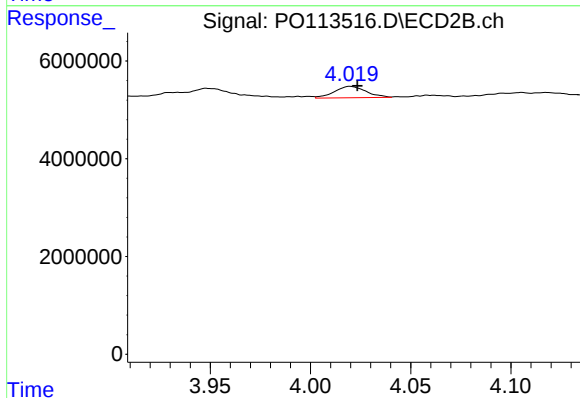


#11 AR-1232-1

R.T.: 4.020 min
Delta R.T.: -0.004 min
Response: 2563462
Conc: 21.83 ng/ml

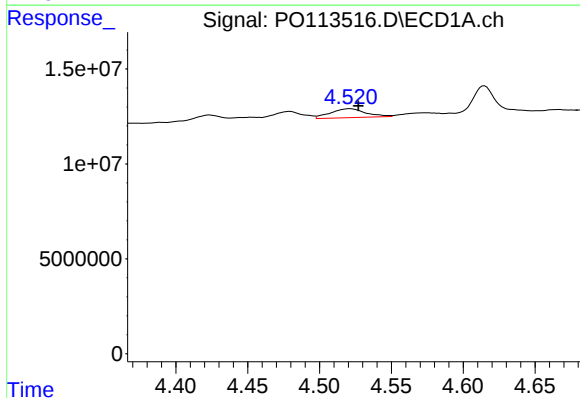


#12 AR-1232-2

R.T.: 4.521 min
Delta R.T.: -0.006 min
Response: 7993691
Conc: 80.06 ng/ml

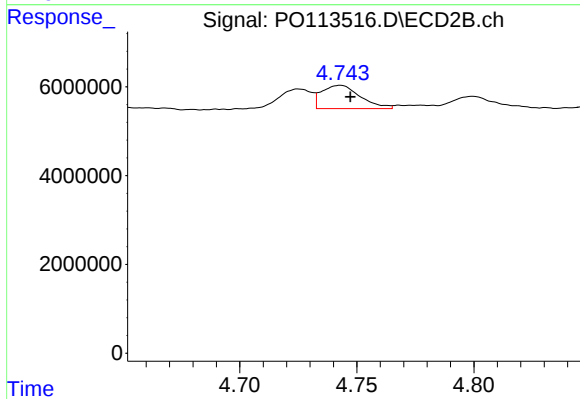

#12 AR-1232-2


R.T.: 4.743 min
Delta R.T.: -0.004 min
Response: 6036296
Conc: 49.26 ng/ml

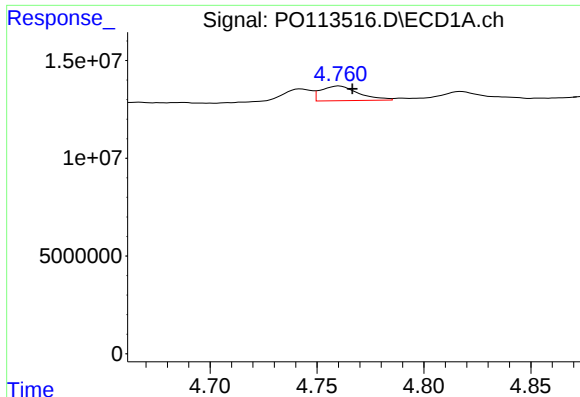

#13 AR-1232-3


R.T.: 4.760 min
Delta R.T.: -0.006 min
Response: 9141528
Conc: 48.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

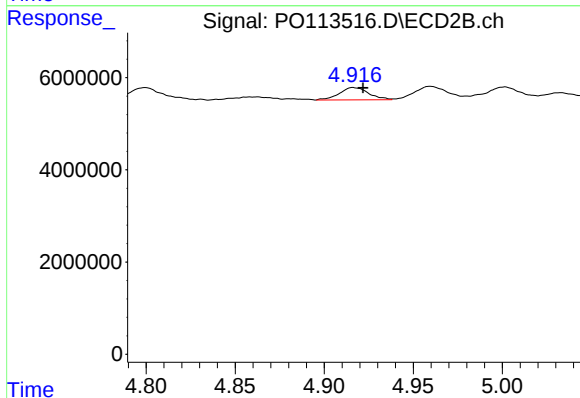


#13 AR-1232-3

R.T.: 4.916 min
Delta R.T.: -0.006 min
Response: 3058782
Conc: 48.29 ng/ml

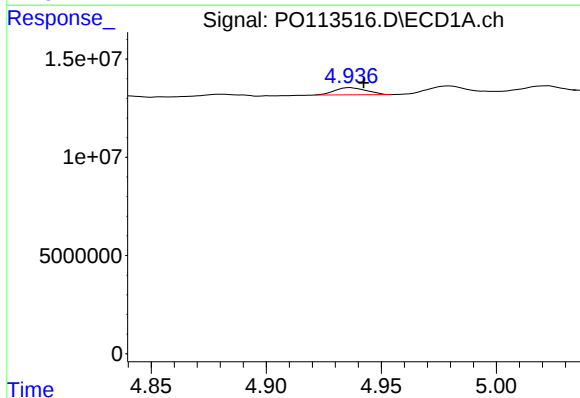


#14 AR-1232-4

R.T.: 4.936 min
Delta R.T.: -0.006 min
Response: 3464345
Conc: 36.79 ng/ml

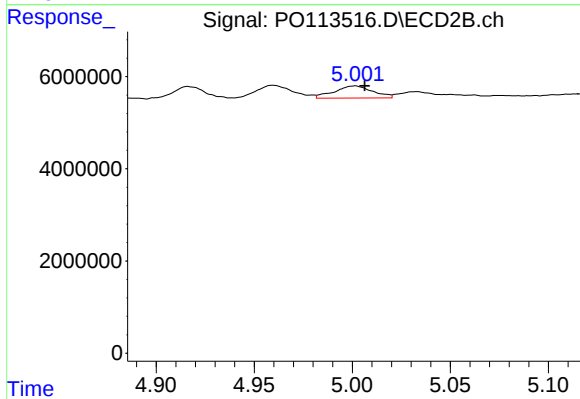

#14 AR-1232-4


R.T.: 5.002 min
Delta R.T.: -0.005 min
Response: 3610958
Conc: 64.23 ng/ml

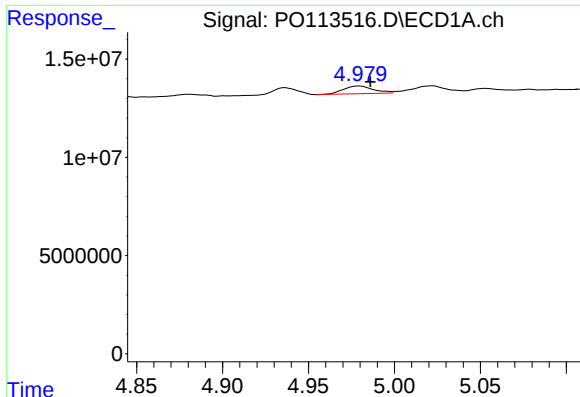

#15 AR-1232-5


R.T.: 4.980 min
Delta R.T.: -0.006 min
Response: 4710305
Conc: 76.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

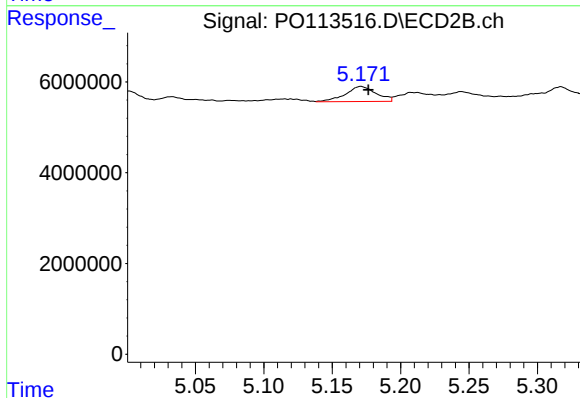


#15 AR-1232-5

R.T.: 5.171 min
Delta R.T.: -0.005 min
Response: 5224125
Conc: 87.27 ng/ml

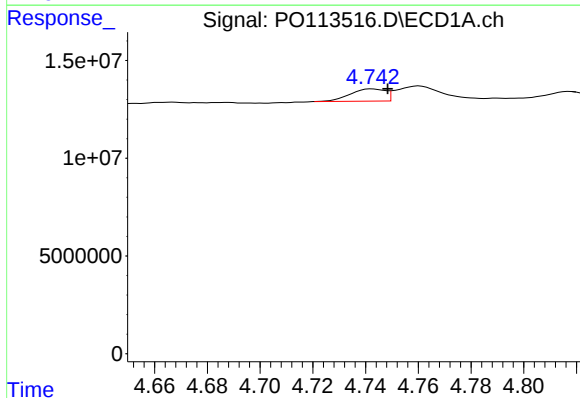


#16 AR-1242-1

R.T.: 4.742 min
Delta R.T.: -0.006 min
Response: 5763227
Conc: 25.06 ng/ml

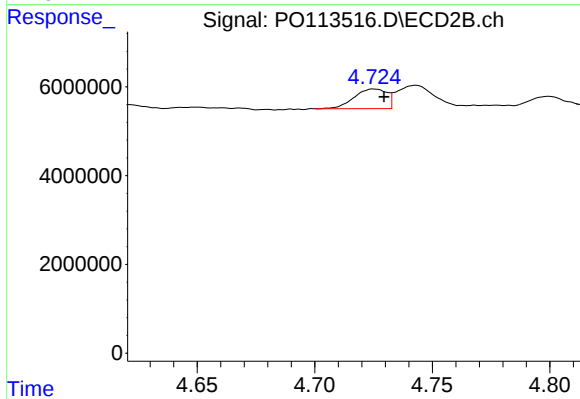

#16 AR-1242-1


R.T.: 4.725 min
Delta R.T.: -0.004 min
Response: 4297785
Conc: 29.74 ng/ml

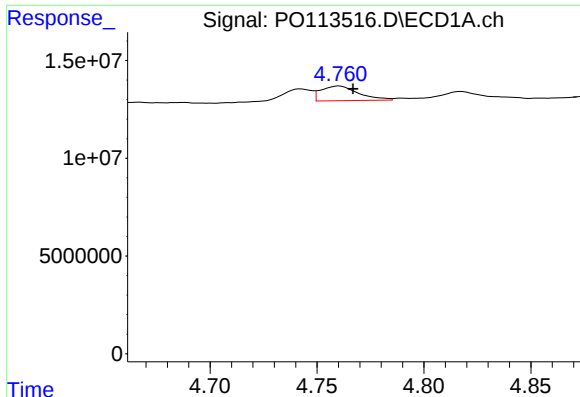

#17 AR-1242-2


R.T.: 4.760 min
Delta R.T.: -0.006 min
Response: 9141528
Conc: 26.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

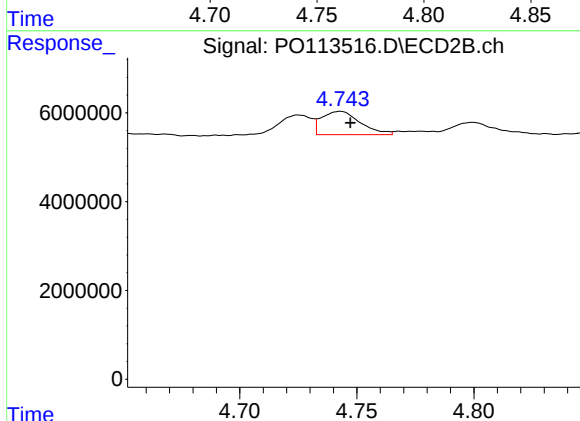


#17 AR-1242-2

R.T.: 4.743 min
Delta R.T.: -0.004 min
Response: 6036296
Conc: 27.83 ng/ml

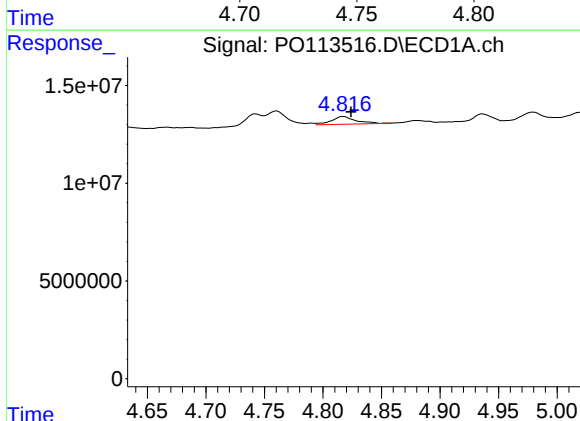


#18 AR-1242-3

R.T.: 4.817 min
Delta R.T.: -0.007 min
Response: 5789065
Conc: 26.09 ng/ml

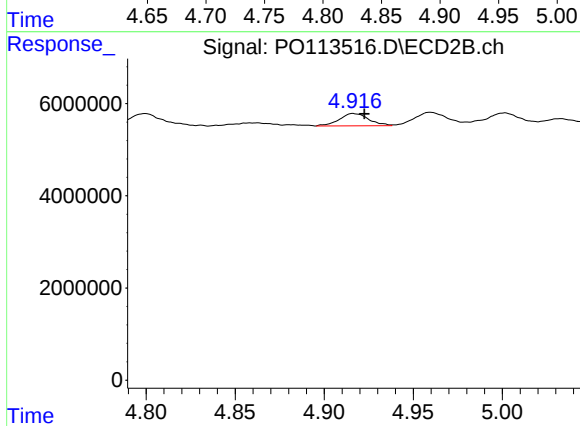

#18 AR-1242-3


R.T.: 4.916 min
Delta R.T.: -0.006 min
Response: 3058782
Conc: 26.15 ng/ml

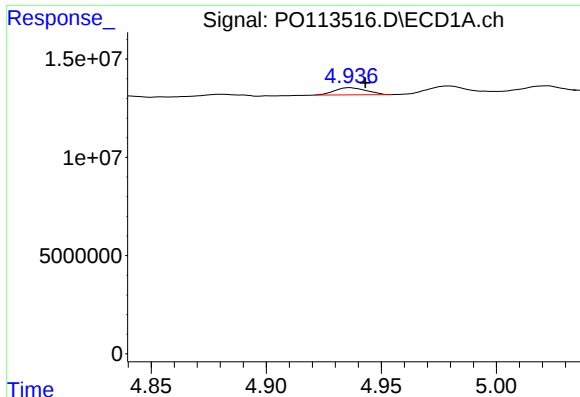

#19 AR-1242-4


R.T.: 4.936 min
Delta R.T.: -0.007 min
Response: 3464345
Conc: 19.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

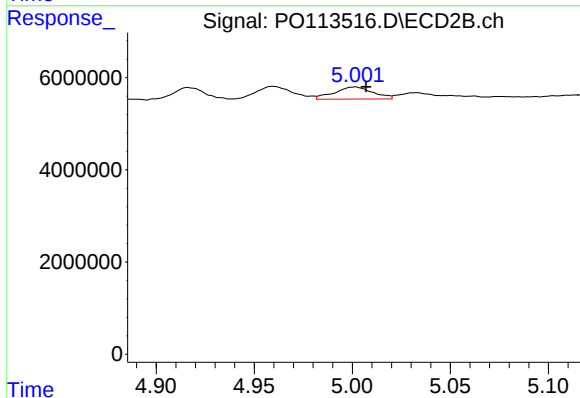


#19 AR-1242-4

R.T.: 5.002 min
Delta R.T.: -0.005 min
Response: 3610958
Conc: 30.70 ng/ml

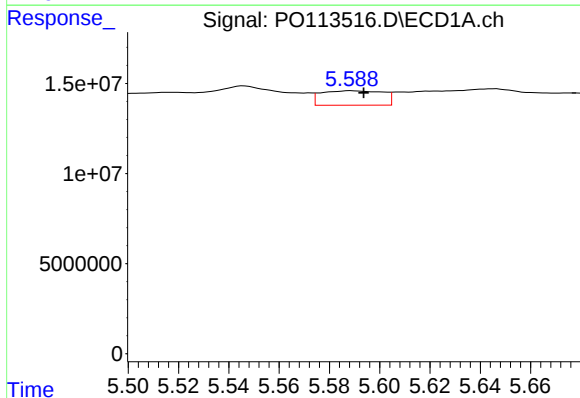


#20 AR-1242-5

R.T.: 5.589 min
Delta R.T.: -0.005 min
Response: 13679199
Conc: 68.34 ng/ml

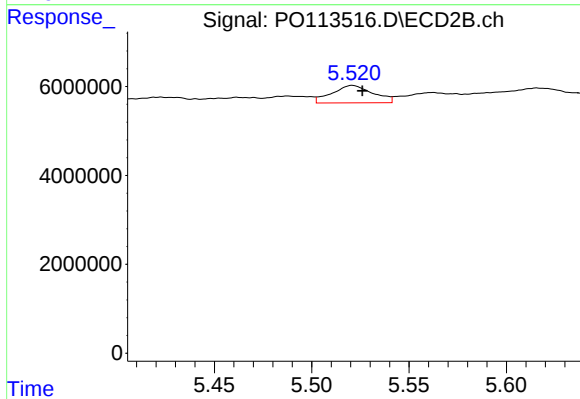

#20 AR-1242-5


R.T.: 5.521 min
Delta R.T.: -0.005 min
Response: 5737882
Conc: 38.47 ng/ml

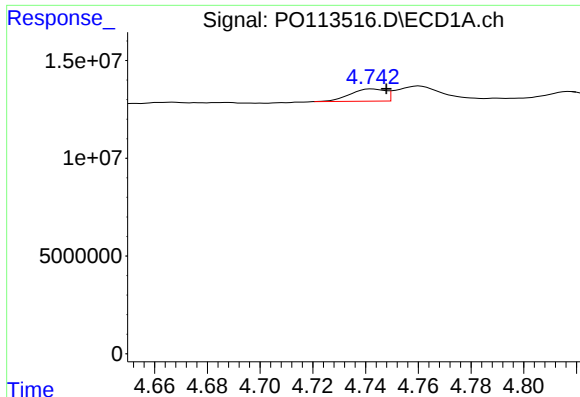

#21 AR-1248-1


R.T.: 4.742 min
Delta R.T.: -0.005 min
Response: 5763227
Conc: 33.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

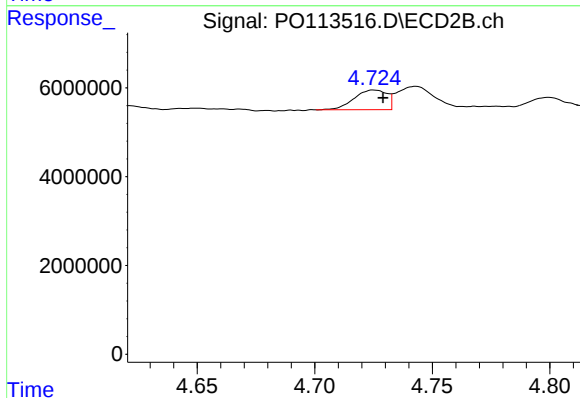


#21 AR-1248-1

R.T.: 4.725 min
Delta R.T.: -0.004 min
Response: 4297785
Conc: 38.54 ng/ml

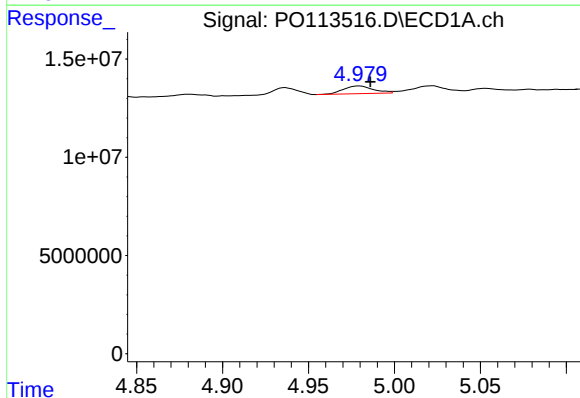


#22 AR-1248-2

R.T.: 4.980 min
Delta R.T.: -0.006 min
Response: 4710305
Conc: 19.47 ng/ml

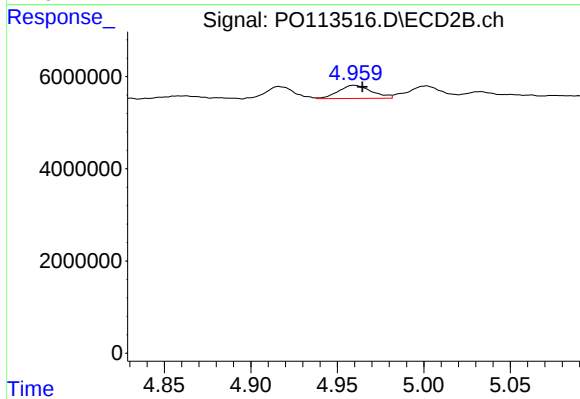

#22 AR-1248-2


R.T.: 4.960 min
Delta R.T.: -0.005 min
Response: 3794926
Conc: 23.62 ng/ml

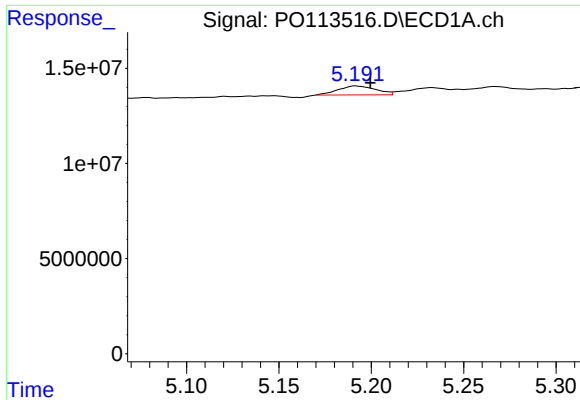

#23 AR-1248-3


R.T.: 5.192 min
Delta R.T.: -0.008 min
Response: 6683333
Conc: 20.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

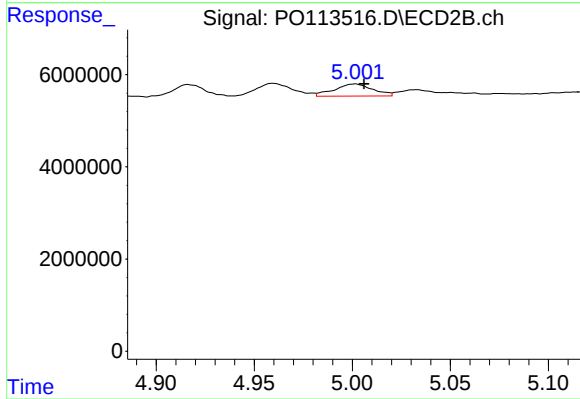


#23 AR-1248-3

R.T.: 5.002 min
Delta R.T.: -0.004 min
Response: 3610958
Conc: 21.28 ng/ml

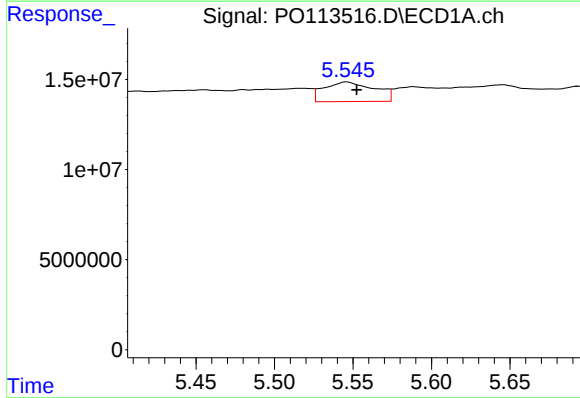


#24 AR-1248-4

R.T.: 5.546 min
Delta R.T.: -0.006 min
Response: 24396868
Conc: 48.83 ng/ml

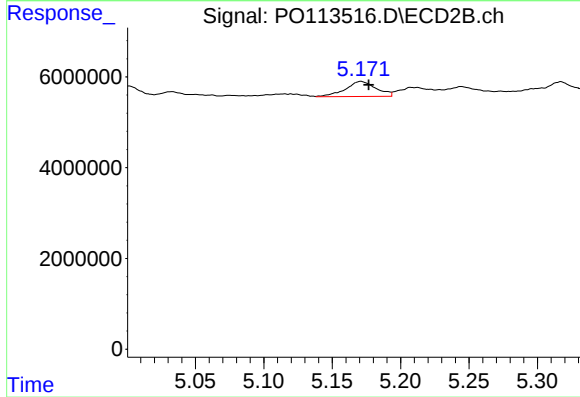

#24 AR-1248-4


R.T.: 5.171 min
Delta R.T.: -0.006 min
Response: 5224125
Conc: 26.22 ng/ml

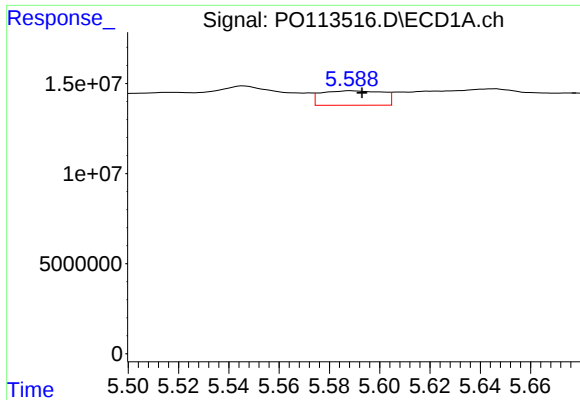

#25 AR-1248-5


R.T.: 5.589 min
Delta R.T.: -0.004 min
Response: 13679199
Conc: 40.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

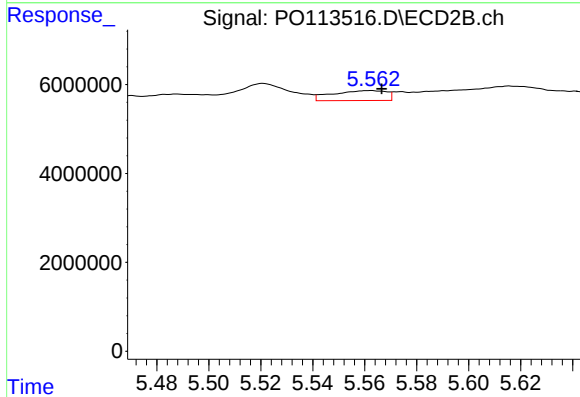


#25 AR-1248-5

R.T.: 5.563 min
Delta R.T.: -0.004 min
Response: 3231342
Conc: 15.22 ng/ml

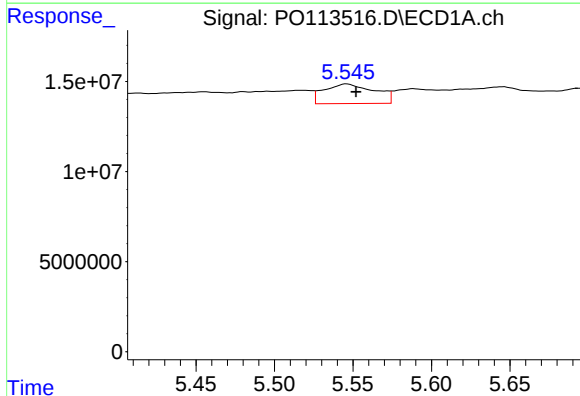


#26 AR-1254-1

R.T.: 5.546 min
Delta R.T.: -0.006 min
Response: 24396868
Conc: 45.18 ng/ml

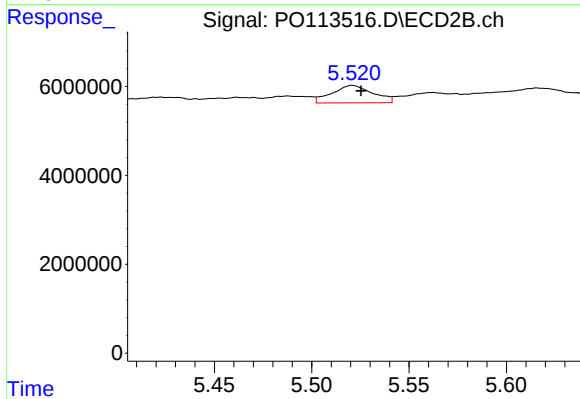

#26 AR-1254-1


R.T.: 5.521 min
Delta R.T.: -0.004 min
Response: 5737882
Conc: 18.20 ng/ml

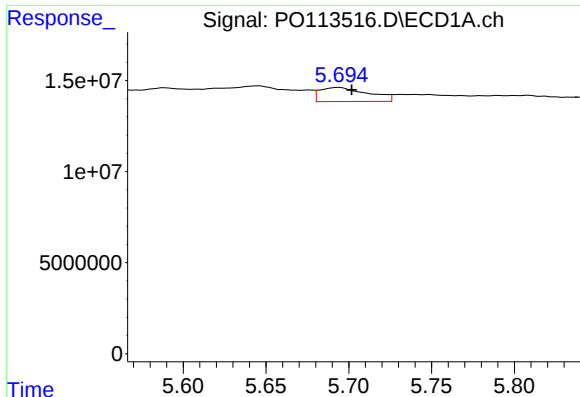

#27 AR-1254-2


R.T.: 5.694 min
Delta R.T.: -0.008 min
Response: 15495390
Conc: 31.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

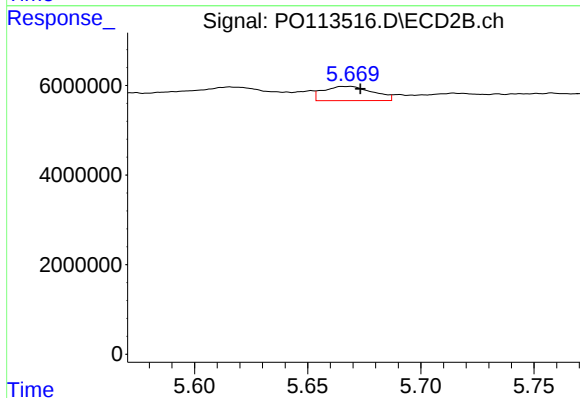


#27 AR-1254-2

R.T.: 5.669 min
Delta R.T.: -0.004 min
Response: 4823293
Conc: 17.21 ng/ml

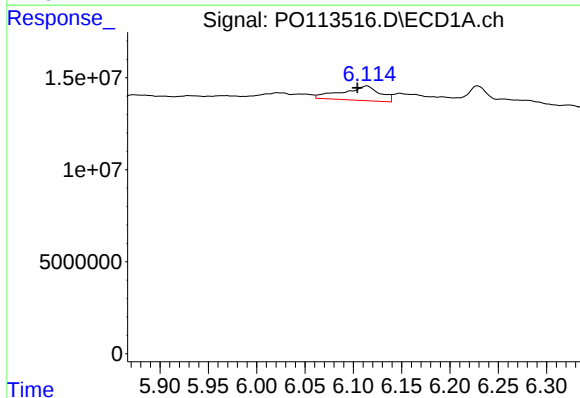


#28 AR-1254-3

R.T.: 6.114 min
Delta R.T.: 0.010 min
Response: 21279268
Conc: 28.80 ng/ml

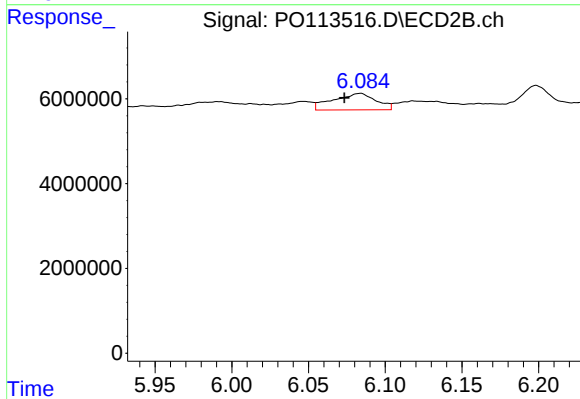

#28 AR-1254-3


R.T.: 6.084 min
Delta R.T.: 0.011 min
Response: 7595413
Conc: 18.22 ng/ml

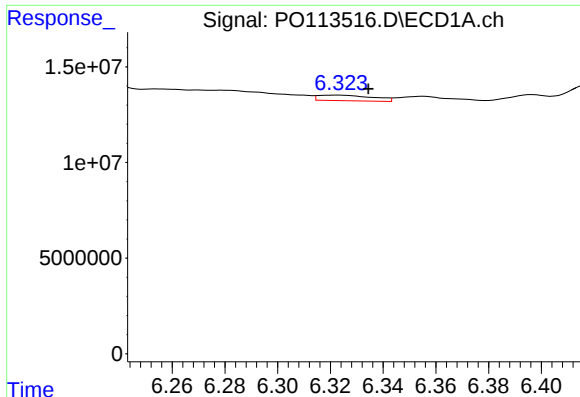

#29 AR-1254-4


R.T.: 6.323 min
Delta R.T.: -0.011 min
Response: 4143861
Conc: 7.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

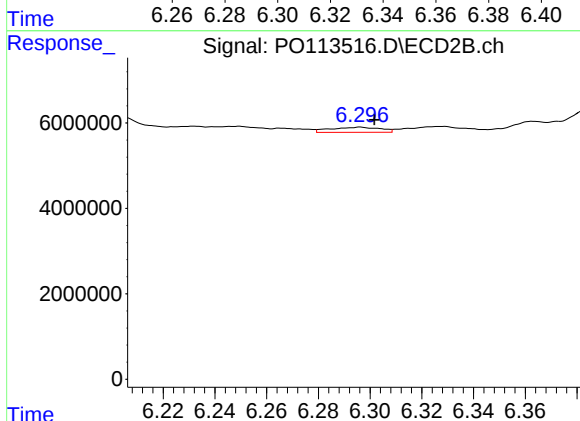


#29 AR-1254-4

R.T.: 6.296 min
Delta R.T.: -0.005 min
Response: 1603007
Conc: 5.83 ng/ml

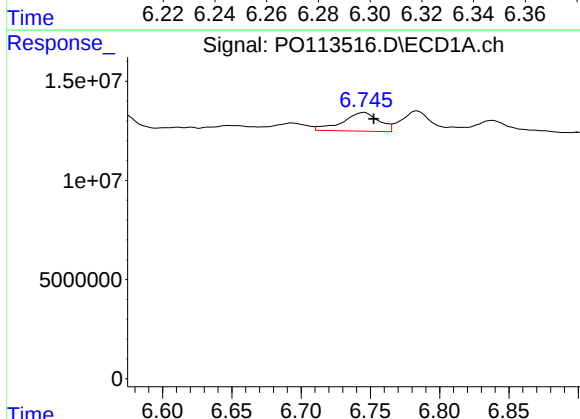


#30 AR-1254-5

R.T.: 6.745 min
Delta R.T.: -0.007 min
Response: 17229178
Conc: 24.58 ng/ml

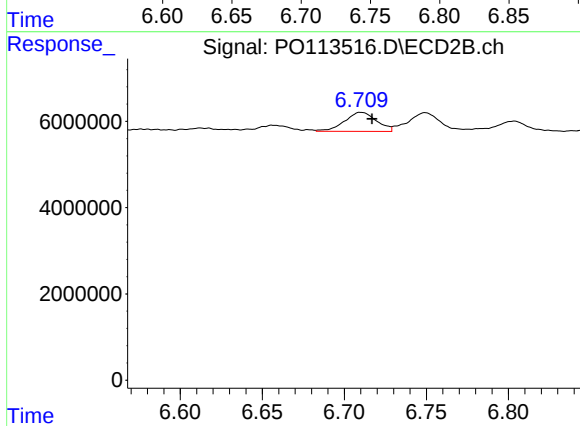

#30 AR-1254-5


R.T.: 6.710 min
Delta R.T.: -0.007 min
Response: 5954666
Conc: 16.66 ng/ml

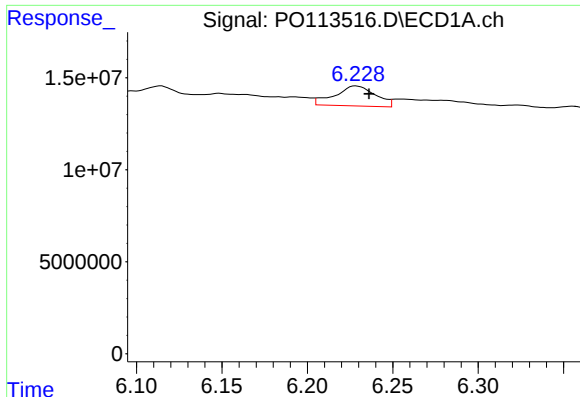

#31 AR-1260-1


R.T.: 6.228 min
Delta R.T.: -0.008 min
Response: 17979431
Conc: 40.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

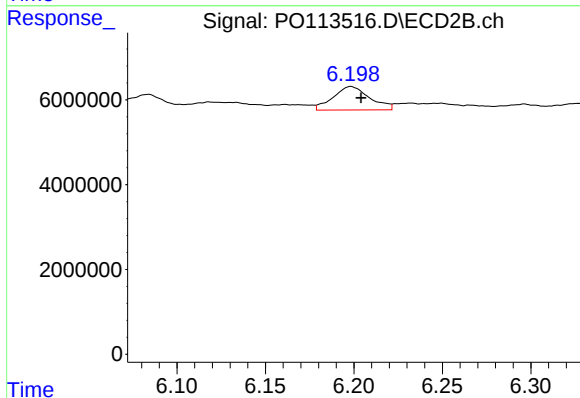


#31 AR-1260-1

R.T.: 6.198 min
Delta R.T.: -0.006 min
Response: 7975846
Conc: 31.27 ng/ml

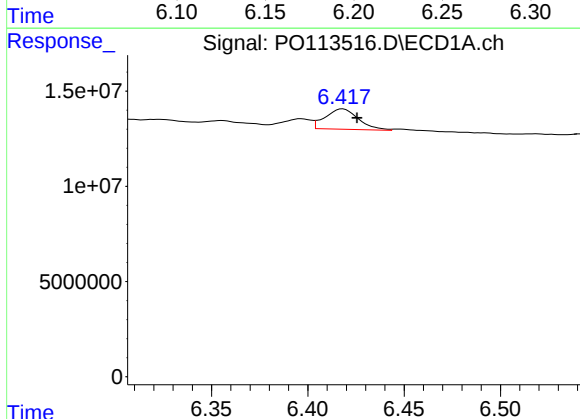


#32 AR-1260-2

R.T.: 6.418 min
Delta R.T.: -0.007 min
Response: 12841117
Conc: 18.70 ng/ml

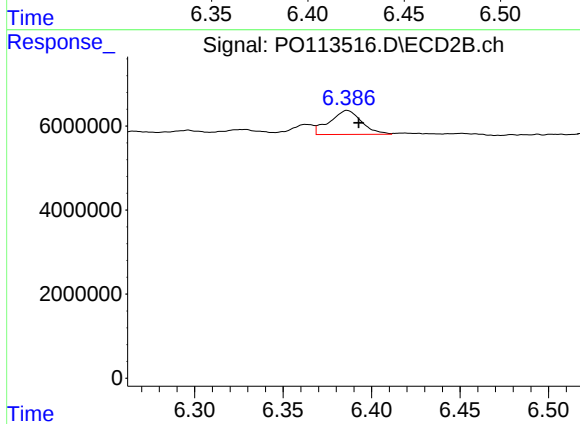

#32 AR-1260-2


R.T.: 6.386 min
Delta R.T.: -0.006 min
Response: 7239107
Conc: 20.94 ng/ml

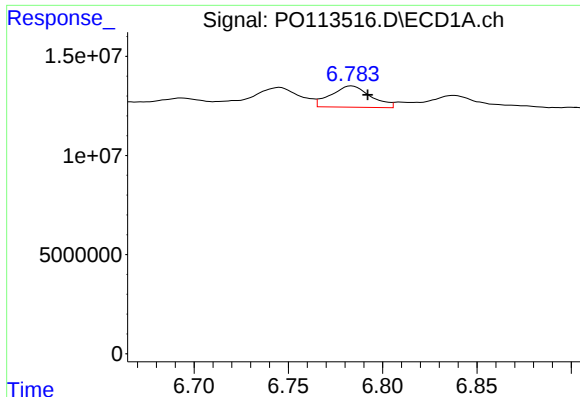

#33 AR-1260-3


R.T.: 6.784 min
Delta R.T.: -0.009 min
Response: 15717089
Conc: 25.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

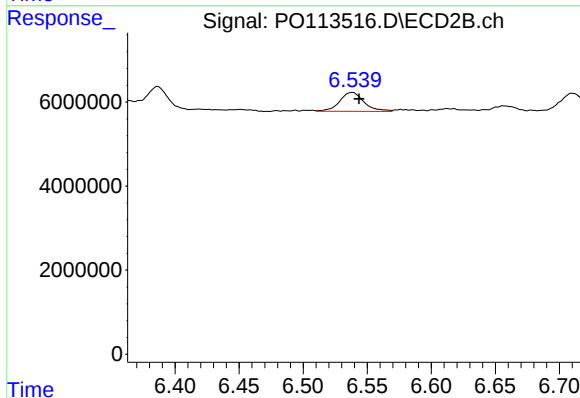


#33 AR-1260-3

R.T.: 6.539 min
Delta R.T.: -0.005 min
Response: 5909009
Conc: 19.87 ng/ml

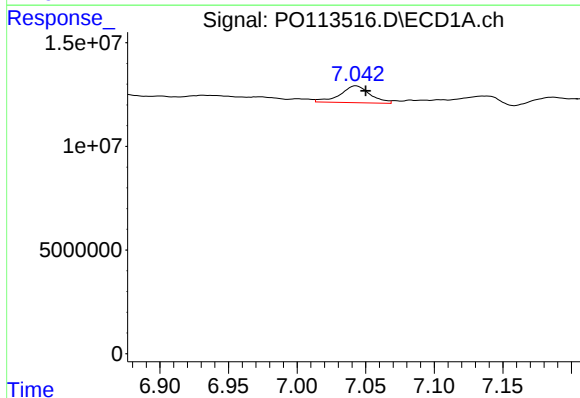


#34 AR-1260-4

R.T.: 7.043 min
Delta R.T.: -0.007 min
Response: 12338590
Conc: 27.55 ng/ml

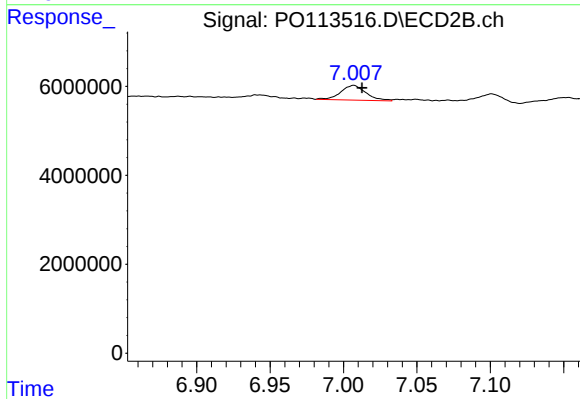

#34 AR-1260-4


R.T.: 7.007 min
Delta R.T.: -0.006 min
Response: 3969081
Conc: 19.15 ng/ml

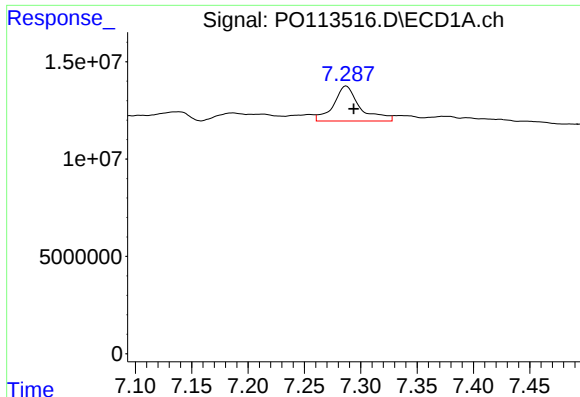

#35 AR-1260-5


R.T.: 7.287 min
Delta R.T.: -0.007 min
Response: 29400717
Conc: 24.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

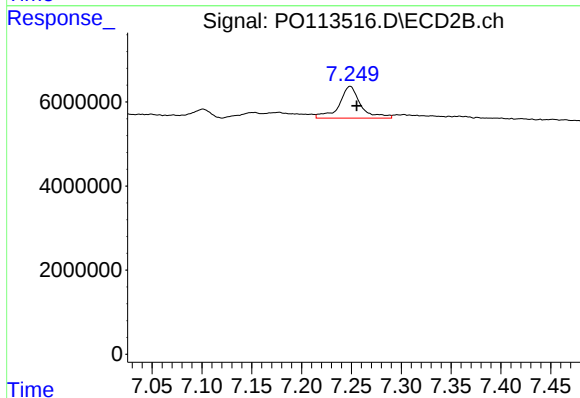


#35 AR-1260-5

R.T.: 7.249 min
Delta R.T.: -0.007 min
Response: 11299387
Conc: 24.12 ng/ml

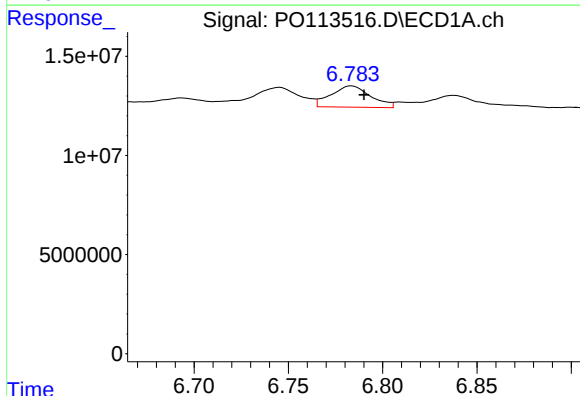


#36 AR-1262-1

R.T.: 6.784 min
Delta R.T.: -0.007 min
Response: 15717089
Conc: 17.16 ng/ml

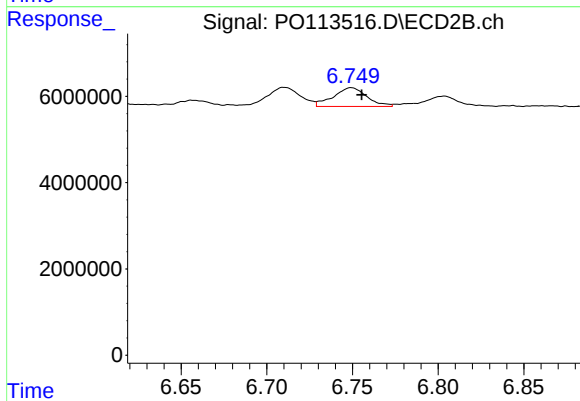

#36 AR-1262-1


R.T.: 6.749 min
Delta R.T.: -0.006 min
Response: 5918996
Conc: 14.28 ng/ml

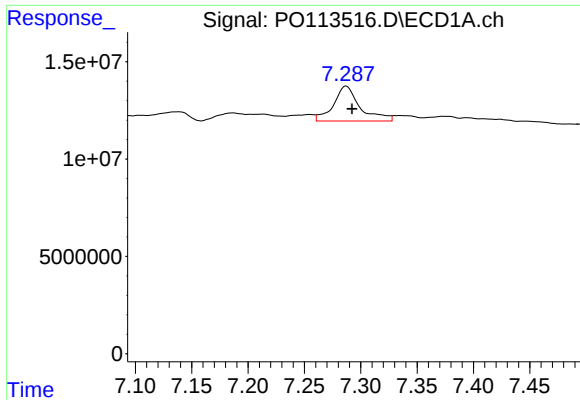

#37 AR-1262-2


R.T.: 7.287 min
Delta R.T.: -0.005 min
Response: 29400717
Conc: 19.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

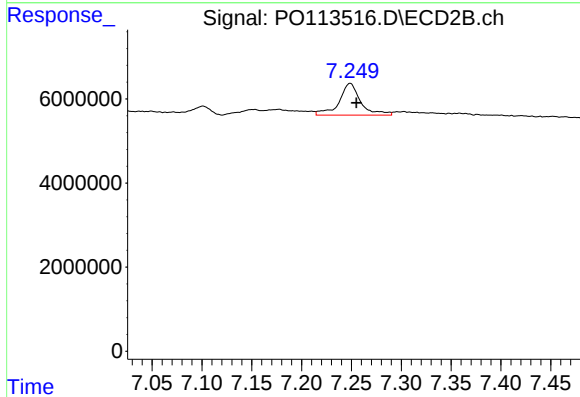


#37 AR-1262-2

R.T.: 7.249 min
Delta R.T.: -0.006 min
Response: 11299387
Conc: 21.83 ng/ml

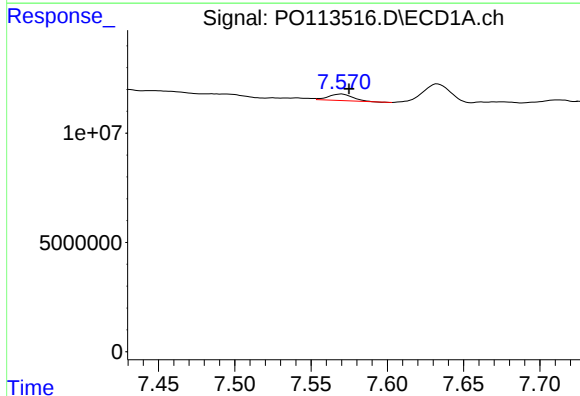


#38 AR-1262-3

R.T.: 7.570 min
Delta R.T.: -0.005 min
Response: 3246157
Conc: 5.86 ng/ml

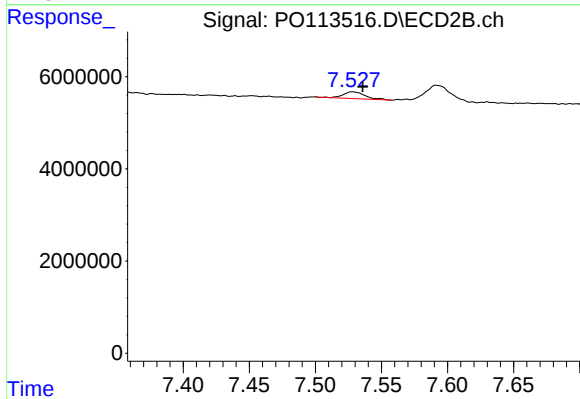

#38 AR-1262-3


R.T.: 7.528 min
Delta R.T.: -0.008 min
Response: 1693072
Conc: 9.43 ng/ml

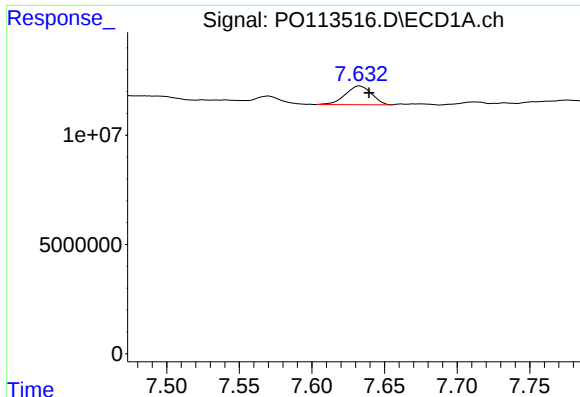

#39 AR-1262-4


R.T.: 7.633 min
Delta R.T.: -0.006 min
Response: 10740130
Conc: 10.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

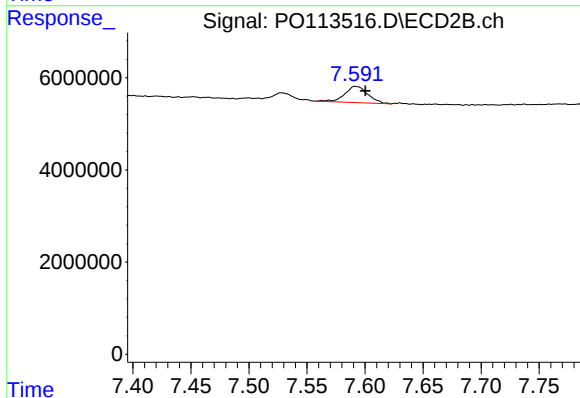


#39 AR-1262-4

R.T.: 7.592 min
Delta R.T.: -0.008 min
Response: 4825245
Conc: 16.64 ng/ml

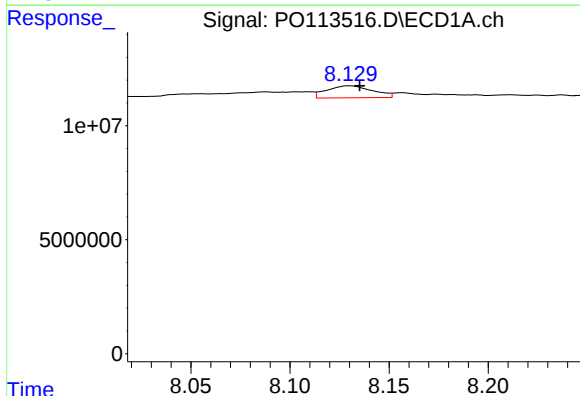


#40 AR-1262-5

R.T.: 8.130 min
Delta R.T.: -0.005 min
Response: 8463006
Conc: 20.30 ng/ml

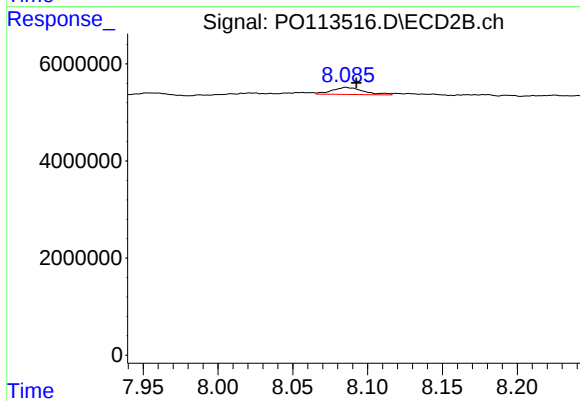

#40 AR-1262-5


R.T.: 8.086 min
Delta R.T.: -0.007 min
Response: 2131951
Conc: 19.68 ng/ml

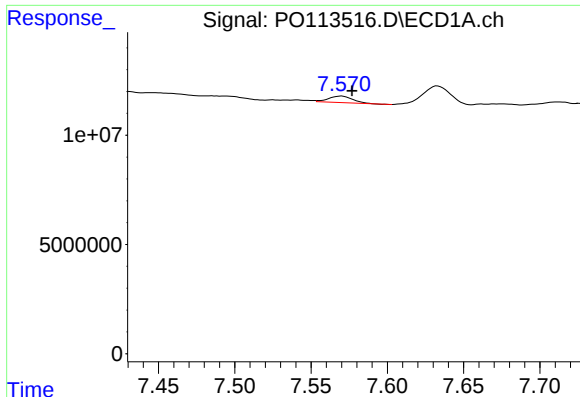

#41 AR-1268-1


R.T.: 7.570 min
Delta R.T.: -0.007 min
Response: 3246157
Conc: 1.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

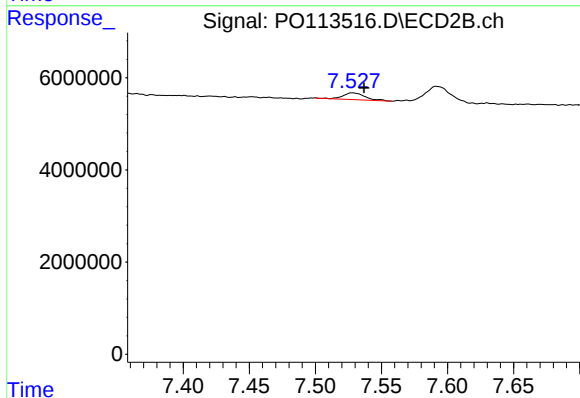


#41 AR-1268-1

R.T.: 7.528 min
Delta R.T.: -0.009 min
Response: 1693072
Conc: 3.32 ng/ml

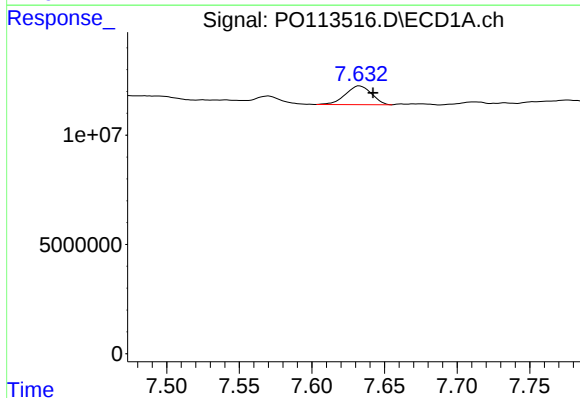


#42 AR-1268-2

R.T.: 7.633 min
Delta R.T.: -0.009 min
Response: 10740130
Conc: 7.42 ng/ml

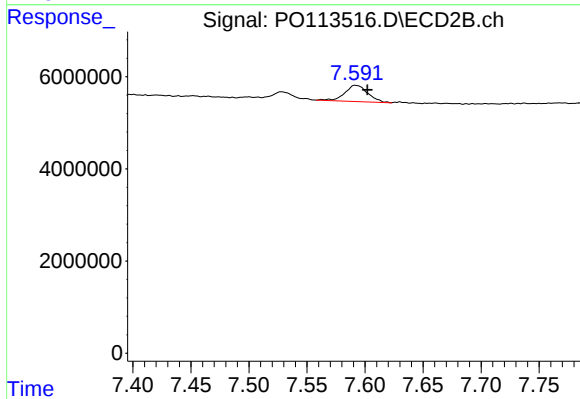

#42 AR-1268-2


R.T.: 7.592 min
Delta R.T.: -0.010 min
Response: 4825245
Conc: 11.62 ng/ml

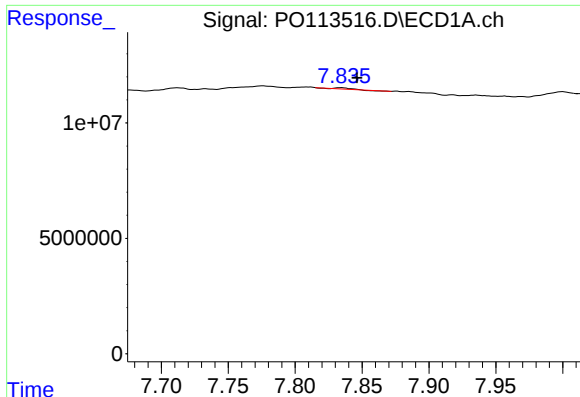

#43 AR-1268-3


R.T.: 7.834 min
Delta R.T.: -0.012 min
Response: 336736
Conc: 0.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

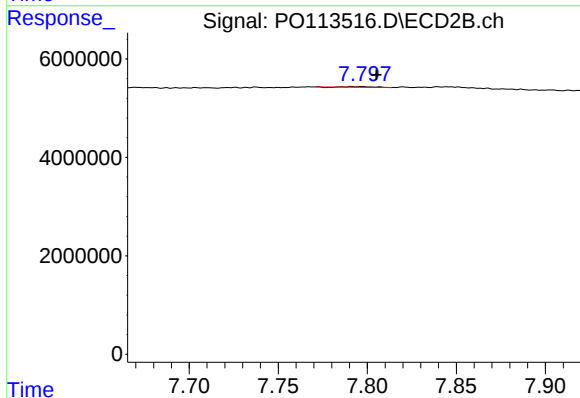


#43 AR-1268-3

R.T.: 7.791 min
Delta R.T.: -0.014 min
Response: 135378
Conc: 0.41 ng/ml

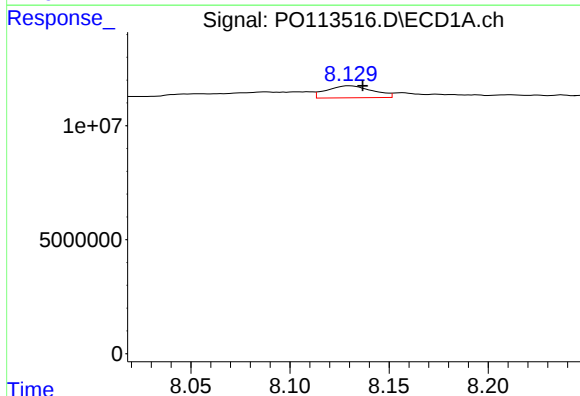


#44 AR-1268-4

R.T.: 8.130 min
Delta R.T.: -0.007 min
Response: 8463006
Conc: 18.37 ng/ml

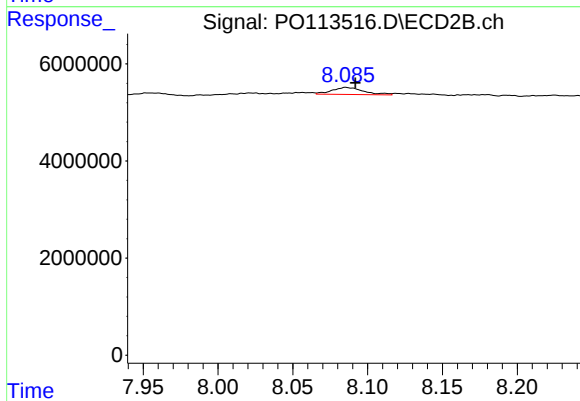

#44 AR-1268-4


R.T.: 8.086 min
Delta R.T.: -0.006 min
Response: 2131951
Conc: 17.70 ng/ml

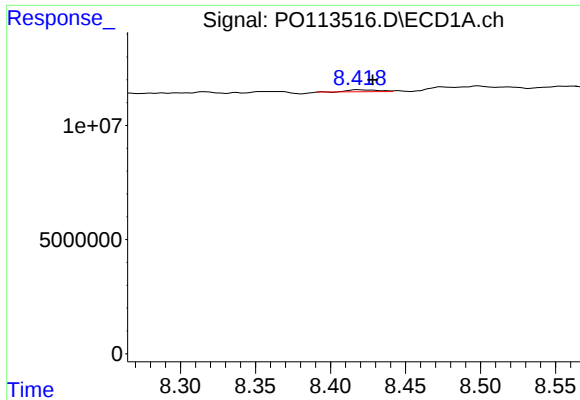

#45 AR-1268-5

R.T.: 8.418 min
Delta R.T.: -0.010 min
Response: 1180959
Conc: 0.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

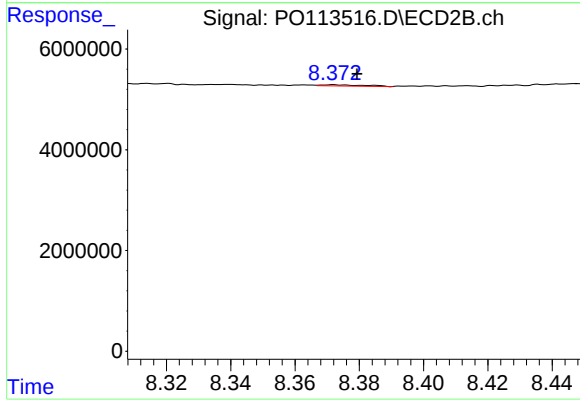

#45 AR-1268-5

R.T.: 8.372 min
Delta R.T.: -0.007 min
Response: 238372
Conc: 0.31 ng/ml