

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090525\
 Data File : P0113517.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 18:35
 Operator : YP/AJ
 Sample : Q2893-09
 Misc : AR1221 WATER LOD 25PPB
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:34:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.659	3.653	164.5E6	98146773	20.093	19.394
2)	SA Decachlor...	8.675	8.620	97316739	32921198	14.040	17.374
Target Compounds							
3)	L1 AR-1016-1	4.739	4.725	539036	278088	2.019	1.630
4)	L1 AR-1016-2	4.759	4.745	1122038	451470	2.795	1.752 #
5)	L1 AR-1016-3	4.817	4.920	736093	317216	2.886	2.272
6)	L1 AR-1016-4	4.941	4.969	416913	627449	1.912	5.377 #
7)	L1 AR-1016-5	5.197	5.174	1741820	1169236	7.859	8.203
8)	L2 AR-1221-1	3.870	3.862	1848855	1309666	19.758	20.748
9)	L2 AR-1221-2	3.959	3.948	3255986	2391862	48.201	51.247
10)	L2 AR-1221-3	4.032	4.021	4413129	3352734	19.937	22.581
11)	L3 AR-1232-1	4.032	4.021	4413129	3352734	25.362	28.558
12)	L3 AR-1232-2	4.532	4.745	695194	451470	6.962	3.684 #
13)	L3 AR-1232-3	4.759	4.920	1122038	317216	5.922	5.008
14)	L3 AR-1232-4	4.941	5.001	416913	419152	4.427	7.455 #
15)	L3 AR-1232-5	5.022f	5.174	1103176	1169236	17.810	19.532
16)	L4 AR-1242-1	4.739	4.725	539036	278088	2.344	1.924
17)	L4 AR-1242-2	4.759	4.745	1122038	451470	3.265	2.081 #
18)	L4 AR-1242-3	4.817	4.920	736093	317216	3.317	2.712
19)	L4 AR-1242-4	4.941	5.001	416913	419152	2.403	3.563 #
20)	L4 AR-1242-5	5.595	5.531	5700674	339006	28.480	2.273 #
21)	L5 AR-1248-1	4.739	4.725	539036	278088	3.090	2.494
22)	L5 AR-1248-2	5.022f	4.969	1103176	627449	4.561	3.904
23)	L5 AR-1248-3	5.197	5.001	1741820	419152	5.463	2.471 #
24)	L5 AR-1248-4	5.565	5.174	7388992	1169236	14.790	5.869 #
25)	L5 AR-1248-5	5.595	5.573	5700674	1846701	16.693	8.699 #
26)	L6 AR-1254-1	5.565	5.531	7388992	339006	13.684	1.075 #
27)	L6 AR-1254-2	5.704	5.676	2616946	569328	5.303	2.031 #
28)	L6 AR-1254-3	6.115	6.073	2843506	385881	3.848	0.926 #
29)	L6 AR-1254-4	6.326	6.300	1009926	264444	1.813	0.962 #
30)	L6 AR-1254-5	6.769	6.719	386232	29107	0.551	0.081 #
31)	L7 AR-1260-1	6.247	6.204	762369	148246	1.709	0.581 #
32)	L7 AR-1260-2	6.442	6.394	368739	46633	0.537	0.135 #
33)	L7 AR-1260-3	6.785	6.543	743518	277544	1.204	0.933
34)	L7 AR-1260-4	7.034	7.014	3707488	316957	8.278	1.529 #
35)	L7 AR-1260-5	7.299	7.254	2925361	273602	2.416	0.584 #
36)	L8 AR-1262-1	6.785	6.755	743518	36160	0.812	0.087 #
37)	L8 AR-1262-2	7.288	7.254	2034253	273602	1.345	0.529 #
38)	L8 AR-1262-3	7.522f	7.540	4468	53322	0.008	0.297 #
39)	L8 AR-1262-4	7.683f	7.599	914744	97953	0.935	0.338 #
40)	L8 AR-1262-5	8.141	8.097	3987946	71817	9.566	0.663 #
41)	L9 AR-1268-1	7.522f	7.540	4468	53322	0.003	0.105 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090525\
 Data File : P0113517.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 18:35
 Operator : YP/AJ
 Sample : Q2893-09
 Misc : AR1221 WATER LOD 25PPB
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:34:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	7.683f	7.599	914744	97953	0.632	0.236 #
43) L9	AR-1268-3	7.796f	7.807	266270	17667	0.221	0.054 #
44) L9	AR-1268-4	8.141	8.097	3987946	71817	8.657	0.596 #
45) L9	AR-1268-5	8.416	8.375	1532744	263022	0.481	0.337 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090525\
Data File : PO113517.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2025 18:35
Operator : YP/AJ
Sample : Q2893-09
Misc : AR1221 WATER LOD 25PPB
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 23:34:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

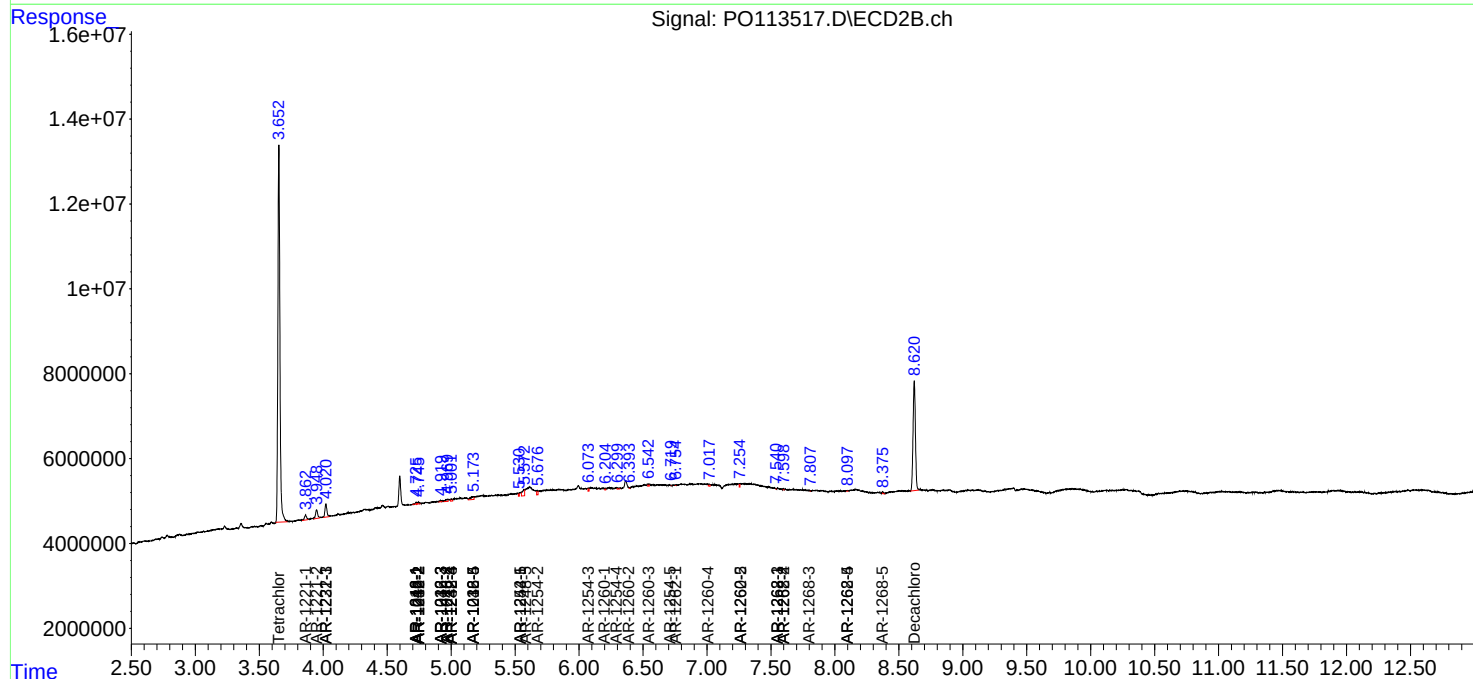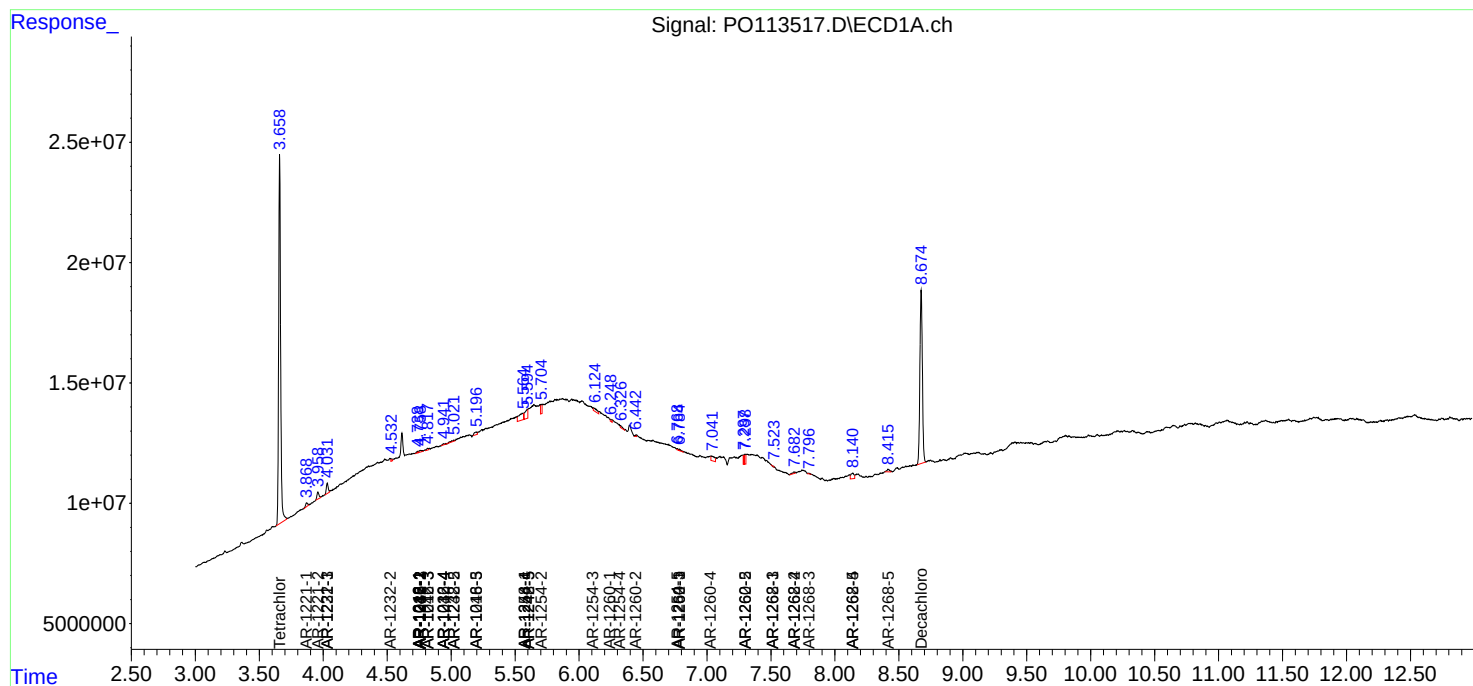


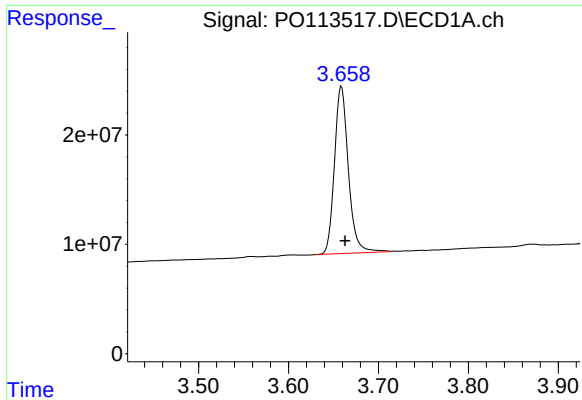

#1 Tetrachloro-m-xylene


R.T.: 3.659 min
Delta R.T.: -0.004 min
Response: 164489322
Conc: 20.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

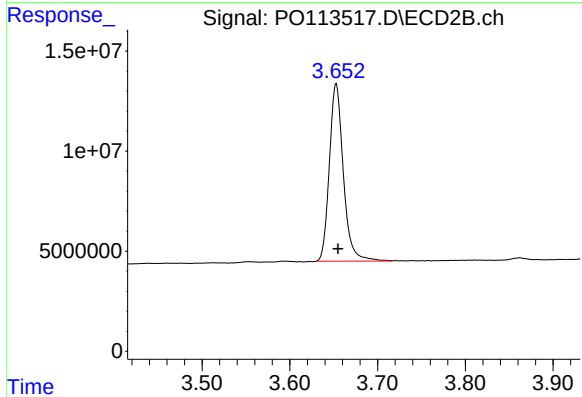


#1 Tetrachloro-m-xylene

R.T.: 3.653 min
Delta R.T.: -0.002 min
Response: 98146773
Conc: 19.39 ng/ml

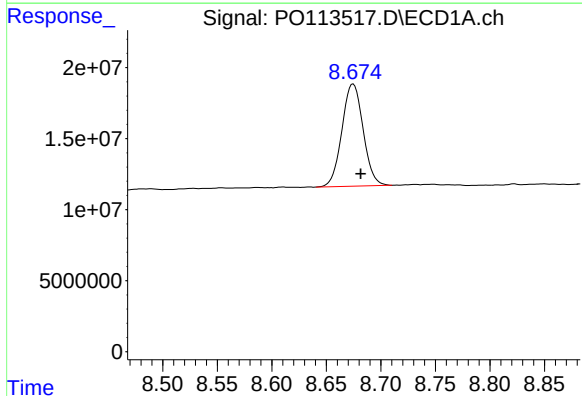


#2 Decachlorobiphenyl

R.T.: 8.675 min
Delta R.T.: -0.007 min
Response: 97316739
Conc: 14.04 ng/ml

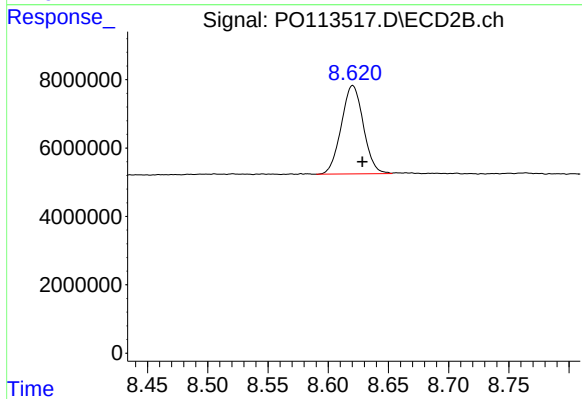

#2 Decachlorobiphenyl


R.T.: 8.620 min
Delta R.T.: -0.008 min
Response: 32921198
Conc: 17.37 ng/ml

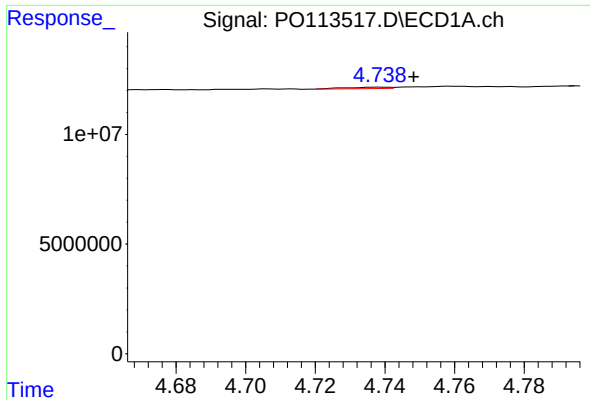

#3 AR-1016-1


R.T.: 4.739 min
Delta R.T.: -0.009 min
Response: 539036
Conc: 2.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

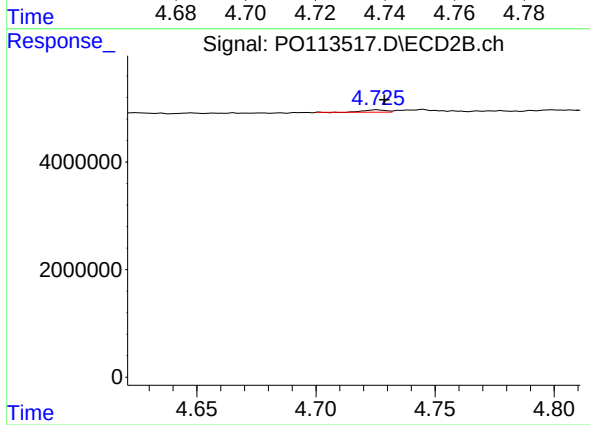


#3 AR-1016-1

R.T.: 4.725 min
Delta R.T.: -0.003 min
Response: 278088
Conc: 1.63 ng/ml

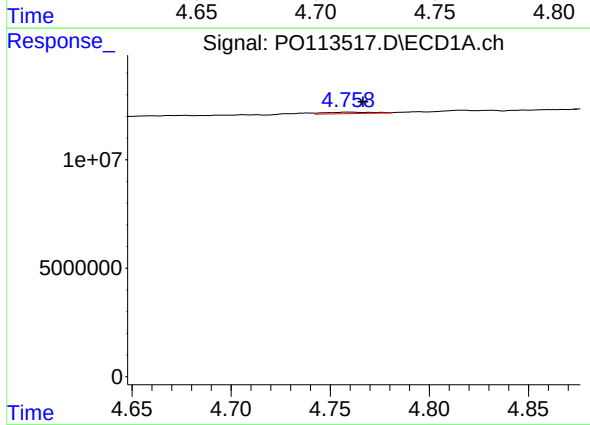


#4 AR-1016-2

R.T.: 4.759 min
Delta R.T.: -0.008 min
Response: 1122038
Conc: 2.80 ng/ml

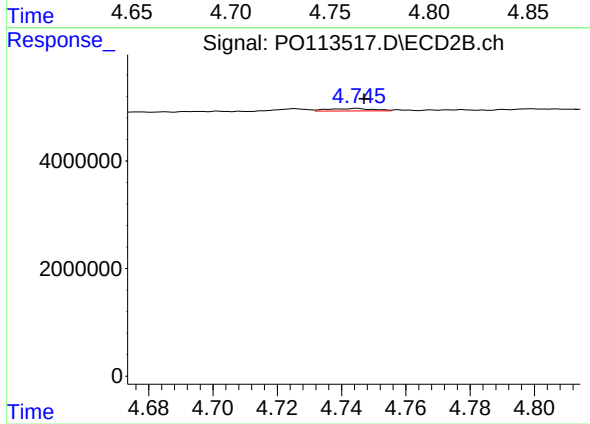

#4 AR-1016-2


R.T.: 4.745 min
Delta R.T.: -0.002 min
Response: 451470
Conc: 1.75 ng/ml

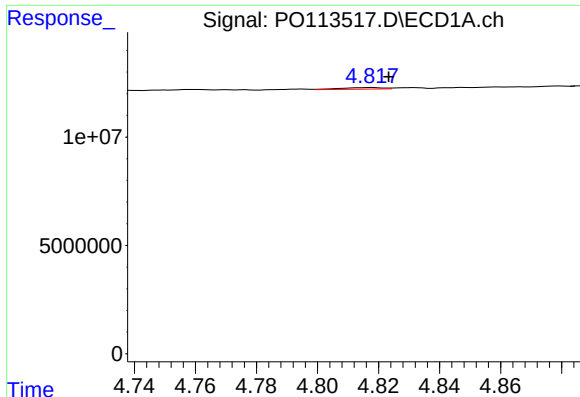

#5 AR-1016-3


R.T.: 4.817 min
Delta R.T.: -0.006 min
Response: 736093
Conc: 2.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

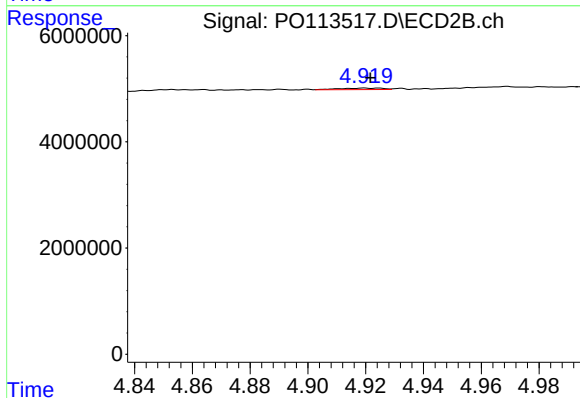


#5 AR-1016-3

R.T.: 4.920 min
Delta R.T.: -0.002 min
Response: 317216
Conc: 2.27 ng/ml

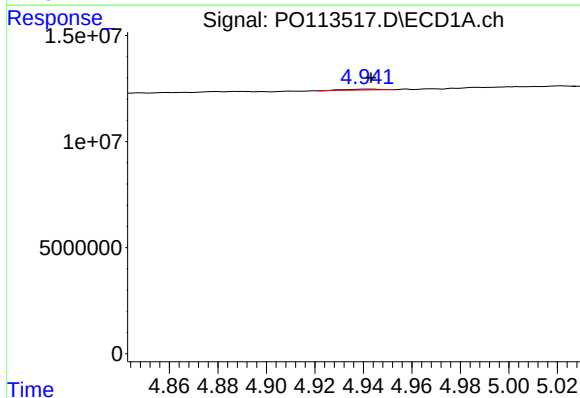


#6 AR-1016-4

R.T.: 4.941 min
Delta R.T.: -0.002 min
Response: 416913
Conc: 1.91 ng/ml

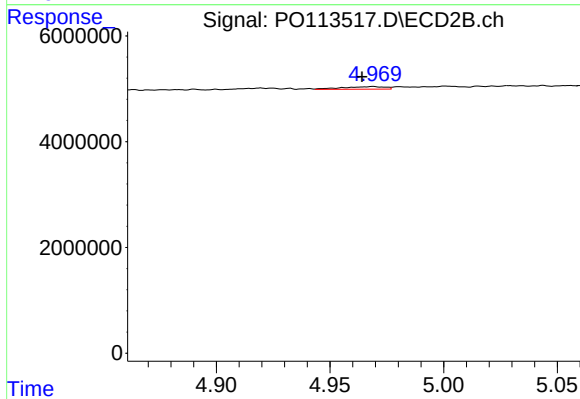

#6 AR-1016-4


R.T.: 4.969 min
Delta R.T.: 0.005 min
Response: 627449
Conc: 5.38 ng/ml

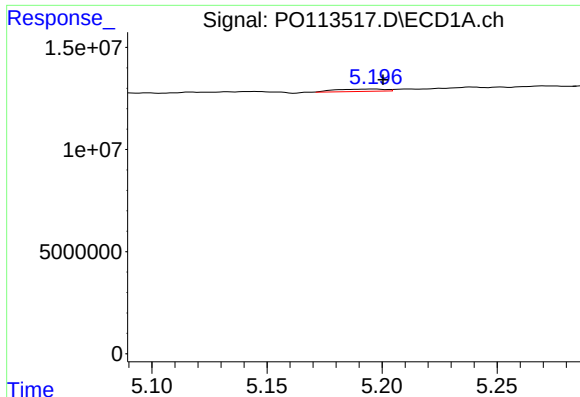

#7 AR-1016-5


R.T.: 5.197 min
Delta R.T.: -0.004 min
Response: 1741820
Conc: 7.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

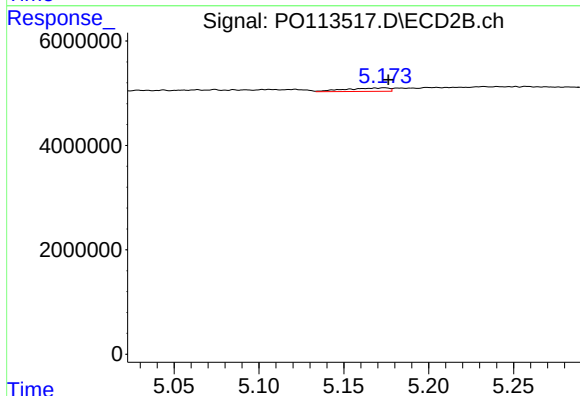


#7 AR-1016-5

R.T.: 5.174 min
Delta R.T.: -0.002 min
Response: 1169236
Conc: 8.20 ng/ml

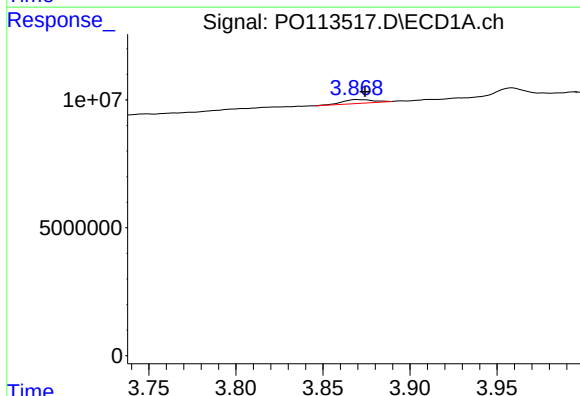


#8 AR-1221-1

R.T.: 3.870 min
Delta R.T.: -0.005 min
Response: 1848855
Conc: 19.76 ng/ml

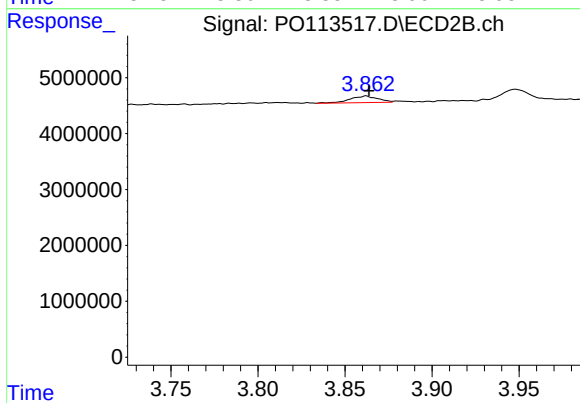

#8 AR-1221-1


R.T.: 3.862 min
Delta R.T.: -0.002 min
Response: 1309666
Conc: 20.75 ng/ml

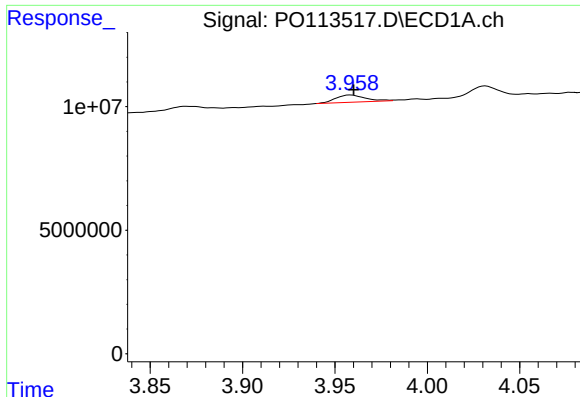

#9 AR-1221-2


R.T.: 3.959 min
Delta R.T.: -0.002 min
Response: 3255986
Conc: 48.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

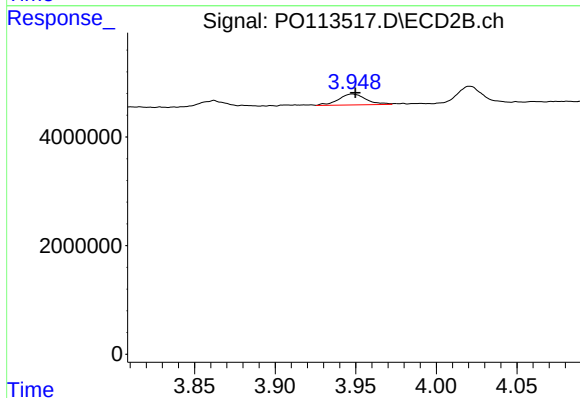


#9 AR-1221-2

R.T.: 3.948 min
Delta R.T.: -0.002 min
Response: 2391862
Conc: 51.25 ng/ml

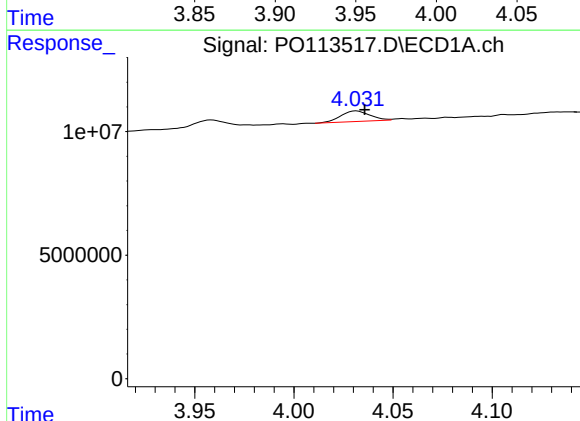


#10 AR-1221-3

R.T.: 4.032 min
Delta R.T.: -0.004 min
Response: 4413129
Conc: 19.94 ng/ml

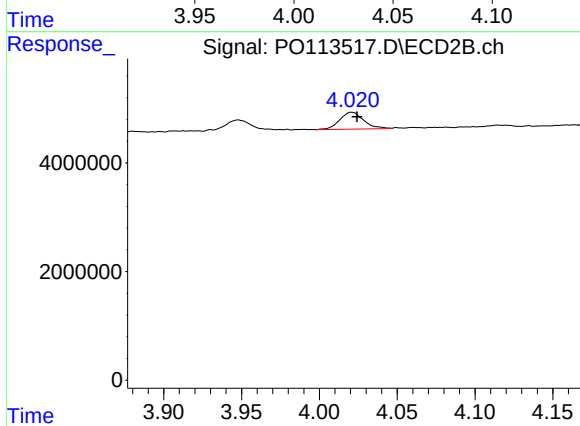

#10 AR-1221-3


R.T.: 4.021 min
Delta R.T.: -0.003 min
Response: 3352734
Conc: 22.58 ng/ml

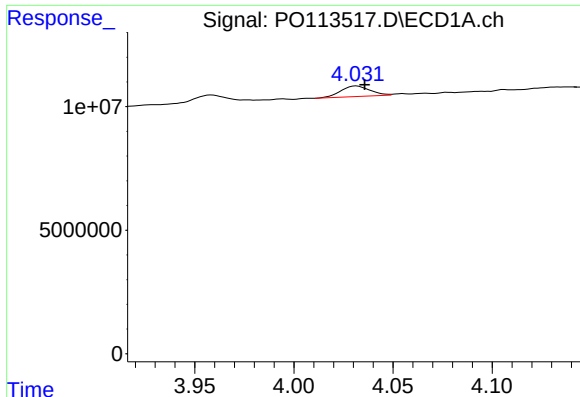

#11 AR-1232-1


R.T.: 4.032 min
Delta R.T.: -0.004 min
Response: 4413129
Conc: 25.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

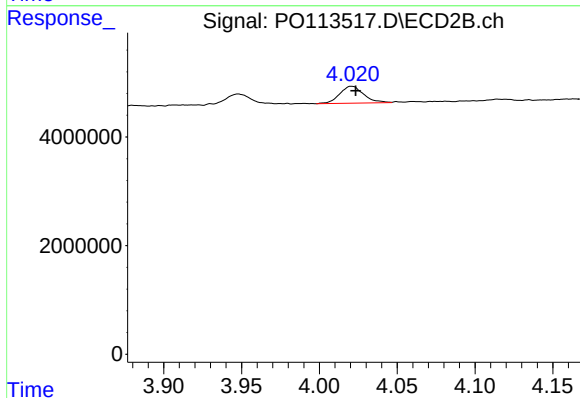


#11 AR-1232-1

R.T.: 4.021 min
Delta R.T.: -0.003 min
Response: 3352734
Conc: 28.56 ng/ml

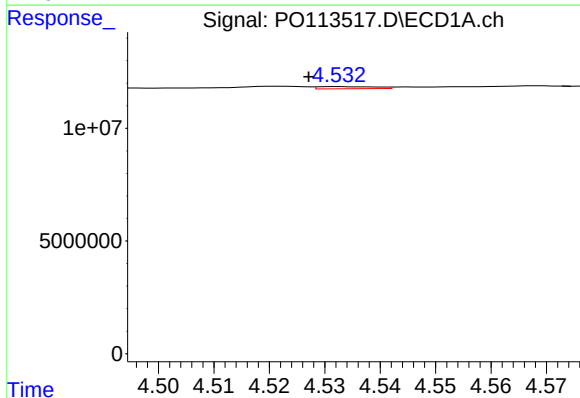


#12 AR-1232-2

R.T.: 4.532 min
Delta R.T.: 0.005 min
Response: 695194
Conc: 6.96 ng/ml

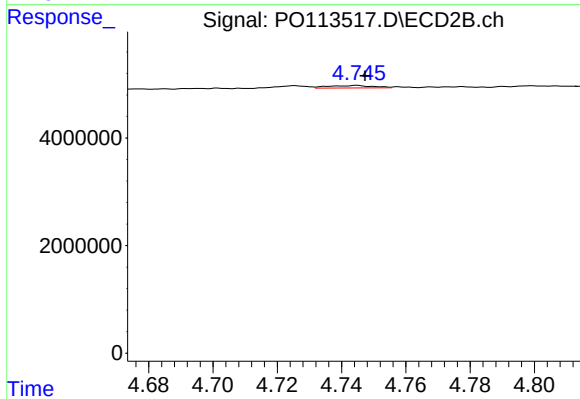

#12 AR-1232-2


R.T.: 4.745 min
Delta R.T.: -0.002 min
Response: 451470
Conc: 3.68 ng/ml

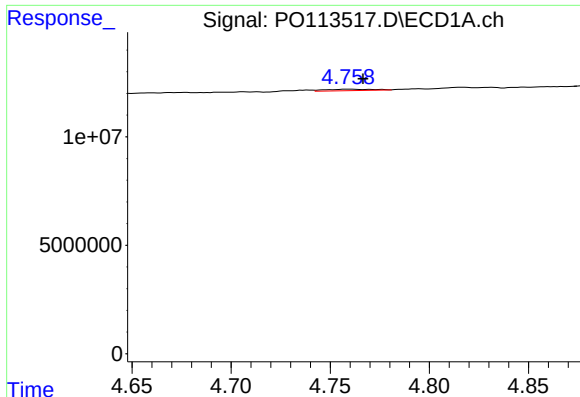

#13 AR-1232-3


R.T.: 4.759 min
Delta R.T.: -0.008 min
Response: 1122038
Conc: 5.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

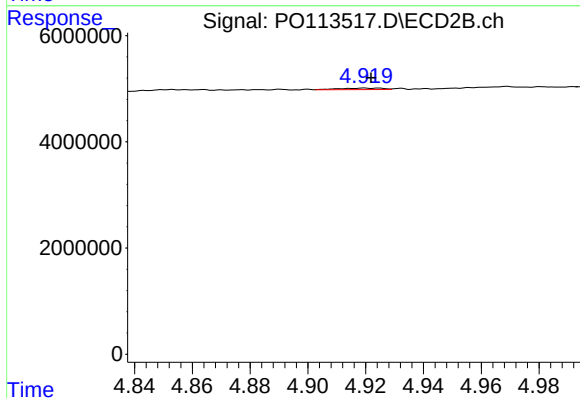


#13 AR-1232-3

R.T.: 4.920 min
Delta R.T.: -0.002 min
Response: 317216
Conc: 5.01 ng/ml

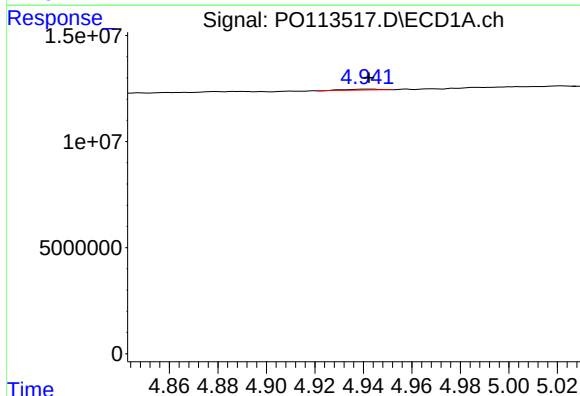


#14 AR-1232-4

R.T.: 4.941 min
Delta R.T.: 0.000 min
Response: 416913
Conc: 4.43 ng/ml

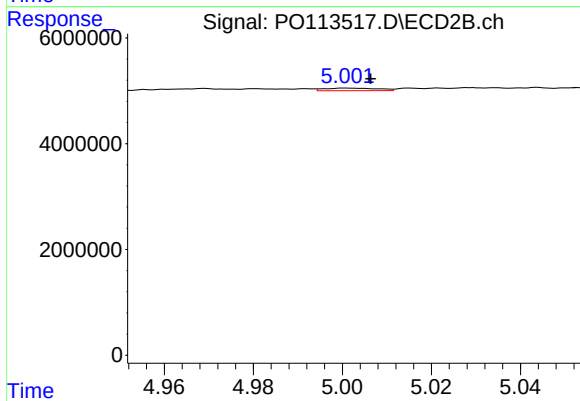

#14 AR-1232-4


R.T.: 5.001 min
Delta R.T.: -0.006 min
Response: 419152
Conc: 7.46 ng/ml

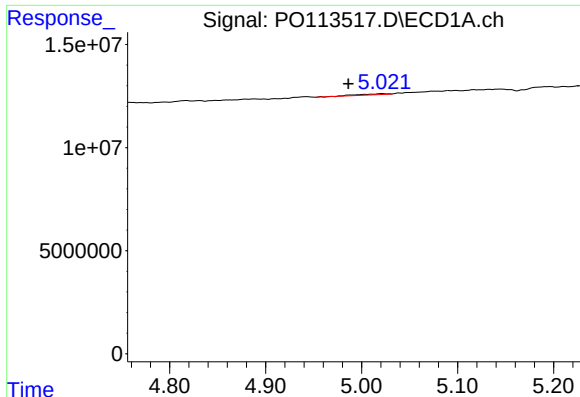

#15 AR-1232-5


R.T.: 5.022 min
Delta R.T.: 0.036 min
Response: 1103176
Conc: 17.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

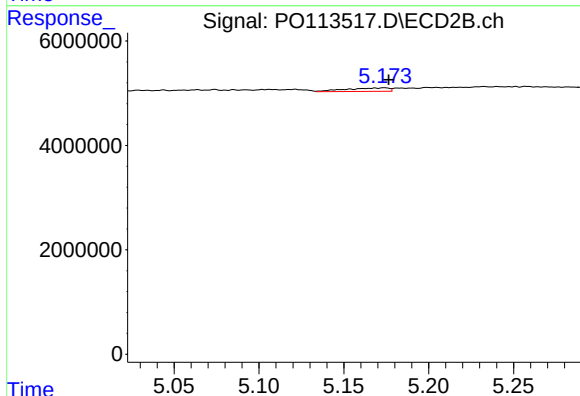


#15 AR-1232-5

R.T.: 5.174 min
Delta R.T.: -0.003 min
Response: 1169236
Conc: 19.53 ng/ml

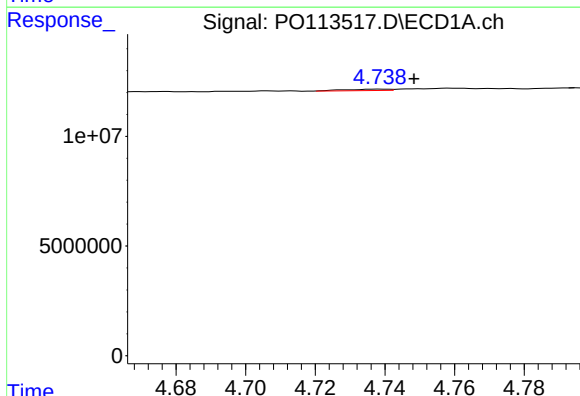


#16 AR-1242-1

R.T.: 4.739 min
Delta R.T.: -0.010 min
Response: 539036
Conc: 2.34 ng/ml

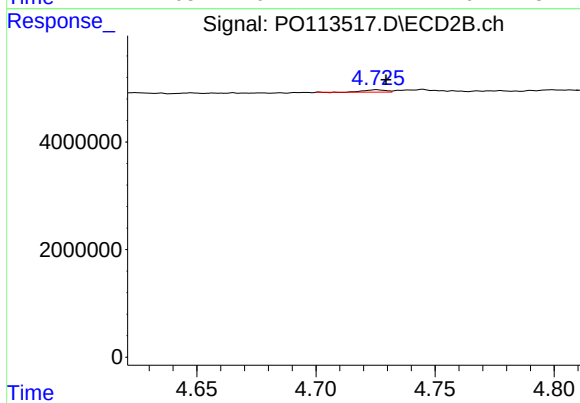

#16 AR-1242-1


R.T.: 4.725 min
Delta R.T.: -0.004 min
Response: 278088
Conc: 1.92 ng/ml

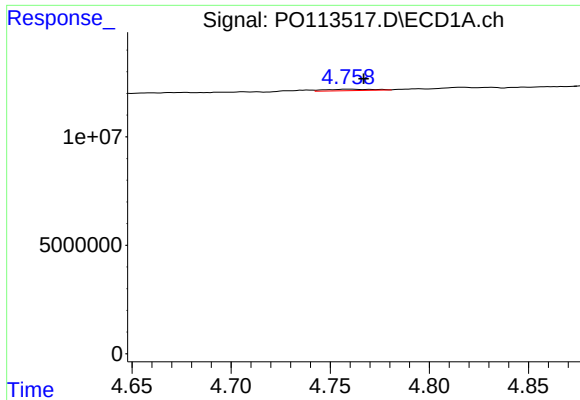

#17 AR-1242-2


R.T.: 4.759 min
Delta R.T.: -0.008 min
Response: 1122038
Conc: 3.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

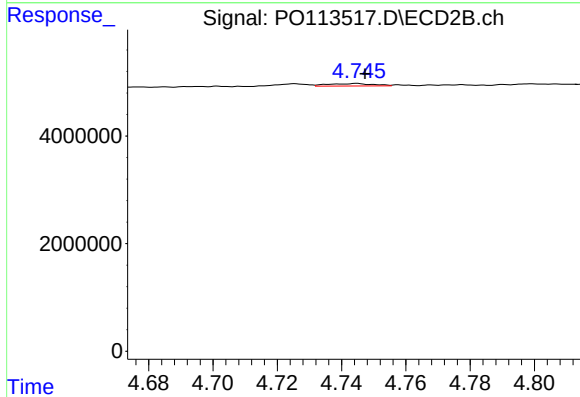


#17 AR-1242-2

R.T.: 4.745 min
Delta R.T.: -0.002 min
Response: 451470
Conc: 2.08 ng/ml

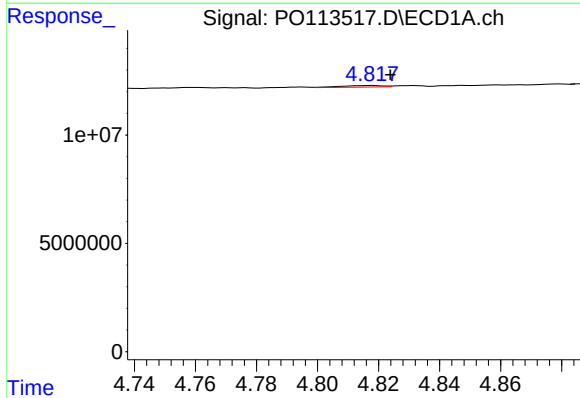


#18 AR-1242-3

R.T.: 4.817 min
Delta R.T.: -0.006 min
Response: 736093
Conc: 3.32 ng/ml

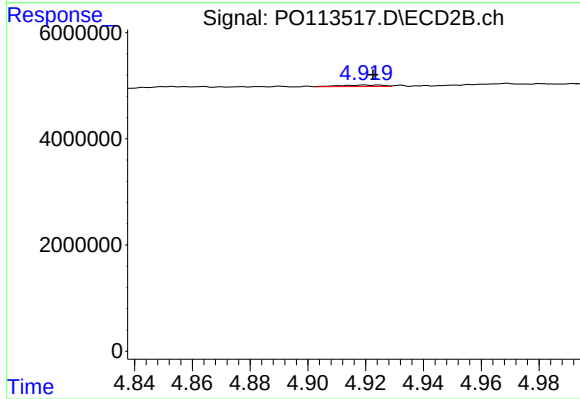

#18 AR-1242-3


R.T.: 4.920 min
Delta R.T.: -0.003 min
Response: 317216
Conc: 2.71 ng/ml

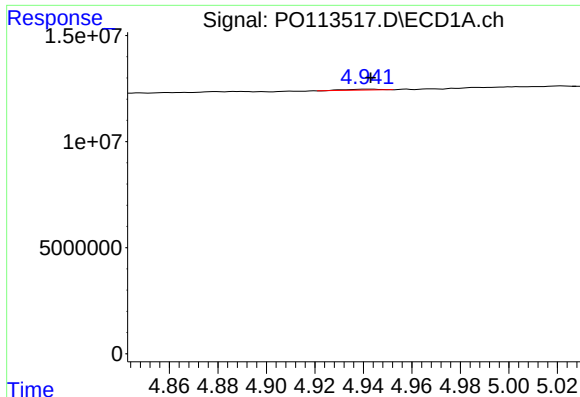

#19 AR-1242-4


R.T.: 4.941 min
Delta R.T.: -0.002 min
Response: 416913
Conc: 2.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

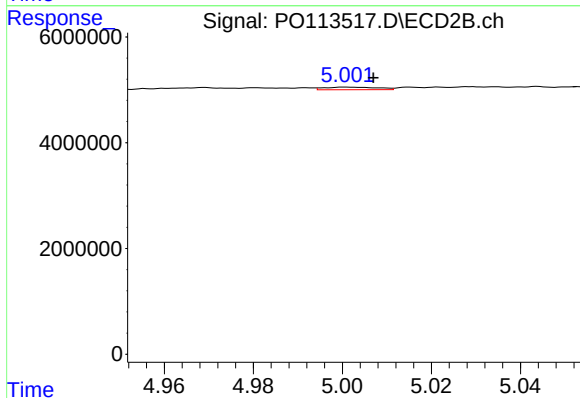


#19 AR-1242-4

R.T.: 5.001 min
Delta R.T.: -0.006 min
Response: 419152
Conc: 3.56 ng/ml

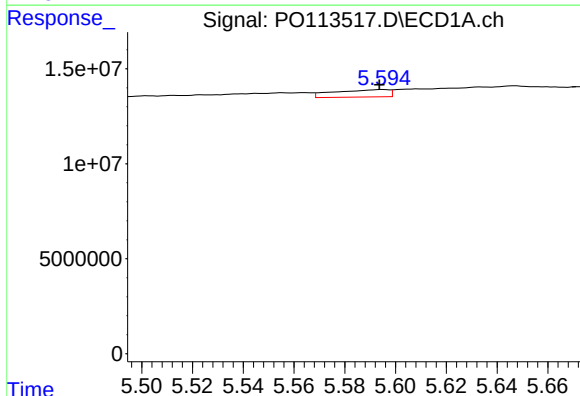


#20 AR-1242-5

R.T.: 5.595 min
Delta R.T.: 0.001 min
Response: 5700674
Conc: 28.48 ng/ml

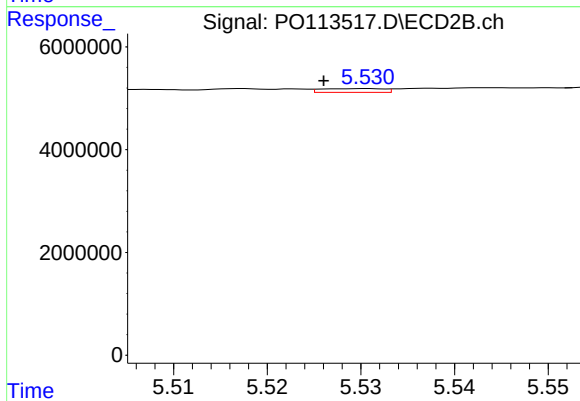

#20 AR-1242-5


R.T.: 5.531 min
Delta R.T.: 0.005 min
Response: 339006
Conc: 2.27 ng/ml

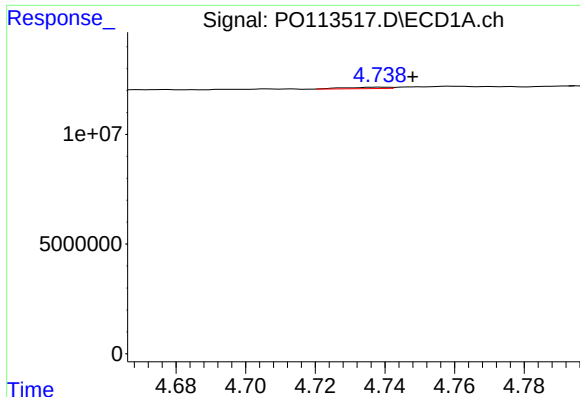

#21 AR-1248-1


R.T.: 4.739 min
Delta R.T.: -0.009 min
Response: 539036
Conc: 3.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

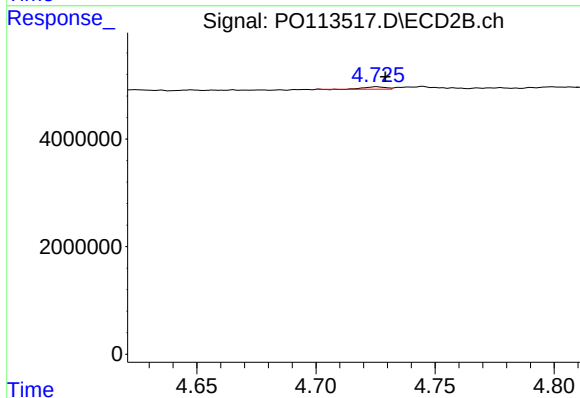


#21 AR-1248-1

R.T.: 4.725 min
Delta R.T.: -0.004 min
Response: 278088
Conc: 2.49 ng/ml

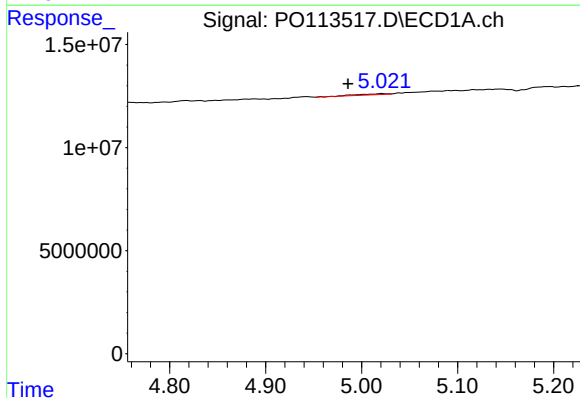


#22 AR-1248-2

R.T.: 5.022 min
Delta R.T.: 0.036 min
Response: 1103176
Conc: 4.56 ng/ml

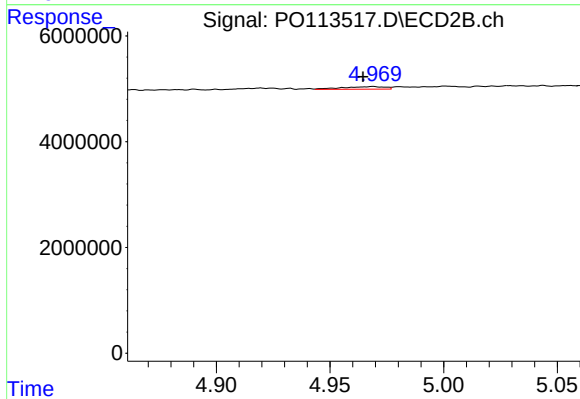

#22 AR-1248-2


R.T.: 4.969 min
Delta R.T.: 0.004 min
Response: 627449
Conc: 3.90 ng/ml

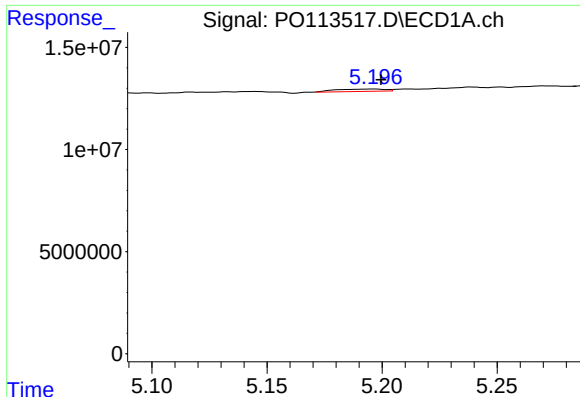

#23 AR-1248-3


R.T.: 5.197 min
Delta R.T.: -0.003 min
Response: 1741820
Conc: 5.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

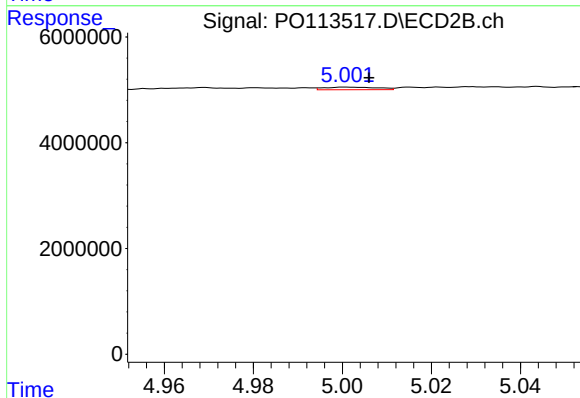


#23 AR-1248-3

R.T.: 5.001 min
Delta R.T.: -0.005 min
Response: 419152
Conc: 2.47 ng/ml

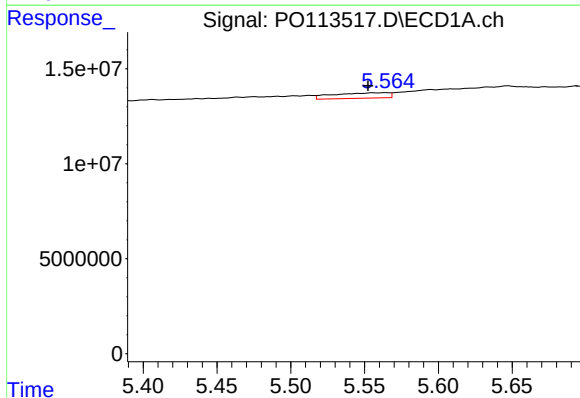


#24 AR-1248-4

R.T.: 5.565 min
Delta R.T.: 0.012 min
Response: 7388992
Conc: 14.79 ng/ml

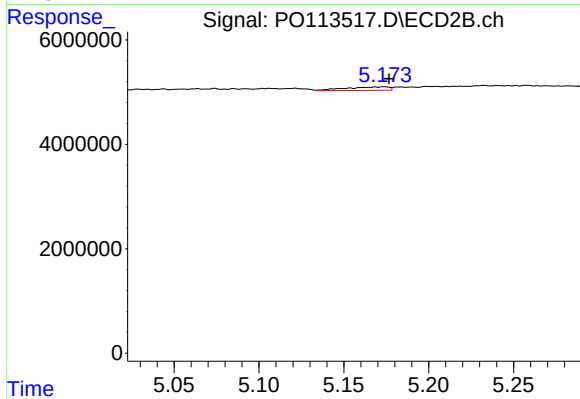

#24 AR-1248-4


R.T.: 5.174 min
Delta R.T.: -0.003 min
Response: 1169236
Conc: 5.87 ng/ml

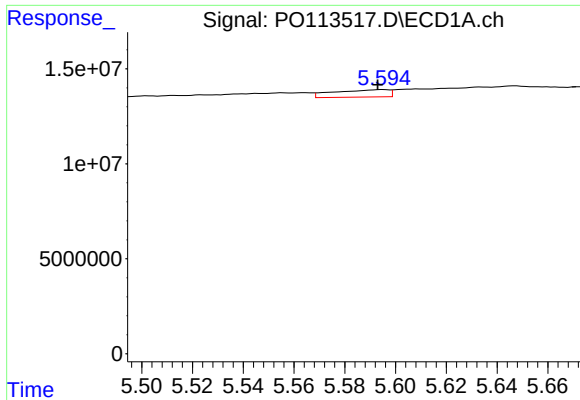

#25 AR-1248-5


R.T.: 5.595 min
Delta R.T.: 0.002 min
Response: 5700674
Conc: 16.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

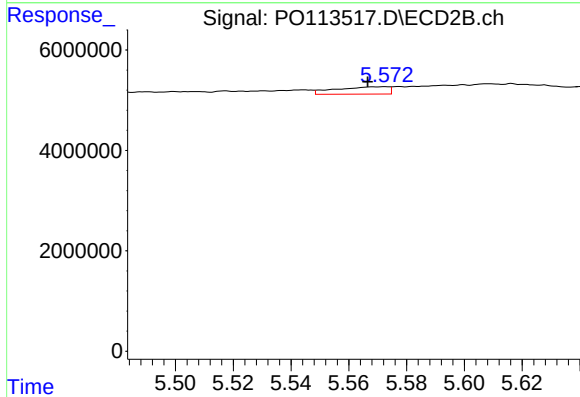


#25 AR-1248-5

R.T.: 5.573 min
Delta R.T.: 0.006 min
Response: 1846701
Conc: 8.70 ng/ml

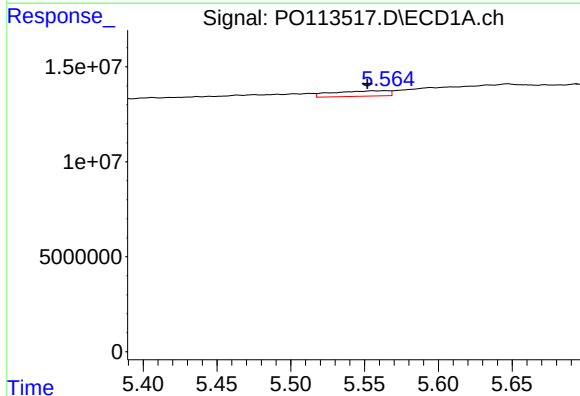


#26 AR-1254-1

R.T.: 5.565 min
Delta R.T.: 0.013 min
Response: 7388992
Conc: 13.68 ng/ml

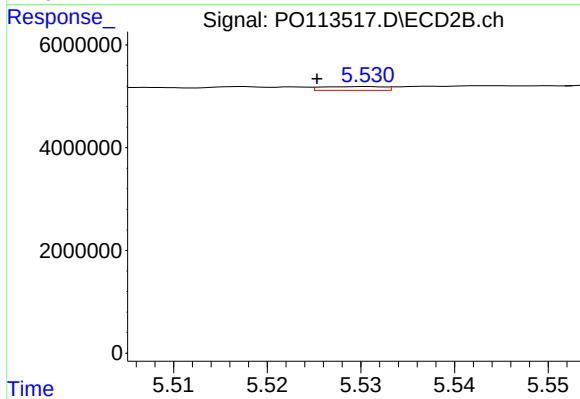

#26 AR-1254-1


R.T.: 5.531 min
Delta R.T.: 0.005 min
Response: 339006
Conc: 1.08 ng/ml

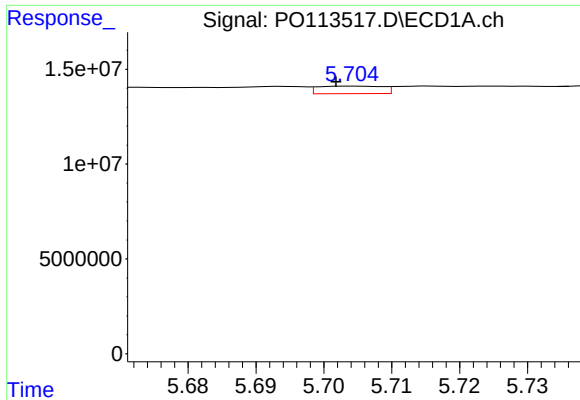

#27 AR-1254-2


R.T.: 5.704 min
Delta R.T.: 0.003 min
Response: 2616946
Conc: 5.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

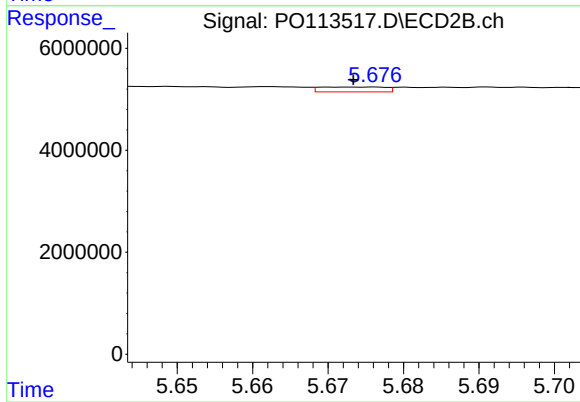


#27 AR-1254-2

R.T.: 5.676 min
Delta R.T.: 0.003 min
Response: 569328
Conc: 2.03 ng/ml

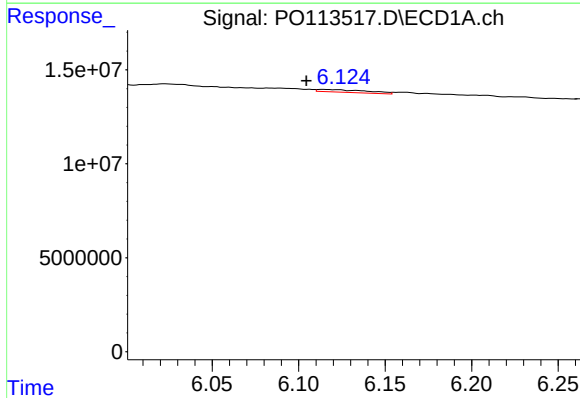


#28 AR-1254-3

R.T.: 6.115 min
Delta R.T.: 0.010 min
Response: 2843506
Conc: 3.85 ng/ml

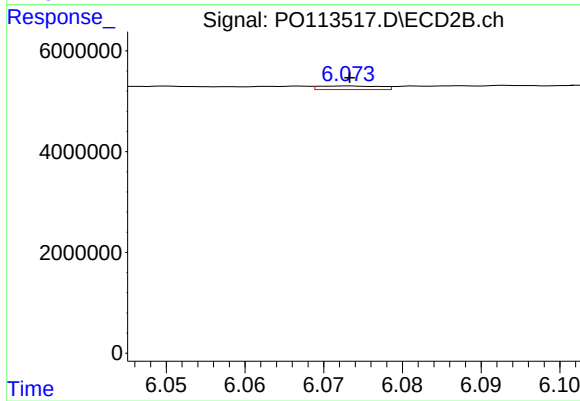

#28 AR-1254-3


R.T.: 6.073 min
Delta R.T.: 0.000 min
Response: 385881
Conc: 0.93 ng/ml

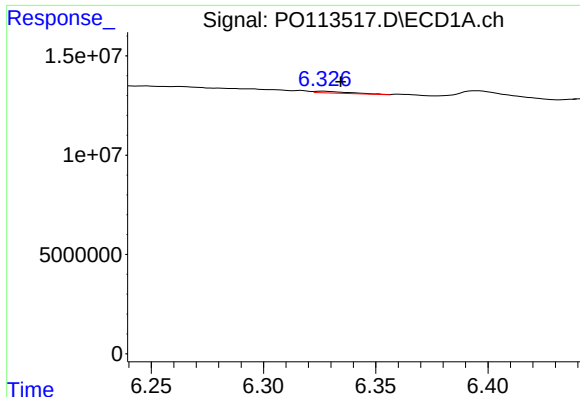

#29 AR-1254-4


R.T.: 6.326 min
Delta R.T.: -0.008 min
Response: 1009926
Conc: 1.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

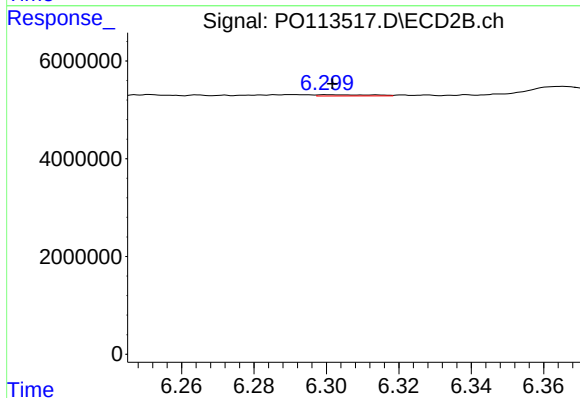


#29 AR-1254-4

R.T.: 6.300 min
Delta R.T.: -0.001 min
Response: 264444
Conc: 0.96 ng/ml

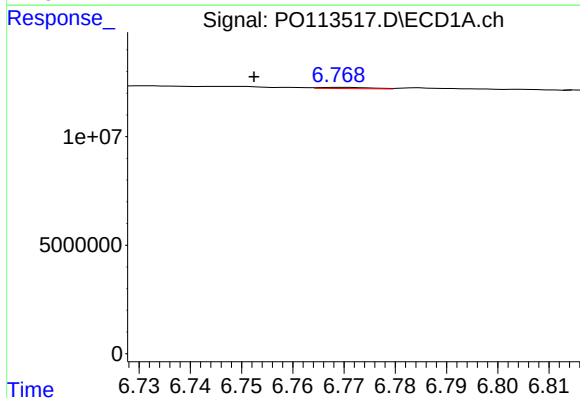


#30 AR-1254-5

R.T.: 6.769 min
Delta R.T.: 0.017 min
Response: 386232
Conc: 0.55 ng/ml

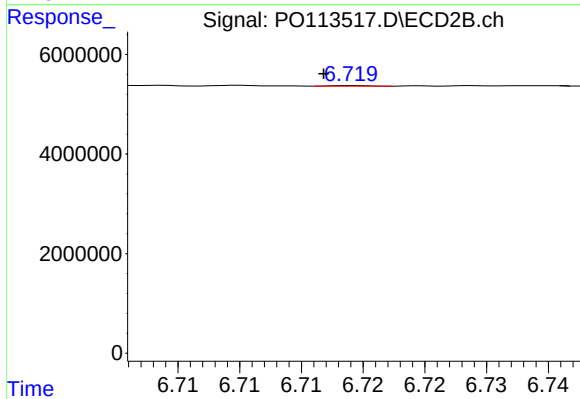

#30 AR-1254-5


R.T.: 6.719 min
Delta R.T.: 0.002 min
Response: 29107
Conc: 0.08 ng/ml

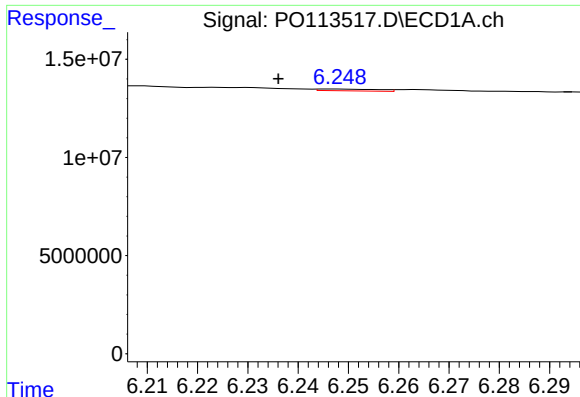

#31 AR-1260-1


R.T.: 6.247 min
Delta R.T.: 0.011 min
Response: 762369
Conc: 1.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

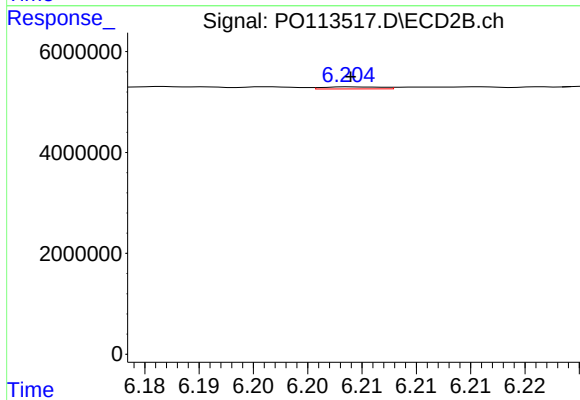


#31 AR-1260-1

R.T.: 6.204 min
Delta R.T.: 0.000 min
Response: 148246
Conc: 0.58 ng/ml

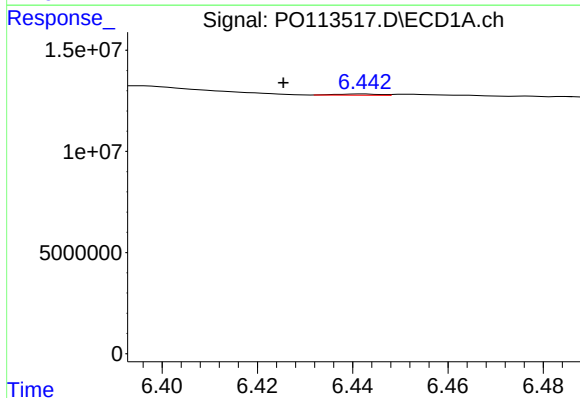


#32 AR-1260-2

R.T.: 6.442 min
Delta R.T.: 0.017 min
Response: 368739
Conc: 0.54 ng/ml

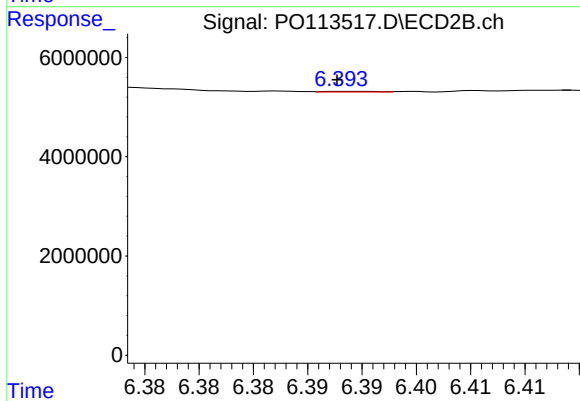

#32 AR-1260-2


R.T.: 6.394 min
Delta R.T.: 0.000 min
Response: 46633
Conc: 0.13 ng/ml

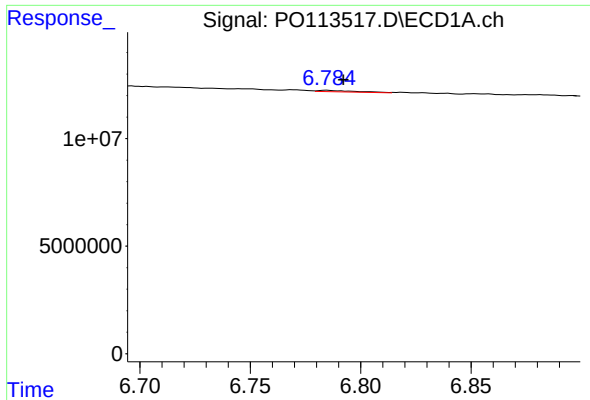

#33 AR-1260-3


R.T.: 6.785 min
Delta R.T.: -0.008 min
Response: 743518
Conc: 1.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

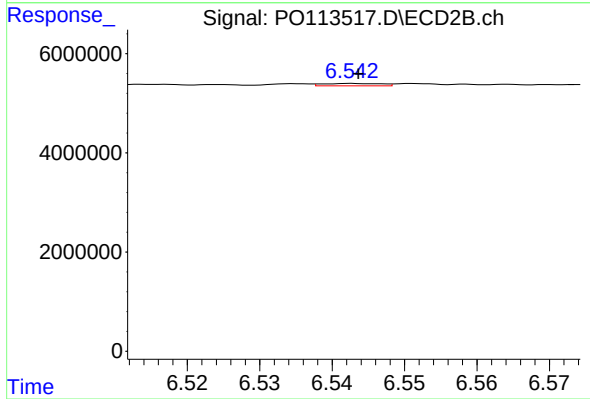


#33 AR-1260-3

R.T.: 6.543 min
Delta R.T.: 0.000 min
Response: 277544
Conc: 0.93 ng/ml

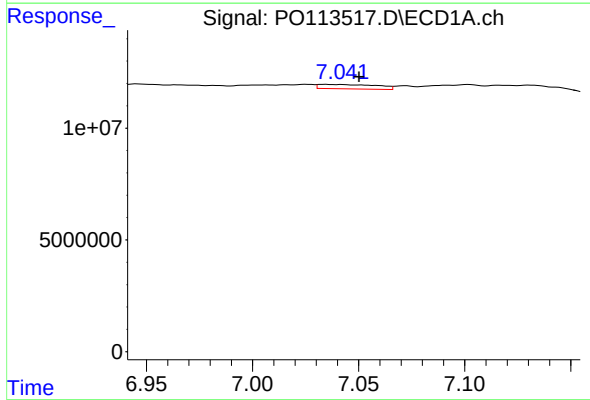


#34 AR-1260-4

R.T.: 7.034 min
Delta R.T.: -0.016 min
Response: 3707488
Conc: 8.28 ng/ml

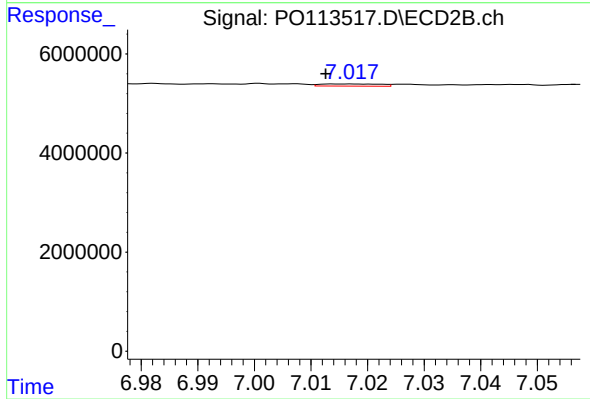

#34 AR-1260-4


R.T.: 7.014 min
Delta R.T.: 0.002 min
Response: 316957
Conc: 1.53 ng/ml

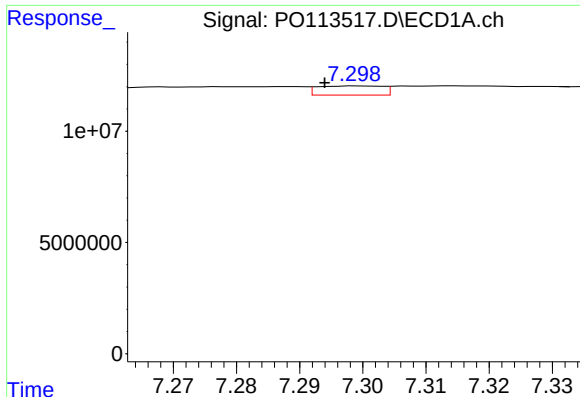

#35 AR-1260-5


R.T.: 7.299 min
Delta R.T.: 0.005 min
Response: 2925361
Conc: 2.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

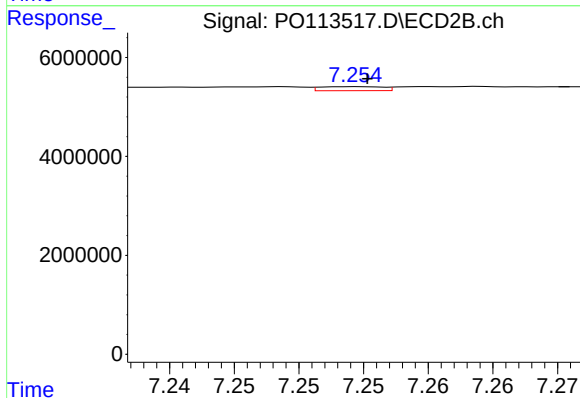


#35 AR-1260-5

R.T.: 7.254 min
Delta R.T.: 0.000 min
Response: 273602
Conc: 0.58 ng/ml

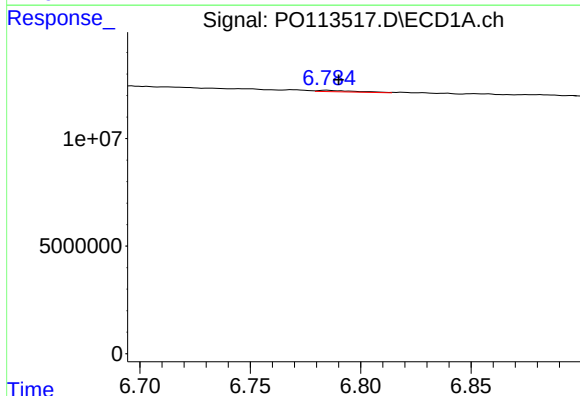


#36 AR-1262-1

R.T.: 6.785 min
Delta R.T.: -0.006 min
Response: 743518
Conc: 0.81 ng/ml

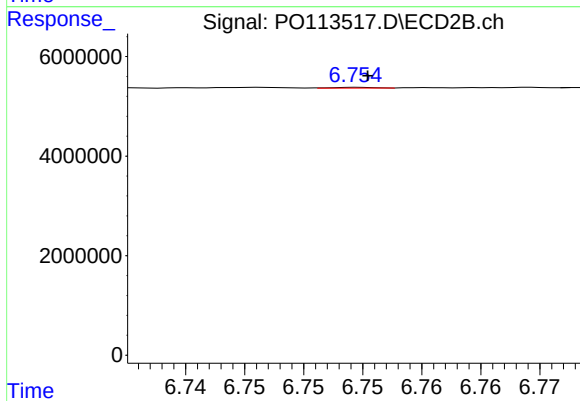

#36 AR-1262-1


R.T.: 6.755 min
Delta R.T.: 0.000 min
Response: 36160
Conc: 0.09 ng/ml

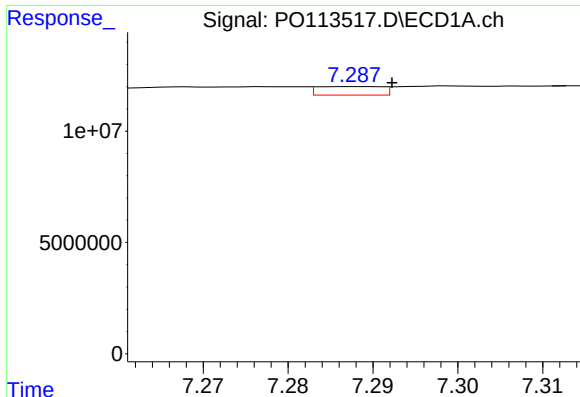

#37 AR-1262-2


R.T.: 7.288 min
Delta R.T.: -0.004 min
Response: 2034253
Conc: 1.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

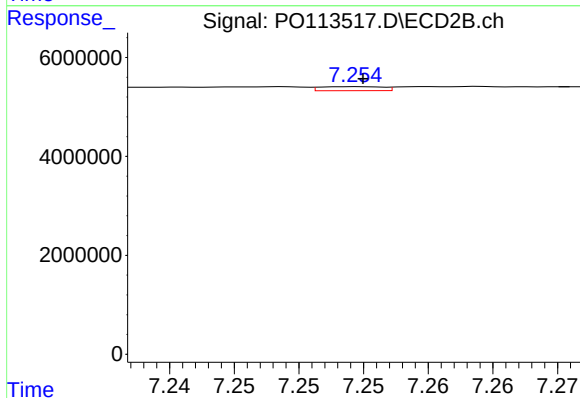


#37 AR-1262-2

R.T.: 7.254 min
Delta R.T.: 0.000 min
Response: 273602
Conc: 0.53 ng/ml

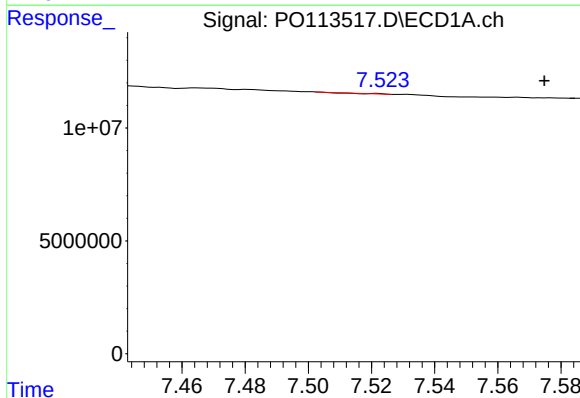


#38 AR-1262-3

R.T.: 7.522 min
Delta R.T.: -0.053 min
Response: 4468
Conc: 0.01 ng/ml

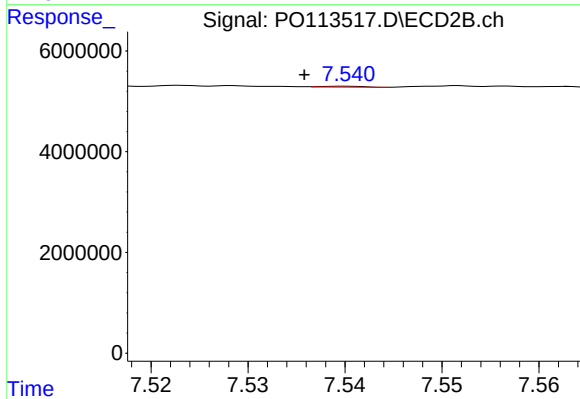

#38 AR-1262-3


R.T.: 7.540 min
Delta R.T.: 0.005 min
Response: 53322
Conc: 0.30 ng/ml

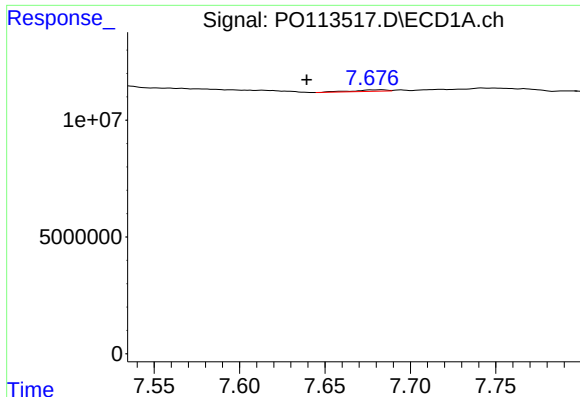

#39 AR-1262-4


R.T.: 7.683 min
Delta R.T.: 0.044 min
Response: 914744
Conc: 0.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

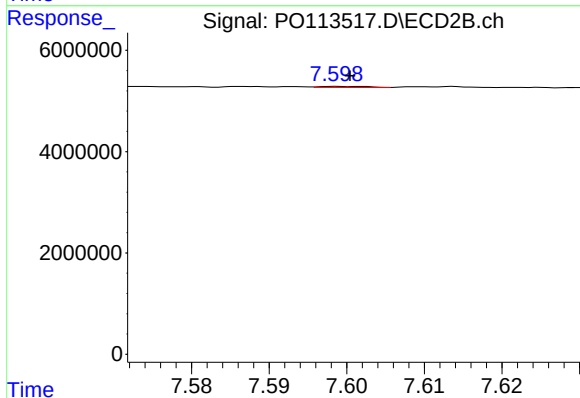


#39 AR-1262-4

R.T.: 7.599 min
Delta R.T.: -0.002 min
Response: 97953
Conc: 0.34 ng/ml

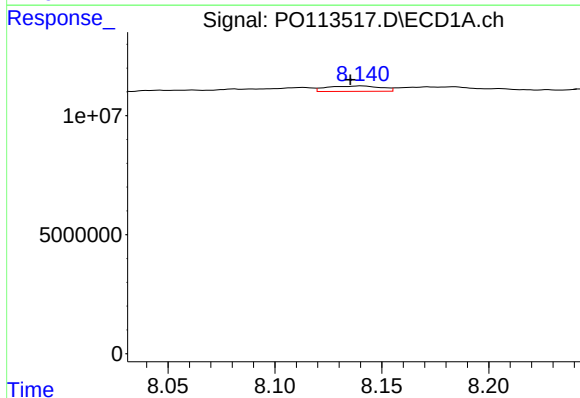


#40 AR-1262-5

R.T.: 8.141 min
Delta R.T.: 0.006 min
Response: 3987946
Conc: 9.57 ng/ml

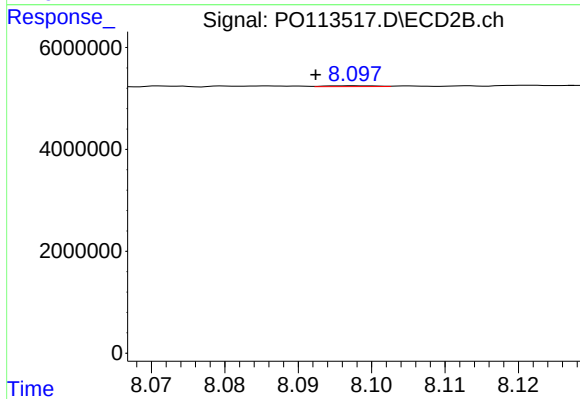

#40 AR-1262-5


R.T.: 8.097 min
Delta R.T.: 0.005 min
Response: 71817
Conc: 0.66 ng/ml

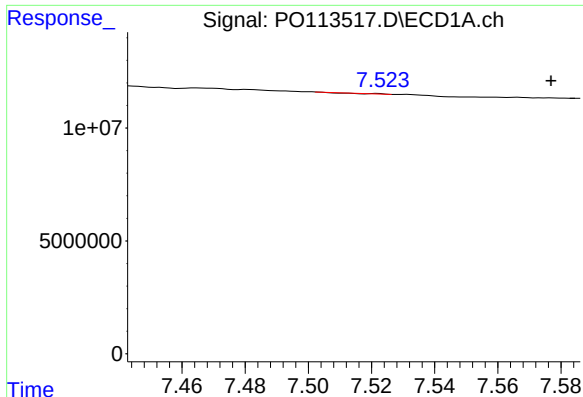

#41 AR-1268-1


R.T.: 7.522 min
Delta R.T.: -0.055 min
Response: 4468
Conc: 0.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

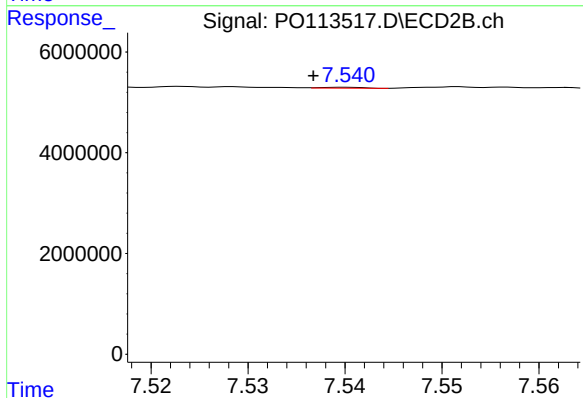


#41 AR-1268-1

R.T.: 7.540 min
Delta R.T.: 0.004 min
Response: 53322
Conc: 0.10 ng/ml

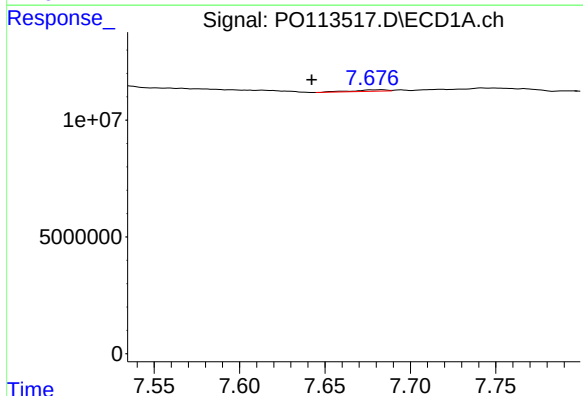


#42 AR-1268-2

R.T.: 7.683 min
Delta R.T.: 0.041 min
Response: 914744
Conc: 0.63 ng/ml

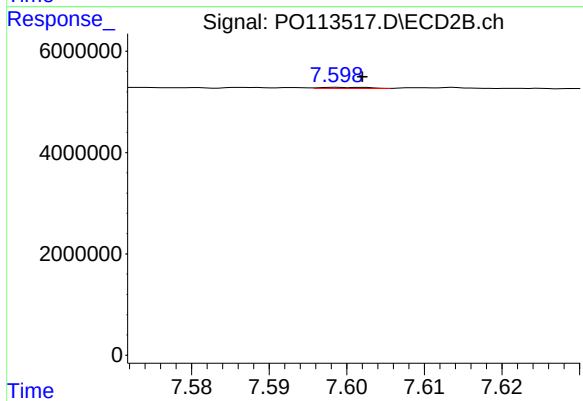

#42 AR-1268-2


R.T.: 7.599 min
Delta R.T.: -0.003 min
Response: 97953
Conc: 0.24 ng/ml

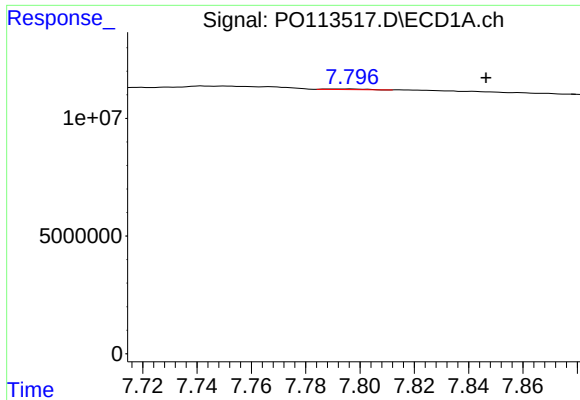

#43 AR-1268-3


R.T.: 7.796 min
Delta R.T.: -0.051 min
Response: 266270
Conc: 0.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

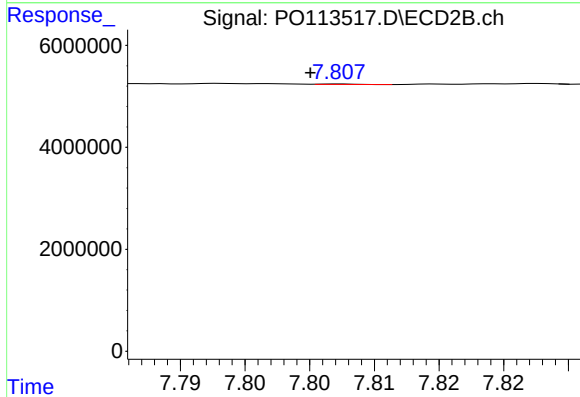


#43 AR-1268-3

R.T.: 7.807 min
Delta R.T.: 0.002 min
Response: 17667
Conc: 0.05 ng/ml

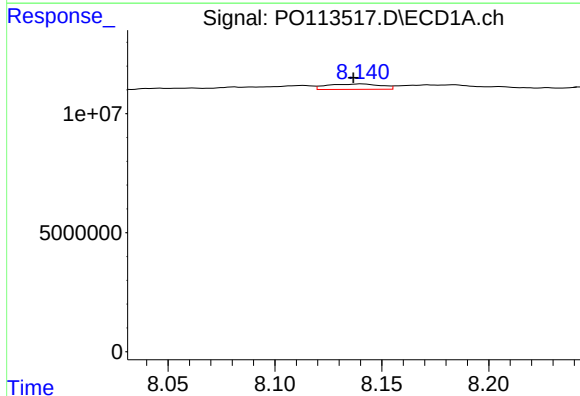


#44 AR-1268-4

R.T.: 8.141 min
Delta R.T.: 0.004 min
Response: 3987946
Conc: 8.66 ng/ml

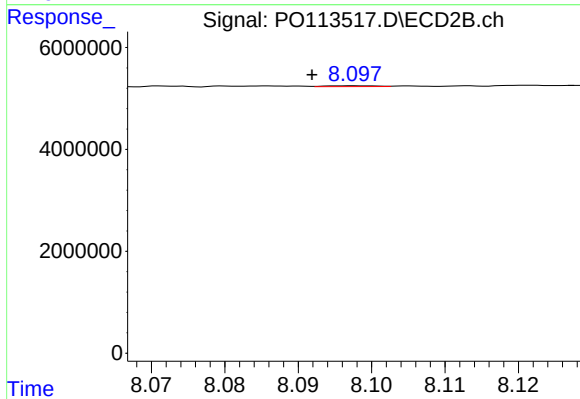

#44 AR-1268-4


R.T.: 8.097 min
Delta R.T.: 0.006 min
Response: 71817
Conc: 0.60 ng/ml

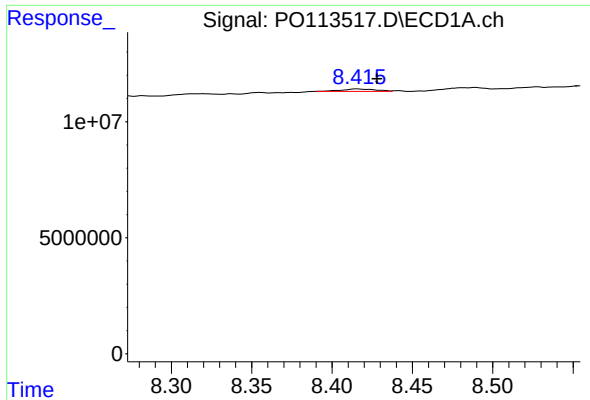

#45 AR-1268-5

R.T.: 8.416 min
Delta R.T.: -0.013 min
Response: 1532744
Conc: 0.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

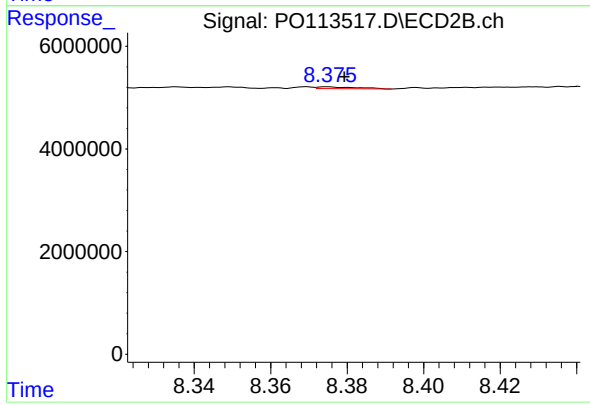

#45 AR-1268-5

R.T.: 8.375 min
Delta R.T.: -0.004 min
Response: 263022
Conc: 0.34 ng/ml