

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090525\
 Data File : P0113518.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 18:52
 Operator : YP/AJ
 Sample : Q2893-09
 Misc : AR1232 WATER LOD 25PPB
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:35:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.659	3.652	169.1E6	100.9E6	20.650	19.941
2)	SA Decachlor...	8.673	8.620	100.6E6	35067498	14.514	18.507 #
Target Compounds							
3)	L1 AR-1016-1	4.743	4.724	2548411	1842408	9.545	10.801
4)	L1 AR-1016-2	4.760	4.742	4481857	3106074	11.165	12.055
5)	L1 AR-1016-3	4.818	4.916	3944127	1225814	15.466	8.780 #
6)	L1 AR-1016-4	4.936	4.961	1945764	1423025	8.923	12.194 #
7)	L1 AR-1016-5	5.194	5.172	3608222	2686943	16.281	18.852
8)	L2 AR-1221-1	3.873	3.860	1114237	1097590	11.908	17.389 #
9)	L2 AR-1221-2	3.959	3.948	2639735	2865228	39.078	61.389 #
10)	L2 AR-1221-3	4.032	4.020	3354793	2981139	15.156	20.078 #
11)	L3 AR-1232-1	4.032	4.020	3354793	2981139	19.280	25.392 #
12)	L3 AR-1232-2	4.522	4.742	3532473	3106074	35.377	25.346 #
13)	L3 AR-1232-3	4.760	4.916	4481857	1225814	23.654	19.351
14)	L3 AR-1232-4	4.936	5.002	1945764	1594719	20.662	28.365 #
15)	L3 AR-1232-5	4.983	5.172	1807337	2686943	29.177	44.884 #
16)	L4 AR-1242-1	4.743	4.724	2548411	1842408	11.083	12.750
17)	L4 AR-1242-2	4.760	4.742	4481857	3106074	13.043	14.320
18)	L4 AR-1242-3	4.818	4.916	3944127	1225814	17.776	10.480 #
19)	L4 AR-1242-4	4.936	5.002	1945764	1594719	11.217	13.556
20)	L4 AR-1242-5	5.589	5.520	2525099	2962226	12.615	19.863 #
21)	L5 AR-1248-1	4.743	4.724	2548411	1842408	14.607	16.522
22)	L5 AR-1248-2	4.983	4.961	1807337	1423025	7.472	8.855
23)	L5 AR-1248-3	5.194	5.002	3608222	1594719	11.316	9.399
24)	L5 AR-1248-4	5.546	5.172	1971303	2686943	3.946	13.487 #
25)	L5 AR-1248-5	5.589	5.564	2525099	4660045	7.394	21.951 #
26)	L6 AR-1254-1	5.546	5.520	1971303	2962226	3.651	9.393 #
27)	L6 AR-1254-2	5.707	5.668	349708	1908555	0.709	6.808 #
28)	L6 AR-1254-3	6.096	6.065	4488109	1488502	6.074	3.570 #
29)	L6 AR-1254-4	6.320	6.296	7331347	530431	13.162	1.930 #
30)	L6 AR-1254-5	6.743	6.713	1306120	190354	1.863	0.532 #
31)	L7 AR-1260-1	6.244	6.203	4105349	208297	9.205	0.817 #
32)	L7 AR-1260-2	6.448	6.410	-194992	254354	N.D.	0.736 #
33)	L7 AR-1260-3	6.813	6.543	155131	623364	0.251	2.096 #
34)	L7 AR-1260-4	7.045	7.014	1342628	610720	2.998	2.947
35)	L7 AR-1260-5	7.293	7.256	951522	472440	0.786	1.009 #
36)	L8 AR-1262-1	6.813	6.761	155131	168469	0.169	0.406 #
37)	L8 AR-1262-2	7.293	7.256	951522	472440	0.629	0.913 #
38)	L8 AR-1262-3	7.587	7.543	188634	40600	0.340	0.226 #
39)	L8 AR-1262-4	7.660	7.599	579176	271339	0.592	0.936 #
40)	L8 AR-1262-5	8.151	8.063	2464123	63508	5.911	0.586 #
41)	L9 AR-1268-1	7.587	7.543	188634	40600	0.110	0.080 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090525\
Data File : P0113518.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2025 18:52
Operator : YP/AJ
Sample : Q2893-09
Misc : AR1232 WATER LOD 25PPB
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 23:35:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	7.660	7.599	579176	271339	0.400	0.653 #
43)	L9 AR-1268-3	0.000	7.790	0	203995	N.D.	0.625 #
44)	L9 AR-1268-4	8.151	8.063	2464123	63508	5.349	0.527 #
45)	L9 AR-1268-5	8.425	8.361	584603	164230	0.183	0.210


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090525\
Data File : PO113518.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2025 18:52
Operator : YP/AJ
Sample : Q2893-09
Misc : AR1232 WATER LOD 25PPB
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 23:35:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

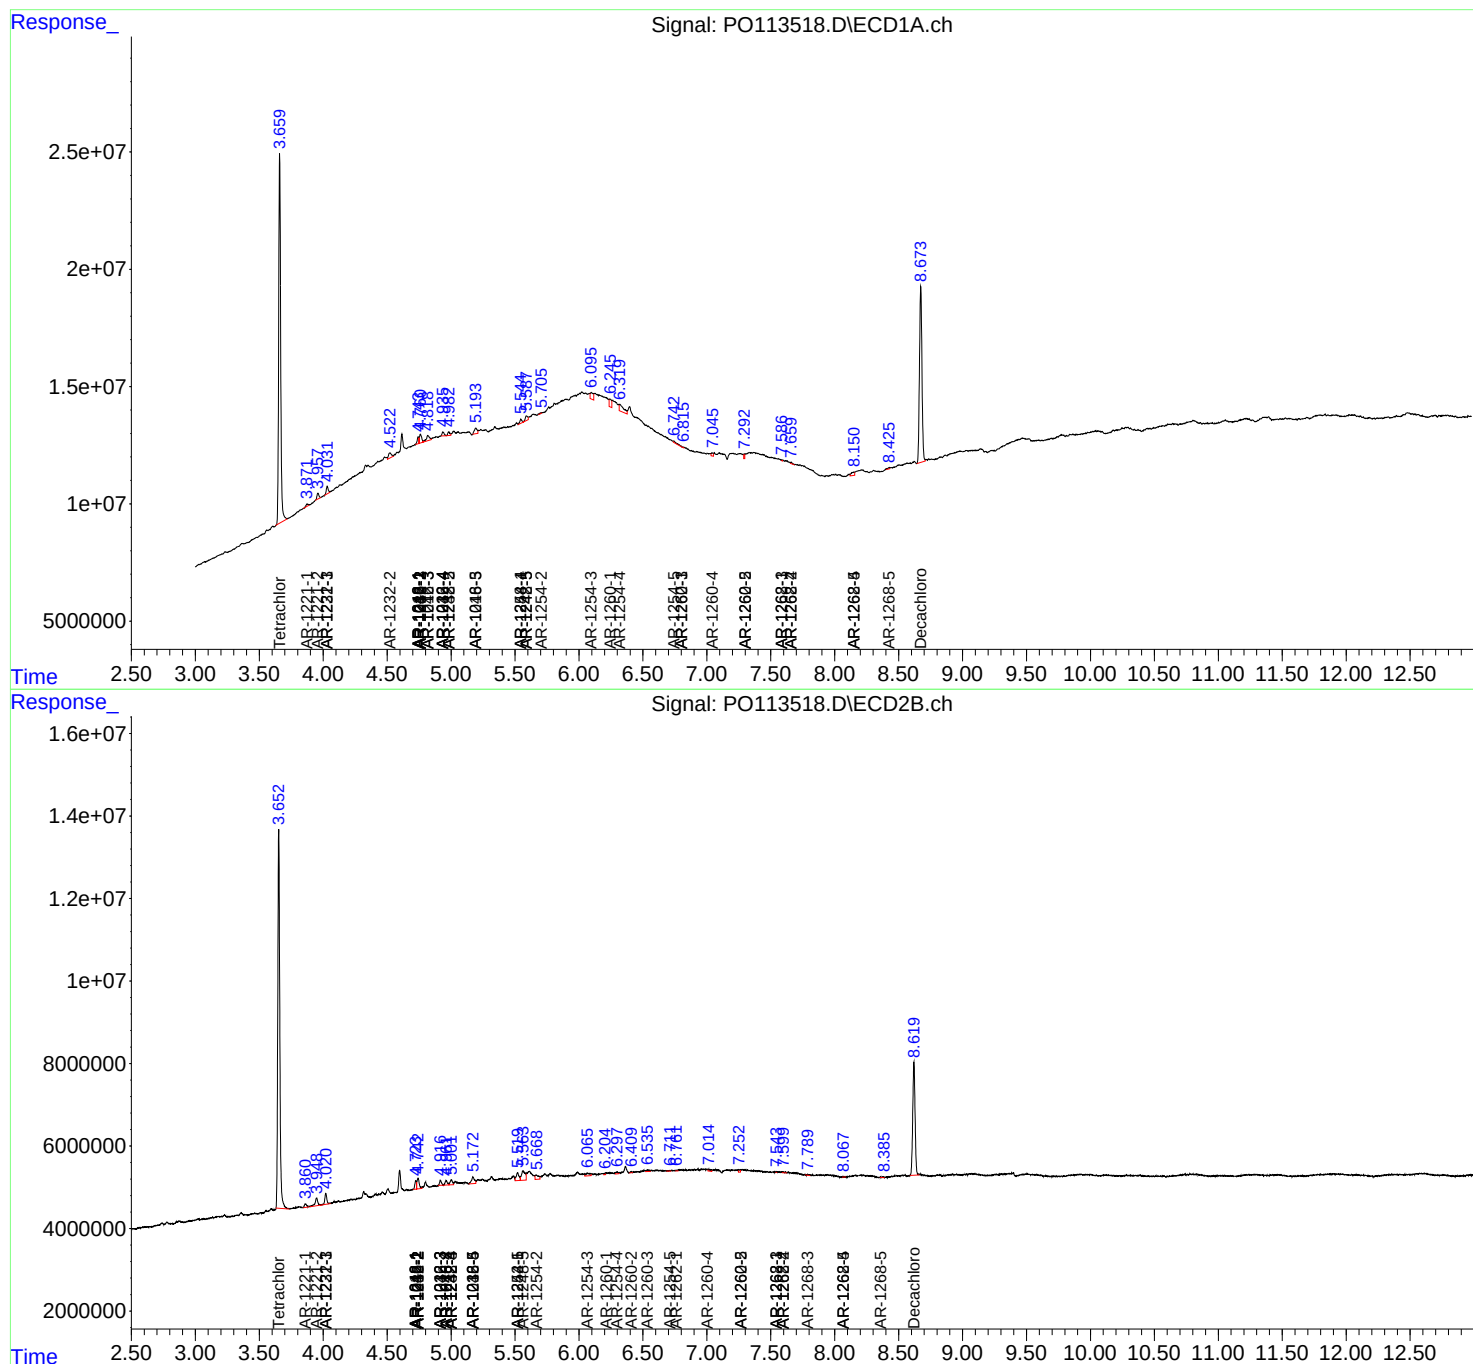


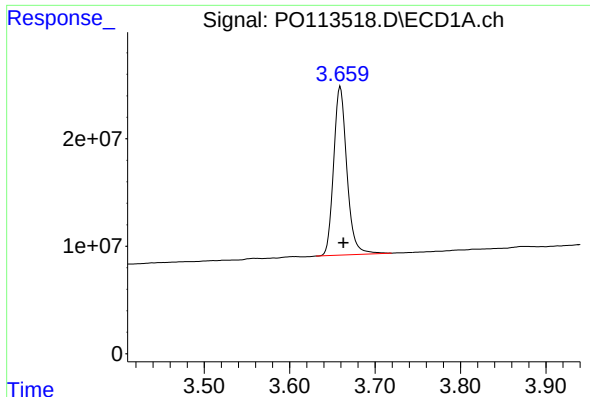

#1 Tetrachloro-m-xylene


R.T.: 3.659 min
Delta R.T.: -0.004 min
Response: 169056777
Conc: 20.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

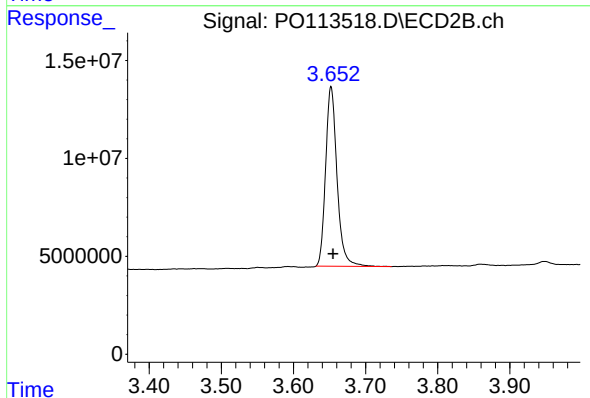


#1 Tetrachloro-m-xylene

R.T.: 3.652 min
Delta R.T.: -0.003 min
Response: 100912169
Conc: 19.94 ng/ml

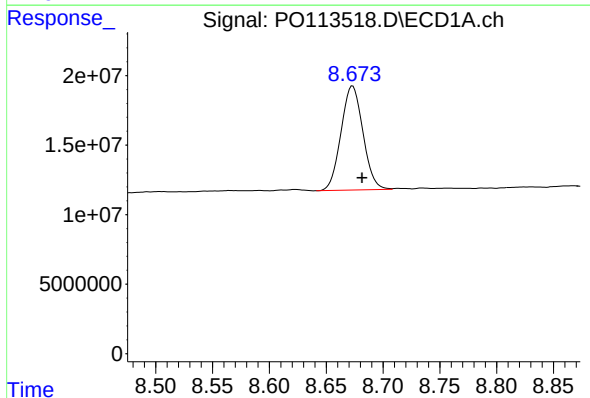


#2 Decachlorobiphenyl

R.T.: 8.673 min
Delta R.T.: -0.008 min
Response: 100605548
Conc: 14.51 ng/ml

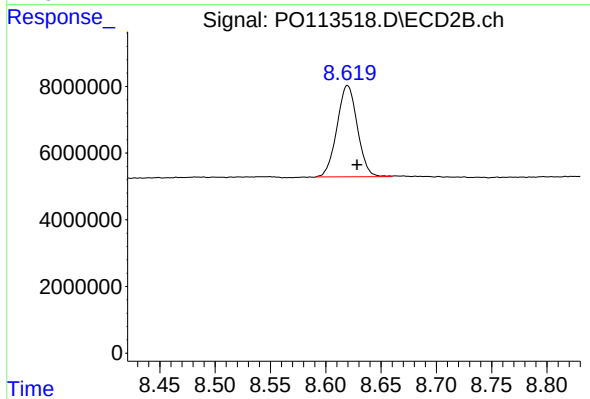

#2 Decachlorobiphenyl


R.T.: 8.620 min
Delta R.T.: -0.009 min
Response: 35067498
Conc: 18.51 ng/ml

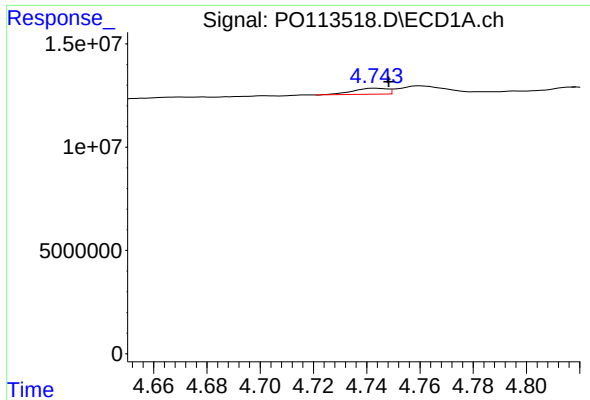

#3 AR-1016-1


R.T.: 4.743 min
Delta R.T.: -0.005 min
Response: 2548411
Conc: 9.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

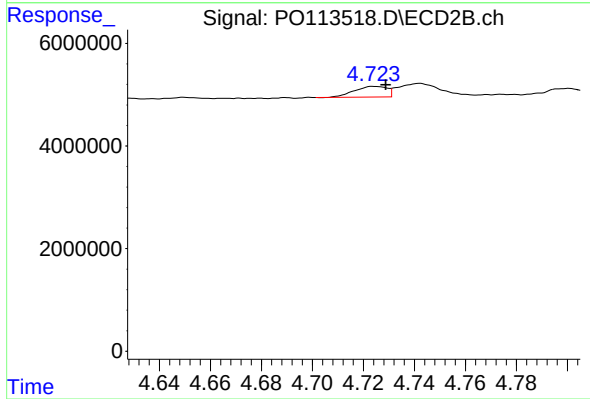


#3 AR-1016-1

R.T.: 4.724 min
Delta R.T.: -0.004 min
Response: 1842408
Conc: 10.80 ng/ml

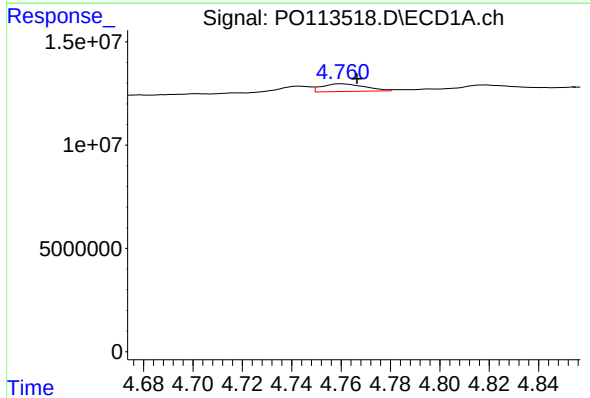


#4 AR-1016-2

R.T.: 4.760 min
Delta R.T.: -0.006 min
Response: 4481857
Conc: 11.16 ng/ml

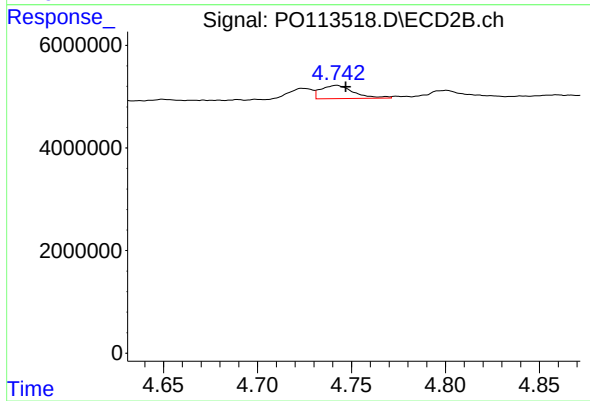

#4 AR-1016-2


R.T.: 4.742 min
Delta R.T.: -0.005 min
Response: 3106074
Conc: 12.06 ng/ml

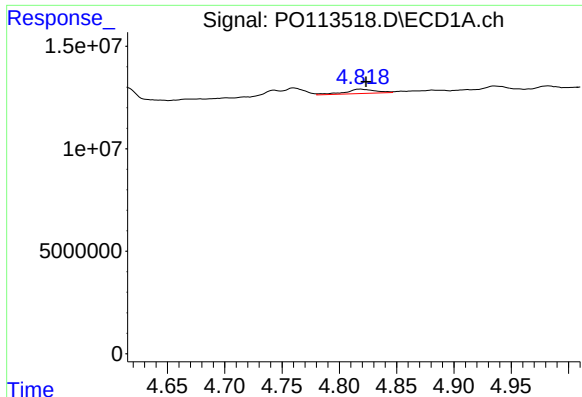

#5 AR-1016-3


R.T.: 4.818 min
Delta R.T.: -0.005 min
Response: 3944127
Conc: 15.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

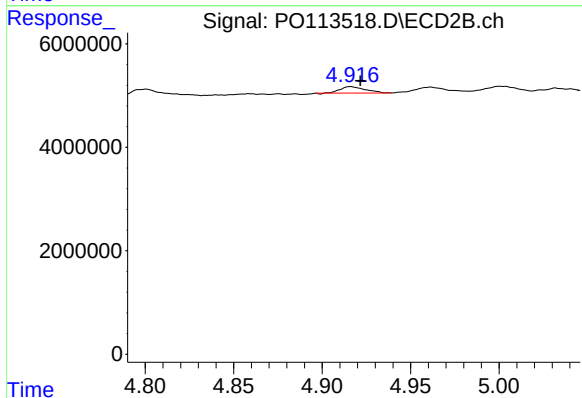


#5 AR-1016-3

R.T.: 4.916 min
Delta R.T.: -0.005 min
Response: 1225814
Conc: 8.78 ng/ml

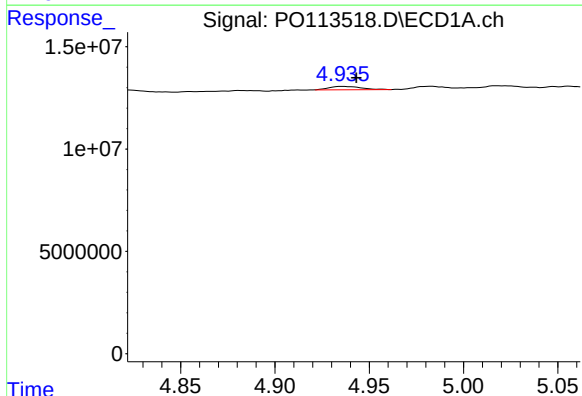


#6 AR-1016-4

R.T.: 4.936 min
Delta R.T.: -0.007 min
Response: 1945764
Conc: 8.92 ng/ml

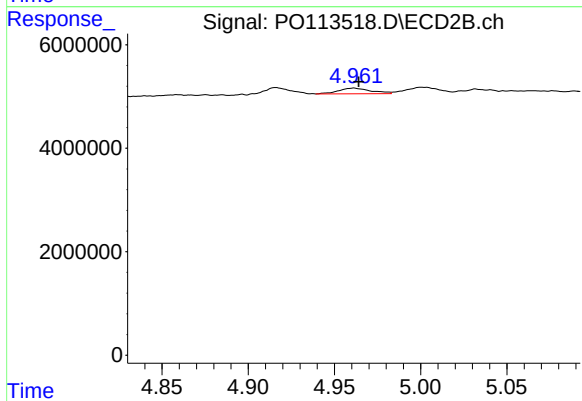

#6 AR-1016-4


R.T.: 4.961 min
Delta R.T.: -0.003 min
Response: 1423025
Conc: 12.19 ng/ml

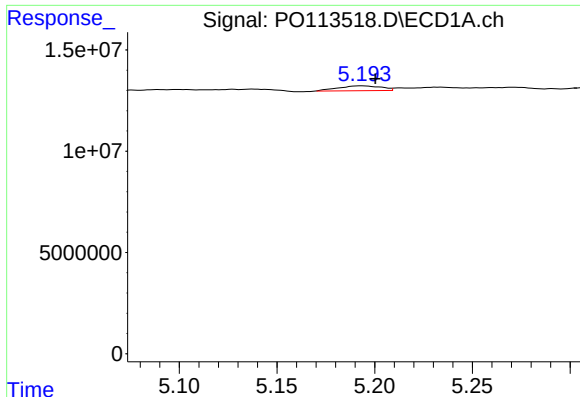

#7 AR-1016-5


R.T.: 5.194 min
Delta R.T.: -0.007 min
Response: 3608222
Conc: 16.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

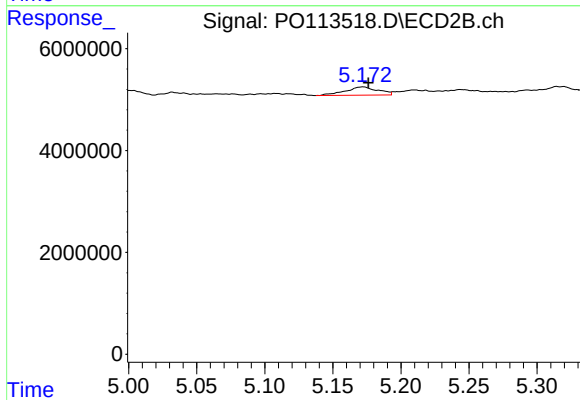


#7 AR-1016-5

R.T.: 5.172 min
Delta R.T.: -0.004 min
Response: 2686943
Conc: 18.85 ng/ml

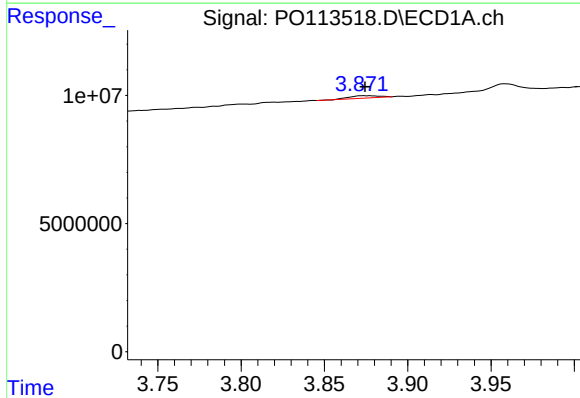


#8 AR-1221-1

R.T.: 3.873 min
Delta R.T.: 0.000 min
Response: 1114237
Conc: 11.91 ng/ml

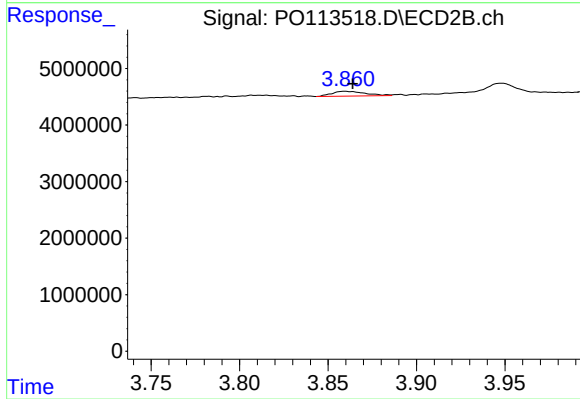

#8 AR-1221-1


R.T.: 3.860 min
Delta R.T.: -0.004 min
Response: 1097590
Conc: 17.39 ng/ml

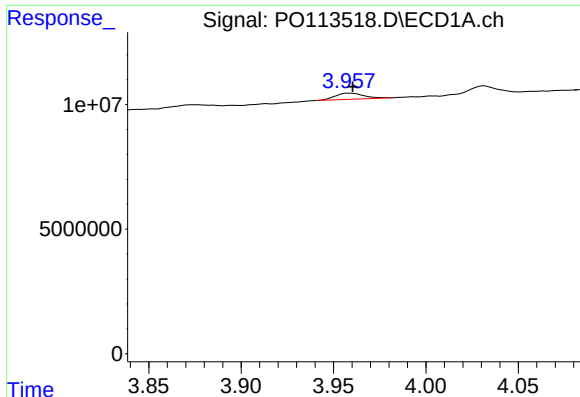

#9 AR-1221-2


R.T.: 3.959 min
Delta R.T.: -0.001 min
Response: 2639735
Conc: 39.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

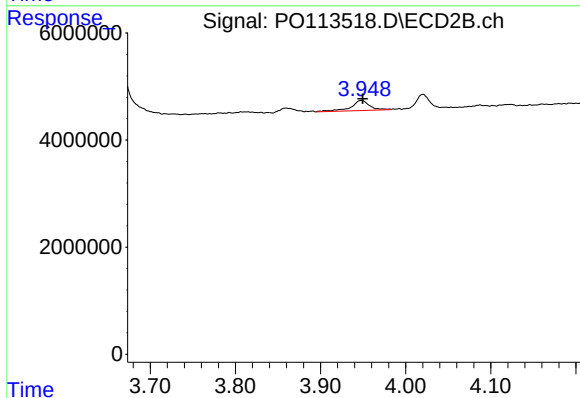


#9 AR-1221-2

R.T.: 3.948 min
Delta R.T.: -0.002 min
Response: 2865228
Conc: 61.39 ng/ml

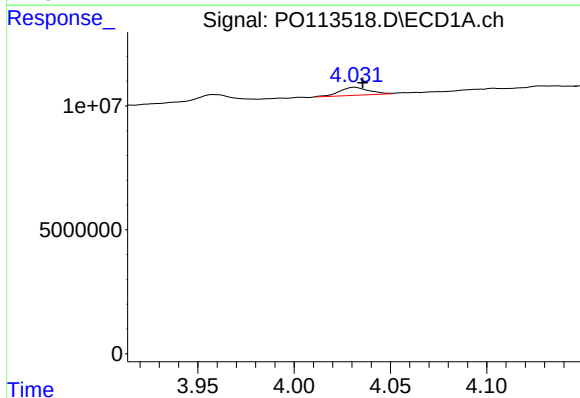


#10 AR-1221-3

R.T.: 4.032 min
Delta R.T.: -0.004 min
Response: 3354793
Conc: 15.16 ng/ml

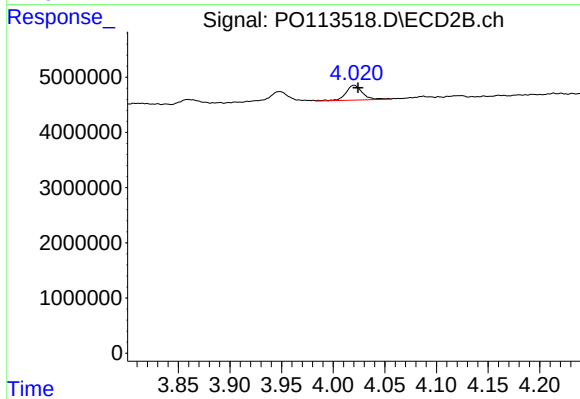

#10 AR-1221-3


R.T.: 4.020 min
Delta R.T.: -0.004 min
Response: 2981139
Conc: 20.08 ng/ml

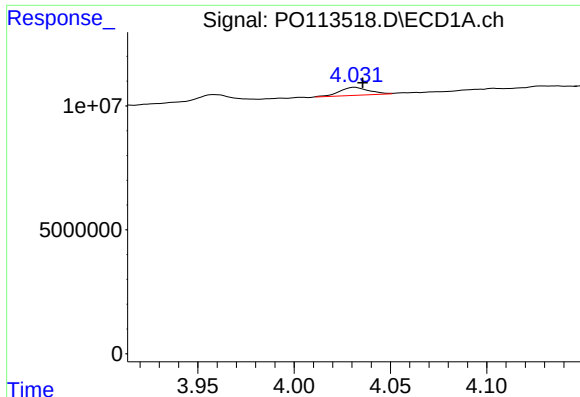

#11 AR-1232-1


R.T.: 4.032 min
Delta R.T.: -0.004 min
Response: 3354793
Conc: 19.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

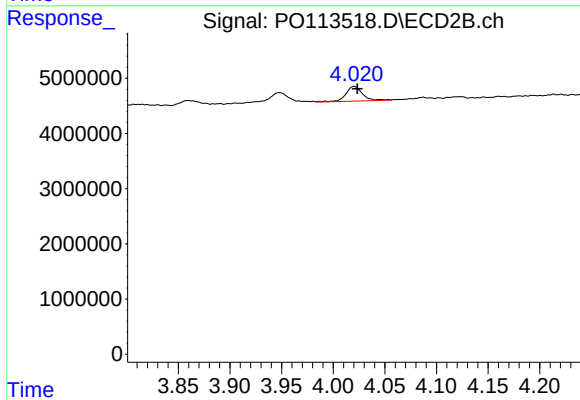


#11 AR-1232-1

R.T.: 4.020 min
Delta R.T.: -0.003 min
Response: 2981139
Conc: 25.39 ng/ml

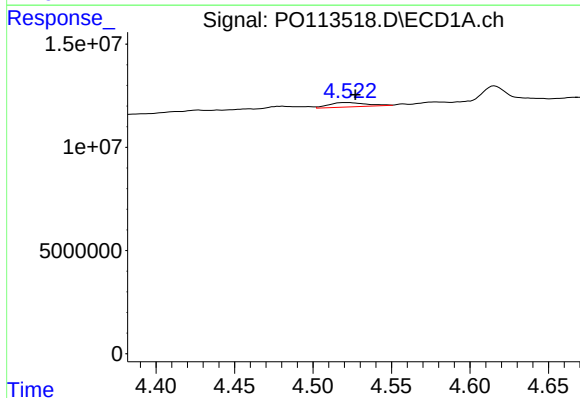


#12 AR-1232-2

R.T.: 4.522 min
Delta R.T.: -0.005 min
Response: 3532473
Conc: 35.38 ng/ml

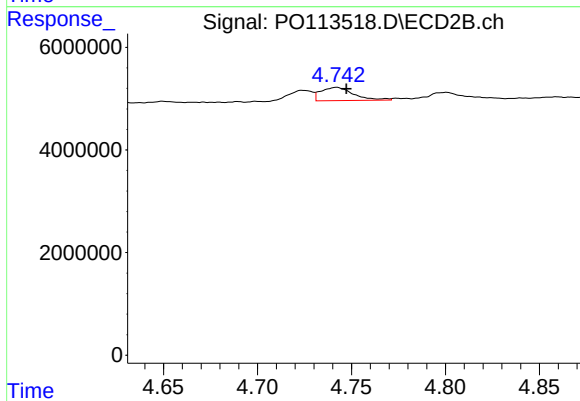

#12 AR-1232-2


R.T.: 4.742 min
Delta R.T.: -0.005 min
Response: 3106074
Conc: 25.35 ng/ml

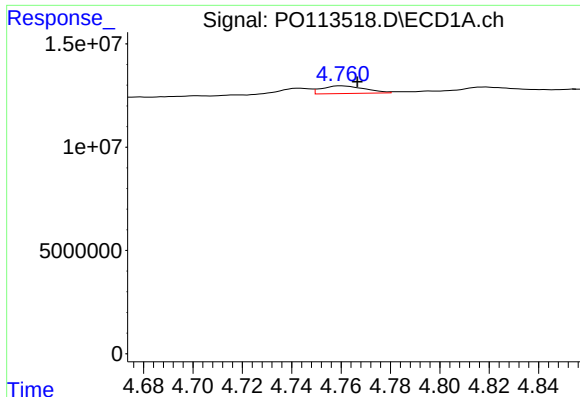

#13 AR-1232-3


R.T.: 4.760 min
Delta R.T.: -0.006 min
Response: 4481857
Conc: 23.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

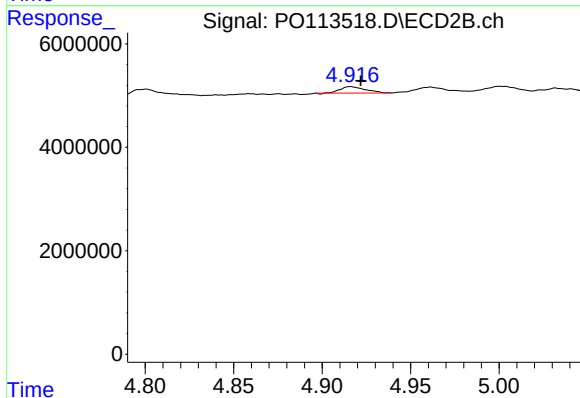


#13 AR-1232-3

R.T.: 4.916 min
Delta R.T.: -0.006 min
Response: 1225814
Conc: 19.35 ng/ml

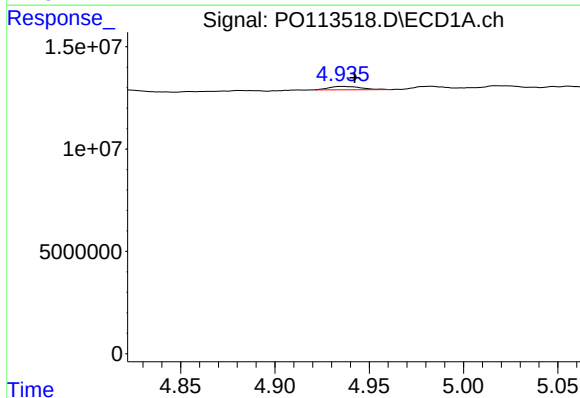


#14 AR-1232-4

R.T.: 4.936 min
Delta R.T.: -0.007 min
Response: 1945764
Conc: 20.66 ng/ml

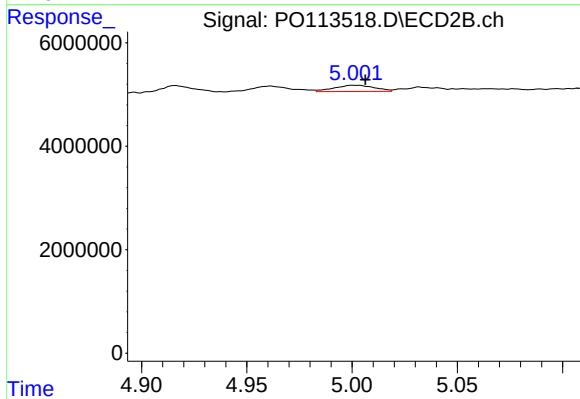

#14 AR-1232-4


R.T.: 5.002 min
Delta R.T.: -0.005 min
Response: 1594719
Conc: 28.37 ng/ml

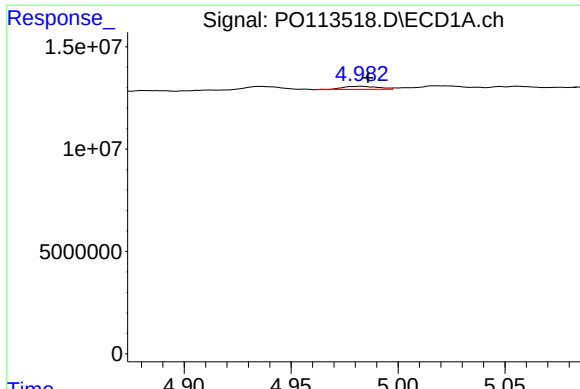

#15 AR-1232-5


R.T.: 4.983 min
Delta R.T.: -0.003 min
Response: 1807337
Conc: 29.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

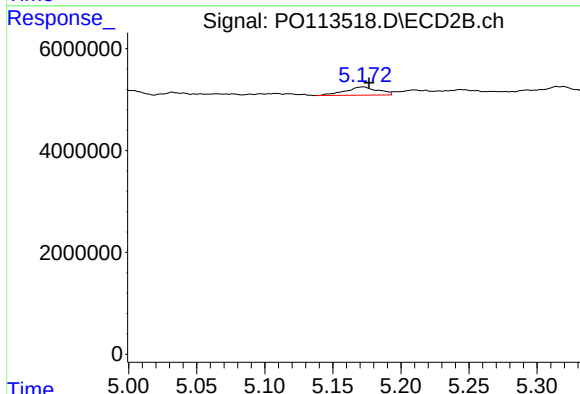


#15 AR-1232-5

R.T.: 5.172 min
Delta R.T.: -0.004 min
Response: 2686943
Conc: 44.88 ng/ml

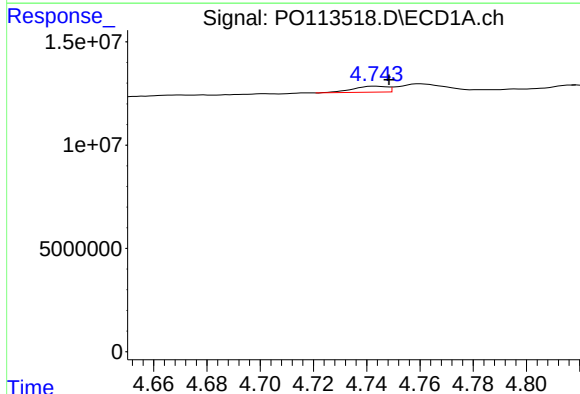


#16 AR-1242-1

R.T.: 4.743 min
Delta R.T.: -0.005 min
Response: 2548411
Conc: 11.08 ng/ml

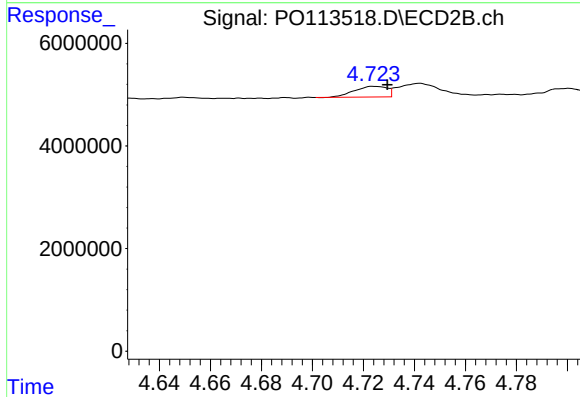

#16 AR-1242-1


R.T.: 4.724 min
Delta R.T.: -0.005 min
Response: 1842408
Conc: 12.75 ng/ml

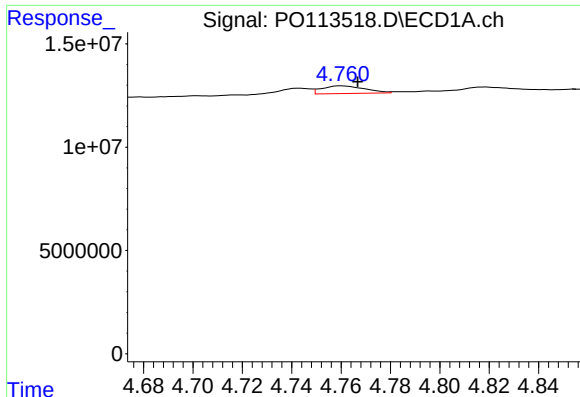

#17 AR-1242-2


R.T.: 4.760 min
Delta R.T.: -0.007 min
Response: 4481857
Conc: 13.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

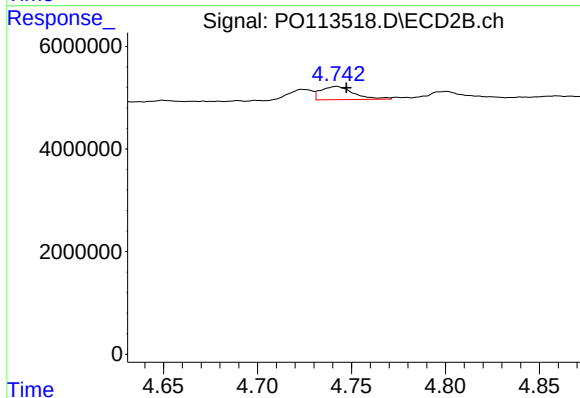


#17 AR-1242-2

R.T.: 4.742 min
Delta R.T.: -0.005 min
Response: 3106074
Conc: 14.32 ng/ml

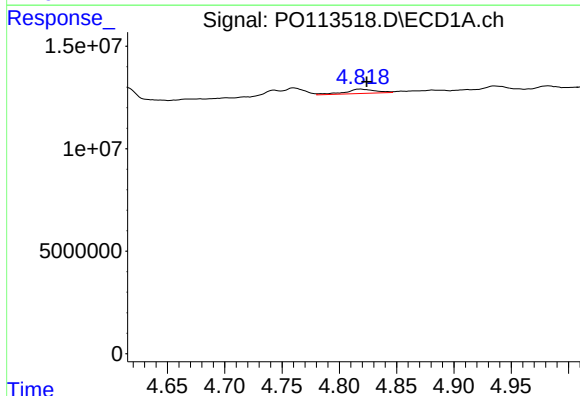


#18 AR-1242-3

R.T.: 4.818 min
Delta R.T.: -0.006 min
Response: 3944127
Conc: 17.78 ng/ml

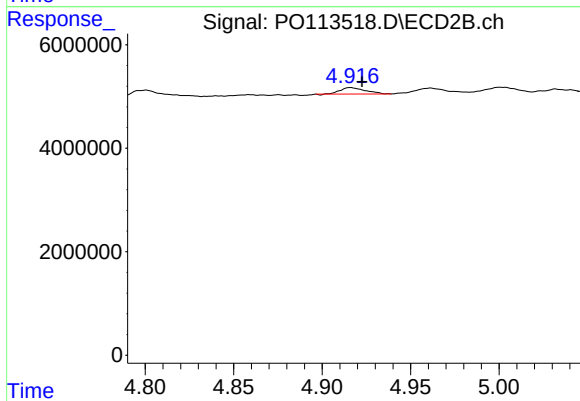

#18 AR-1242-3


R.T.: 4.916 min
Delta R.T.: -0.006 min
Response: 1225814
Conc: 10.48 ng/ml

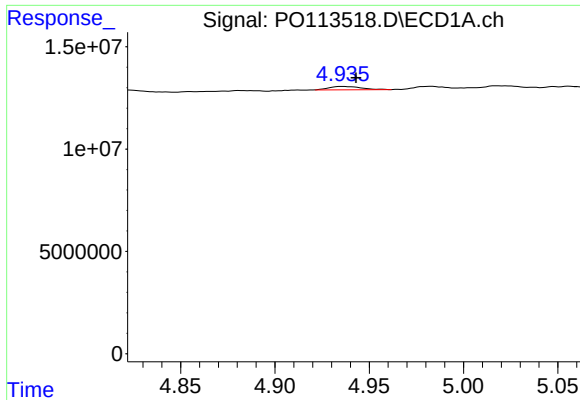

#19 AR-1242-4


R.T.: 4.936 min
Delta R.T.: -0.007 min
Response: 1945764
Conc: 11.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

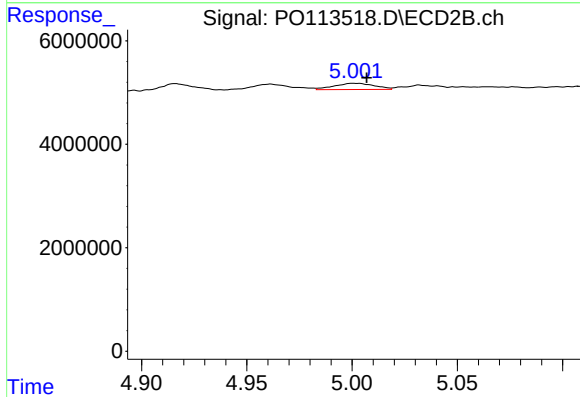


#19 AR-1242-4

R.T.: 5.002 min
Delta R.T.: -0.005 min
Response: 1594719
Conc: 13.56 ng/ml

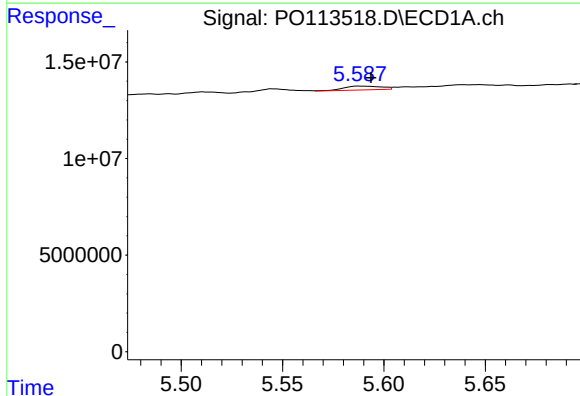


#20 AR-1242-5

R.T.: 5.589 min
Delta R.T.: -0.005 min
Response: 2525099
Conc: 12.62 ng/ml

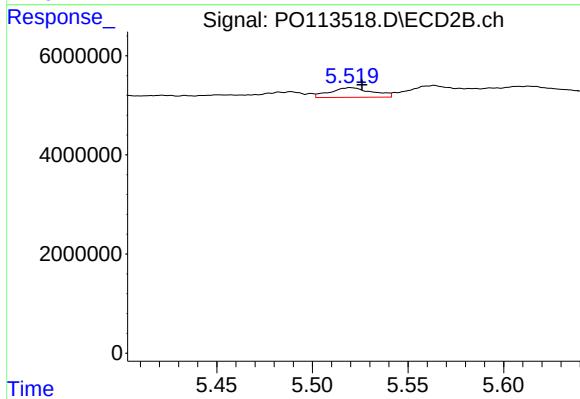

#20 AR-1242-5


R.T.: 5.520 min
Delta R.T.: -0.006 min
Response: 2962226
Conc: 19.86 ng/ml

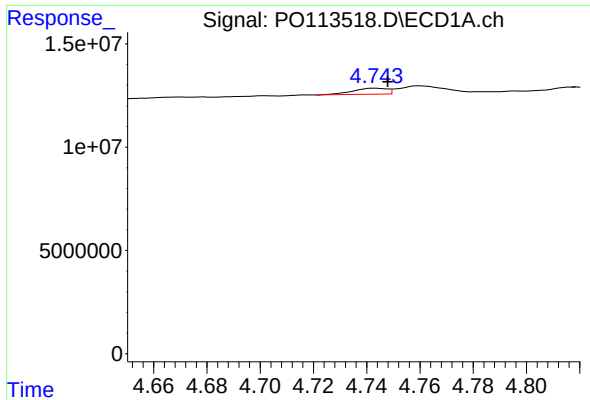

#21 AR-1248-1


R.T.: 4.743 min
Delta R.T.: -0.005 min
Response: 2548411
Conc: 14.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

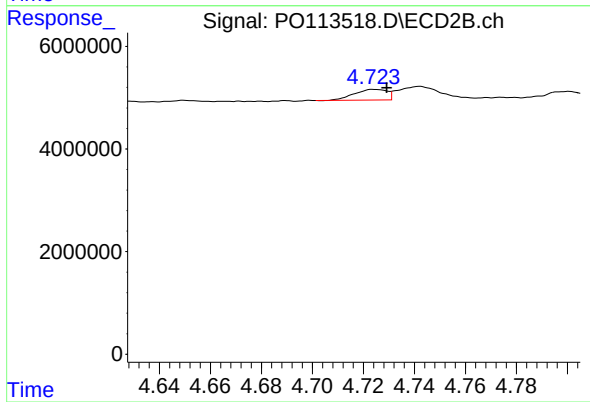


#21 AR-1248-1

R.T.: 4.724 min
Delta R.T.: -0.005 min
Response: 1842408
Conc: 16.52 ng/ml

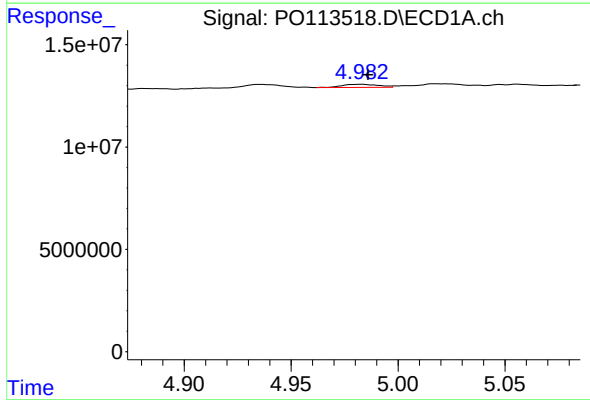


#22 AR-1248-2

R.T.: 4.983 min
Delta R.T.: -0.003 min
Response: 1807337
Conc: 7.47 ng/ml

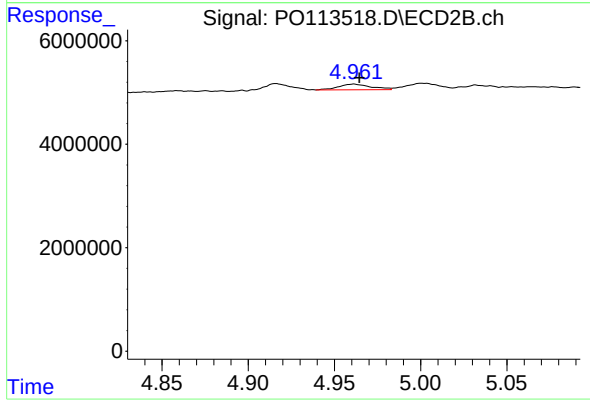

#22 AR-1248-2


R.T.: 4.961 min
Delta R.T.: -0.003 min
Response: 1423025
Conc: 8.86 ng/ml

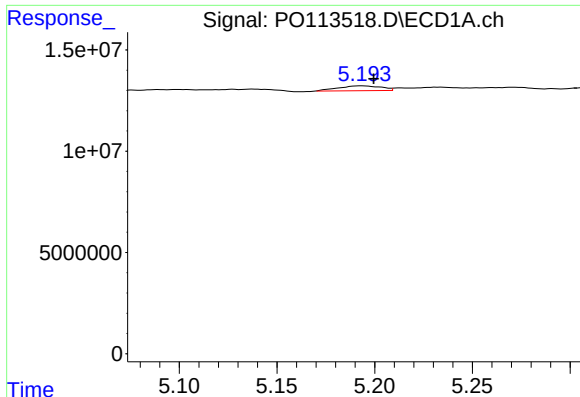

#23 AR-1248-3


R.T.: 5.194 min
Delta R.T.: -0.006 min
Response: 3608222
Conc: 11.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

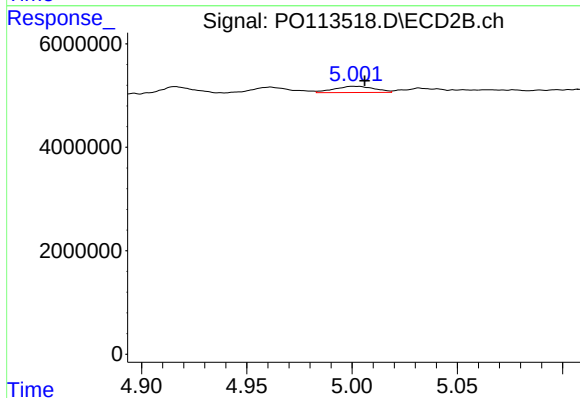


#23 AR-1248-3

R.T.: 5.002 min
Delta R.T.: -0.004 min
Response: 1594719
Conc: 9.40 ng/ml

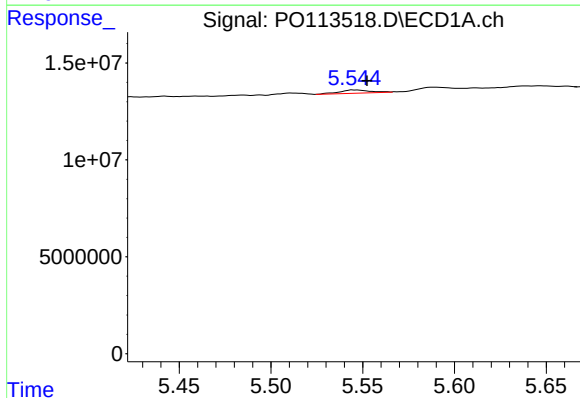


#24 AR-1248-4

R.T.: 5.546 min
Delta R.T.: -0.007 min
Response: 1971303
Conc: 3.95 ng/ml

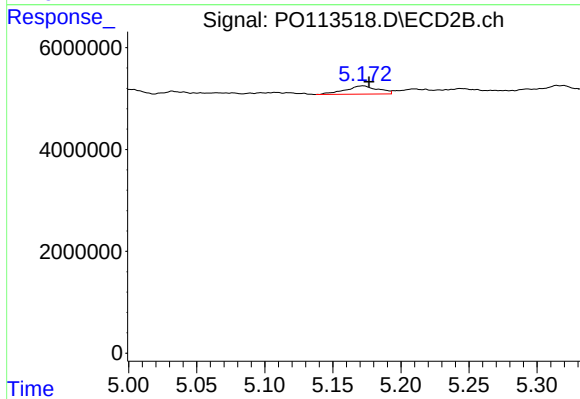

#24 AR-1248-4


R.T.: 5.172 min
Delta R.T.: -0.005 min
Response: 2686943
Conc: 13.49 ng/ml

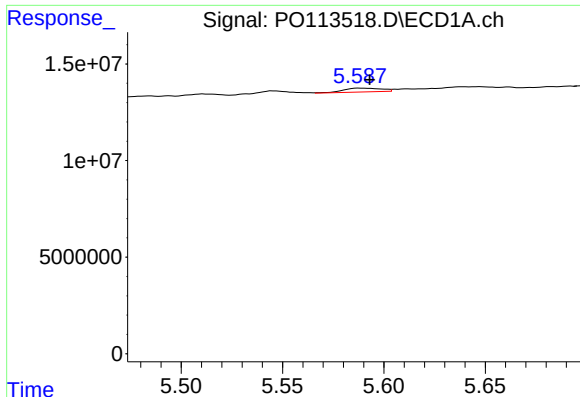

#25 AR-1248-5


R.T.: 5.589 min
Delta R.T.: -0.004 min
Response: 2525099
Conc: 7.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

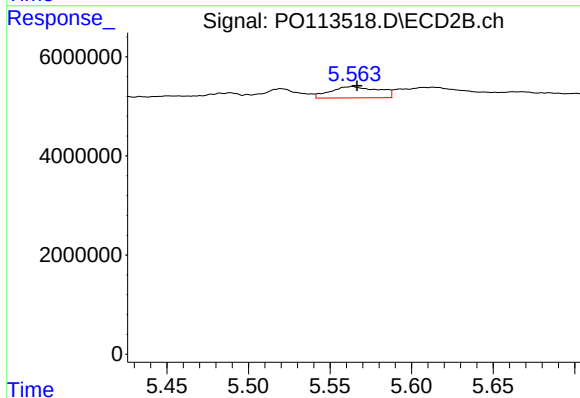


#25 AR-1248-5

R.T.: 5.564 min
Delta R.T.: -0.003 min
Response: 4660045
Conc: 21.95 ng/ml

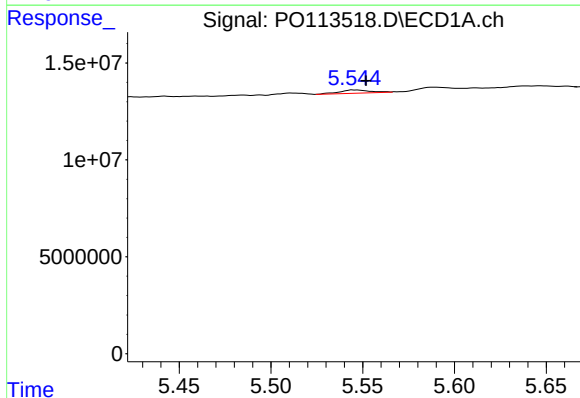


#26 AR-1254-1

R.T.: 5.546 min
Delta R.T.: -0.006 min
Response: 1971303
Conc: 3.65 ng/ml

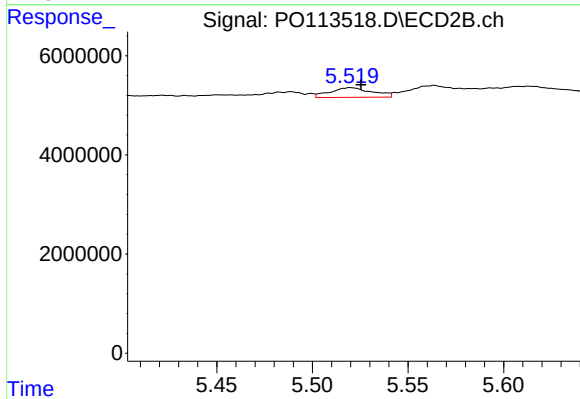

#26 AR-1254-1


R.T.: 5.520 min
Delta R.T.: -0.005 min
Response: 2962226
Conc: 9.39 ng/ml

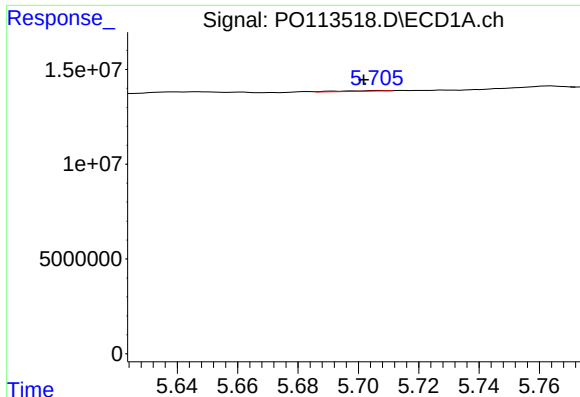

#27 AR-1254-2


R.T.: 5.707 min
Delta R.T.: 0.005 min
Response: 349708
Conc: 0.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

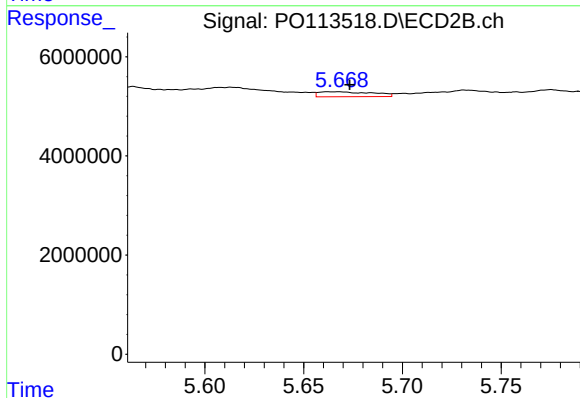


#27 AR-1254-2

R.T.: 5.668 min
Delta R.T.: -0.005 min
Response: 1908555
Conc: 6.81 ng/ml

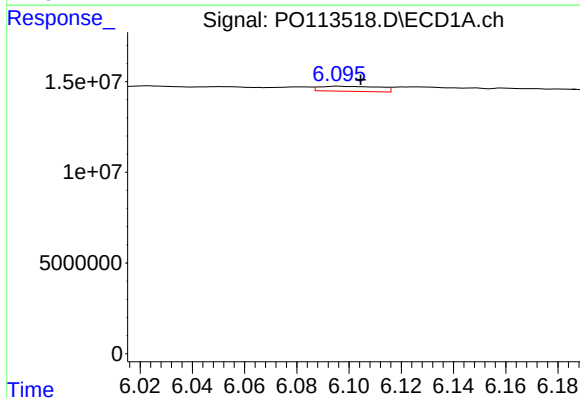


#28 AR-1254-3

R.T.: 6.096 min
Delta R.T.: -0.009 min
Response: 4488109
Conc: 6.07 ng/ml

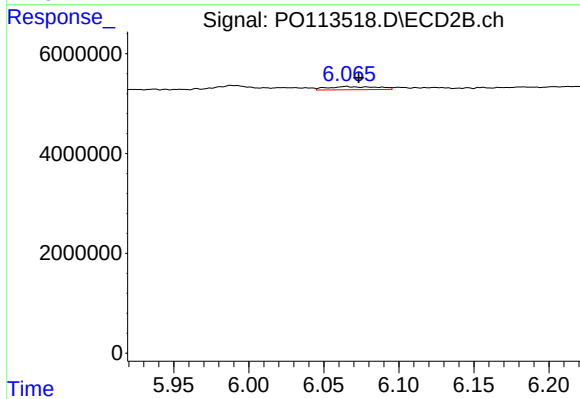

#28 AR-1254-3


R.T.: 6.065 min
Delta R.T.: -0.008 min
Response: 1488502
Conc: 3.57 ng/ml

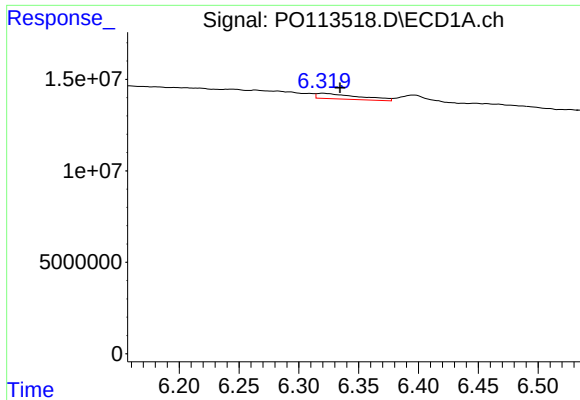

#29 AR-1254-4


R.T.: 6.320 min
Delta R.T.: -0.014 min
Response: 7331347
Conc: 13.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

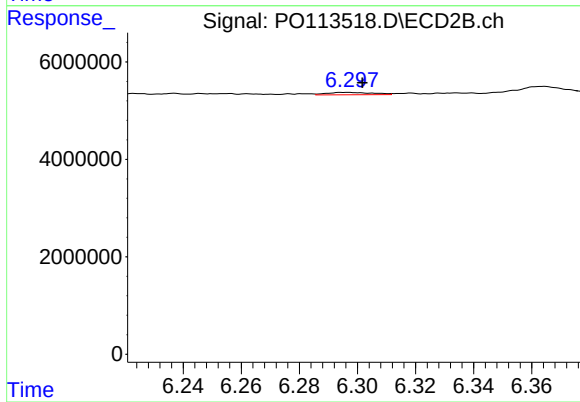


#29 AR-1254-4

R.T.: 6.296 min
Delta R.T.: -0.006 min
Response: 530431
Conc: 1.93 ng/ml

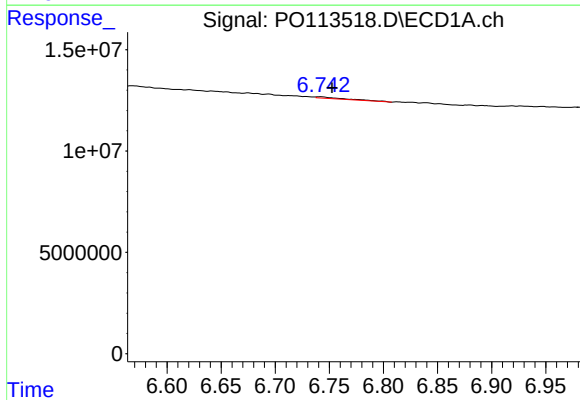


#30 AR-1254-5

R.T.: 6.743 min
Delta R.T.: -0.010 min
Response: 1306120
Conc: 1.86 ng/ml

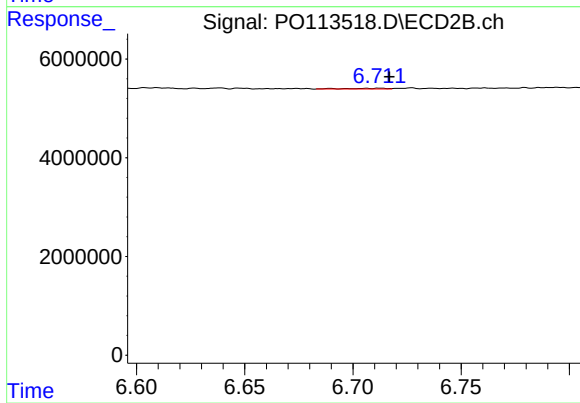

#30 AR-1254-5


R.T.: 6.713 min
Delta R.T.: -0.004 min
Response: 190354
Conc: 0.53 ng/ml

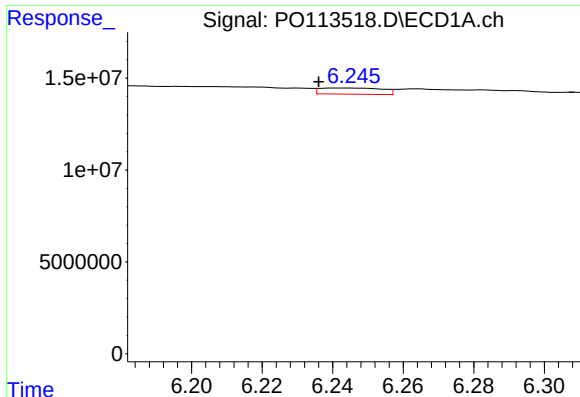

#31 AR-1260-1


R.T.: 6.244 min
Delta R.T.: 0.008 min
Response: 4105349
Conc: 9.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

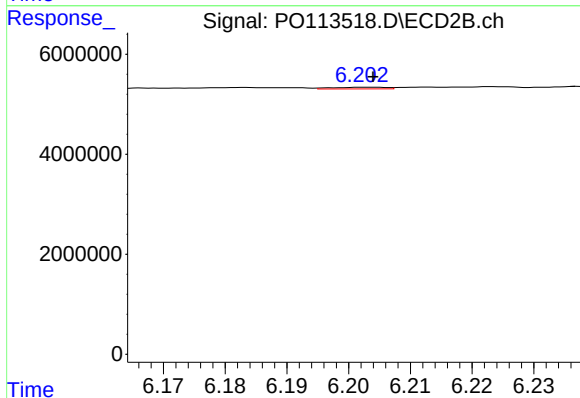


#31 AR-1260-1

R.T.: 6.203 min
Delta R.T.: 0.000 min
Response: 208297
Conc: 0.82 ng/ml

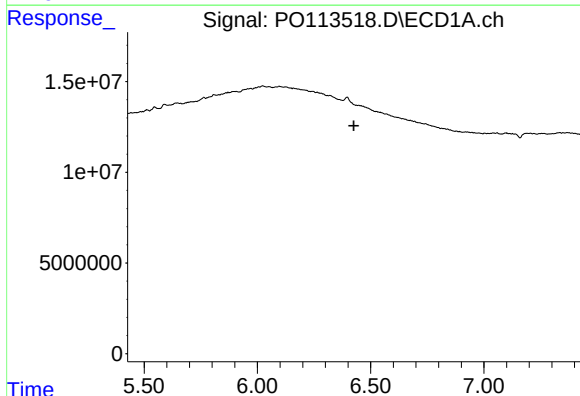


#32 AR-1260-2

R.T.: 6.448 min
Delta R.T.: 0.022 min
Response: -194992
Conc: N.D.

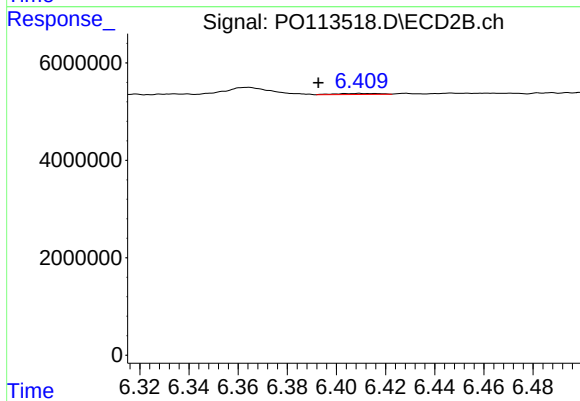

#32 AR-1260-2


R.T.: 6.410 min
Delta R.T.: 0.017 min
Response: 254354
Conc: 0.74 ng/ml

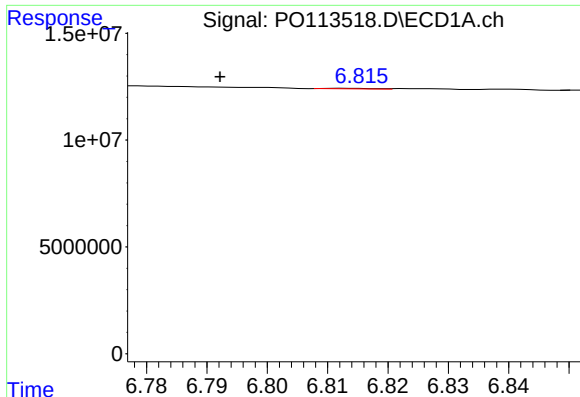

#33 AR-1260-3


R.T.: 6.813 min
Delta R.T.: 0.021 min
Response: 155131
Conc: 0.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

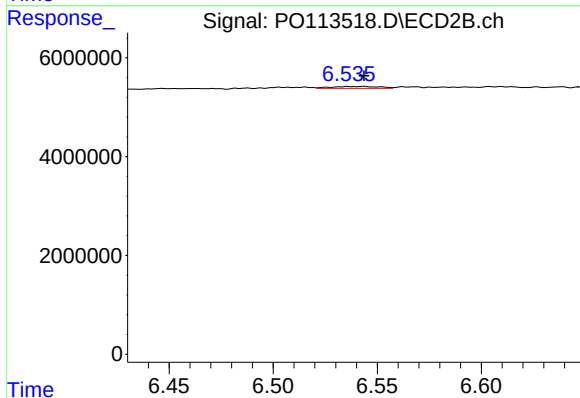


#33 AR-1260-3

R.T.: 6.543 min
Delta R.T.: 0.000 min
Response: 623364
Conc: 2.10 ng/ml

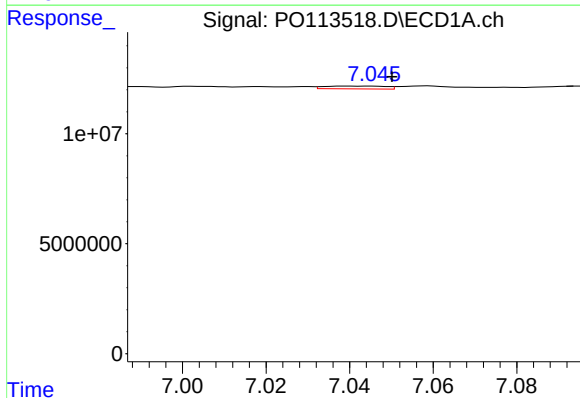


#34 AR-1260-4

R.T.: 7.045 min
Delta R.T.: -0.006 min
Response: 1342628
Conc: 3.00 ng/ml

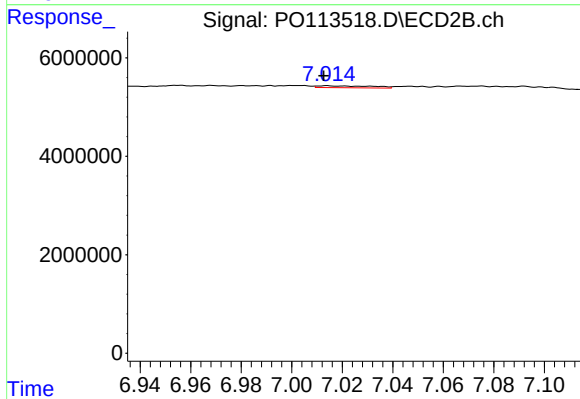

#34 AR-1260-4


R.T.: 7.014 min
Delta R.T.: 0.001 min
Response: 610720
Conc: 2.95 ng/ml

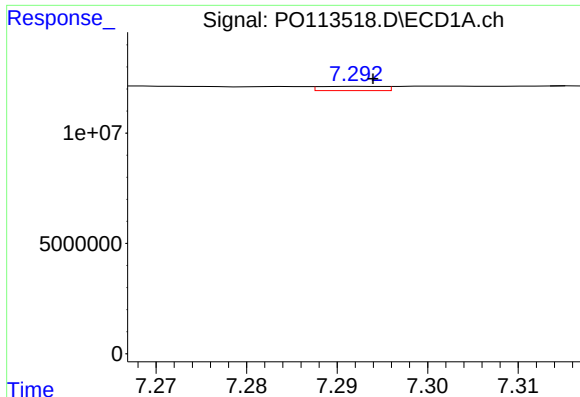

#35 AR-1260-5


R.T.: 7.293 min
Delta R.T.: -0.001 min
Response: 951522
Conc: 0.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

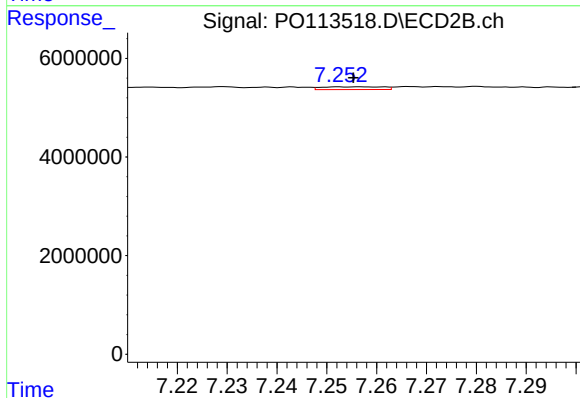


#35 AR-1260-5

R.T.: 7.256 min
Delta R.T.: 0.001 min
Response: 472440
Conc: 1.01 ng/ml

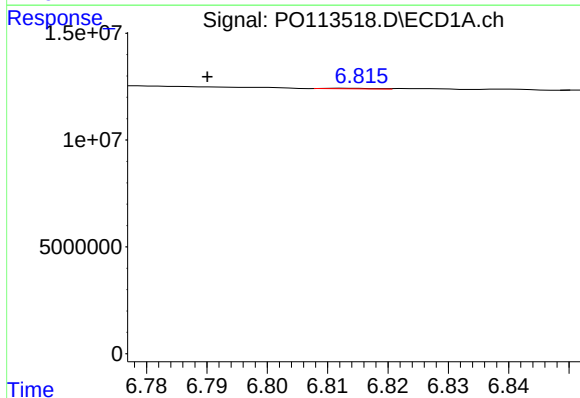


#36 AR-1262-1

R.T.: 6.813 min
Delta R.T.: 0.023 min
Response: 155131
Conc: 0.17 ng/ml

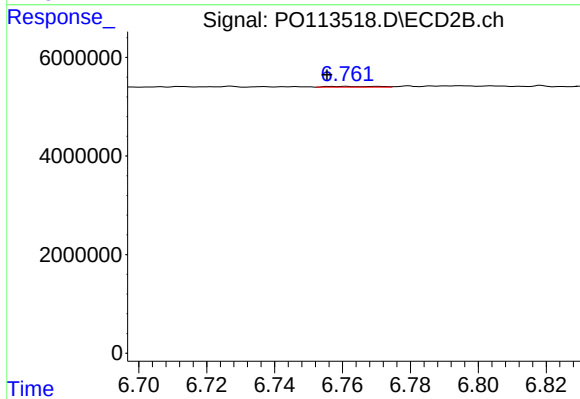

#36 AR-1262-1


R.T.: 6.761 min
Delta R.T.: 0.005 min
Response: 168469
Conc: 0.41 ng/ml

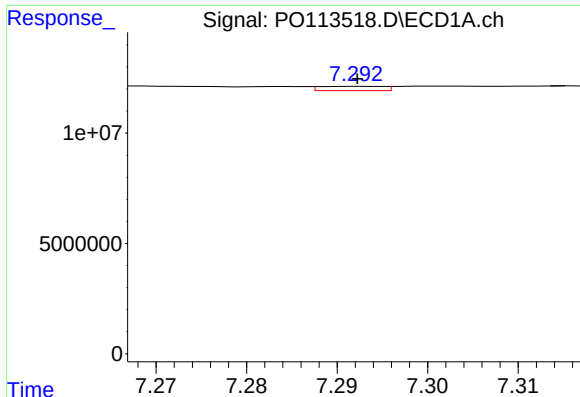

#37 AR-1262-2


R.T.: 7.293 min
Delta R.T.: 0.000 min
Response: 951522
Conc: 0.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

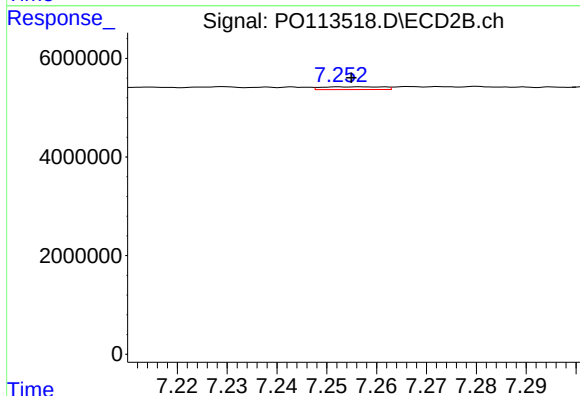


#37 AR-1262-2

R.T.: 7.256 min
Delta R.T.: 0.002 min
Response: 472440
Conc: 0.91 ng/ml

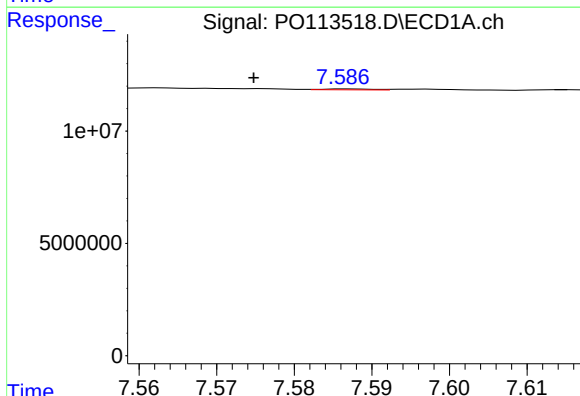


#38 AR-1262-3

R.T.: 7.587 min
Delta R.T.: 0.012 min
Response: 188634
Conc: 0.34 ng/ml

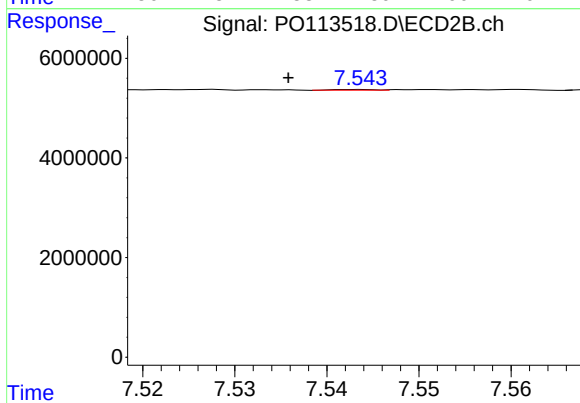

#38 AR-1262-3


R.T.: 7.543 min
Delta R.T.: 0.007 min
Response: 40600
Conc: 0.23 ng/ml

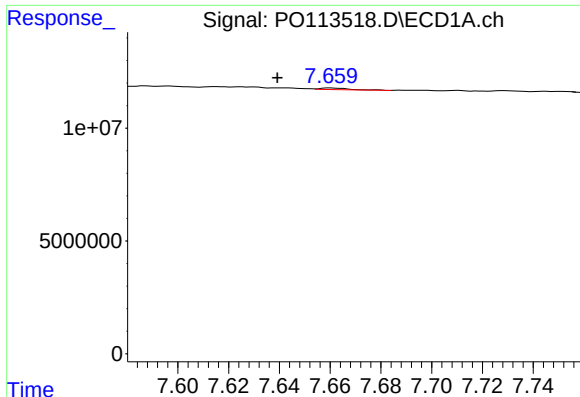

#39 AR-1262-4


R.T.: 7.660 min
Delta R.T.: 0.021 min
Response: 579176
Conc: 0.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

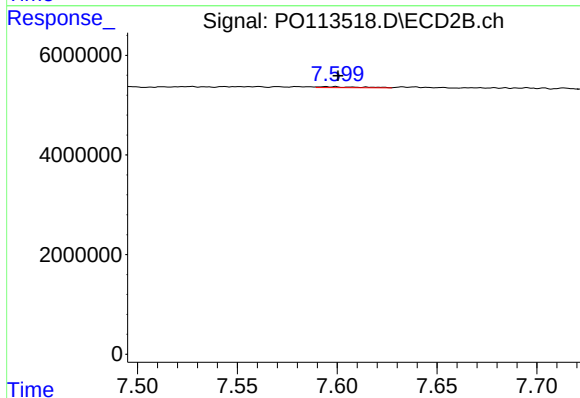


#39 AR-1262-4

R.T.: 7.599 min
Delta R.T.: -0.002 min
Response: 271339
Conc: 0.94 ng/ml

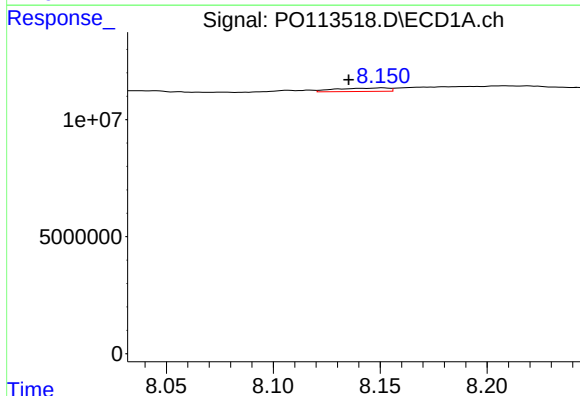


#40 AR-1262-5

R.T.: 8.151 min
Delta R.T.: 0.016 min
Response: 2464123
Conc: 5.91 ng/ml

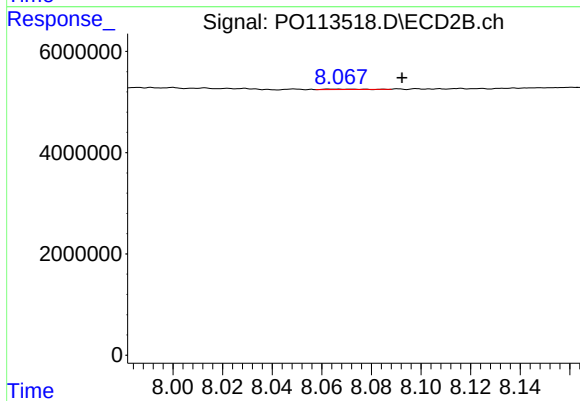

#40 AR-1262-5


R.T.: 8.063 min
Delta R.T.: -0.029 min
Response: 63508
Conc: 0.59 ng/ml

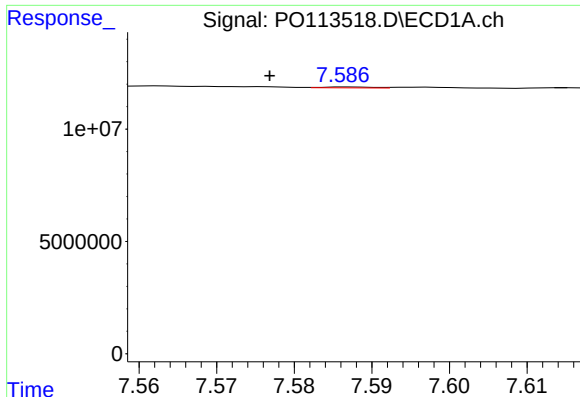

#41 AR-1268-1


R.T.: 7.587 min
Delta R.T.: 0.010 min
Response: 188634
Conc: 0.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

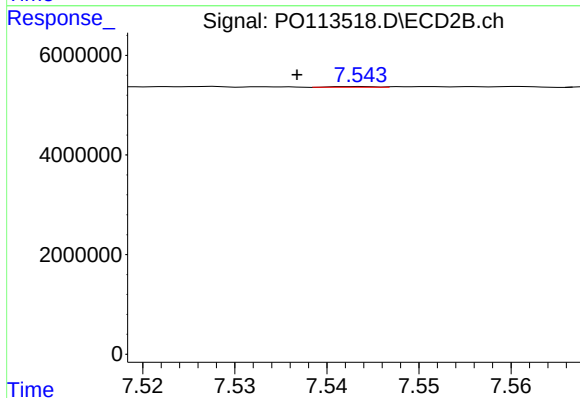


#41 AR-1268-1

R.T.: 7.543 min
Delta R.T.: 0.007 min
Response: 40600
Conc: 0.08 ng/ml

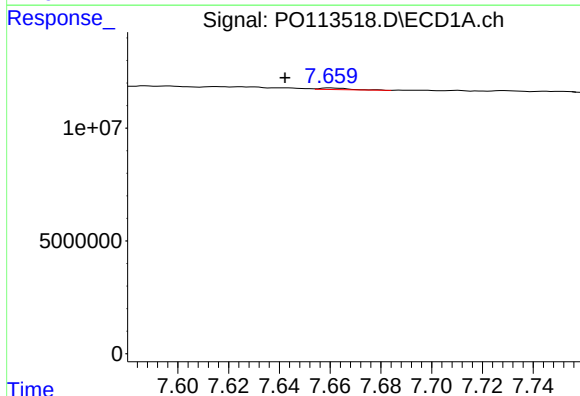


#42 AR-1268-2

R.T.: 7.660 min
Delta R.T.: 0.018 min
Response: 579176
Conc: 0.40 ng/ml

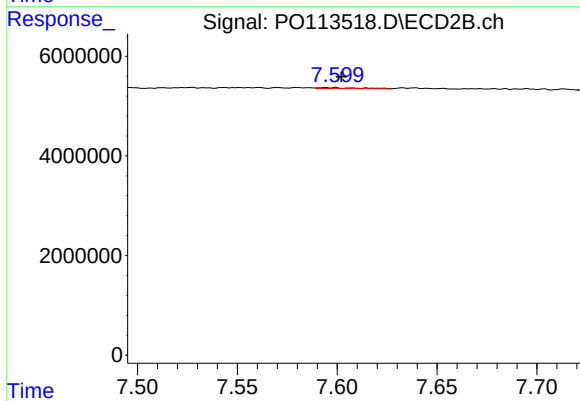

#42 AR-1268-2


R.T.: 7.599 min
Delta R.T.: -0.003 min
Response: 271339
Conc: 0.65 ng/ml

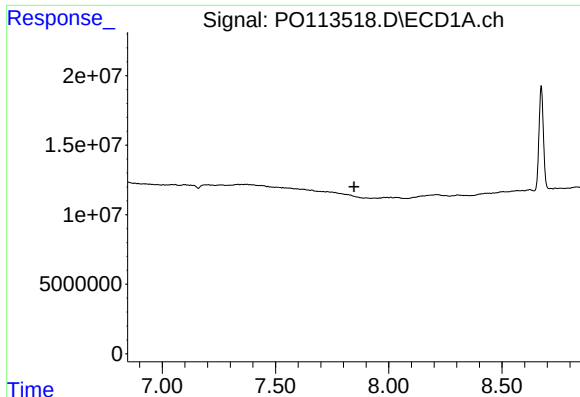

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 7.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

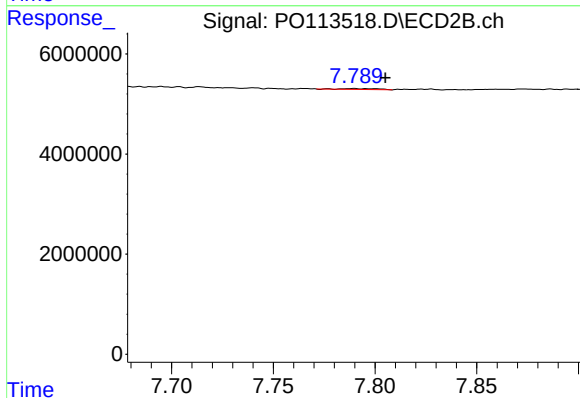


#43 AR-1268-3

R.T.: 7.790 min
Delta R.T.: -0.016 min
Response: 203995
Conc: 0.62 ng/ml

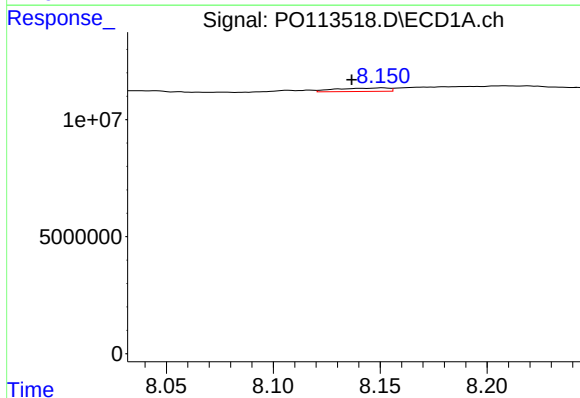


#44 AR-1268-4

R.T.: 8.151 min
Delta R.T.: 0.014 min
Response: 2464123
Conc: 5.35 ng/ml

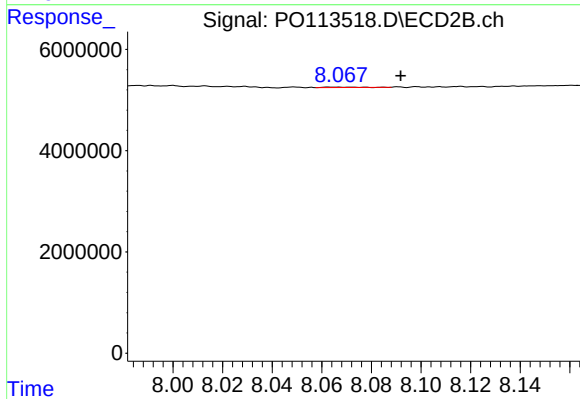

#44 AR-1268-4


R.T.: 8.063 min
Delta R.T.: -0.028 min
Response: 63508
Conc: 0.53 ng/ml

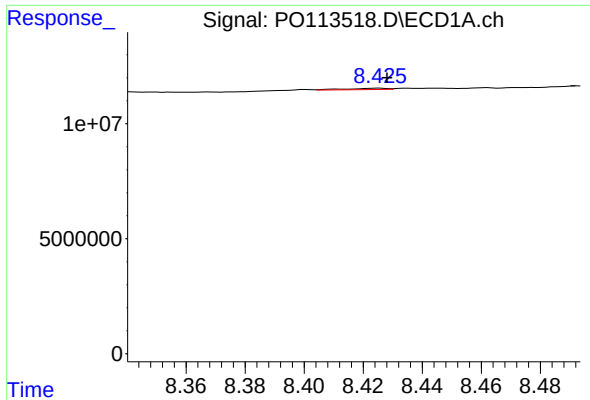

#45 AR-1268-5

R.T.: 8.425 min
Delta R.T.: -0.003 min
Response: 584603
Conc: 0.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

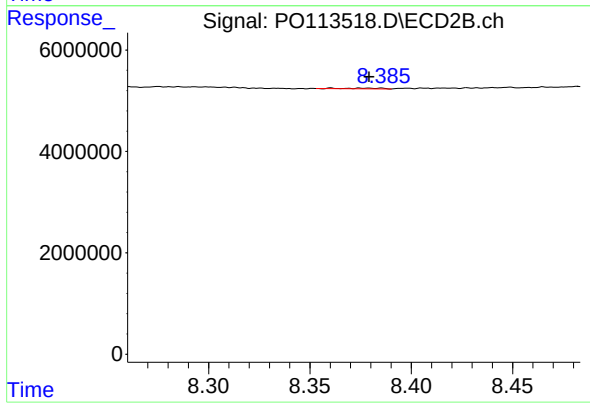

#45 AR-1268-5

R.T.: 8.361 min
Delta R.T.: -0.019 min
Response: 164230
Conc: 0.21 ng/ml