

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090525\
 Data File : P0113519.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 19:09
 Operator : YP/AJ
 Sample : Q2893-09
 Misc : AR1242 WATER LOD 25PPB
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:35:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.660	3.652	164.8E6	98192015	20.130	19.403
2)	SA Decachlor...	8.674	8.620	103.0E6	34971242	14.863	18.456
Target Compounds							
3)	L1 AR-1016-1	4.744	4.725	8710356	6216828	32.625	36.447
4)	L1 AR-1016-2	4.761	4.743	12025603	7855172	29.957	30.487
5)	L1 AR-1016-3	4.819	4.919	7021356	4408214	27.532	31.574
6)	L1 AR-1016-4	4.938	4.960	6545402	6684983	30.015	57.284 #
7)	L1 AR-1016-5	5.193	5.172	13977612	9460432	63.068	66.375
8)	L2 AR-1221-1	3.884	3.857	829745	143951	8.867	2.281 #
9)	L2 AR-1221-2	3.959	3.948	1432431	2874052	21.205	61.578 #
10)	L2 AR-1221-3	4.032	4.020	2497753	2191970	11.284	14.763 #
11)	L3 AR-1232-1	4.032	4.020	2497753	2191970	14.354	18.671 #
12)	L3 AR-1232-2	4.521	4.743	6539392	7855172	65.491	64.100
13)	L3 AR-1232-3	4.761	4.919	12025603	4408214	63.468	69.590
14)	L3 AR-1232-4	4.938	5.001	6545402	7460183	69.507	132.693 #
15)	L3 AR-1232-5	4.981	5.172	9510851	9460432	153.542	158.033
16)	L4 AR-1242-1	4.744	4.725	8710356	6216828	37.882	43.022
17)	L4 AR-1242-2	4.761	4.743	12025603	7855172	34.996	36.214
18)	L4 AR-1242-3	4.819	4.919	7021356	4408214	31.644	37.689
19)	L4 AR-1242-4	4.938	5.001	6545402	7460183	37.734	63.417 #
20)	L4 AR-1242-5	5.588	5.520	9387937	11939049	46.902	80.056 #
21)	L5 AR-1248-1	4.744	4.725	8710356	6216828	49.926	55.750
22)	L5 AR-1248-2	4.981	4.960	9510851	6684983	39.323	41.599
23)	L5 AR-1248-3	5.193	5.001	13977612	7460183	43.836	43.971
24)	L5 AR-1248-4	5.546	5.172	13268197	9460432	26.557	47.487 #
25)	L5 AR-1248-5	5.588	5.561	9387937	10354179	27.491	48.772 #
26)	L6 AR-1254-1	5.546	5.520	13268197	11939049	24.572	37.859 #
27)	L6 AR-1254-2	5.695	5.667	4122289	6427077	8.354	22.926 #
28)	L6 AR-1254-3	6.099	6.068	10735617	4588412	14.530	11.005
29)	L6 AR-1254-4	6.327	6.296	21952028	3273236	39.411	11.910 #
30)	L6 AR-1254-5	6.739	6.710	2359520	888477	3.366	2.485 #
31)	L7 AR-1260-1	6.243	6.213	12939865	3767333	29.014	14.770 #
32)	L7 AR-1260-2	6.453	6.365	1124829	3623726	1.638	10.482 #
33)	L7 AR-1260-3	6.842f	6.539	933834	897454	1.512	3.017 #
34)	L7 AR-1260-4	7.055	7.005	4293646	1658035	9.587	8.000
35)	L7 AR-1260-5	7.298	7.255	3569632	1791267	2.948	3.824 #
36)	L8 AR-1262-1	6.842f	6.747	933834	646127	1.020	1.558 #
37)	L8 AR-1262-2	7.288	7.255	5972265	1791267	3.950	3.460
38)	L8 AR-1262-3	7.580	7.521	1166393	302760	2.105	1.686
39)	L8 AR-1262-4	7.617	7.616	1084816	37138	1.109	0.128 #
40)	L8 AR-1262-5	8.141	8.104	276620	104043	0.664	0.960 #
41)	L9 AR-1268-1	7.580	7.521	1166393	302760	0.678	0.594

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090525\
Data File : P0113519.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2025 19:09
Operator : YP/AJ
Sample : Q2893-09
Misc : AR1242 WATER LOD 25PPB
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 23:35:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	7.617	7.616	1084816	37138	0.749	0.089 #
43)	L9 AR-1268-3	7.860	7.797	439395	113726	0.364	0.348
44)	L9 AR-1268-4	8.141	8.104	276620	104043	0.600	0.864 #
45)	L9 AR-1268-5	8.426	8.376	1070739	306777	0.336	0.393


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090525\
Data File : P0113519.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2025 19:09
Operator : YP/AJ
Sample : Q2893-09
Misc : AR1242 WATER LOD 25PPB
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 23:35:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

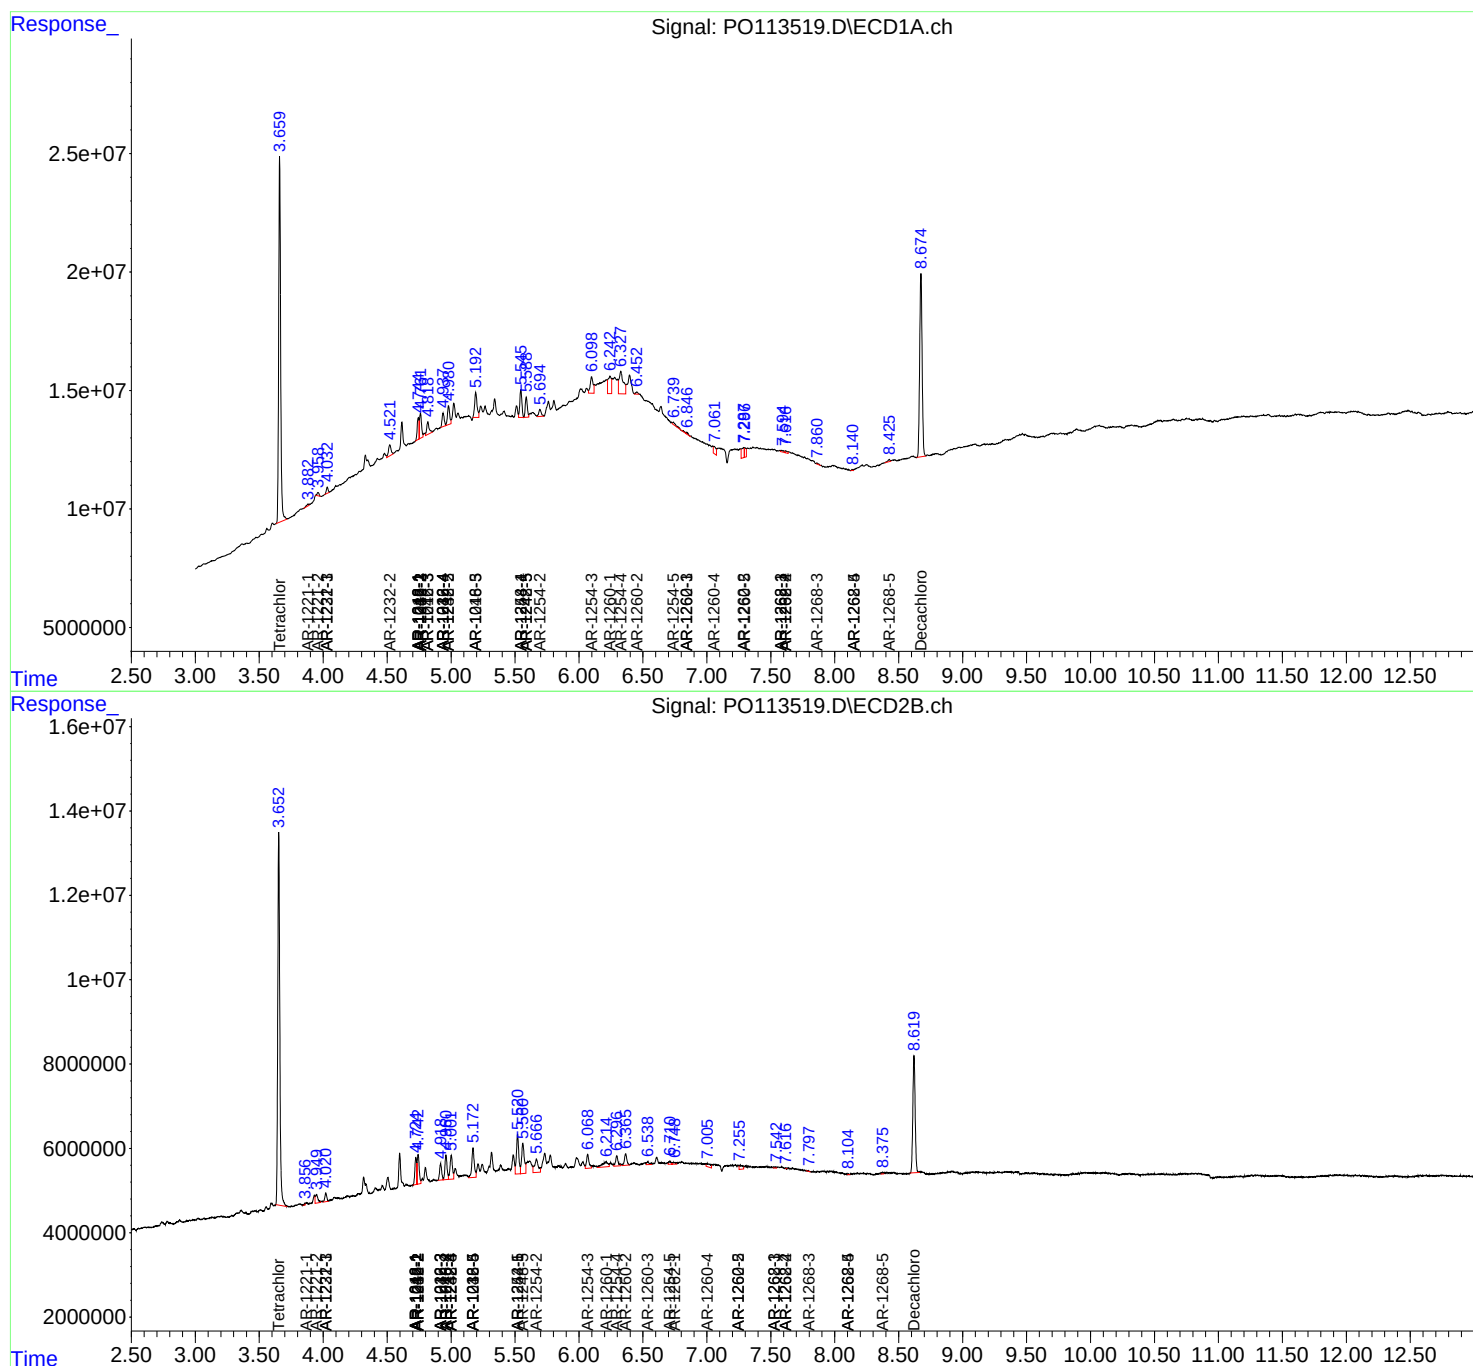


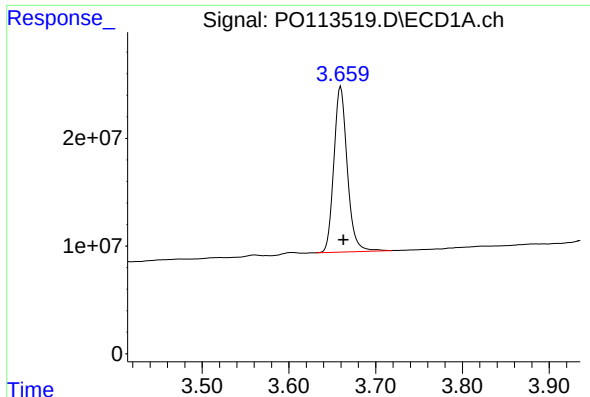

#1 Tetrachloro-m-xylene


R.T.: 3.660 min
Delta R.T.: -0.003 min
Response: 164792308
Conc: 20.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

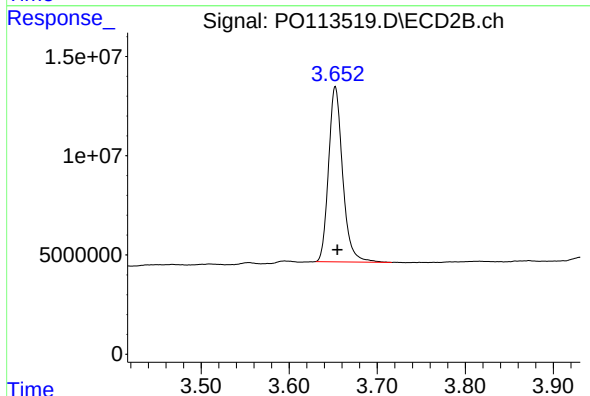


#1 Tetrachloro-m-xylene

R.T.: 3.652 min
Delta R.T.: -0.002 min
Response: 98192015
Conc: 19.40 ng/ml

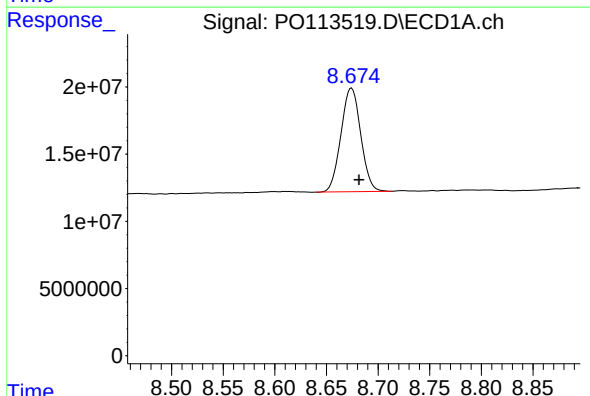


#2 Decachlorobiphenyl

R.T.: 8.674 min
Delta R.T.: -0.007 min
Response: 103019543
Conc: 14.86 ng/ml

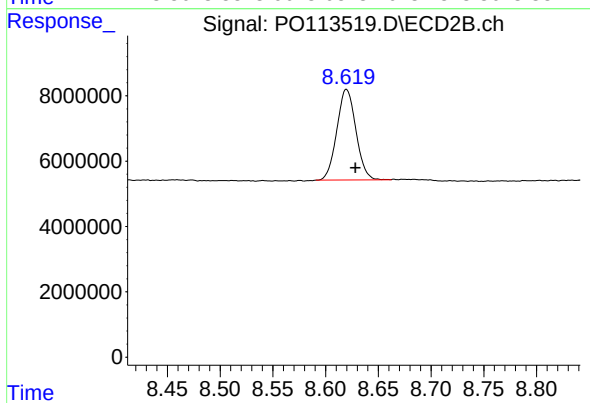

#2 Decachlorobiphenyl


R.T.: 8.620 min
Delta R.T.: -0.009 min
Response: 34971242
Conc: 18.46 ng/ml

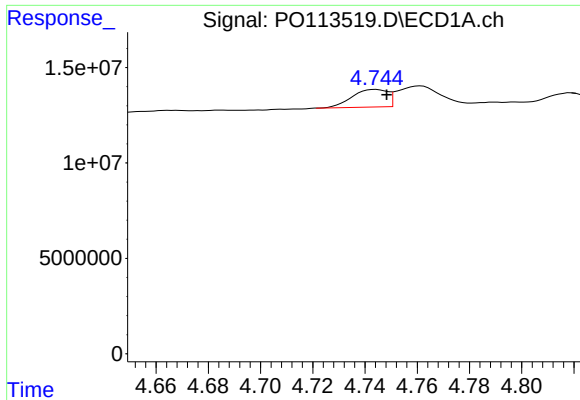

#3 AR-1016-1


R.T.: 4.744 min
Delta R.T.: -0.004 min
Response: 8710356
Conc: 32.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

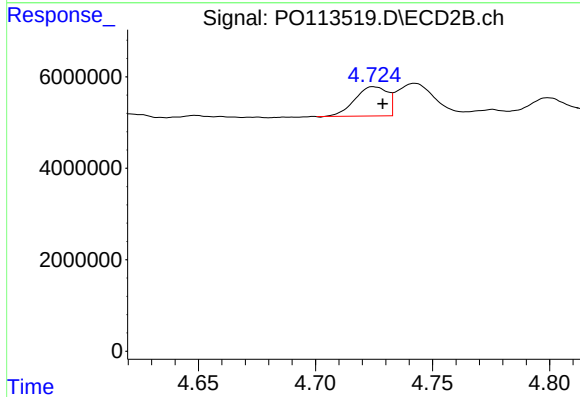


#3 AR-1016-1

R.T.: 4.725 min
Delta R.T.: -0.004 min
Response: 6216828
Conc: 36.45 ng/ml

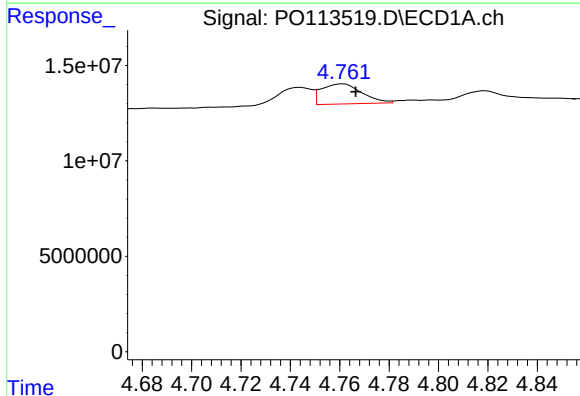


#4 AR-1016-2

R.T.: 4.761 min
Delta R.T.: -0.005 min
Response: 12025603
Conc: 29.96 ng/ml

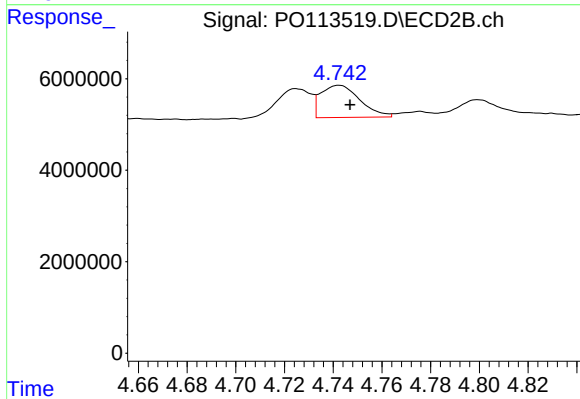

#4 AR-1016-2


R.T.: 4.743 min
Delta R.T.: -0.004 min
Response: 7855172
Conc: 30.49 ng/ml

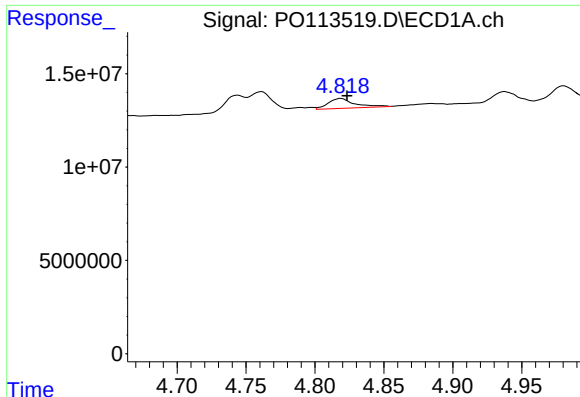

#5 AR-1016-3


R.T.: 4.819 min
Delta R.T.: -0.004 min
Response: 7021356
Conc: 27.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

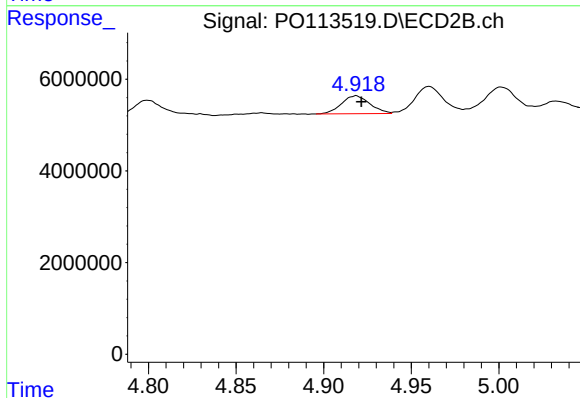


#5 AR-1016-3

R.T.: 4.919 min
Delta R.T.: -0.003 min
Response: 4408214
Conc: 31.57 ng/ml

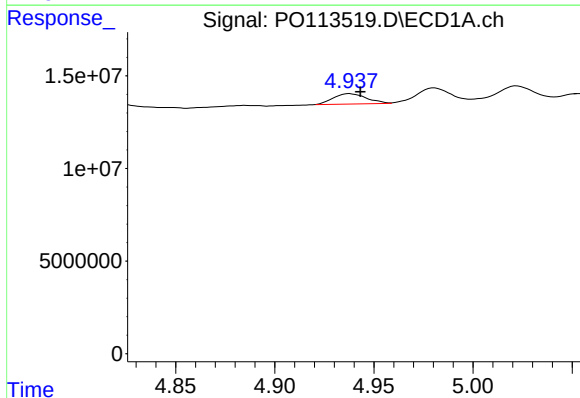


#6 AR-1016-4

R.T.: 4.938 min
Delta R.T.: -0.005 min
Response: 6545402
Conc: 30.02 ng/ml

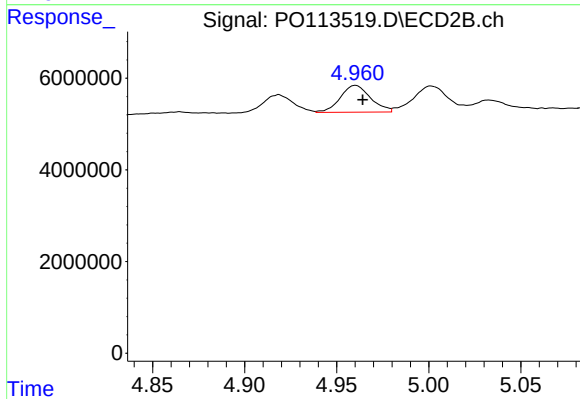

#6 AR-1016-4


R.T.: 4.960 min
Delta R.T.: -0.004 min
Response: 6684983
Conc: 57.28 ng/ml

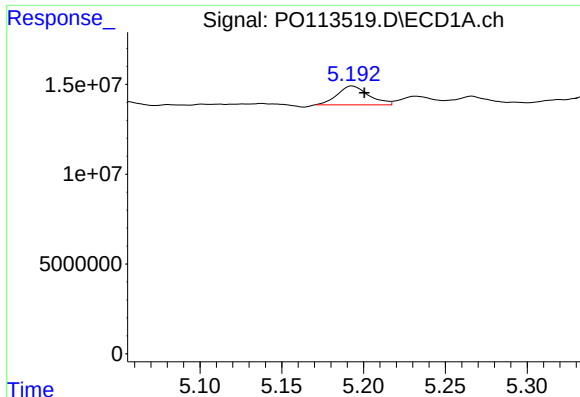

#7 AR-1016-5


R.T.: 5.193 min
Delta R.T.: -0.007 min
Response: 13977612
Conc: 63.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

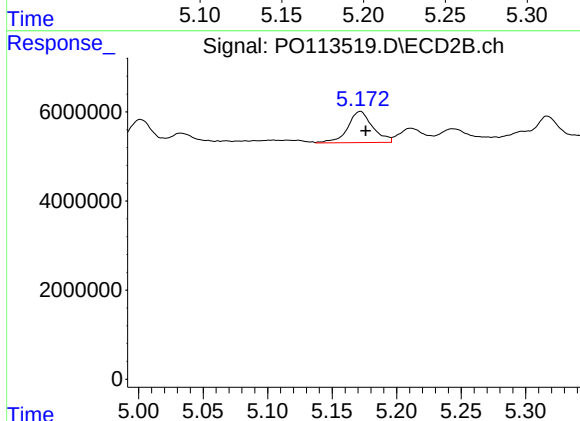


#7 AR-1016-5

R.T.: 5.172 min
Delta R.T.: -0.004 min
Response: 9460432
Conc: 66.38 ng/ml

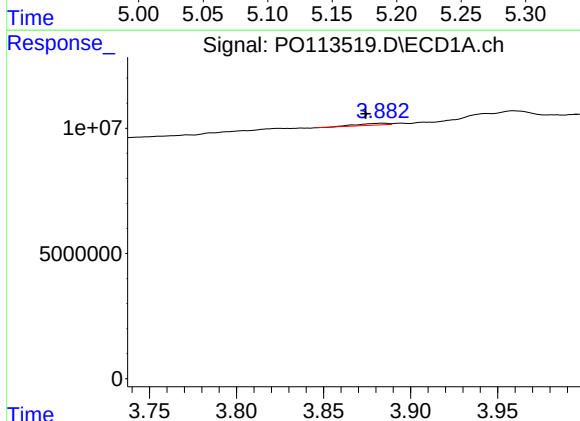


#8 AR-1221-1

R.T.: 3.884 min
Delta R.T.: 0.010 min
Response: 829745
Conc: 8.87 ng/ml

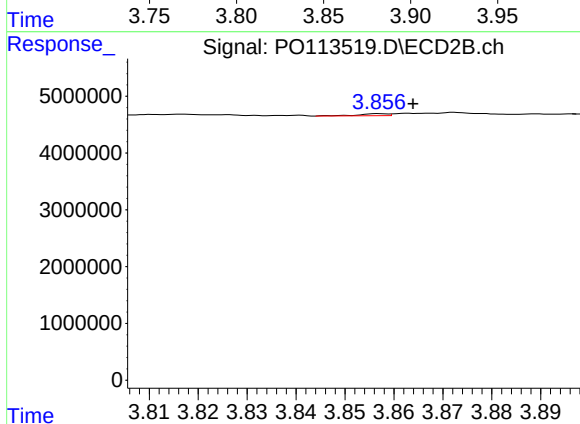

#8 AR-1221-1


R.T.: 3.857 min
Delta R.T.: -0.007 min
Response: 143951
Conc: 2.28 ng/ml

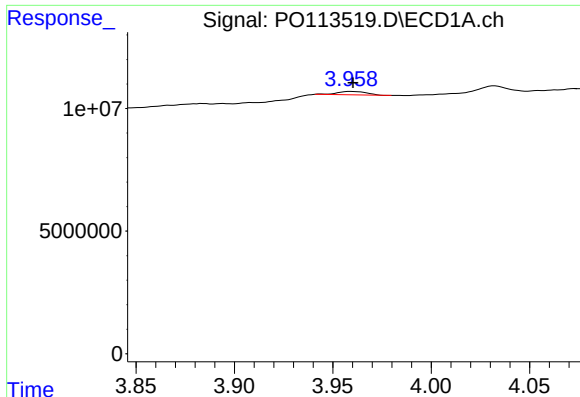

#9 AR-1221-2


R.T.: 3.959 min
Delta R.T.: -0.001 min
Response: 1432431
Conc: 21.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

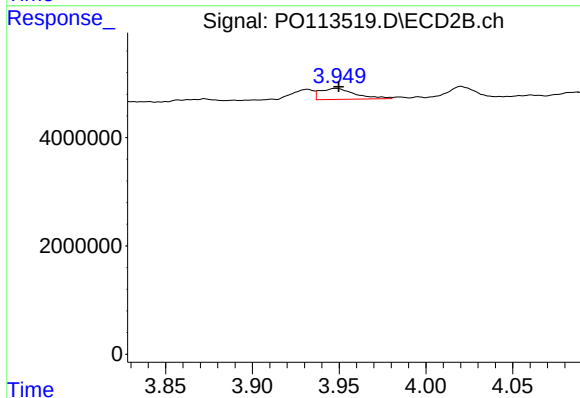


#9 AR-1221-2

R.T.: 3.948 min
Delta R.T.: -0.002 min
Response: 2874052
Conc: 61.58 ng/ml

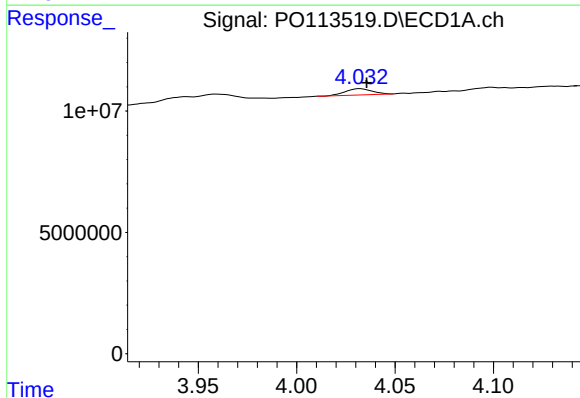


#10 AR-1221-3

R.T.: 4.032 min
Delta R.T.: -0.003 min
Response: 2497753
Conc: 11.28 ng/ml

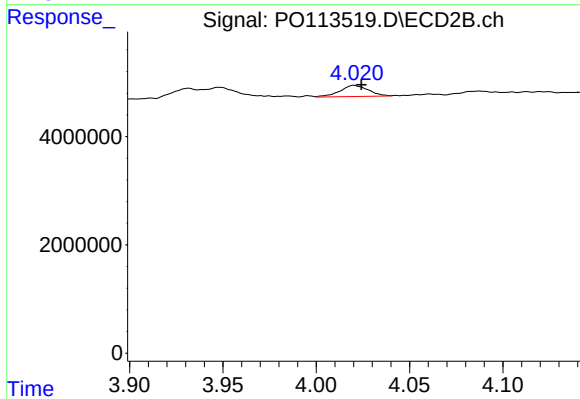

#10 AR-1221-3


R.T.: 4.020 min
Delta R.T.: -0.004 min
Response: 2191970
Conc: 14.76 ng/ml

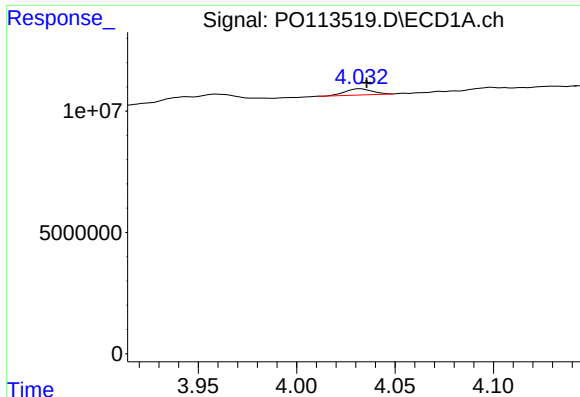

#11 AR-1232-1


R.T.: 4.032 min
Delta R.T.: -0.003 min
Response: 2497753
Conc: 14.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

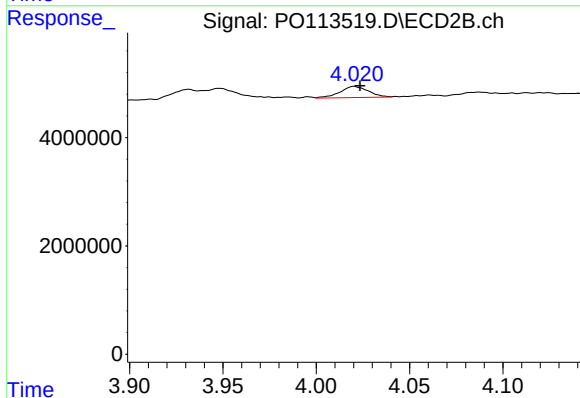


#11 AR-1232-1

R.T.: 4.020 min
Delta R.T.: -0.003 min
Response: 2191970
Conc: 18.67 ng/ml

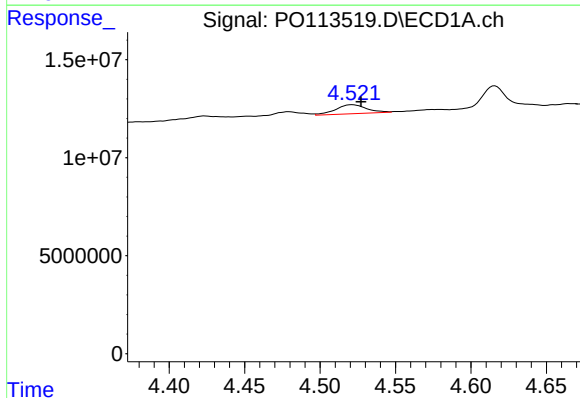


#12 AR-1232-2

R.T.: 4.521 min
Delta R.T.: -0.006 min
Response: 6539392
Conc: 65.49 ng/ml

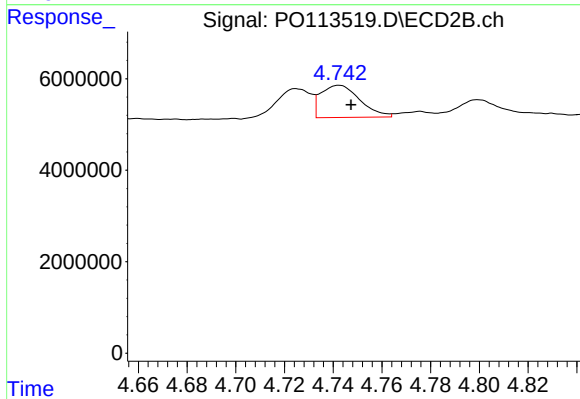

#12 AR-1232-2


R.T.: 4.743 min
Delta R.T.: -0.005 min
Response: 7855172
Conc: 64.10 ng/ml

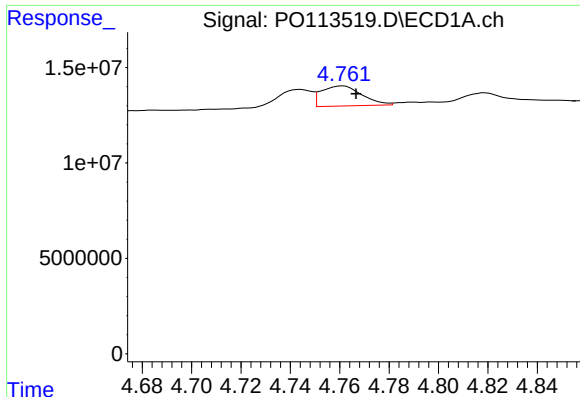

#13 AR-1232-3


R.T.: 4.761 min
Delta R.T.: -0.005 min
Response: 12025603
Conc: 63.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

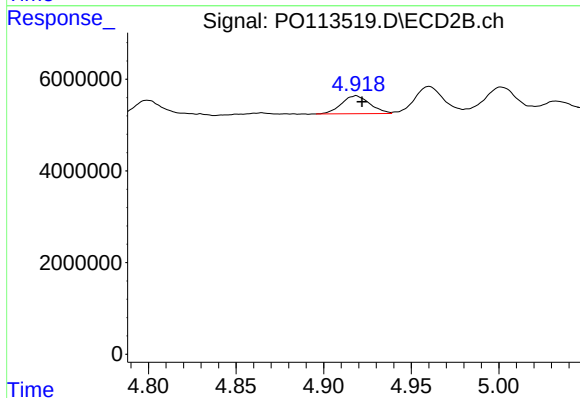


#13 AR-1232-3

R.T.: 4.919 min
Delta R.T.: -0.003 min
Response: 4408214
Conc: 69.59 ng/ml

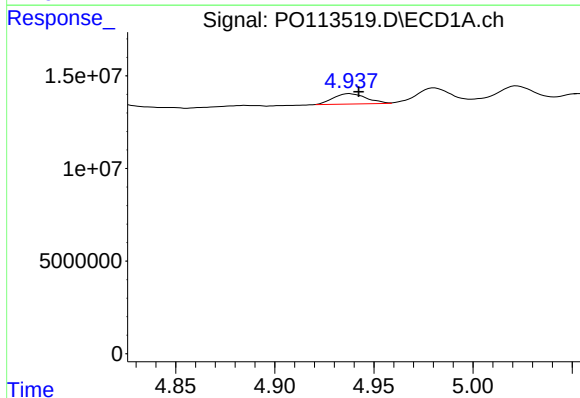


#14 AR-1232-4

R.T.: 4.938 min
Delta R.T.: -0.004 min
Response: 6545402
Conc: 69.51 ng/ml

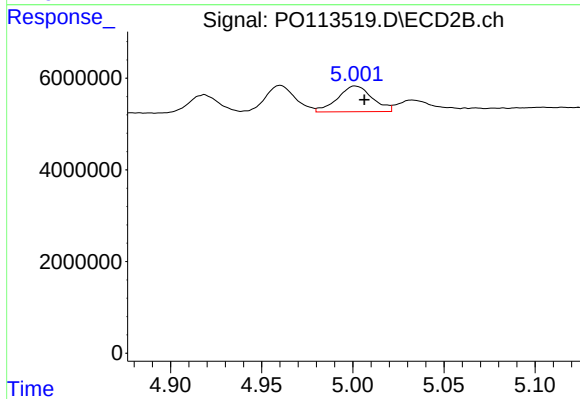

#14 AR-1232-4


R.T.: 5.001 min
Delta R.T.: -0.005 min
Response: 7460183
Conc: 132.69 ng/ml

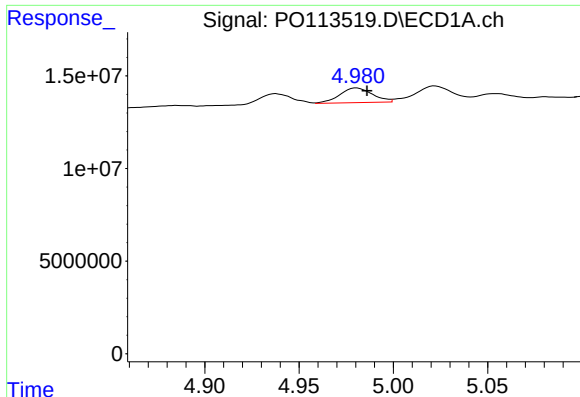

#15 AR-1232-5


R.T.: 4.981 min
Delta R.T.: -0.005 min
Response: 9510851
Conc: 153.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

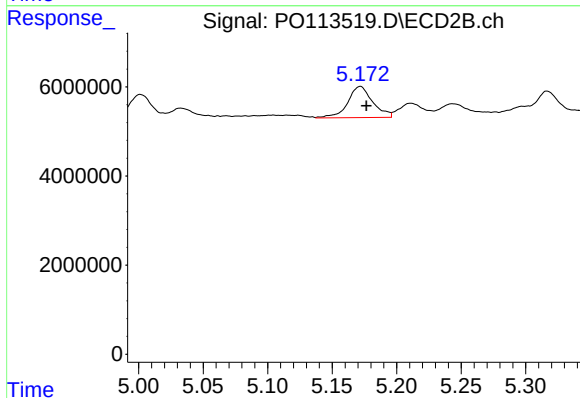


#15 AR-1232-5

R.T.: 5.172 min
Delta R.T.: -0.004 min
Response: 9460432
Conc: 158.03 ng/ml

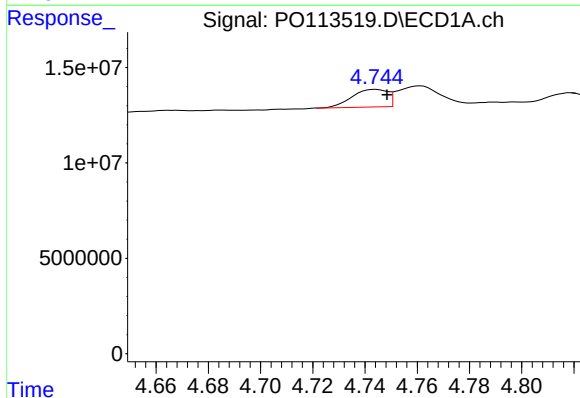


#16 AR-1242-1

R.T.: 4.744 min
Delta R.T.: -0.004 min
Response: 8710356
Conc: 37.88 ng/ml

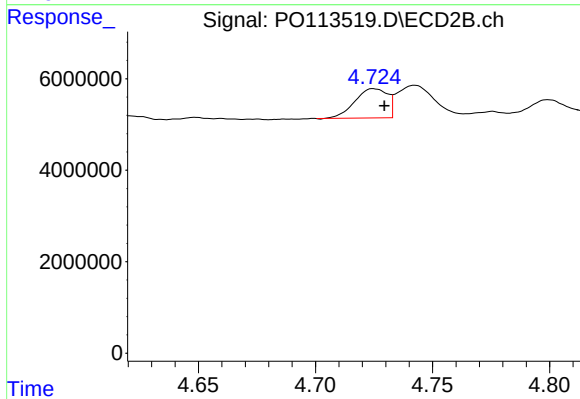

#16 AR-1242-1


R.T.: 4.725 min
Delta R.T.: -0.005 min
Response: 6216828
Conc: 43.02 ng/ml

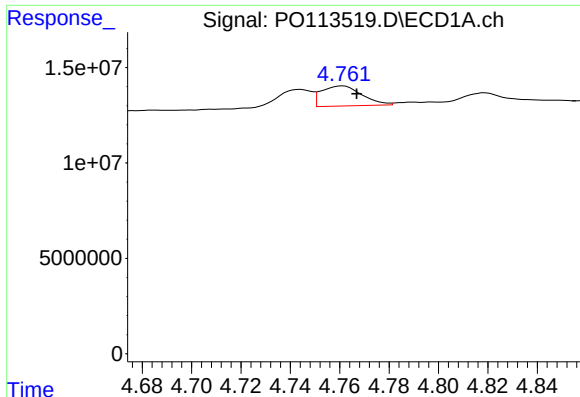

#17 AR-1242-2


R.T.: 4.761 min
Delta R.T.: -0.006 min
Response: 12025603
Conc: 35.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

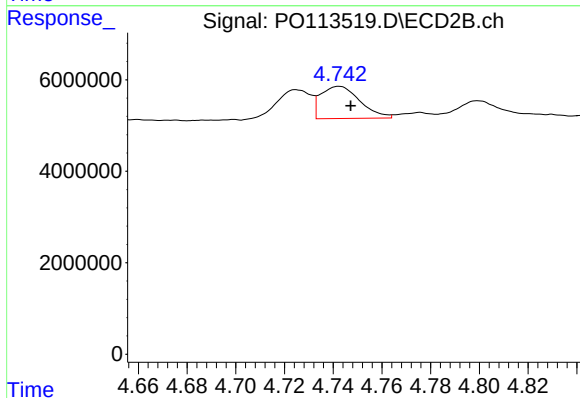


#17 AR-1242-2

R.T.: 4.743 min
Delta R.T.: -0.005 min
Response: 7855172
Conc: 36.21 ng/ml

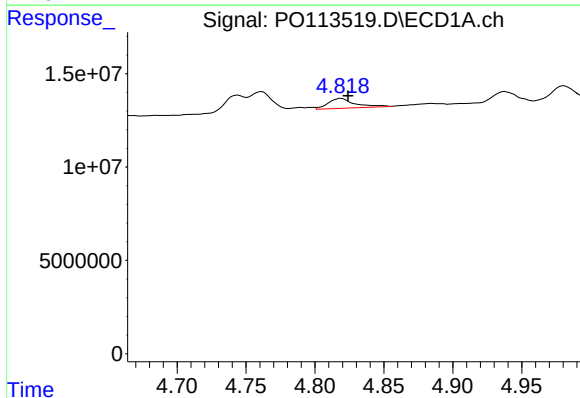


#18 AR-1242-3

R.T.: 4.819 min
Delta R.T.: -0.005 min
Response: 7021356
Conc: 31.64 ng/ml

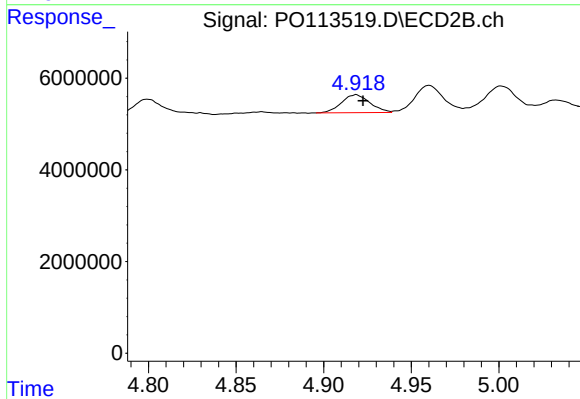

#18 AR-1242-3


R.T.: 4.919 min
Delta R.T.: -0.004 min
Response: 4408214
Conc: 37.69 ng/ml

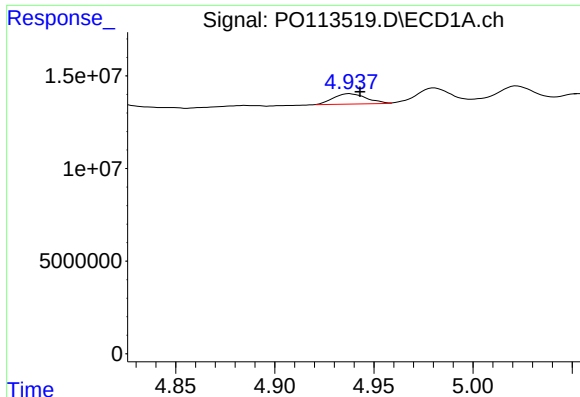

#19 AR-1242-4


R.T.: 4.938 min
Delta R.T.: -0.005 min
Response: 6545402
Conc: 37.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

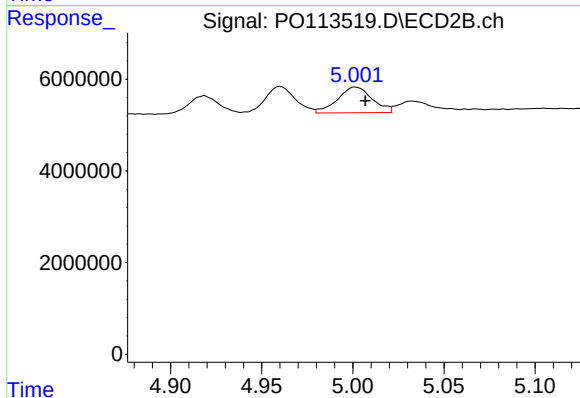


#19 AR-1242-4

R.T.: 5.001 min
Delta R.T.: -0.006 min
Response: 7460183
Conc: 63.42 ng/ml

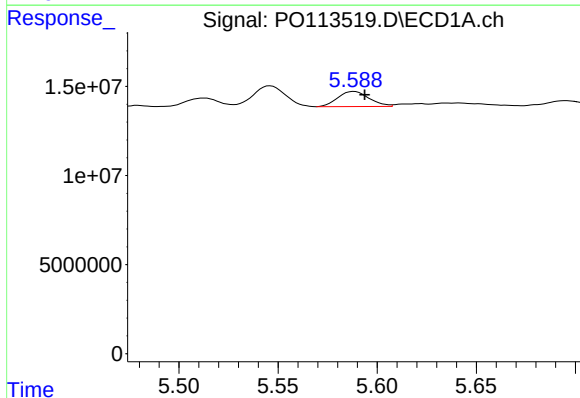


#20 AR-1242-5

R.T.: 5.588 min
Delta R.T.: -0.005 min
Response: 9387937
Conc: 46.90 ng/ml

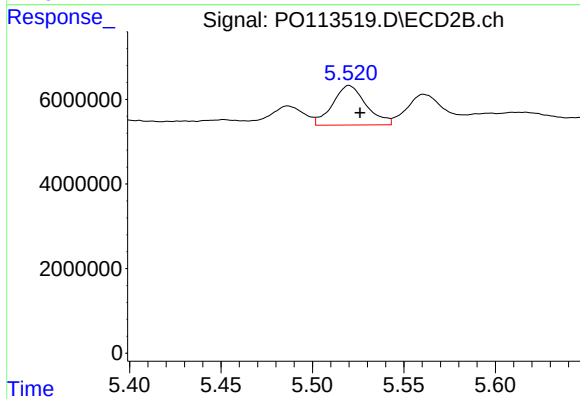

#20 AR-1242-5


R.T.: 5.520 min
Delta R.T.: -0.006 min
Response: 11939049
Conc: 80.06 ng/ml

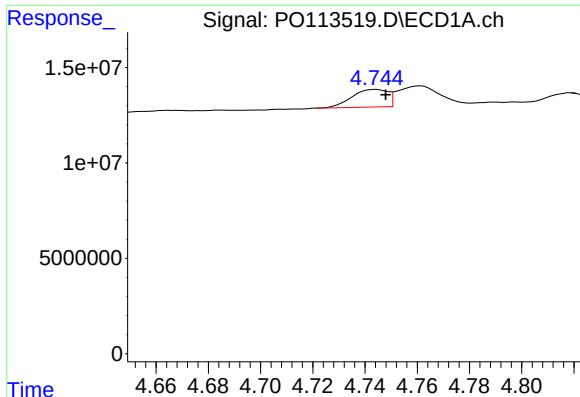

#21 AR-1248-1


R.T.: 4.744 min
Delta R.T.: -0.004 min
Response: 8710356
Conc: 49.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

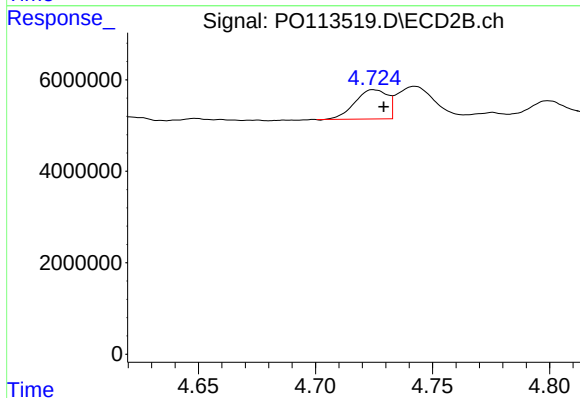


#21 AR-1248-1

R.T.: 4.725 min
Delta R.T.: -0.005 min
Response: 6216828
Conc: 55.75 ng/ml

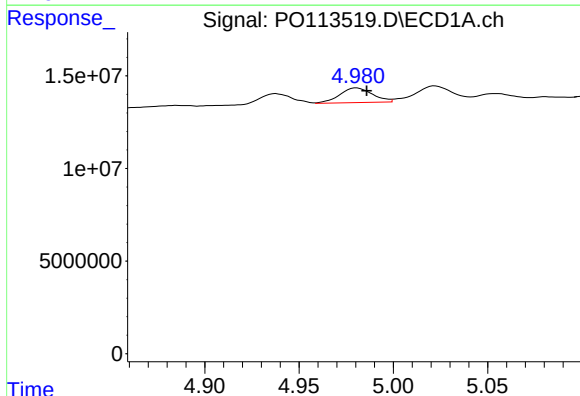


#22 AR-1248-2

R.T.: 4.981 min
Delta R.T.: -0.005 min
Response: 9510851
Conc: 39.32 ng/ml

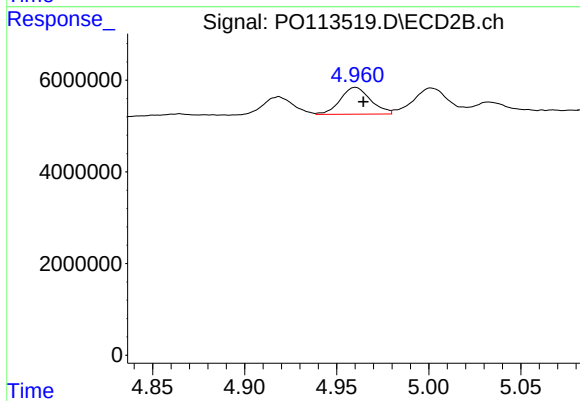

#22 AR-1248-2


R.T.: 4.960 min
Delta R.T.: -0.004 min
Response: 6684983
Conc: 41.60 ng/ml

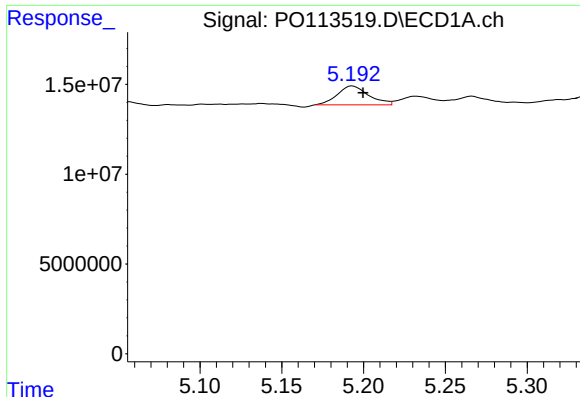

#23 AR-1248-3


R.T.: 5.193 min
Delta R.T.: -0.006 min
Response: 13977612
Conc: 43.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

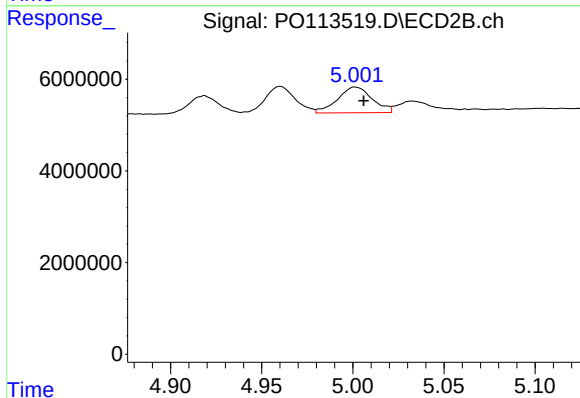


#23 AR-1248-3

R.T.: 5.001 min
Delta R.T.: -0.005 min
Response: 7460183
Conc: 43.97 ng/ml

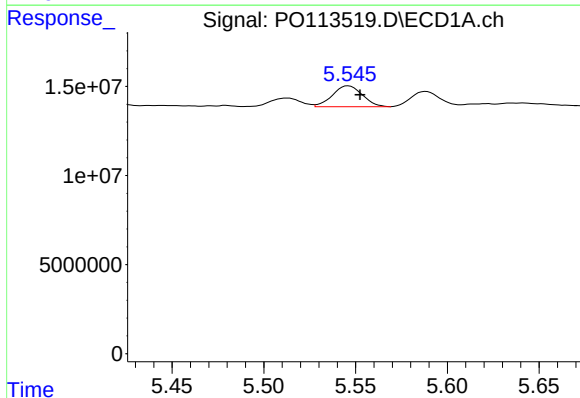


#24 AR-1248-4

R.T.: 5.546 min
Delta R.T.: -0.006 min
Response: 13268197
Conc: 26.56 ng/ml

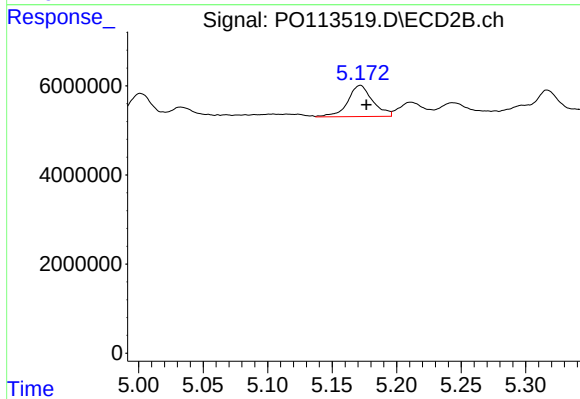

#24 AR-1248-4


R.T.: 5.172 min
Delta R.T.: -0.005 min
Response: 9460432
Conc: 47.49 ng/ml

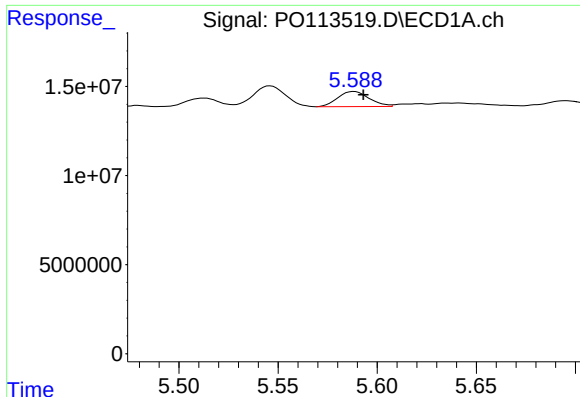

#25 AR-1248-5


R.T.: 5.588 min
Delta R.T.: -0.005 min
Response: 9387937
Conc: 27.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

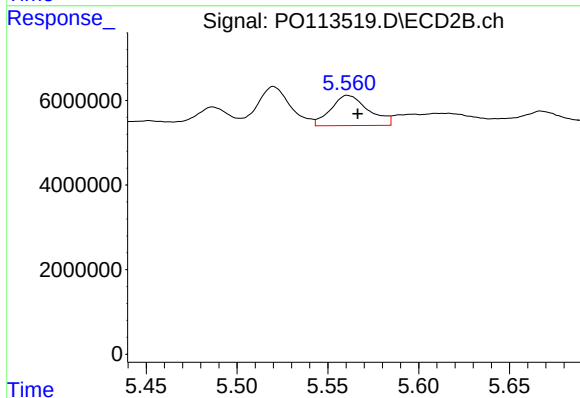


#25 AR-1248-5

R.T.: 5.561 min
Delta R.T.: -0.006 min
Response: 10354179
Conc: 48.77 ng/ml

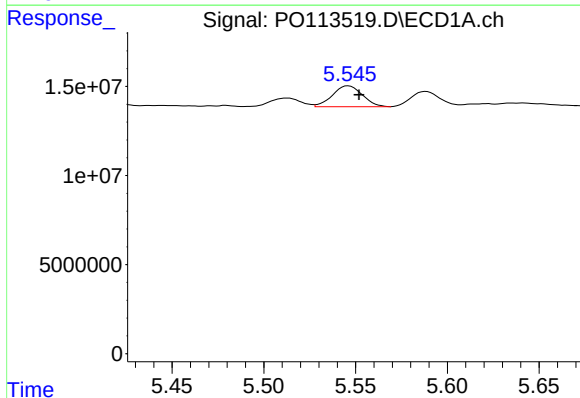


#26 AR-1254-1

R.T.: 5.546 min
Delta R.T.: -0.006 min
Response: 13268197
Conc: 24.57 ng/ml

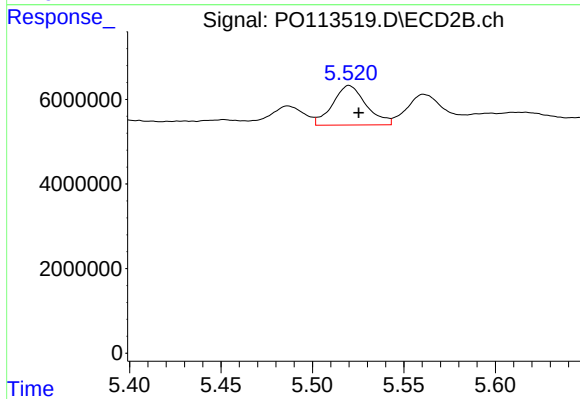

#26 AR-1254-1


R.T.: 5.520 min
Delta R.T.: -0.005 min
Response: 11939049
Conc: 37.86 ng/ml

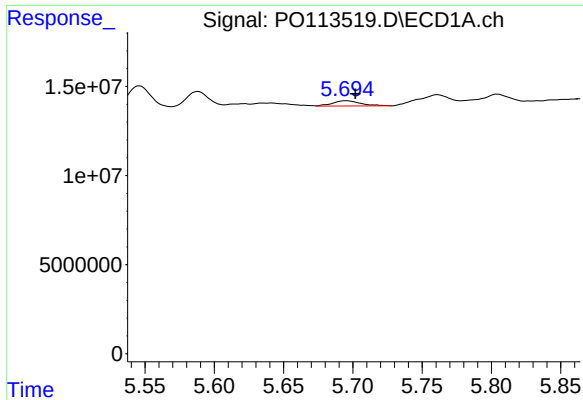

#27 AR-1254-2


R.T.: 5.695 min
Delta R.T.: -0.007 min
Response: 4122289
Conc: 8.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

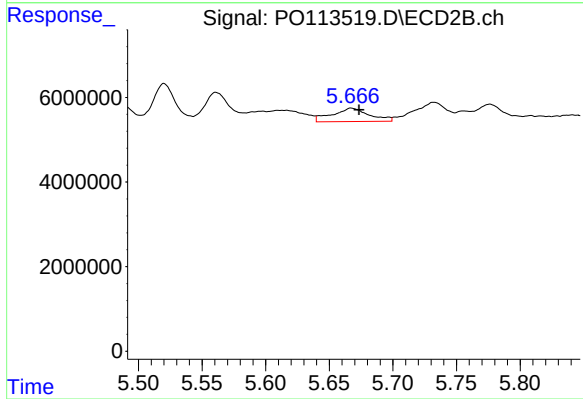


#27 AR-1254-2

R.T.: 5.667 min
Delta R.T.: -0.006 min
Response: 6427077
Conc: 22.93 ng/ml

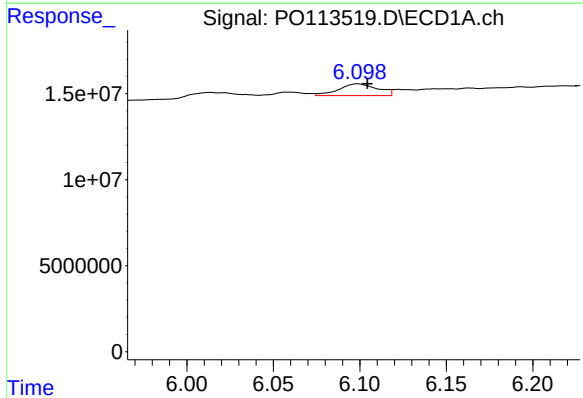


#28 AR-1254-3

R.T.: 6.099 min
Delta R.T.: -0.005 min
Response: 10735617
Conc: 14.53 ng/ml

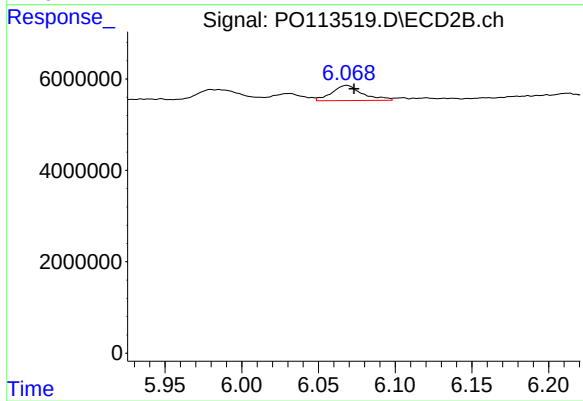

#28 AR-1254-3


R.T.: 6.068 min
Delta R.T.: -0.005 min
Response: 4588412
Conc: 11.01 ng/ml

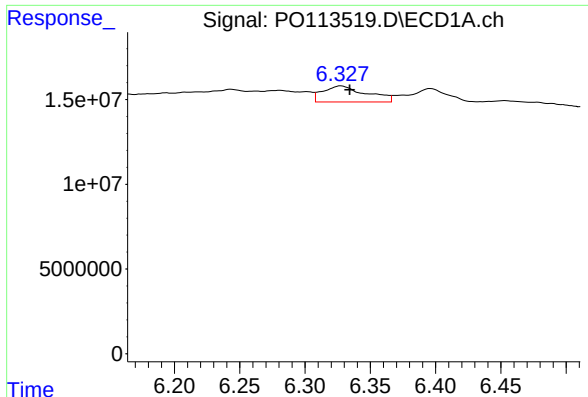

#29 AR-1254-4


R.T.: 6.327 min
Delta R.T.: -0.007 min
Response: 21952028
Conc: 39.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

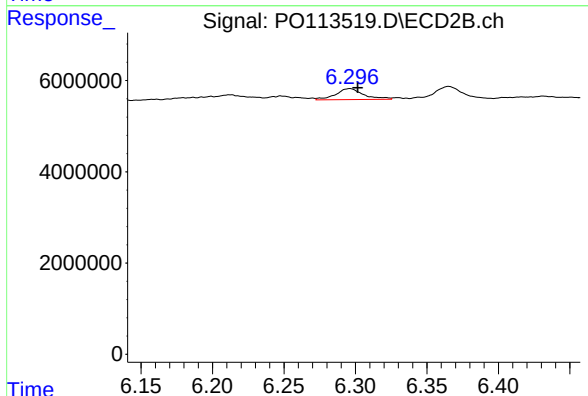


#29 AR-1254-4

R.T.: 6.296 min
Delta R.T.: -0.006 min
Response: 3273236
Conc: 11.91 ng/ml

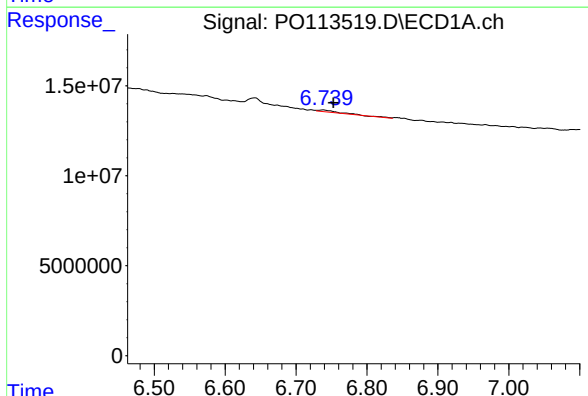


#30 AR-1254-5

R.T.: 6.739 min
Delta R.T.: -0.014 min
Response: 2359520
Conc: 3.37 ng/ml

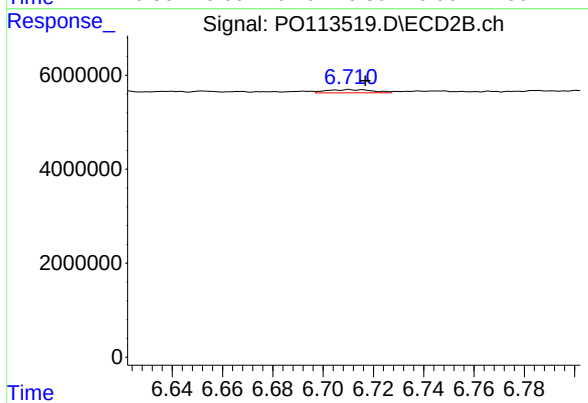

#30 AR-1254-5


R.T.: 6.710 min
Delta R.T.: -0.006 min
Response: 888477
Conc: 2.49 ng/ml

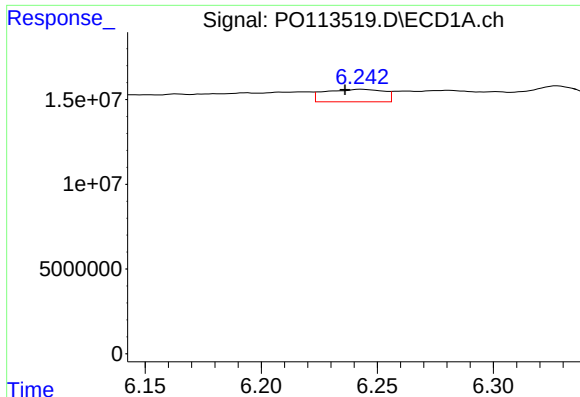

#31 AR-1260-1


R.T.: 6.243 min
Delta R.T.: 0.007 min
Response: 12939865
Conc: 29.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

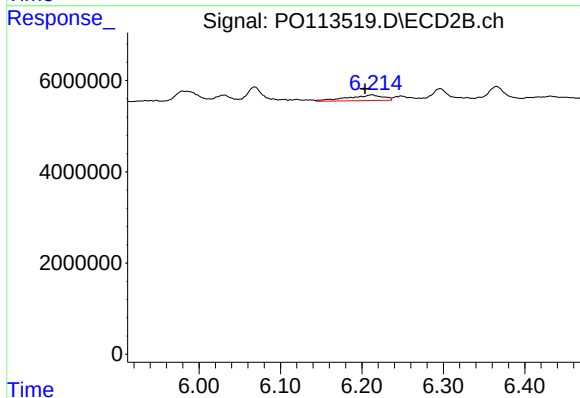


#31 AR-1260-1

R.T.: 6.213 min
Delta R.T.: 0.009 min
Response: 3767333
Conc: 14.77 ng/ml

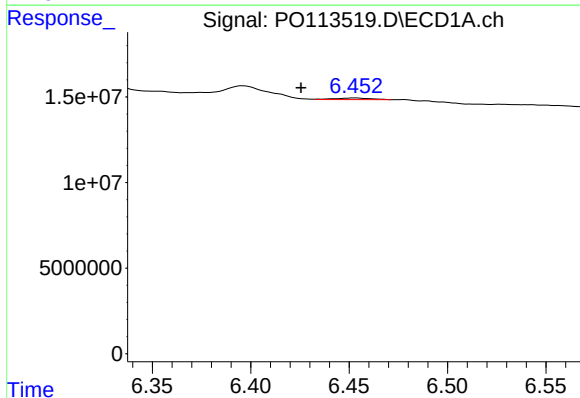


#32 AR-1260-2

R.T.: 6.453 min
Delta R.T.: 0.027 min
Response: 1124829
Conc: 1.64 ng/ml

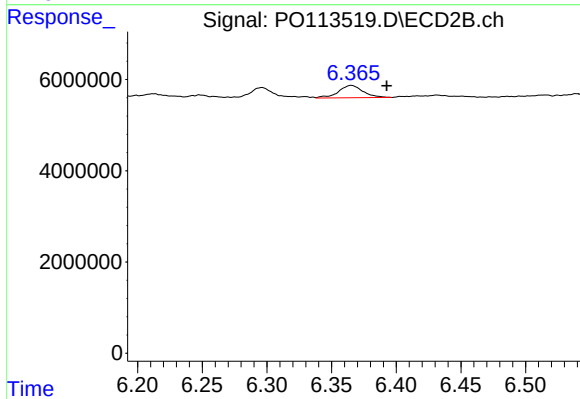

#32 AR-1260-2


R.T.: 6.365 min
Delta R.T.: -0.027 min
Response: 3623726
Conc: 10.48 ng/ml

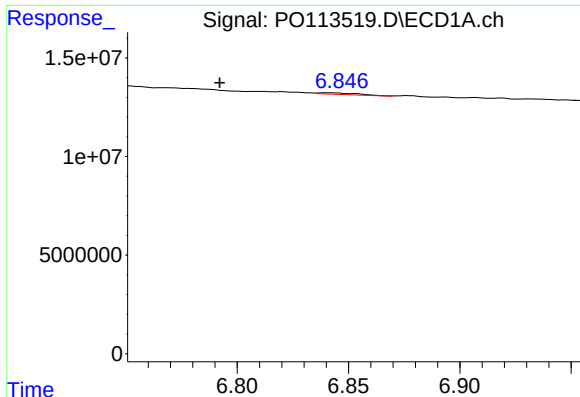

#33 AR-1260-3


R.T.: 6.842 min
Delta R.T.: 0.049 min
Response: 933834
Conc: 1.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

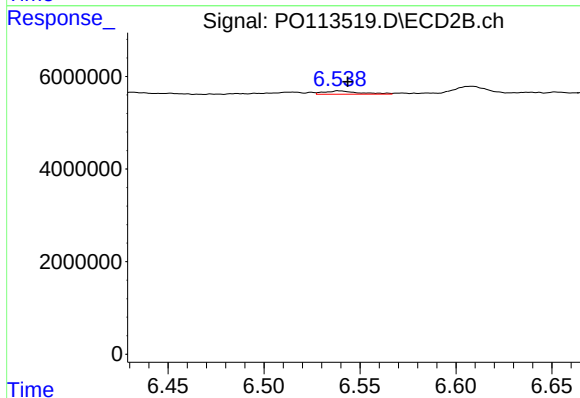


#33 AR-1260-3

R.T.: 6.539 min
Delta R.T.: -0.004 min
Response: 897454
Conc: 3.02 ng/ml

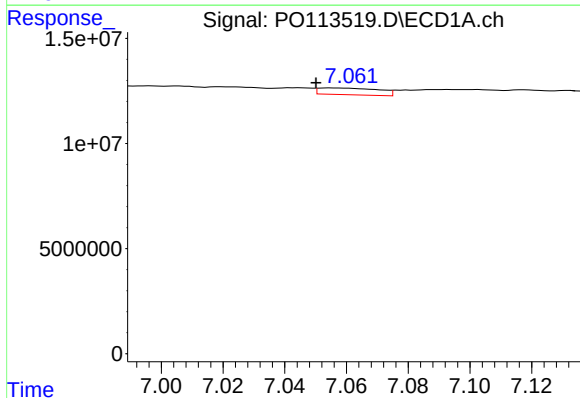


#34 AR-1260-4

R.T.: 7.055 min
Delta R.T.: 0.005 min
Response: 4293646
Conc: 9.59 ng/ml

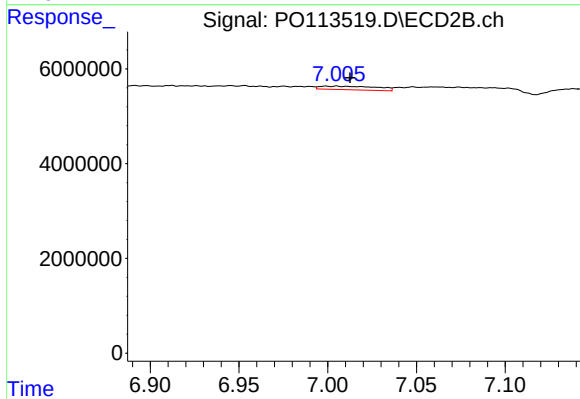

#34 AR-1260-4


R.T.: 7.005 min
Delta R.T.: -0.008 min
Response: 1658035
Conc: 8.00 ng/ml

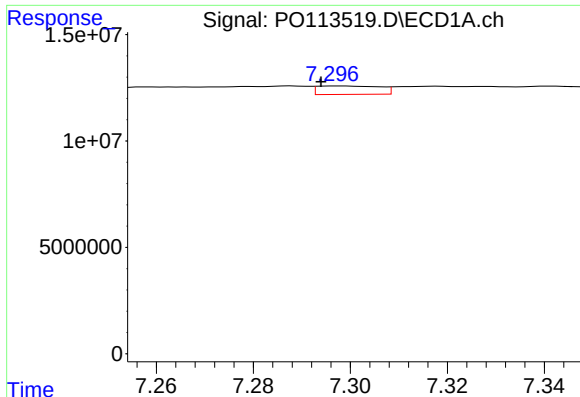

#35 AR-1260-5


R.T.: 7.298 min
Delta R.T.: 0.004 min
Response: 3569632
Conc: 2.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

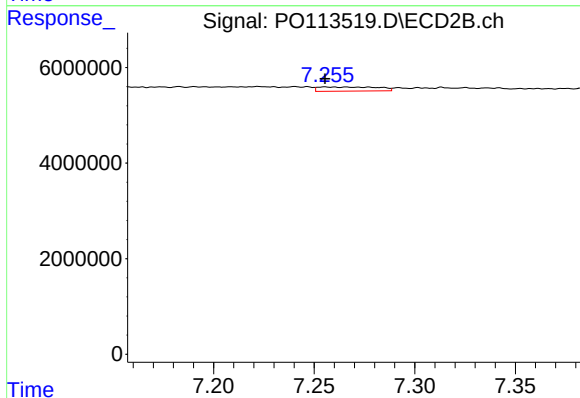


#35 AR-1260-5

R.T.: 7.255 min
Delta R.T.: 0.000 min
Response: 1791267
Conc: 3.82 ng/ml

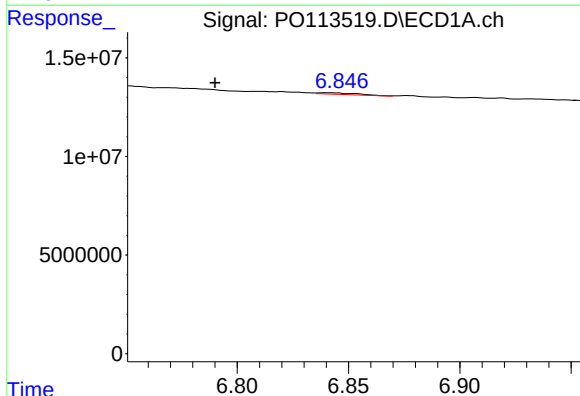


#36 AR-1262-1

R.T.: 6.842 min
Delta R.T.: 0.051 min
Response: 933834
Conc: 1.02 ng/ml

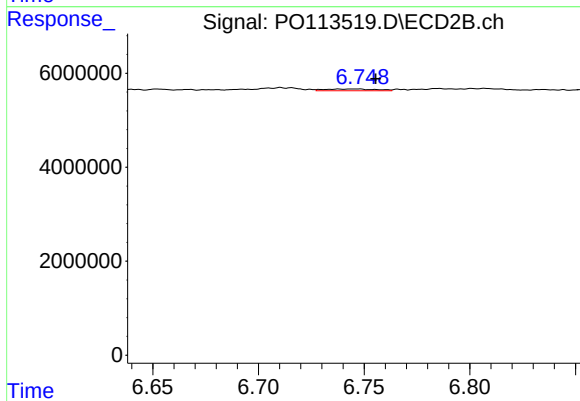

#36 AR-1262-1


R.T.: 6.747 min
Delta R.T.: -0.009 min
Response: 646127
Conc: 1.56 ng/ml

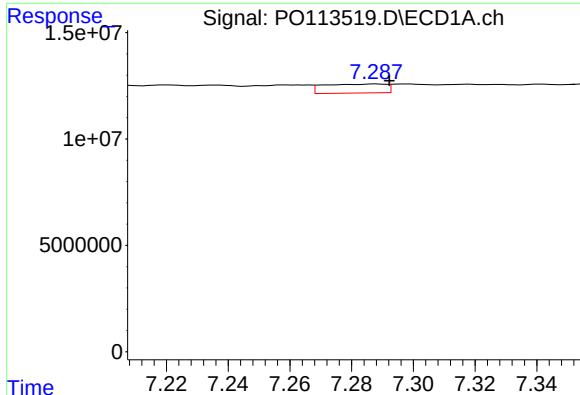

#37 AR-1262-2


R.T.: 7.288 min
Delta R.T.: -0.004 min
Response: 5972265
Conc: 3.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

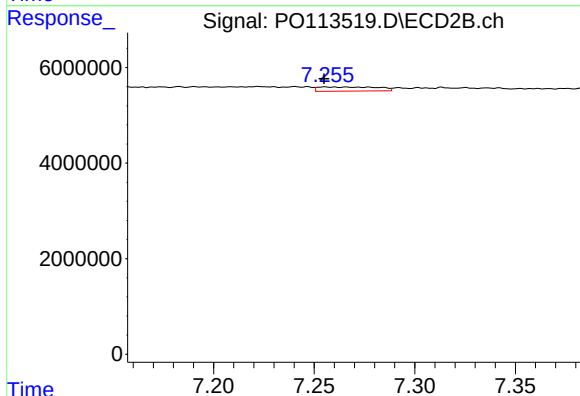


#37 AR-1262-2

R.T.: 7.255 min
Delta R.T.: 0.000 min
Response: 1791267
Conc: 3.46 ng/ml

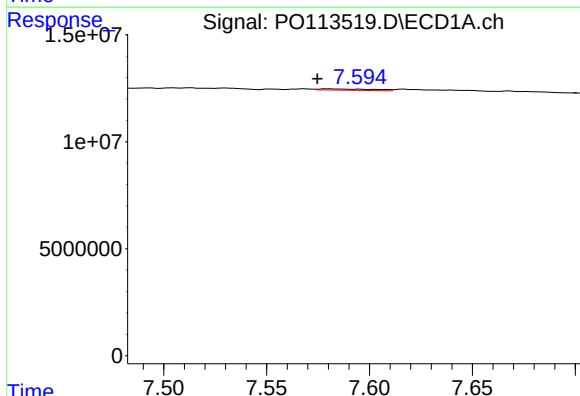


#38 AR-1262-3

R.T.: 7.580 min
Delta R.T.: 0.005 min
Response: 1166393
Conc: 2.10 ng/ml

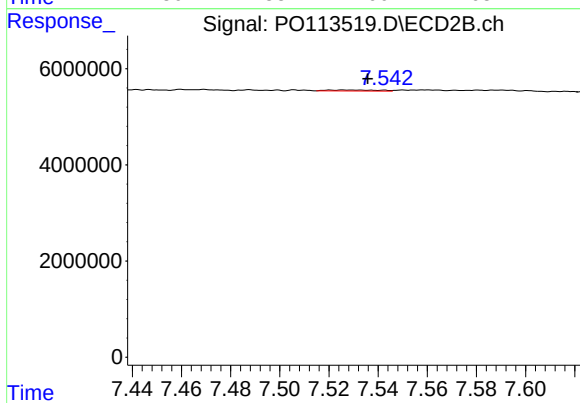

#38 AR-1262-3


R.T.: 7.521 min
Delta R.T.: -0.015 min
Response: 302760
Conc: 1.69 ng/ml

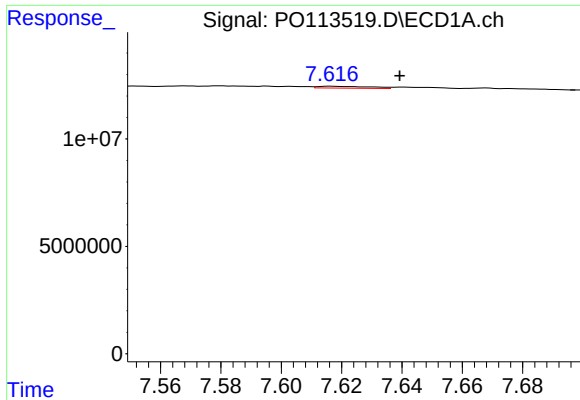

#39 AR-1262-4


R.T.: 7.617 min
Delta R.T.: -0.023 min
Response: 1084816
Conc: 1.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

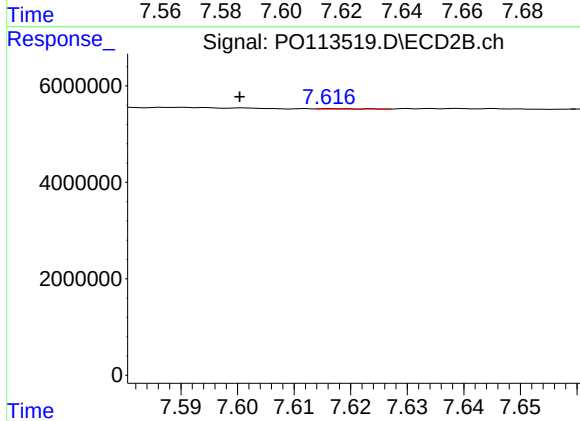


#39 AR-1262-4

R.T.: 7.616 min
Delta R.T.: 0.016 min
Response: 37138
Conc: 0.13 ng/ml

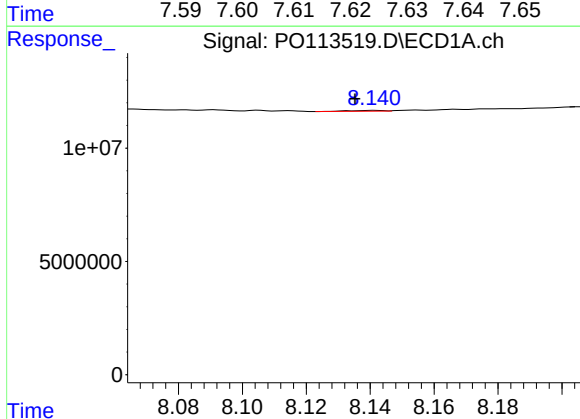


#40 AR-1262-5

R.T.: 8.141 min
Delta R.T.: 0.006 min
Response: 276620
Conc: 0.66 ng/ml

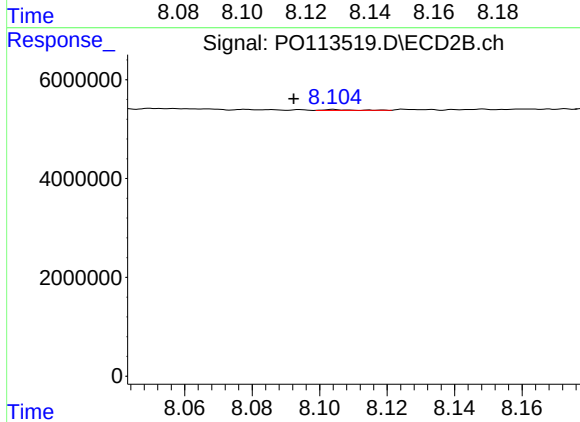

#40 AR-1262-5


R.T.: 8.104 min
Delta R.T.: 0.012 min
Response: 104043
Conc: 0.96 ng/ml

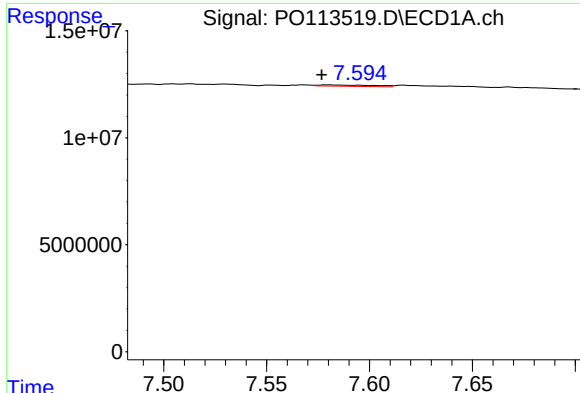

#41 AR-1268-1


R.T.: 7.580 min
Delta R.T.: 0.003 min
Response: 1166393
Conc: 0.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

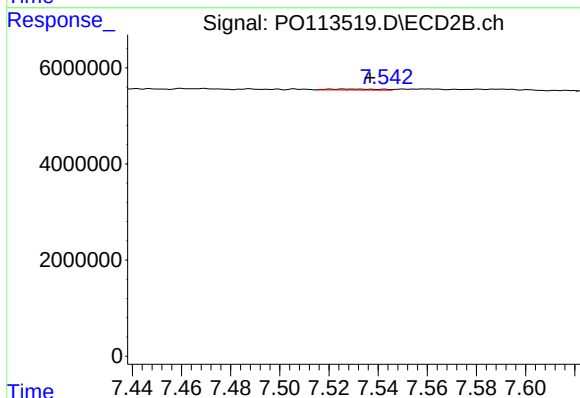


#41 AR-1268-1

R.T.: 7.521 min
Delta R.T.: -0.016 min
Response: 302760
Conc: 0.59 ng/ml

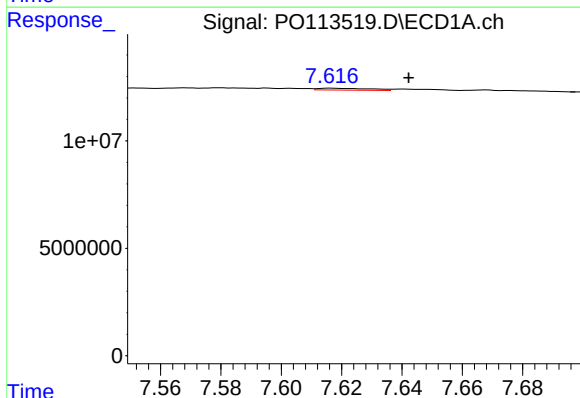


#42 AR-1268-2

R.T.: 7.617 min
Delta R.T.: -0.025 min
Response: 1084816
Conc: 0.75 ng/ml

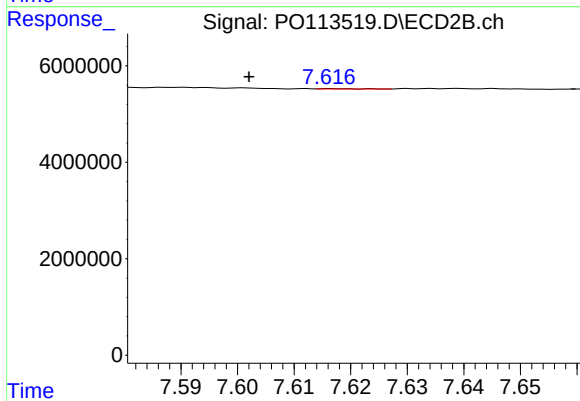

#42 AR-1268-2


R.T.: 7.616 min
Delta R.T.: 0.014 min
Response: 37138
Conc: 0.09 ng/ml

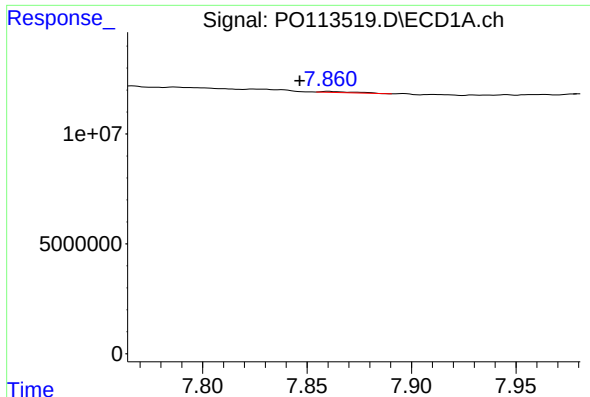

#43 AR-1268-3


R.T.: 7.860 min
Delta R.T.: 0.014 min
Response: 439395
Conc: 0.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

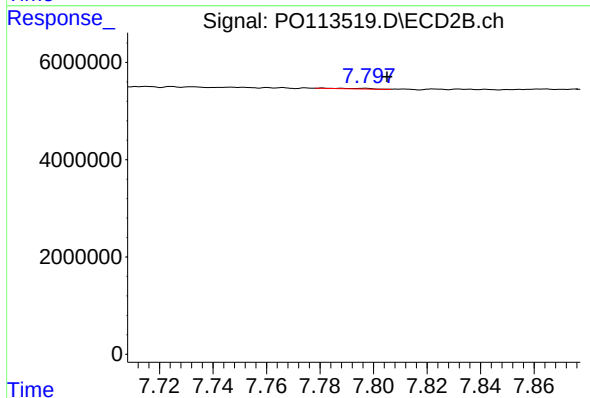


#43 AR-1268-3

R.T.: 7.797 min
Delta R.T.: -0.008 min
Response: 113726
Conc: 0.35 ng/ml

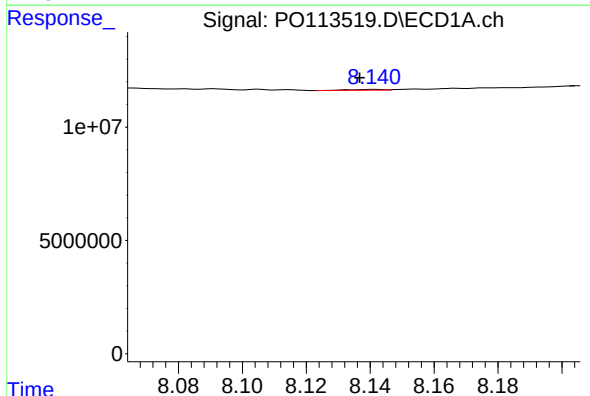


#44 AR-1268-4

R.T.: 8.141 min
Delta R.T.: 0.004 min
Response: 276620
Conc: 0.60 ng/ml

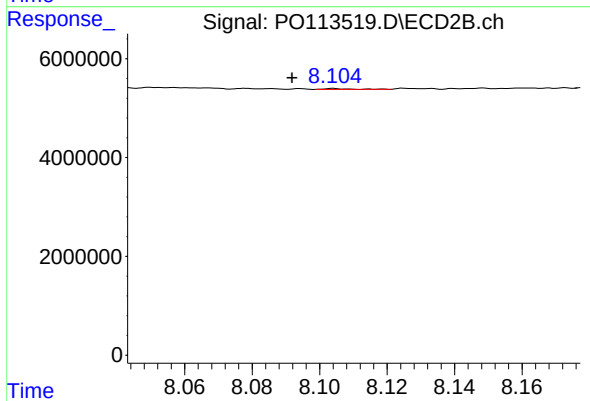

#44 AR-1268-4


R.T.: 8.104 min
Delta R.T.: 0.012 min
Response: 104043
Conc: 0.86 ng/ml

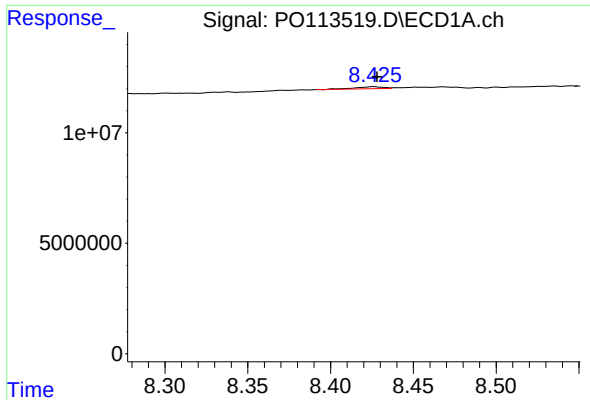

#45 AR-1268-5

R.T.: 8.426 min
Delta R.T.: -0.002 min
Response: 1070739
Conc: 0.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

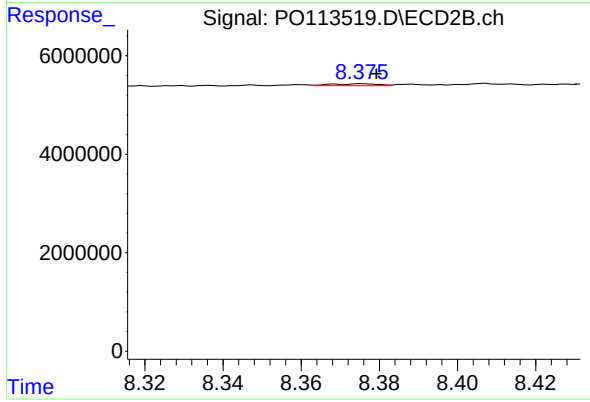

#45 AR-1268-5

R.T.: 8.376 min
Delta R.T.: -0.004 min
Response: 306777
Conc: 0.39 ng/ml