

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0090525\
 Data File : P0113520.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 19:27
 Operator : YP/AJ
 Sample : Q2893-09
 Misc : AR1248 WATER LOD 25PPB
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:35:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.652	164.4E6	97864724	20.087	19.338
2) SA Decachlor...	8.672	8.620	103.7E6	34790180	14.962	18.360
Target Compounds						
3) L1 AR-1016-1	4.748	4.730	567759	103234	2.127	0.605 #
4) L1 AR-1016-2	4.774	4.742	280555	49965	0.699	0.194 #
5) L1 AR-1016-3	4.849	4.920	442672	90191	1.736	0.646 #
6) L1 AR-1016-4	4.944	4.968	40779	853564	0.187	7.314 #
7) L1 AR-1016-5	5.200	5.177	859994	253636	3.880	1.780 #
8) L2 AR-1221-1	3.825f	3.871	1399084	526036	14.952	8.334 #
9) L2 AR-1221-2	3.959	3.949	1846365	1827826	27.333	39.162 #
10) L2 AR-1221-3	0.000	4.028	0	183945	N.D.	1.239 #
11) L3 AR-1232-1	0.000	4.028	0	183945	N.D.	1.567 #
12) L3 AR-1232-2	4.513	4.742	1022989	49965	10.245	0.408 #
13) L3 AR-1232-3	4.774	4.920	280555	90191	1.481	1.424
14) L3 AR-1232-4	4.944	5.005	40779	426121	0.433	7.579 #
15) L3 AR-1232-5	4.969	5.177	261629	253636	4.224	4.237
16) L4 AR-1242-1	4.748	4.730	567759	103234	2.469	0.714 #
17) L4 AR-1242-2	4.774	4.742	280555	49965	0.816	0.230 #
18) L4 AR-1242-3	4.849	4.920	442672	90191	1.995	0.771 #
19) L4 AR-1242-4	4.944	5.005	40779	426121	0.235	3.622 #
20) L4 AR-1242-5	5.588	5.520	2386423	1597170	11.922	10.710
21) L5 AR-1248-1	4.748	4.730	567759	103234	3.254	0.926 #
22) L5 AR-1248-2	4.969	4.968	261629	853564	1.082	5.312 #
23) L5 AR-1248-3	5.200	5.005	859994	426121	2.697	2.512
24) L5 AR-1248-4	5.557	5.177	6463189	253636	12.937	1.273 #
25) L5 AR-1248-5	5.588	5.571	2386423	3357498	6.988	15.815 #
26) L6 AR-1254-1	5.557	5.520	6463189	1597170	11.969	5.065 #
27) L6 AR-1254-2	5.715	5.671	1670779	381056	3.386	1.359 #
28) L6 AR-1254-3	6.127	6.071	1944755	225745	2.632	0.541 #
29) L6 AR-1254-4	6.325	6.300	3587211	292057	6.440	1.063 #
30) L6 AR-1254-5	6.770	6.720	608788	48184	0.868	0.135 #
31) L7 AR-1260-1	6.218	6.205	2816268	91057	6.315	0.357 #
32) L7 AR-1260-2	6.454	6.392	816844	19852	1.189	0.057 #
33) L7 AR-1260-3	6.770	6.541	608788	578516	0.986	1.945 #
34) L7 AR-1260-4	7.041	6.996	4448629	1030857	9.933	4.974 #
35) L7 AR-1260-5	7.291	7.260	1721027	568329	1.422	1.213
36) L8 AR-1262-1	6.770	6.761	608788	236801	0.665	0.571
37) L8 AR-1262-2	7.291	7.260	1721027	568329	1.138	1.098
38) L8 AR-1262-3	7.565	7.537	319946	216439	0.577	1.205 #
39) L8 AR-1262-4	7.641	7.584	564988	255558	0.578	0.882 #
40) L8 AR-1262-5	8.133	8.087	143415	193359	0.344	1.785 #
41) L9 AR-1268-1	7.585	7.537	812863	216439	0.472	0.425

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090525\
Data File : P0113520.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2025 19:27
Operator : YP/AJ
Sample : Q2893-09
Misc : AR1248 WATER LOD 25PPB
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 23:35:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	7.641	7.584	564988	255558	0.390	0.615 #
43)	L9 AR-1268-3	7.832	7.816	657363	-134159	0.545	N.D. #
44)	L9 AR-1268-4	8.133	8.087	143415	193359	0.311	1.606 #
45)	L9 AR-1268-5	8.426	8.371	204792	290311	0.064	0.372 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090525\
Data File : PO113520.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2025 19:27
Operator : YP/AJ
Sample : Q2893-09
Misc : AR1248 WATER LOD 25PPB
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 23:35:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

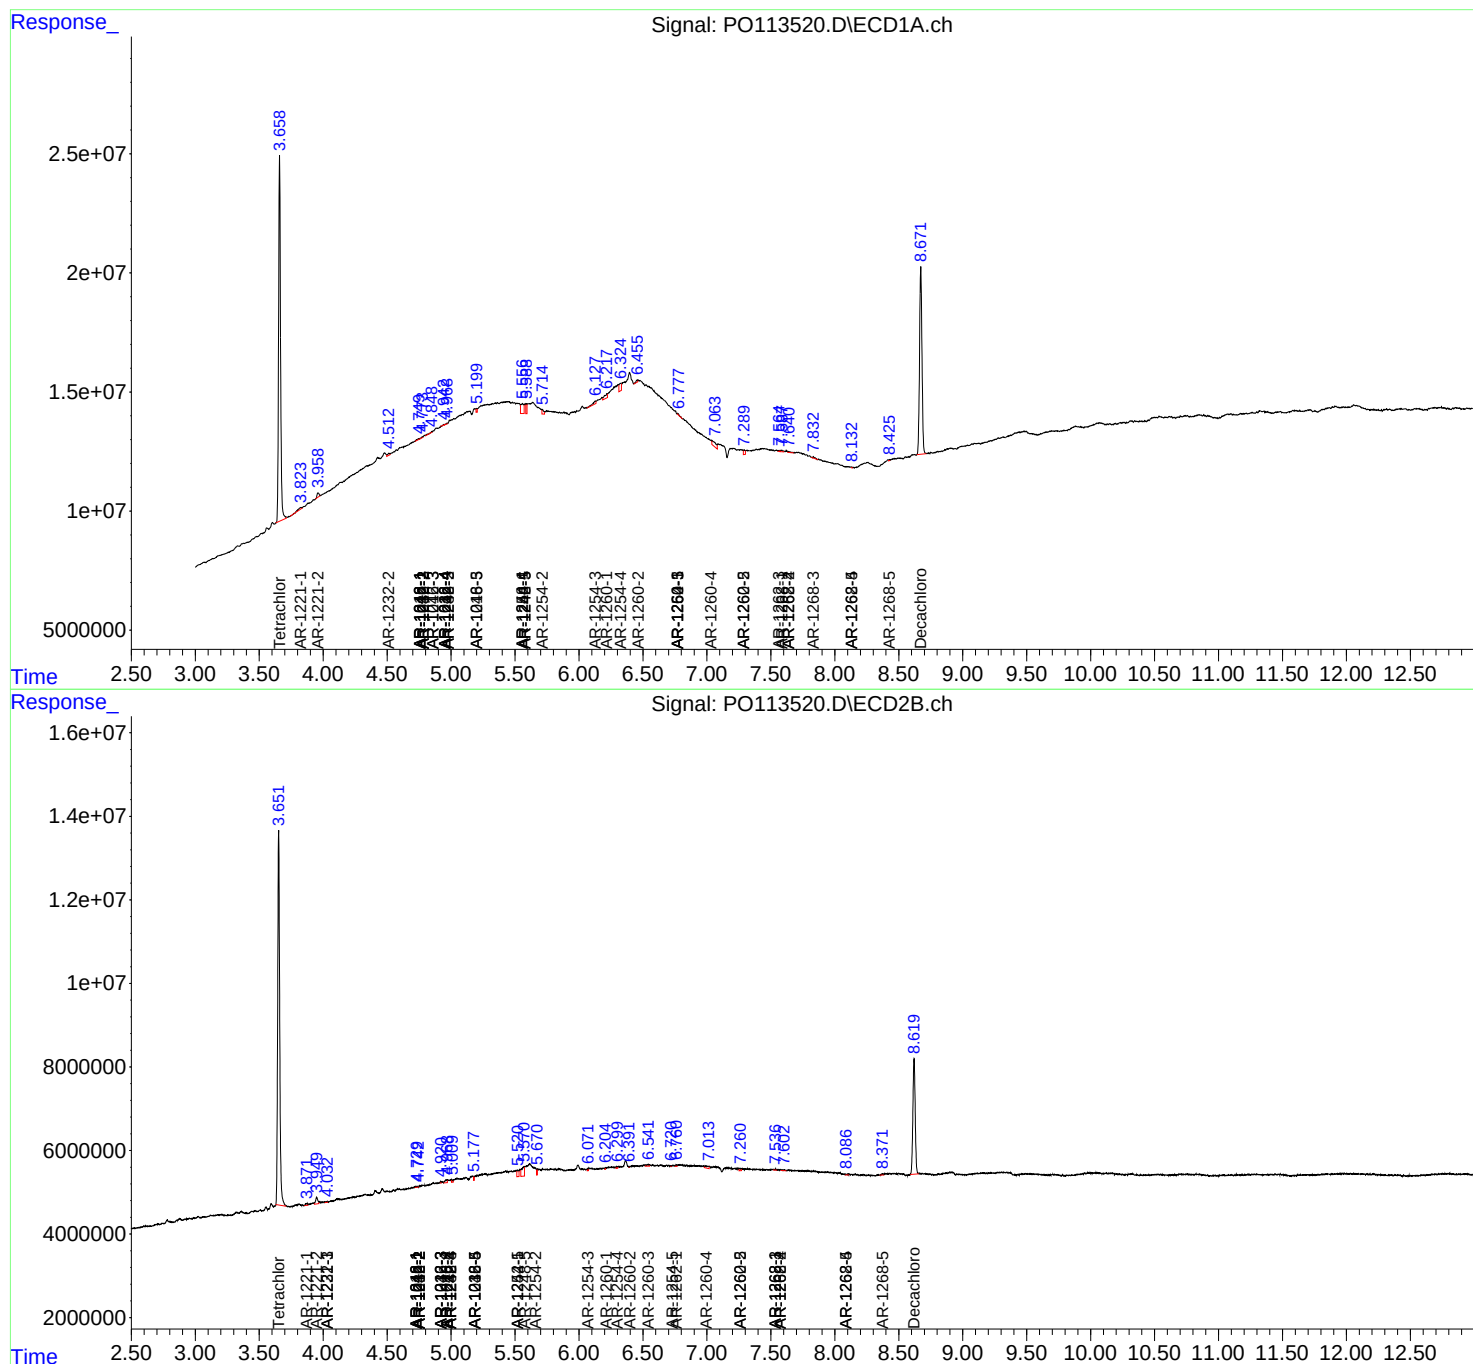


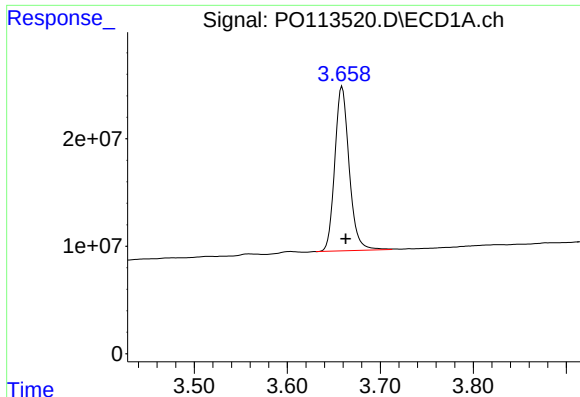

#1 Tetrachloro-m-xylene


R.T.: 3.659 min
Delta R.T.: -0.004 min
Response: 164442831
Conc: 20.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

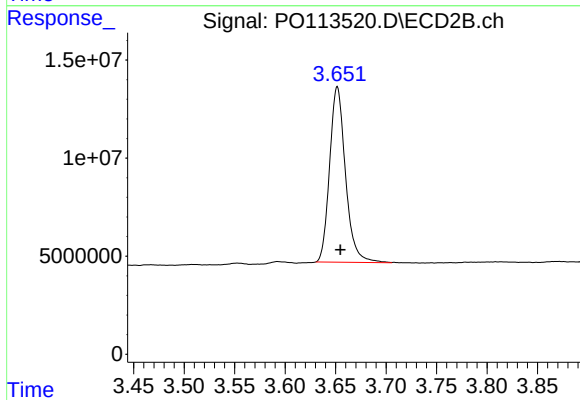


#1 Tetrachloro-m-xylene

R.T.: 3.652 min
Delta R.T.: -0.003 min
Response: 97864724
Conc: 19.34 ng/ml

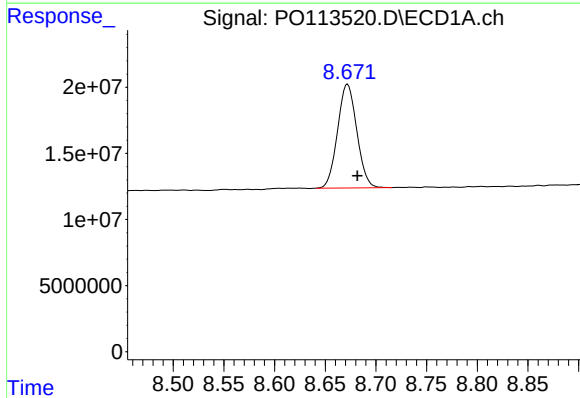


#2 Decachlorobiphenyl

R.T.: 8.672 min
Delta R.T.: -0.009 min
Response: 103707055
Conc: 14.96 ng/ml

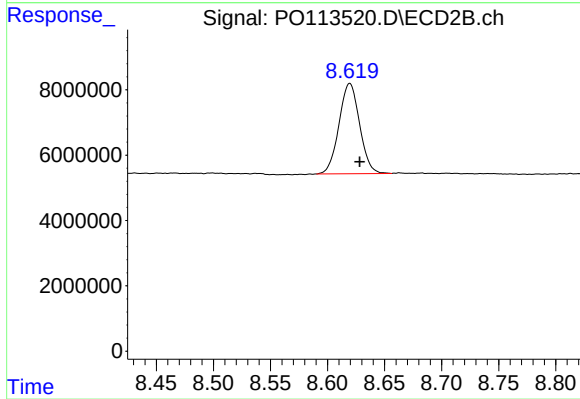

#2 Decachlorobiphenyl


R.T.: 8.620 min
Delta R.T.: -0.009 min
Response: 34790180
Conc: 18.36 ng/ml

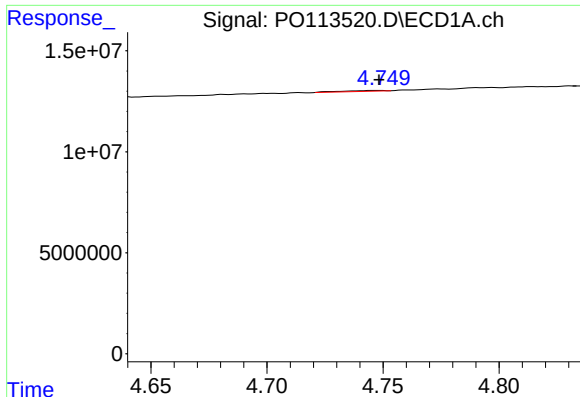

#3 AR-1016-1


R.T.: 4.748 min
Delta R.T.: 0.000 min
Response: 567759
Conc: 2.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

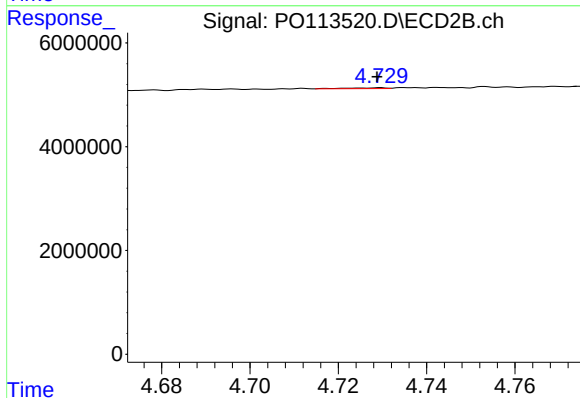


#3 AR-1016-1

R.T.: 4.730 min
Delta R.T.: 0.000 min
Response: 103234
Conc: 0.61 ng/ml

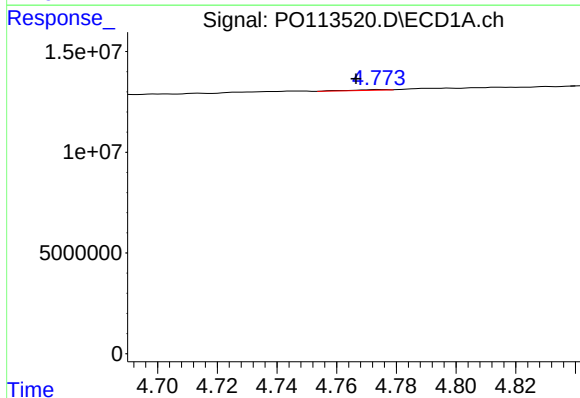


#4 AR-1016-2

R.T.: 4.774 min
Delta R.T.: 0.008 min
Response: 280555
Conc: 0.70 ng/ml

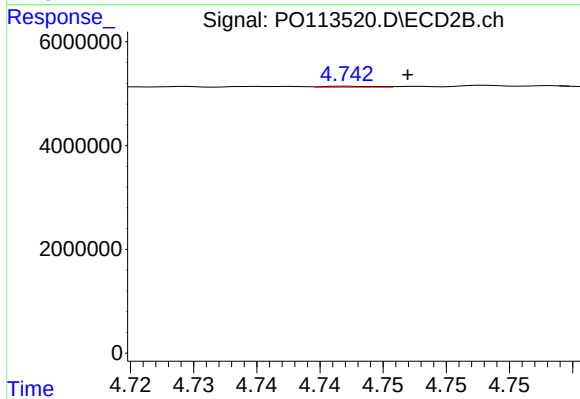

#4 AR-1016-2


R.T.: 4.742 min
Delta R.T.: -0.005 min
Response: 49965
Conc: 0.19 ng/ml

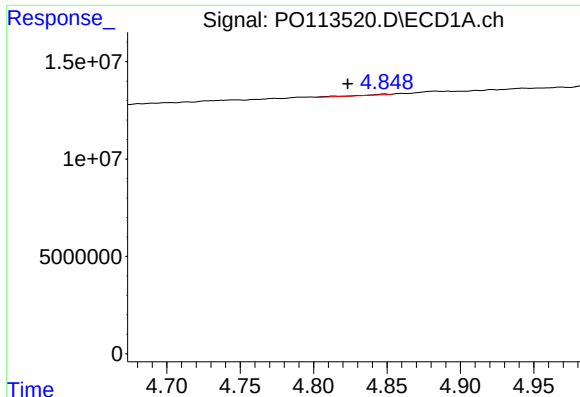

#5 AR-1016-3


R.T.: 4.849 min
Delta R.T.: 0.025 min
Response: 442672
Conc: 1.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

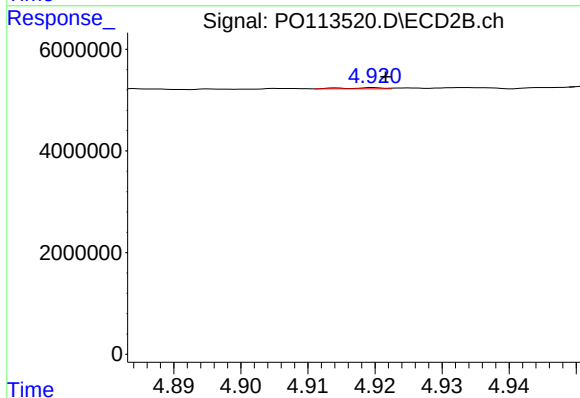


#5 AR-1016-3

R.T.: 4.920 min
Delta R.T.: -0.002 min
Response: 90191
Conc: 0.65 ng/ml

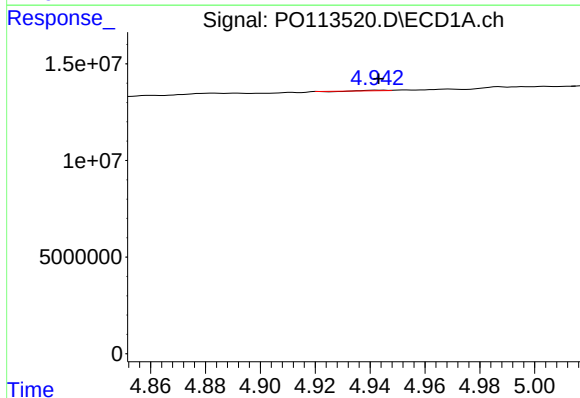


#6 AR-1016-4

R.T.: 4.944 min
Delta R.T.: 0.000 min
Response: 40779
Conc: 0.19 ng/ml

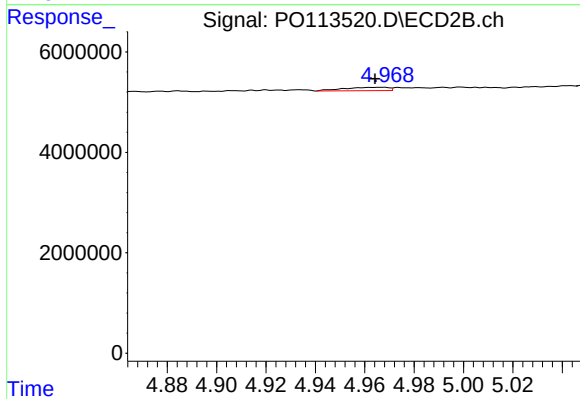

#6 AR-1016-4


R.T.: 4.968 min
Delta R.T.: 0.004 min
Response: 853564
Conc: 7.31 ng/ml

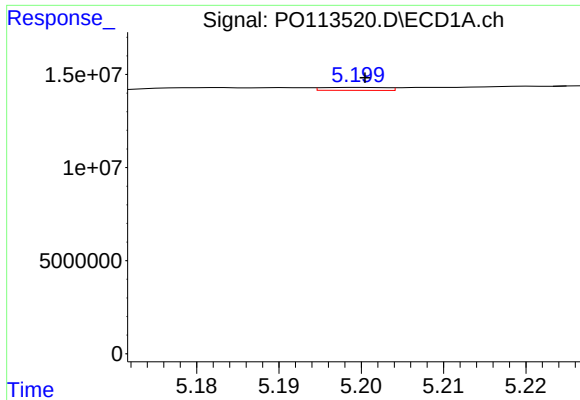

#7 AR-1016-5


R.T.: 5.200 min
Delta R.T.: 0.000 min
Response: 859994
Conc: 3.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

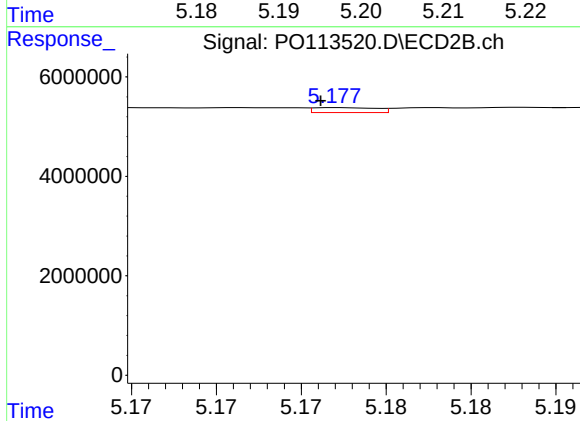


#7 AR-1016-5

R.T.: 5.177 min
Delta R.T.: 0.000 min
Response: 253636
Conc: 1.78 ng/ml

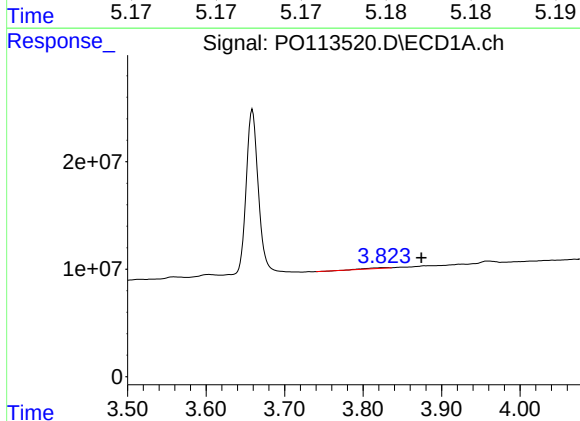


#8 AR-1221-1

R.T.: 3.825 min
Delta R.T.: -0.049 min
Response: 1399084
Conc: 14.95 ng/ml

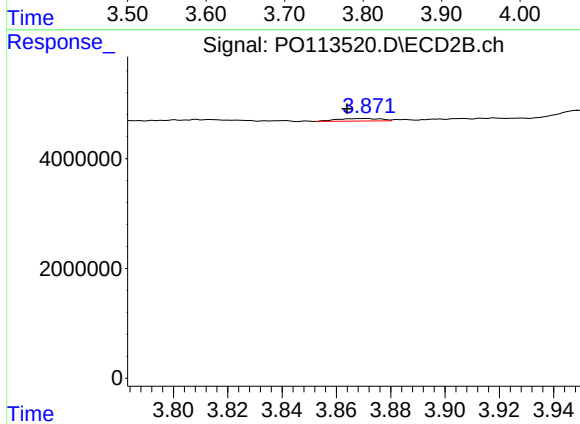

#8 AR-1221-1


R.T.: 3.871 min
Delta R.T.: 0.007 min
Response: 526036
Conc: 8.33 ng/ml

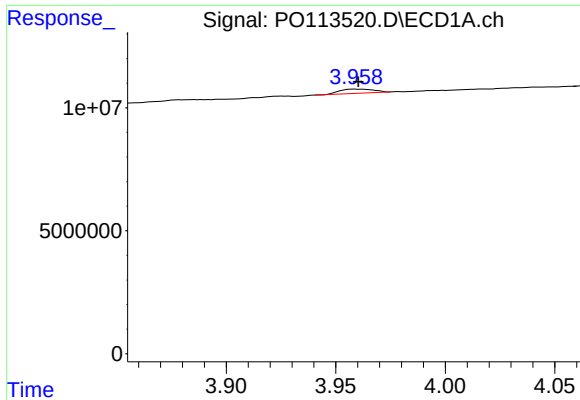

#9 AR-1221-2


R.T.: 3.959 min
Delta R.T.: -0.002 min
Response: 1846365
Conc: 27.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

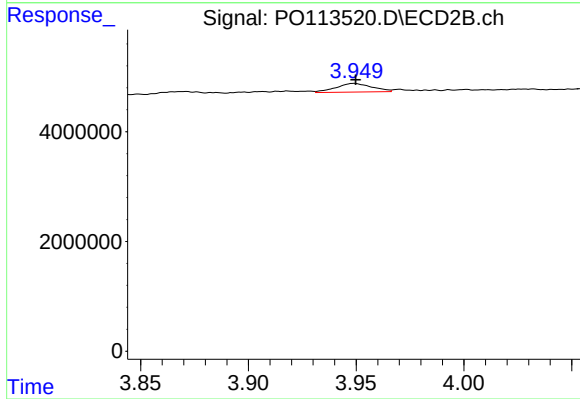


#9 AR-1221-2

R.T.: 3.949 min
Delta R.T.: 0.000 min
Response: 1827826
Conc: 39.16 ng/ml

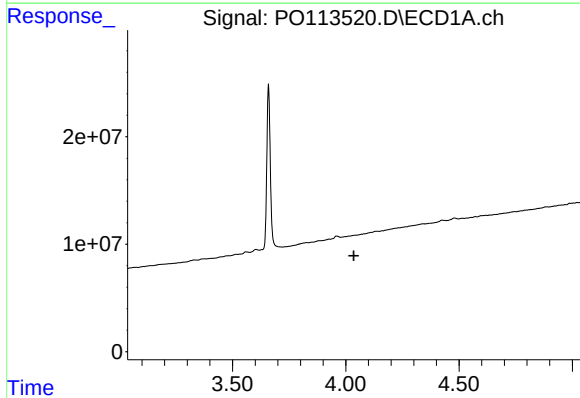


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.036 min
Response: 0
Conc: N.D.

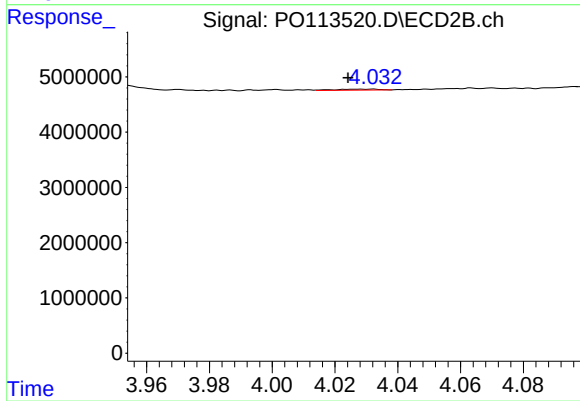

#10 AR-1221-3


R.T.: 4.028 min
Delta R.T.: 0.004 min
Response: 183945
Conc: 1.24 ng/ml

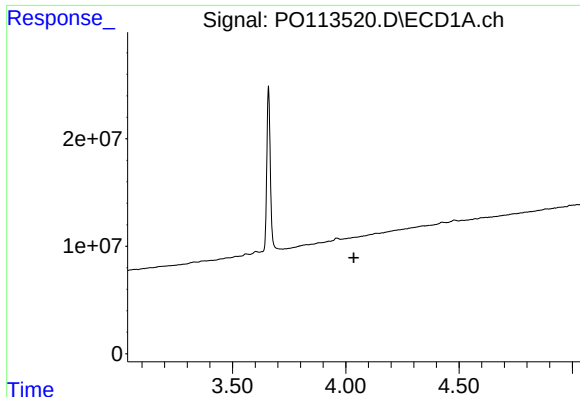

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 4.036 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

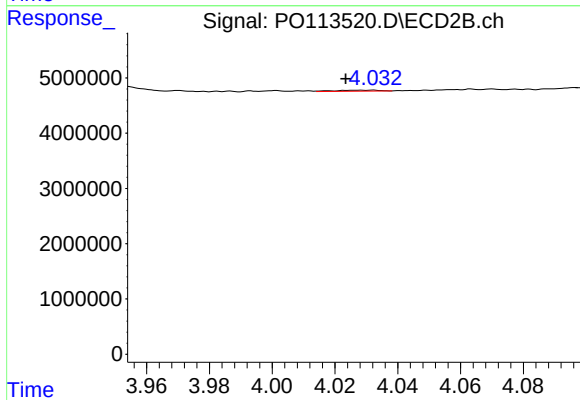


#11 AR-1232-1

R.T.: 4.028 min
Delta R.T.: 0.005 min
Response: 183945
Conc: 1.57 ng/ml

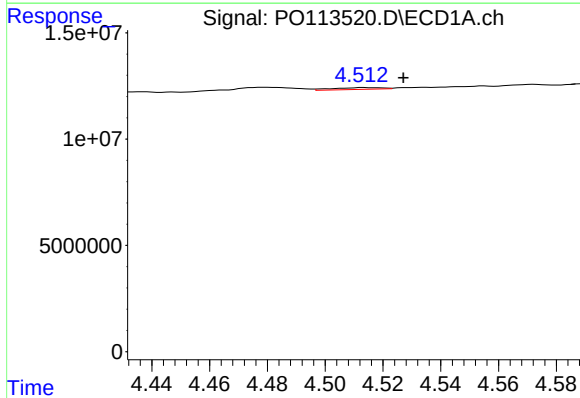


#12 AR-1232-2

R.T.: 4.513 min
Delta R.T.: -0.014 min
Response: 1022989
Conc: 10.25 ng/ml

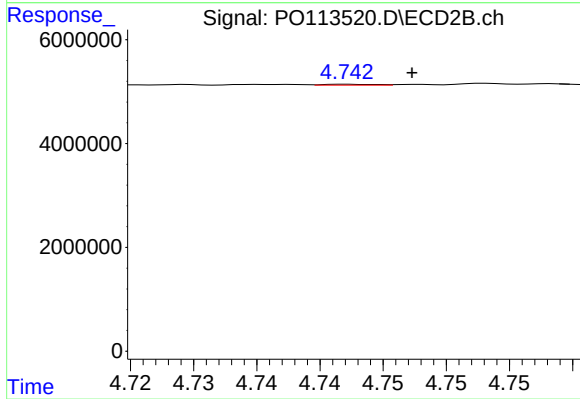

#12 AR-1232-2


R.T.: 4.742 min
Delta R.T.: -0.005 min
Response: 49965
Conc: 0.41 ng/ml

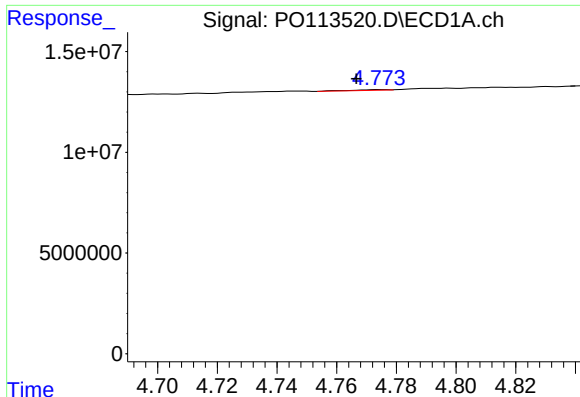

#13 AR-1232-3


R.T.: 4.774 min
Delta R.T.: 0.008 min
Response: 280555
Conc: 1.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

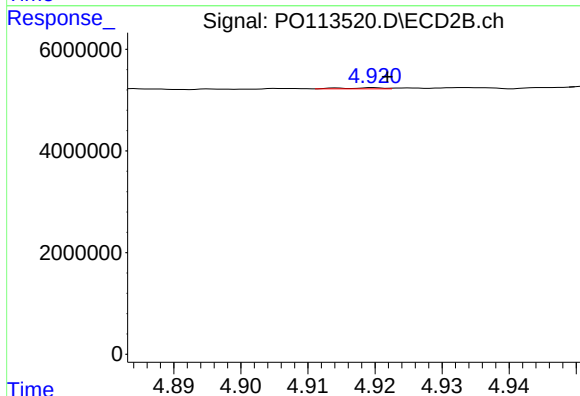


#13 AR-1232-3

R.T.: 4.920 min
Delta R.T.: -0.002 min
Response: 90191
Conc: 1.42 ng/ml

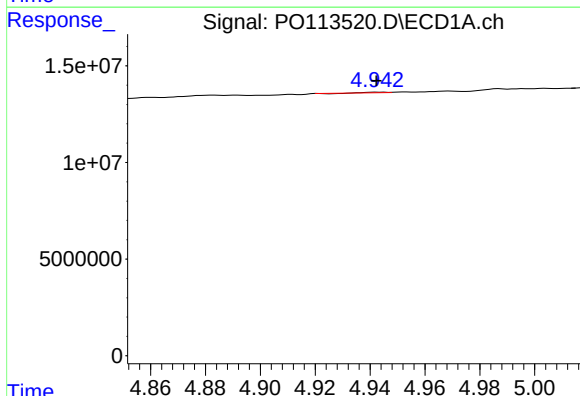


#14 AR-1232-4

R.T.: 4.944 min
Delta R.T.: 0.001 min
Response: 40779
Conc: 0.43 ng/ml

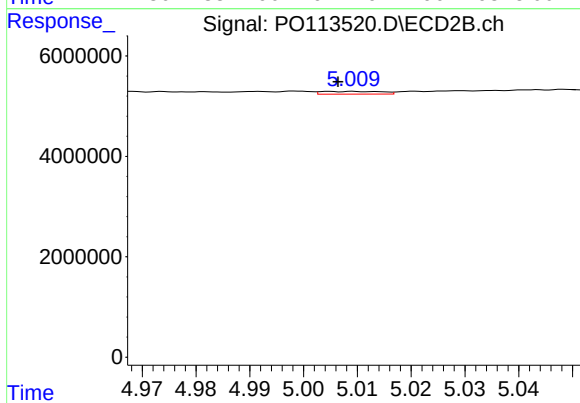

#14 AR-1232-4


R.T.: 5.005 min
Delta R.T.: -0.002 min
Response: 426121
Conc: 7.58 ng/ml

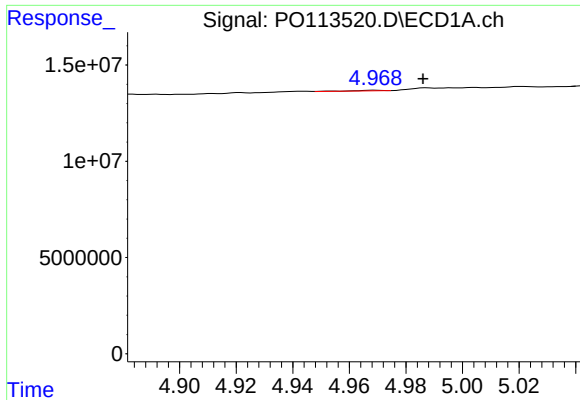

#15 AR-1232-5


R.T.: 4.969 min
Delta R.T.: -0.017 min
Response: 261629
Conc: 4.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

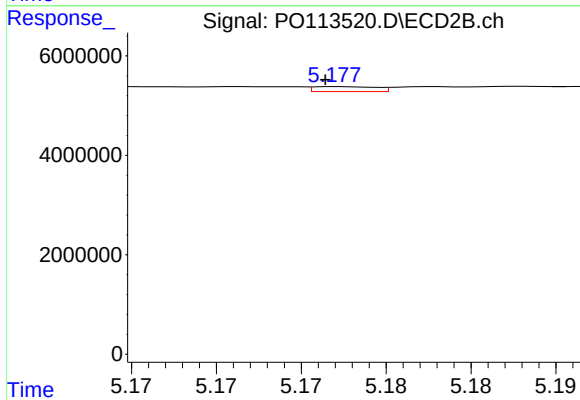


#15 AR-1232-5

R.T.: 5.177 min
Delta R.T.: 0.000 min
Response: 253636
Conc: 4.24 ng/ml

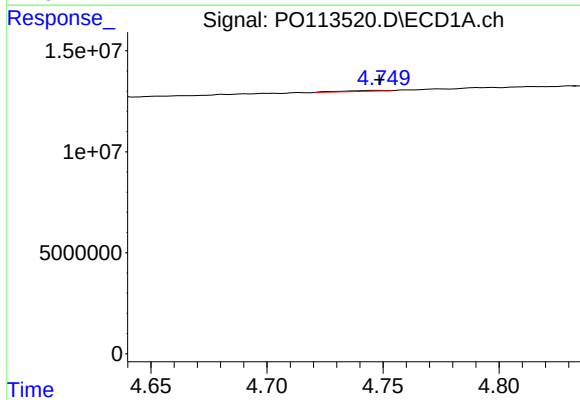


#16 AR-1242-1

R.T.: 4.748 min
Delta R.T.: 0.000 min
Response: 567759
Conc: 2.47 ng/ml

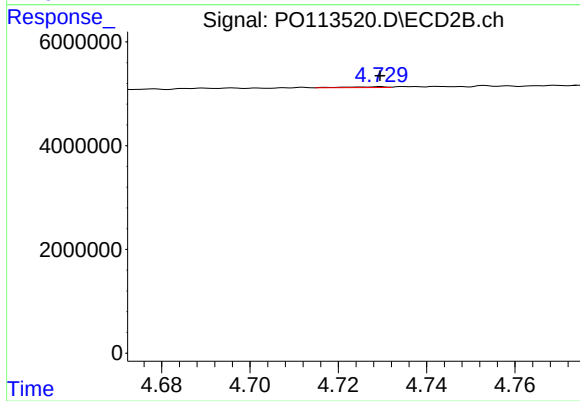

#16 AR-1242-1


R.T.: 4.730 min
Delta R.T.: 0.000 min
Response: 103234
Conc: 0.71 ng/ml

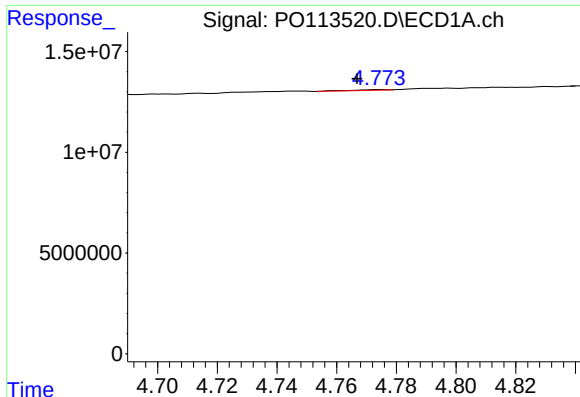

#17 AR-1242-2


R.T.: 4.774 min
Delta R.T.: 0.008 min
Response: 280555
Conc: 0.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

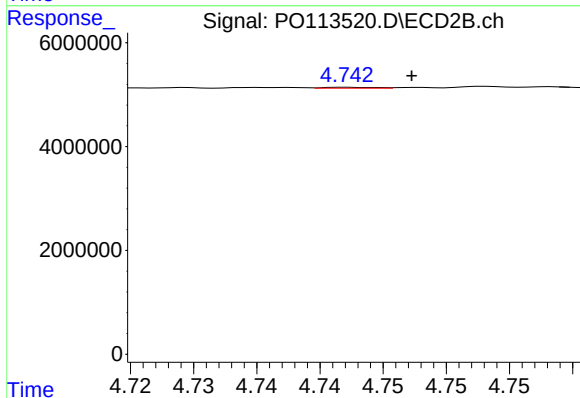


#17 AR-1242-2

R.T.: 4.742 min
Delta R.T.: -0.005 min
Response: 49965
Conc: 0.23 ng/ml

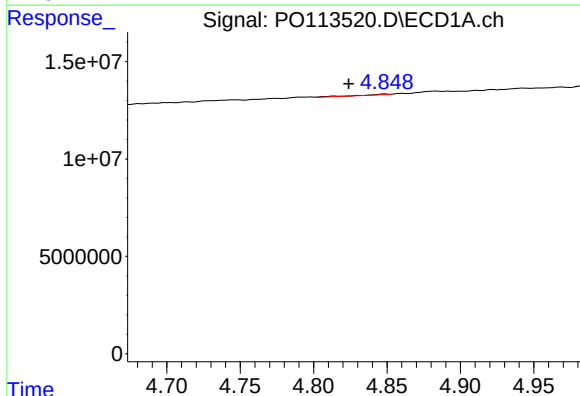


#18 AR-1242-3

R.T.: 4.849 min
Delta R.T.: 0.025 min
Response: 442672
Conc: 2.00 ng/ml

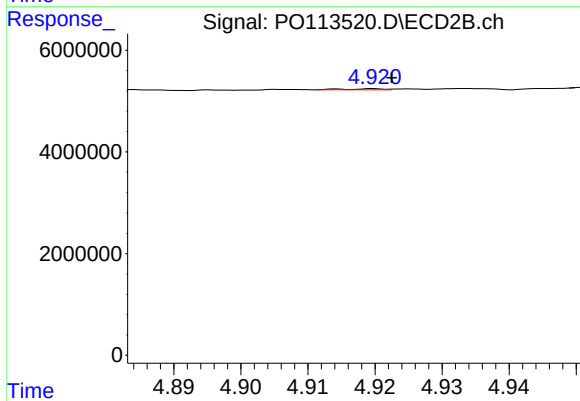

#18 AR-1242-3


R.T.: 4.920 min
Delta R.T.: -0.003 min
Response: 90191
Conc: 0.77 ng/ml

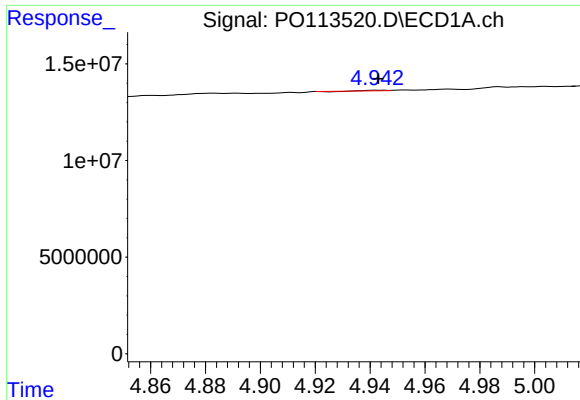

#19 AR-1242-4


R.T.: 4.944 min
Delta R.T.: 0.000 min
Response: 40779
Conc: 0.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

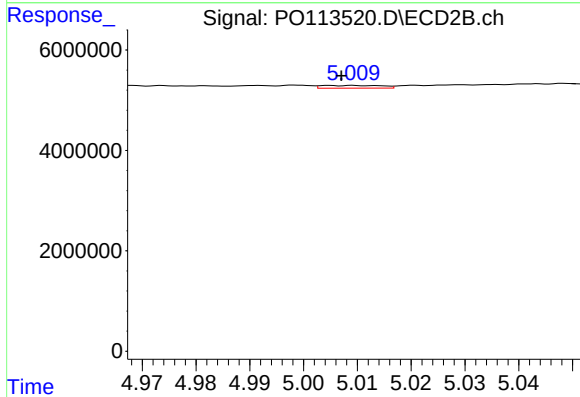


#19 AR-1242-4

R.T.: 5.005 min
Delta R.T.: -0.002 min
Response: 426121
Conc: 3.62 ng/ml

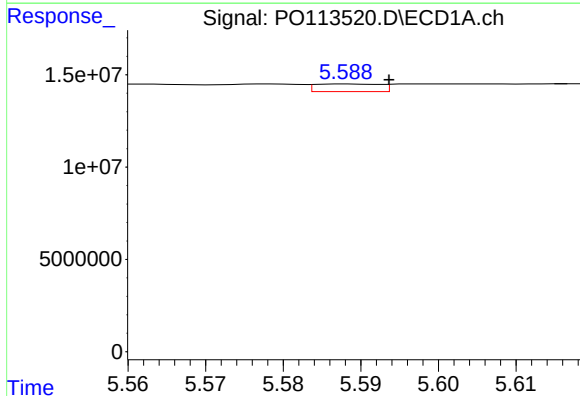


#20 AR-1242-5

R.T.: 5.588 min
Delta R.T.: -0.005 min
Response: 2386423
Conc: 11.92 ng/ml

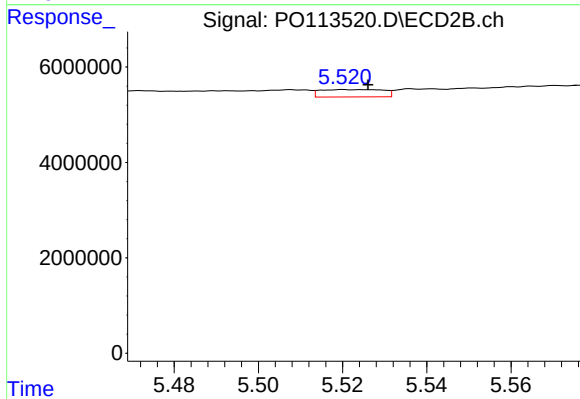

#20 AR-1242-5


R.T.: 5.520 min
Delta R.T.: -0.006 min
Response: 1597170
Conc: 10.71 ng/ml

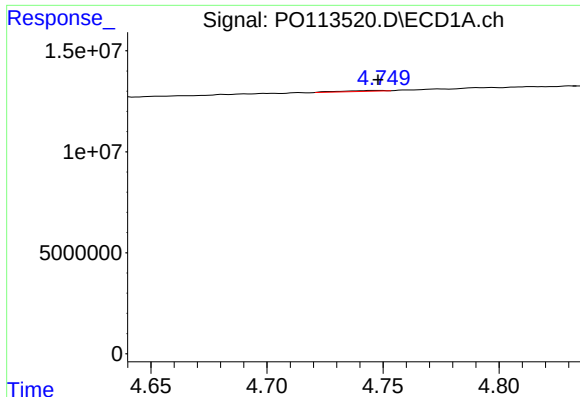

#21 AR-1248-1


R.T.: 4.748 min
Delta R.T.: 0.000 min
Response: 567759
Conc: 3.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

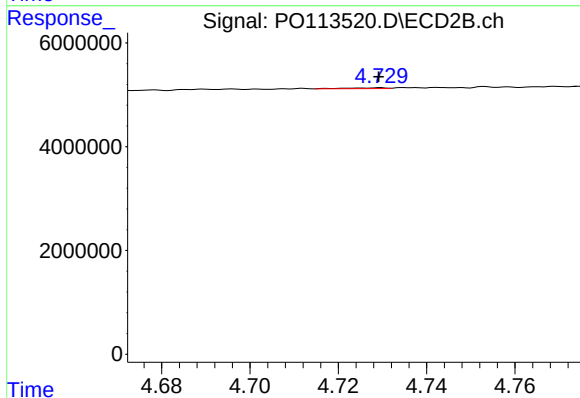


#21 AR-1248-1

R.T.: 4.730 min
Delta R.T.: 0.000 min
Response: 103234
Conc: 0.93 ng/ml

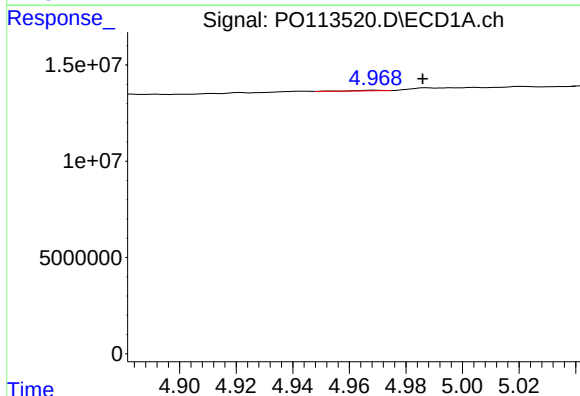


#22 AR-1248-2

R.T.: 4.969 min
Delta R.T.: -0.017 min
Response: 261629
Conc: 1.08 ng/ml

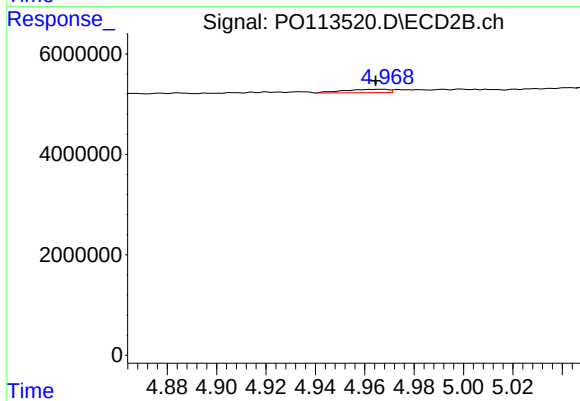

#22 AR-1248-2


R.T.: 4.968 min
Delta R.T.: 0.003 min
Response: 853564
Conc: 5.31 ng/ml

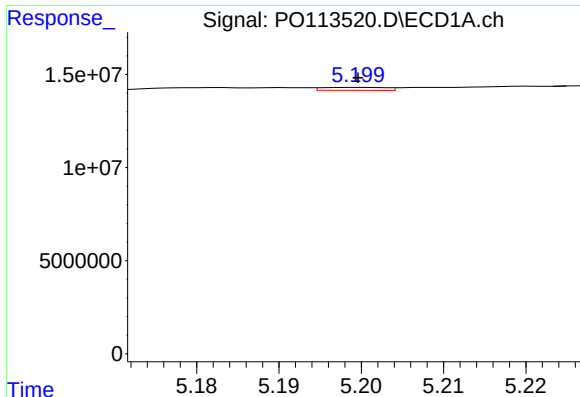

#23 AR-1248-3


R.T.: 5.200 min
Delta R.T.: 0.000 min
Response: 859994
Conc: 2.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

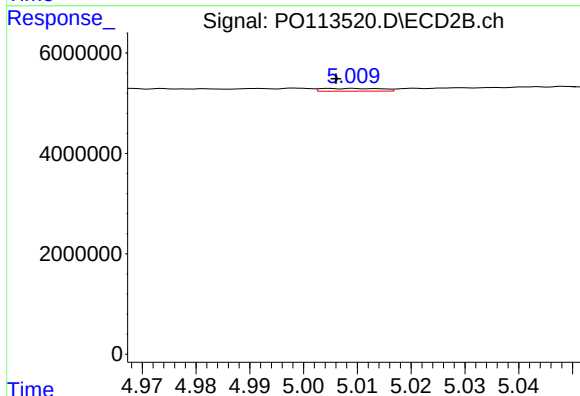


#23 AR-1248-3

R.T.: 5.005 min
Delta R.T.: -0.001 min
Response: 426121
Conc: 2.51 ng/ml

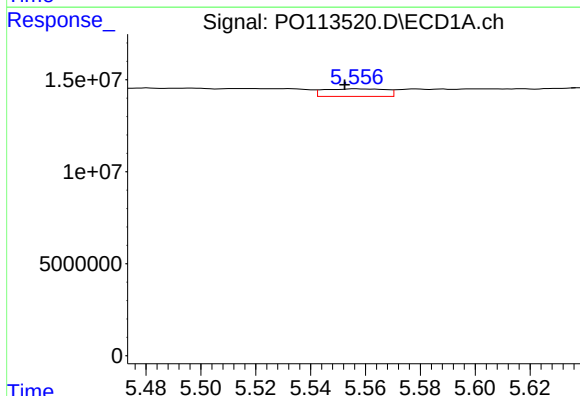


#24 AR-1248-4

R.T.: 5.557 min
Delta R.T.: 0.004 min
Response: 6463189
Conc: 12.94 ng/ml

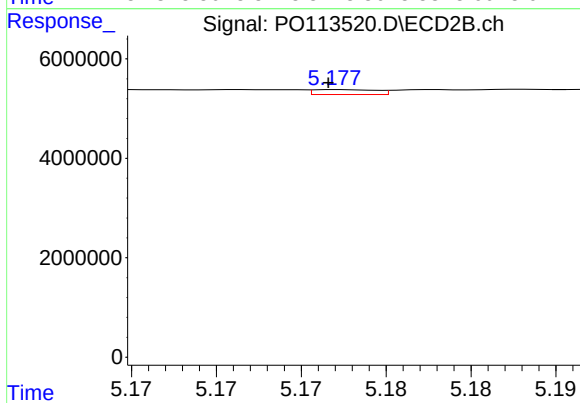

#24 AR-1248-4


R.T.: 5.177 min
Delta R.T.: 0.000 min
Response: 253636
Conc: 1.27 ng/ml

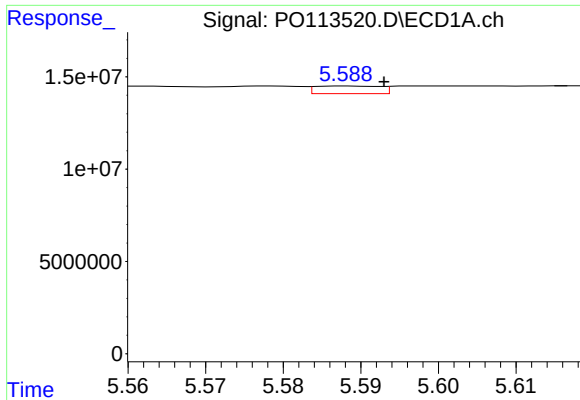

#25 AR-1248-5


R.T.: 5.588 min
Delta R.T.: -0.005 min
Response: 2386423
Conc: 6.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

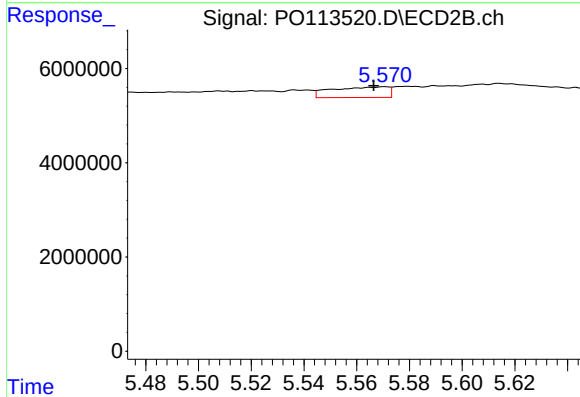


#25 AR-1248-5

R.T.: 5.571 min
Delta R.T.: 0.004 min
Response: 3357498
Conc: 15.82 ng/ml

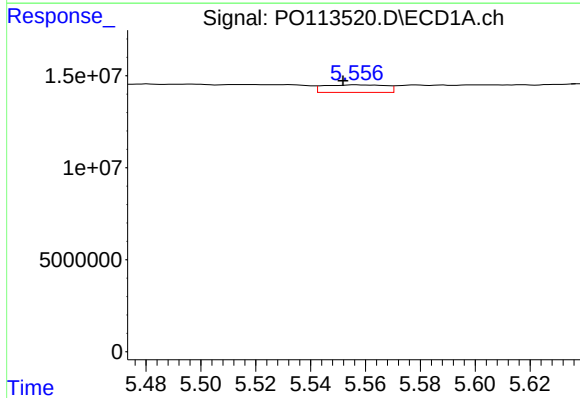


#26 AR-1254-1

R.T.: 5.557 min
Delta R.T.: 0.005 min
Response: 6463189
Conc: 11.97 ng/ml

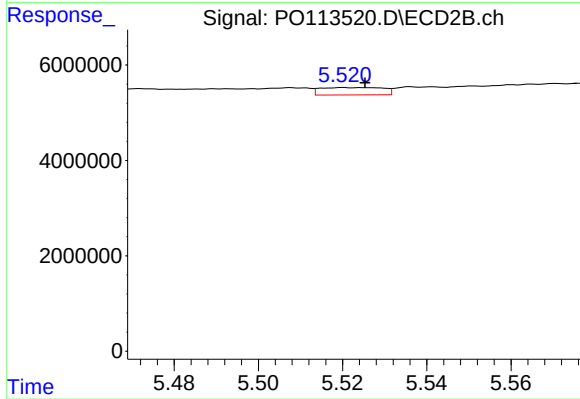

#26 AR-1254-1


R.T.: 5.520 min
Delta R.T.: -0.005 min
Response: 1597170
Conc: 5.06 ng/ml

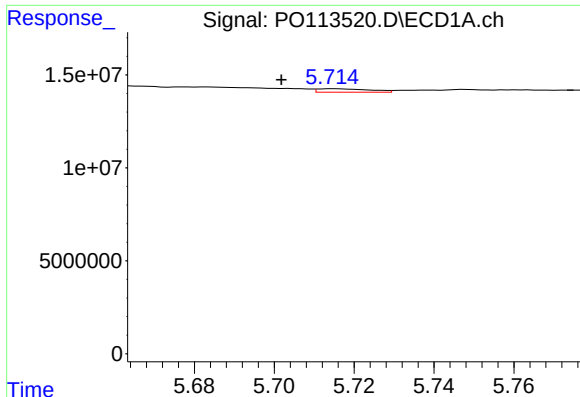

#27 AR-1254-2


R.T.: 5.715 min
Delta R.T.: 0.013 min
Response: 1670779
Conc: 3.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

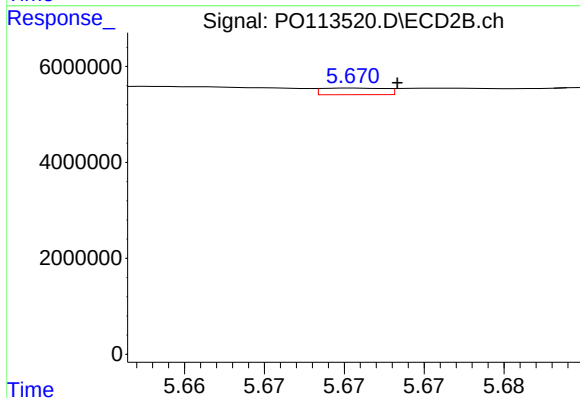


#27 AR-1254-2

R.T.: 5.671 min
Delta R.T.: -0.003 min
Response: 381056
Conc: 1.36 ng/ml

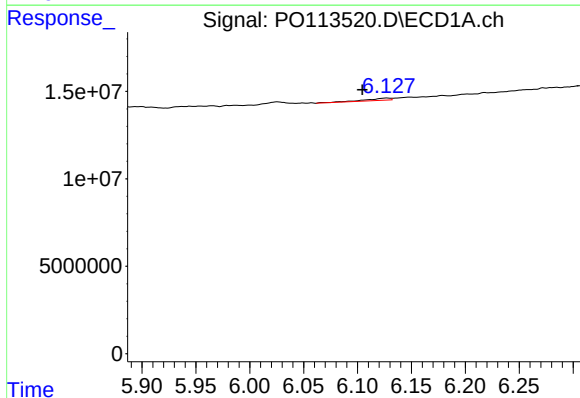


#28 AR-1254-3

R.T.: 6.127 min
Delta R.T.: 0.023 min
Response: 1944755
Conc: 2.63 ng/ml

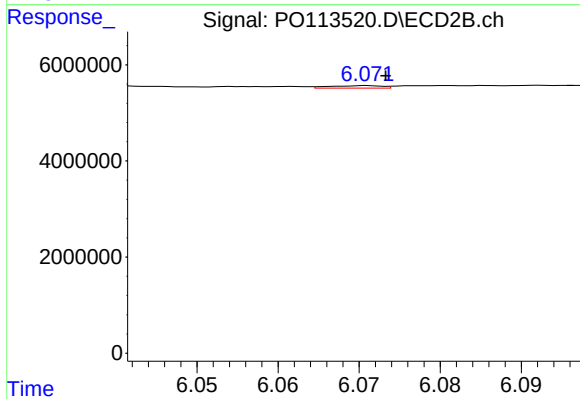

#28 AR-1254-3


R.T.: 6.071 min
Delta R.T.: -0.002 min
Response: 225745
Conc: 0.54 ng/ml

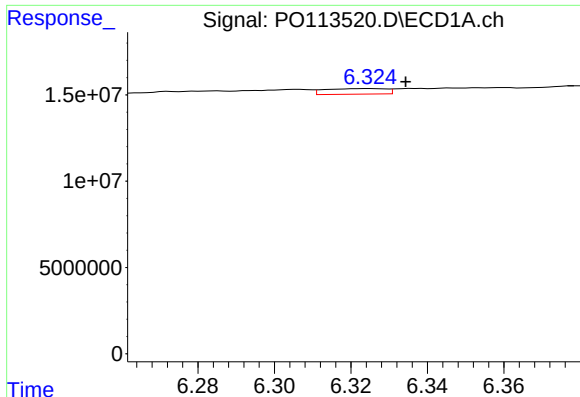

#29 AR-1254-4


R.T.: 6.325 min
Delta R.T.: -0.009 min
Response: 3587211
Conc: 6.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

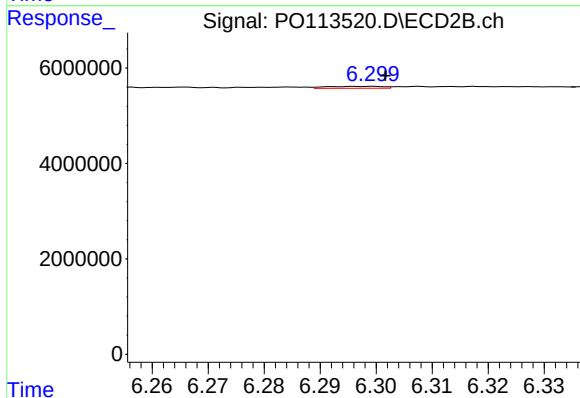


#29 AR-1254-4

R.T.: 6.300 min
Delta R.T.: -0.002 min
Response: 292057
Conc: 1.06 ng/ml

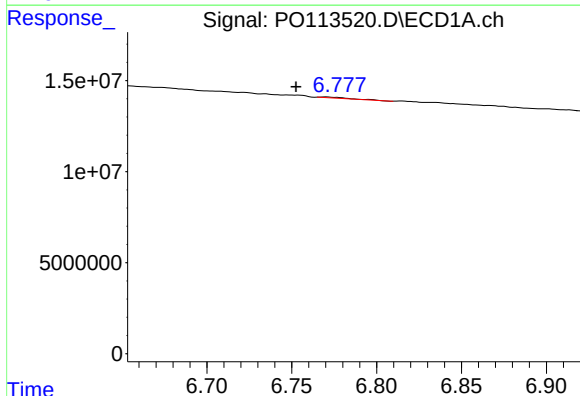


#30 AR-1254-5

R.T.: 6.770 min
Delta R.T.: 0.018 min
Response: 608788
Conc: 0.87 ng/ml

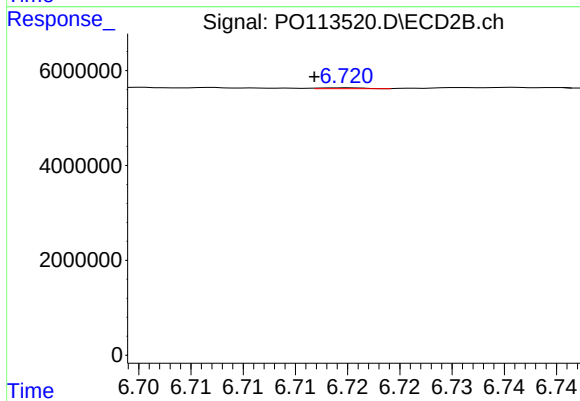

#30 AR-1254-5


R.T.: 6.720 min
Delta R.T.: 0.003 min
Response: 48184
Conc: 0.13 ng/ml

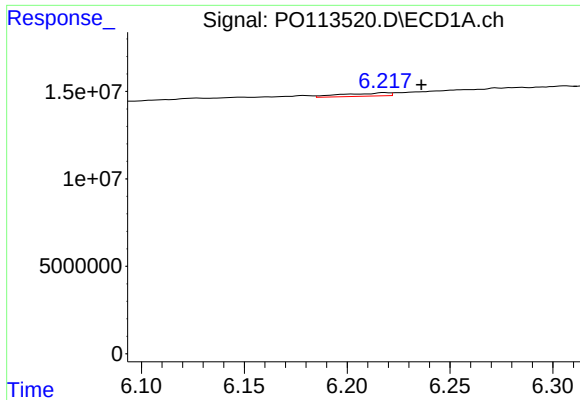

#31 AR-1260-1


R.T.: 6.218 min
Delta R.T.: -0.018 min
Response: 2816268
Conc: 6.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

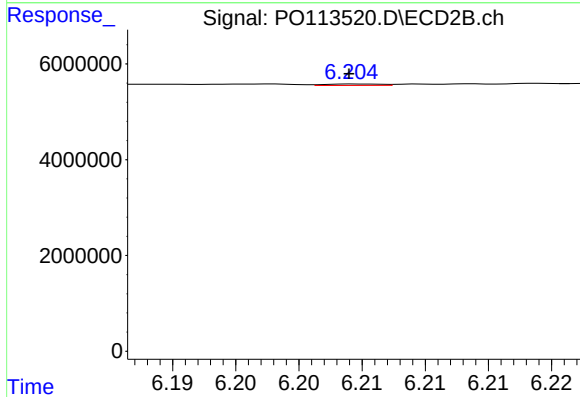


#31 AR-1260-1

R.T.: 6.205 min
Delta R.T.: 0.000 min
Response: 91057
Conc: 0.36 ng/ml

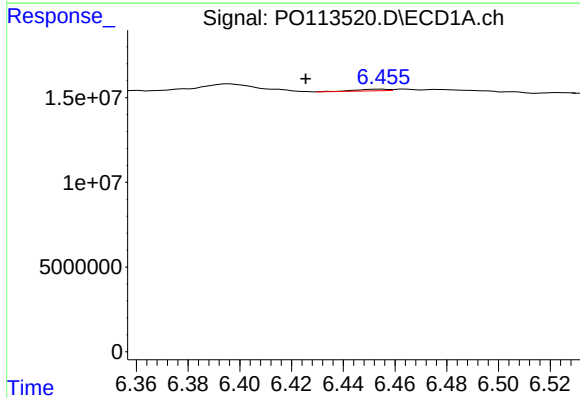


#32 AR-1260-2

R.T.: 6.454 min
Delta R.T.: 0.028 min
Response: 816844
Conc: 1.19 ng/ml

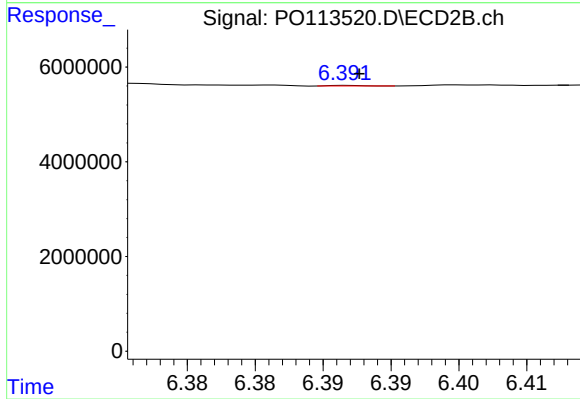

#32 AR-1260-2


R.T.: 6.392 min
Delta R.T.: 0.000 min
Response: 19852
Conc: 0.06 ng/ml

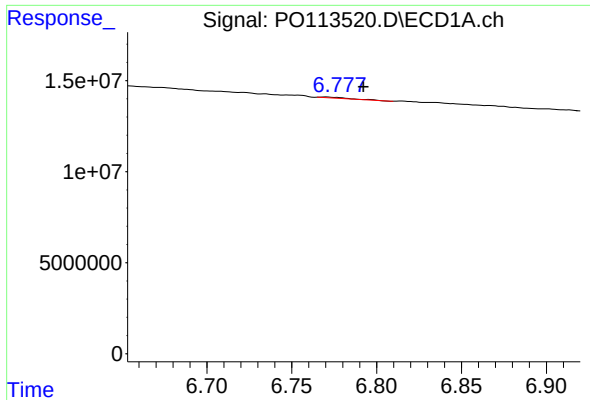

#33 AR-1260-3


R.T.: 6.770 min
Delta R.T.: -0.022 min
Response: 608788
Conc: 0.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

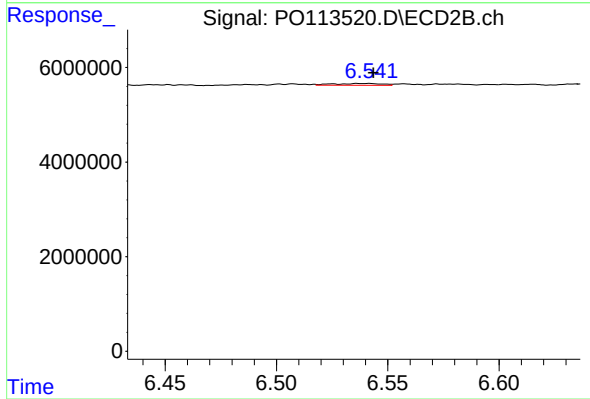


#33 AR-1260-3

R.T.: 6.541 min
Delta R.T.: -0.002 min
Response: 578516
Conc: 1.95 ng/ml

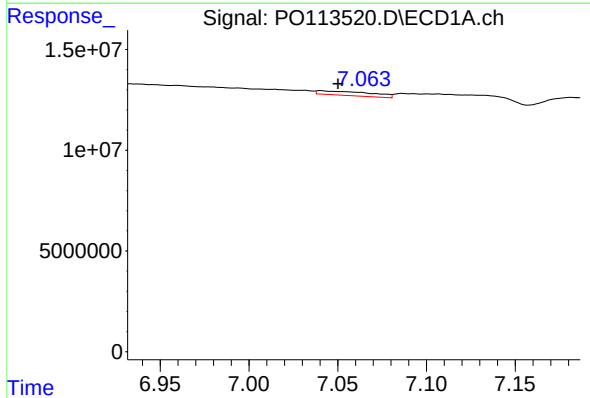


#34 AR-1260-4

R.T.: 7.041 min
Delta R.T.: -0.009 min
Response: 4448629
Conc: 9.93 ng/ml

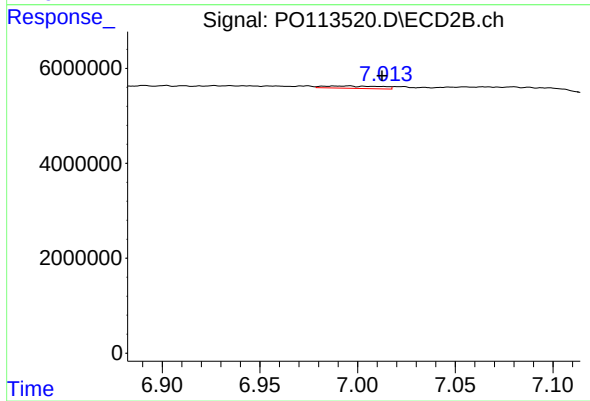

#34 AR-1260-4


R.T.: 6.996 min
Delta R.T.: -0.017 min
Response: 1030857
Conc: 4.97 ng/ml

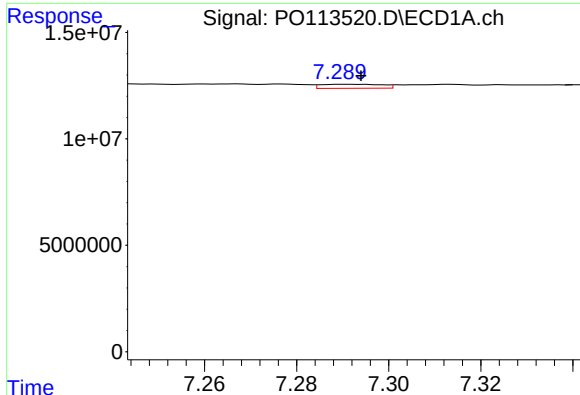

#35 AR-1260-5


R.T.: 7.291 min
Delta R.T.: -0.003 min
Response: 1721027
Conc: 1.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

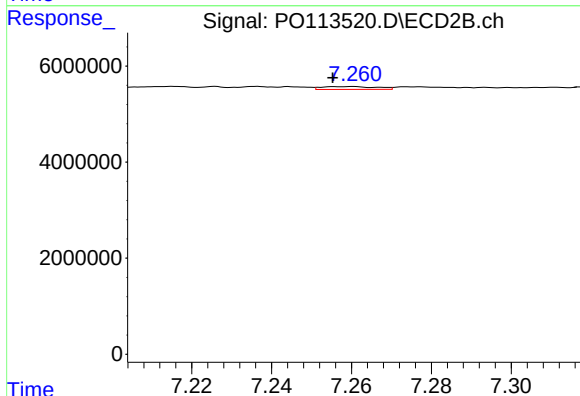


#35 AR-1260-5

R.T.: 7.260 min
Delta R.T.: 0.004 min
Response: 568329
Conc: 1.21 ng/ml

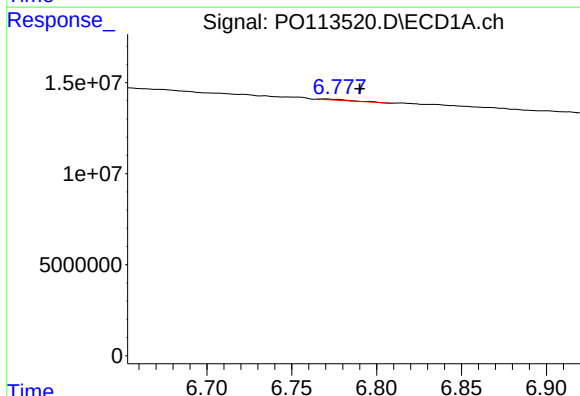


#36 AR-1262-1

R.T.: 6.770 min
Delta R.T.: -0.020 min
Response: 608788
Conc: 0.66 ng/ml

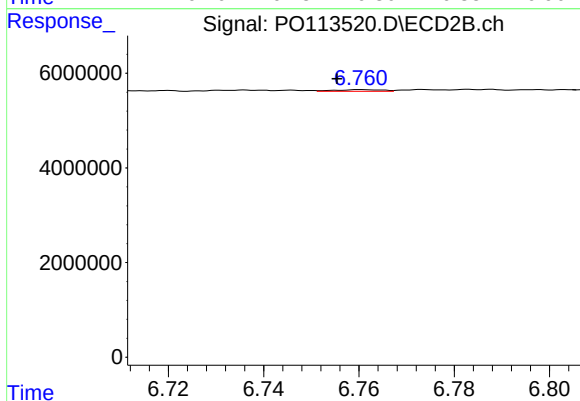

#36 AR-1262-1


R.T.: 6.761 min
Delta R.T.: 0.005 min
Response: 236801
Conc: 0.57 ng/ml

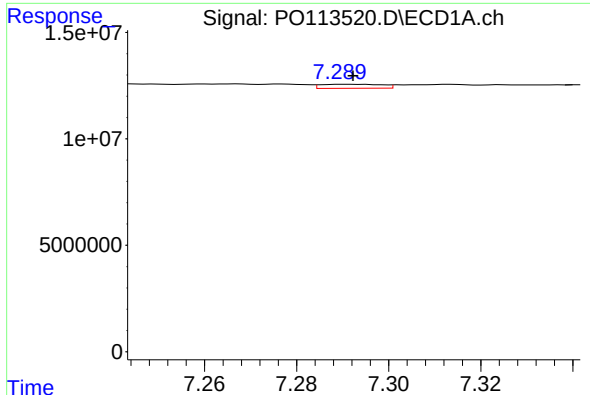

#37 AR-1262-2


R.T.: 7.291 min
Delta R.T.: -0.002 min
Response: 1721027
Conc: 1.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

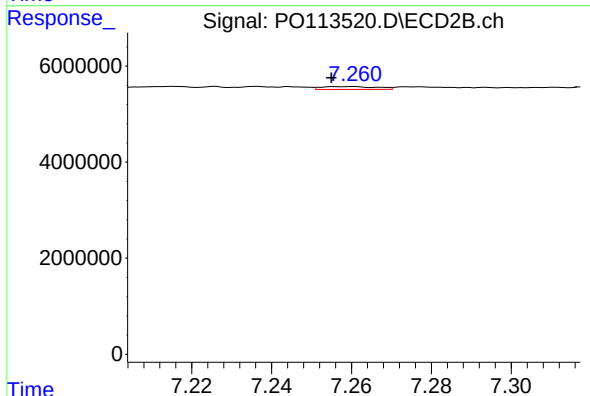


#37 AR-1262-2

R.T.: 7.260 min
Delta R.T.: 0.005 min
Response: 568329
Conc: 1.10 ng/ml

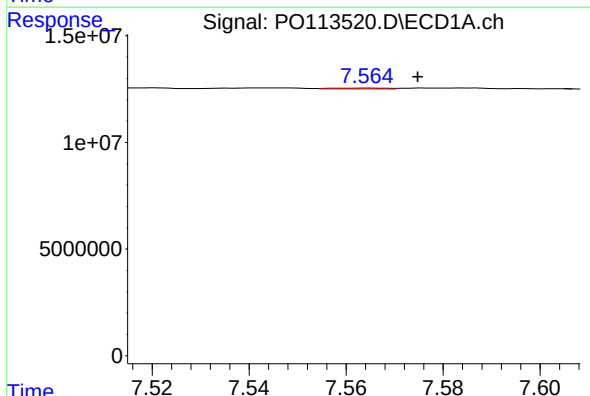


#38 AR-1262-3

R.T.: 7.565 min
Delta R.T.: -0.010 min
Response: 319946
Conc: 0.58 ng/ml

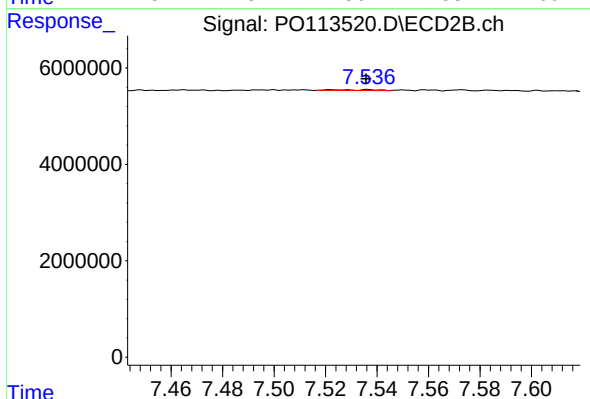

#38 AR-1262-3


R.T.: 7.537 min
Delta R.T.: 0.000 min
Response: 216439
Conc: 1.21 ng/ml

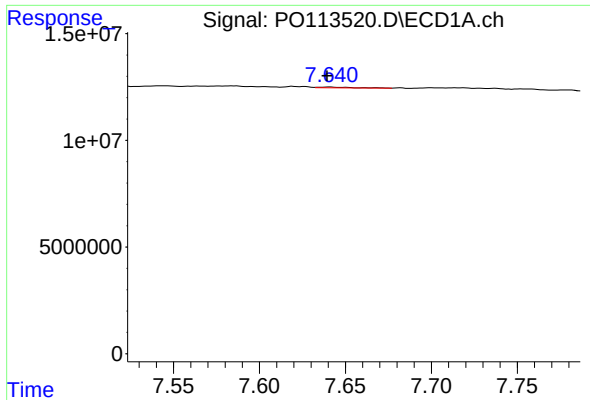

#39 AR-1262-4


R.T.: 7.641 min
Delta R.T.: 0.001 min
Response: 564988
Conc: 0.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

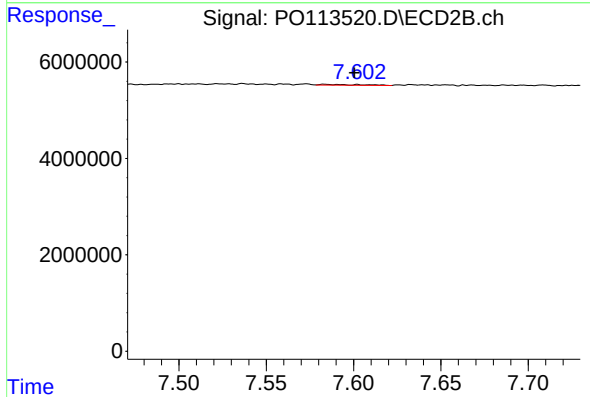


#39 AR-1262-4

R.T.: 7.584 min
Delta R.T.: -0.017 min
Response: 255558
Conc: 0.88 ng/ml

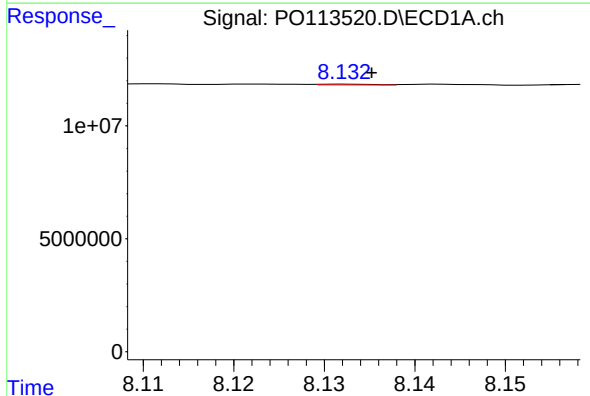


#40 AR-1262-5

R.T.: 8.133 min
Delta R.T.: -0.003 min
Response: 143415
Conc: 0.34 ng/ml

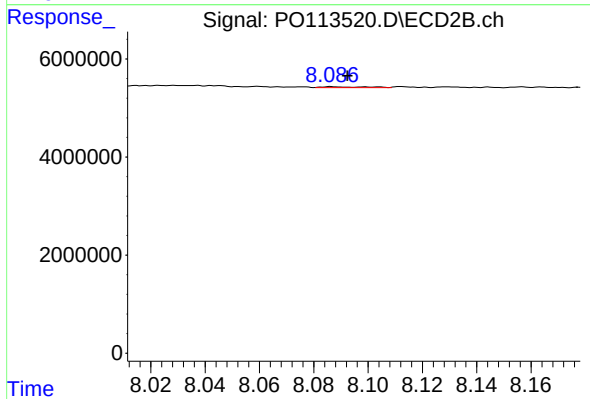

#40 AR-1262-5


R.T.: 8.087 min
Delta R.T.: -0.006 min
Response: 193359
Conc: 1.78 ng/ml

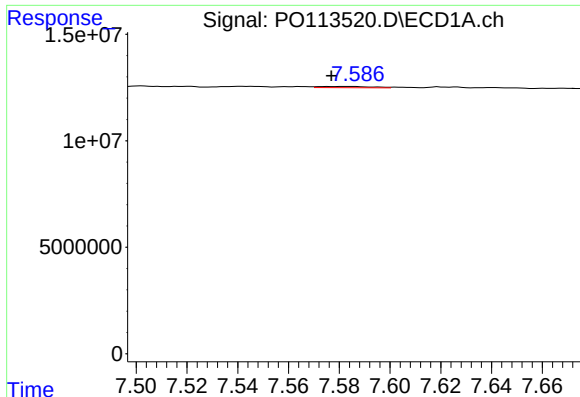

#41 AR-1268-1


R.T.: 7.585 min
Delta R.T.: 0.008 min
Response: 812863
Conc: 0.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

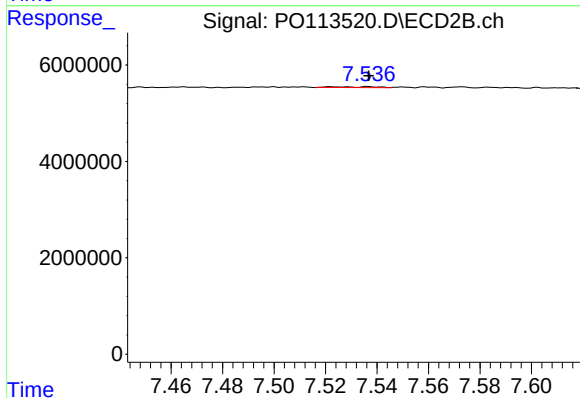


#41 AR-1268-1

R.T.: 7.537 min
Delta R.T.: 0.000 min
Response: 216439
Conc: 0.42 ng/ml

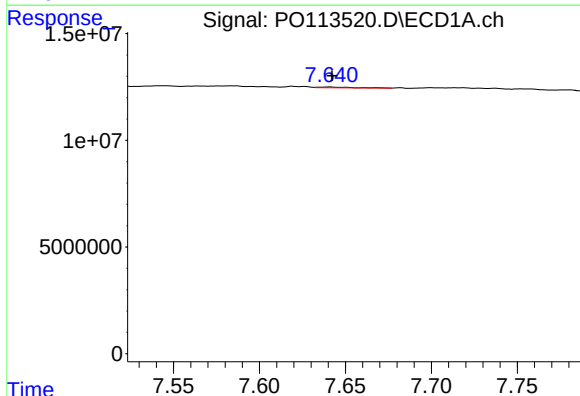


#42 AR-1268-2

R.T.: 7.641 min
Delta R.T.: -0.001 min
Response: 564988
Conc: 0.39 ng/ml

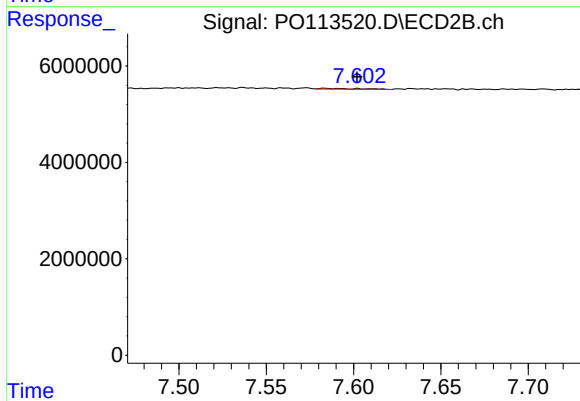

#42 AR-1268-2


R.T.: 7.584 min
Delta R.T.: -0.018 min
Response: 255558
Conc: 0.62 ng/ml

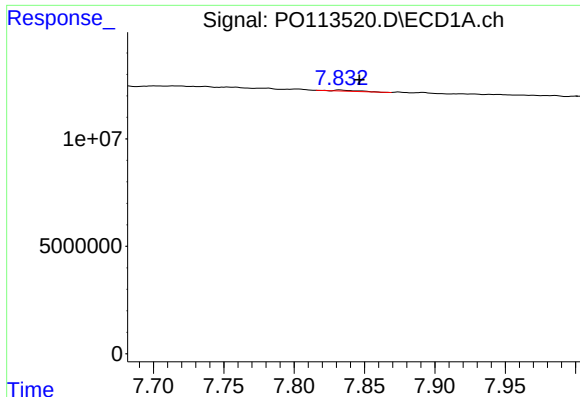

#43 AR-1268-3


R.T.: 7.832 min
Delta R.T.: -0.014 min
Response: 657363
Conc: 0.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

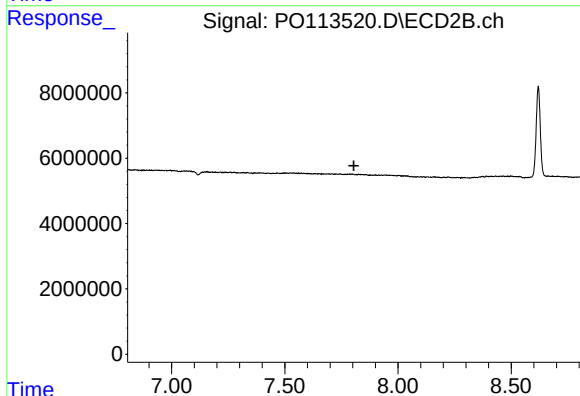


#43 AR-1268-3

R.T.: 7.816 min
Delta R.T.: 0.011 min
Response: -134159
Conc: N.D.

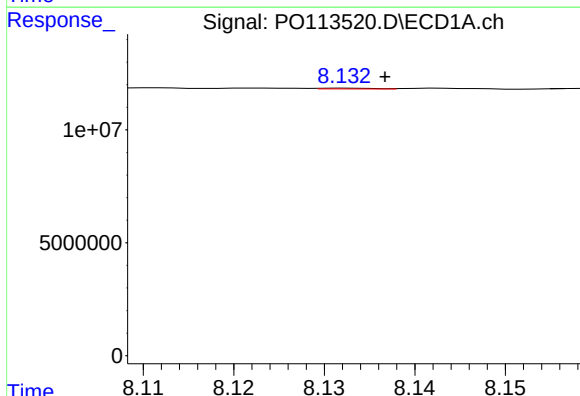


#44 AR-1268-4

R.T.: 8.133 min
Delta R.T.: -0.004 min
Response: 143415
Conc: 0.31 ng/ml

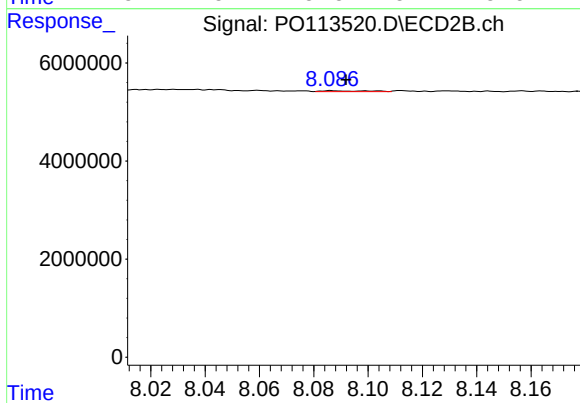

#44 AR-1268-4


R.T.: 8.087 min
Delta R.T.: -0.005 min
Response: 193359
Conc: 1.61 ng/ml

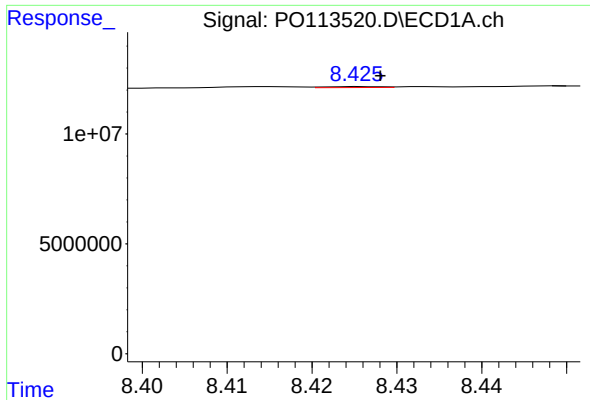

#45 AR-1268-5

R.T.: 8.426 min
Delta R.T.: -0.002 min
Response: 204792
Conc: 0.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

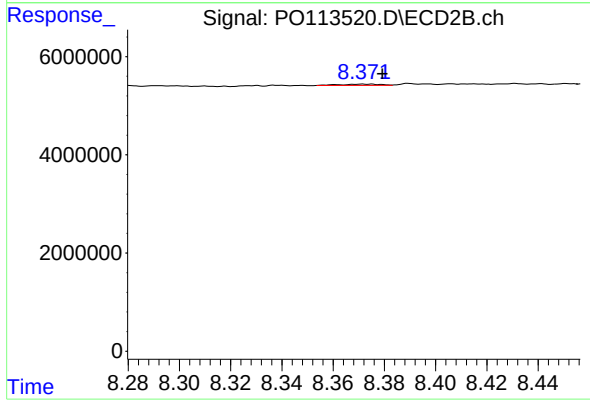

#45 AR-1268-5

R.T.: 8.371 min
Delta R.T.: -0.008 min
Response: 290311
Conc: 0.37 ng/ml