

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0090525\
 Data File : P0113521.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 19:44
 Operator : YP/AJ
 Sample : Q2893-09
 Misc : AR1254 WATER LOD 25PPB
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:36:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.658	3.652	164.1E6	97314289	20.043	19.230
2) SA Decachlor...	8.673	8.619	107.6E6	35537264	15.522	18.755
Target Compounds						
3) L1 AR-1016-1	4.779	4.735	853439	119635	3.197	0.701 #
4) L1 AR-1016-2	4.779	4.751	853439	77918	2.126	0.302 #
5) L1 AR-1016-3	4.827	4.917	739503	225358	2.900	1.614 #
6) L1 AR-1016-4	4.938	4.960	129818	3581854	0.595	30.693 #
7) L1 AR-1016-5	5.194	5.172	4637086	3858560	20.923	27.072 #
8) L2 AR-1221-1	3.890	3.872	312041	328992	3.335	5.212 #
9) L2 AR-1221-2	3.959	3.948	1959502	2172872	29.008	46.555 #
10) L2 AR-1221-3	0.000	4.021	0	70947	N.D.	0.478 #
11) L3 AR-1232-1	0.000	4.021	0	70947	N.D.	0.604 #
12) L3 AR-1232-2	4.520	4.751	1113318	77918	11.150	0.636 #
13) L3 AR-1232-3	4.779	4.917	853439	225358	4.504	3.558
14) L3 AR-1232-4	4.938	5.000	129818	1693236	1.379	30.117 #
15) L3 AR-1232-5	4.979	5.172	4570238	3858560	73.781	64.456
16) L4 AR-1242-1	4.779	4.735	853439	119635	3.712	0.828 #
17) L4 AR-1242-2	4.779	4.751	853439	77918	2.484	0.359 #
18) L4 AR-1242-3	4.827	4.917	739503	225358	3.333	1.927 #
19) L4 AR-1242-4	4.938	5.000	129818	1693236	0.748	14.394 #
20) L4 AR-1242-5	5.597	5.520	5157763	11065537	25.768	74.199 #
21) L5 AR-1248-1	4.779	4.735	853439	119635	4.892	1.073 #
22) L5 AR-1248-2	4.979	4.960	4570238	3581854	18.896	22.289
23) L5 AR-1248-3	5.194	5.000	4637086	1693236	14.543	9.980 #
24) L5 AR-1248-4	5.546	5.172	31032487	3858560	62.114	19.368 #
25) L5 AR-1248-5	5.597	5.562	5157763	4288584	15.104	20.201 #
26) L6 AR-1254-1	5.546	5.520	31032487	11065537	57.470	35.089 #
27) L6 AR-1254-2	5.695	5.668	29563033	11293119	59.910	40.284 #
28) L6 AR-1254-3	6.097	6.068	12088115	9800367	16.360	23.506 #
29) L6 AR-1254-4	6.328	6.296	8086032	5434103	14.517	19.772 #
30) L6 AR-1254-5	6.745	6.710	20997695	7796775	29.955	21.810 #
31) L7 AR-1260-1	6.230	6.198	4047248	4098147	9.075	16.067 #
32) L7 AR-1260-2	6.418	6.386	6542587	3429454	9.527	9.920
33) L7 AR-1260-3	6.808	6.535	11786363	4212923	19.088	14.164 #
34) L7 AR-1260-4	7.076	7.009	6713740	970007	14.990	4.680 #
35) L7 AR-1260-5	7.290	7.249	2825918	1215235	2.334	2.594
36) L8 AR-1262-1	6.808	6.761	11786363	274147	12.871	0.661 #
37) L8 AR-1262-2	7.290	7.249	2825918	1215235	1.869	2.348 #
38) L8 AR-1262-3	7.580	7.541	208021	163349	0.375	0.910 #
39) L8 AR-1262-4	7.630	7.588	1767174	721417	1.807	2.488 #
40) L8 AR-1262-5	8.157	8.092	274195	44966	0.658	0.415 #
41) L9 AR-1268-1	7.580	7.541	208021	163349	0.121	0.321 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090525\
 Data File : P0113521.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 19:44
 Operator : YP/AJ
 Sample : Q2893-09
 Misc : AR1254 WATER LOD 25PPB
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:36:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	7.630	7.588	1767174	721417	1.220	1.737 #
43) L9	AR-1268-3	7.853	7.802	51403	229160	0.043	0.702 #
44) L9	AR-1268-4	8.157	8.092	274195	44966	0.595	0.373 #
45) L9	AR-1268-5	8.446	8.375	1895925	155502	0.595	0.199 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090525\
Data File : P0113521.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2025 19:44
Operator : YP/AJ
Sample : Q2893-09
Misc : AR1254 WATER LOD 25PPB
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 23:36:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

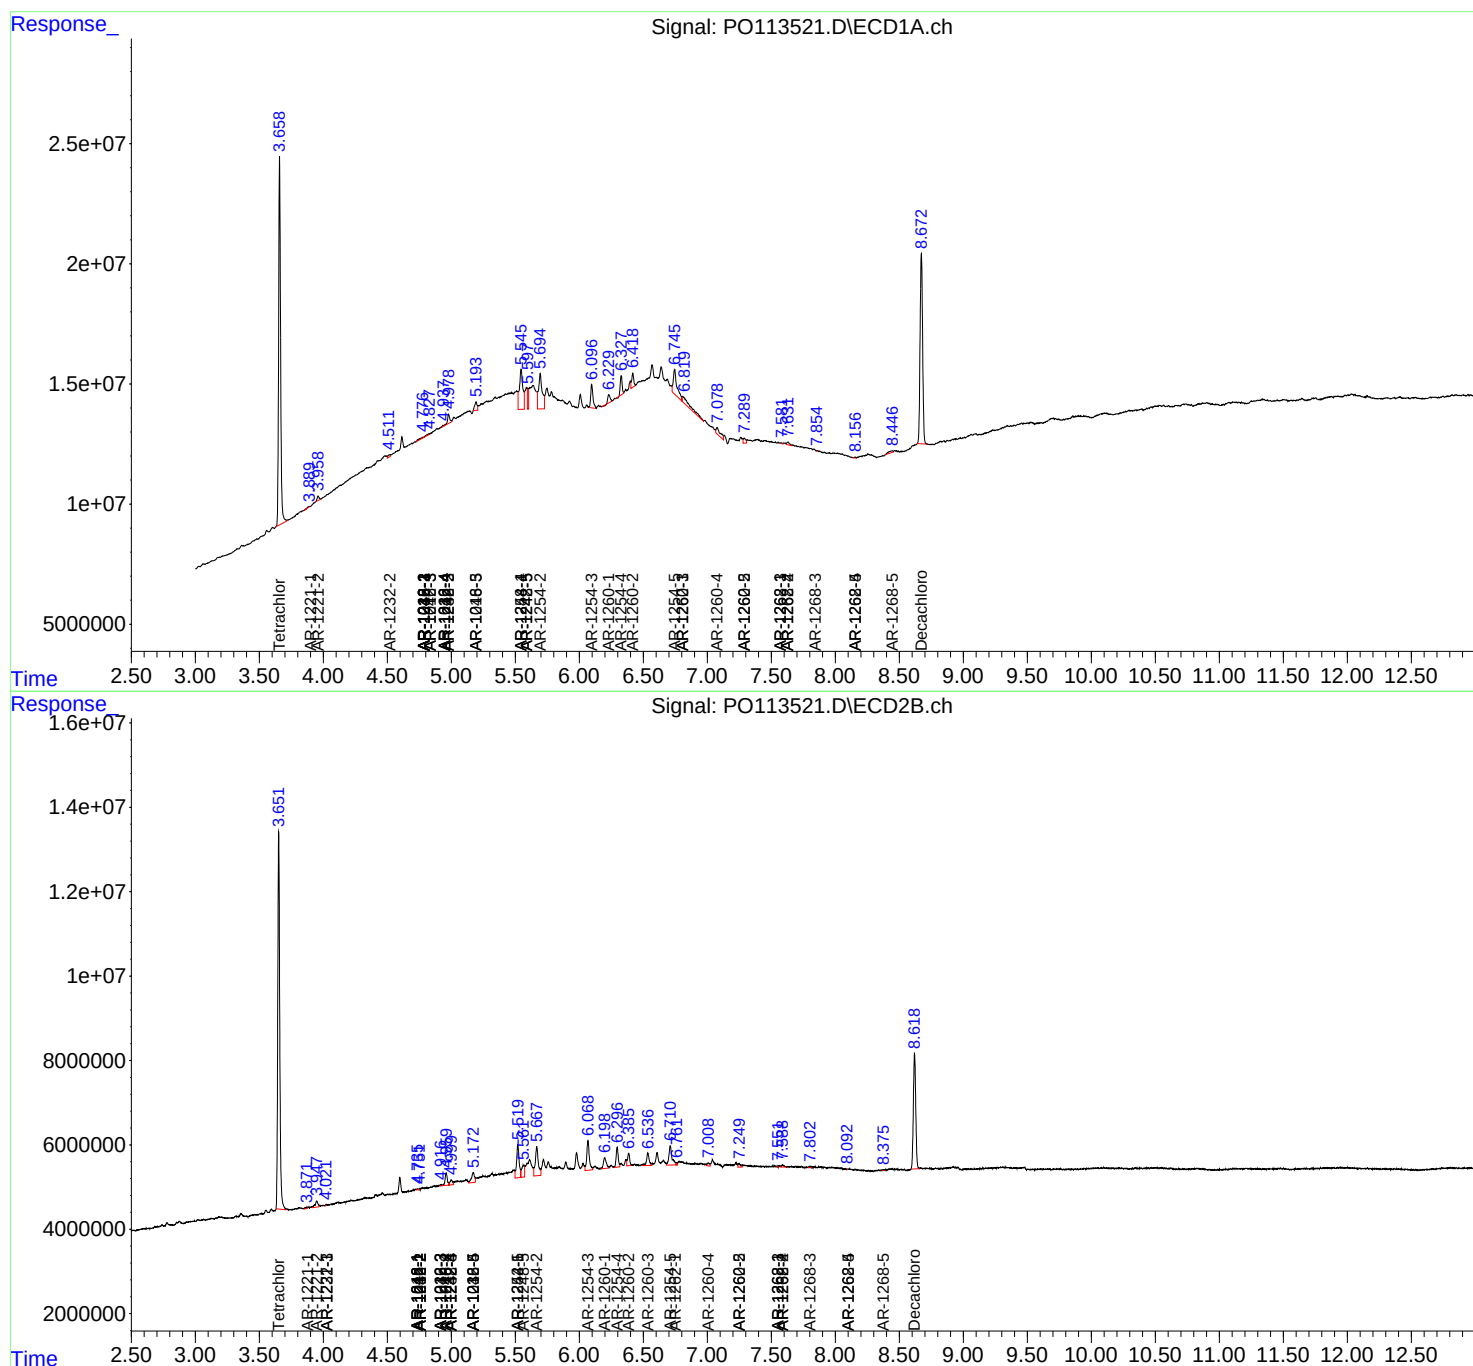


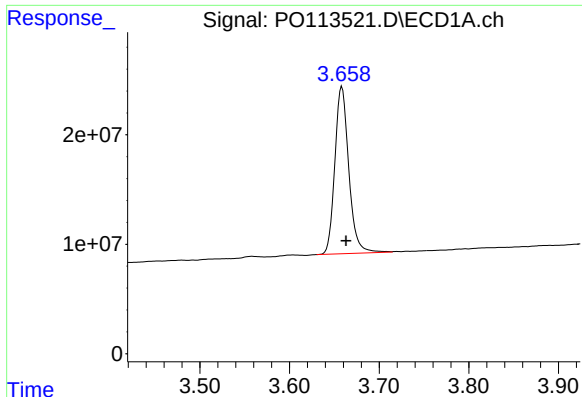

#1 Tetrachloro-m-xylene


R.T.: 3.658 min
Delta R.T.: -0.005 min
Response: 164081863
Conc: 20.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

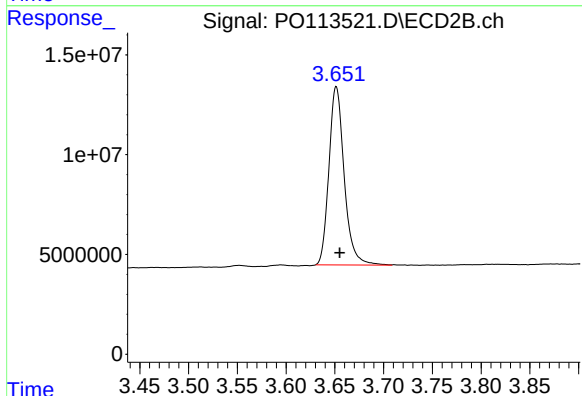


#1 Tetrachloro-m-xylene

R.T.: 3.652 min
Delta R.T.: -0.003 min
Response: 97314289
Conc: 19.23 ng/ml

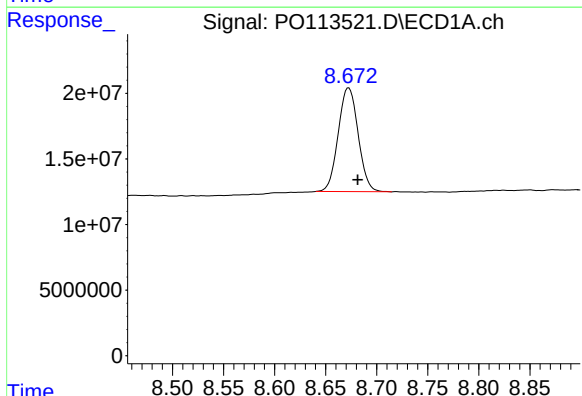


#2 Decachlorobiphenyl

R.T.: 8.673 min
Delta R.T.: -0.009 min
Response: 107592658
Conc: 15.52 ng/ml

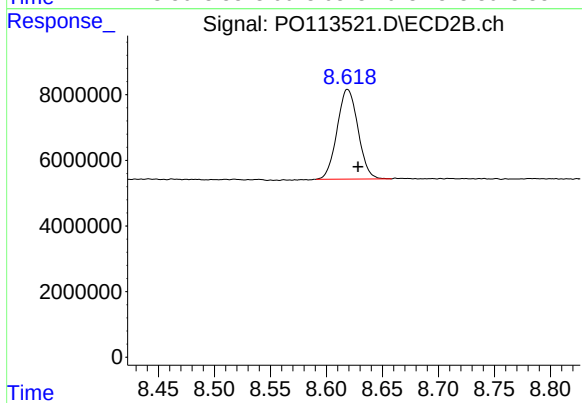

#2 Decachlorobiphenyl


R.T.: 8.619 min
Delta R.T.: -0.009 min
Response: 35537264
Conc: 18.75 ng/ml

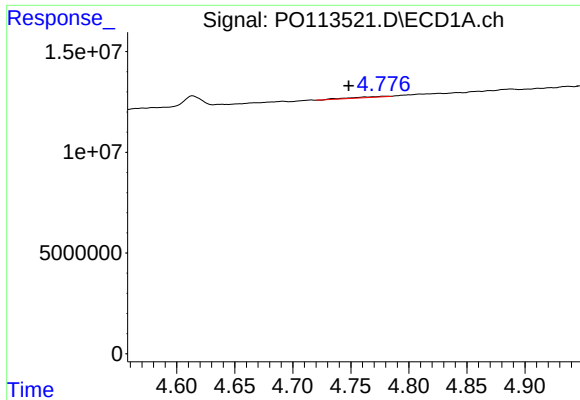

#3 AR-1016-1


R.T.: 4.779 min
Delta R.T.: 0.030 min
Response: 853439
Conc: 3.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

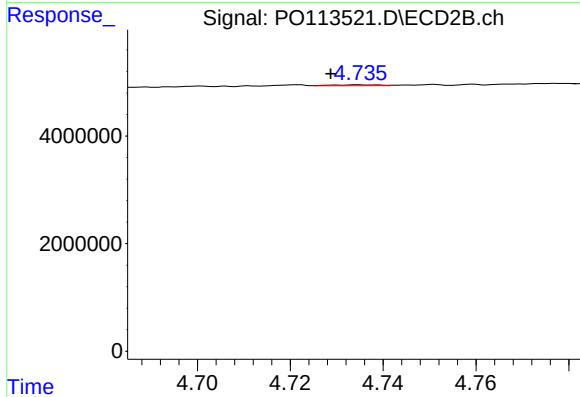


#3 AR-1016-1

R.T.: 4.735 min
Delta R.T.: 0.006 min
Response: 119635
Conc: 0.70 ng/ml

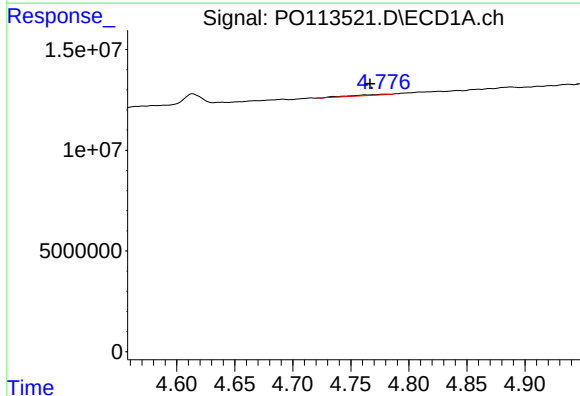


#4 AR-1016-2

R.T.: 4.779 min
Delta R.T.: 0.012 min
Response: 853439
Conc: 2.13 ng/ml

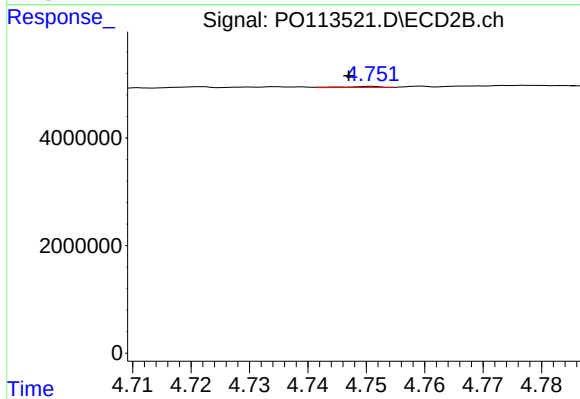

#4 AR-1016-2


R.T.: 4.751 min
Delta R.T.: 0.004 min
Response: 77918
Conc: 0.30 ng/ml

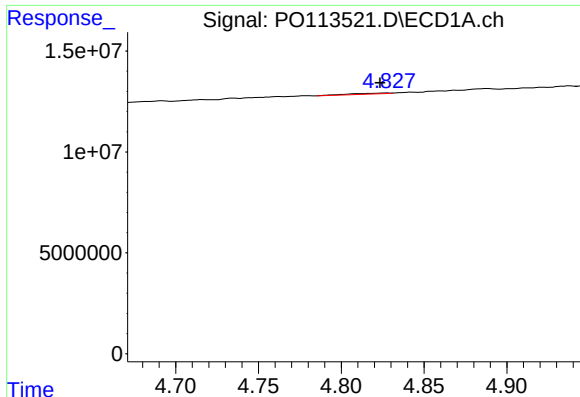

#5 AR-1016-3


R.T.: 4.827 min
Delta R.T.: 0.004 min
Response: 739503
Conc: 2.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

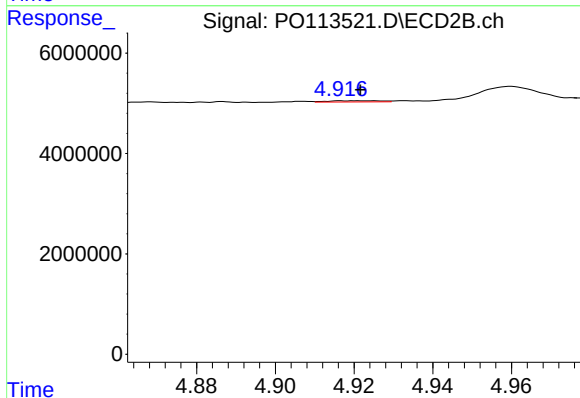


#5 AR-1016-3

R.T.: 4.917 min
Delta R.T.: -0.005 min
Response: 225358
Conc: 1.61 ng/ml

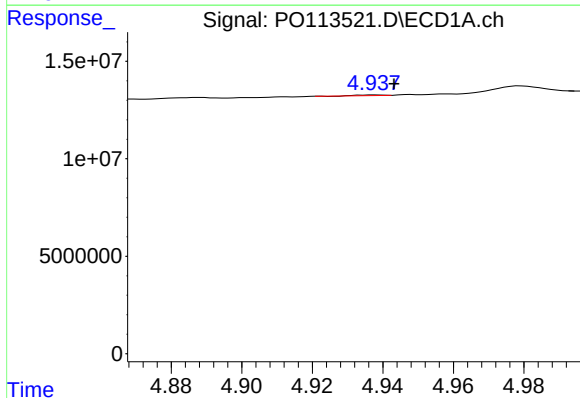


#6 AR-1016-4

R.T.: 4.938 min
Delta R.T.: -0.005 min
Response: 129818
Conc: 0.60 ng/ml

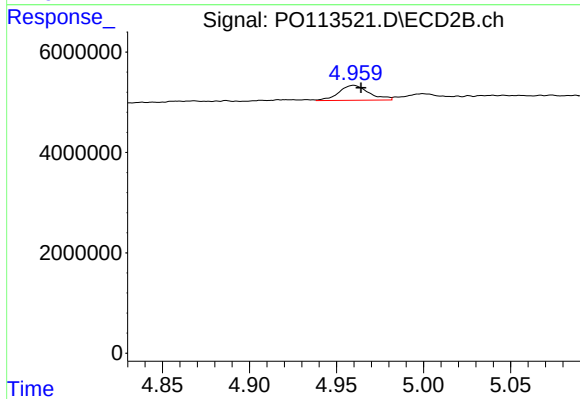

#6 AR-1016-4


R.T.: 4.960 min
Delta R.T.: -0.004 min
Response: 3581854
Conc: 30.69 ng/ml

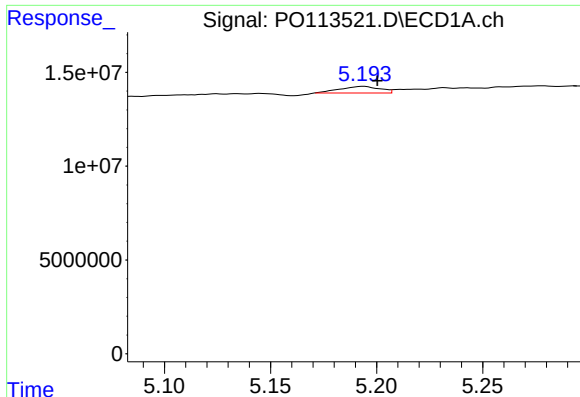

#7 AR-1016-5


R.T.: 5.194 min
Delta R.T.: -0.007 min
Response: 4637086
Conc: 20.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

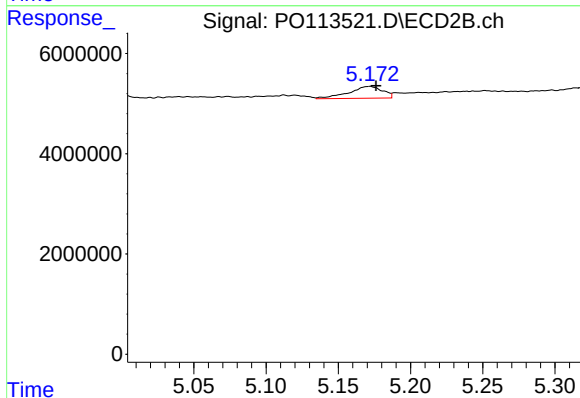


#7 AR-1016-5

R.T.: 5.172 min
Delta R.T.: -0.004 min
Response: 3858560
Conc: 27.07 ng/ml

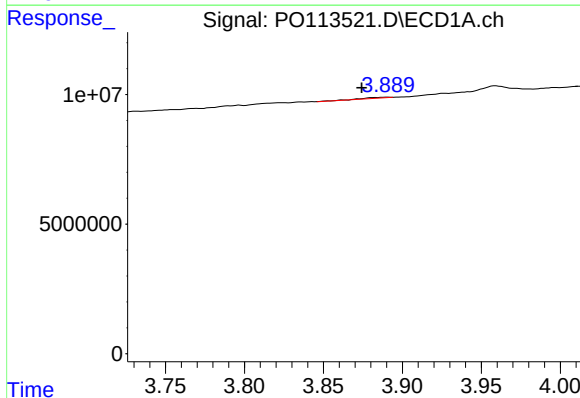


#8 AR-1221-1

R.T.: 3.890 min
Delta R.T.: 0.016 min
Response: 312041
Conc: 3.33 ng/ml

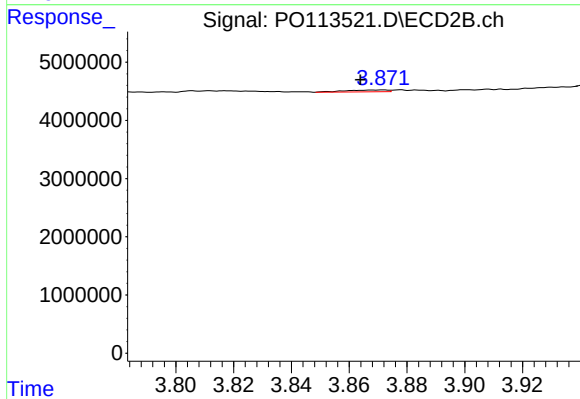

#8 AR-1221-1


R.T.: 3.872 min
Delta R.T.: 0.008 min
Response: 328992
Conc: 5.21 ng/ml

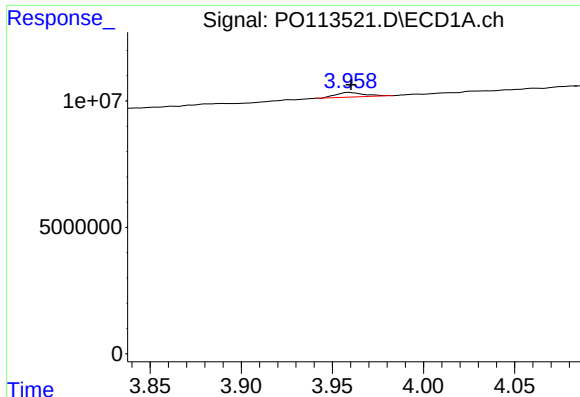

#9 AR-1221-2


R.T.: 3.959 min
Delta R.T.: -0.001 min
Response: 1959502
Conc: 29.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

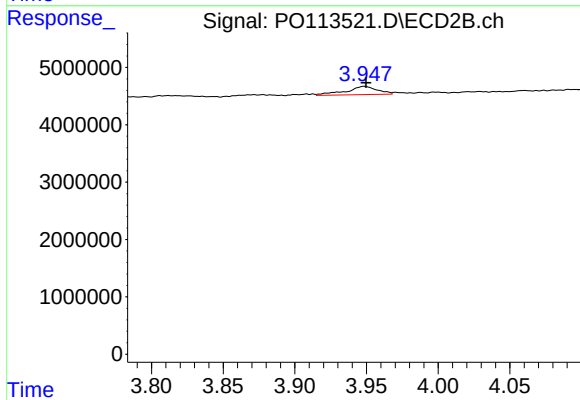


#9 AR-1221-2

R.T.: 3.948 min
Delta R.T.: -0.001 min
Response: 2172872
Conc: 46.56 ng/ml

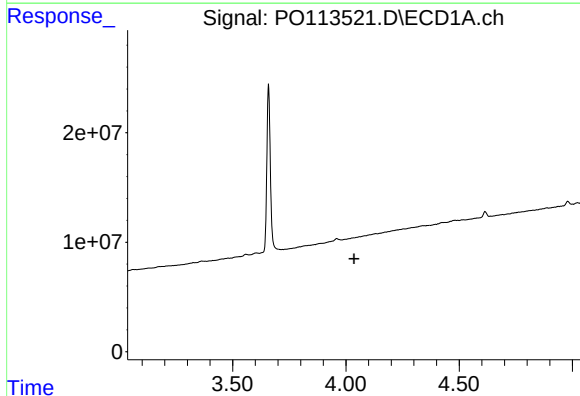


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.036 min
Response: 0
Conc: N.D.

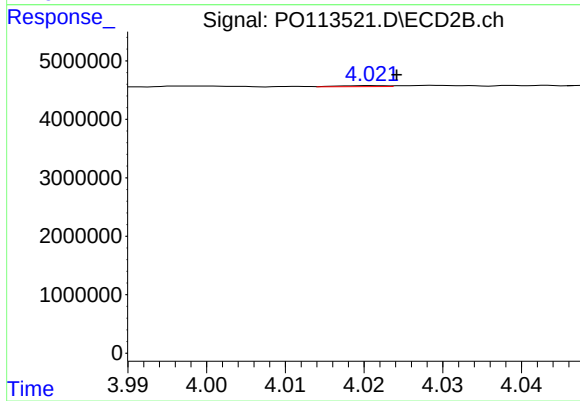

#10 AR-1221-3


R.T.: 4.021 min
Delta R.T.: -0.003 min
Response: 70947
Conc: 0.48 ng/ml

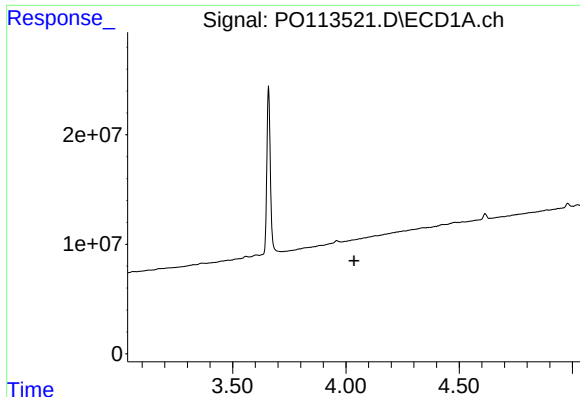

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 4.036 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

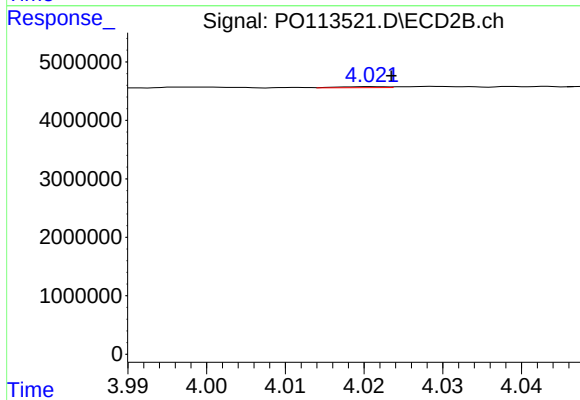


#11 AR-1232-1

R.T.: 4.021 min
Delta R.T.: -0.003 min
Response: 70947
Conc: 0.60 ng/ml

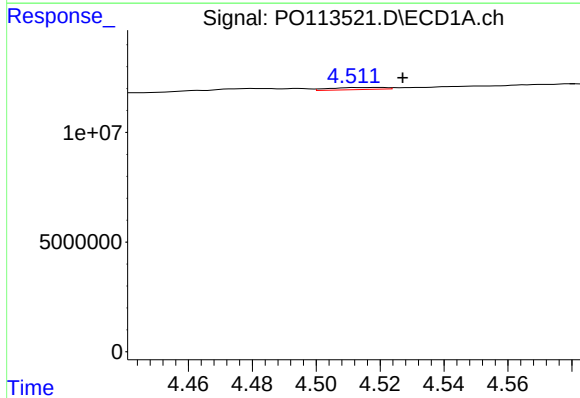


#12 AR-1232-2

R.T.: 4.520 min
Delta R.T.: -0.007 min
Response: 1113318
Conc: 11.15 ng/ml

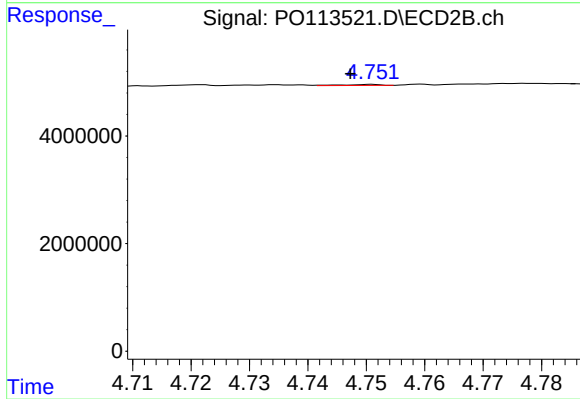

#12 AR-1232-2


R.T.: 4.751 min
Delta R.T.: 0.004 min
Response: 77918
Conc: 0.64 ng/ml

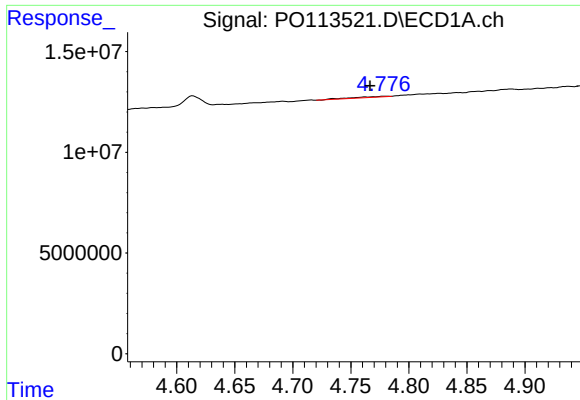

#13 AR-1232-3


R.T.: 4.779 min
Delta R.T.: 0.012 min
Response: 853439
Conc: 4.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

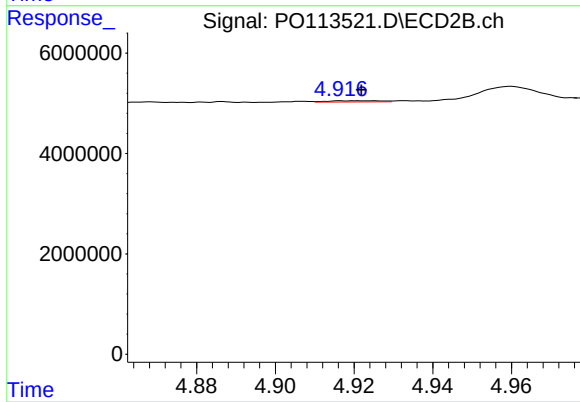


#13 AR-1232-3

R.T.: 4.917 min
Delta R.T.: -0.005 min
Response: 225358
Conc: 3.56 ng/ml

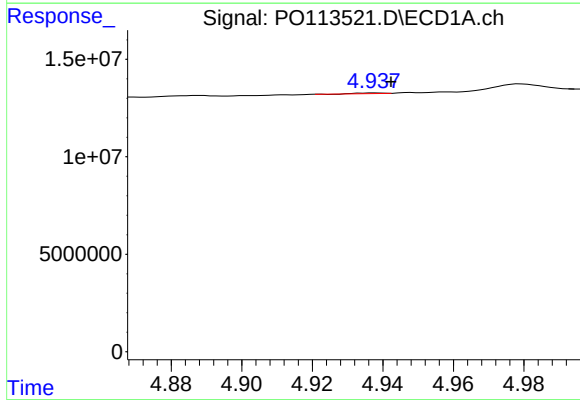


#14 AR-1232-4

R.T.: 4.938 min
Delta R.T.: -0.004 min
Response: 129818
Conc: 1.38 ng/ml

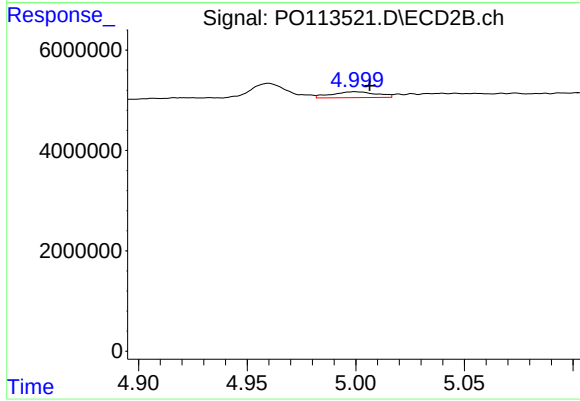

#14 AR-1232-4


R.T.: 5.000 min
Delta R.T.: -0.007 min
Response: 1693236
Conc: 30.12 ng/ml

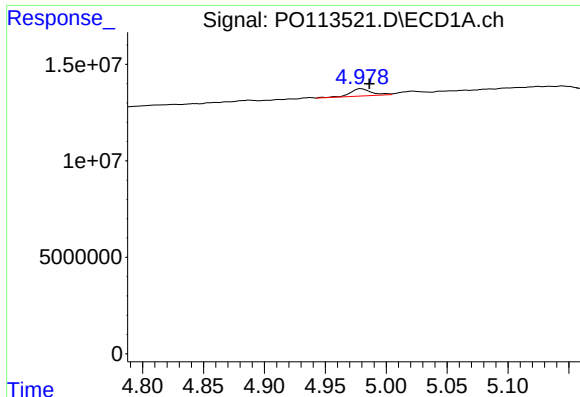

#15 AR-1232-5


R.T.: 4.979 min
Delta R.T.: -0.007 min
Response: 4570238
Conc: 73.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

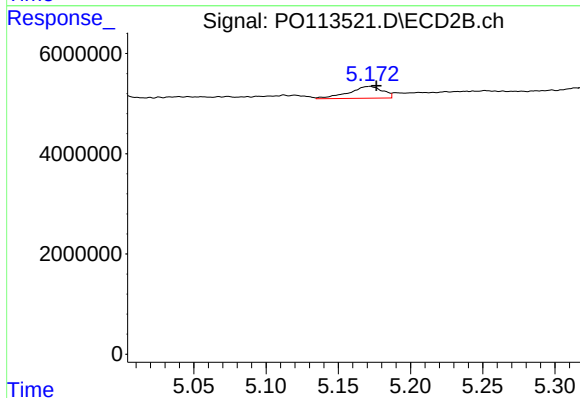


#15 AR-1232-5

R.T.: 5.172 min
Delta R.T.: -0.004 min
Response: 3858560
Conc: 64.46 ng/ml

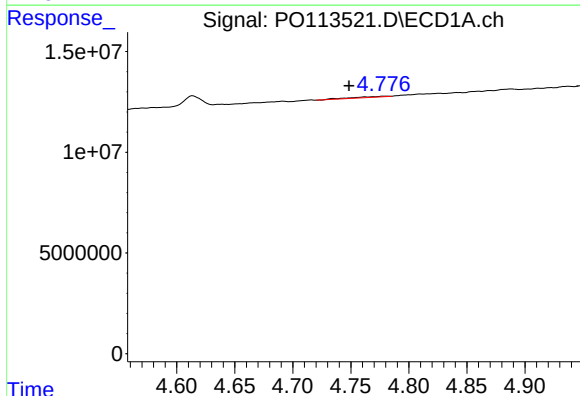


#16 AR-1242-1

R.T.: 4.779 min
Delta R.T.: 0.030 min
Response: 853439
Conc: 3.71 ng/ml

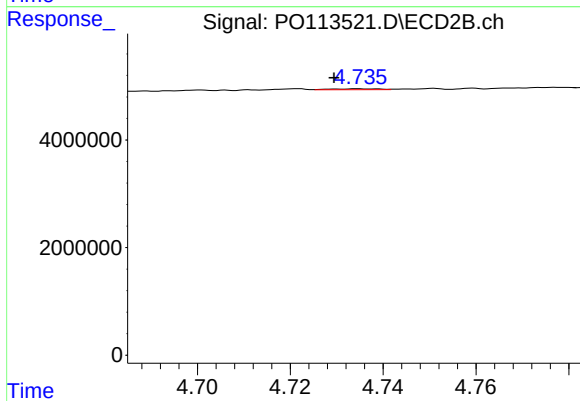

#16 AR-1242-1


R.T.: 4.735 min
Delta R.T.: 0.005 min
Response: 119635
Conc: 0.83 ng/ml

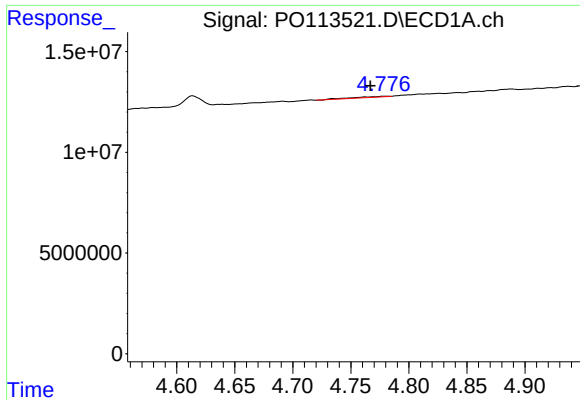

#17 AR-1242-2


R.T.: 4.779 min
Delta R.T.: 0.012 min
Response: 853439
Conc: 2.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

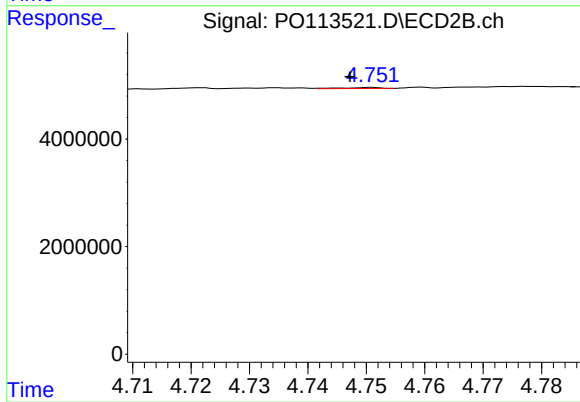


#17 AR-1242-2

R.T.: 4.751 min
Delta R.T.: 0.004 min
Response: 77918
Conc: 0.36 ng/ml

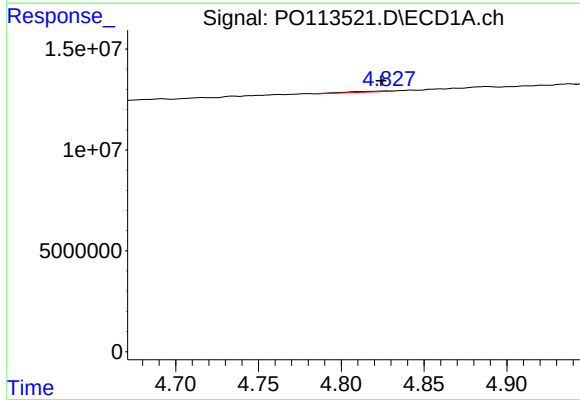


#18 AR-1242-3

R.T.: 4.827 min
Delta R.T.: 0.003 min
Response: 739503
Conc: 3.33 ng/ml

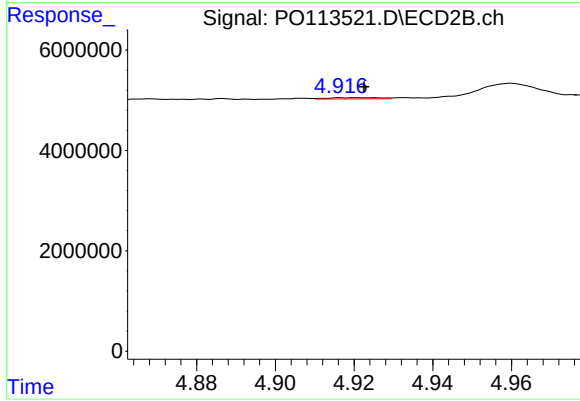

#18 AR-1242-3


R.T.: 4.917 min
Delta R.T.: -0.006 min
Response: 225358
Conc: 1.93 ng/ml

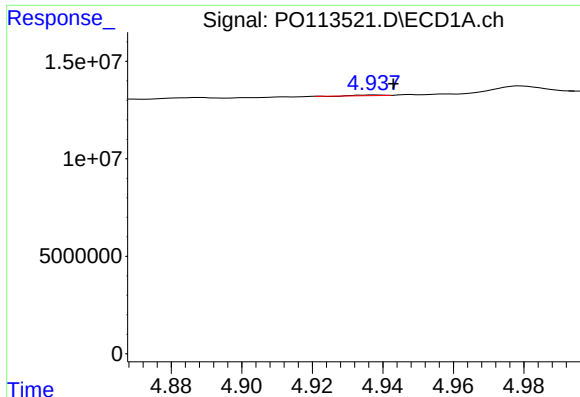

#19 AR-1242-4


R.T.: 4.938 min
Delta R.T.: -0.005 min
Response: 129818
Conc: 0.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

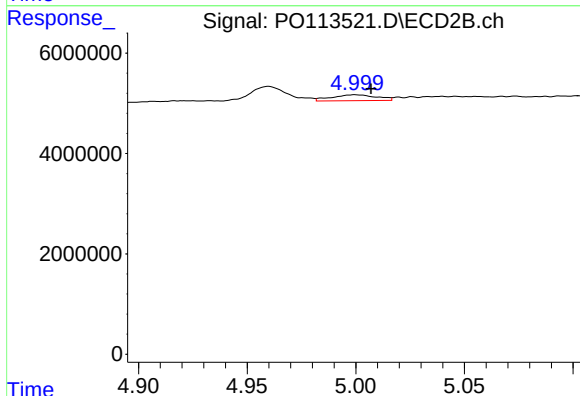


#19 AR-1242-4

R.T.: 5.000 min
Delta R.T.: -0.007 min
Response: 1693236
Conc: 14.39 ng/ml

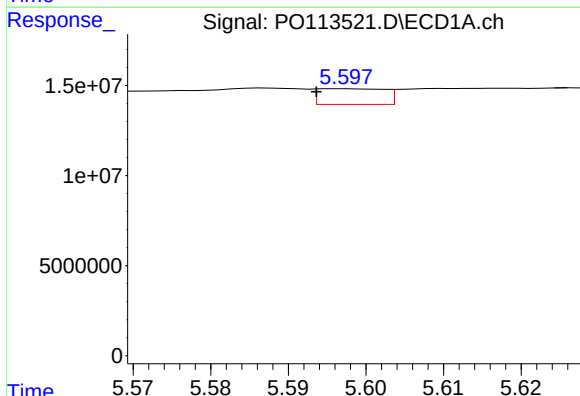


#20 AR-1242-5

R.T.: 5.597 min
Delta R.T.: 0.003 min
Response: 5157763
Conc: 25.77 ng/ml

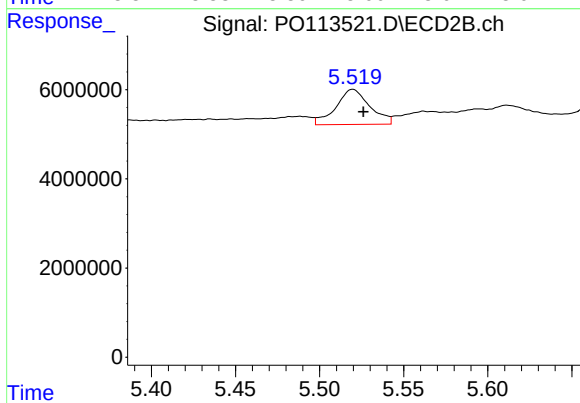

#20 AR-1242-5


R.T.: 5.520 min
Delta R.T.: -0.006 min
Response: 11065537
Conc: 74.20 ng/ml

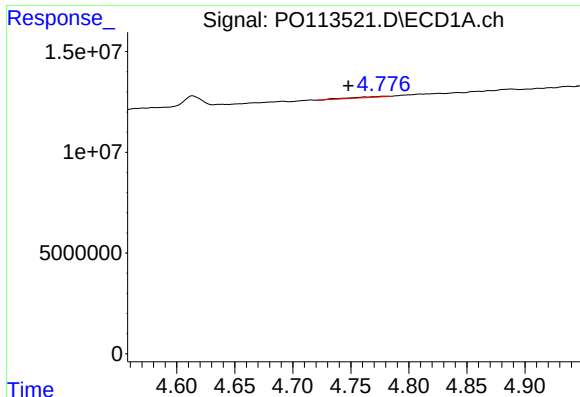

#21 AR-1248-1


R.T.: 4.779 min
Delta R.T.: 0.031 min
Response: 853439
Conc: 4.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

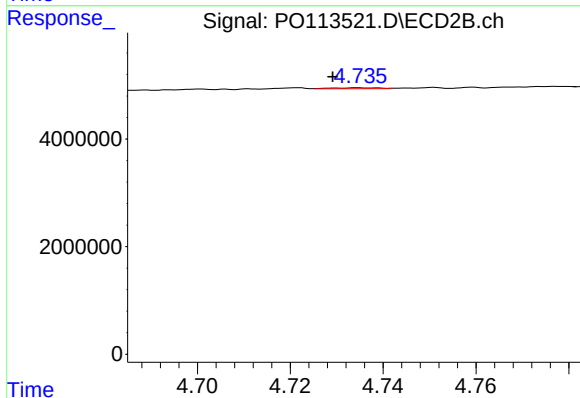


#21 AR-1248-1

R.T.: 4.735 min
Delta R.T.: 0.006 min
Response: 119635
Conc: 1.07 ng/ml

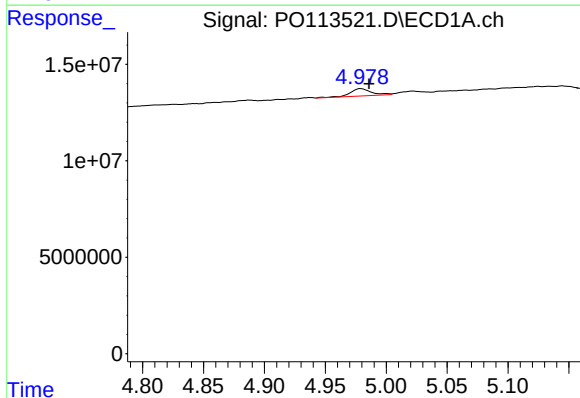


#22 AR-1248-2

R.T.: 4.979 min
Delta R.T.: -0.007 min
Response: 4570238
Conc: 18.90 ng/ml

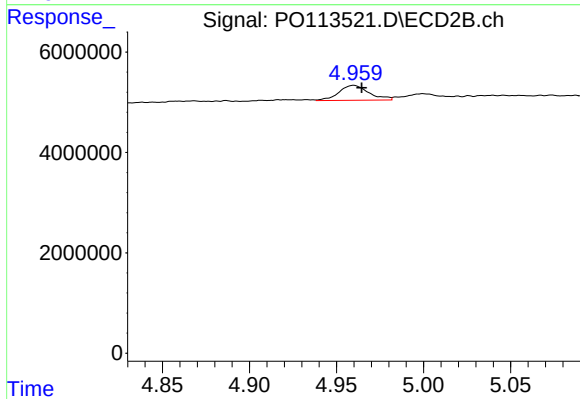

#22 AR-1248-2


R.T.: 4.960 min
Delta R.T.: -0.005 min
Response: 3581854
Conc: 22.29 ng/ml

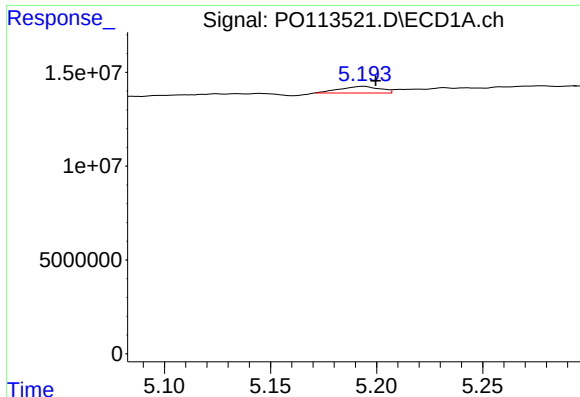

#23 AR-1248-3


R.T.: 5.194 min
Delta R.T.: -0.006 min
Response: 4637086
Conc: 14.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

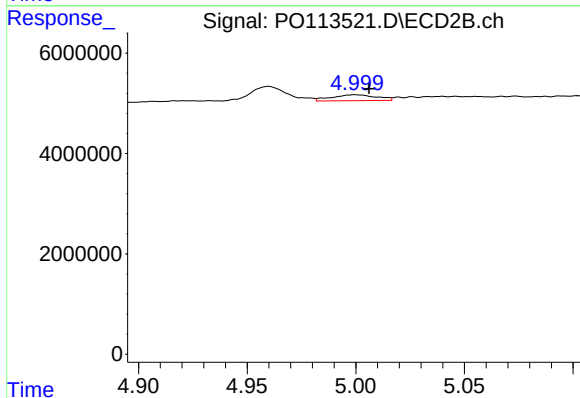


#23 AR-1248-3

R.T.: 5.000 min
Delta R.T.: -0.006 min
Response: 1693236
Conc: 9.98 ng/ml

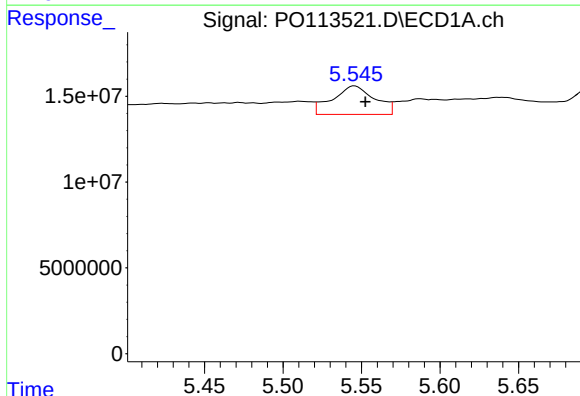


#24 AR-1248-4

R.T.: 5.546 min
Delta R.T.: -0.007 min
Response: 31032487
Conc: 62.11 ng/ml

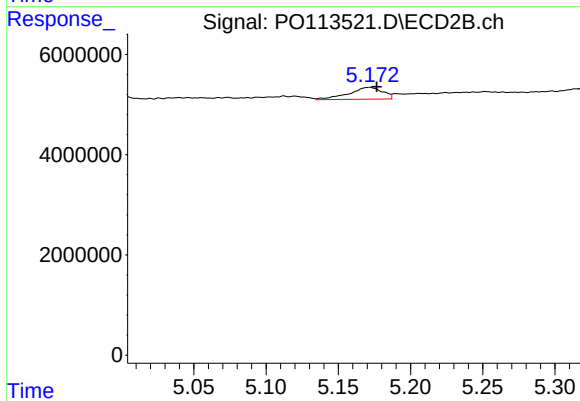

#24 AR-1248-4


R.T.: 5.172 min
Delta R.T.: -0.005 min
Response: 3858560
Conc: 19.37 ng/ml

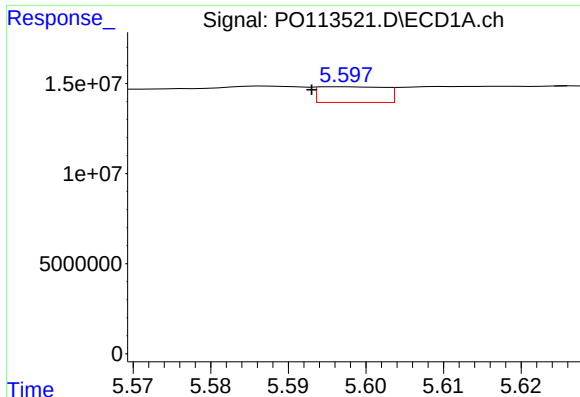

#25 AR-1248-5


R.T.: 5.597 min
Delta R.T.: 0.004 min
Response: 5157763
Conc: 15.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

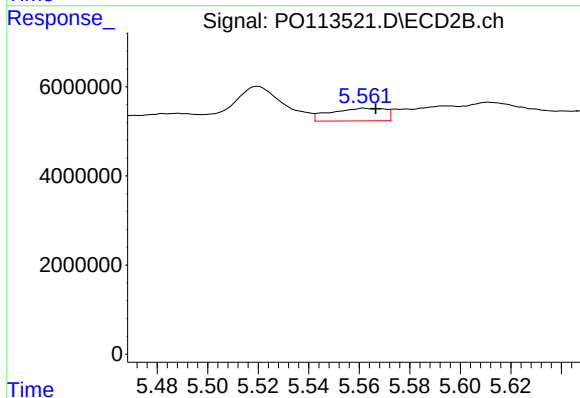


#25 AR-1248-5

R.T.: 5.562 min
Delta R.T.: -0.004 min
Response: 4288584
Conc: 20.20 ng/ml

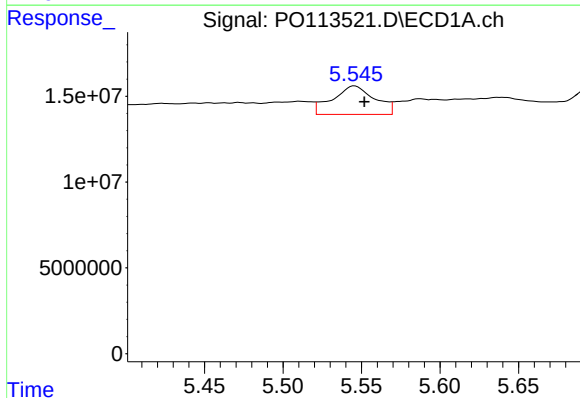


#26 AR-1254-1

R.T.: 5.546 min
Delta R.T.: -0.006 min
Response: 31032487
Conc: 57.47 ng/ml

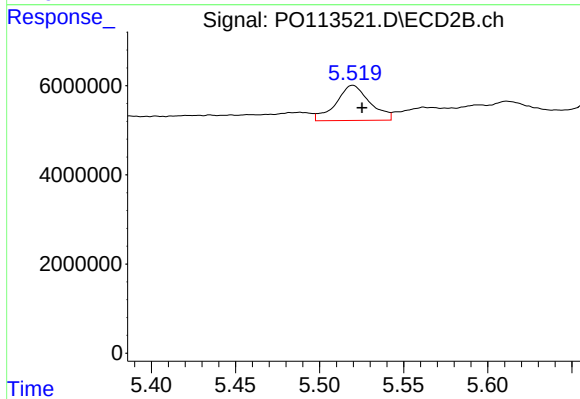

#26 AR-1254-1


R.T.: 5.520 min
Delta R.T.: -0.006 min
Response: 11065537
Conc: 35.09 ng/ml

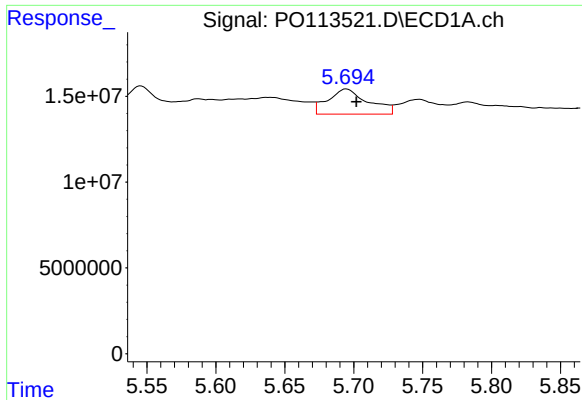

#27 AR-1254-2


R.T.: 5.695 min
Delta R.T.: -0.007 min
Response: 29563033
Conc: 59.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

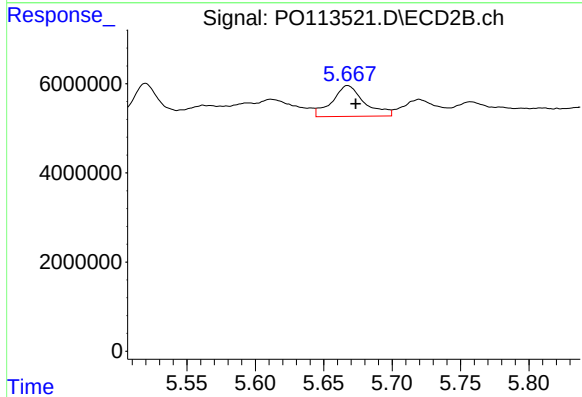


#27 AR-1254-2

R.T.: 5.668 min
Delta R.T.: -0.006 min
Response: 11293119
Conc: 40.28 ng/ml

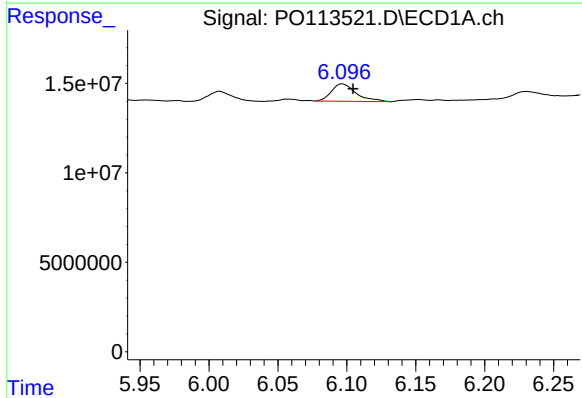


#28 AR-1254-3

R.T.: 6.097 min
Delta R.T.: -0.008 min
Response: 12088115
Conc: 16.36 ng/ml

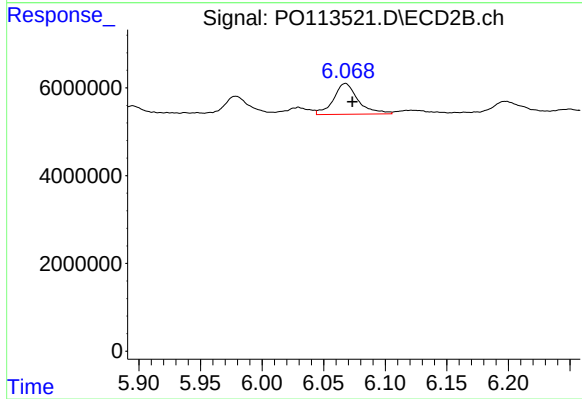

#28 AR-1254-3


R.T.: 6.068 min
Delta R.T.: -0.006 min
Response: 9800367
Conc: 23.51 ng/ml

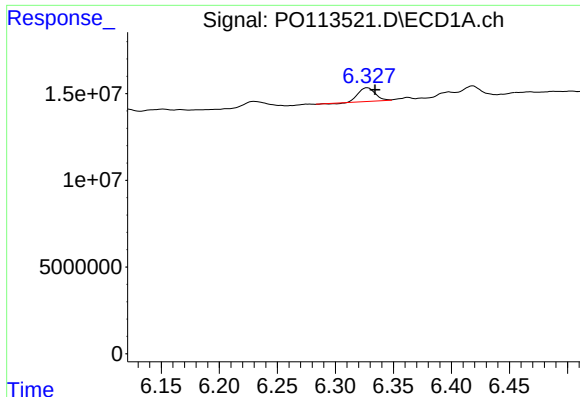

#29 AR-1254-4


R.T.: 6.328 min
Delta R.T.: -0.007 min
Response: 8086032
Conc: 14.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

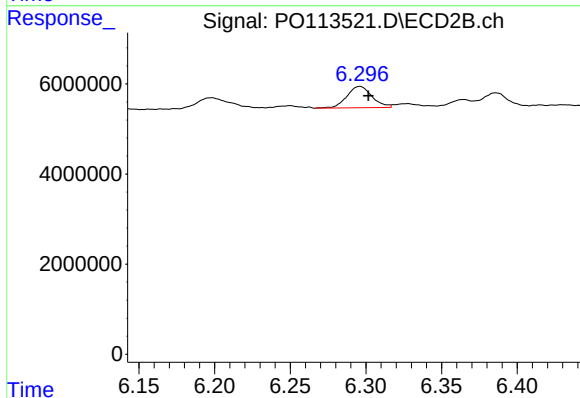


#29 AR-1254-4

R.T.: 6.296 min
Delta R.T.: -0.006 min
Response: 5434103
Conc: 19.77 ng/ml

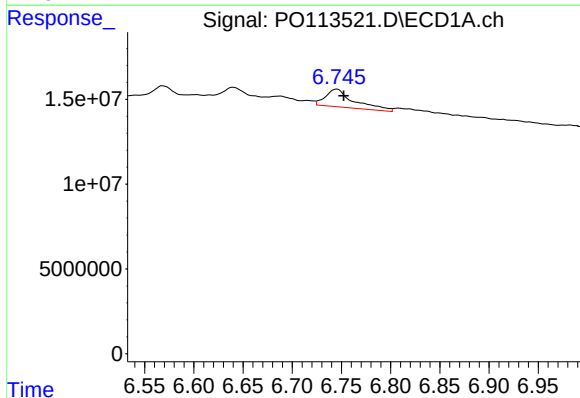


#30 AR-1254-5

R.T.: 6.745 min
Delta R.T.: -0.007 min
Response: 20997695
Conc: 29.96 ng/ml

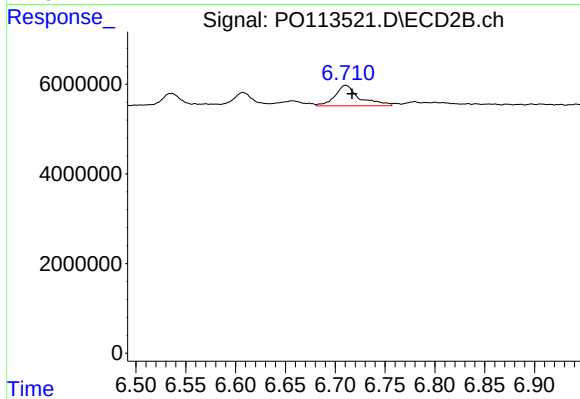

#30 AR-1254-5


R.T.: 6.710 min
Delta R.T.: -0.006 min
Response: 7796775
Conc: 21.81 ng/ml

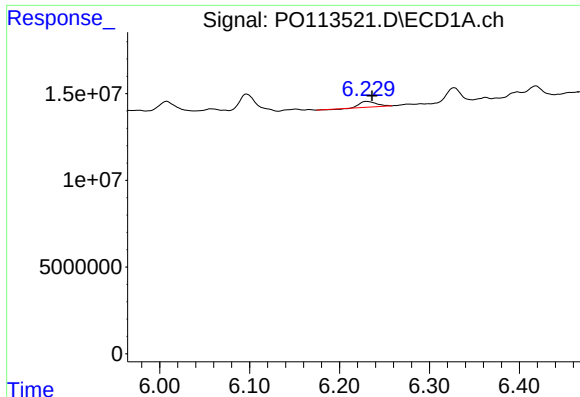

#31 AR-1260-1


R.T.: 6.230 min
Delta R.T.: -0.006 min
Response: 4047248
Conc: 9.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

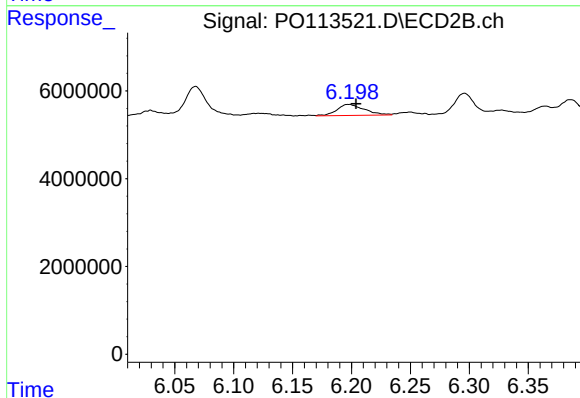


#31 AR-1260-1

R.T.: 6.198 min
Delta R.T.: -0.006 min
Response: 4098147
Conc: 16.07 ng/ml

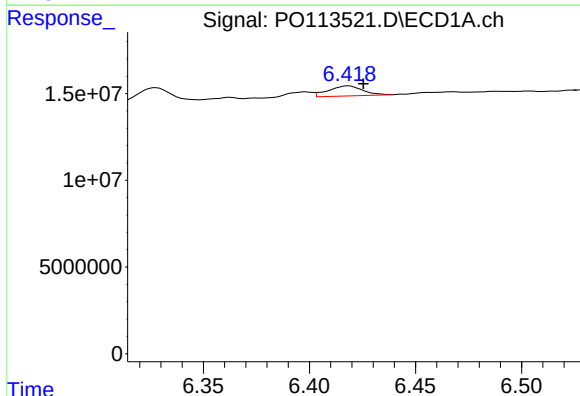


#32 AR-1260-2

R.T.: 6.418 min
Delta R.T.: -0.007 min
Response: 6542587
Conc: 9.53 ng/ml

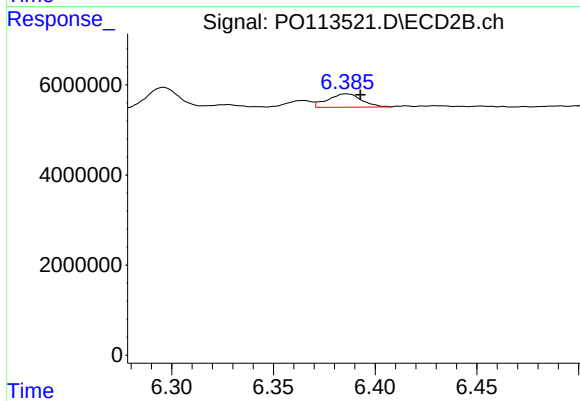

#32 AR-1260-2


R.T.: 6.386 min
Delta R.T.: -0.007 min
Response: 3429454
Conc: 9.92 ng/ml

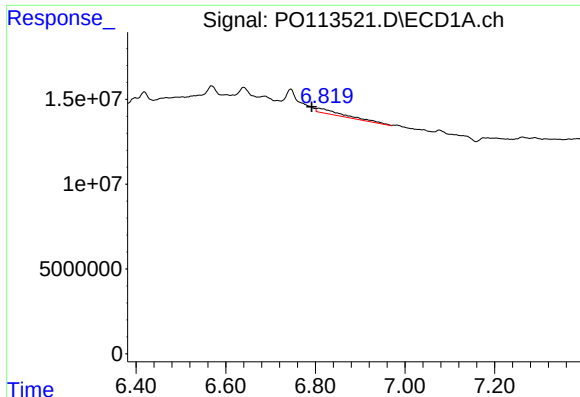

#33 AR-1260-3


R.T.: 6.808 min
Delta R.T.: 0.016 min
Response: 11786363
Conc: 19.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

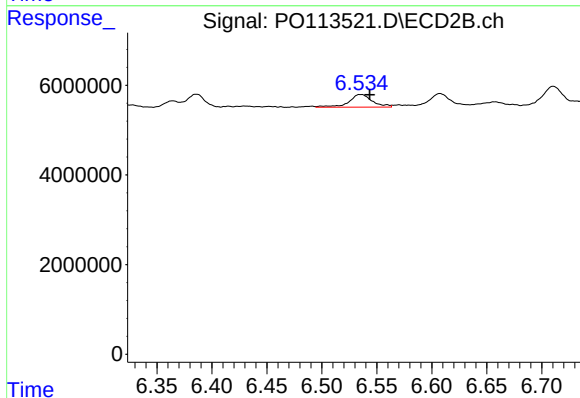


#33 AR-1260-3

R.T.: 6.535 min
Delta R.T.: -0.008 min
Response: 4212923
Conc: 14.16 ng/ml

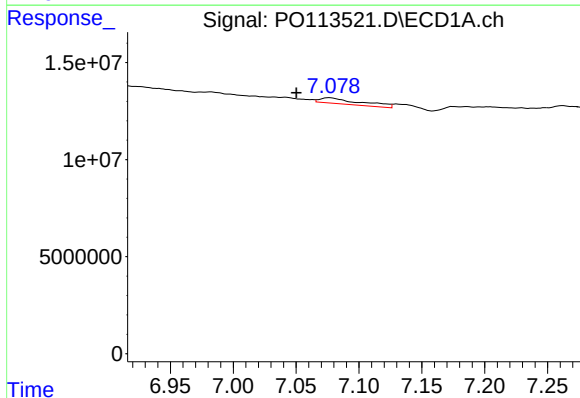


#34 AR-1260-4

R.T.: 7.076 min
Delta R.T.: 0.026 min
Response: 6713740
Conc: 14.99 ng/ml

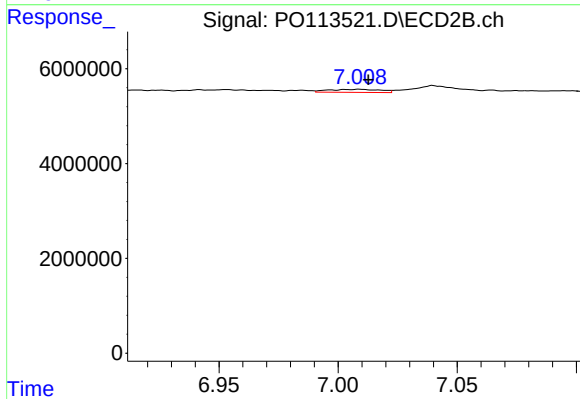

#34 AR-1260-4


R.T.: 7.009 min
Delta R.T.: -0.004 min
Response: 970007
Conc: 4.68 ng/ml

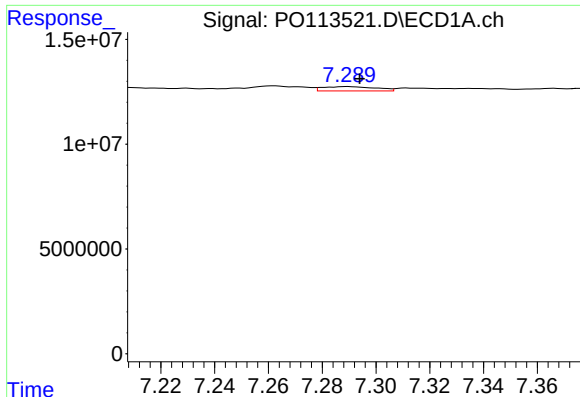

#35 AR-1260-5


R.T.: 7.290 min
Delta R.T.: -0.004 min
Response: 2825918
Conc: 2.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

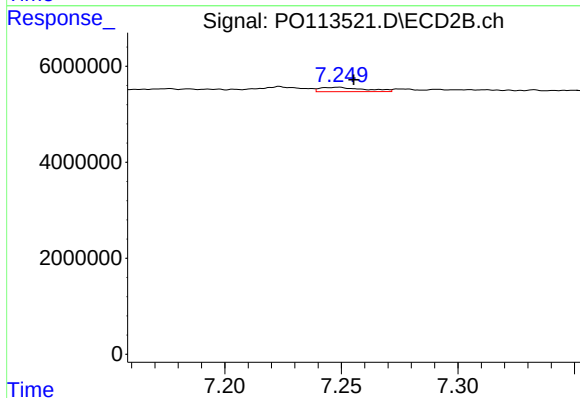


#35 AR-1260-5

R.T.: 7.249 min
Delta R.T.: -0.007 min
Response: 1215235
Conc: 2.59 ng/ml

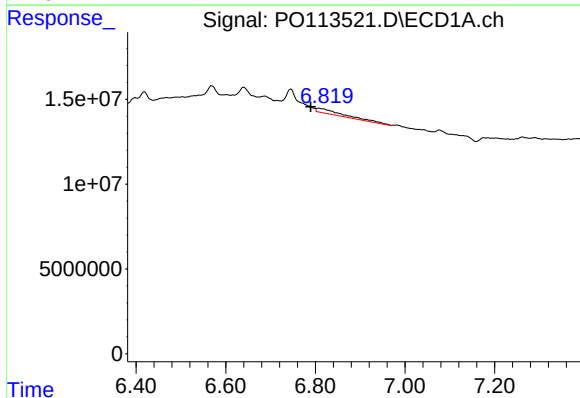


#36 AR-1262-1

R.T.: 6.808 min
Delta R.T.: 0.018 min
Response: 11786363
Conc: 12.87 ng/ml

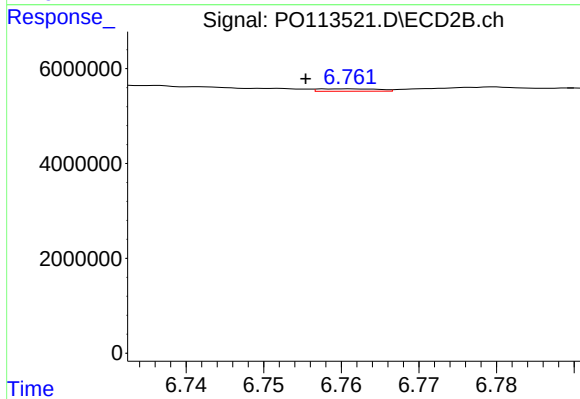

#36 AR-1262-1


R.T.: 6.761 min
Delta R.T.: 0.005 min
Response: 274147
Conc: 0.66 ng/ml

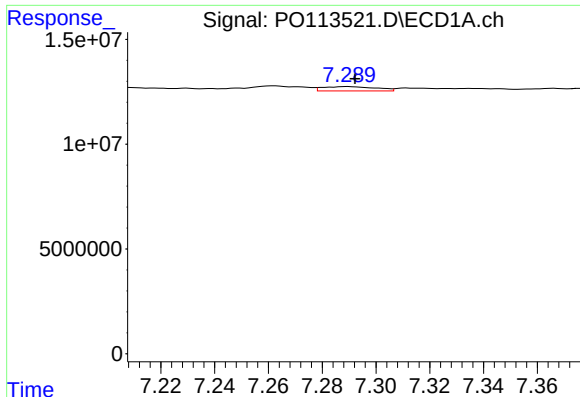

#37 AR-1262-2


R.T.: 7.290 min
Delta R.T.: -0.003 min
Response: 2825918
Conc: 1.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

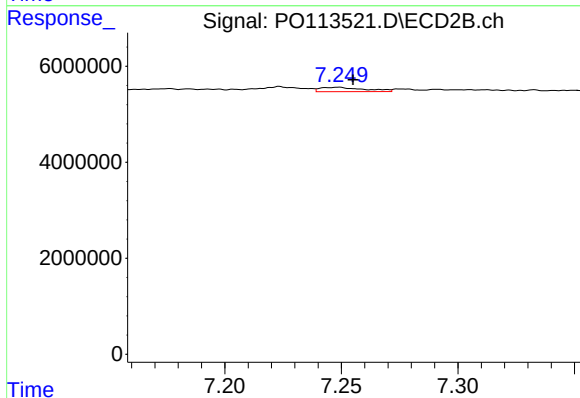


#37 AR-1262-2

R.T.: 7.249 min
Delta R.T.: -0.006 min
Response: 1215235
Conc: 2.35 ng/ml

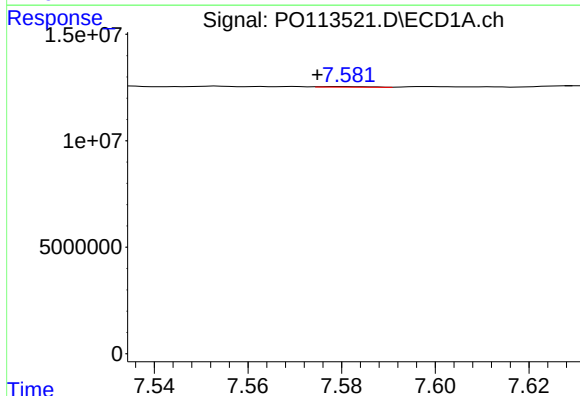


#38 AR-1262-3

R.T.: 7.580 min
Delta R.T.: 0.005 min
Response: 208021
Conc: 0.38 ng/ml

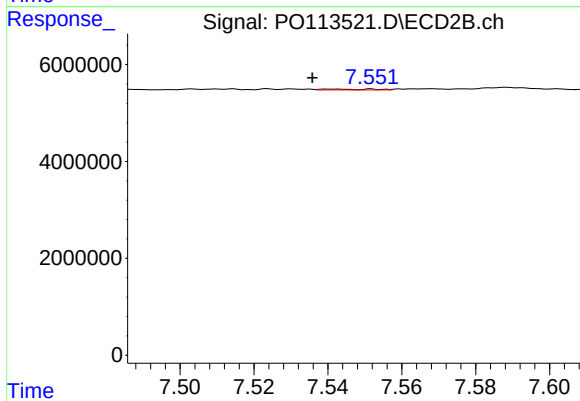

#38 AR-1262-3


R.T.: 7.541 min
Delta R.T.: 0.005 min
Response: 163349
Conc: 0.91 ng/ml

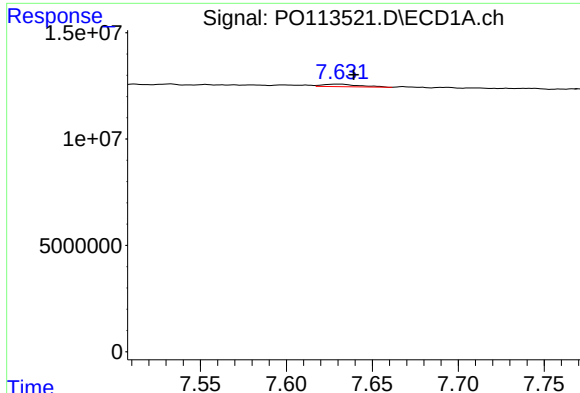

#39 AR-1262-4


R.T.: 7.630 min
Delta R.T.: -0.009 min
Response: 1767174
Conc: 1.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

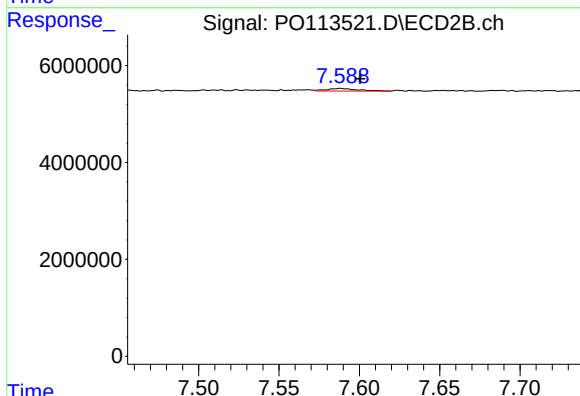


#39 AR-1262-4

R.T.: 7.588 min
Delta R.T.: -0.012 min
Response: 721417
Conc: 2.49 ng/ml

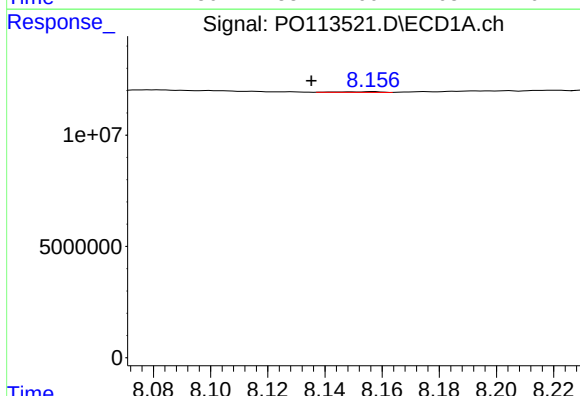


#40 AR-1262-5

R.T.: 8.157 min
Delta R.T.: 0.022 min
Response: 274195
Conc: 0.66 ng/ml

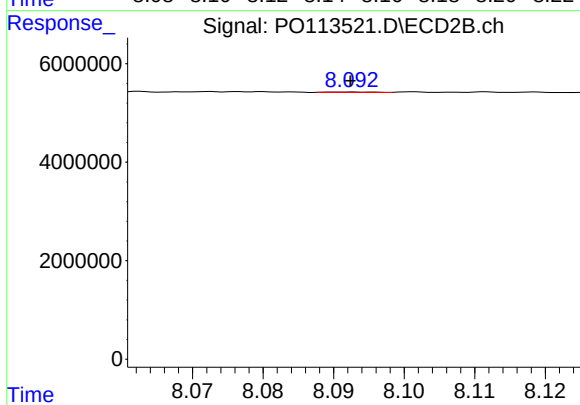

#40 AR-1262-5


R.T.: 8.092 min
Delta R.T.: 0.000 min
Response: 44966
Conc: 0.42 ng/ml

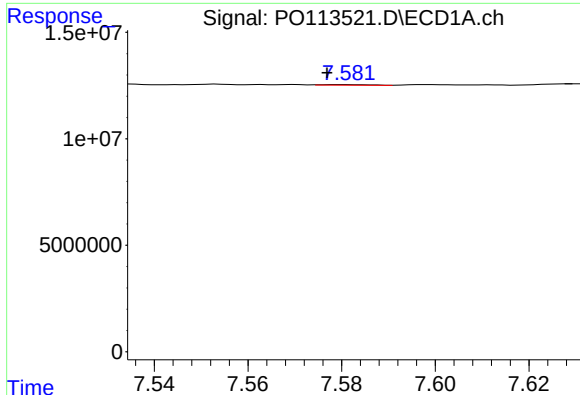

#41 AR-1268-1


R.T.: 7.580 min
Delta R.T.: 0.003 min
Response: 208021
Conc: 0.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

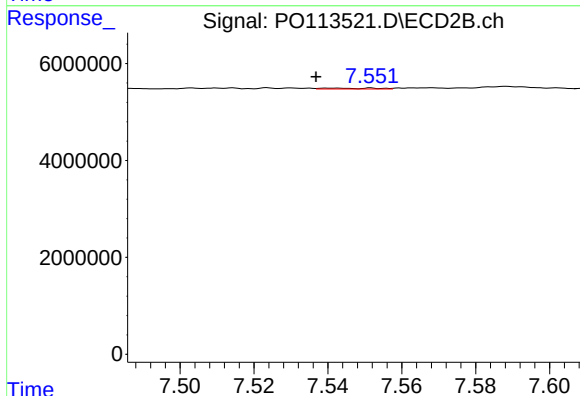


#41 AR-1268-1

R.T.: 7.541 min
Delta R.T.: 0.004 min
Response: 163349
Conc: 0.32 ng/ml

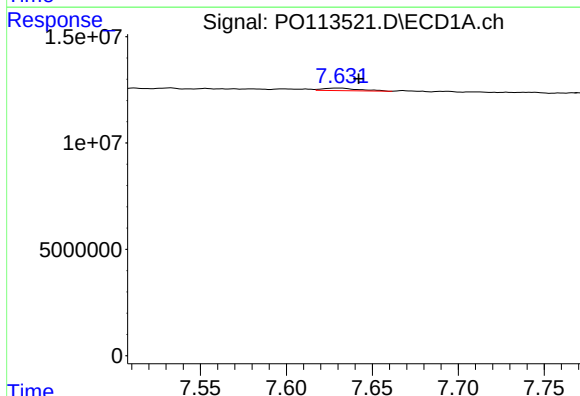


#42 AR-1268-2

R.T.: 7.630 min
Delta R.T.: -0.012 min
Response: 1767174
Conc: 1.22 ng/ml

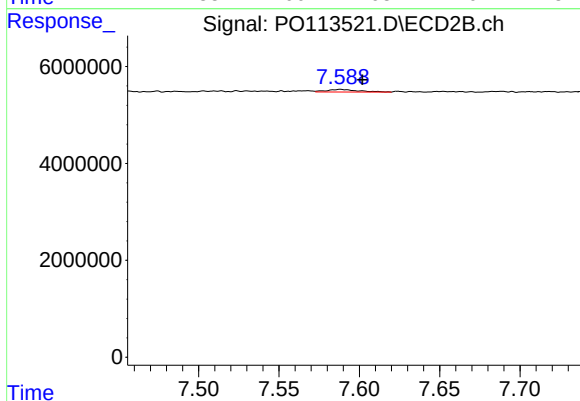

#42 AR-1268-2


R.T.: 7.588 min
Delta R.T.: -0.014 min
Response: 721417
Conc: 1.74 ng/ml

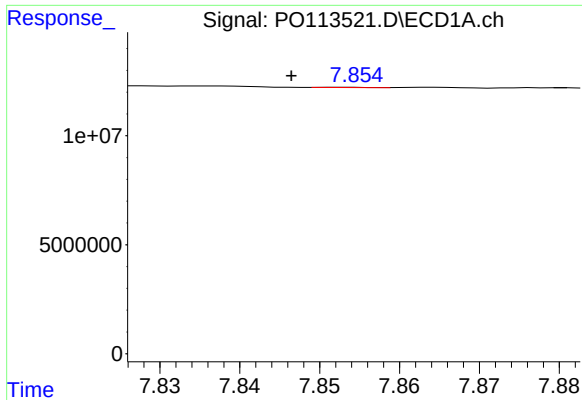

#43 AR-1268-3


R.T.: 7.853 min
Delta R.T.: 0.007 min
Response: 51403
Conc: 0.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

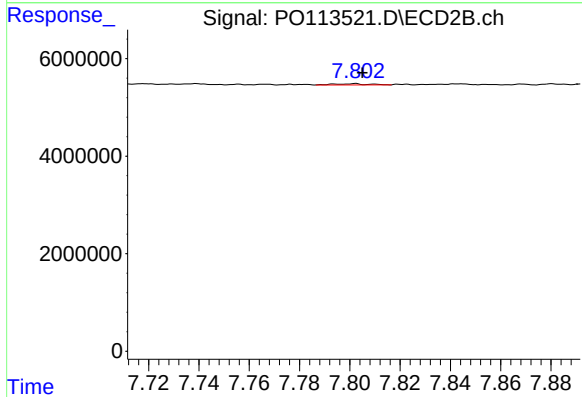


#43 AR-1268-3

R.T.: 7.802 min
Delta R.T.: -0.003 min
Response: 229160
Conc: 0.70 ng/ml

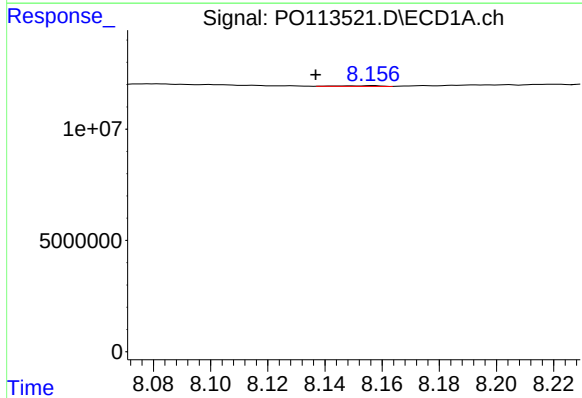


#44 AR-1268-4

R.T.: 8.157 min
Delta R.T.: 0.020 min
Response: 274195
Conc: 0.60 ng/ml

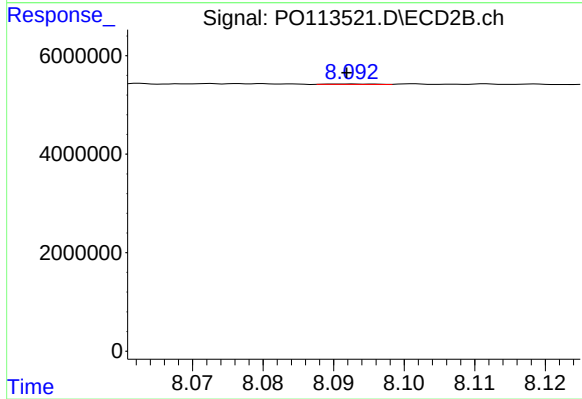

#44 AR-1268-4


R.T.: 8.092 min
Delta R.T.: 0.000 min
Response: 44966
Conc: 0.37 ng/ml

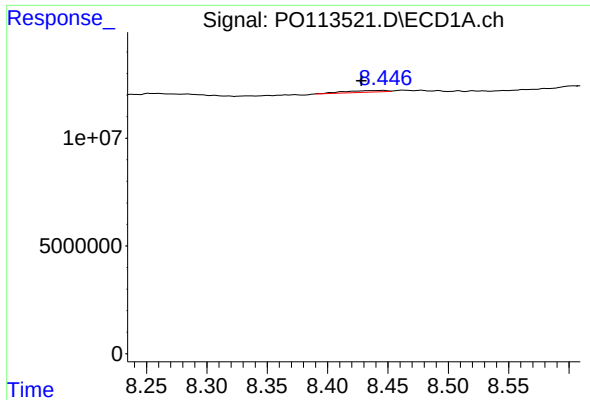

#45 AR-1268-5

R.T.: 8.446 min
Delta R.T.: 0.018 min
Response: 1895925
Conc: 0.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

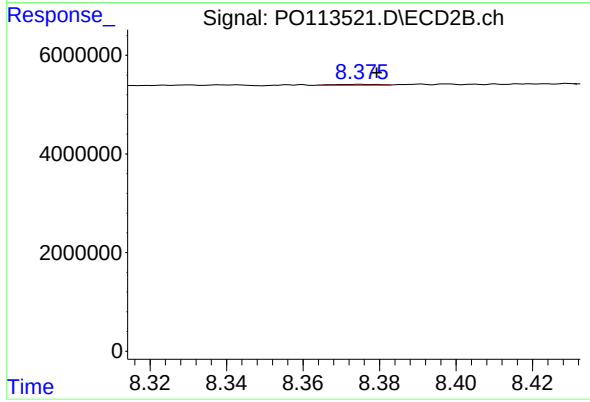

#45 AR-1268-5

R.T.: 8.375 min
Delta R.T.: -0.004 min
Response: 155502
Conc: 0.20 ng/ml