

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090525\
 Data File : P0113528.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 22:57
 Operator : YP/AJ
 Sample : Q2893-09
 Misc : AR1268 WATER LOD 25PPB
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:37:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.658	3.652	160.7E6	96397606	19.632	19.048
2)	SA Decachlor...	8.672	8.618	125.5E6	40243794	18.104	21.239
Target Compounds							
3)	L1 AR-1016-1	4.804f	4.731	1139427	48510	4.268	0.284 #
4)	L1 AR-1016-2	4.804f	4.748	1139427	105738	2.838	0.410 #
5)	L1 AR-1016-3	4.816	4.918	182425	198741	0.715	1.423 #
6)	L1 AR-1016-4	4.945	4.963	288115	389337	1.321	3.336 #
7)	L1 AR-1016-5	5.193	5.174	1569991	392324	7.084	2.753 #
8)	L2 AR-1221-1	3.881	3.861	172480	105468	1.843	1.671
9)	L2 AR-1221-2	3.958	3.950	1803379	1752270	26.697	37.543 #
10)	L2 AR-1221-3	0.000	4.024	0	24533	N.D.	0.165 #
11)	L3 AR-1232-1	0.000	4.024	0	24533	N.D.	0.209 #
12)	L3 AR-1232-2	4.527	4.748	1008896	105738	10.104	0.863 #
13)	L3 AR-1232-3	4.804f	4.918	1139427	198741	6.014	3.137 #
14)	L3 AR-1232-4	4.945	5.003	288115	271046	3.060	4.821 #
15)	L3 AR-1232-5	4.966	5.174	125703	392324	2.029	6.554 #
16)	L4 AR-1242-1	4.804f	4.731	1139427	48510	4.955	0.336 #
17)	L4 AR-1242-2	4.804f	4.748	1139427	105738	3.316	0.487 #
18)	L4 AR-1242-3	4.816	4.926	182425	73407	0.822	0.628
19)	L4 AR-1242-4	4.945	5.003	288115	271046	1.661	2.304 #
20)	L4 AR-1242-5	5.601	5.536	5200484	2000121	25.981	13.412 #
21)	L5 AR-1248-1	4.804f	4.731	1139427	48510	6.531	0.435 #
22)	L5 AR-1248-2	4.966	4.963	125703	389337	0.520	2.423 #
23)	L5 AR-1248-3	5.193	5.003	1569991	271046	4.924	1.598 #
24)	L5 AR-1248-4	5.550	5.174	4486476	392324	8.980	1.969 #
25)	L5 AR-1248-5	5.601	5.574	5200484	2558599	15.229	12.052
26)	L6 AR-1254-1	5.550	5.536	4486476	2000121	8.309	6.342
27)	L6 AR-1254-2	5.693	5.676	2849426	599265	5.774	2.138 #
28)	L6 AR-1254-3	6.104	6.078	1910147	837080	2.585	2.008
29)	L6 AR-1254-4	6.330	6.297	2801774	373577	5.030	1.359 #
30)	L6 AR-1254-5	6.735	6.719	3346516	339433	4.774	0.949 #
31)	L7 AR-1260-1	6.239	6.201	1249133	577301	2.801	2.263
32)	L7 AR-1260-2	6.451	6.418	1333341	311337	1.942	0.901 #
33)	L7 AR-1260-3	6.783	6.540	11961356	680626	19.371	2.288 #
34)	L7 AR-1260-4	7.039	7.002	22033898	4994436	49.197	24.099 #
35)	L7 AR-1260-5	7.286	7.248	8797647	2796433	7.267	5.970
36)	L8 AR-1262-1	6.783	6.748	11961356	3698933	13.062	8.921 #
37)	L8 AR-1262-2	7.286	7.248	8797647	2796433	5.818	5.402
38)	L8 AR-1262-3	7.568	7.528	31194025	9363122	56.296	52.136
39)	L8 AR-1262-4	7.634	7.593	29109781	7807688	29.766	26.932
40)	L8 AR-1262-5	8.128	8.084	8896581	2326141	21.341	21.472
41)	L9 AR-1268-1	7.568	7.528	31194025	9363122	18.127	18.378

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090525\
Data File : P0113528.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2025 22:57
Operator : YP/AJ
Sample : Q2893-09
Misc : AR1268 WATER LOD 25PPB
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 23:37:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	7.634	7.593	29109781	7807688	20.101	18.795
43)	L9 AR-1268-3	7.837	7.796	18441931	5852090	15.288	17.923
44)	L9 AR-1268-4	8.128	8.084	8896581	2326141	19.313	19.315
45)	L9 AR-1268-5	8.419	8.370	47344815	12534662	14.849	16.050


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090525\
Data File : PO113528.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2025 22:57
Operator : YP/AJ
Sample : Q2893-09
Misc : AR1268 WATER LOD 25PPB
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 23:37:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

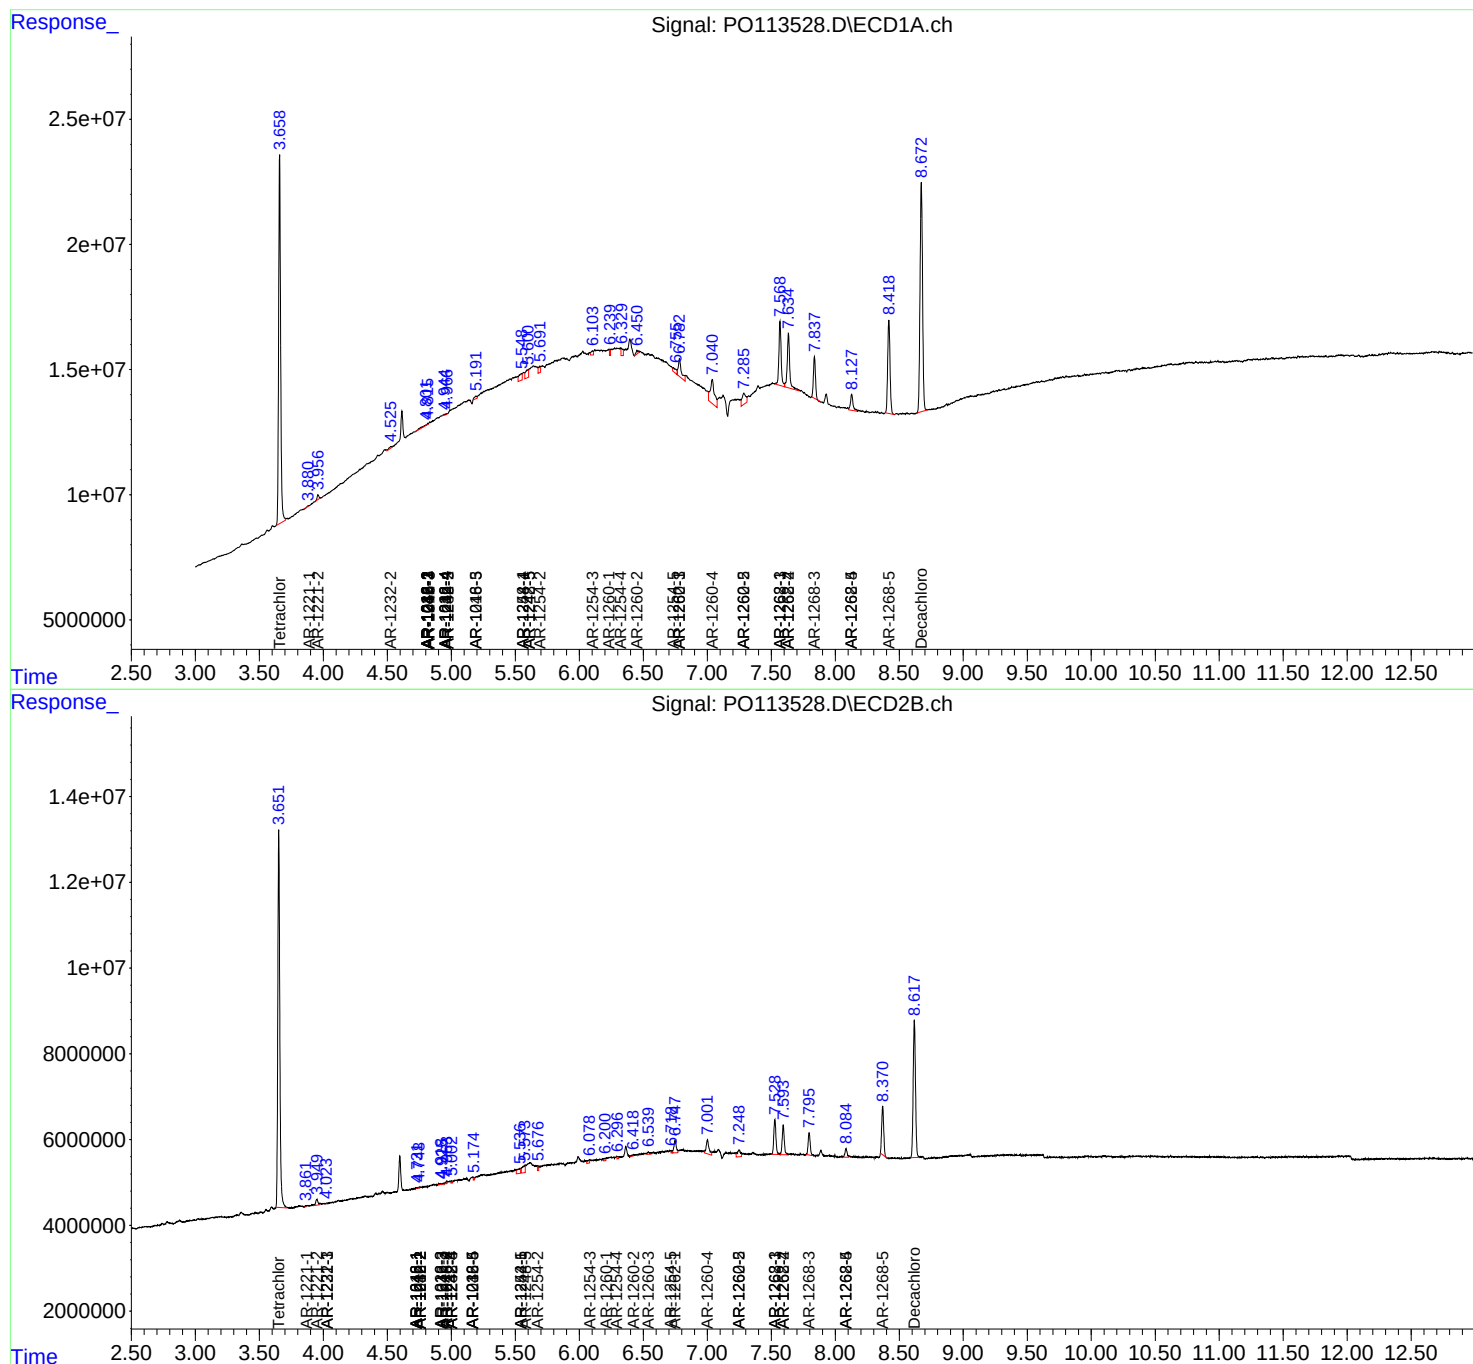


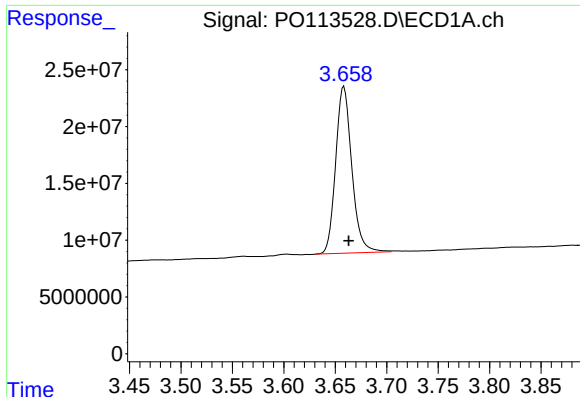

#1 Tetrachloro-m-xylene


R.T.: 3.658 min
Delta R.T.: -0.005 min
Response: 160717193
Conc: 19.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

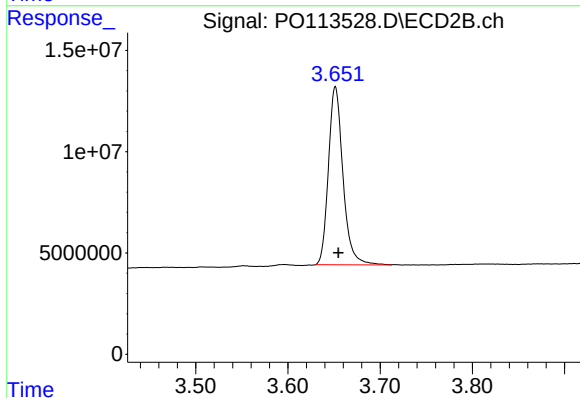


#1 Tetrachloro-m-xylene

R.T.: 3.652 min
Delta R.T.: -0.003 min
Response: 96397606
Conc: 19.05 ng/ml

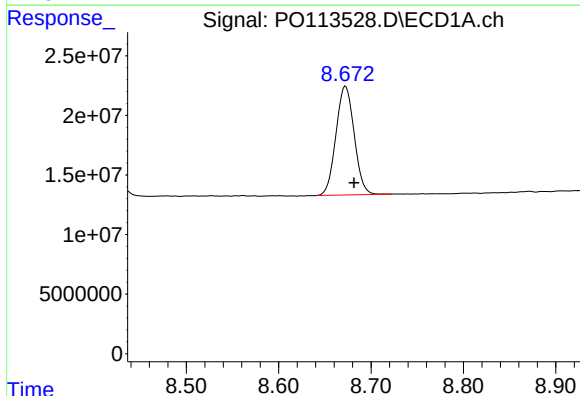


#2 Decachlorobiphenyl

R.T.: 8.672 min
Delta R.T.: -0.009 min
Response: 125487449
Conc: 18.10 ng/ml

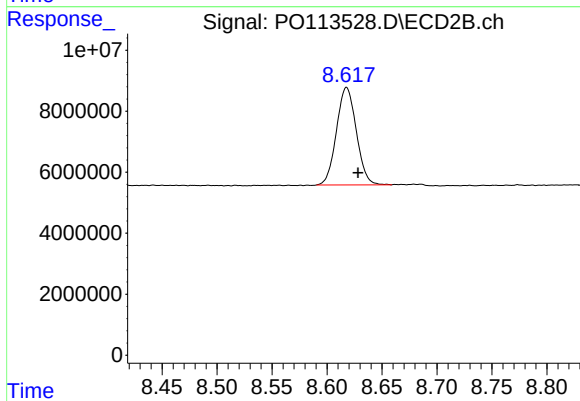

#2 Decachlorobiphenyl


R.T.: 8.618 min
Delta R.T.: -0.011 min
Response: 40243794
Conc: 21.24 ng/ml

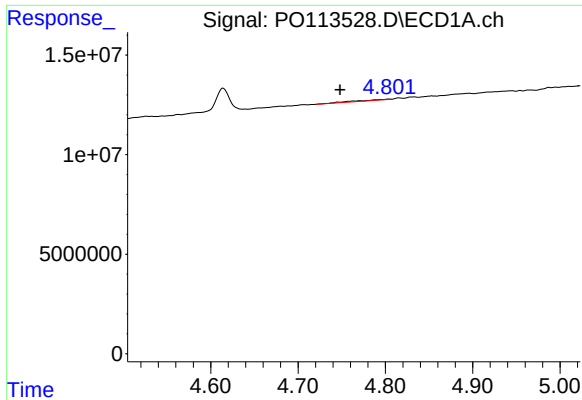

#3 AR-1016-1


R.T.: 4.804 min
Delta R.T.: 0.055 min
Response: 1139427
Conc: 4.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

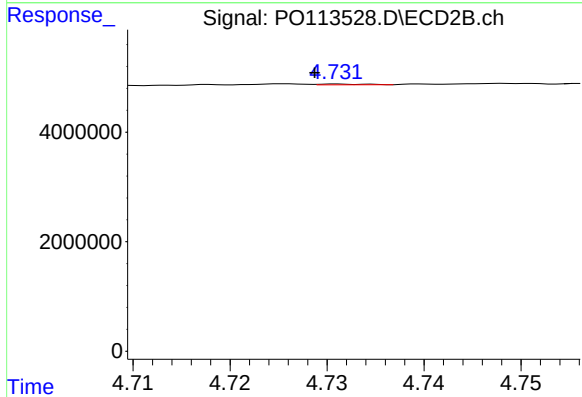


#3 AR-1016-1

R.T.: 4.731 min
Delta R.T.: 0.002 min
Response: 48510
Conc: 0.28 ng/ml

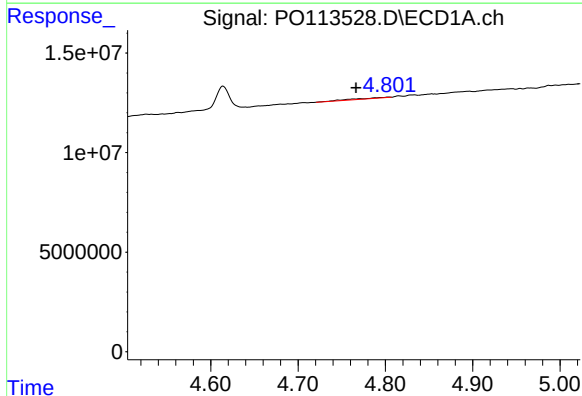


#4 AR-1016-2

R.T.: 4.804 min
Delta R.T.: 0.037 min
Response: 1139427
Conc: 2.84 ng/ml

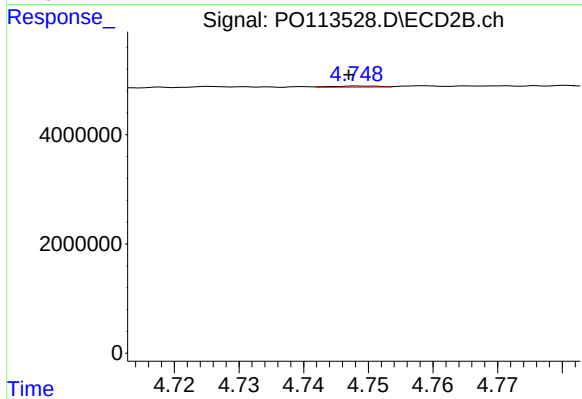

#4 AR-1016-2


R.T.: 4.748 min
Delta R.T.: 0.001 min
Response: 105738
Conc: 0.41 ng/ml

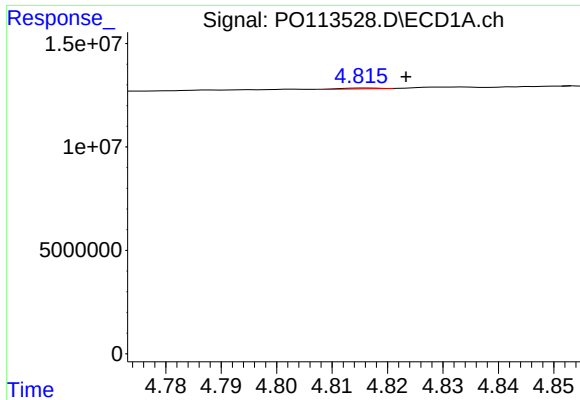

#5 AR-1016-3


R.T.: 4.816 min
Delta R.T.: -0.008 min
Response: 182425
Conc: 0.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

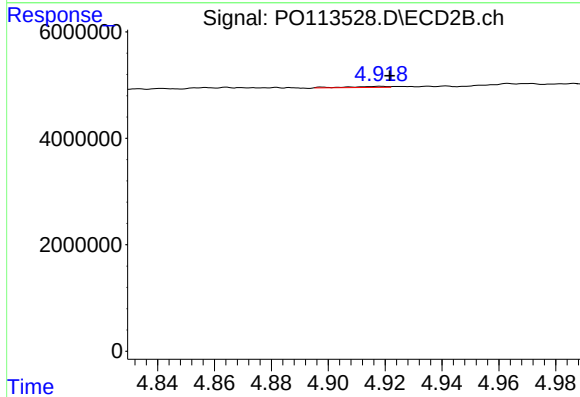


#5 AR-1016-3

R.T.: 4.918 min
Delta R.T.: -0.003 min
Response: 198741
Conc: 1.42 ng/ml

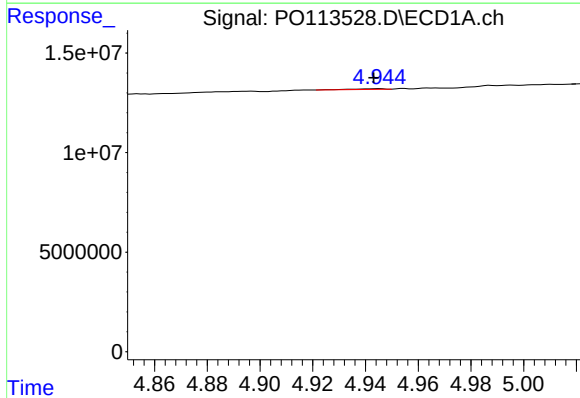


#6 AR-1016-4

R.T.: 4.945 min
Delta R.T.: 0.002 min
Response: 288115
Conc: 1.32 ng/ml

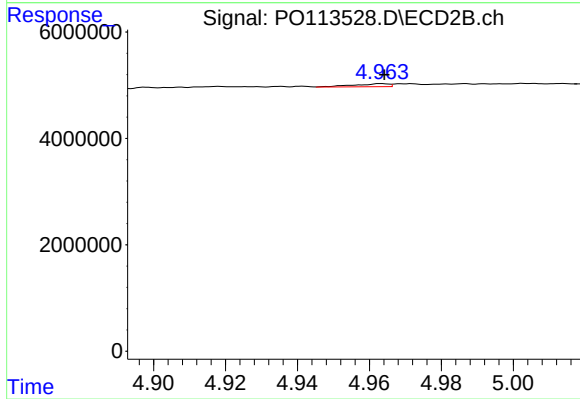

#6 AR-1016-4


R.T.: 4.963 min
Delta R.T.: 0.000 min
Response: 389337
Conc: 3.34 ng/ml

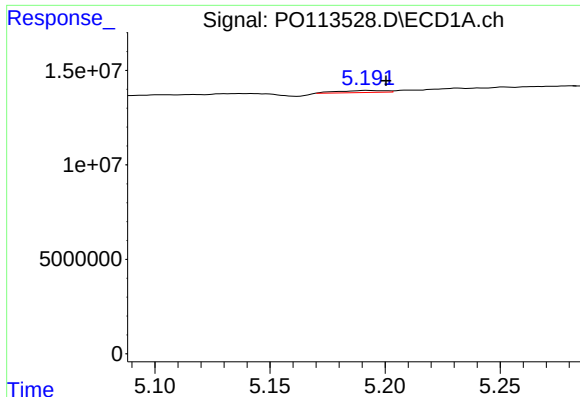

#7 AR-1016-5


R.T.: 5.193 min
Delta R.T.: -0.008 min
Response: 1569991
Conc: 7.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

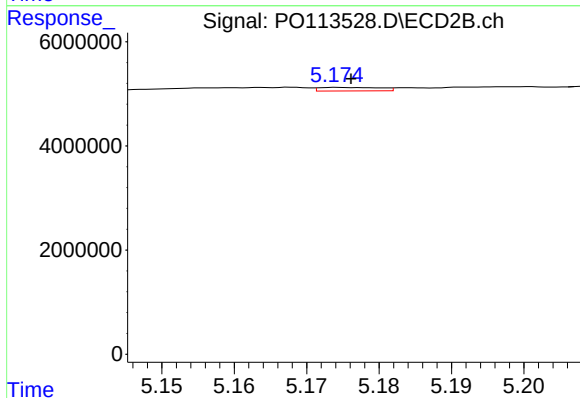


#7 AR-1016-5

R.T.: 5.174 min
Delta R.T.: -0.002 min
Response: 392324
Conc: 2.75 ng/ml

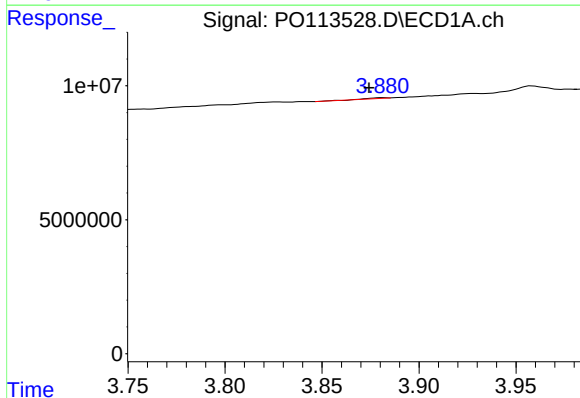


#8 AR-1221-1

R.T.: 3.881 min
Delta R.T.: 0.007 min
Response: 172480
Conc: 1.84 ng/ml

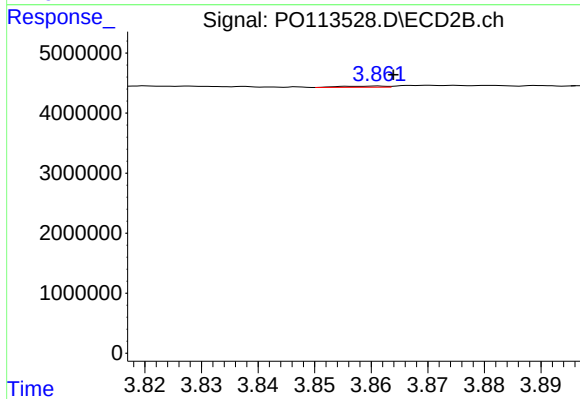

#8 AR-1221-1


R.T.: 3.861 min
Delta R.T.: -0.003 min
Response: 105468
Conc: 1.67 ng/ml

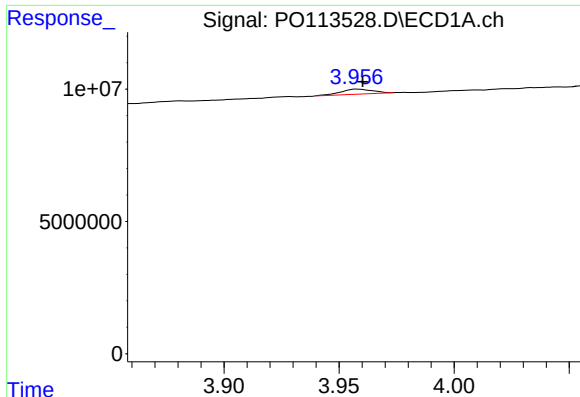

#9 AR-1221-2


R.T.: 3.958 min
Delta R.T.: -0.002 min
Response: 1803379
Conc: 26.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

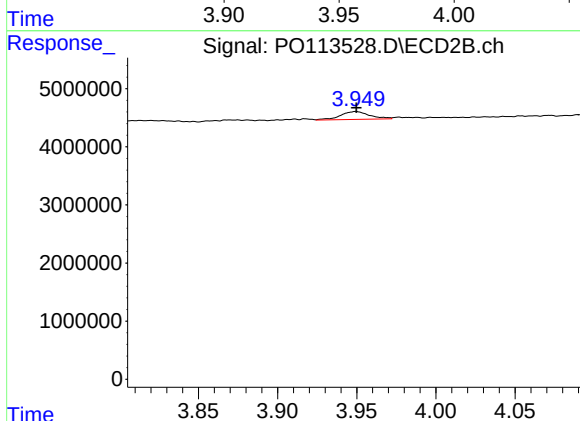


#9 AR-1221-2

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 1752270
Conc: 37.54 ng/ml

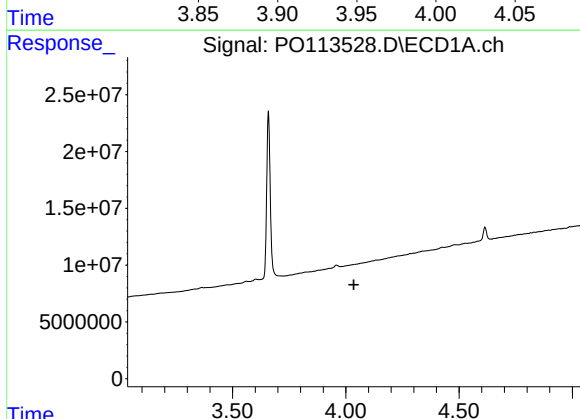


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.036 min
Response: 0
Conc: N.D.

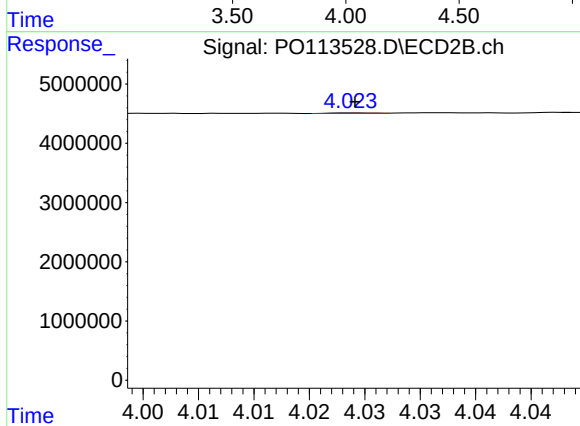

#10 AR-1221-3


R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 24533
Conc: 0.17 ng/ml

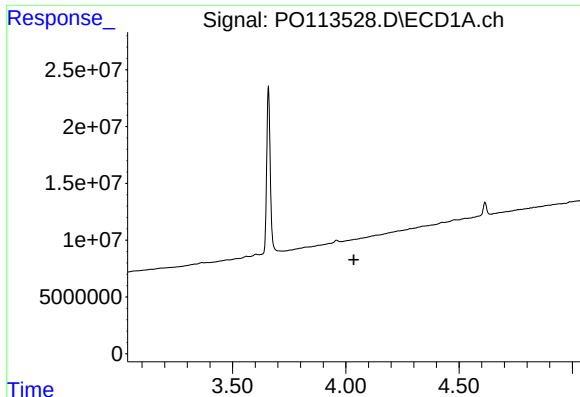

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 4.036 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

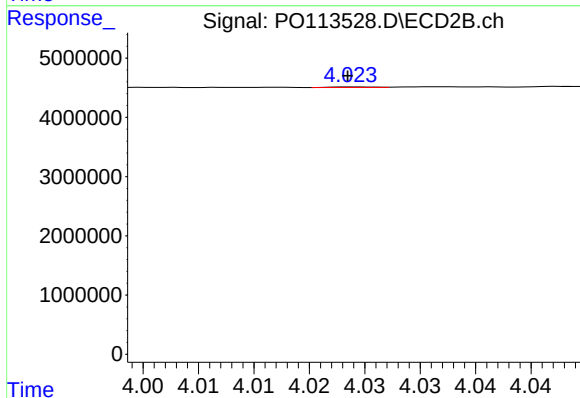


#11 AR-1232-1

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 24533
Conc: 0.21 ng/ml

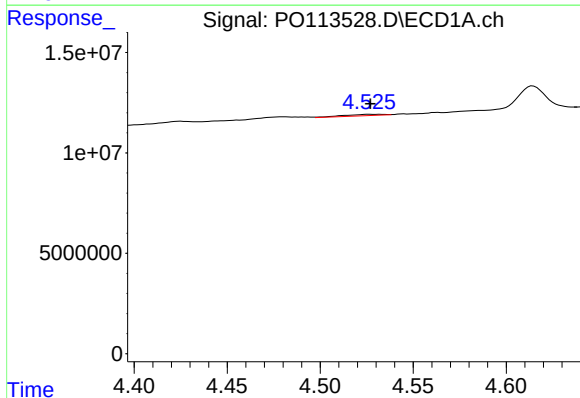


#12 AR-1232-2

R.T.: 4.527 min
Delta R.T.: 0.000 min
Response: 1008896
Conc: 10.10 ng/ml

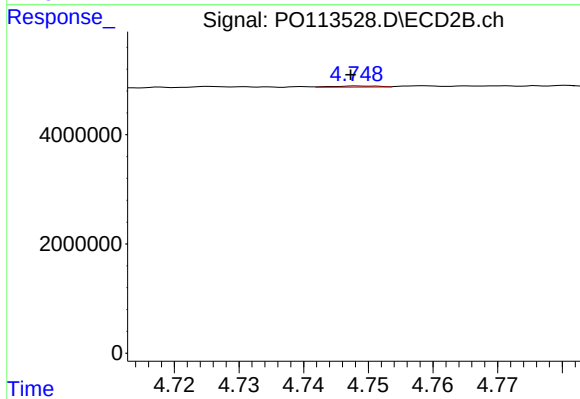

#12 AR-1232-2


R.T.: 4.748 min
Delta R.T.: 0.001 min
Response: 105738
Conc: 0.86 ng/ml

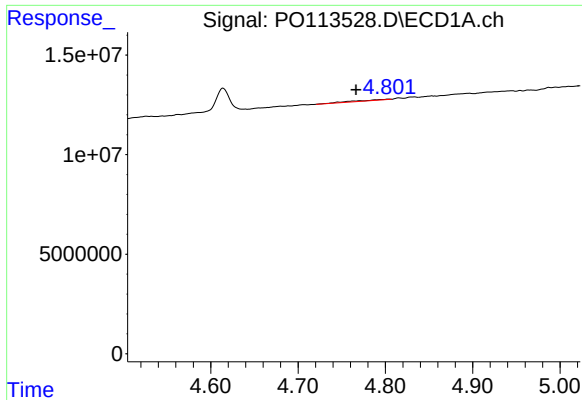

#13 AR-1232-3


R.T.: 4.804 min
Delta R.T.: 0.037 min
Response: 1139427
Conc: 6.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

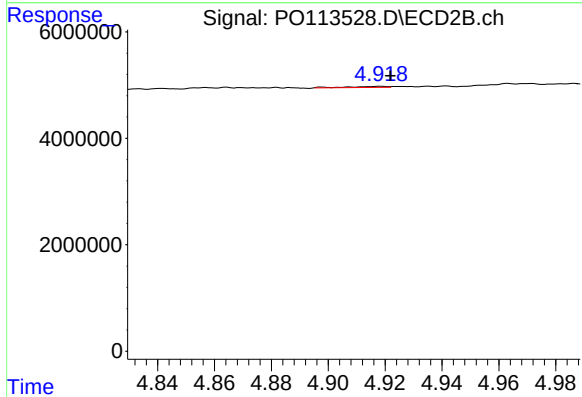


#13 AR-1232-3

R.T.: 4.918 min
Delta R.T.: -0.004 min
Response: 198741
Conc: 3.14 ng/ml

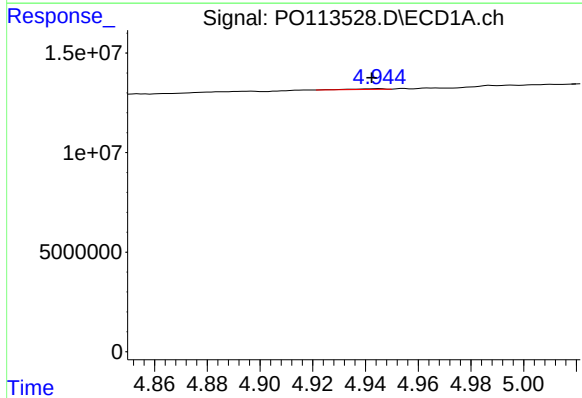


#14 AR-1232-4

R.T.: 4.945 min
Delta R.T.: 0.003 min
Response: 288115
Conc: 3.06 ng/ml

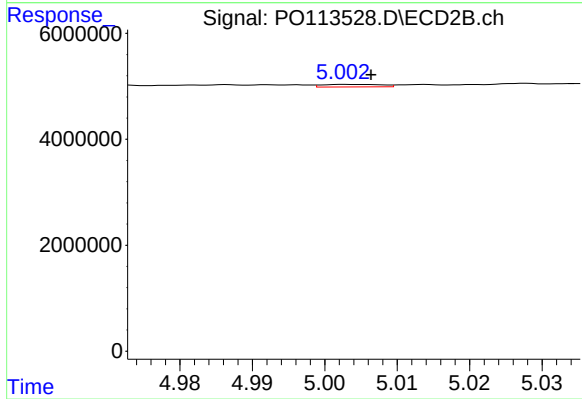

#14 AR-1232-4


R.T.: 5.003 min
Delta R.T.: -0.004 min
Response: 271046
Conc: 4.82 ng/ml

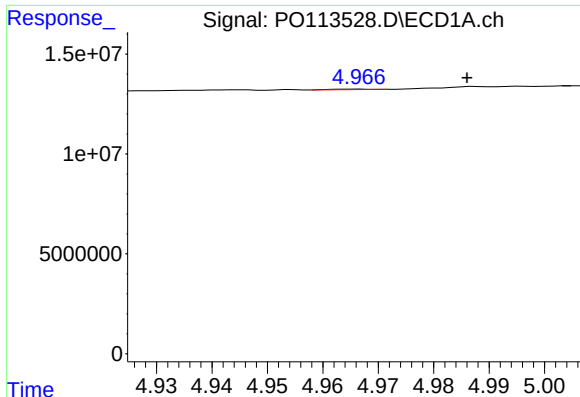

#15 AR-1232-5


R.T.: 4.966 min
Delta R.T.: -0.020 min
Response: 125703
Conc: 2.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

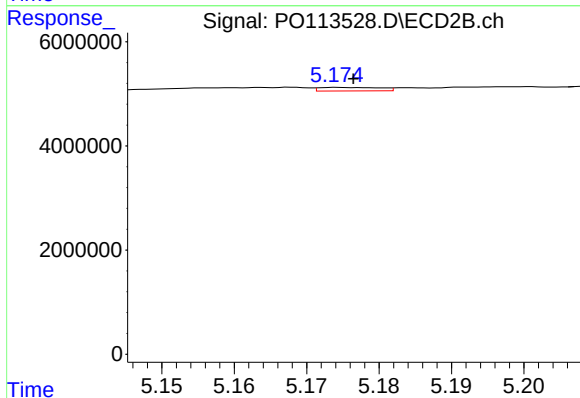


#15 AR-1232-5

R.T.: 5.174 min
Delta R.T.: -0.002 min
Response: 392324
Conc: 6.55 ng/ml

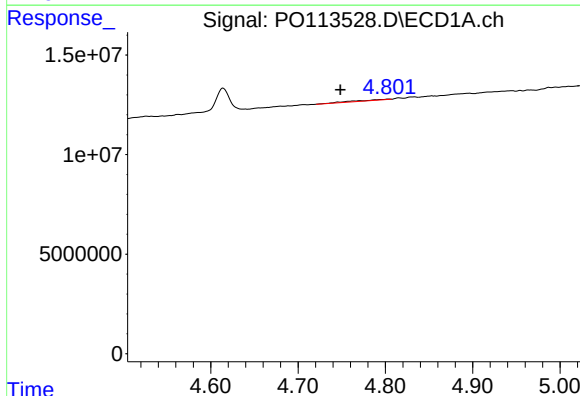


#16 AR-1242-1

R.T.: 4.804 min
Delta R.T.: 0.055 min
Response: 1139427
Conc: 4.96 ng/ml

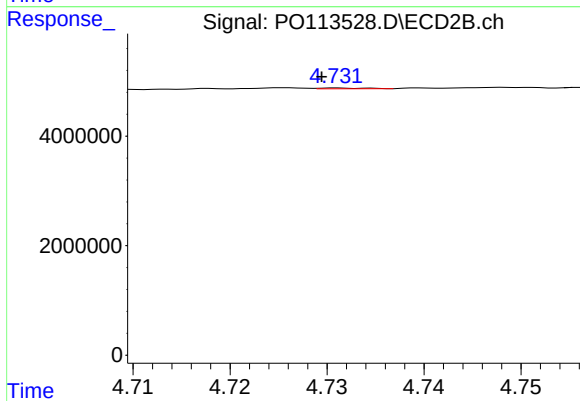

#16 AR-1242-1


R.T.: 4.731 min
Delta R.T.: 0.002 min
Response: 48510
Conc: 0.34 ng/ml

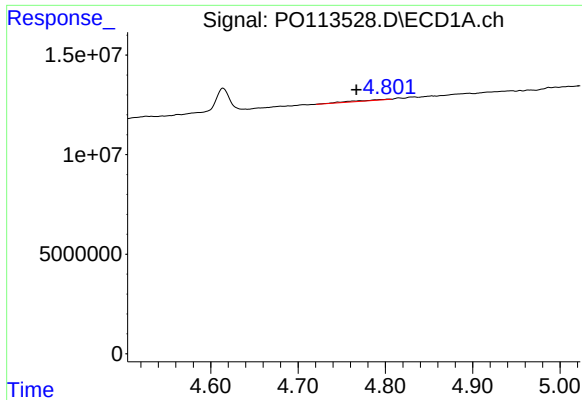

#17 AR-1242-2


R.T.: 4.804 min
Delta R.T.: 0.037 min
Response: 1139427
Conc: 3.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

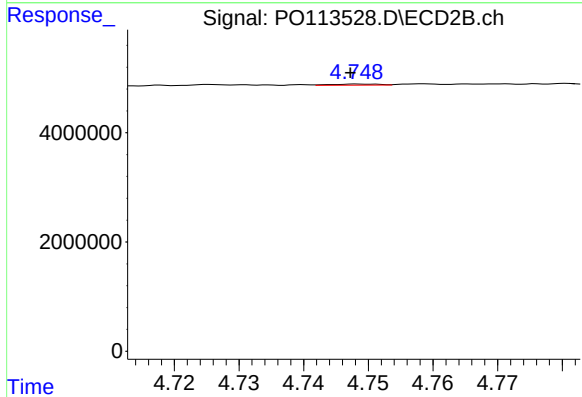


#17 AR-1242-2

R.T.: 4.748 min
Delta R.T.: 0.001 min
Response: 105738
Conc: 0.49 ng/ml

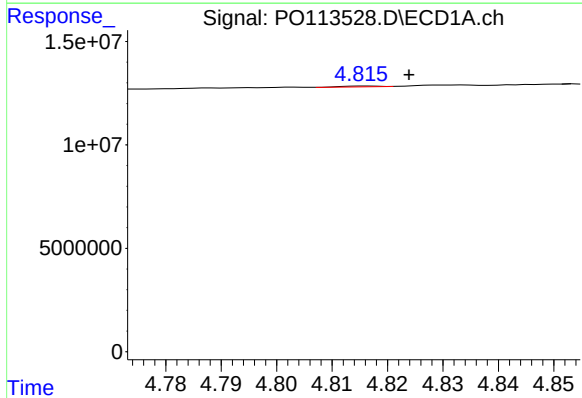


#18 AR-1242-3

R.T.: 4.816 min
Delta R.T.: -0.008 min
Response: 182425
Conc: 0.82 ng/ml

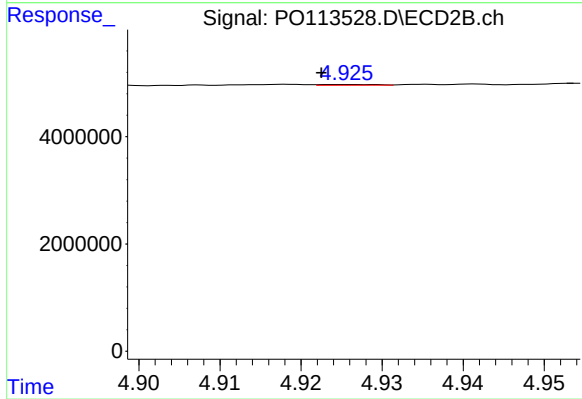

#18 AR-1242-3


R.T.: 4.926 min
Delta R.T.: 0.003 min
Response: 73407
Conc: 0.63 ng/ml

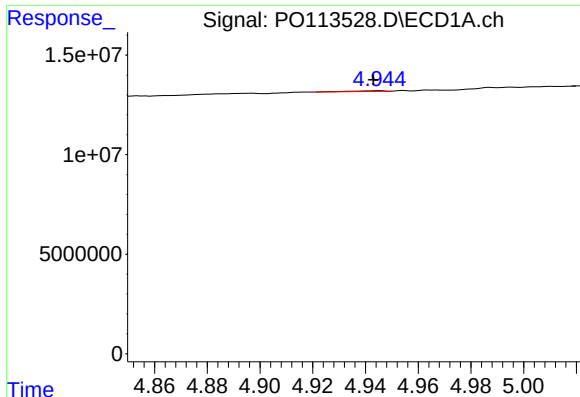

#19 AR-1242-4


R.T.: 4.945 min
Delta R.T.: 0.002 min
Response: 288115
Conc: 1.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

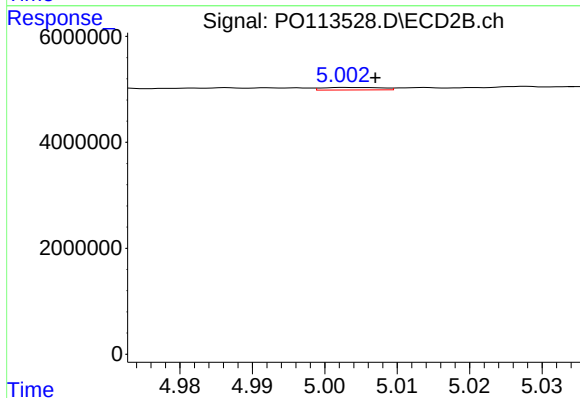


#19 AR-1242-4

R.T.: 5.003 min
Delta R.T.: -0.004 min
Response: 271046
Conc: 2.30 ng/ml

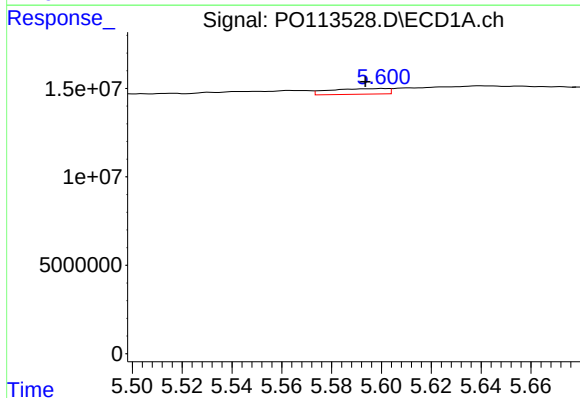


#20 AR-1242-5

R.T.: 5.601 min
Delta R.T.: 0.007 min
Response: 5200484
Conc: 25.98 ng/ml

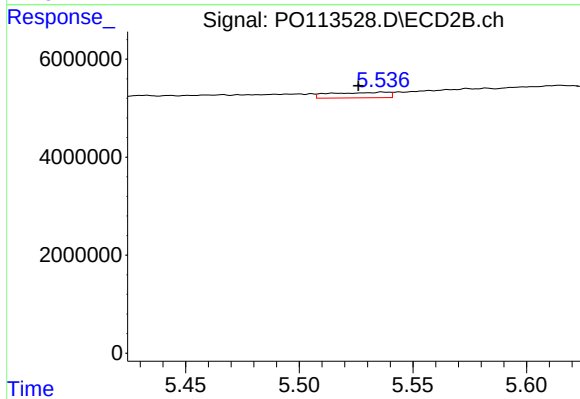

#20 AR-1242-5


R.T.: 5.536 min
Delta R.T.: 0.010 min
Response: 2000121
Conc: 13.41 ng/ml

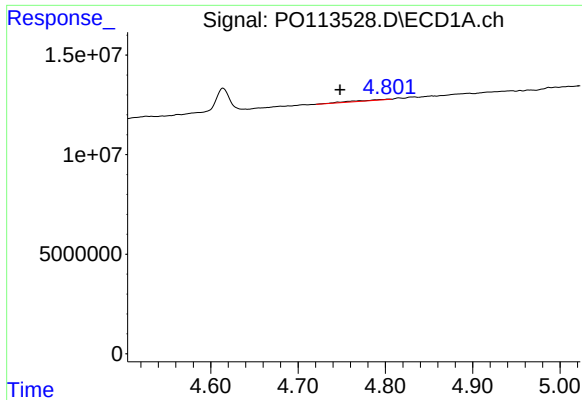

#21 AR-1248-1


R.T.: 4.804 min
Delta R.T.: 0.056 min
Response: 1139427
Conc: 6.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

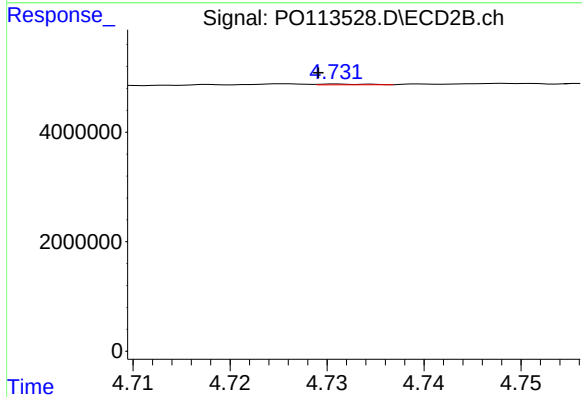


#21 AR-1248-1

R.T.: 4.731 min
Delta R.T.: 0.002 min
Response: 48510
Conc: 0.44 ng/ml

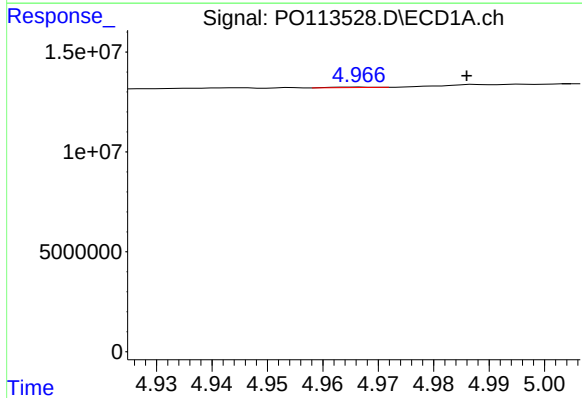


#22 AR-1248-2

R.T.: 4.966 min
Delta R.T.: -0.020 min
Response: 125703
Conc: 0.52 ng/ml

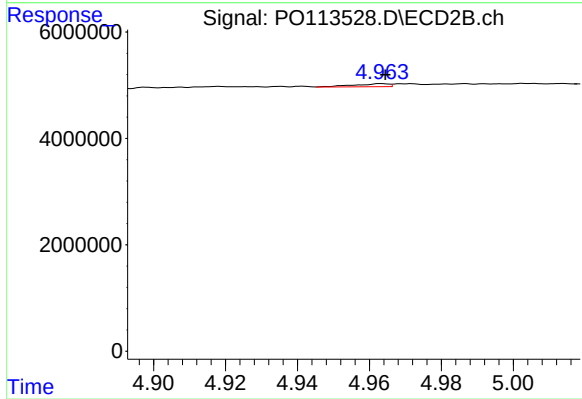

#22 AR-1248-2


R.T.: 4.963 min
Delta R.T.: -0.001 min
Response: 389337
Conc: 2.42 ng/ml

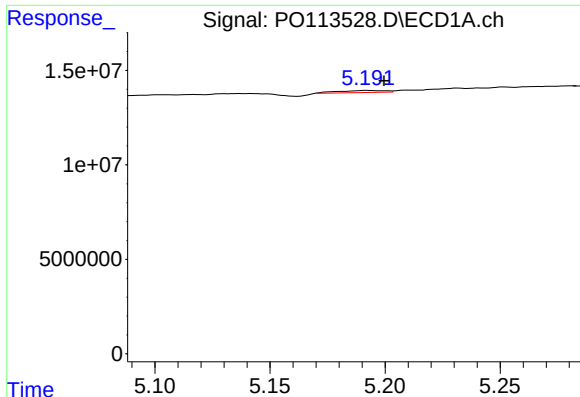

#23 AR-1248-3


R.T.: 5.193 min
Delta R.T.: -0.007 min
Response: 1569991
Conc: 4.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

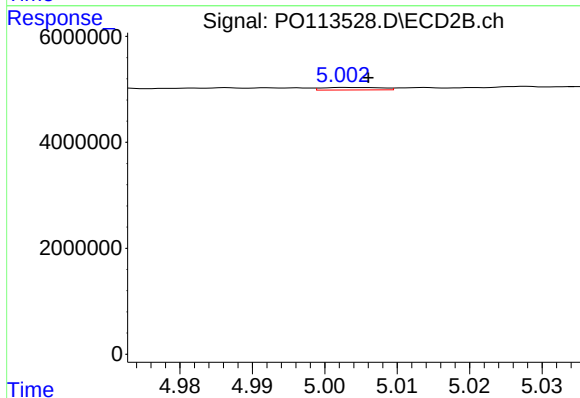


#23 AR-1248-3

R.T.: 5.003 min
Delta R.T.: -0.003 min
Response: 271046
Conc: 1.60 ng/ml

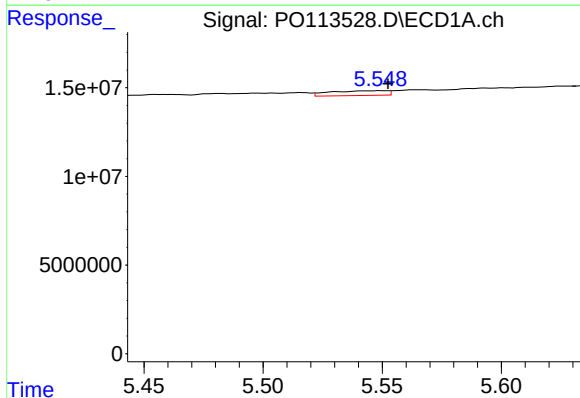


#24 AR-1248-4

R.T.: 5.550 min
Delta R.T.: -0.003 min
Response: 4486476
Conc: 8.98 ng/ml

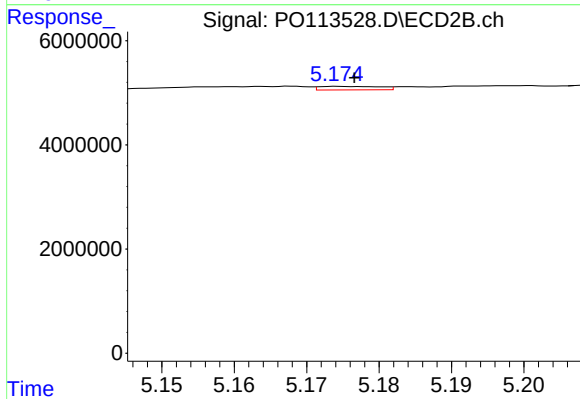

#24 AR-1248-4


R.T.: 5.174 min
Delta R.T.: -0.002 min
Response: 392324
Conc: 1.97 ng/ml

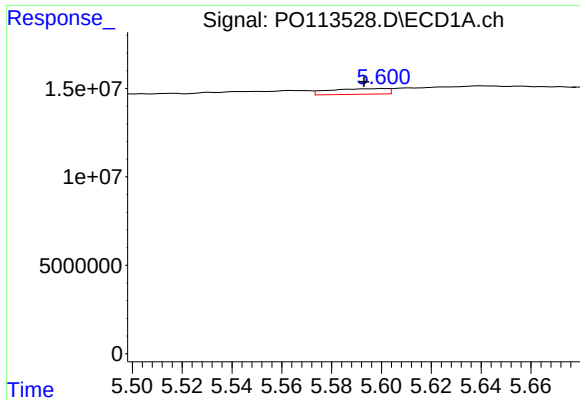

#25 AR-1248-5


R.T.: 5.601 min
Delta R.T.: 0.008 min
Response: 5200484
Conc: 15.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

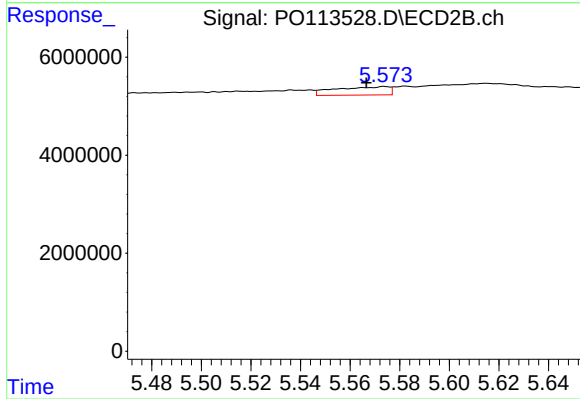


#25 AR-1248-5

R.T.: 5.574 min
Delta R.T.: 0.007 min
Response: 2558599
Conc: 12.05 ng/ml

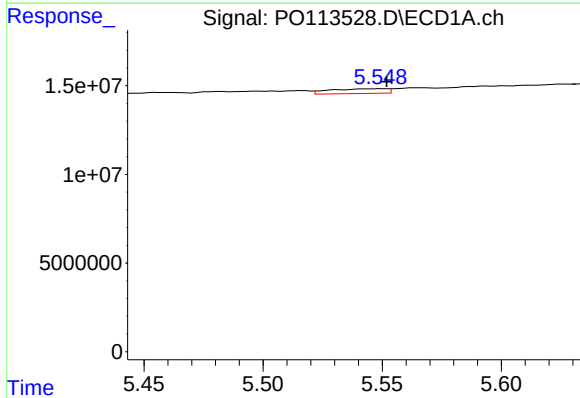


#26 AR-1254-1

R.T.: 5.550 min
Delta R.T.: -0.002 min
Response: 4486476
Conc: 8.31 ng/ml

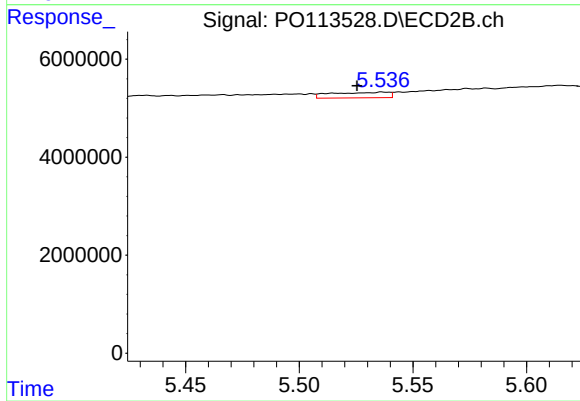

#26 AR-1254-1


R.T.: 5.536 min
Delta R.T.: 0.011 min
Response: 2000121
Conc: 6.34 ng/ml

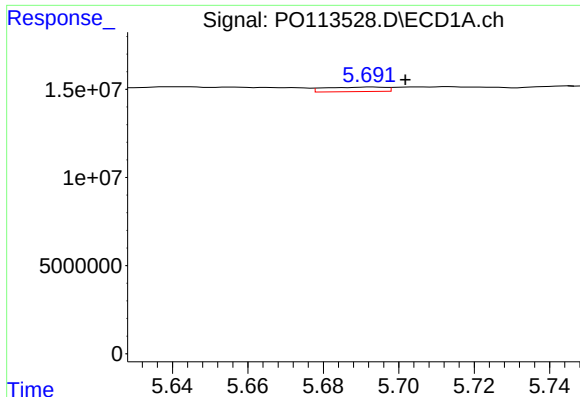

#27 AR-1254-2


R.T.: 5.693 min
Delta R.T.: -0.009 min
Response: 2849426
Conc: 5.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

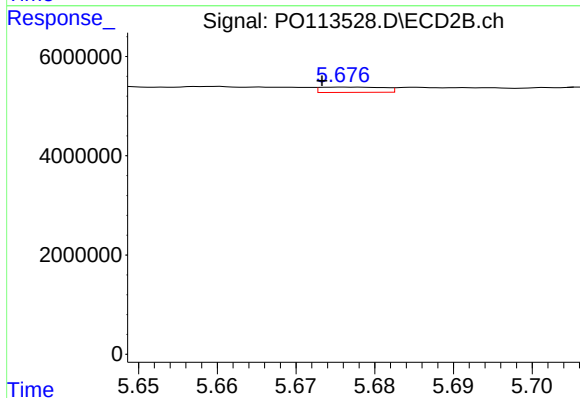


#27 AR-1254-2

R.T.: 5.676 min
Delta R.T.: 0.003 min
Response: 599265
Conc: 2.14 ng/ml

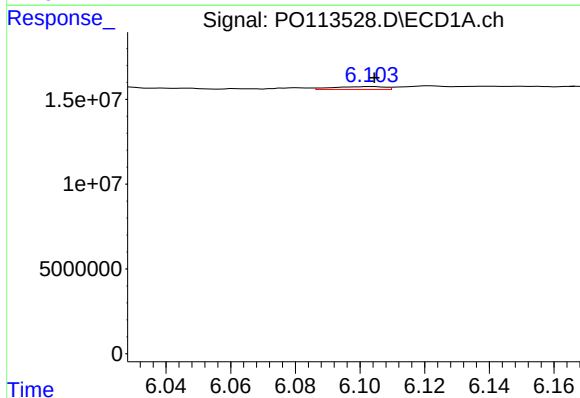


#28 AR-1254-3

R.T.: 6.104 min
Delta R.T.: 0.000 min
Response: 1910147
Conc: 2.59 ng/ml

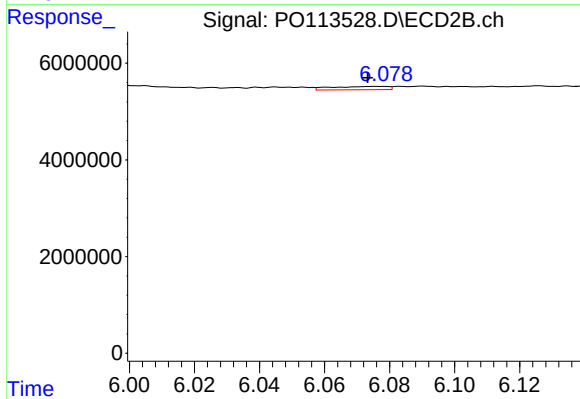

#28 AR-1254-3


R.T.: 6.078 min
Delta R.T.: 0.005 min
Response: 837080
Conc: 2.01 ng/ml

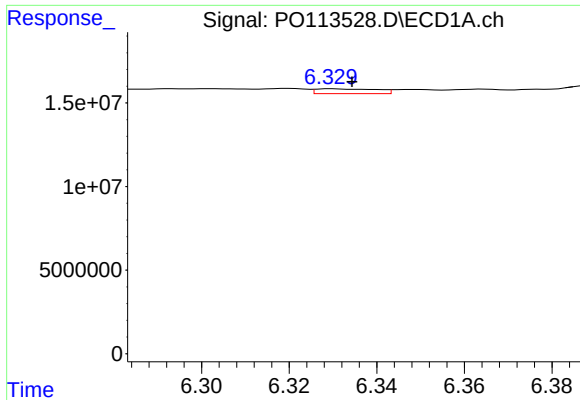

#29 AR-1254-4


R.T.: 6.330 min
Delta R.T.: -0.005 min
Response: 2801774
Conc: 5.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

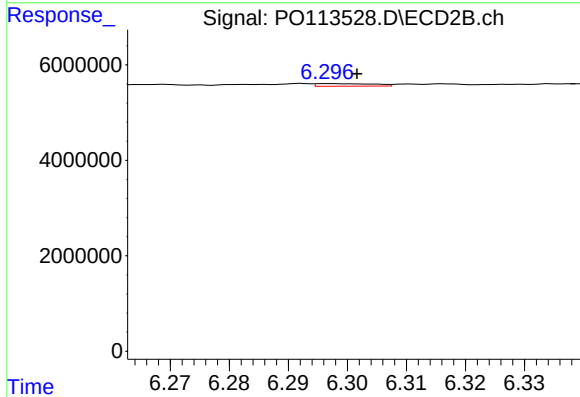


#29 AR-1254-4

R.T.: 6.297 min
Delta R.T.: -0.005 min
Response: 373577
Conc: 1.36 ng/ml

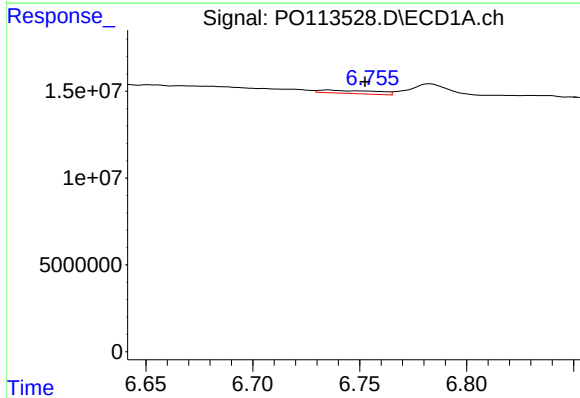


#30 AR-1254-5

R.T.: 6.735 min
Delta R.T.: -0.017 min
Response: 3346516
Conc: 4.77 ng/ml

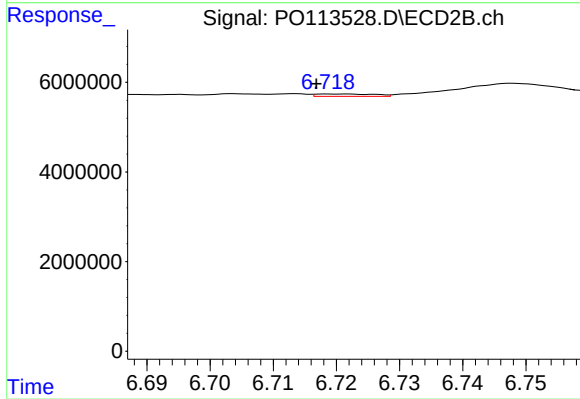

#30 AR-1254-5


R.T.: 6.719 min
Delta R.T.: 0.002 min
Response: 339433
Conc: 0.95 ng/ml

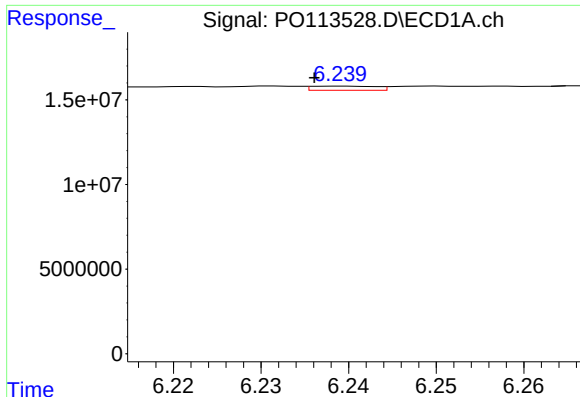

#31 AR-1260-1


R.T.: 6.239 min
Delta R.T.: 0.003 min
Response: 1249133
Conc: 2.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

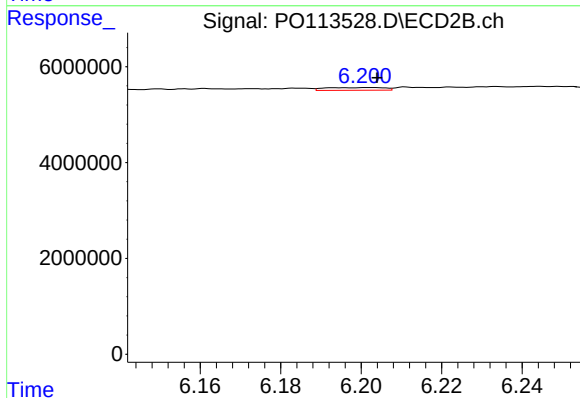


#31 AR-1260-1

R.T.: 6.201 min
Delta R.T.: -0.003 min
Response: 577301
Conc: 2.26 ng/ml

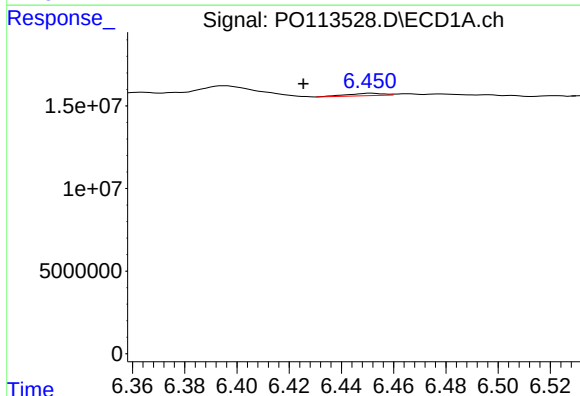


#32 AR-1260-2

R.T.: 6.451 min
Delta R.T.: 0.026 min
Response: 1333341
Conc: 1.94 ng/ml

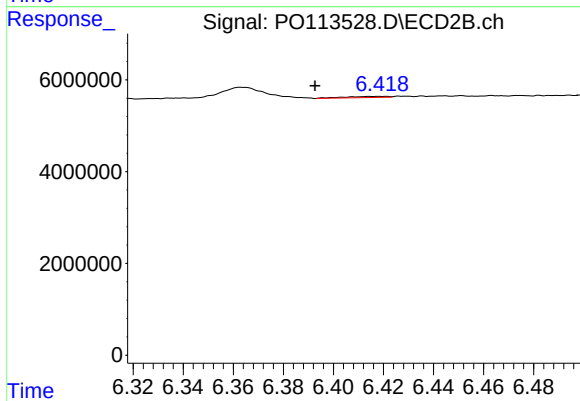

#32 AR-1260-2


R.T.: 6.418 min
Delta R.T.: 0.026 min
Response: 311337
Conc: 0.90 ng/ml

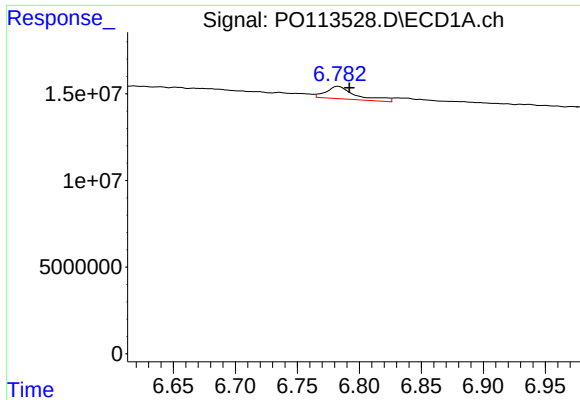

#33 AR-1260-3


R.T.: 6.783 min
Delta R.T.: -0.009 min
Response: 11961356
Conc: 19.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

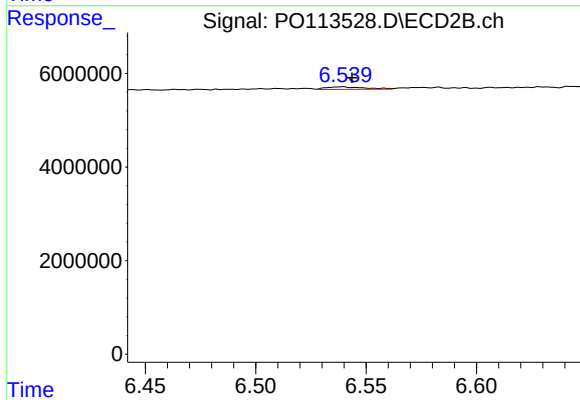


#33 AR-1260-3

R.T.: 6.540 min
Delta R.T.: -0.004 min
Response: 680626
Conc: 2.29 ng/ml

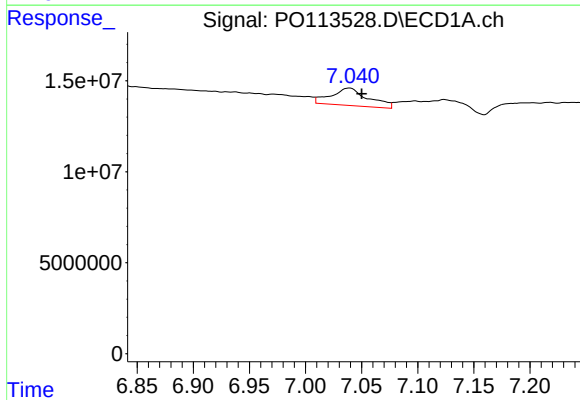


#34 AR-1260-4

R.T.: 7.039 min
Delta R.T.: -0.011 min
Response: 22033898
Conc: 49.20 ng/ml

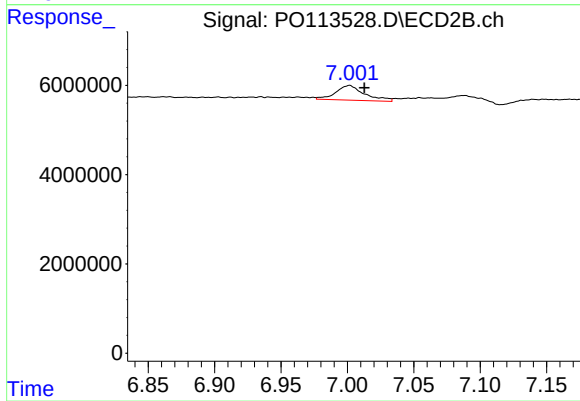

#34 AR-1260-4


R.T.: 7.002 min
Delta R.T.: -0.011 min
Response: 4994436
Conc: 24.10 ng/ml

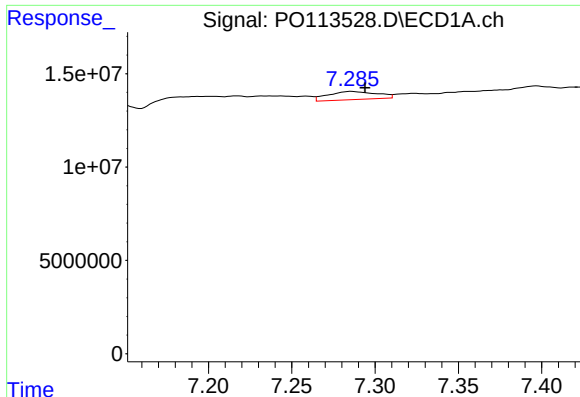

#35 AR-1260-5


R.T.: 7.286 min
Delta R.T.: -0.008 min
Response: 8797647
Conc: 7.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

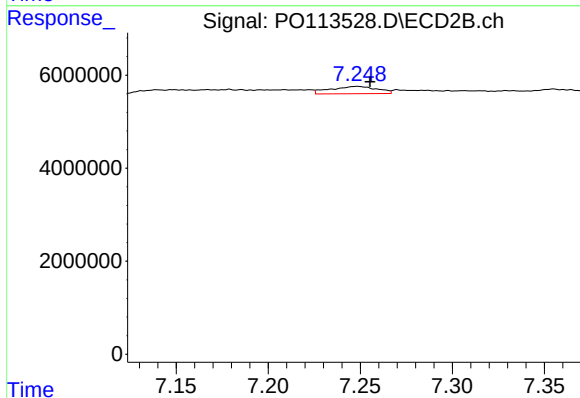


#35 AR-1260-5

R.T.: 7.248 min
Delta R.T.: -0.007 min
Response: 2796433
Conc: 5.97 ng/ml

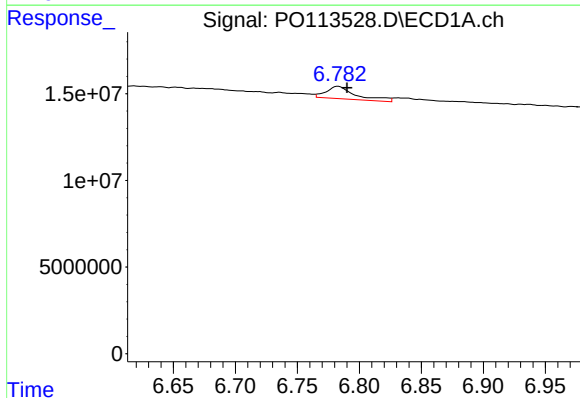


#36 AR-1262-1

R.T.: 6.783 min
Delta R.T.: -0.007 min
Response: 11961356
Conc: 13.06 ng/ml

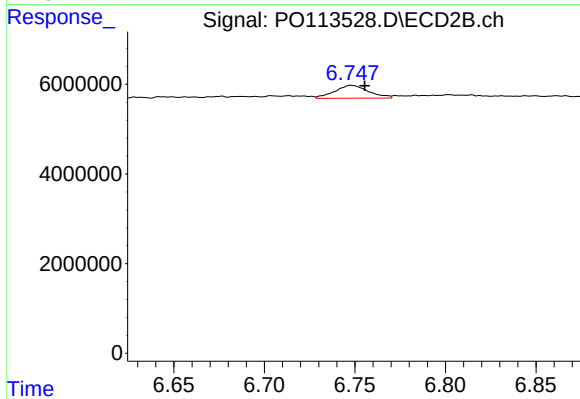

#36 AR-1262-1


R.T.: 6.748 min
Delta R.T.: -0.007 min
Response: 3698933
Conc: 8.92 ng/ml

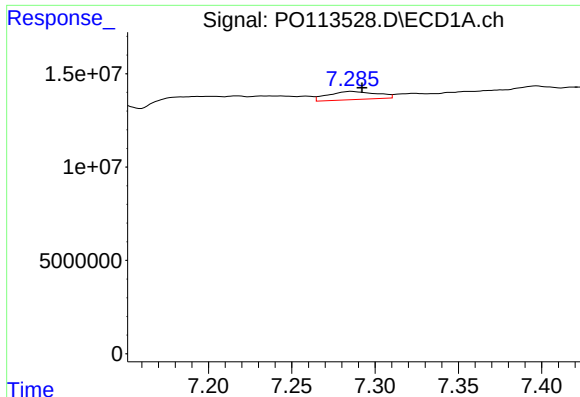

#37 AR-1262-2


R.T.: 7.286 min
Delta R.T.: -0.007 min
Response: 8797647
Conc: 5.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

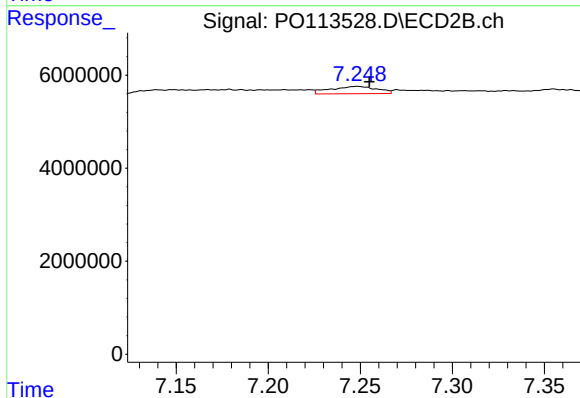


#37 AR-1262-2

R.T.: 7.248 min
Delta R.T.: -0.007 min
Response: 2796433
Conc: 5.40 ng/ml

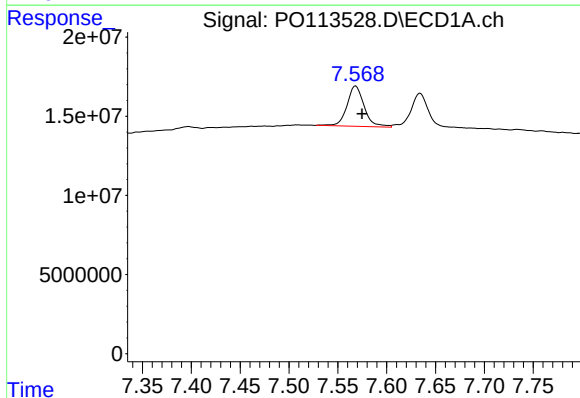


#38 AR-1262-3

R.T.: 7.568 min
Delta R.T.: -0.006 min
Response: 31194025
Conc: 56.30 ng/ml

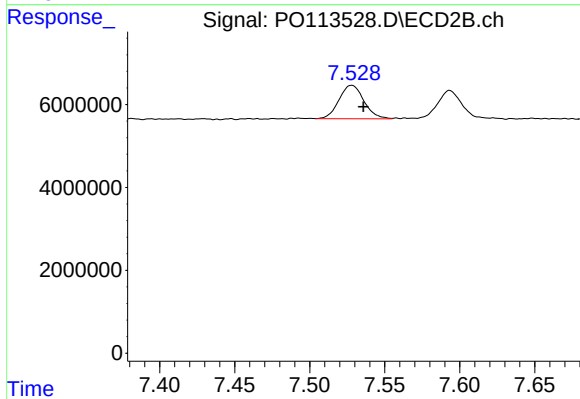

#38 AR-1262-3


R.T.: 7.528 min
Delta R.T.: -0.008 min
Response: 9363122
Conc: 52.14 ng/ml

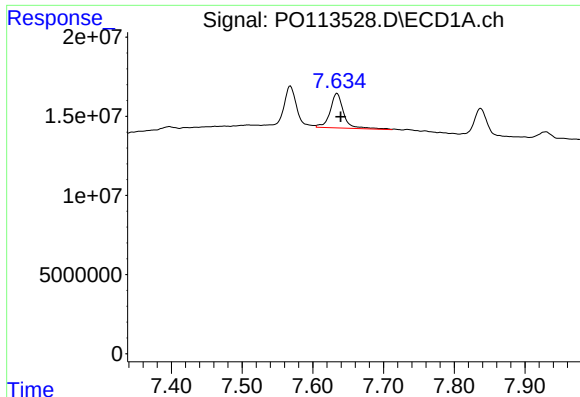

#39 AR-1262-4


R.T.: 7.634 min
Delta R.T.: -0.005 min
Response: 29109781
Conc: 29.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

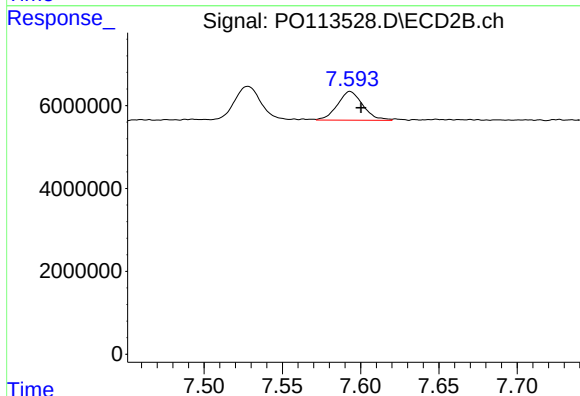


#39 AR-1262-4

R.T.: 7.593 min
Delta R.T.: -0.007 min
Response: 7807688
Conc: 26.93 ng/ml

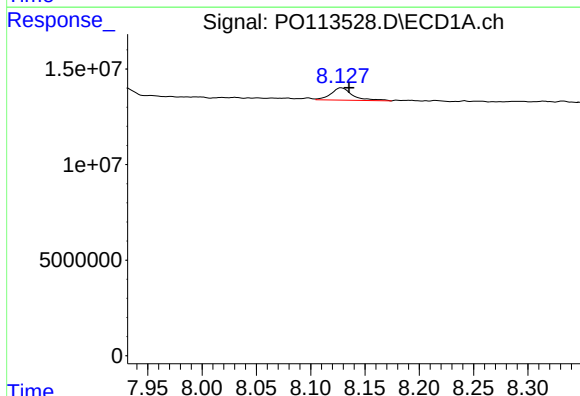


#40 AR-1262-5

R.T.: 8.128 min
Delta R.T.: -0.007 min
Response: 8896581
Conc: 21.34 ng/ml

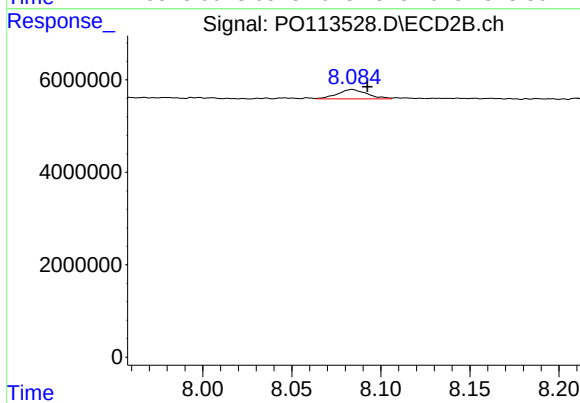

#40 AR-1262-5


R.T.: 8.084 min
Delta R.T.: -0.008 min
Response: 2326141
Conc: 21.47 ng/ml

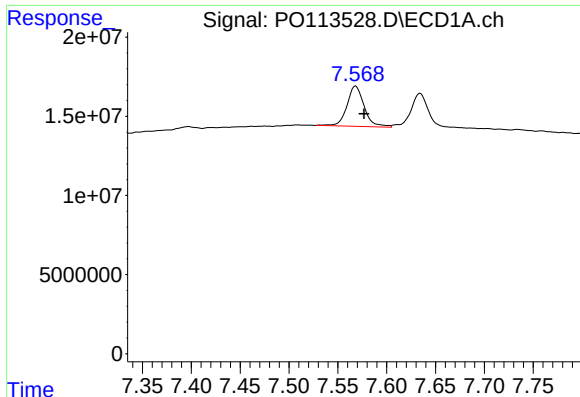

#41 AR-1268-1


R.T.: 7.568 min
Delta R.T.: -0.009 min
Response: 31194025
Conc: 18.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

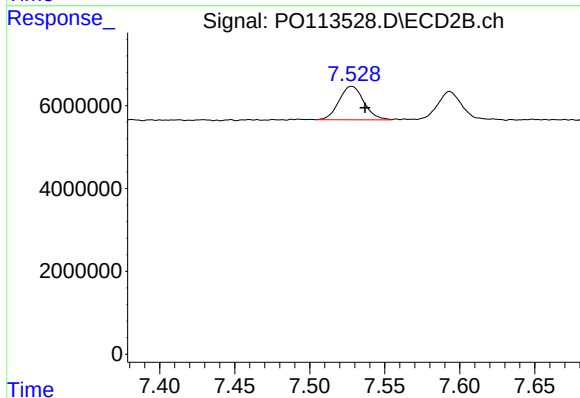


#41 AR-1268-1

R.T.: 7.528 min
Delta R.T.: -0.009 min
Response: 9363122
Conc: 18.38 ng/ml

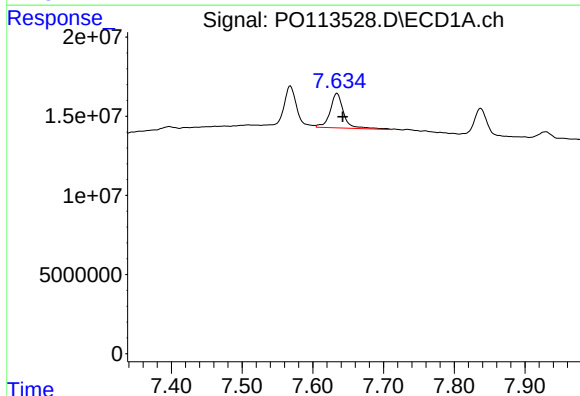


#42 AR-1268-2

R.T.: 7.634 min
Delta R.T.: -0.008 min
Response: 29109781
Conc: 20.10 ng/ml

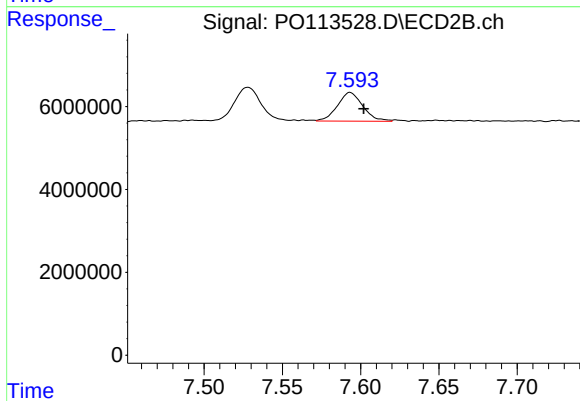

#42 AR-1268-2


R.T.: 7.593 min
Delta R.T.: -0.009 min
Response: 7807688
Conc: 18.80 ng/ml

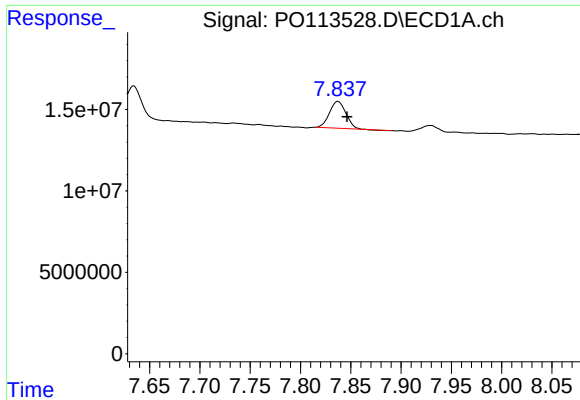

#43 AR-1268-3


R.T.: 7.837 min
Delta R.T.: -0.009 min
Response: 18441931
Conc: 15.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

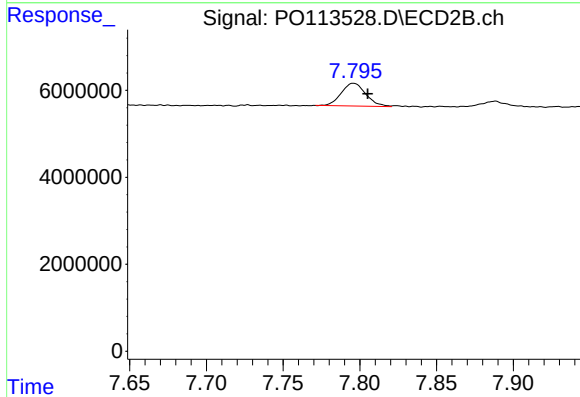


#43 AR-1268-3

R.T.: 7.796 min
Delta R.T.: -0.009 min
Response: 5852090
Conc: 17.92 ng/ml

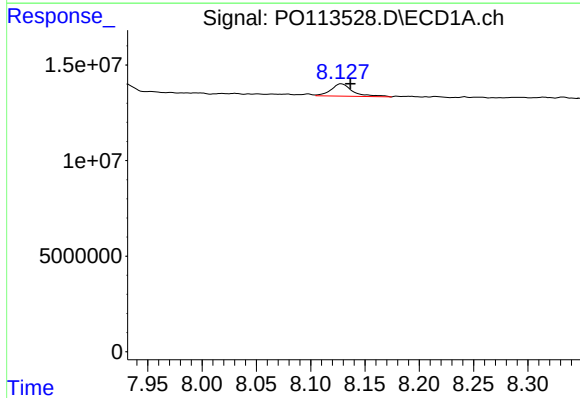


#44 AR-1268-4

R.T.: 8.128 min
Delta R.T.: -0.009 min
Response: 8896581
Conc: 19.31 ng/ml

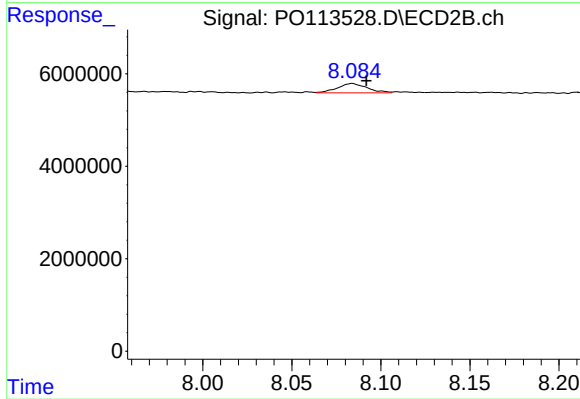

#44 AR-1268-4


R.T.: 8.084 min
Delta R.T.: -0.008 min
Response: 2326141
Conc: 19.31 ng/ml

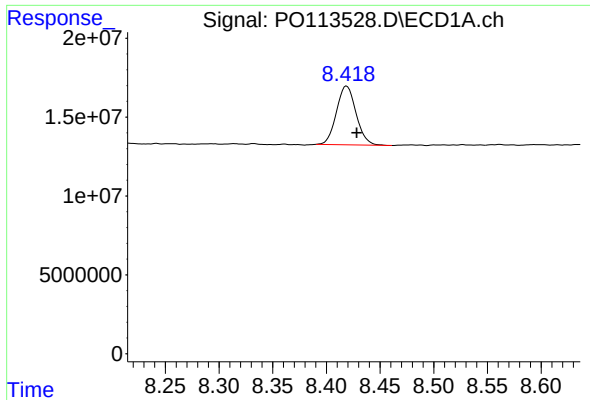

#45 AR-1268-5

R.T.: 8.419 min
Delta R.T.: -0.009 min
Response: 47344815
Conc: 14.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2025

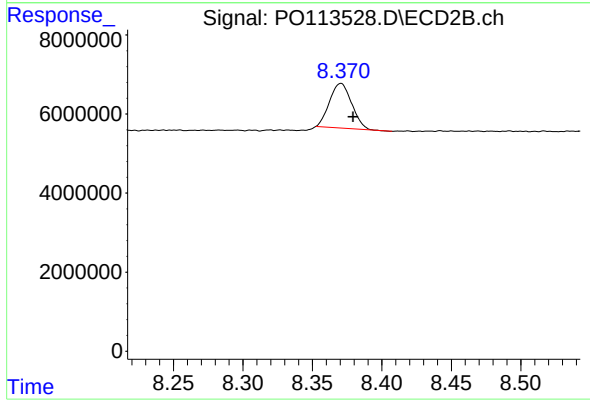

#45 AR-1268-5

R.T.: 8.370 min
Delta R.T.: -0.009 min
Response: 12534662
Conc: 16.05 ng/ml