

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090525\
 Data File : P0113513.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 17:08
 Operator : YP/AJ
 Sample : Q3026-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EO-02-09042025

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/08/2025
 Supervised By :mohammad ahmed 09/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:33:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.658	3.652	151.4E6	87876972	18.499m	17.365
2) SA Decachlor...	8.675	8.621	92336434	28915493	13.321	15.260

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090525\
Data File : PO113513.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2025 17:08
Operator : YP/AJ
Sample : Q3026-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
EO-02-09042025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/08/2025
Supervised By :mohammad ahmed 09/09/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 23:33:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

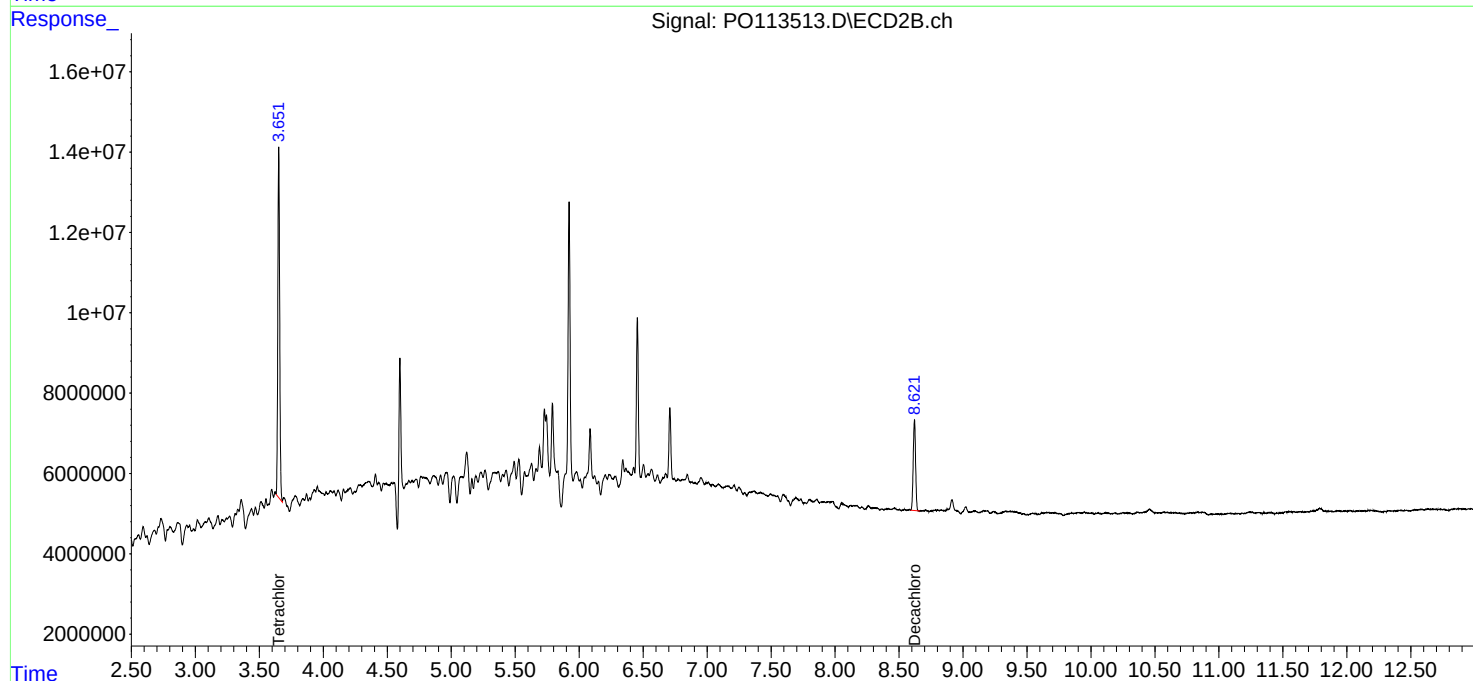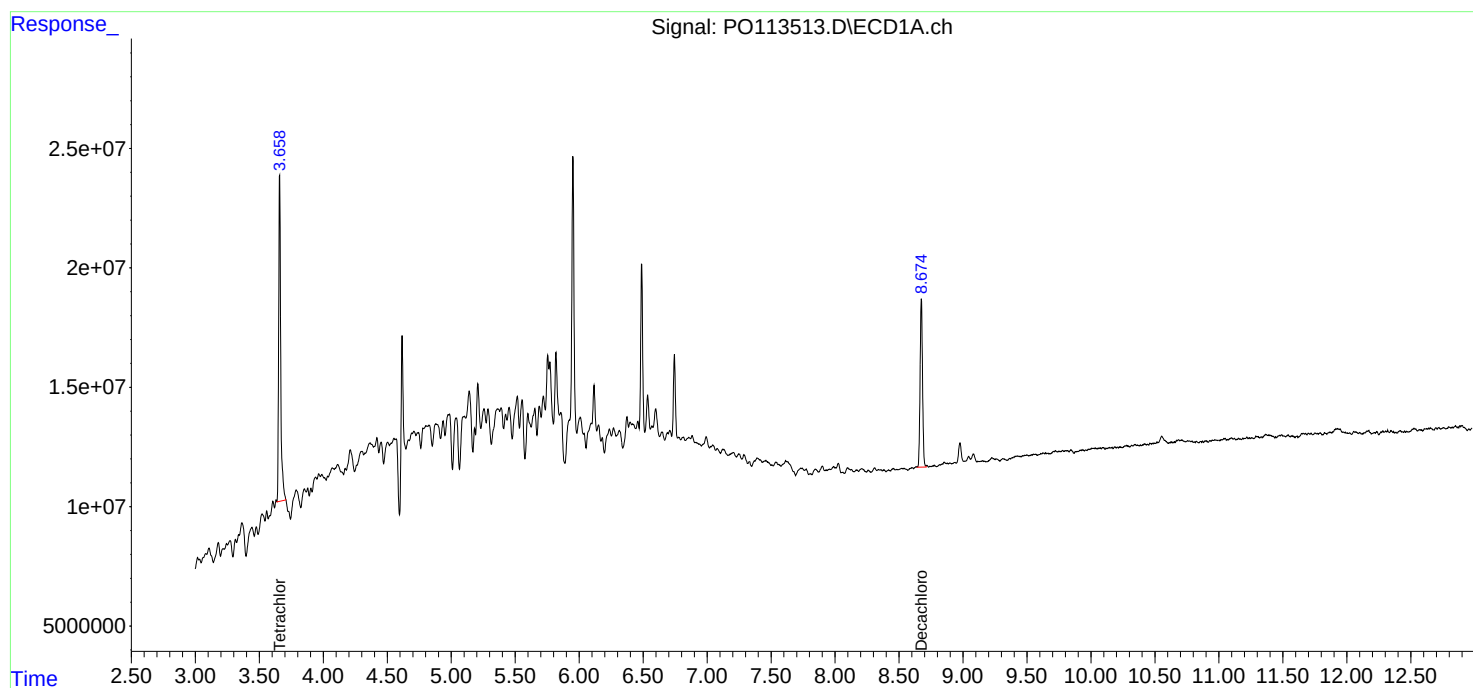

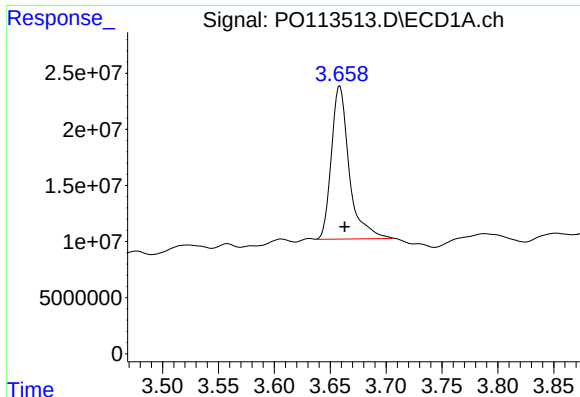


#1 Tetrachloro-m-xylene

R.T.: 3.658 min
Delta R.T.: -0.005 min
Response: 151447560
Conc: 18.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
EO-02-09042025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/08/2025
Supervised By :mohammad ahmed 09/09/2025

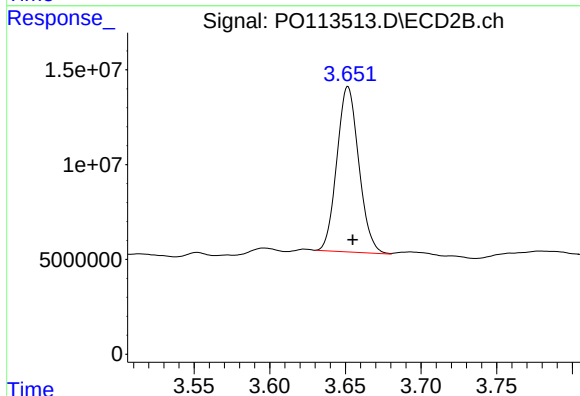


#1 Tetrachloro-m-xylene

R.T.: 3.652 min
Delta R.T.: -0.003 min
Response: 87876972
Conc: 17.36 ng/ml

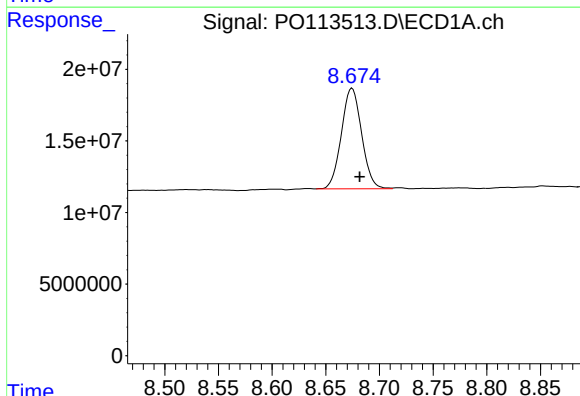

#2 Decachlorobiphenyl

R.T.: 8.675 min
Delta R.T.: -0.007 min
Response: 92336434
Conc: 13.32 ng/ml

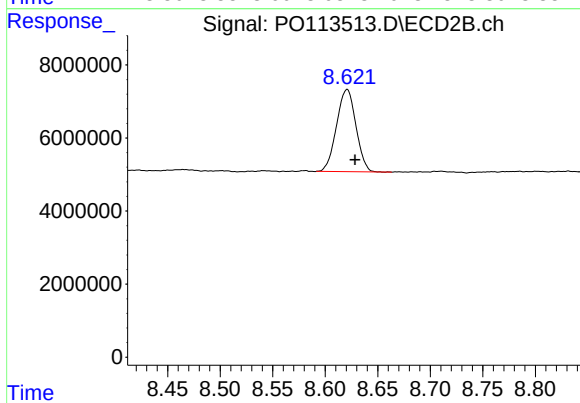

#2 Decachlorobiphenyl

R.T.: 8.621 min
Delta R.T.: -0.008 min
Response: 28915493
Conc: 15.26 ng/ml