

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090618\
 Data File : P0048792.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Sep 2018 16:43
 Operator : SM/SJ
 Sample : J4720-01DL 4X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BZTRANS-1DL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 00:42:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 06 03:44:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.453	3.529	753019	650464	6.241	4.162 #
2)	SA Decachlor...	10.198	8.467	736914	854836	5.282	5.782
Target Compounds							
31)	L7 AR-1260-1	7.228	6.066	7030368	7680810	853.319	737.813
32)	L7 AR-1260-2	7.485	6.252	6494829	7073106	660.947	564.827
33)	L7 AR-1260-3	7.768	6.405	8278760	8221443	693.823	692.956
34)	L7 AR-1260-4	8.069	6.873	8487677	8912239	988.898	941.992
35)	L7 AR-1260-5	8.391	7.112	15409697	19129996	928.197	880.964



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090618\
Data File : P0048792.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Sep 2018 16:43
Operator : SM/SJ
Sample : J4720-01DL 4X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
BZTRANS-1DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 00:42:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090418.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 06 03:44:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

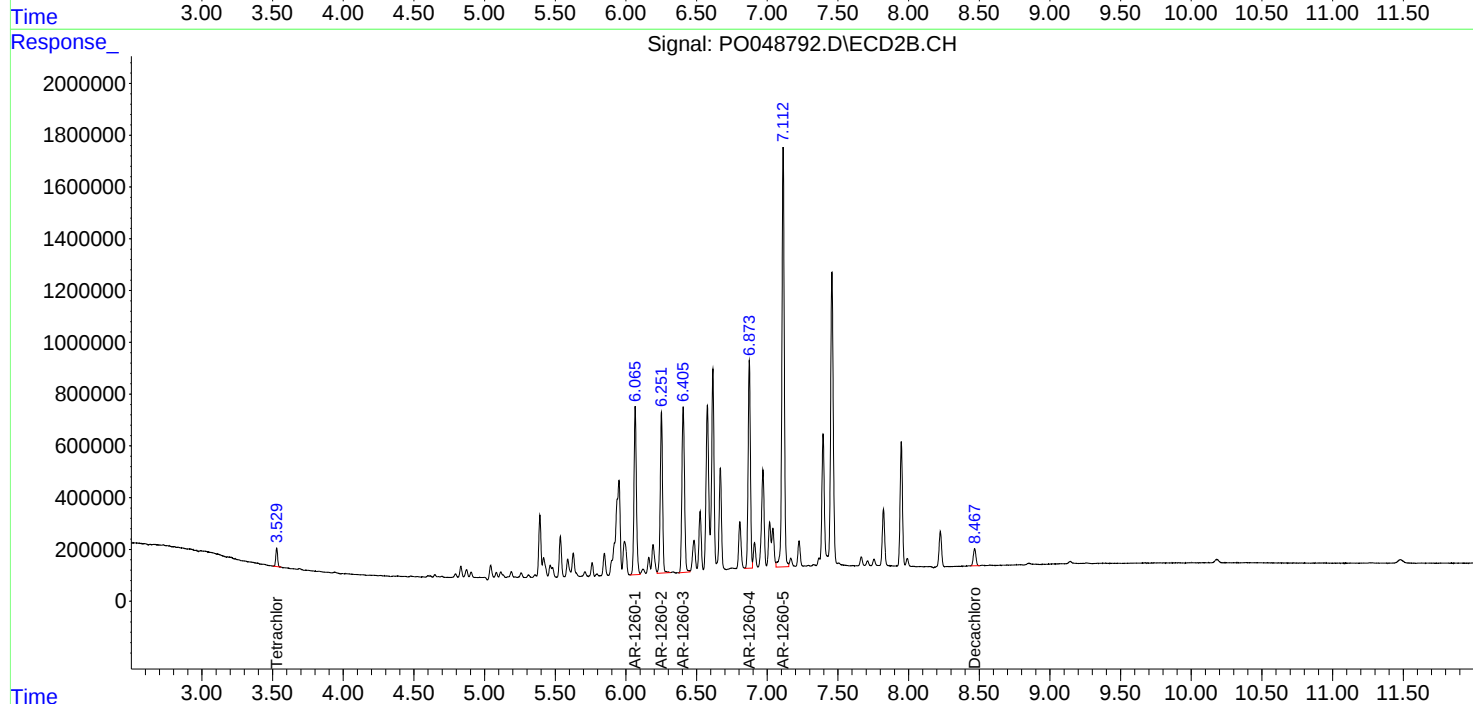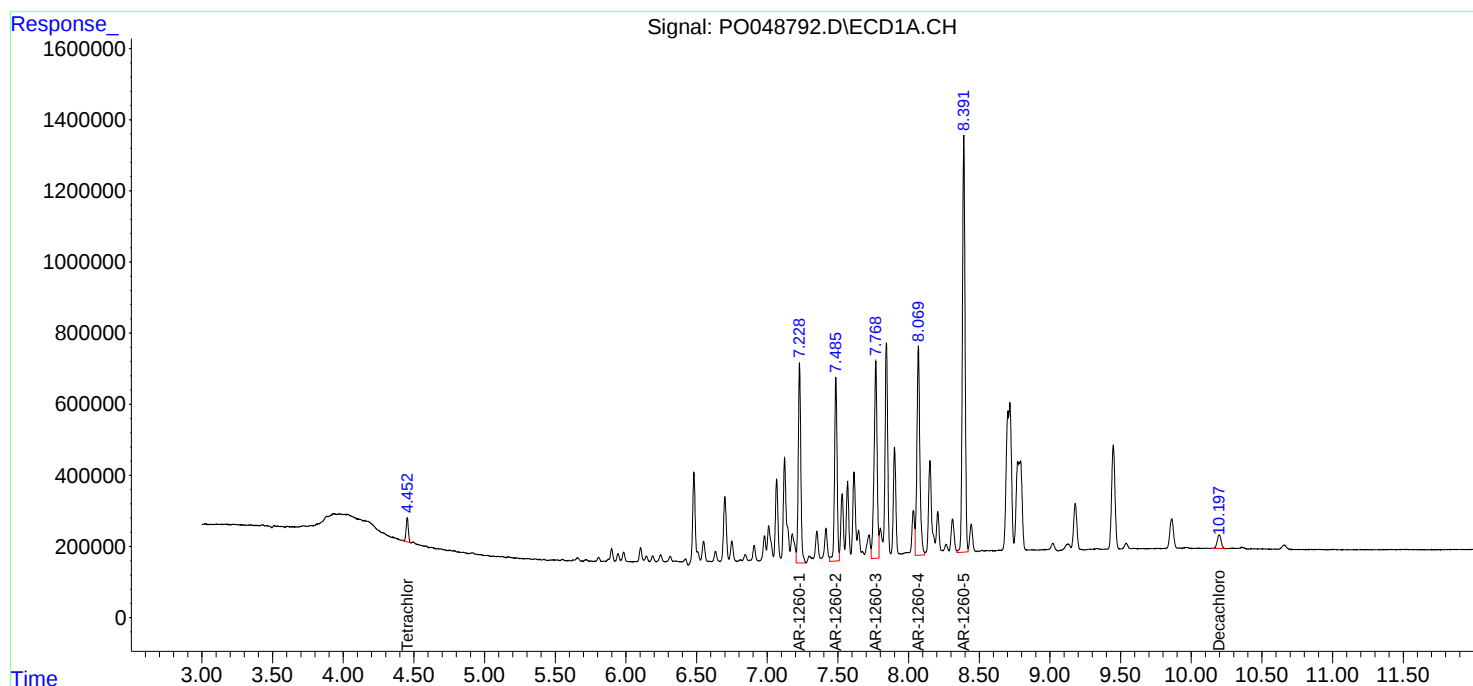


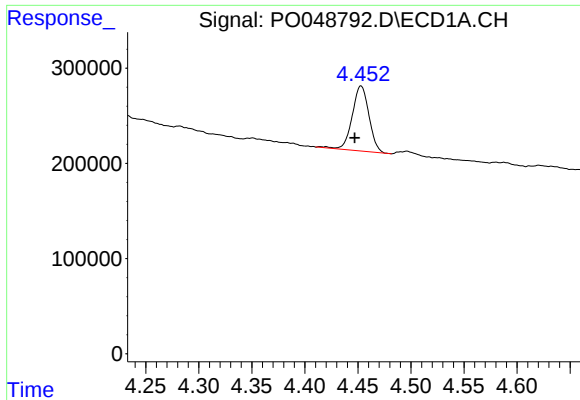

#1 Tetrachloro-m-xylene


R.T.: 4.453 min
Delta R.T.: 0.006 min
Response: 753019
Conc: 6.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
BZTRANS-1DL

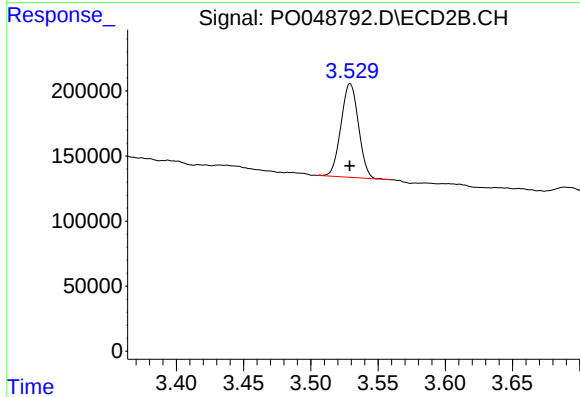


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: 0.000 min
Response: 650464
Conc: 4.16 ng/ml

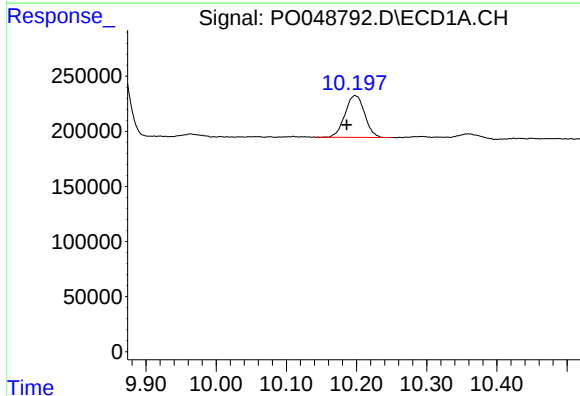


#2 Decachlorobiphenyl

R.T.: 10.198 min
Delta R.T.: 0.012 min
Response: 736914
Conc: 5.28 ng/ml

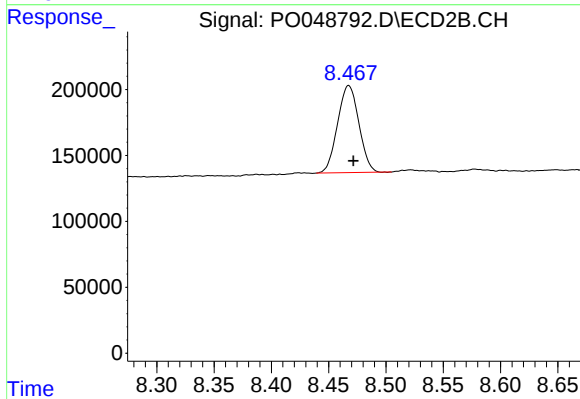

#2 Decachlorobiphenyl


R.T.: 8.467 min
Delta R.T.: -0.004 min
Response: 854836
Conc: 5.78 ng/ml

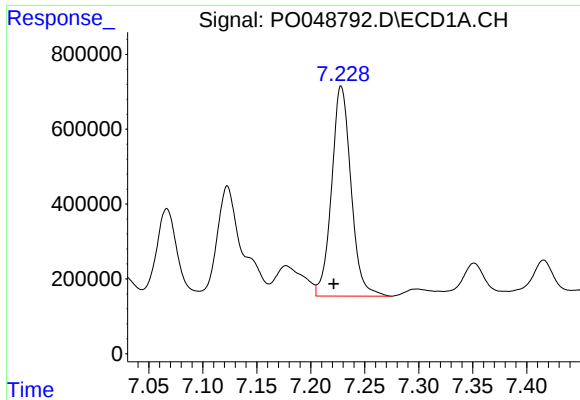

#31 AR-1260-1


R.T.: 7.228 min
Delta R.T.: 0.007 min
Response: 7030368
Conc: 853.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
BZTRANS-1DL

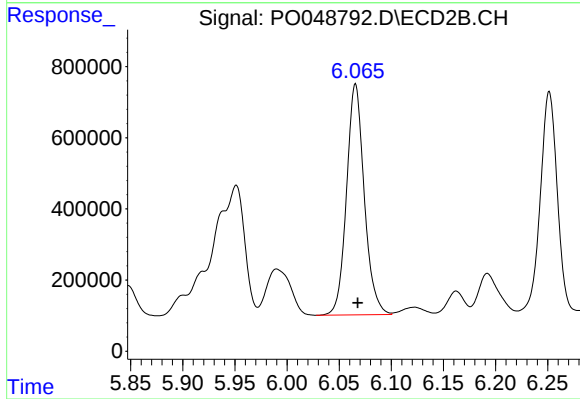


#31 AR-1260-1

R.T.: 6.066 min
Delta R.T.: -0.002 min
Response: 7680810
Conc: 737.81 ng/ml

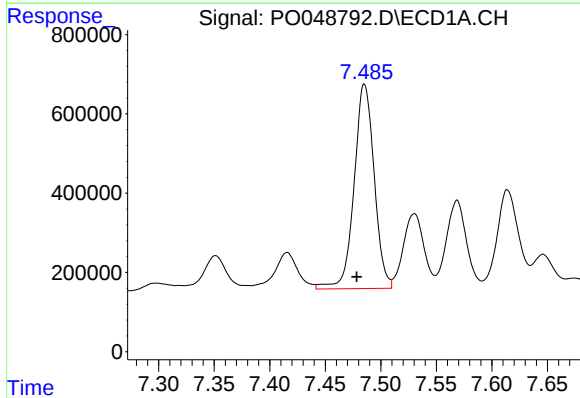


#32 AR-1260-2

R.T.: 7.485 min
Delta R.T.: 0.007 min
Response: 6494829
Conc: 660.95 ng/ml

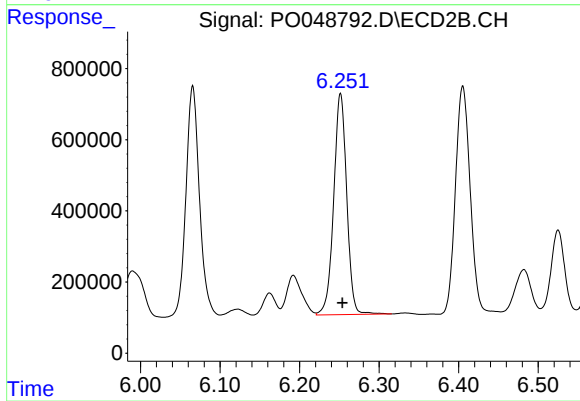

#32 AR-1260-2


R.T.: 6.252 min
Delta R.T.: -0.002 min
Response: 7073106
Conc: 564.83 ng/ml

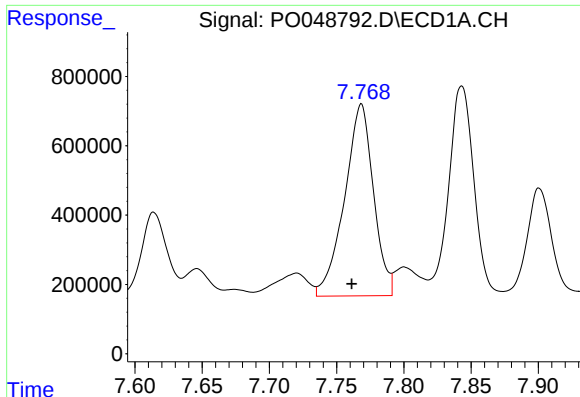

#33 AR-1260-3


R.T.: 7.768 min
Delta R.T.: 0.007 min
Response: 8278760
Conc: 693.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
BZTRANS-1DL

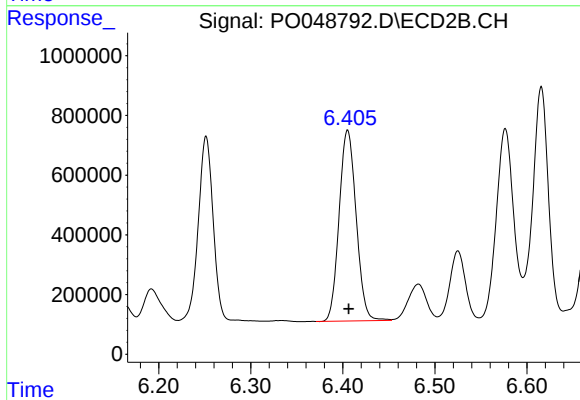


#33 AR-1260-3

R.T.: 6.405 min
Delta R.T.: 0.000 min
Response: 8221443
Conc: 692.96 ng/ml

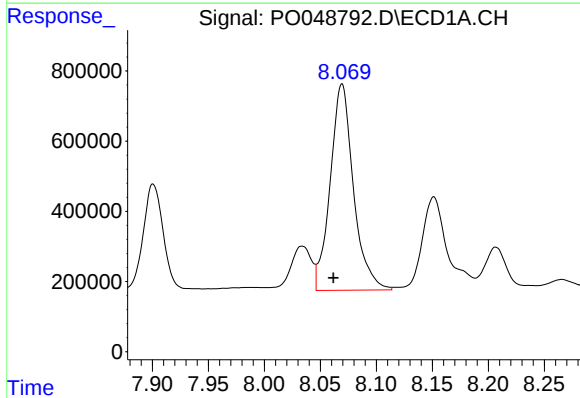


#34 AR-1260-4

R.T.: 8.069 min
Delta R.T.: 0.008 min
Response: 8487677
Conc: 988.90 ng/ml

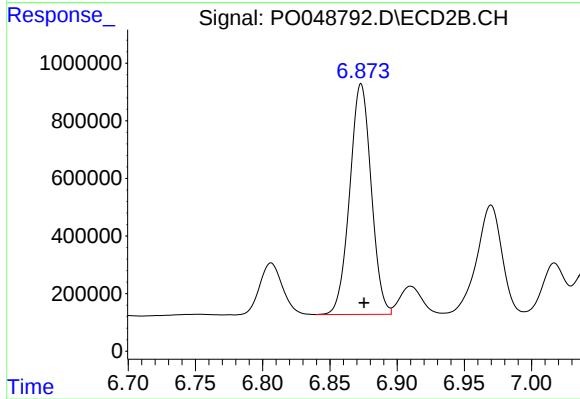

#34 AR-1260-4


R.T.: 6.873 min
Delta R.T.: -0.002 min
Response: 8912239
Conc: 941.99 ng/ml

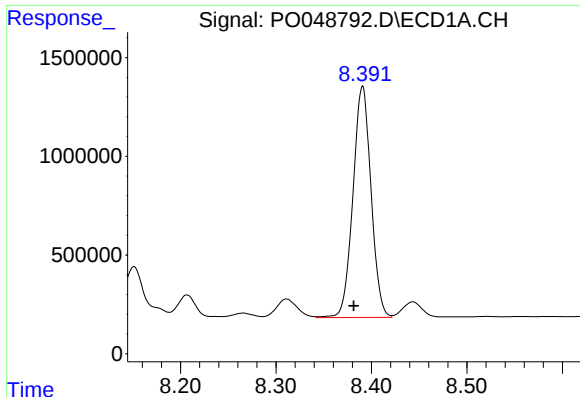

#35 AR-1260-5

R.T.: 8.391 min
Delta R.T.: 0.009 min
Response: 15409697
Conc: 928.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
BZTRANS-1DL

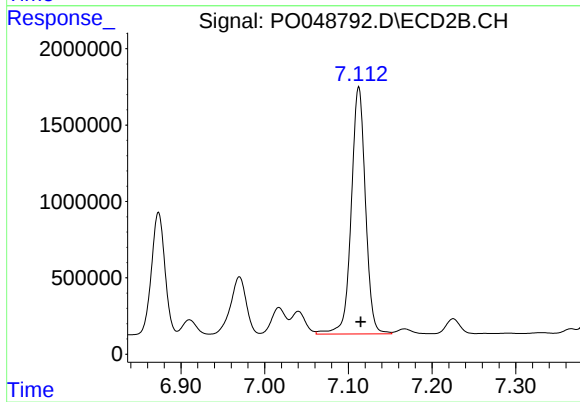

#35 AR-1260-5

R.T.: 7.112 min
Delta R.T.: -0.002 min
Response: 19129996
Conc: 880.96 ng/ml