

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090619\
 Data File : P0060428.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Sep 2019 15:08
 Operator : SM/AJ
 Sample : K4655-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-15-D

Manual Integrations
 APPROVED

Ankita
 9/9/2019 12:15:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 17:07:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 06 16:33:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.108	3.487	926877	817954	26.473m	22.724
2)	SA Decachlor...	9.555	8.337	1073126	806483	20.171	20.002
Target Compounds							
26)	L6 AR-1254-1	6.090	5.315	43870	47211	21.027m	19.905
27)	L6 AR-1254-2	6.307	5.458	187205	56013	56.112	26.694m#
28)	L6 AR-1254-3	6.672	5.862	215961	64114	60.861	19.067m#
29)	L6 AR-1254-4	6.953	6.080	178301	102613	60.533	49.768m
30)	L6 AR-1254-5	7.367	6.487	342380	200730	110.717	64.648m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090619\
Data File : PO060428.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Sep 2019 15:08
Operator : SM/AJ
Sample : K4655-07
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-15-D


Manual Integrations
APPROVED

Ankita
9/9/2019 12:15:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 17:07:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 06 16:33:49 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

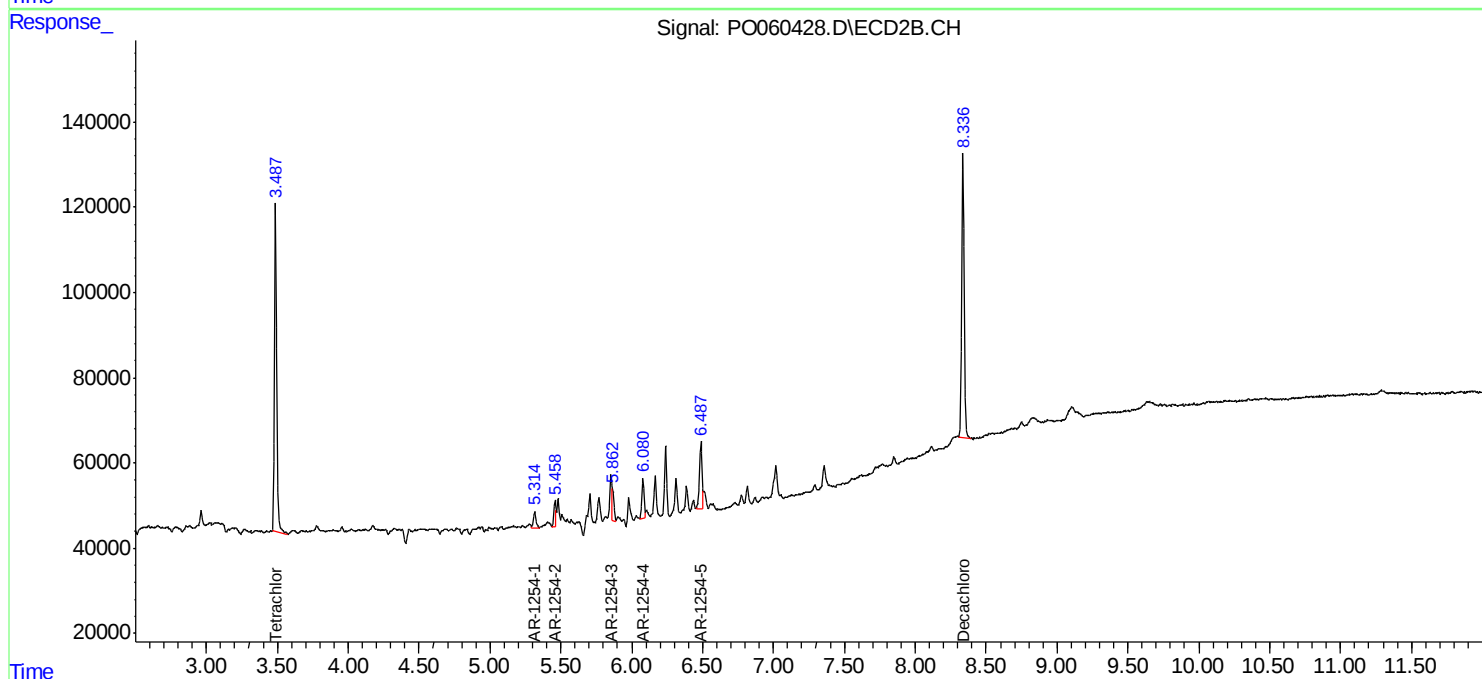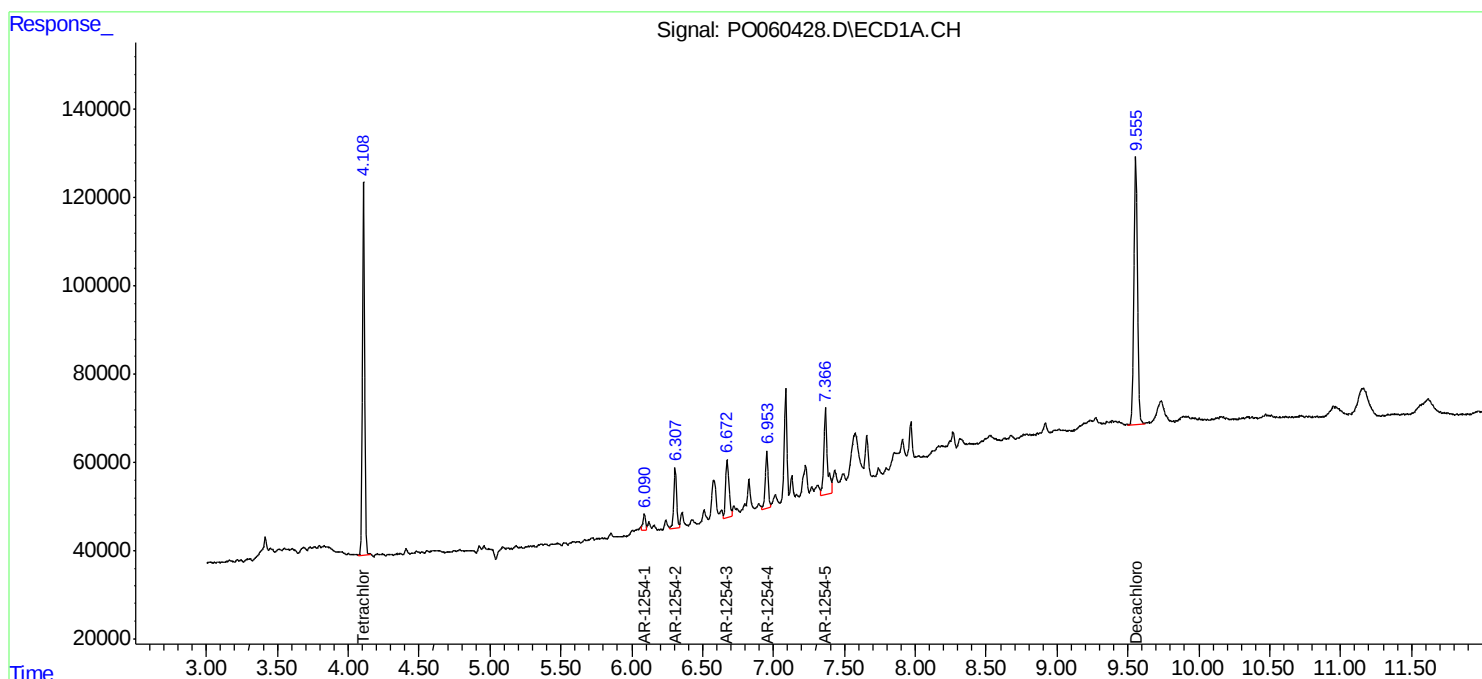

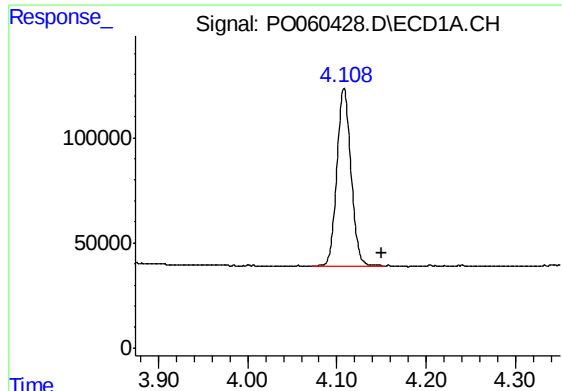


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: -0.042 min
Response: 926877
Conc: 26.47 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-15-D


Manual Integrations
APPROVED

Ankita
9/9/2019 12:15:12 PM

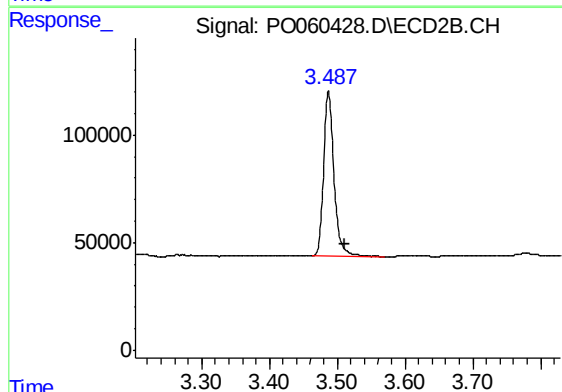


#1 Tetrachloro-m-xylene

R.T.: 3.487 min
Delta R.T.: -0.023 min
Response: 817954
Conc: 22.72 ng/ml

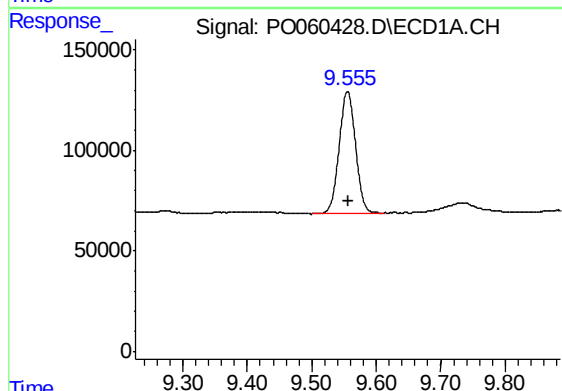


#2 Decachlorobiphenyl

R.T.: 9.555 min
Delta R.T.: -0.002 min
Response: 1073126
Conc: 20.17 ng/ml

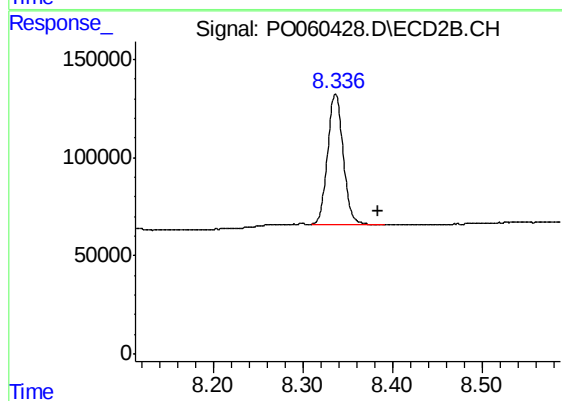

#2 Decachlorobiphenyl

R.T.: 8.337 min
Delta R.T.: -0.048 min
Response: 806483
Conc: 20.00 ng/ml

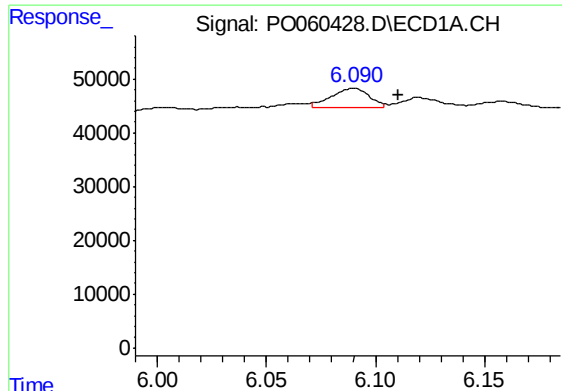


#26 AR-1254-1

R.T.: 6.090 min
Delta R.T.: -0.021 min
Response: 43870
Conc: 21.03 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-15-D


Manual Integrations
APPROVED

Ankita
9/9/2019 12:15:12 PM

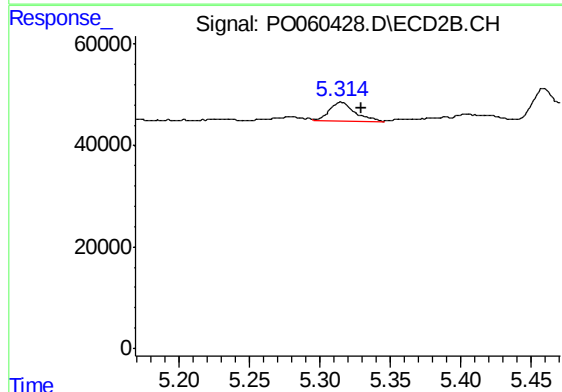


#26 AR-1254-1

R.T.: 5.315 min
Delta R.T.: -0.014 min
Response: 47211
Conc: 19.91 ng/ml

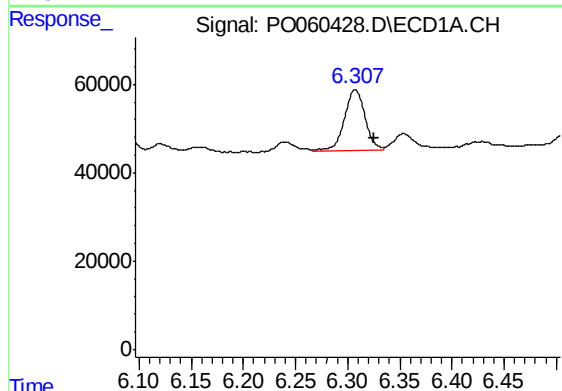


#27 AR-1254-2

R.T.: 6.307 min
Delta R.T.: -0.018 min
Response: 187205
Conc: 56.11 ng/ml

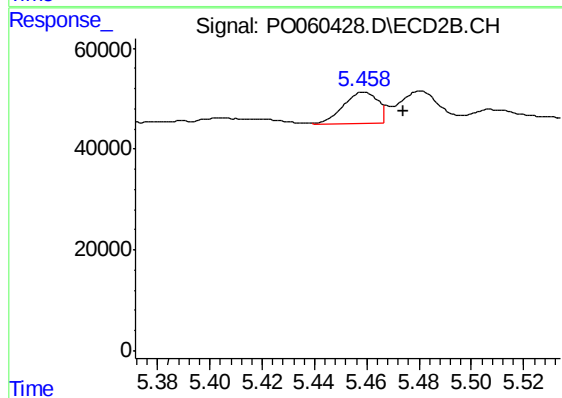

#27 AR-1254-2

R.T.: 5.458 min
Delta R.T.: -0.016 min
Response: 56013
Conc: 26.69 ng/ml m

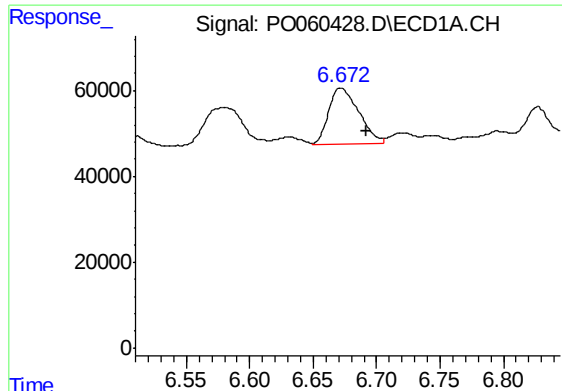


#28 AR-1254-3

R.T.: 6.672 min
Delta R.T.: -0.020 min
Response: 215961
Conc: 60.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-15-D


Manual Integrations
APPROVED

Ankita
9/9/2019 12:15:12 PM

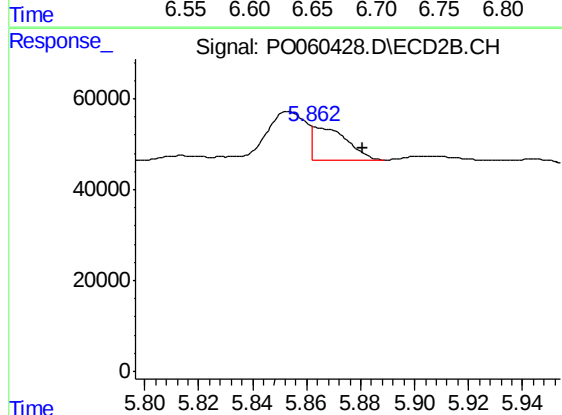


#28 AR-1254-3

R.T.: 5.862 min
Delta R.T.: -0.019 min
Response: 64114
Conc: 19.07 ng/ml m

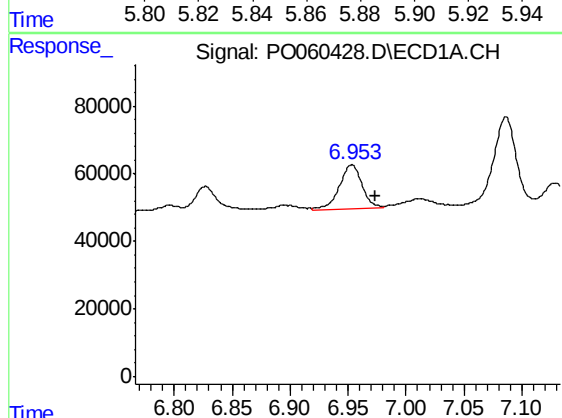


#29 AR-1254-4

R.T.: 6.953 min
Delta R.T.: -0.021 min
Response: 178301
Conc: 60.53 ng/ml

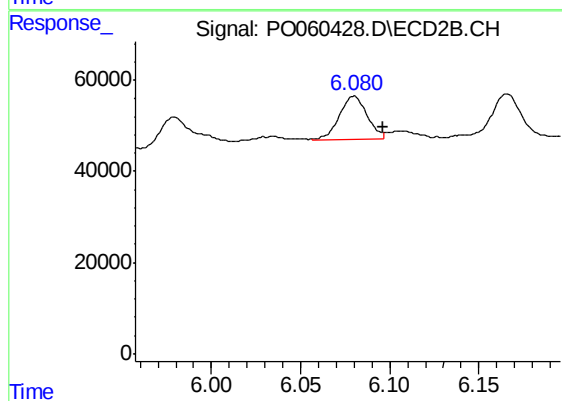

#29 AR-1254-4

R.T.: 6.080 min
Delta R.T.: -0.017 min
Response: 102613
Conc: 49.77 ng/ml m

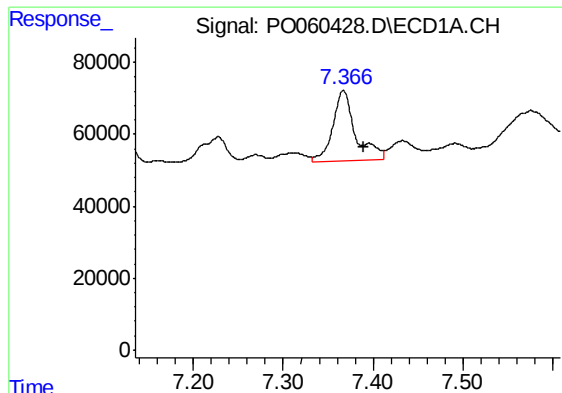


#30 AR-1254-5

R.T.: 7.367 min
Delta R.T.: -0.023 min
Response: 342380
Conc: 110.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-15-D

Manual Integrations
APPROVED

Ankita
9/9/2019 12:15:12 PM

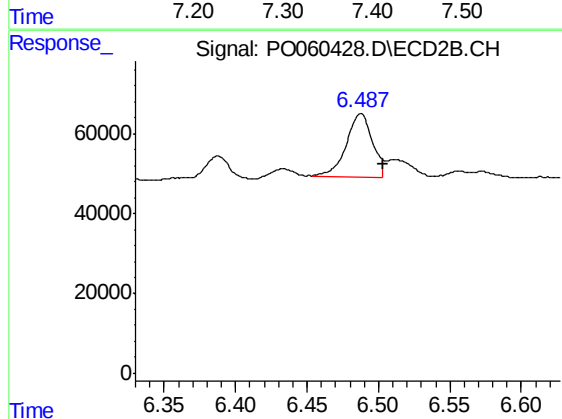

#30 AR-1254-5

R.T.: 6.487 min
Delta R.T.: -0.016 min
Response: 200730
Conc: 64.65 ng/ml m