

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090619\
 Data File : P0060436.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Sep 2019 17:22
 Operator : SM/AJ
 Sample : PB122832BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB122832BL

Manual Integrations
 APPROVED

Ankita
 9/9/2019 12:15:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 23:02:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 06 17:58:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.104	3.486	1033942	871660	29.531m	24.216
2)	SA Decachlor...	9.549	8.334	1244765	966403	23.398	23.968m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090619\
Data File : PO060436.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Sep 2019 17:22
Operator : SM/AJ
Sample : PB122832BL
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB122832BL


Manual Integrations
APPROVED

Ankita
9/9/2019 12:15:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 23:02:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 06 17:58:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

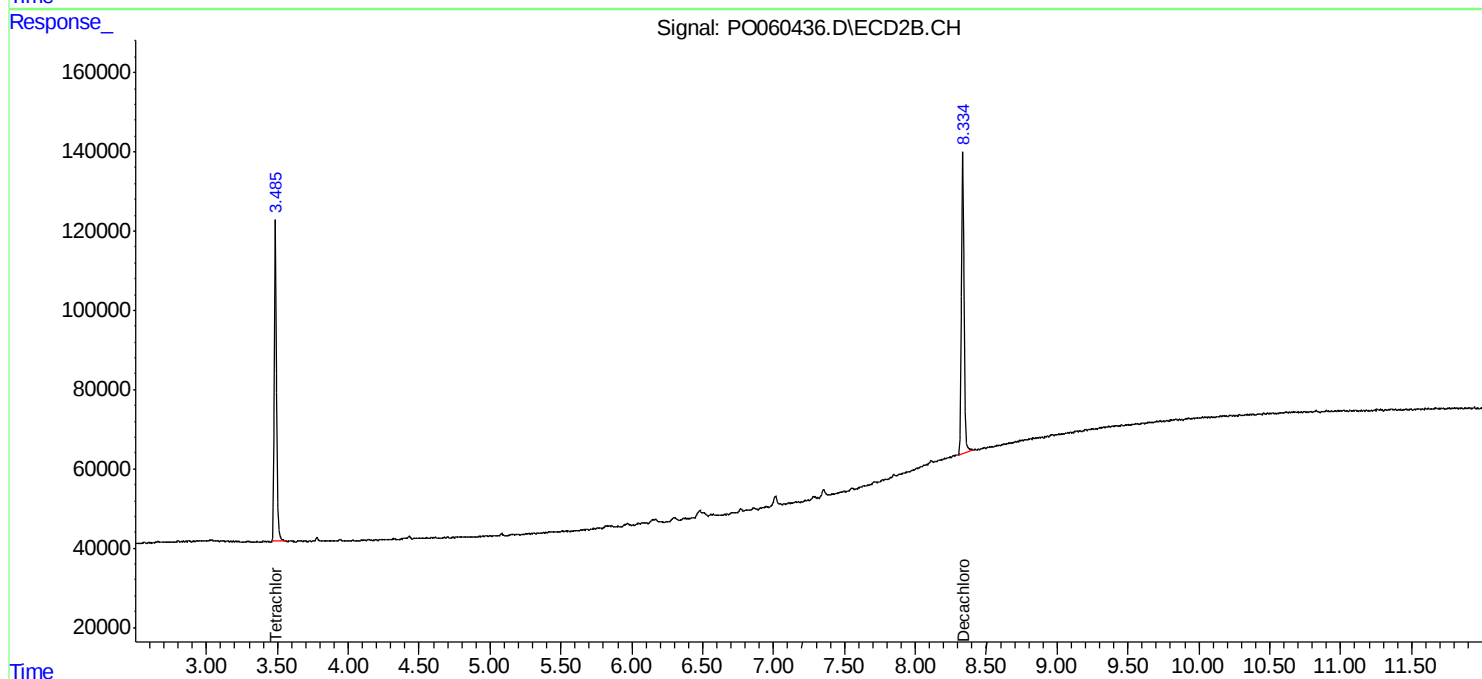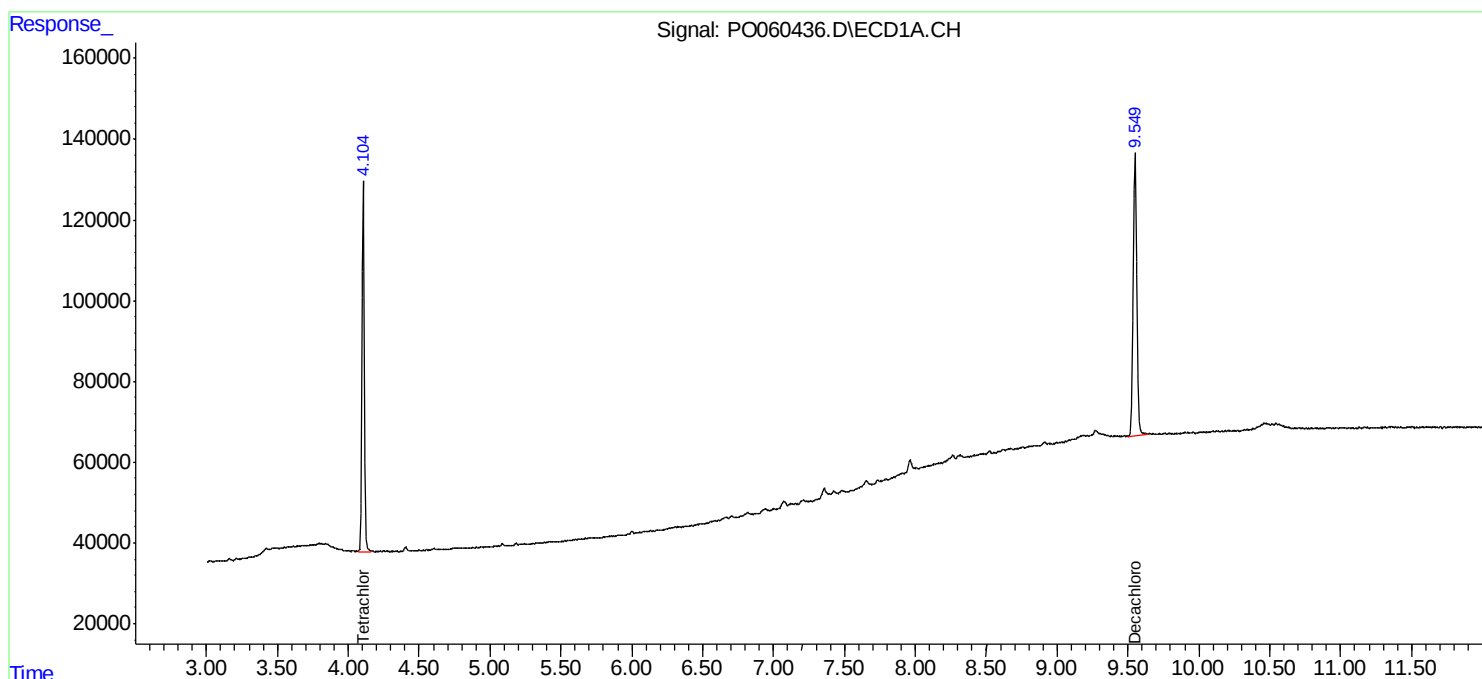

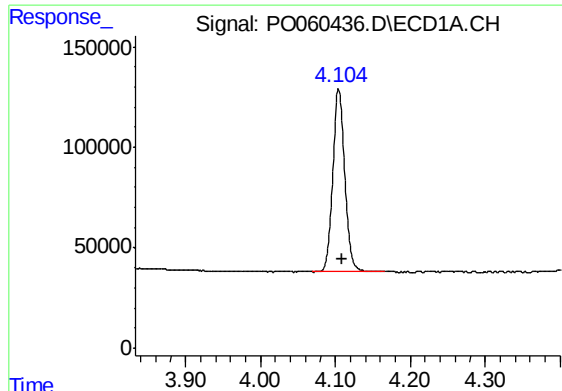


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: -0.005 min
Response: 1033942
Conc: 29.53 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PB122832BL

Manual Integrations
APPROVED

Ankita
9/9/2019 12:15:23 PM

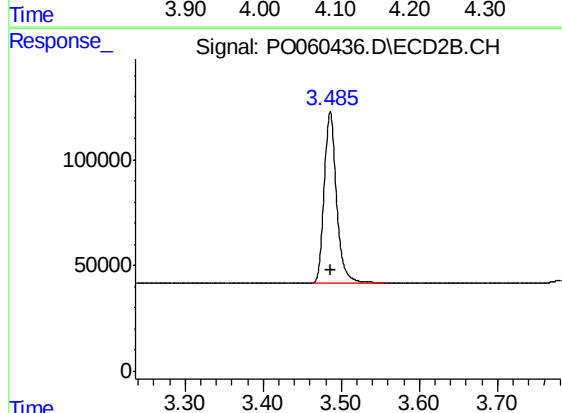

#1 Tetrachloro-m-xylene

R.T.: 3.486 min
Delta R.T.: -0.001 min
Response: 871660
Conc: 24.22 ng/ml

#2 Decachlorobiphenyl

R.T.: 9.549 min
Delta R.T.: -0.008 min
Response: 1244765
Conc: 23.40 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.334 min
Delta R.T.: -0.050 min
Response: 966403
Conc: 23.97 ng/ml m