

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090619\
 Data File : P0060438.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Sep 2019 17:54
 Operator : SM/AJ
 Sample : K4650-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-1

Manual Integrations
 APPROVED

Ankita
 9/9/2019 12:15:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 23:03:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 06 17:58:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.102	3.486	1126075	933178	32.162	25.925
2)	SA Decachlor...	9.548	8.335	1043480	778535	19.614	19.308
Target Compounds							
31)	L7 AR-1260-1	6.820	5.977	94038	98159	34.883m	43.073
32)	L7 AR-1260-2	7.075	6.163	175174	136412	47.211m	46.559
33)	L7 AR-1260-3	7.424	6.312	82455	84800	25.167m	32.011 #
34)	L7 AR-1260-4	7.653	6.772	127908	35032	41.646m	15.483 #
35)	L7 AR-1260-5	7.963	7.016	118471	141025	16.731m	25.625 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090619\
Data File : PO060438.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Sep 2019 17:54
Operator : SM/AJ
Sample : K4650-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-1


Manual Integrations
APPROVED

Ankita
9/9/2019 12:15:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 23:03:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 06 17:58:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

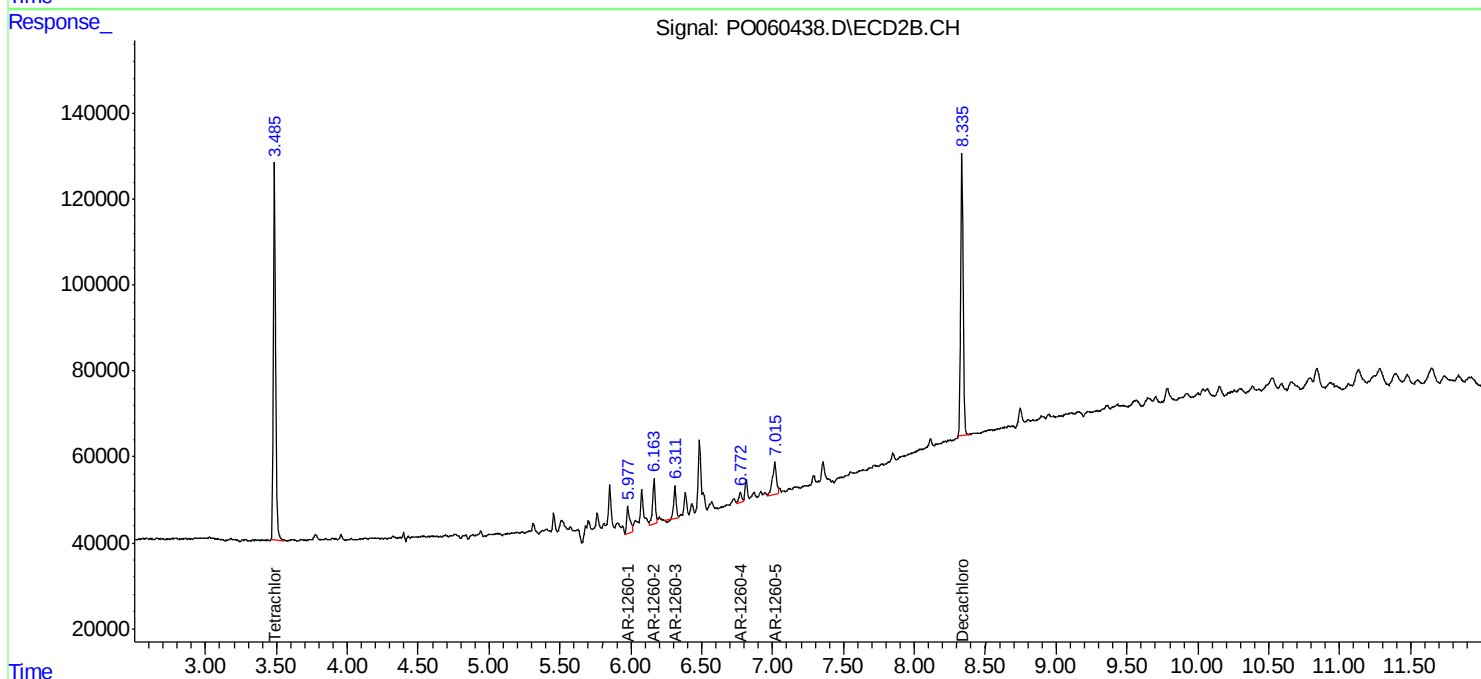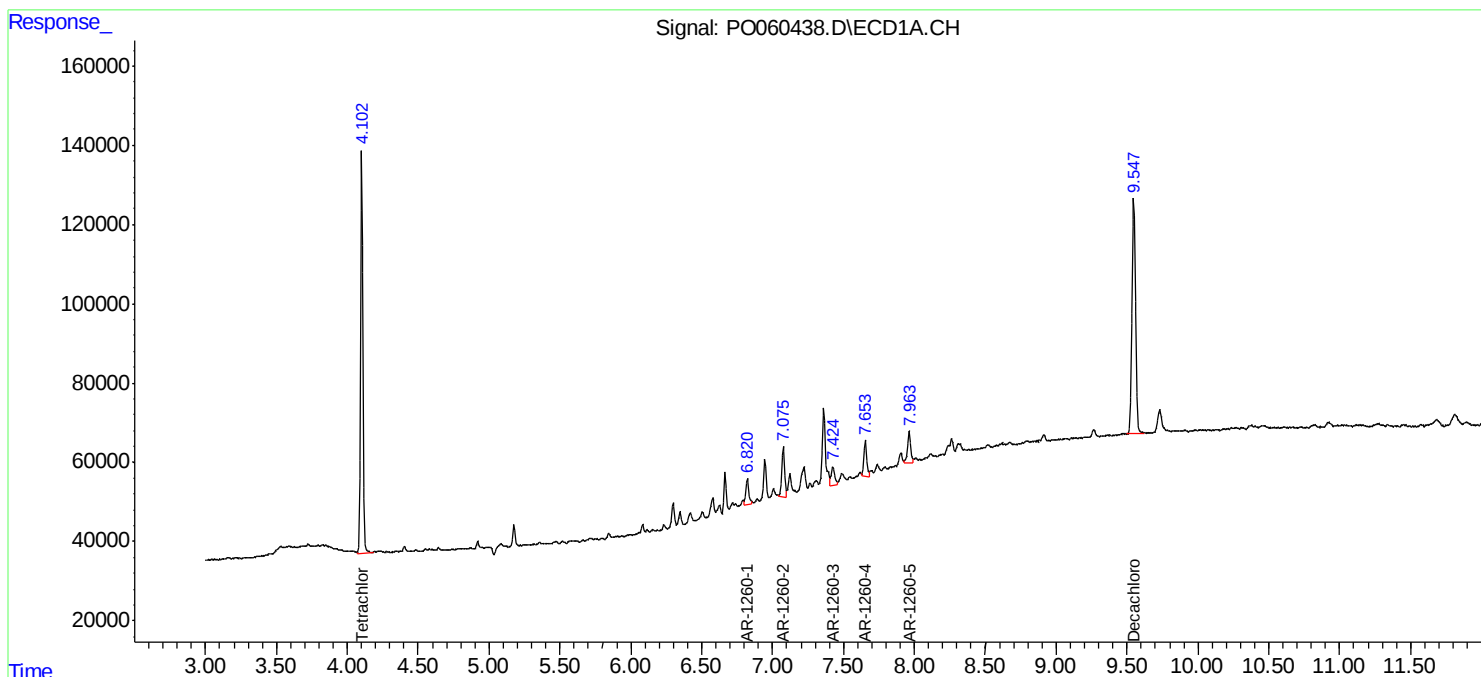

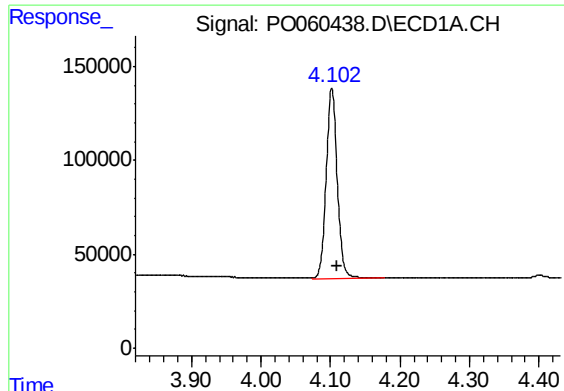


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: -0.007 min
Response: 1126075
Conc: 32.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
9/9/2019 12:15:28 PM

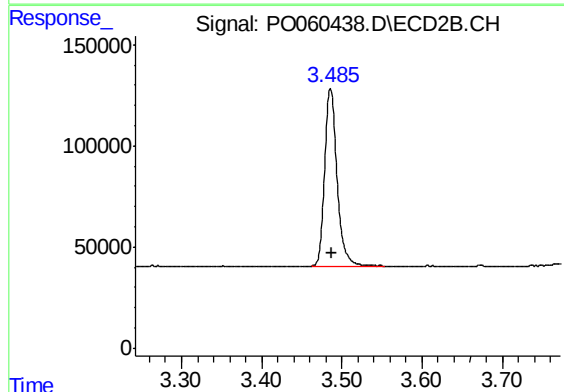


#1 Tetrachloro-m-xylene

R.T.: 3.486 min
Delta R.T.: -0.001 min
Response: 933178
Conc: 25.92 ng/ml

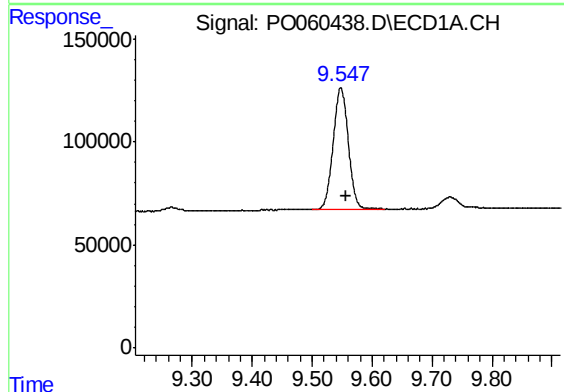


#2 Decachlorobiphenyl

R.T.: 9.548 min
Delta R.T.: -0.009 min
Response: 1043480
Conc: 19.61 ng/ml

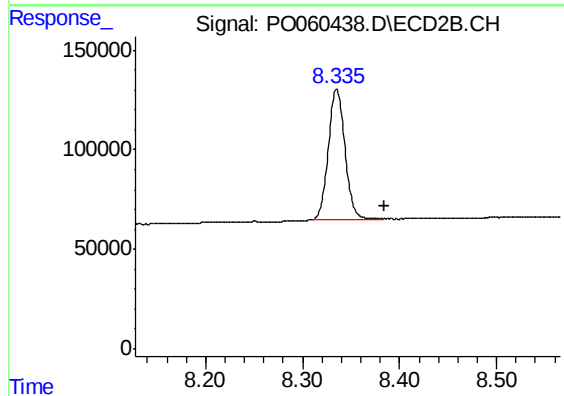

#2 Decachlorobiphenyl

R.T.: 8.335 min
Delta R.T.: -0.049 min
Response: 778535
Conc: 19.31 ng/ml

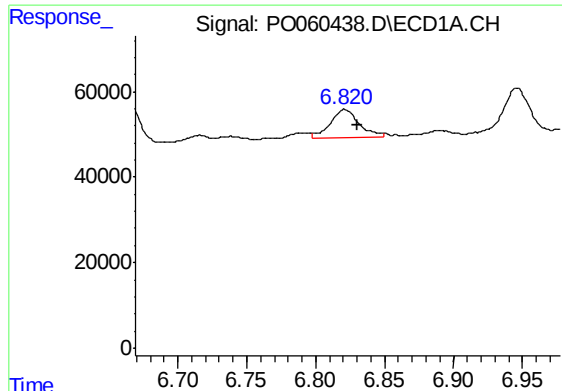


#31 AR-1260-1

R.T.: 6.820 min
Delta R.T.: -0.010 min
Response: 94038
Conc: 34.88 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
9/9/2019 12:15:28 PM

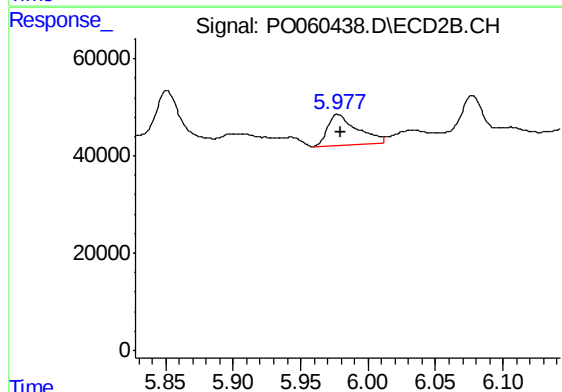


#31 AR-1260-1

R.T.: 5.977 min
Delta R.T.: -0.003 min
Response: 98159
Conc: 43.07 ng/ml

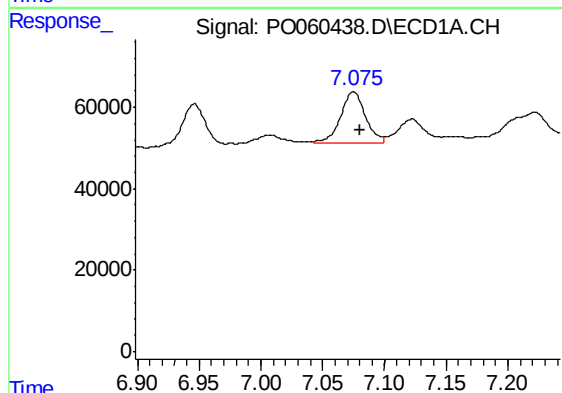


#32 AR-1260-2

R.T.: 7.075 min
Delta R.T.: -0.005 min
Response: 175174
Conc: 47.21 ng/ml m

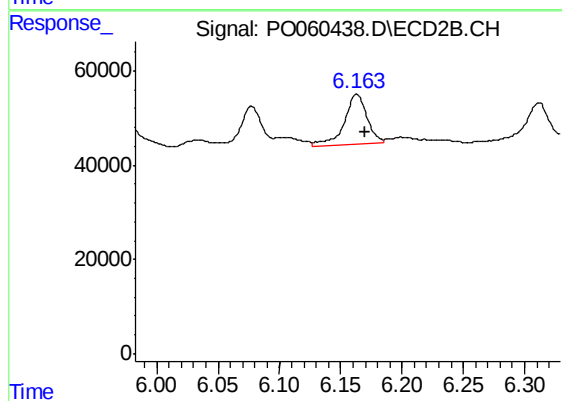

#32 AR-1260-2

R.T.: 6.163 min
Delta R.T.: -0.007 min
Response: 136412
Conc: 46.56 ng/ml

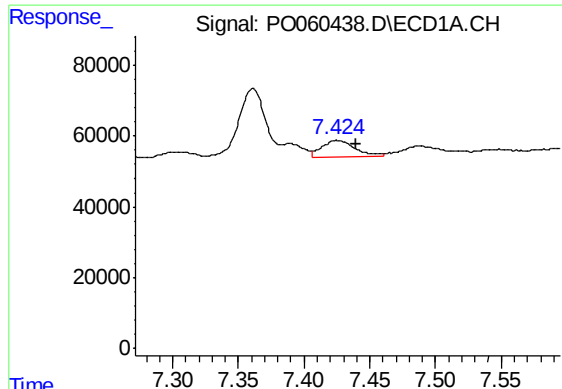


#33 AR-1260-3

R.T.: 7.424 min
Delta R.T.: -0.016 min
Response: 82455
Conc: 25.17 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
9/9/2019 12:15:28 PM

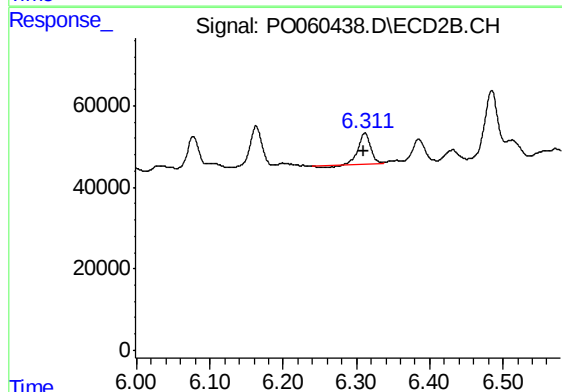


#33 AR-1260-3

R.T.: 6.312 min
Delta R.T.: 0.002 min
Response: 84800
Conc: 32.01 ng/ml

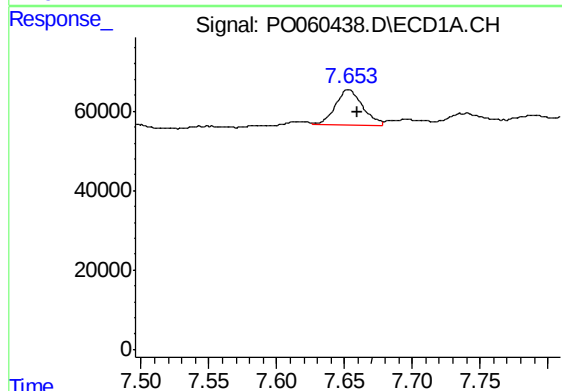


#34 AR-1260-4

R.T.: 7.653 min
Delta R.T.: -0.007 min
Response: 127908
Conc: 41.65 ng/ml m

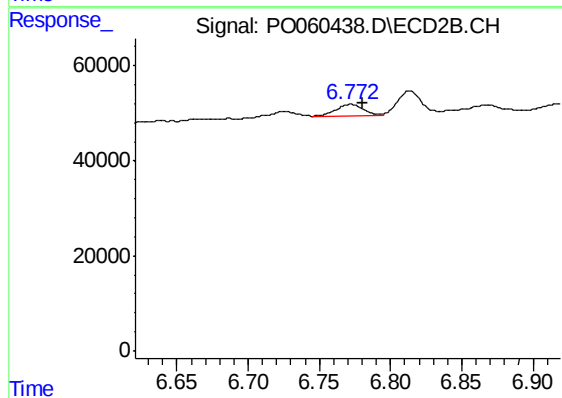

#34 AR-1260-4

R.T.: 6.772 min
Delta R.T.: -0.008 min
Response: 35032
Conc: 15.48 ng/ml

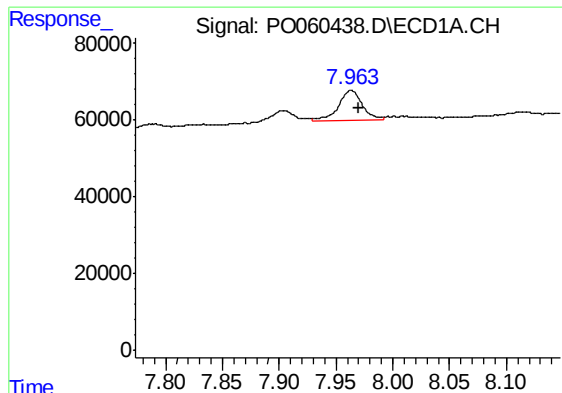


#35 AR-1260-5

R.T.: 7.963 min
Delta R.T.: -0.007 min
Response: 118471
Conc: 16.73 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-1

Manual Integrations
APPROVED

Ankita
9/9/2019 12:15:28 PM

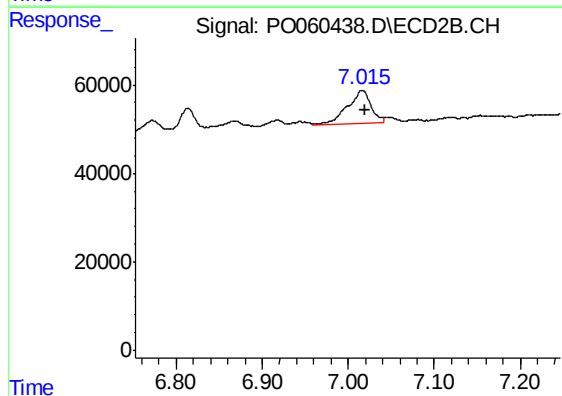

#35 AR-1260-5

R.T.: 7.016 min
Delta R.T.: -0.004 min
Response: 141025
Conc: 25.63 ng/ml