

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090619\
 Data File : P0060449.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Sep 2019 20:51
 Operator : SM/AJ
 Sample : K4692-04
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-31-COMP

Manual Integrations
 APPROVED

Ankita
 9/9/2019 12:16:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 23:07:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 06 17:58:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.101	3.485	1078177	871642	30.794m	24.215
2)	SA Decachlor...	9.547	8.332	1044655	794906	19.636	19.714m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090619\
Data File : PO060449.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Sep 2019 20:51
Operator : SM/AJ
Sample : K4692-04
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-31-COMP


Manual Integrations
APPROVED

Ankita
9/9/2019 12:16:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 23:07:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 06 17:58:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

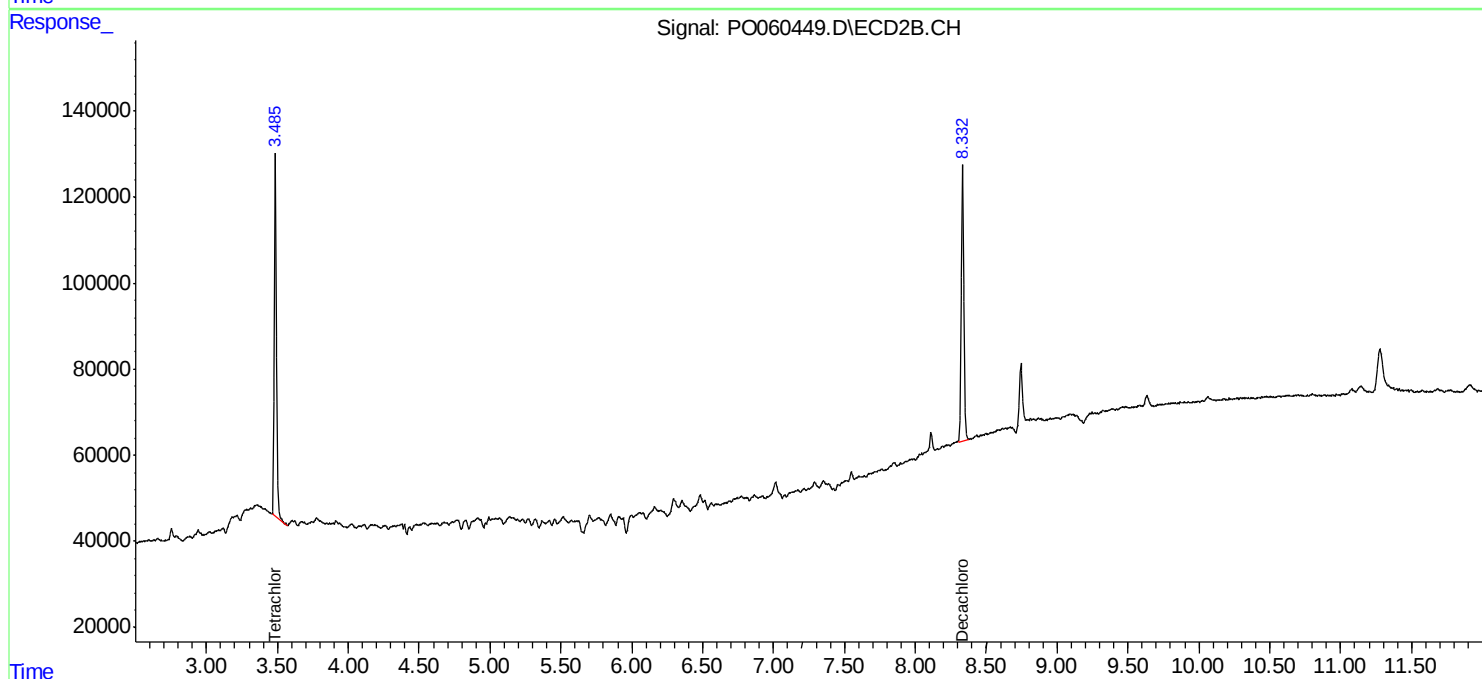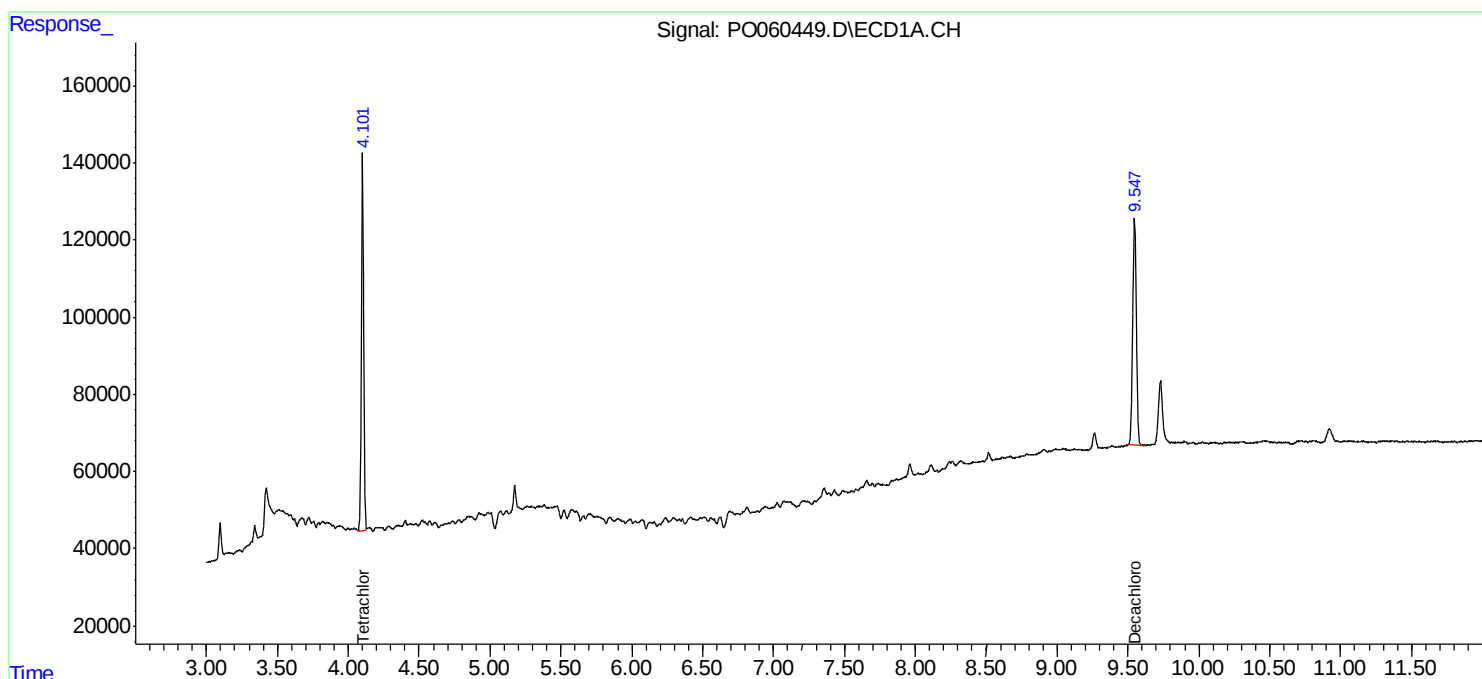

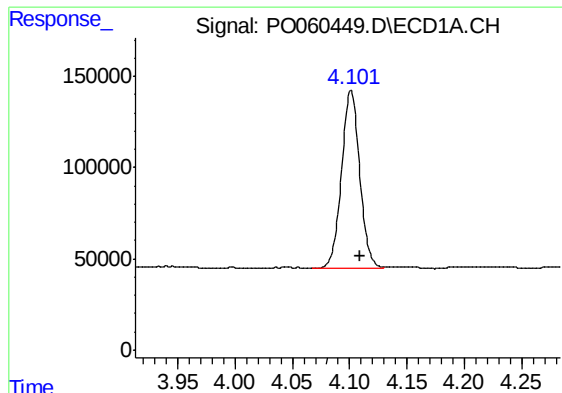


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: -0.008 min
Response: 1078177
Conc: 30.79 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-31-COMP


Manual Integrations
APPROVED

Ankita
9/9/2019 12:16:05 PM

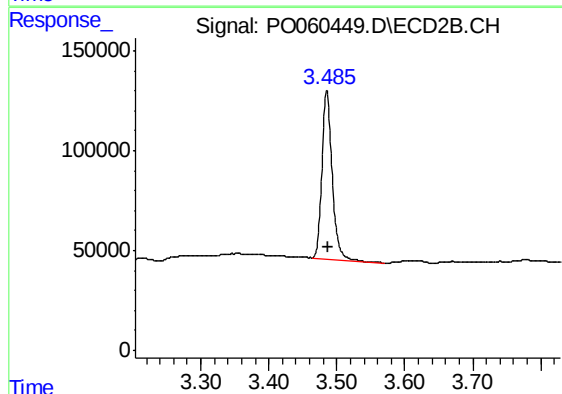


#1 Tetrachloro-m-xylene

R.T.: 3.485 min
Delta R.T.: -0.002 min
Response: 871642
Conc: 24.22 ng/ml

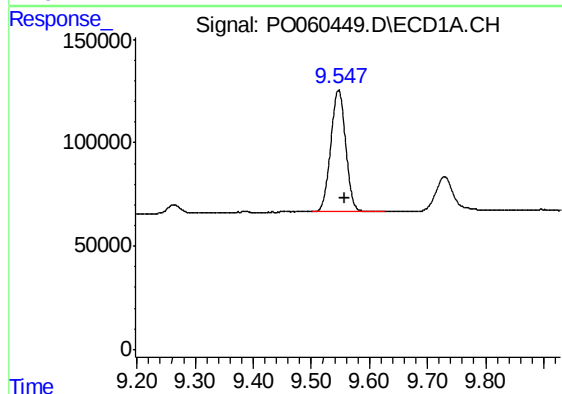

#2 Decachlorobiphenyl

R.T.: 9.547 min
Delta R.T.: -0.010 min
Response: 1044655
Conc: 19.64 ng/ml

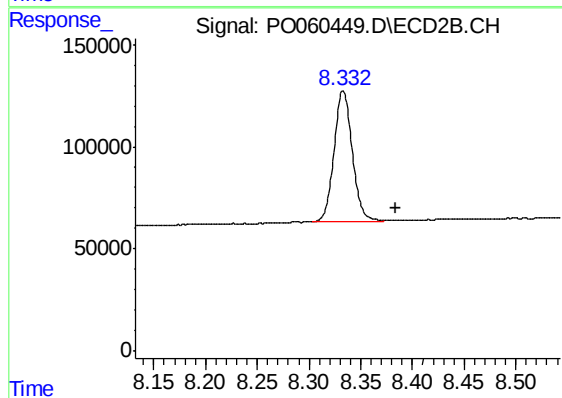

#2 Decachlorobiphenyl

R.T.: 8.332 min
Delta R.T.: -0.052 min
Response: 794906
Conc: 19.71 ng/ml m