

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090619\
 Data File : P0060453.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Sep 2019 21:56
 Operator : SM/AJ
 Sample : K4692-12
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-25-COMP

Manual Integrations
 APPROVED

Ankita
 9/9/2019 12:16:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 23:09:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 06 17:58:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.101	3.486	1210075	1012205	34.561m	28.120
2) SA Decachlor...	9.549	8.334	1314328	1055523	24.705	26.178m
Target Compounds						
31) L7 AR-1260-1	6.820	5.978	243001	139567	90.140m	61.243 #
32) L7 AR-1260-2	7.078	6.164	352282	171594	94.942m	58.567 #
33) L7 AR-1260-3	7.428	6.311	223164	170723	68.114m	64.445
34) L7 AR-1260-4	7.655	6.773	228332	108862	74.343m	48.114 #
35) L7 AR-1260-5	7.964	7.017	289913	345394	40.943m	62.761 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090619\
Data File : PO060453.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Sep 2019 21:56
Operator : SM/AJ
Sample : K4692-12
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-25-COMP


Manual Integrations
APPROVED

Ankita
9/9/2019 12:16:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 23:09:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 06 17:58:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

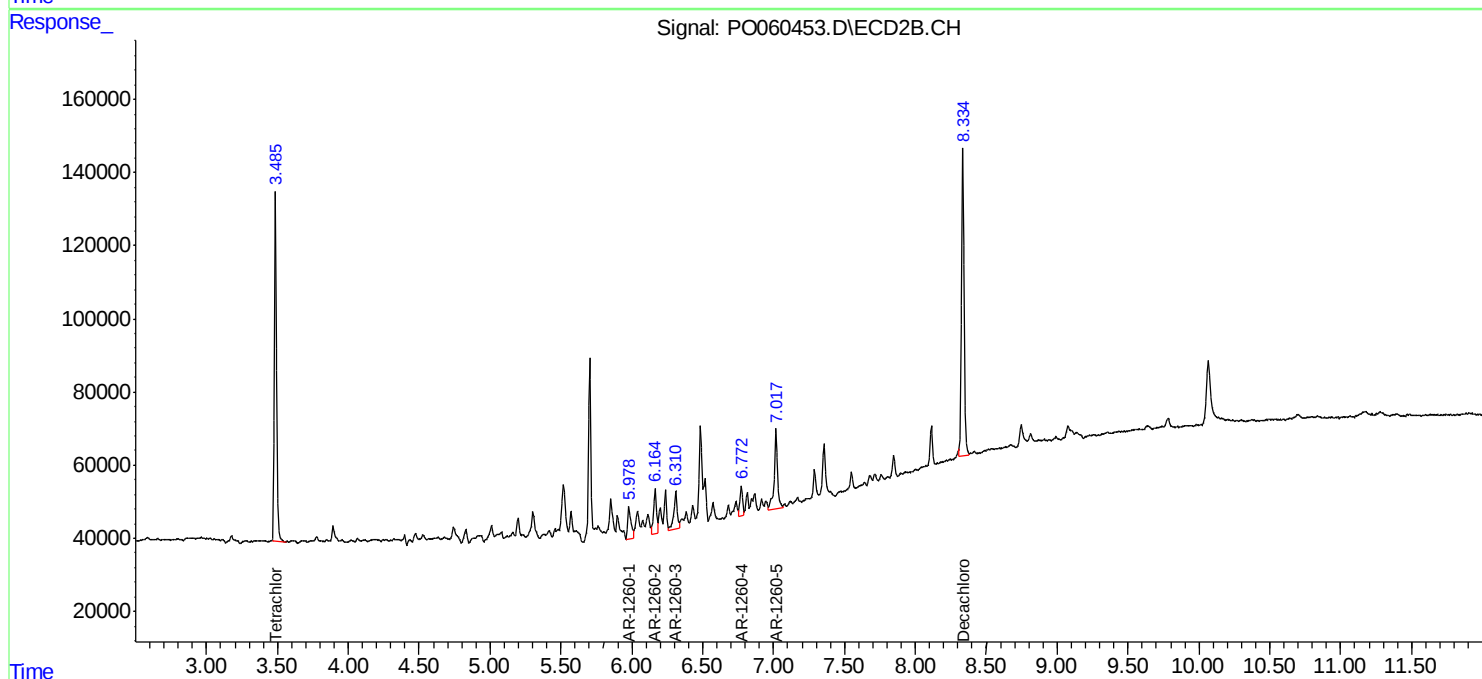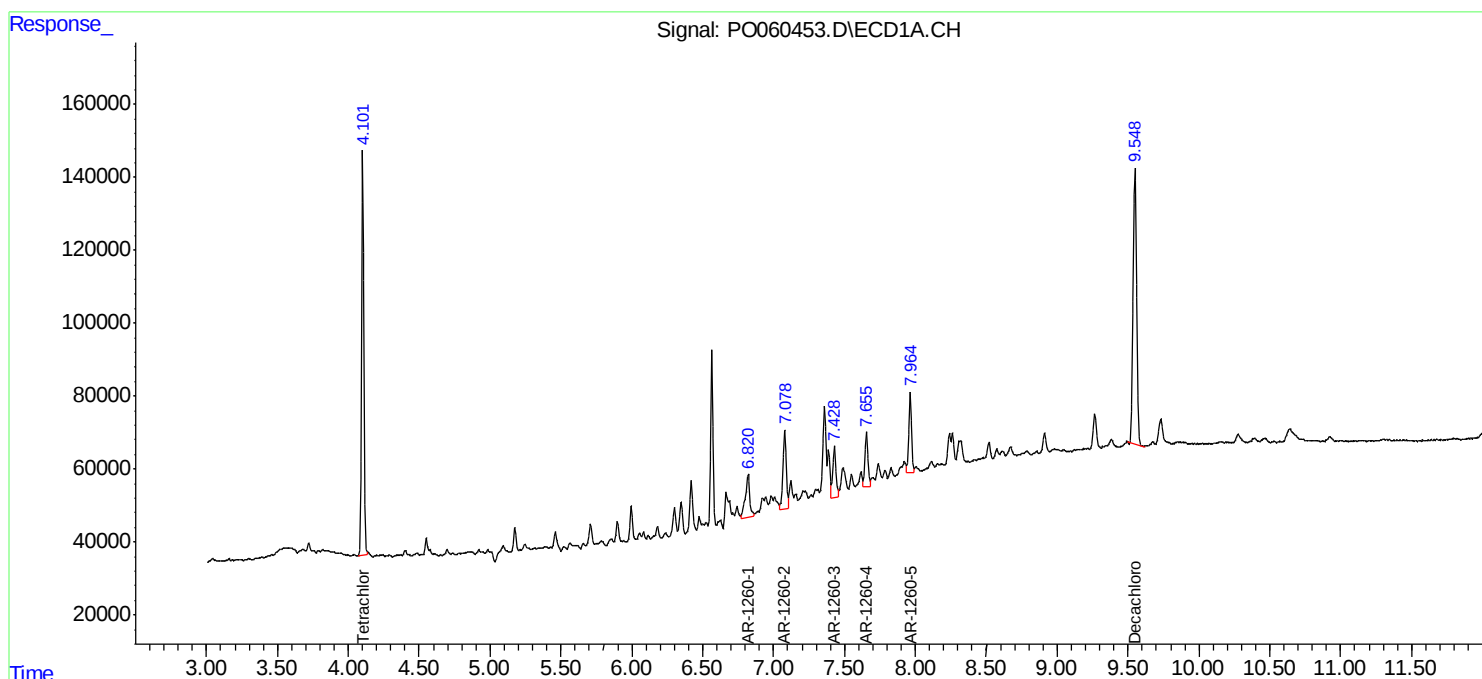

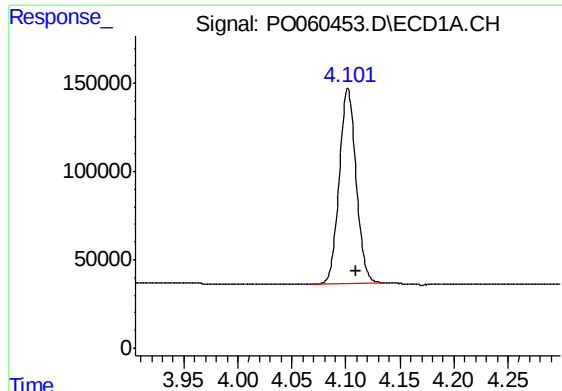


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: -0.008 min
Response: 1210075
Conc: 34.56 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-25-COMP


Manual Integrations
APPROVED

Ankita
9/9/2019 12:16:15 PM

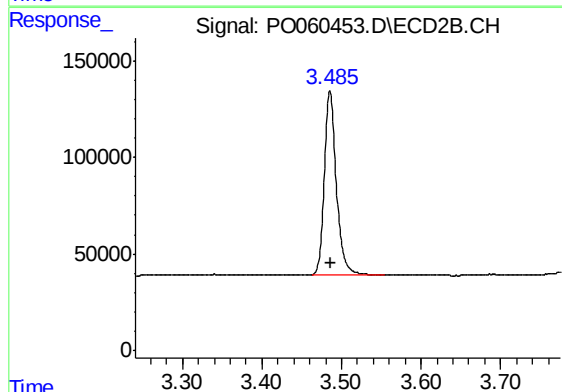


#1 Tetrachloro-m-xylene

R.T.: 3.486 min
Delta R.T.: -0.001 min
Response: 1012205
Conc: 28.12 ng/ml

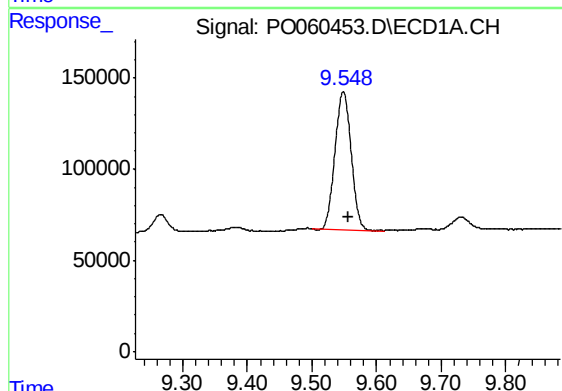


#2 Decachlorobiphenyl

R.T.: 9.549 min
Delta R.T.: -0.008 min
Response: 1314328
Conc: 24.71 ng/ml

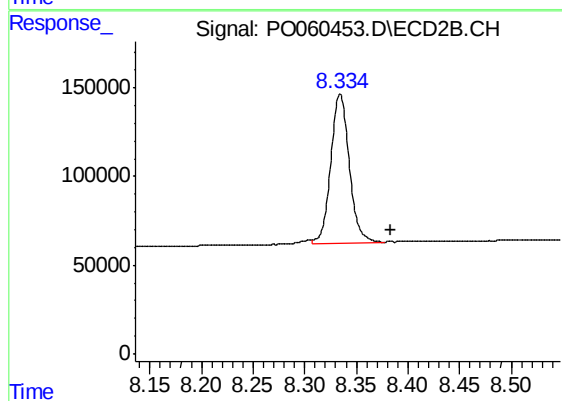

#2 Decachlorobiphenyl

R.T.: 8.334 min
Delta R.T.: -0.050 min
Response: 1055523
Conc: 26.18 ng/ml m

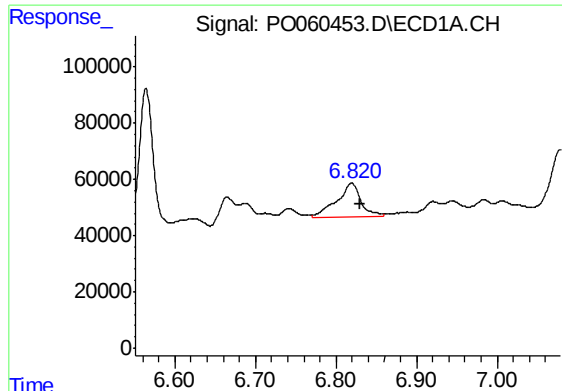


#31 AR-1260-1

R.T.: 6.820 min
Delta R.T.: -0.010 min
Response: 243001
Conc: 90.14 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-25-COMP


Manual Integrations
APPROVED

Ankita
9/9/2019 12:16:15 PM

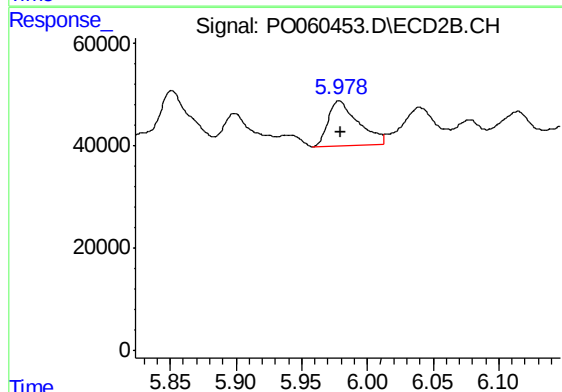


#31 AR-1260-1

R.T.: 5.978 min
Delta R.T.: -0.002 min
Response: 139567
Conc: 61.24 ng/ml

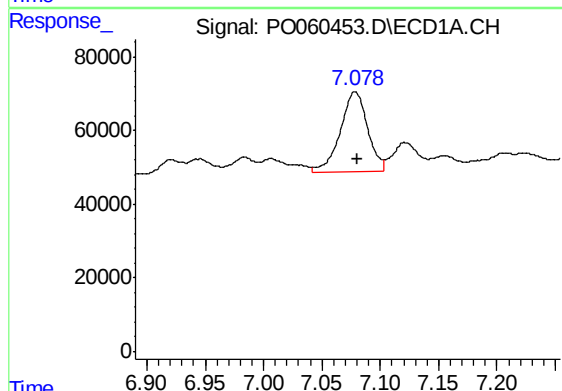


#32 AR-1260-2

R.T.: 7.078 min
Delta R.T.: -0.002 min
Response: 352282
Conc: 94.94 ng/ml m

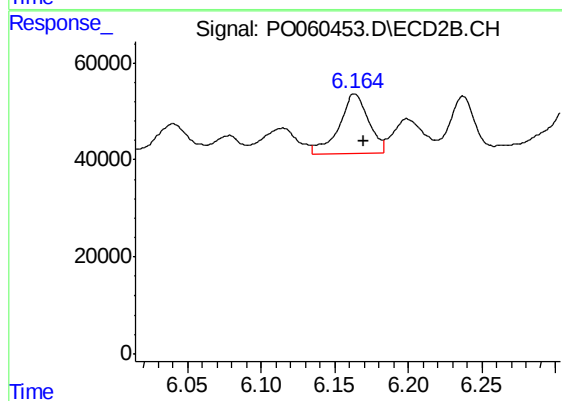

#32 AR-1260-2

R.T.: 6.164 min
Delta R.T.: -0.006 min
Response: 171594
Conc: 58.57 ng/ml

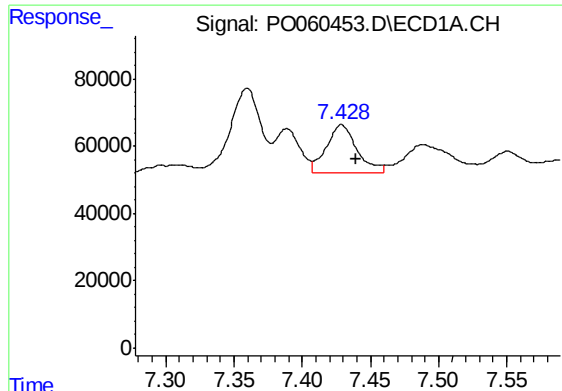


#33 AR-1260-3

R.T.: 7.428 min
Delta R.T.: -0.012 min
Response: 223164
Conc: 68.11 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-25-COMP


Manual Integrations
APPROVED

Ankita
9/9/2019 12:16:15 PM

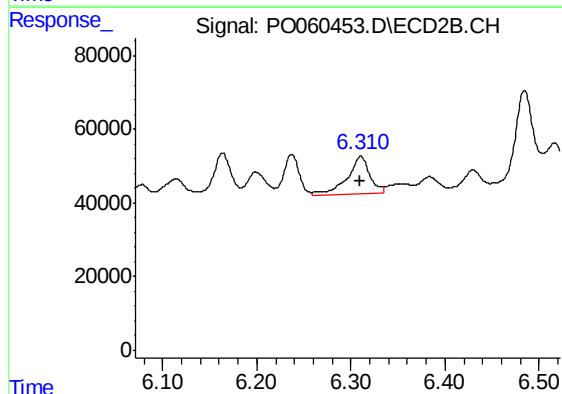


#33 AR-1260-3

R.T.: 6.311 min
Delta R.T.: 0.000 min
Response: 170723
Conc: 64.44 ng/ml

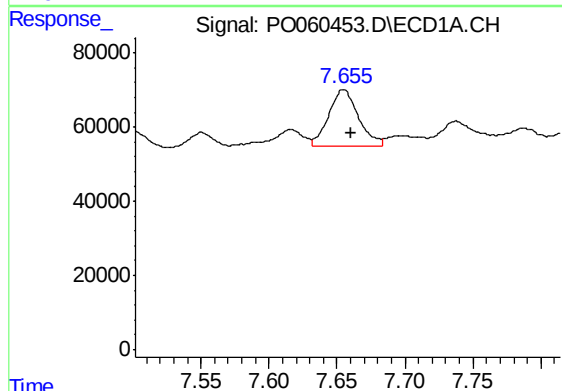


#34 AR-1260-4

R.T.: 7.655 min
Delta R.T.: -0.005 min
Response: 228332
Conc: 74.34 ng/ml m

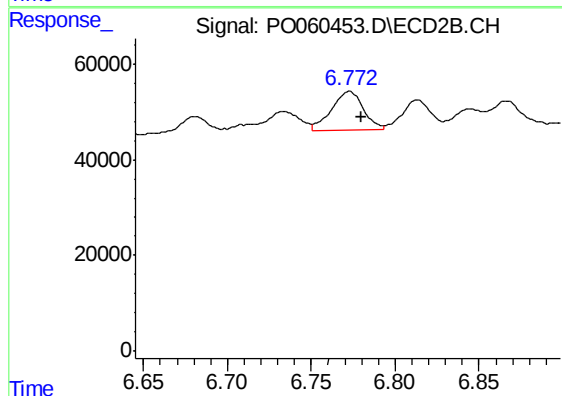

#34 AR-1260-4

R.T.: 6.773 min
Delta R.T.: -0.007 min
Response: 108862
Conc: 48.11 ng/ml

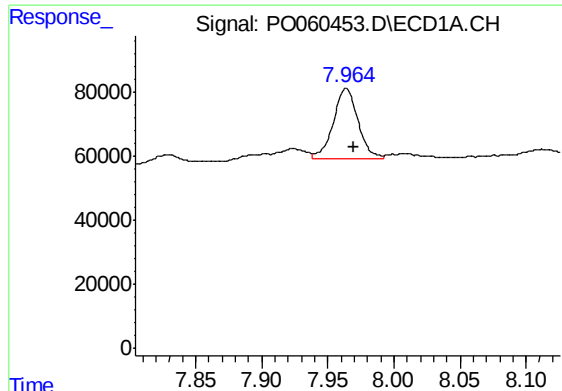


#35 AR-1260-5

R.T.: 7.964 min
Delta R.T.: -0.006 min
Response: 289913
Conc: 40.94 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-25-COMP

Manual Integrations
APPROVED

Ankita
9/9/2019 12:16:15 PM

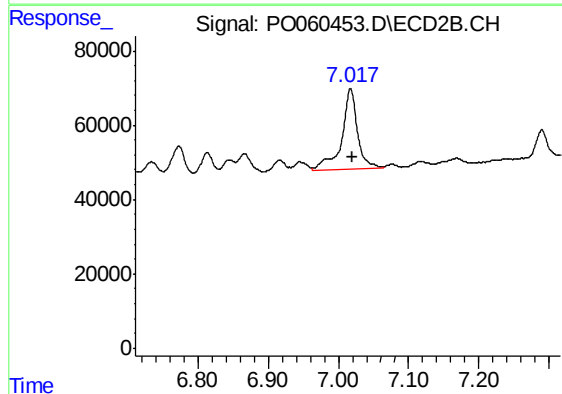

#35 AR-1260-5

R.T.: 7.017 min
Delta R.T.: -0.003 min
Response: 345394
Conc: 62.76 ng/ml