

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090619\
 Data File : P0060455.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Sep 2019 22:28
 Operator : SM/AJ
 Sample : K4692-16
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-27-COMP

Manual Integrations
 APPROVED

Ankita
 9/9/2019 12:16:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 23:10:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 06 17:58:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.102	3.486	1105724	825456	31.581	22.932 #
2)	SA Decachlor...	9.546	8.333	520276	396417	9.780	9.832m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090619\
Data File : PO060455.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Sep 2019 22:28
Operator : SM/AJ
Sample : K4692-16
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-27-COMP


Manual Integrations
APPROVED

Ankita
9/9/2019 12:16:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 23:10:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 06 17:58:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

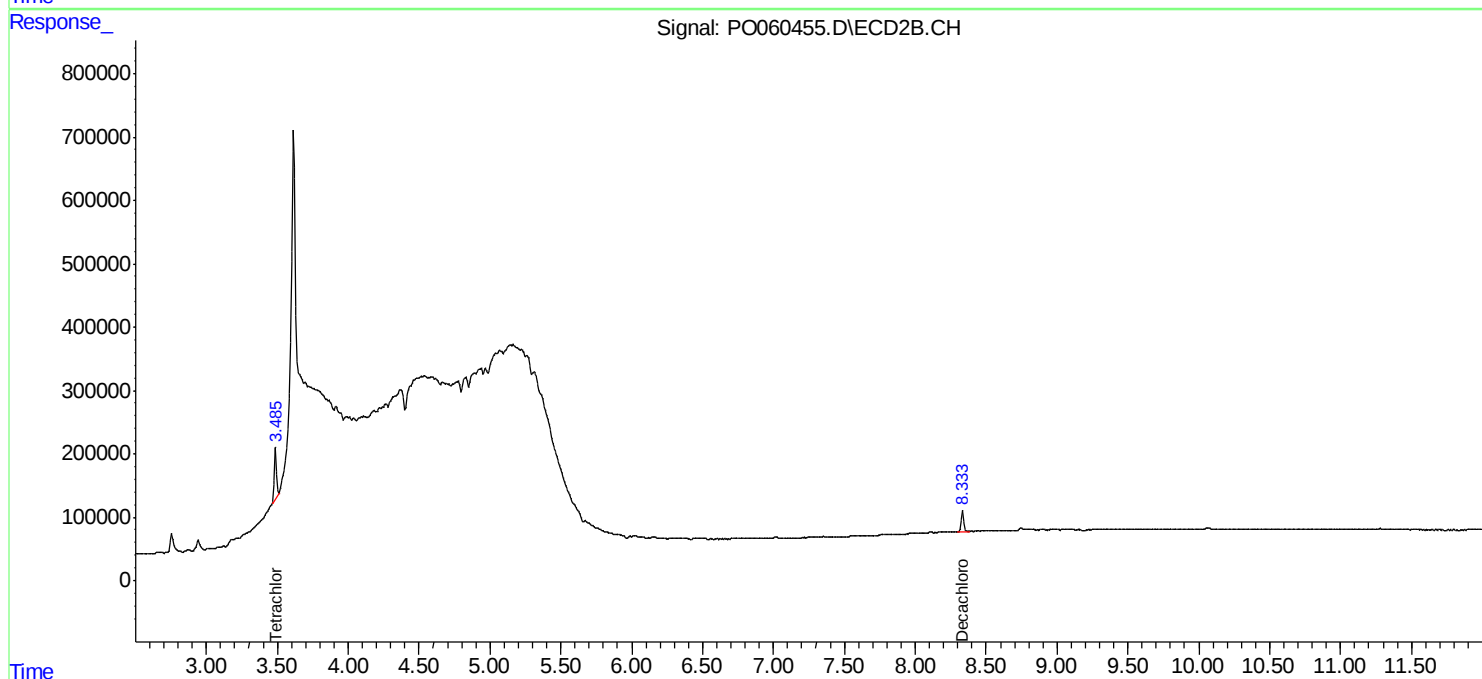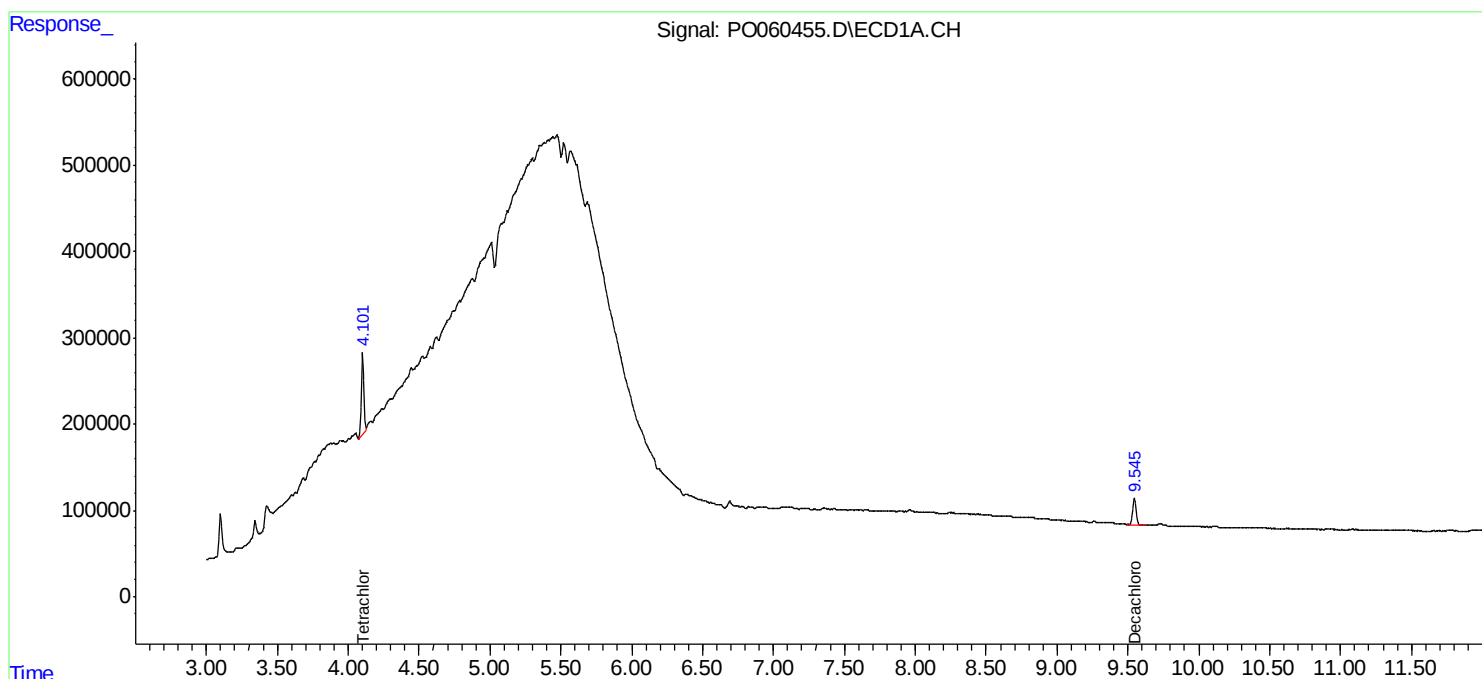

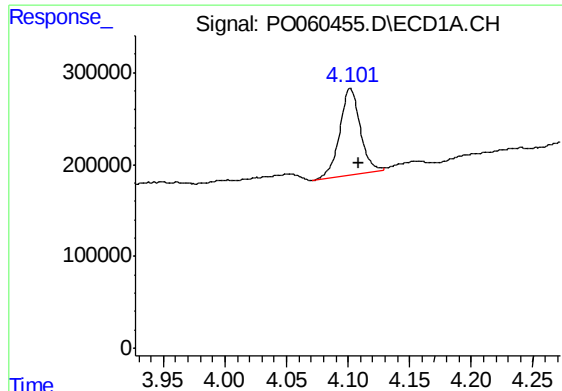


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: -0.007 min
Response: 1105724
Conc: 31.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-27-COMP


Manual Integrations
APPROVED

Ankita
9/9/2019 12:16:21 PM

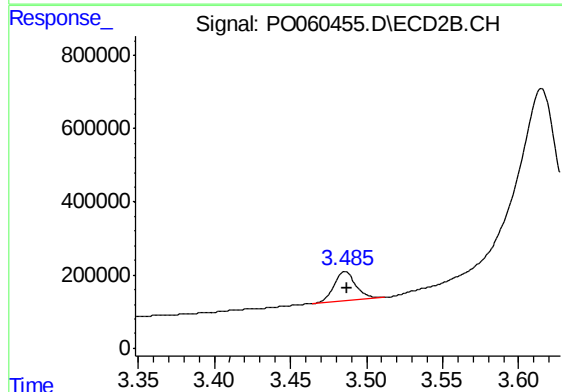


#1 Tetrachloro-m-xylene

R.T.: 3.486 min
Delta R.T.: -0.001 min
Response: 825456
Conc: 22.93 ng/ml

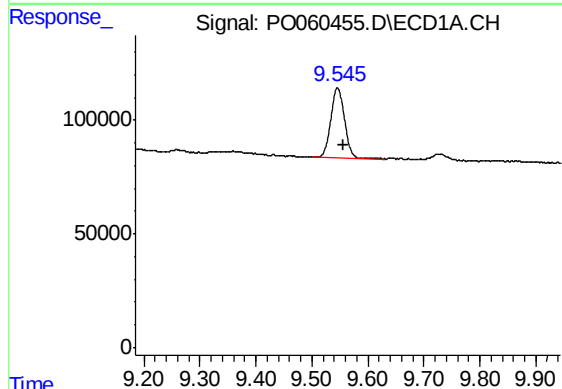

#2 Decachlorobiphenyl

R.T.: 9.546 min
Delta R.T.: -0.011 min
Response: 520276
Conc: 9.78 ng/ml

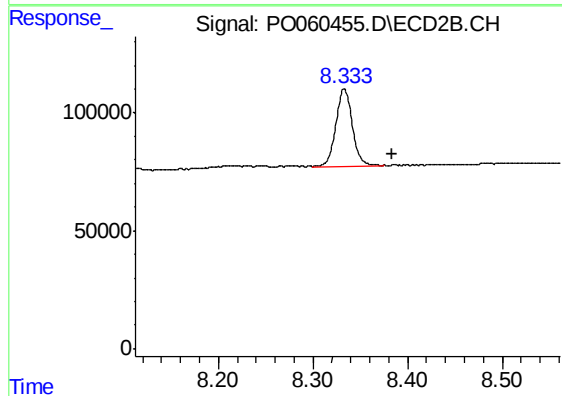

#2 Decachlorobiphenyl

R.T.: 8.333 min
Delta R.T.: -0.051 min
Response: 396417
Conc: 9.83 ng/ml m