

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090619\
 Data File : P0060458.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Sep 2019 00:05
 Operator : SM/AJ
 Sample : PB122844BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB122844BL

Manual Integrations
 APPROVED

Ankita
 9/9/2019 12:16:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 00:42:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 06 17:58:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.101	3.485	1143274	884001	32.653	24.559
2) SA Decachlor...	9.547	8.333	1224167	963271	23.011	23.890m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090619\
Data File : PO060458.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Sep 2019 00:05
Operator : SM/AJ
Sample : PB122844BL
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB122844BL


Manual Integrations
APPROVED

Ankita
9/9/2019 12:16:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 00:42:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 06 17:58:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

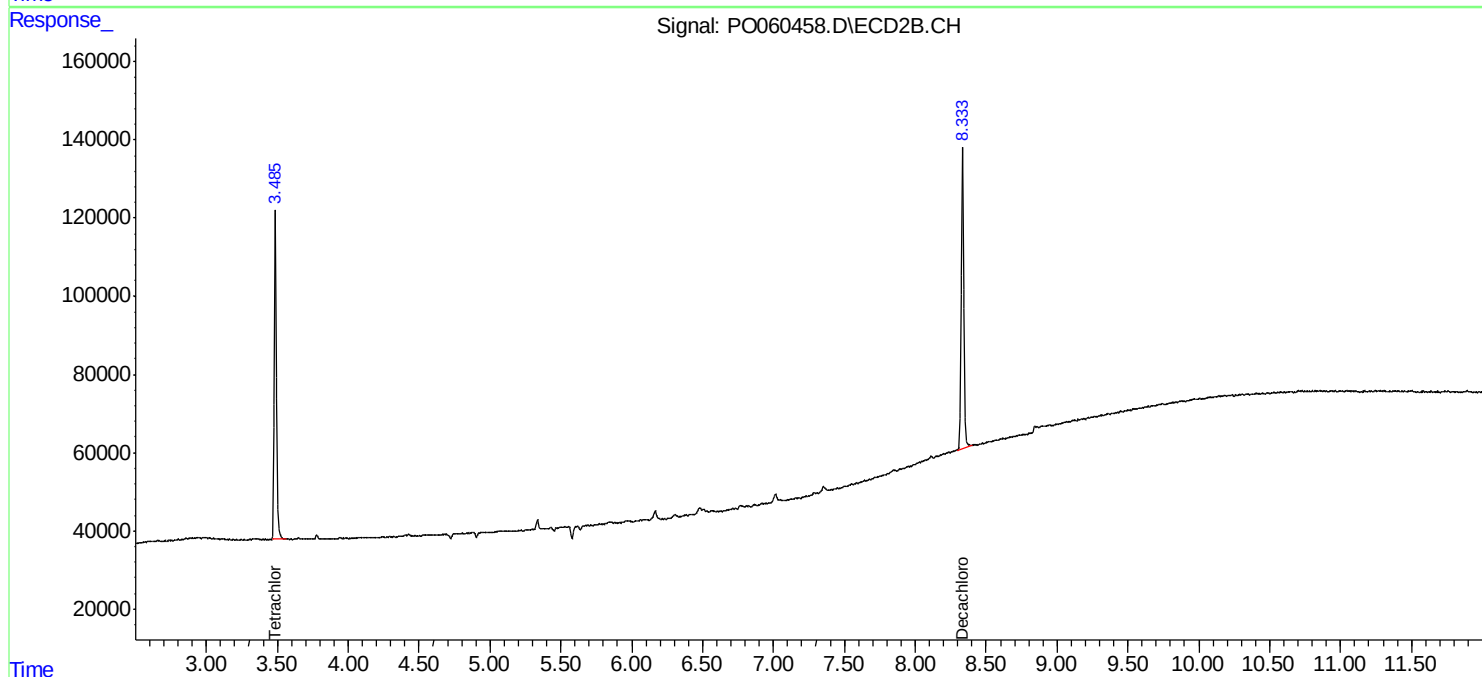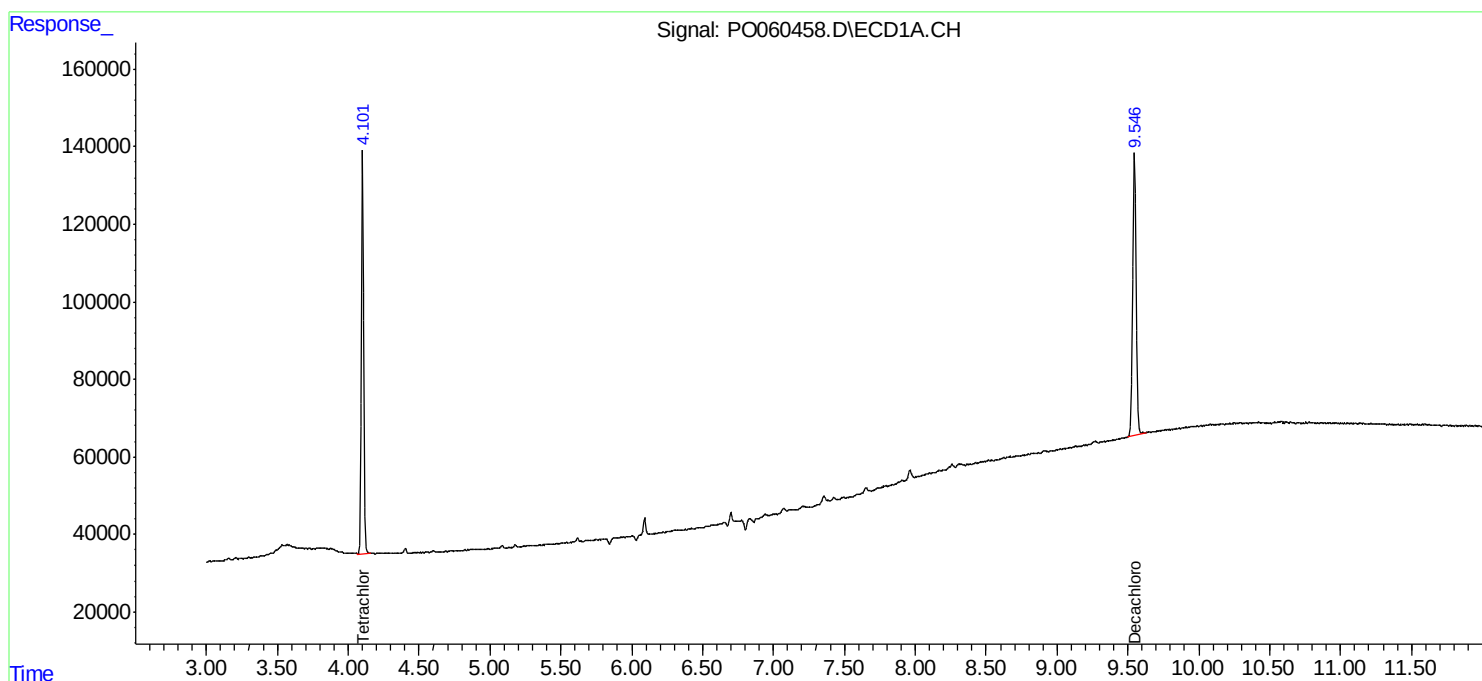

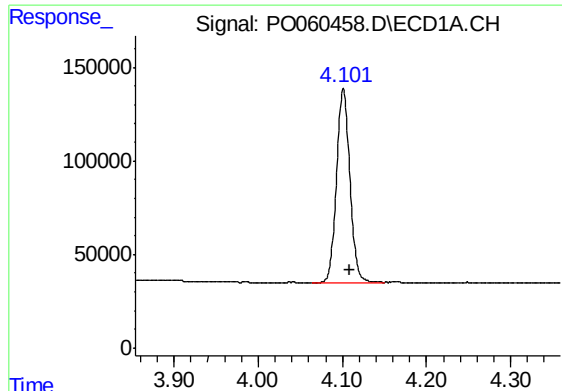


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: -0.008 min
Response: 1143274
Conc: 32.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB122844BL


Manual Integrations
APPROVED

Ankita
9/9/2019 12:16:25 PM

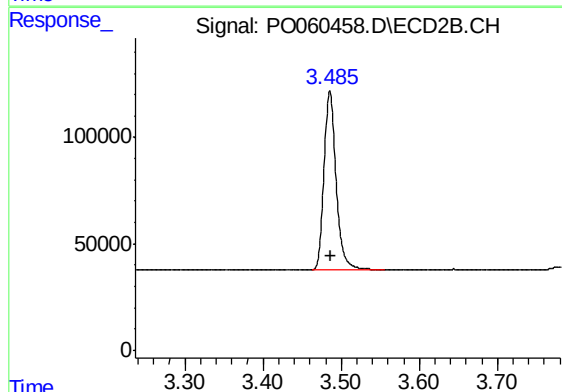


#1 Tetrachloro-m-xylene

R.T.: 3.485 min
Delta R.T.: -0.002 min
Response: 884001
Conc: 24.56 ng/ml

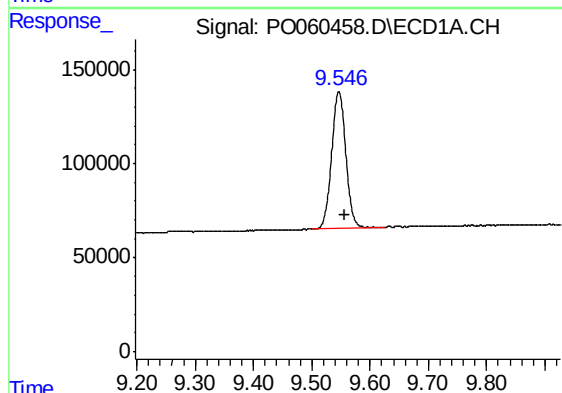

#2 Decachlorobiphenyl

R.T.: 9.547 min
Delta R.T.: -0.010 min
Response: 1224167
Conc: 23.01 ng/ml

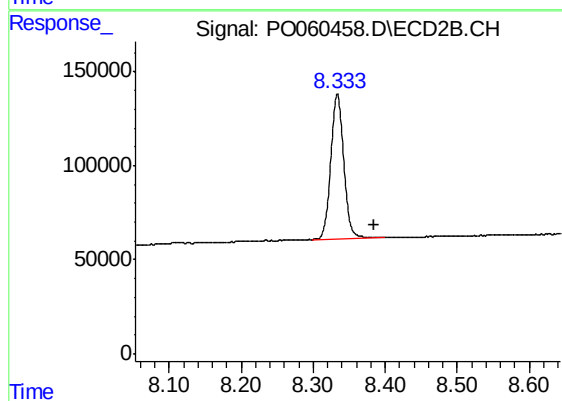

#2 Decachlorobiphenyl

R.T.: 8.333 min
Delta R.T.: -0.051 min
Response: 963271
Conc: 23.89 ng/ml m