

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090619\
 Data File : P0060460.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Sep 2019 00:37
 Operator : SM/AJ
 Sample : K4656-01
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AU-06-090519

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 04:35:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 06 17:58:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.102	3.486	1373900	1049198	39.240	29.148 #
2)	SA Decachlor...	9.547	8.334	1164475	895128	21.889	22.200

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090619\
Data File : PO060460.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Sep 2019 00:37
Operator : SM/AJ
Sample : K4656-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AU-06-090519

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 04:35:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 06 17:58:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

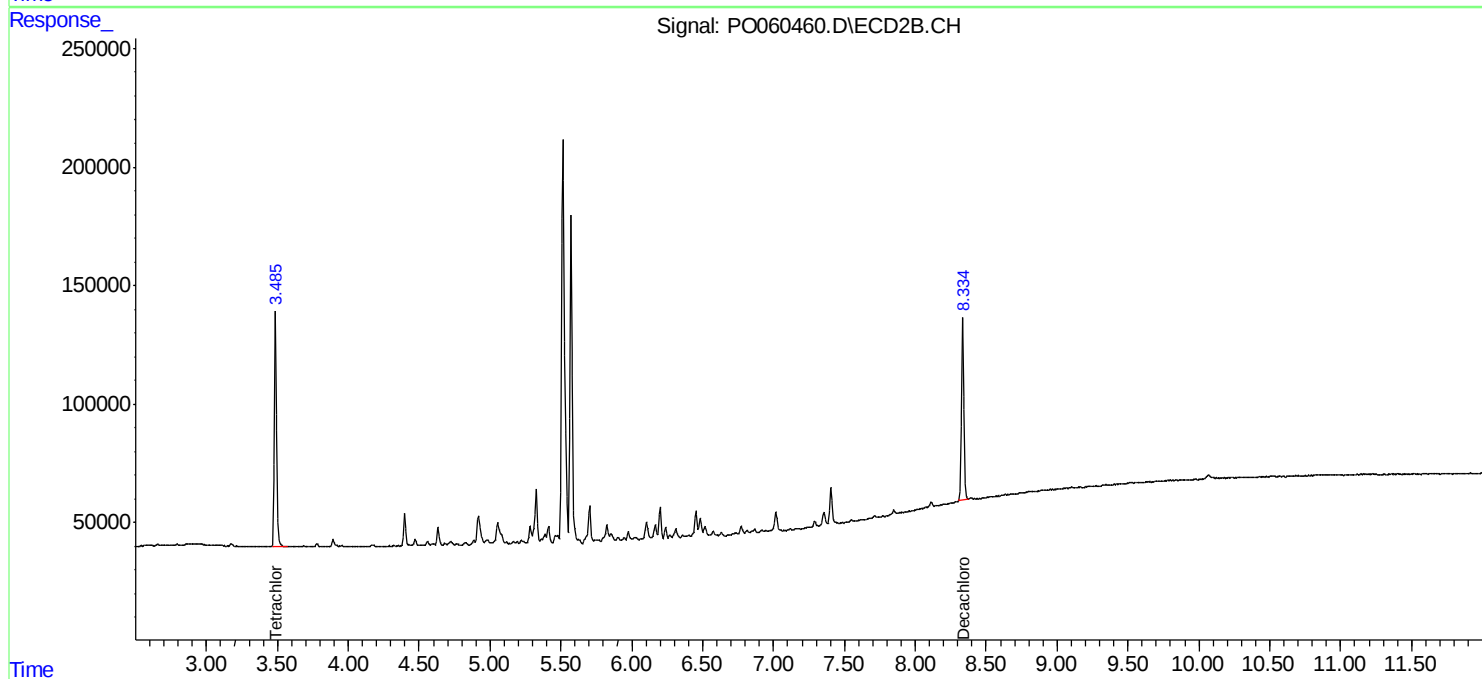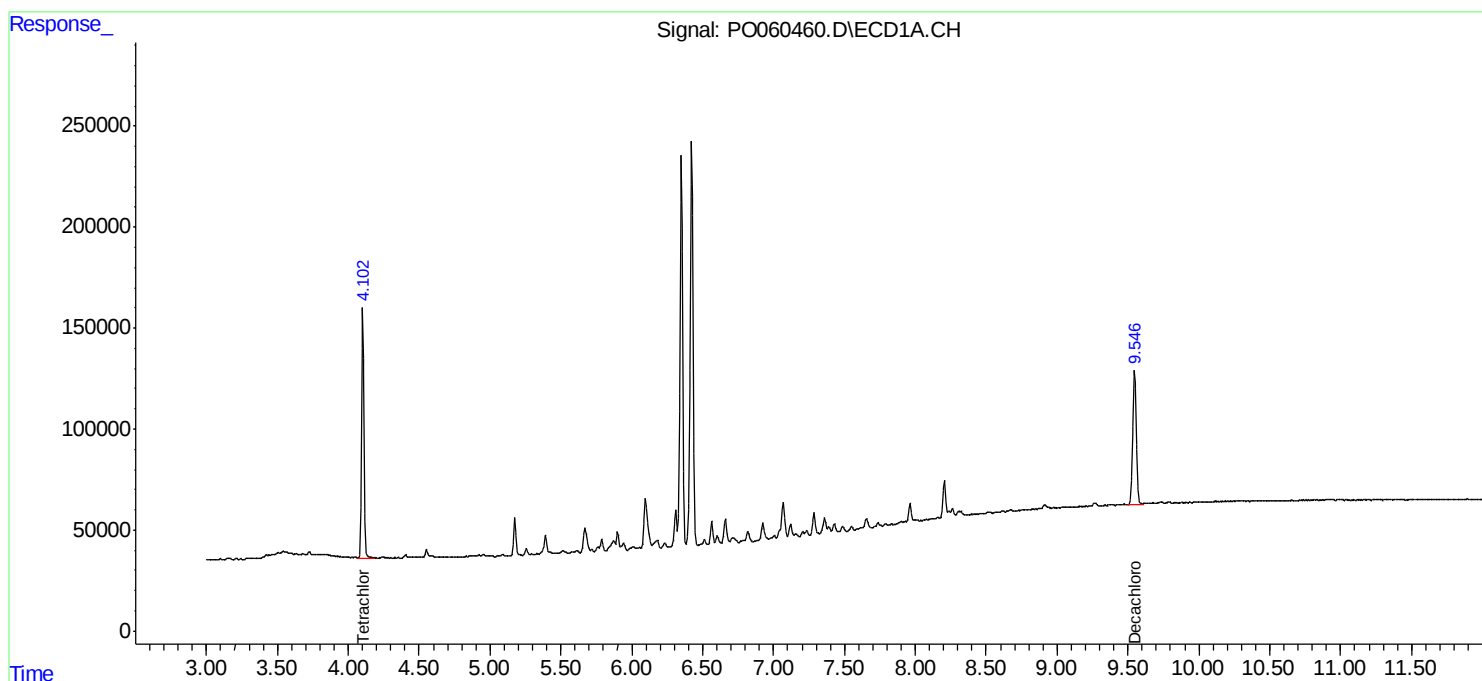


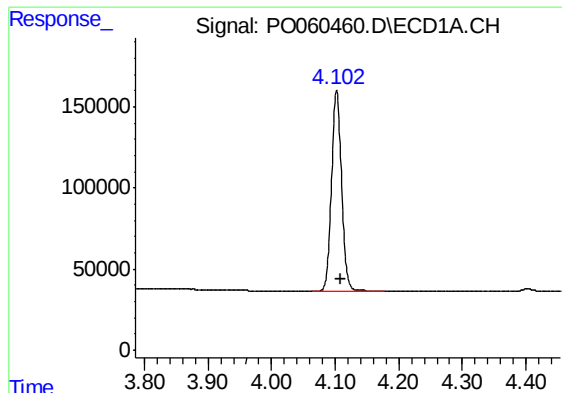

#1 Tetrachloro-m-xylene


R.T.: 4.102 min
Delta R.T.: -0.007 min
Response: 1373900
Conc: 39.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
AU-06-090519

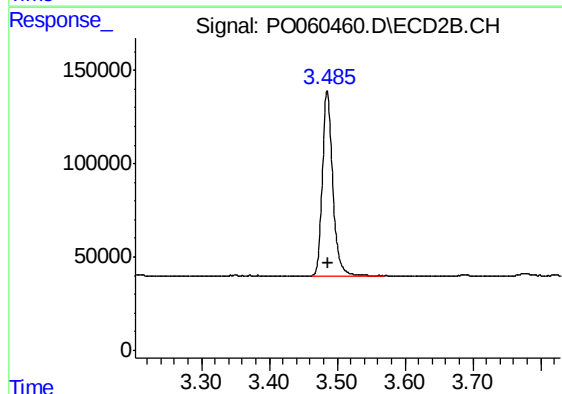


#1 Tetrachloro-m-xylene

R.T.: 3.486 min
Delta R.T.: -0.001 min
Response: 1049198
Conc: 29.15 ng/ml

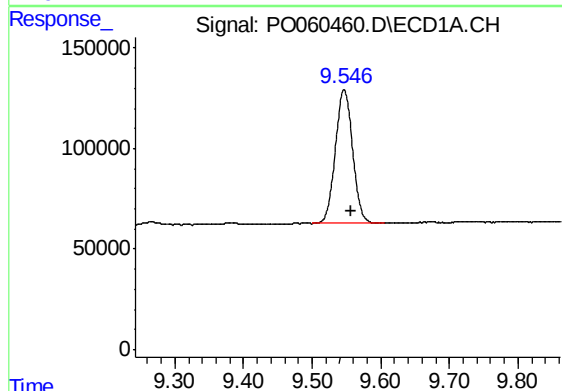

#2 Decachlorobiphenyl

R.T.: 9.547 min
Delta R.T.: -0.010 min
Response: 1164475
Conc: 21.89 ng/ml

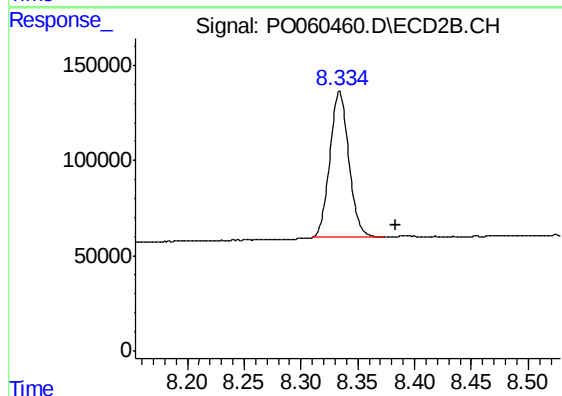

#2 Decachlorobiphenyl

R.T.: 8.334 min
Delta R.T.: -0.050 min
Response: 895128
Conc: 22.20 ng/ml