

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090619\
 Data File : P0060472.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Sep 2019 3:51
 Operator : SM/AJ
 Sample : K4716-03
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-20-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 04:40:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 06 17:58:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.103	3.486	1456468	1200436	41.598	33.349
2) SA Decachlor...	9.548	8.335	1000407	794712	18.805	19.710

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090619\
Data File : PO060472.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Sep 2019 3:51
Operator : SM/AJ
Sample : K4716-03
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-20-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 04:40:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 06 17:58:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

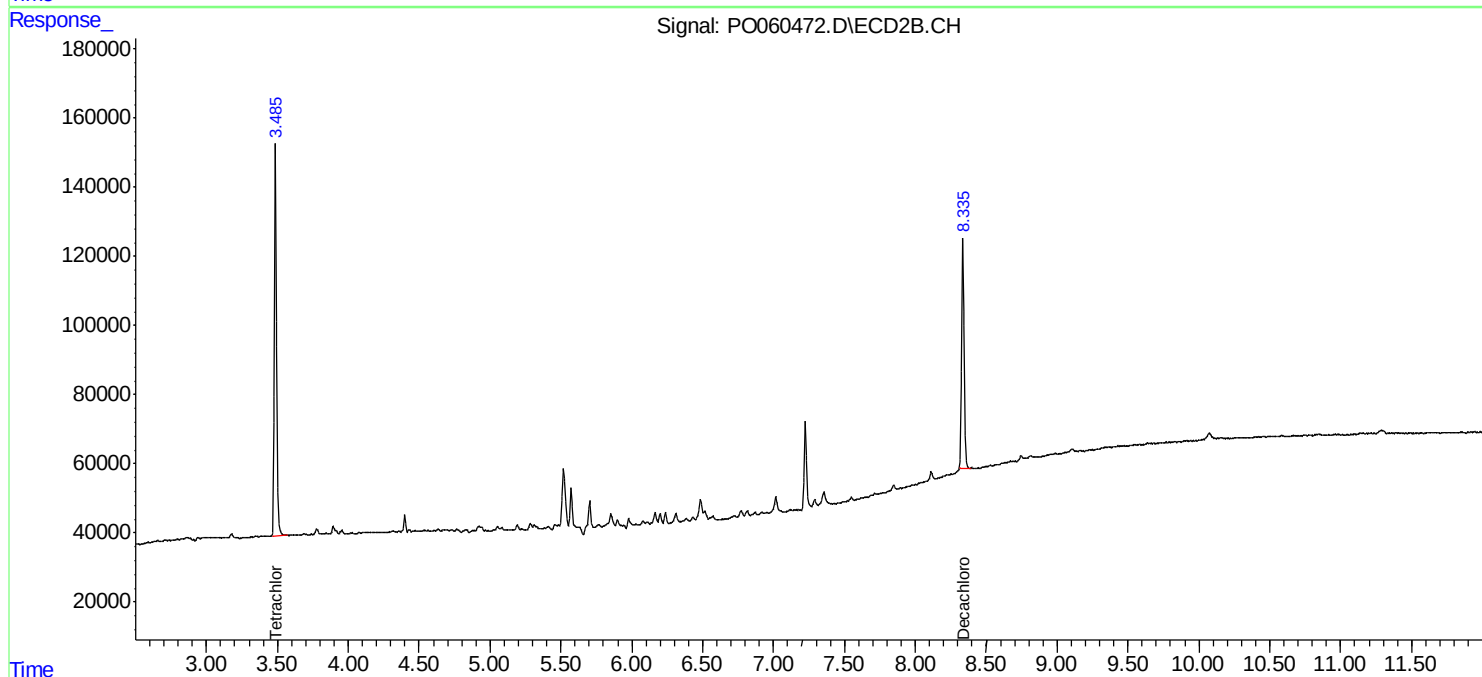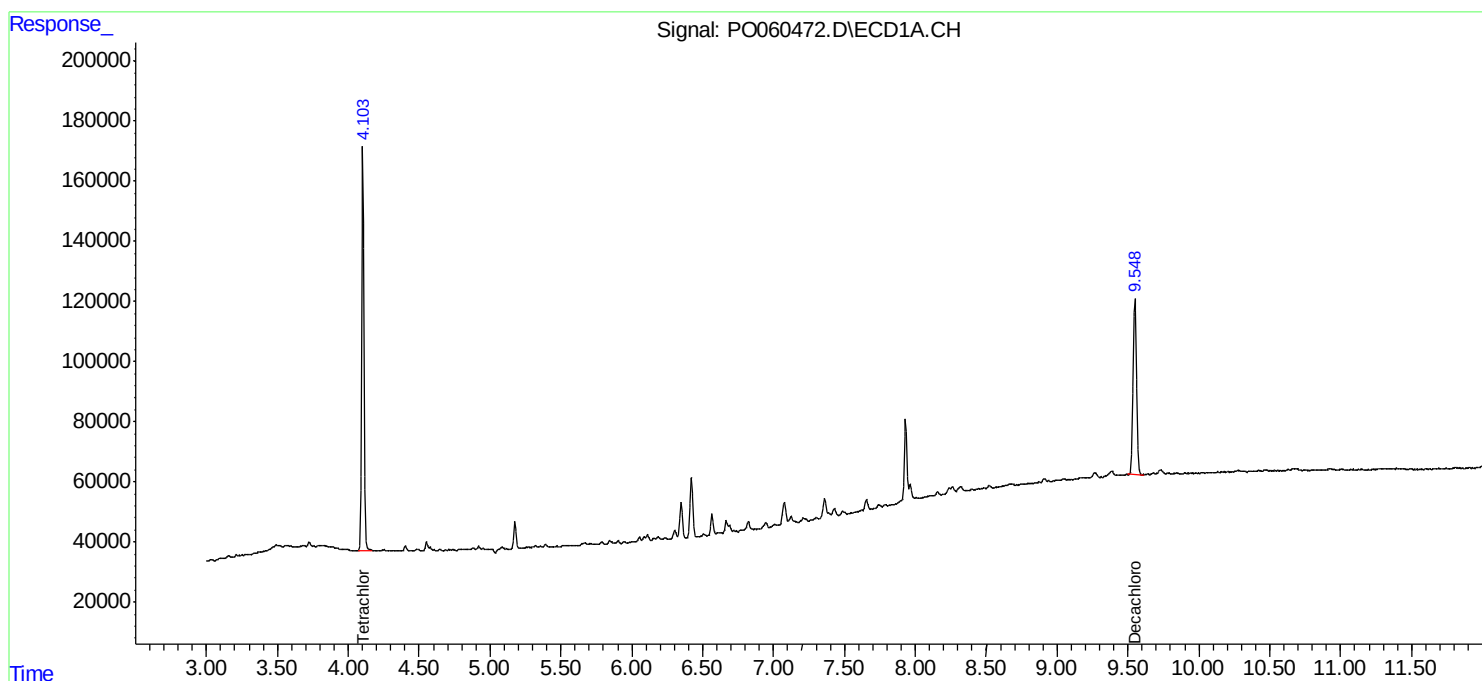


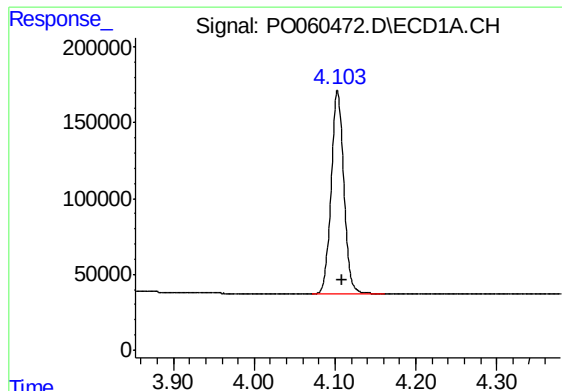

#1 Tetrachloro-m-xylene


R.T.: 4.103 min
Delta R.T.: -0.006 min
Response: 1456468
Conc: 41.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-20-S

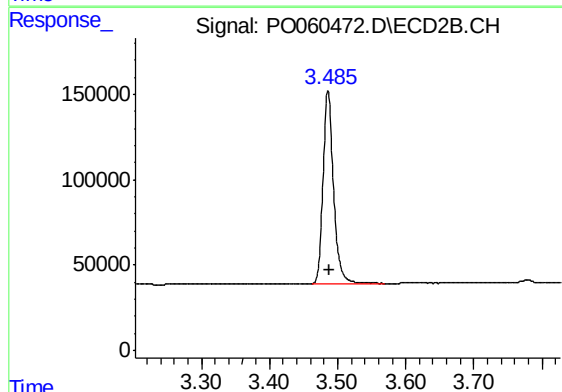


#1 Tetrachloro-m-xylene

R.T.: 3.486 min
Delta R.T.: -0.001 min
Response: 1200436
Conc: 33.35 ng/ml

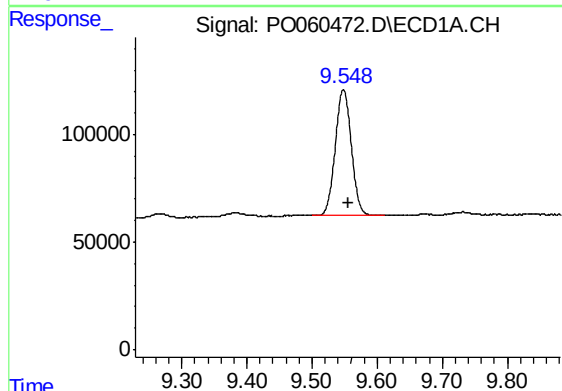

#2 Decachlorobiphenyl

R.T.: 9.548 min
Delta R.T.: -0.009 min
Response: 1000407
Conc: 18.80 ng/ml

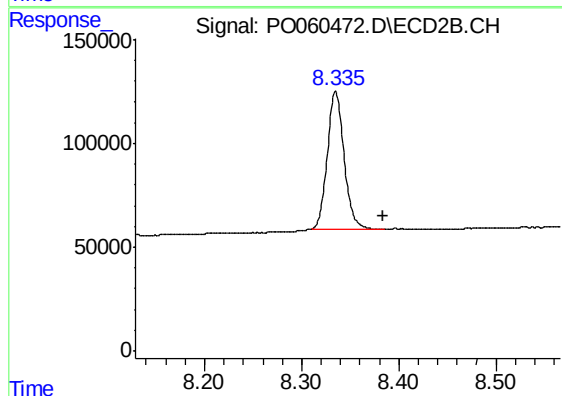

#2 Decachlorobiphenyl

R.T.: 8.335 min
Delta R.T.: -0.049 min
Response: 794712
Conc: 19.71 ng/ml