

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090622\
 Data File : P0089312.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2022 17:20
 Operator : YP/AJ
 Sample : N4498-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-02-090222

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/07/2022
 Supervised By :Ankita Jodhani 09/07/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 18:19:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 29 17:48:02 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.428	3.586	79416953	23159136	21.180	23.993
2) SA Decachlor...	10.255	8.567	40411652	16621172	17.553	18.796m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090622\
Data File : PO089312.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2022 17:20
Operator : YP/AJ
Sample : N4498-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CL-02-090222


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/07/2022
Supervised By :Ankita Jodhani 09/07/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 18:19:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082922.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 29 17:48:02 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

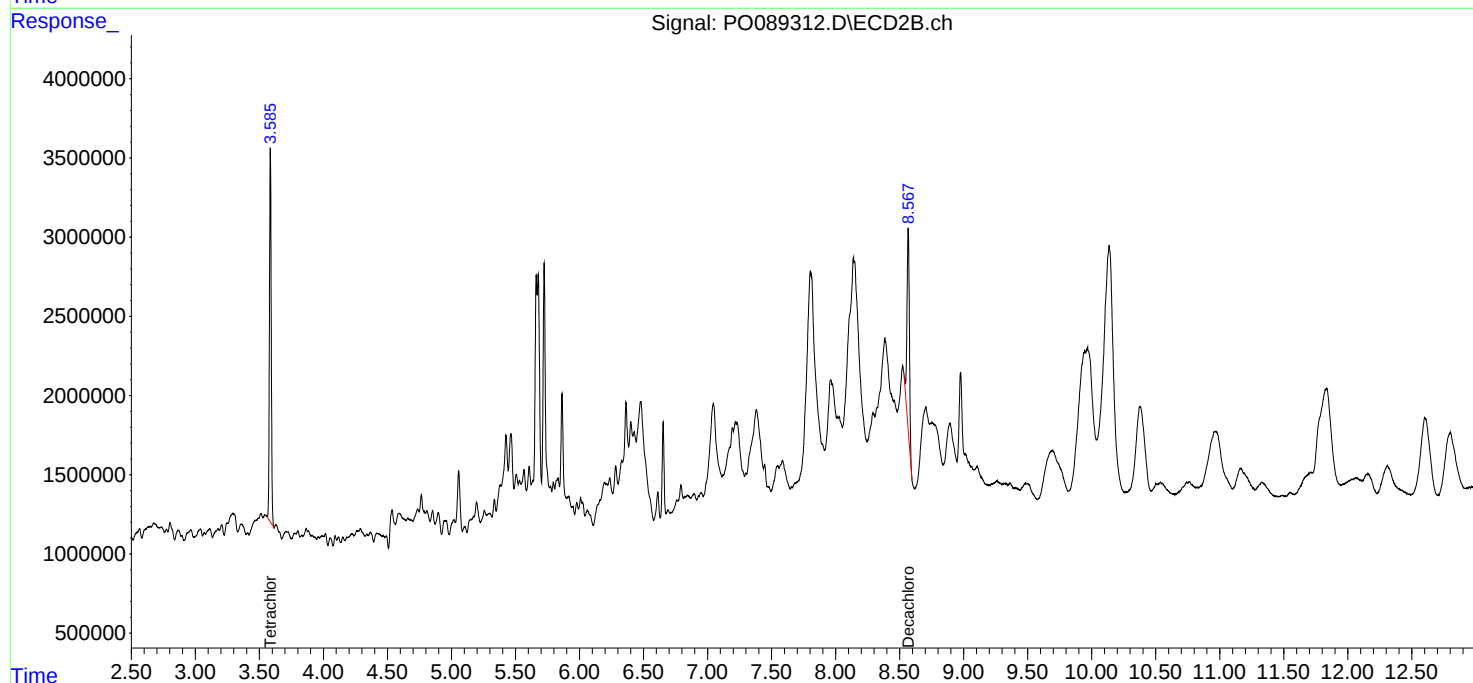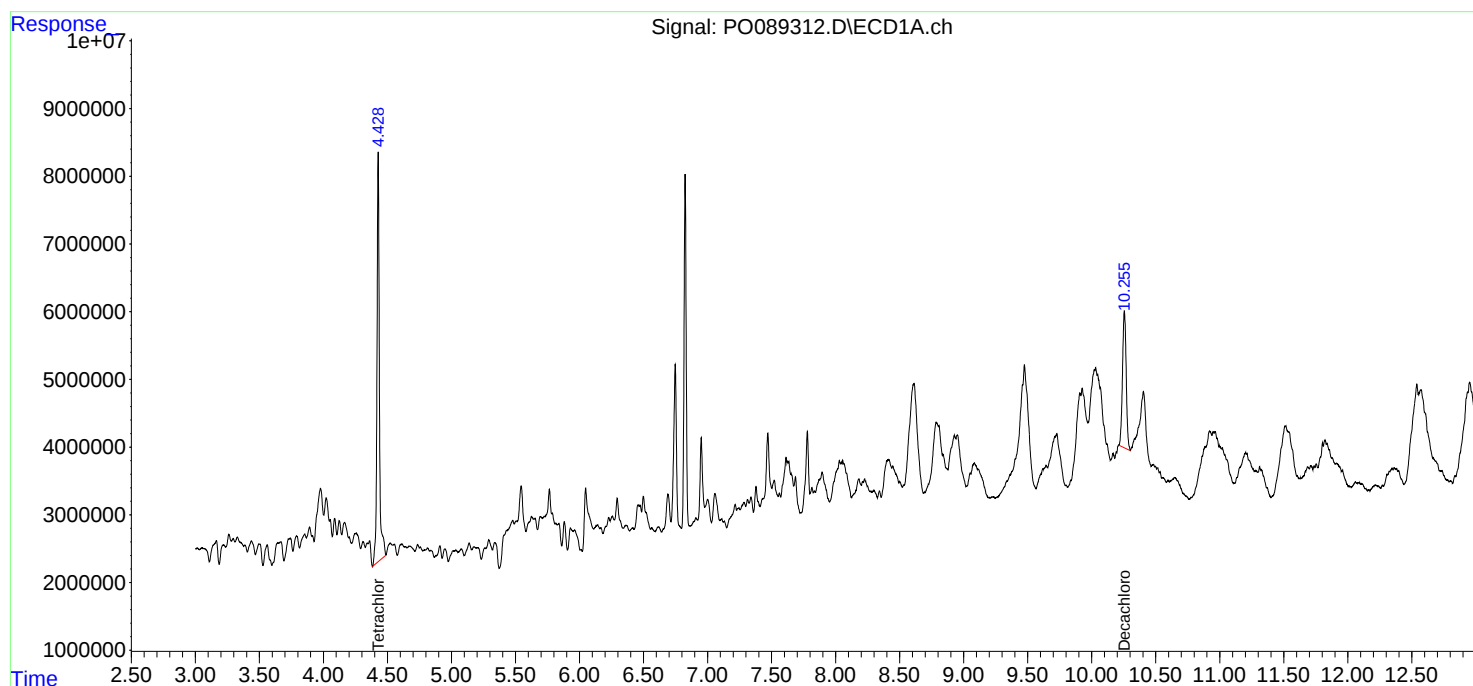

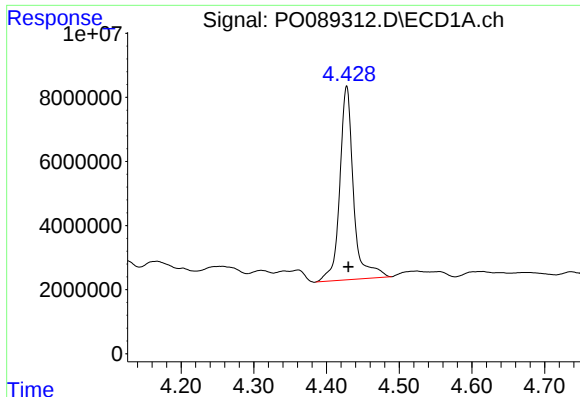


#1 Tetrachloro-m-xylene

R.T.: 4.428 min
Delta R.T.: -0.002 min
Response: 79416953
Conc: 21.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
CL-02-090222


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/07/2022
Supervised By :Ankita Jodhani 09/07/2022

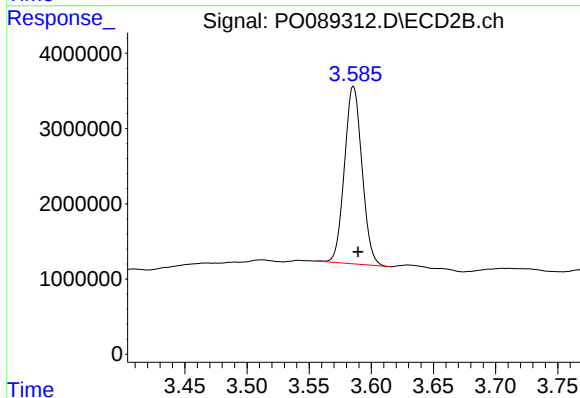


#1 Tetrachloro-m-xylene

R.T.: 3.586 min
Delta R.T.: -0.004 min
Response: 23159136
Conc: 23.99 ng/ml

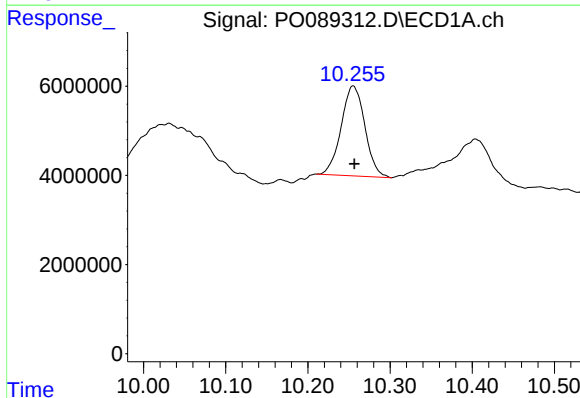

#2 Decachlorobiphenyl

R.T.: 10.255 min
Delta R.T.: -0.002 min
Response: 40411652
Conc: 17.55 ng/ml

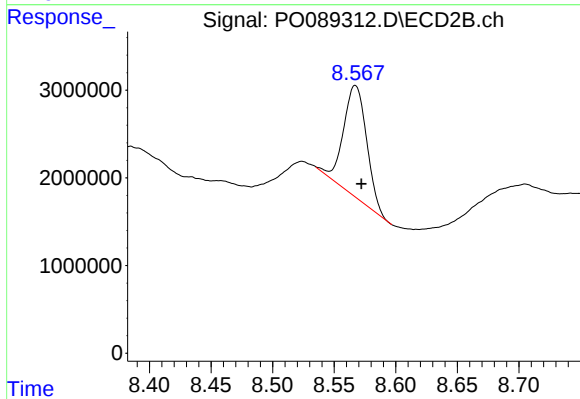

#2 Decachlorobiphenyl

R.T.: 8.567 min
Delta R.T.: -0.005 min
Response: 16621172
Conc: 18.80 ng/ml m