

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090718\
Data File : P0048851.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Sep 2018 19:18
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 23:03:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090418.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 06 03:44:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.459	3.529	3253949	3491287	26.968	22.336
2) SA Decachlor...	10.203	8.467	2820440	3299673	20.214	22.317

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090718\
Data File : P0048851.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Sep 2018 19:18
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 23:03:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090418.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 06 03:44:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

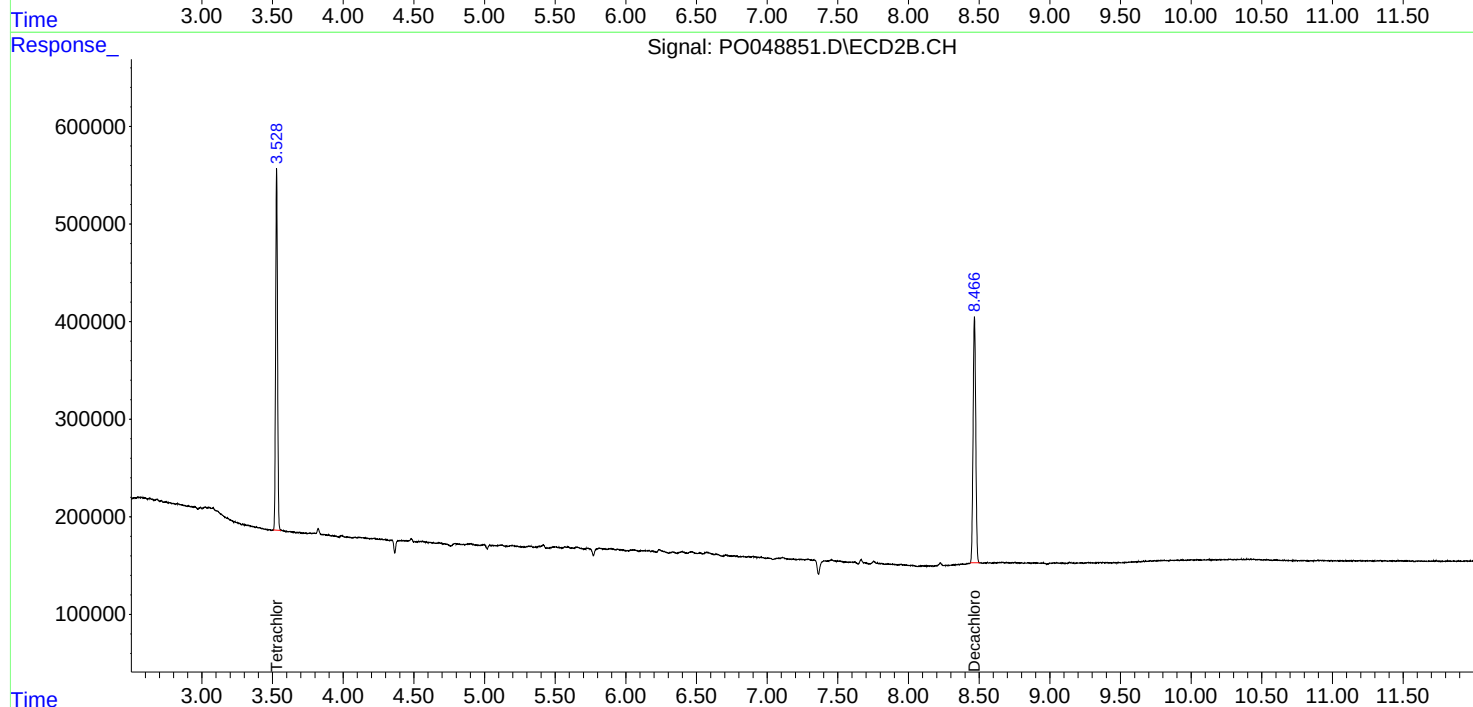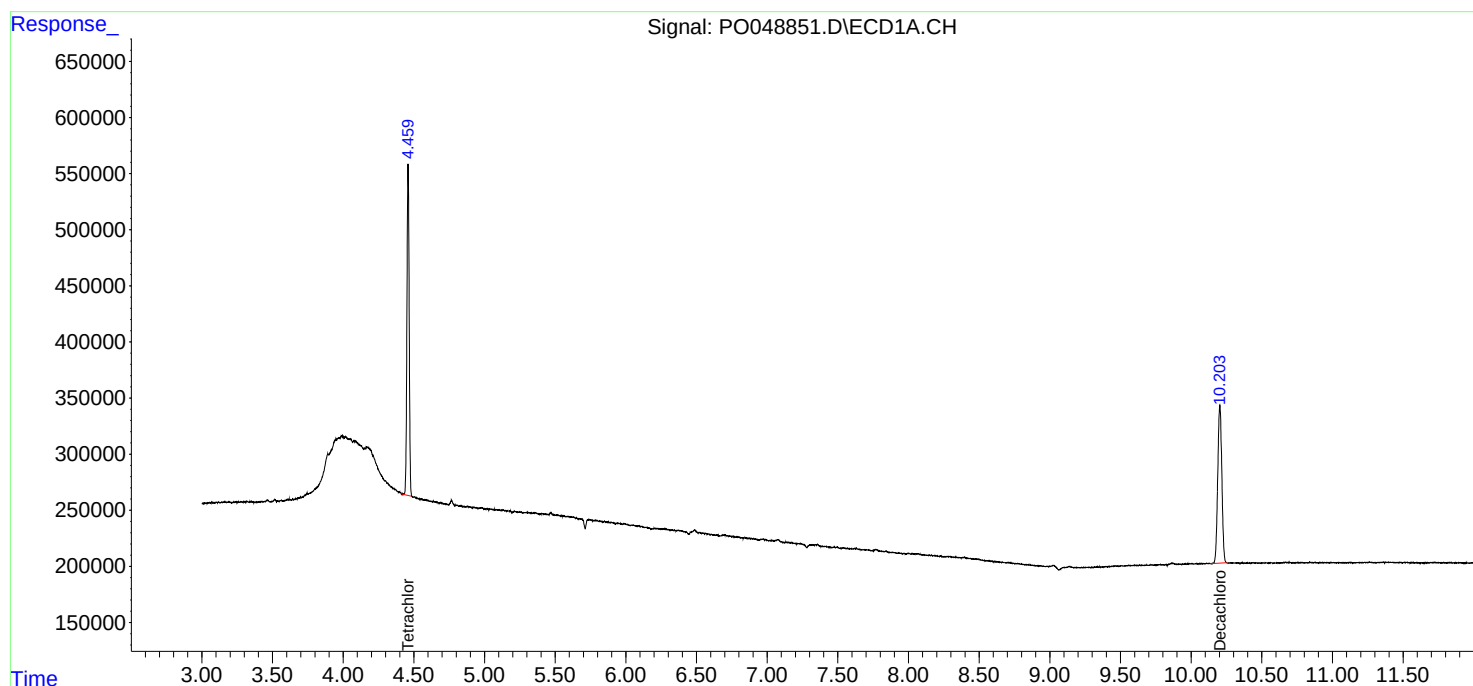


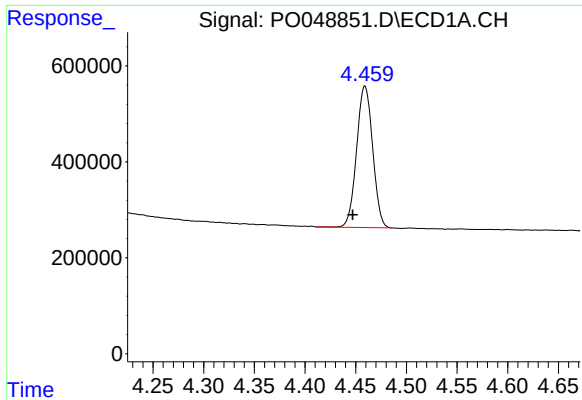

#1 Tetrachloro-m-xylene


R.T.: 4.459 min
Delta R.T.: 0.012 min
Response: 3253949
Conc: 26.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

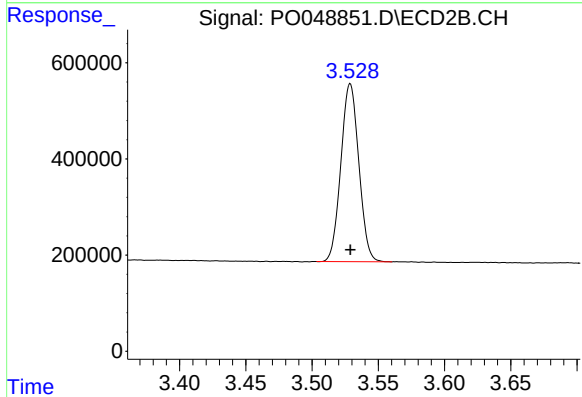


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: 0.000 min
Response: 3491287
Conc: 22.34 ng/ml

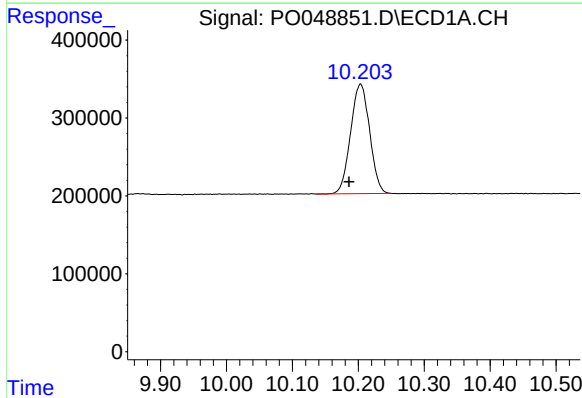

#2 Decachlorobiphenyl

R.T.: 10.203 min
Delta R.T.: 0.017 min
Response: 2820440
Conc: 20.21 ng/ml

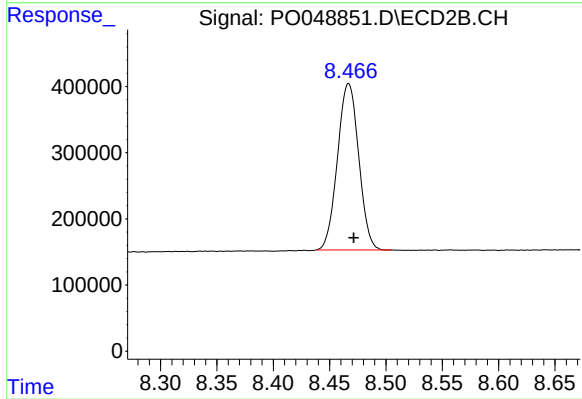

#2 Decachlorobiphenyl

R.T.: 8.467 min
Delta R.T.: -0.005 min
Response: 3299673
Conc: 22.32 ng/ml