

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090718\
Data File : P0048860.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Sep 2018 21:57
Operator : SM/SJ
Sample : J4809-05
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MS-SLUDGE-V24129

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 03:38:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090418.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 06 03:44:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.451	3.531	1709456	2442284	14.168	15.625
2) SA Decachlor...	10.176	8.468	840230	734483	6.022	4.968

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090718\
Data File : PO048860.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Sep 2018 21:57
Operator : SM/SJ
Sample : J4809-05
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MS-SLUDGE-V24129

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 03:38:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090418.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 06 03:44:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

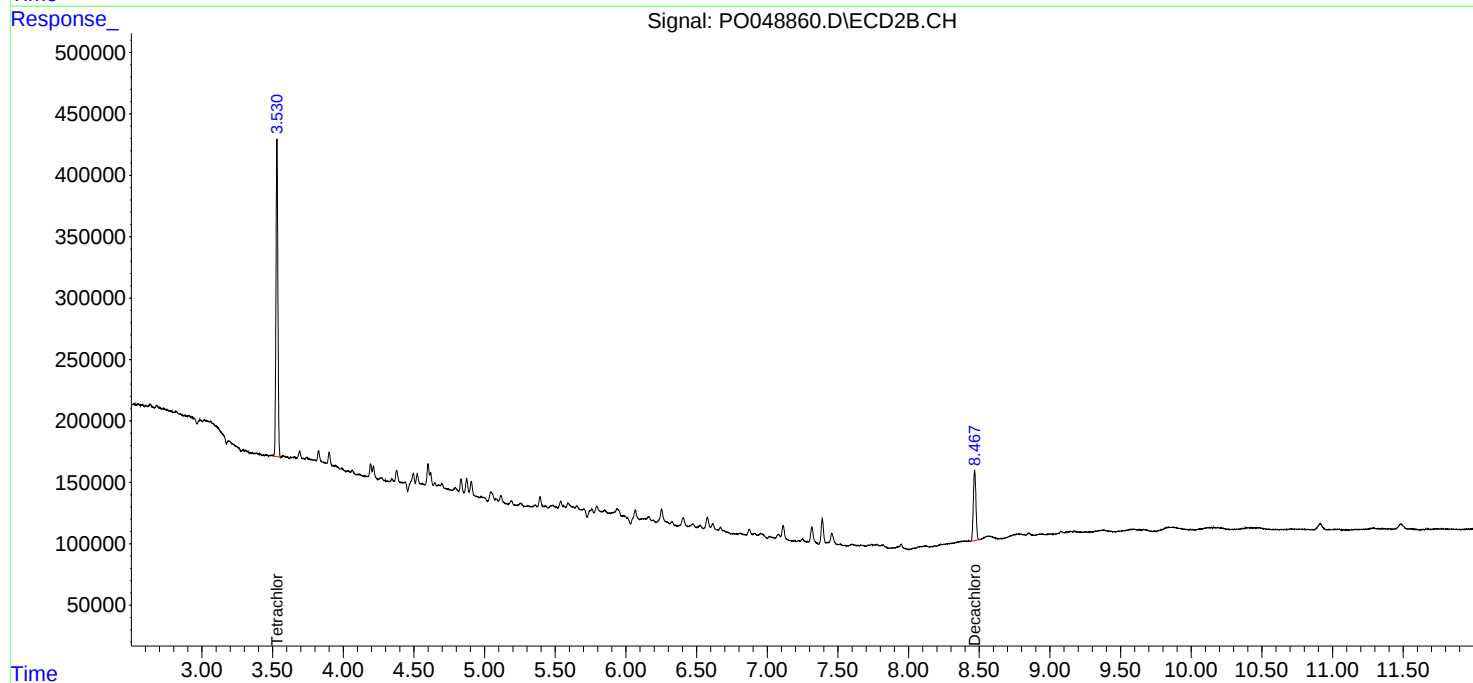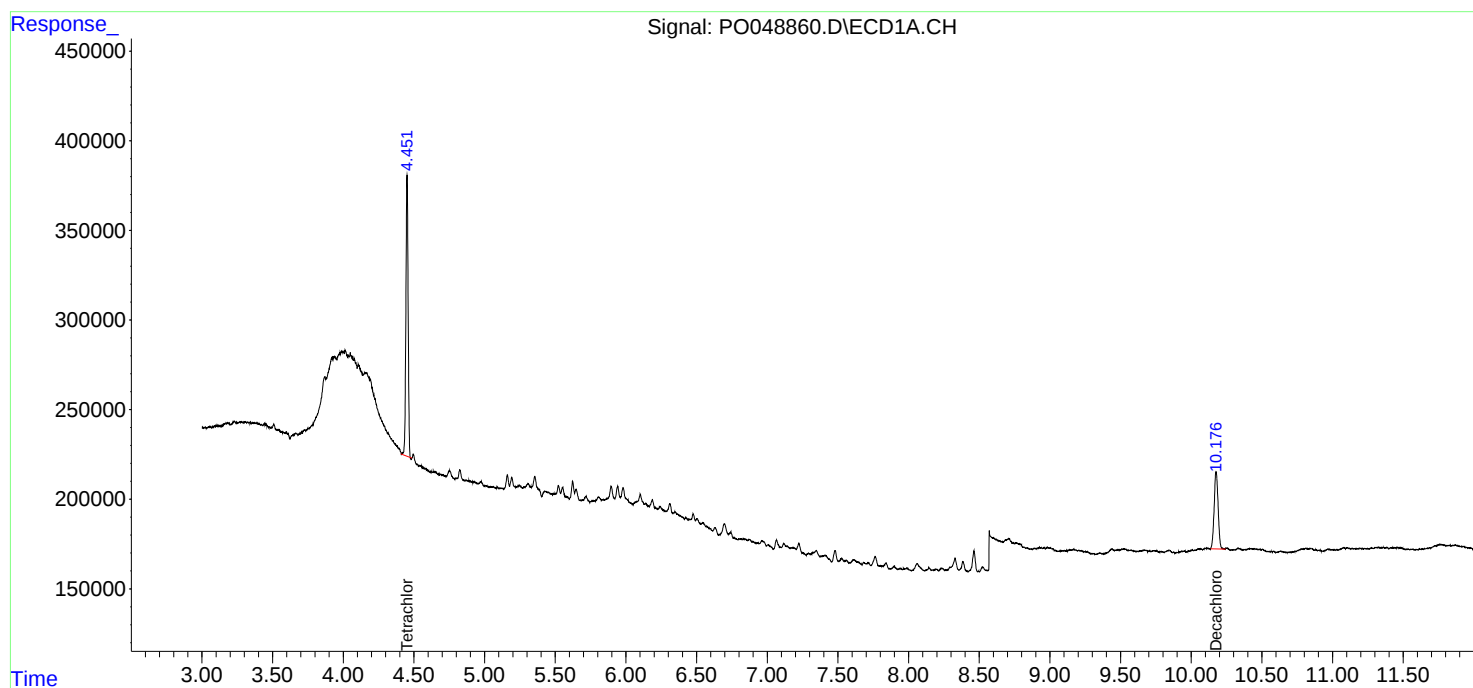


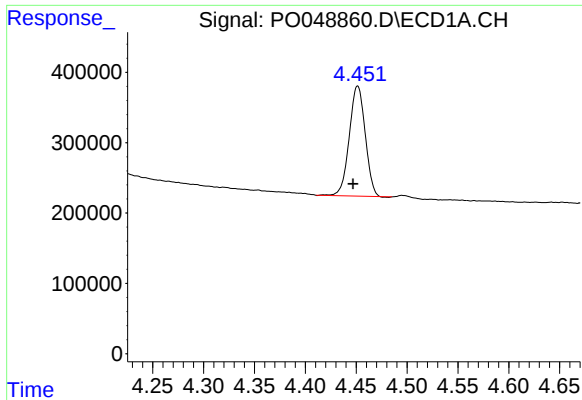

#1 Tetrachloro-m-xylene


R.T.: 4.451 min
Delta R.T.: 0.004 min
Response: 1709456
Conc: 14.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-SLUDGE-V24129

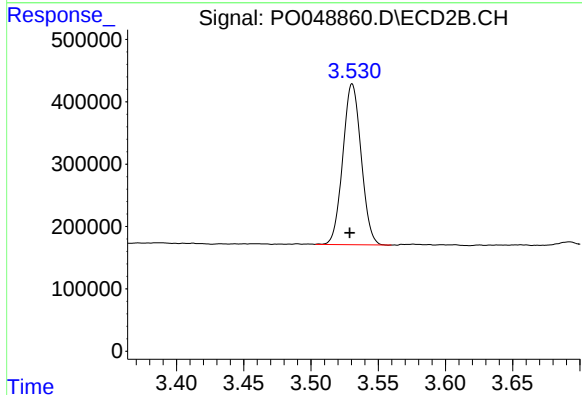


#1 Tetrachloro-m-xylene

R.T.: 3.531 min
Delta R.T.: 0.002 min
Response: 2442284
Conc: 15.63 ng/ml

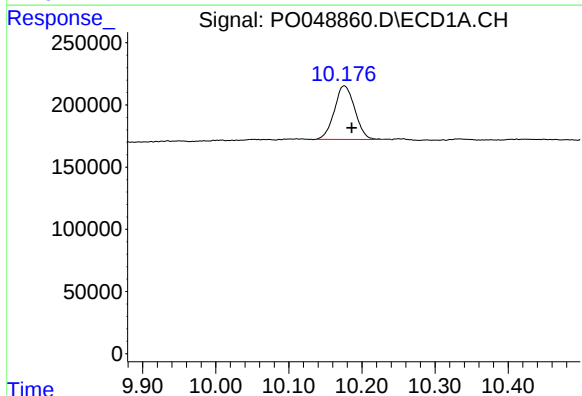

#2 Decachlorobiphenyl

R.T.: 10.176 min
Delta R.T.: -0.010 min
Response: 840230
Conc: 6.02 ng/ml

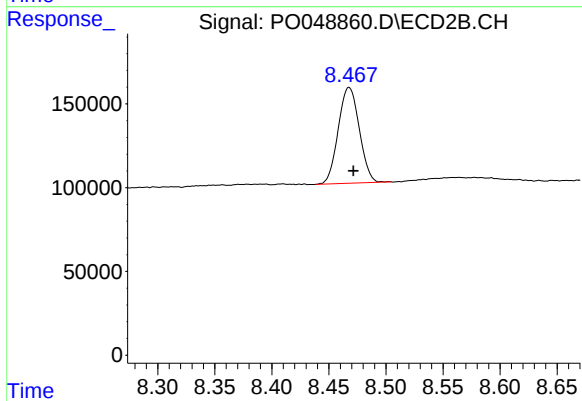

#2 Decachlorobiphenyl

R.T.: 8.468 min
Delta R.T.: -0.004 min
Response: 734483
Conc: 4.97 ng/ml