

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090719\
Data File : P0060501.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Sep 2019 3:56
Operator : SM/AJ
Sample : K4663-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OK-03-090519

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 01:15:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Sep 08 02:12:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.369	3.536	1102445	904523	26.570	29.449
2)	SA Decachlor...	10.037	8.428	904266	638251	17.142	17.242

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090719\
Data File : PO060501.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Sep 2019 3:56
Operator : SM/AJ
Sample : K4663-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OK-03-090519

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 01:15:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Sep 08 02:12:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

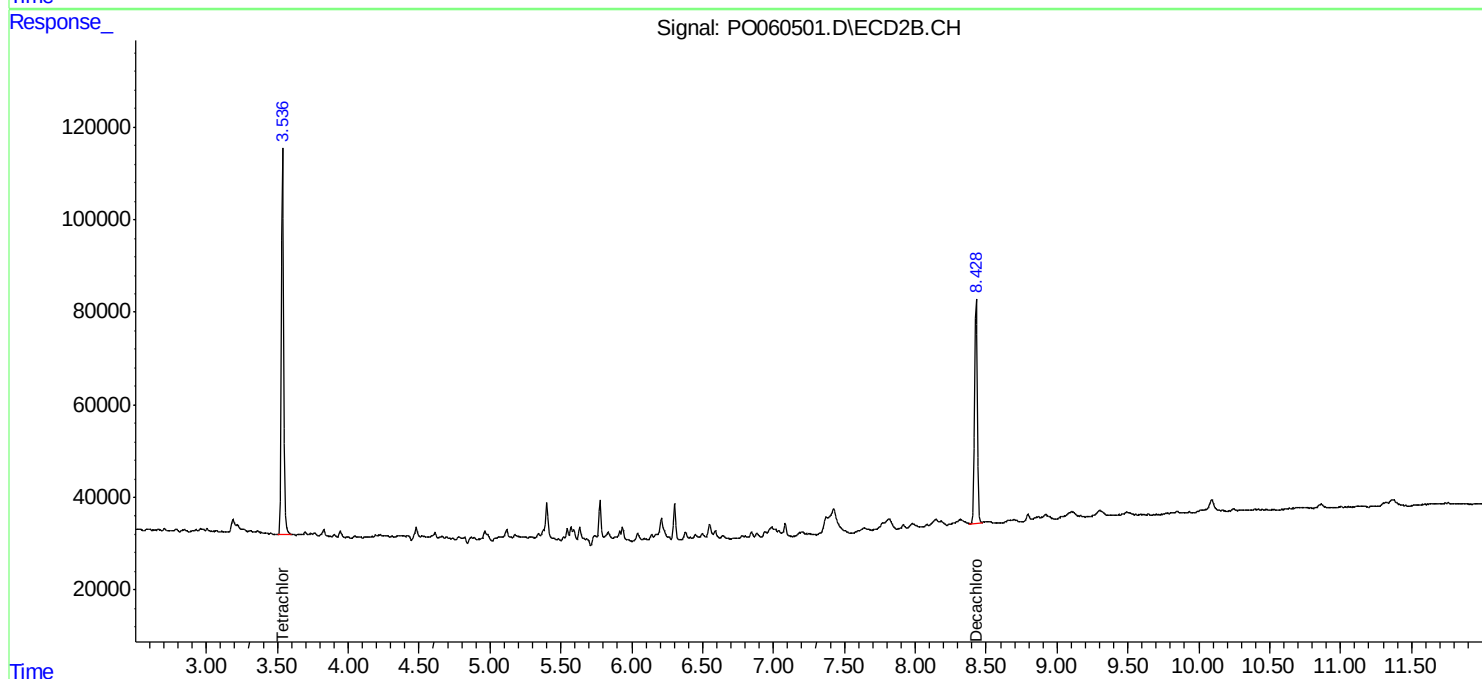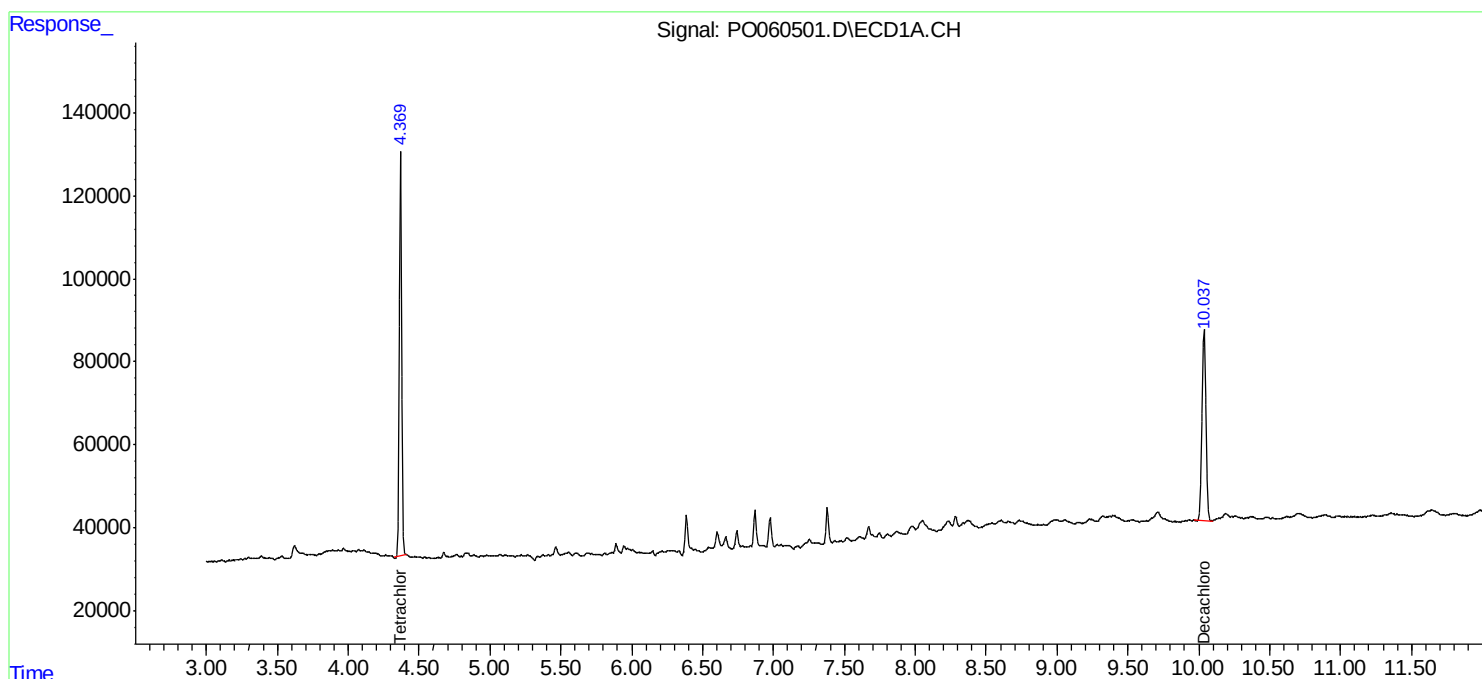


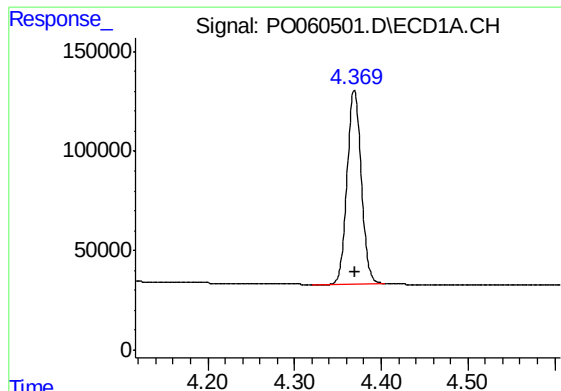

#1 Tetrachloro-m-xylene


R.T.: 4.369 min
Delta R.T.: 0.000 min
Response: 1102445
Conc: 26.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-03-090519

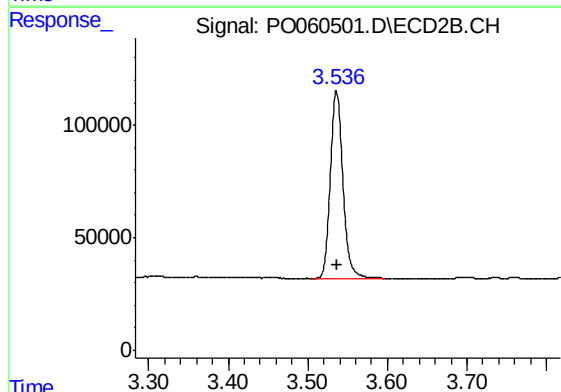


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: 0.000 min
Response: 904523
Conc: 29.45 ng/ml

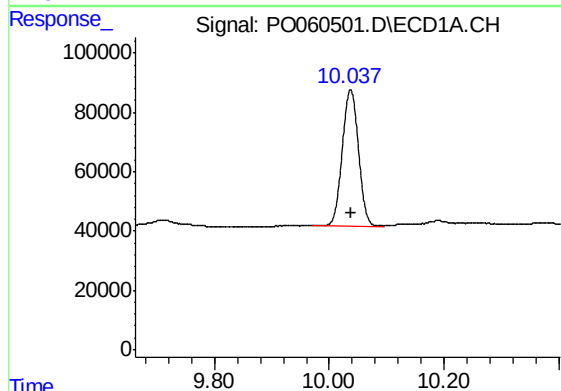

#2 Decachlorobiphenyl

R.T.: 10.037 min
Delta R.T.: 0.000 min
Response: 904266
Conc: 17.14 ng/ml

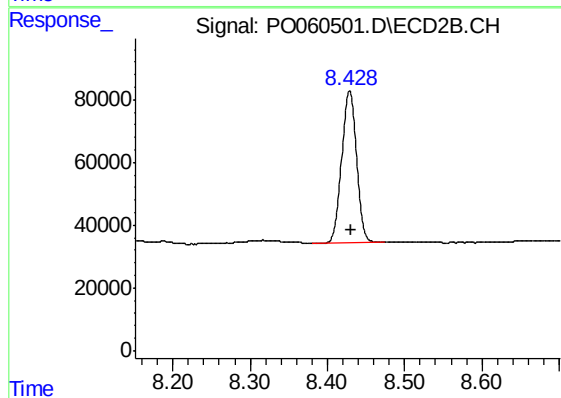

#2 Decachlorobiphenyl

R.T.: 8.428 min
Delta R.T.: -0.003 min
Response: 638251
Conc: 17.24 ng/ml