

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090719\
 Data File : P0060504.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Sep 2019 4:45
 Operator : SM/AJ
 Sample : K4696-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WS-SB05-COMP

Manual Integrations
 APPROVED

Ankita
 9/9/2019 1:11:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 01:16:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Sep 08 02:12:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.369	3.536	1035130	879181	24.947	28.624
2)	SA Decachlor...	10.036	8.429	710163	529660	13.463m	14.308

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090719\
Data File : PO060504.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Sep 2019 4:45
Operator : SM/AJ
Sample : K4696-04
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WS-SB05-COMP


Manual Integrations
APPROVED

Ankita
9/9/2019 1:11:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 01:16:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Sep 08 02:12:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

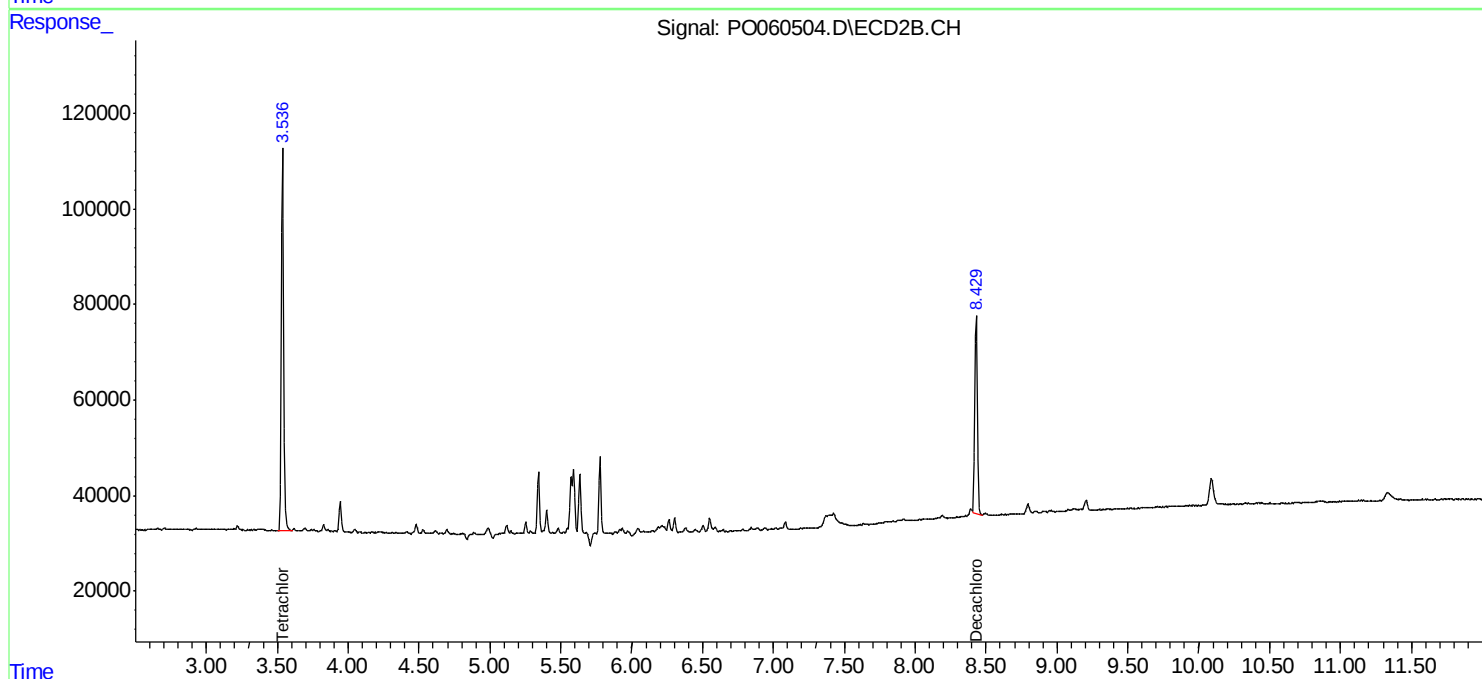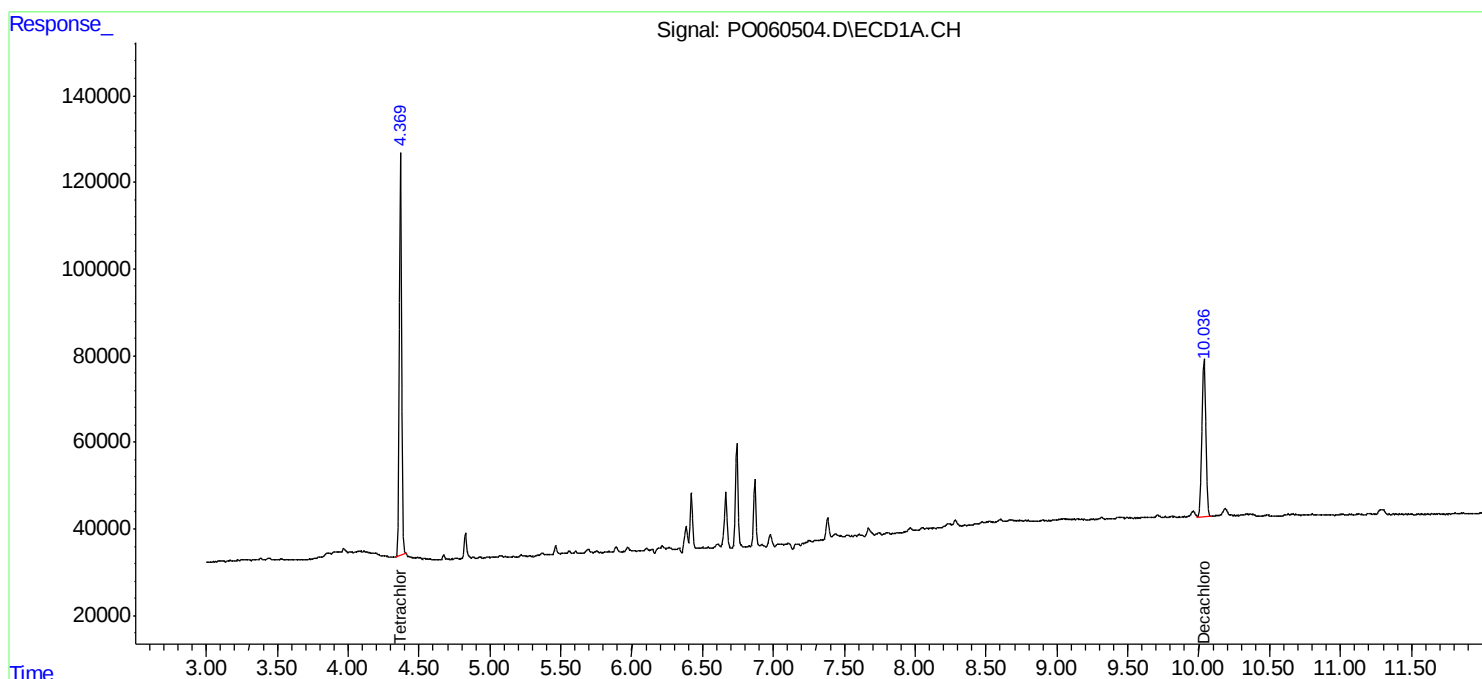

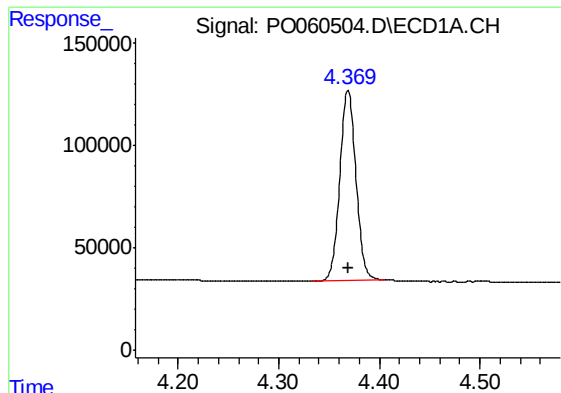


#1 Tetrachloro-m-xylene

R.T.: 4.369 min
Delta R.T.: 0.000 min
Response: 1035130
Conc: 24.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
WS-SB05-COMP


Manual Integrations
APPROVED

Ankita
9/9/2019 1:11:35 PM

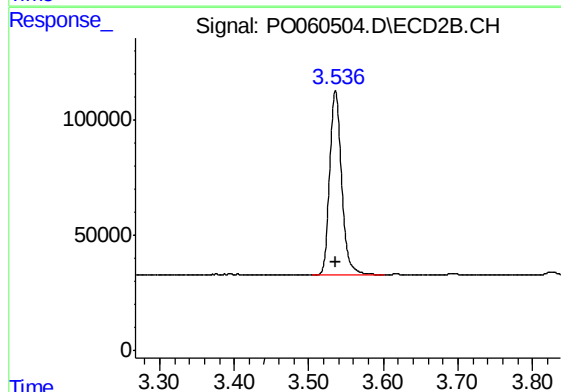


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: 0.000 min
Response: 879181
Conc: 28.62 ng/ml

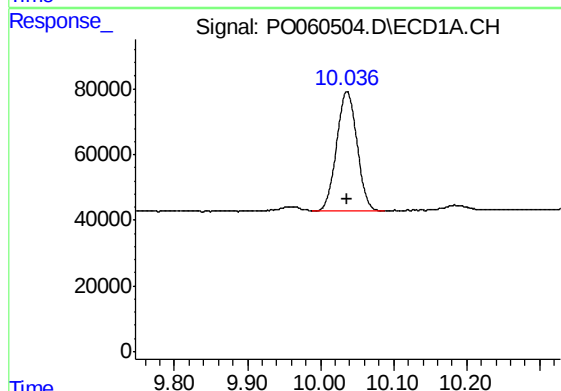

#2 Decachlorobiphenyl

R.T.: 10.036 min
Delta R.T.: 0.000 min
Response: 710163
Conc: 13.46 ng/ml m

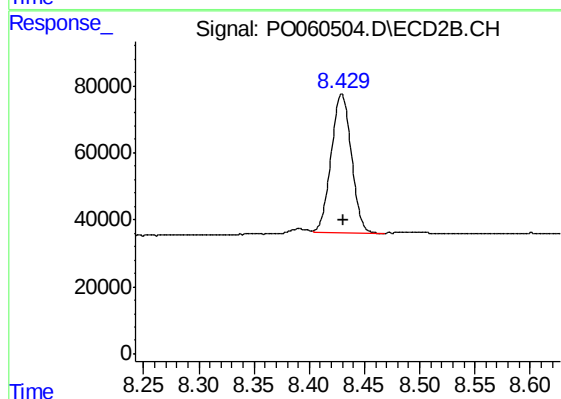

#2 Decachlorobiphenyl

R.T.: 8.429 min
Delta R.T.: -0.002 min
Response: 529660
Conc: 14.31 ng/ml