

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090721\
Data File : P0080986.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Sep 2021 10:55
Operator : DD\AJ
Sample : M3634-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OK-01-090121

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 12:21:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.928	4.055	1948631	626238	24.684	25.341
2) SA Decachlor...	10.994	9.417	1287625	487395	21.686	20.879

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090721\
Data File : P0080986.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Sep 2021 10:55
Operator : DD\AJ
Sample : M3634-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OK-01-090121

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 12:21:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

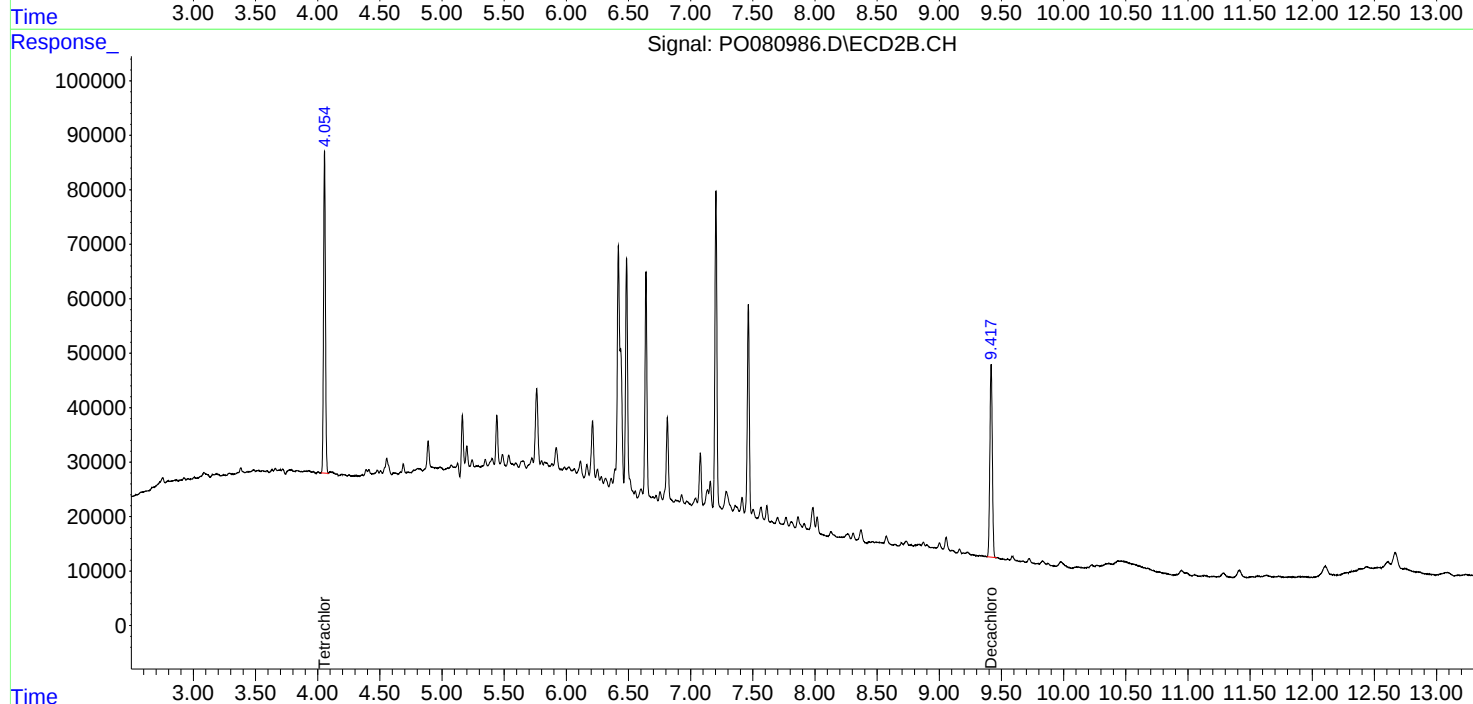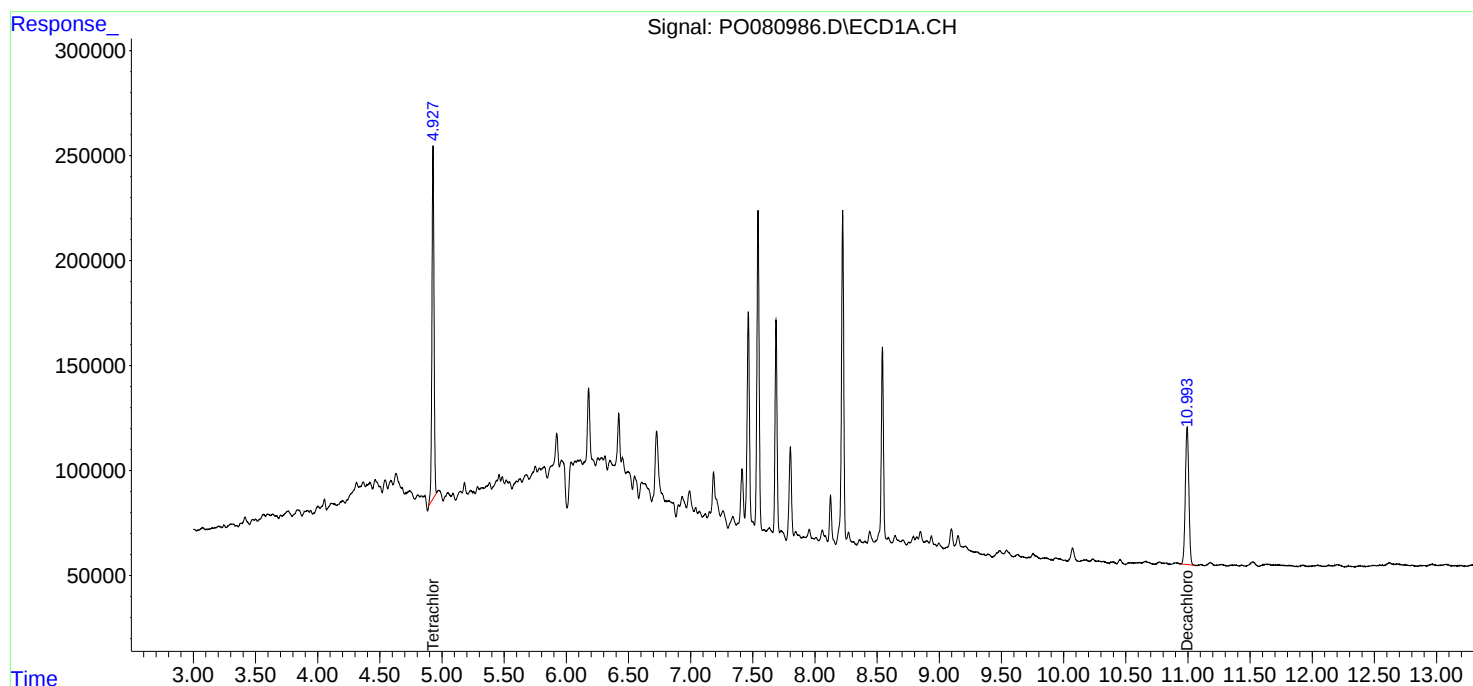


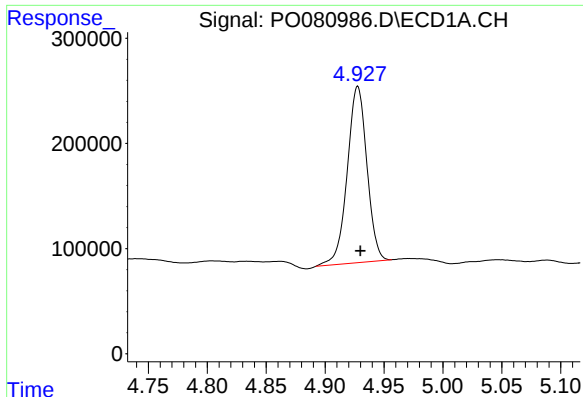

#1 Tetrachloro-m-xylene


R.T.: 4.928 min
Delta R.T.: -0.002 min
Response: 1948631
Conc: 24.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-01-090121

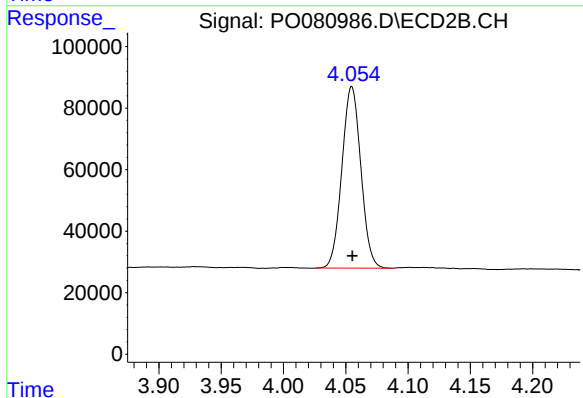


#1 Tetrachloro-m-xylene

R.T.: 4.055 min
Delta R.T.: 0.000 min
Response: 626238
Conc: 25.34 ng/ml

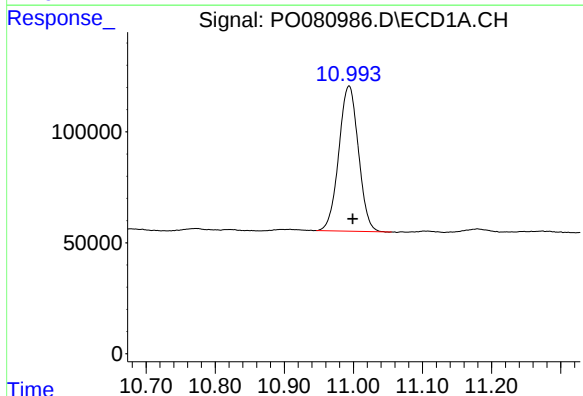

#2 Decachlorobiphenyl

R.T.: 10.994 min
Delta R.T.: -0.005 min
Response: 1287625
Conc: 21.69 ng/ml

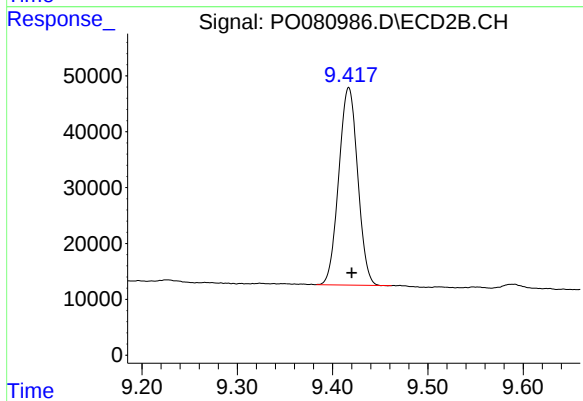

#2 Decachlorobiphenyl

R.T.: 9.417 min
Delta R.T.: -0.003 min
Response: 487395
Conc: 20.88 ng/ml