

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090721\
 Data File : P0081017.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Sep 2021 20:25
 Operator : DD\AJ
 Sample : M3648-09
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20211058-SI-COMP-3-MODIFIED-EL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 09:26:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.928	4.055	1680626	530744	21.289	21.477
2) SA Decachlor...	10.996	9.417	1052173	389966	17.721	16.705

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090721\
Data File : P0081017.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Sep 2021 20:25
Operator : DD\AJ
Sample : M3648-09
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20211058-SI-COMP-3-MODIFIED-EL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 09:26:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

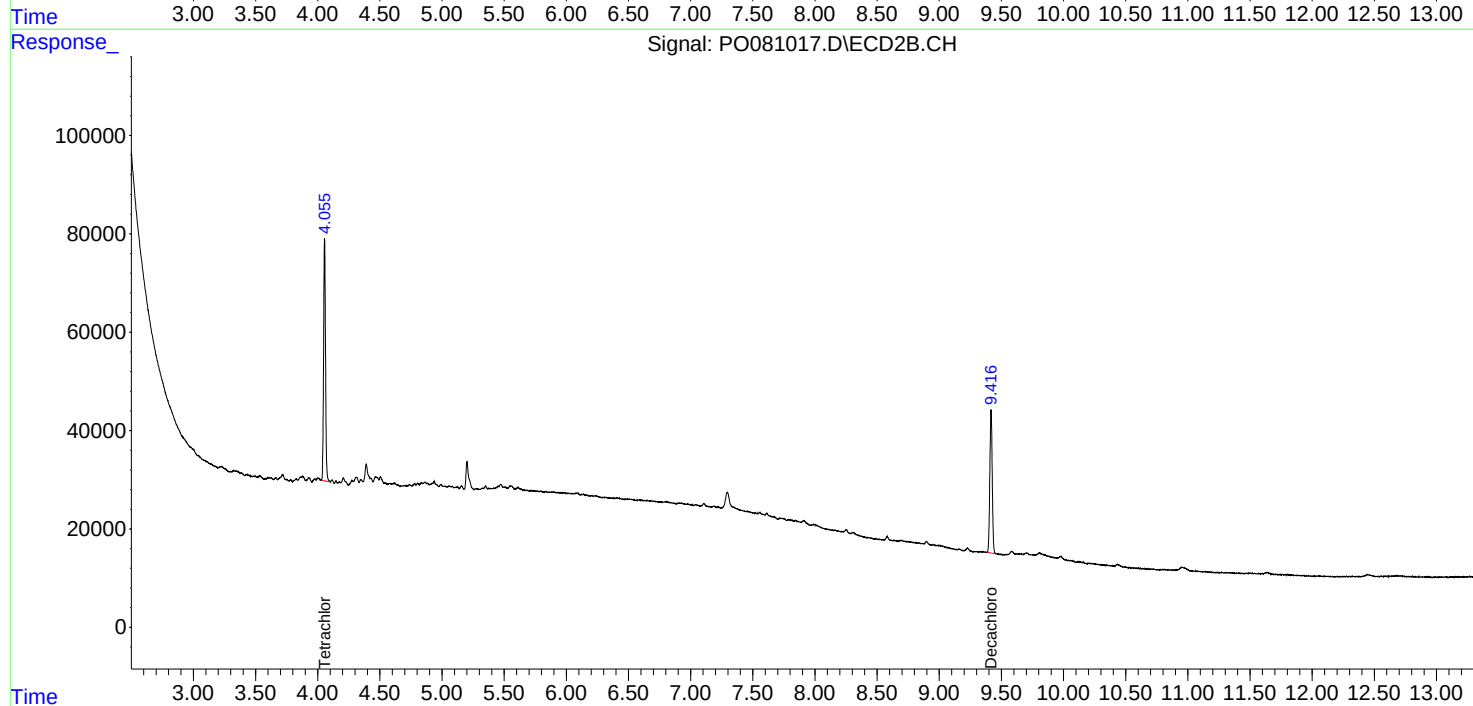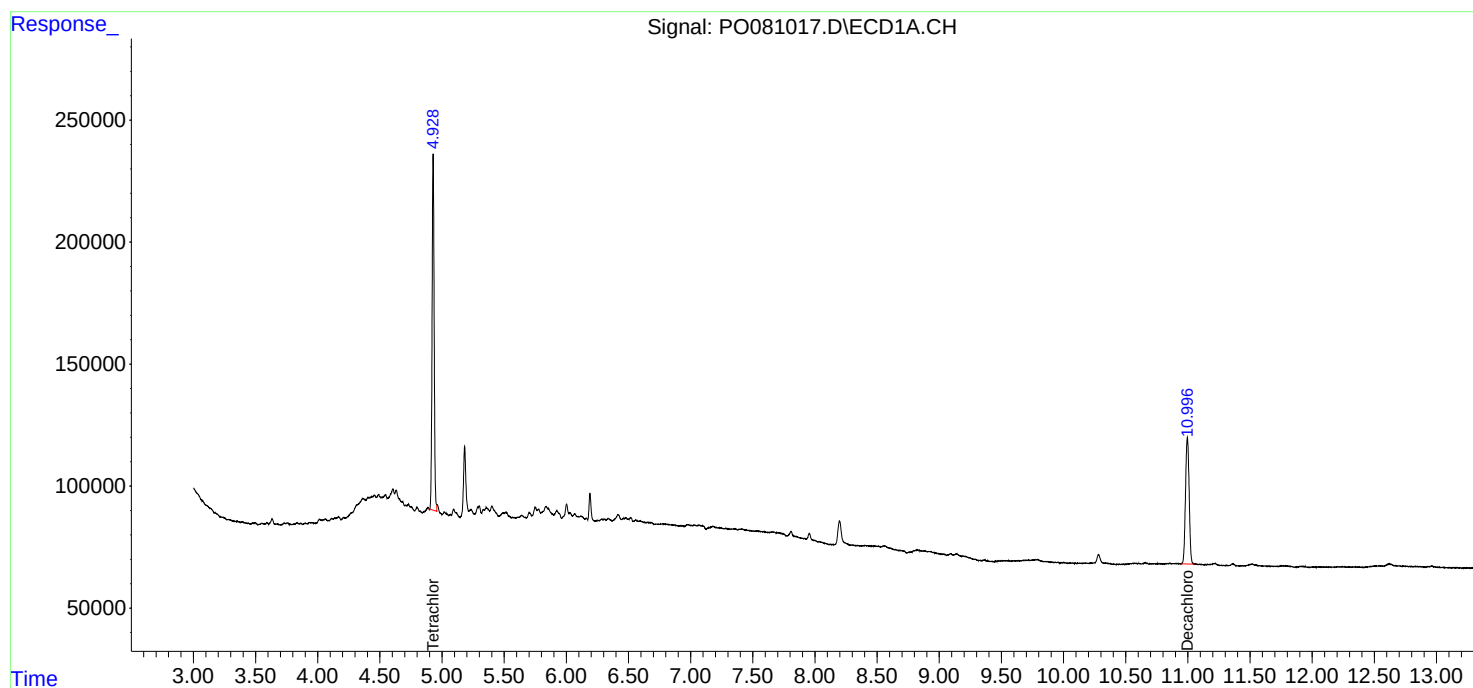


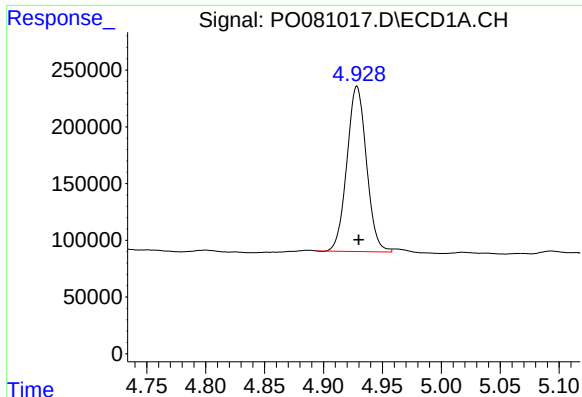

#1 Tetrachloro-m-xylene


R.T.: 4.928 min
Delta R.T.: -0.002 min
Response: 1680626
Conc: 21.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
20211058-SI-COMP-3-MODIFIED-EL

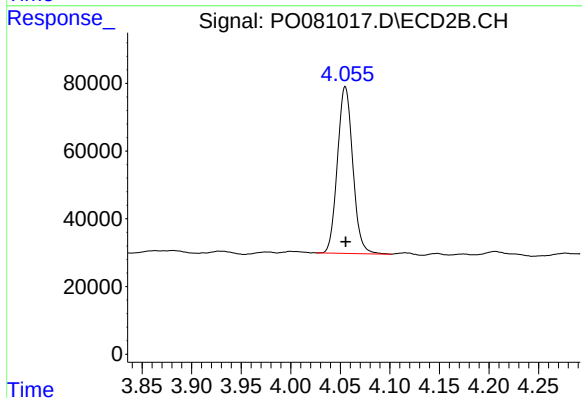


#1 Tetrachloro-m-xylene

R.T.: 4.055 min
Delta R.T.: 0.000 min
Response: 530744
Conc: 21.48 ng/ml

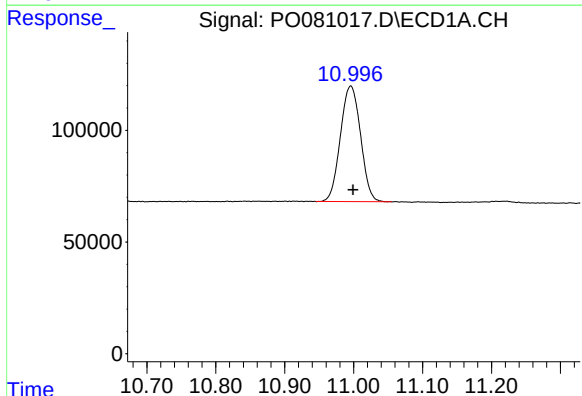

#2 Decachlorobiphenyl

R.T.: 10.996 min
Delta R.T.: -0.003 min
Response: 1052173
Conc: 17.72 ng/ml

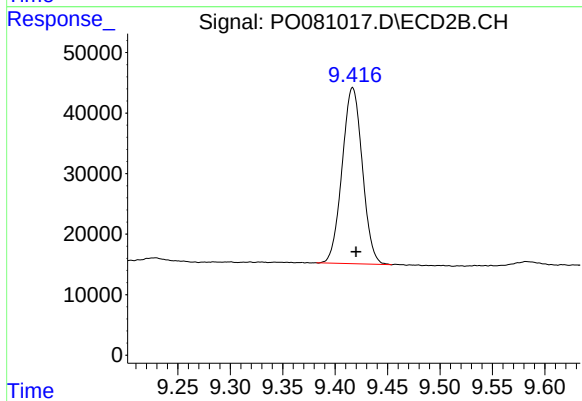

#2 Decachlorobiphenyl

R.T.: 9.417 min
Delta R.T.: -0.003 min
Response: 389966
Conc: 16.71 ng/ml