

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0090723\
 Data File : P0097809.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2023 23:27
 Operator : YP/AJ
 Sample : 04321-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 RT2345

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/08/2023
 Supervised By :Ankita Jodhani 09/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 02:03:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0090623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 07 02:56:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.441	3.623	41280437	10280381	10.361	10.735
2) SA Decachlor...	10.290	8.658	26493124	11757341	14.179	13.761
Target Compounds						
31) L7 AR-1260-1	7.231	6.204	6460960	1052701	45.719	19.786 #
32) L7 AR-1260-2	7.497	6.392	4445651	1213426	29.411	19.378 #
33) L7 AR-1260-3	7.861	6.547	3414757	1232050	30.145	21.366 #
34) L7 AR-1260-4	8.088	7.021	5199239	1041837	43.737	22.209 #
35) L7 AR-1260-5	8.417	7.263	5301533	2179188	25.897	21.984

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090723\
Data File : PO097809.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2023 23:27
Operator : YP/AJ
Sample : 04321-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RT2345


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/08/2023
Supervised By :Ankita Jodhani 09/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 02:03:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090623.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 07 02:56:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

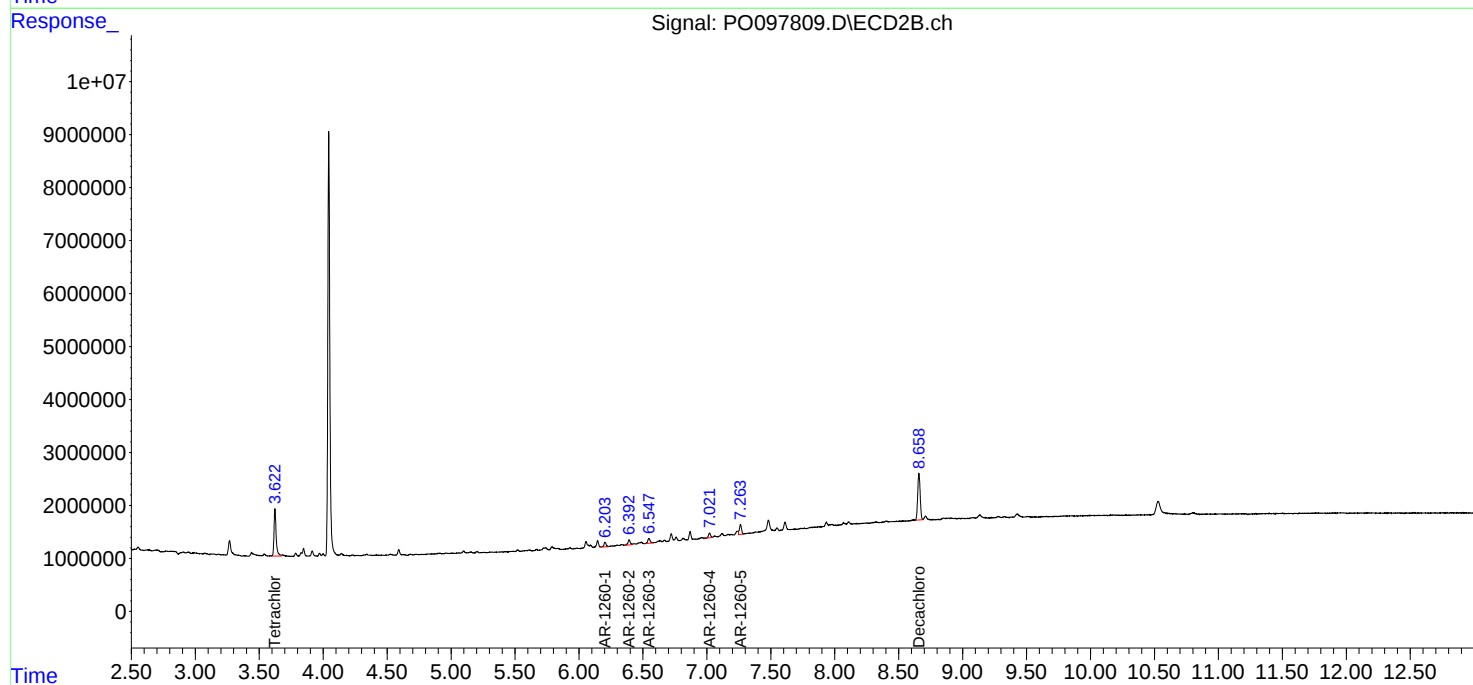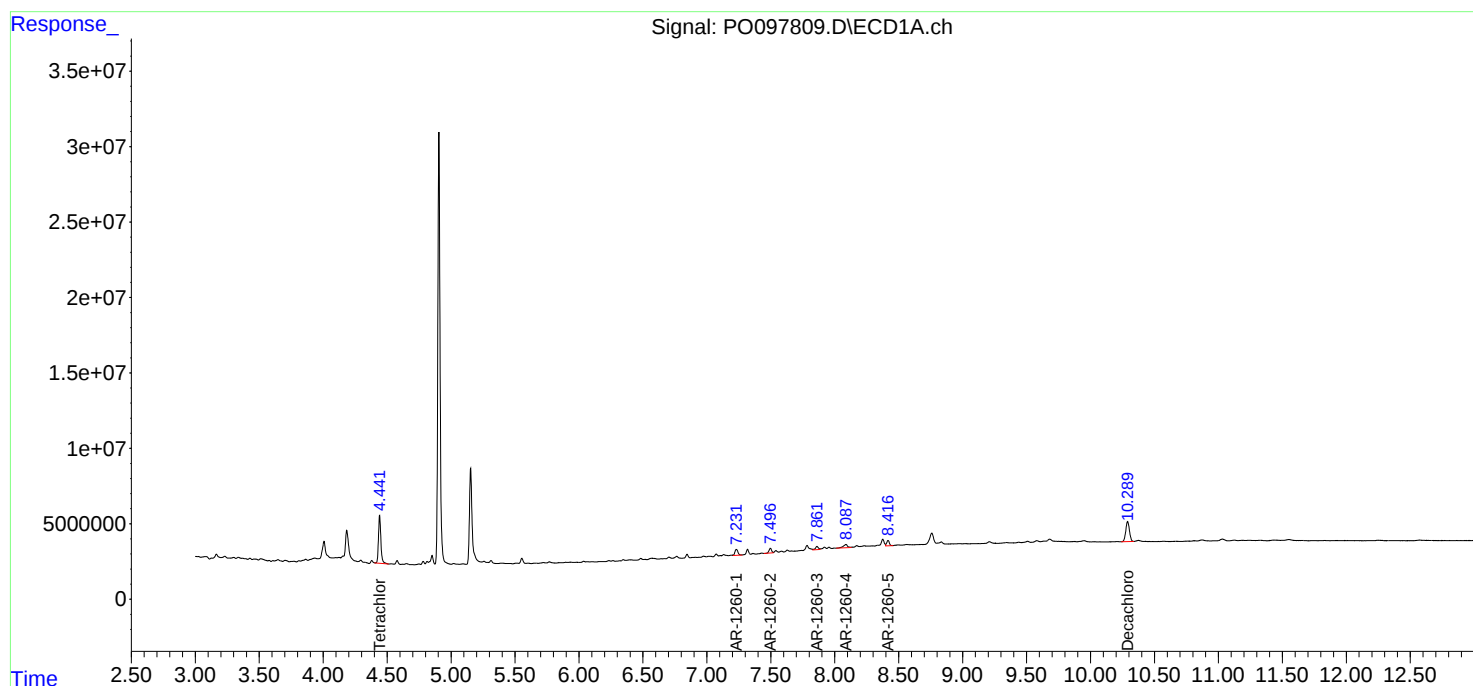

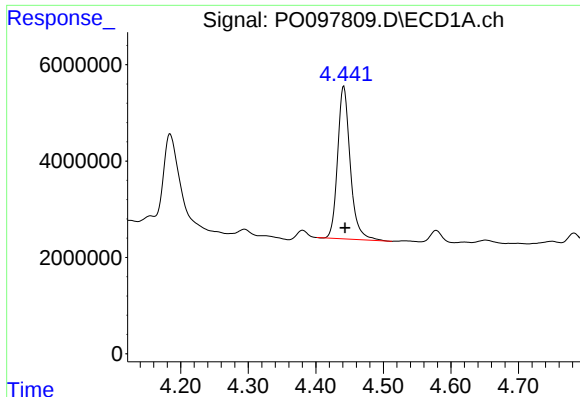


#1 Tetrachloro-m-xylene

R.T.: 4.441 min
Delta R.T.: -0.002 min
Response: 41280437
Conc: 10.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
RT2345


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/08/2023
Supervised By :Ankita Jodhani 09/08/2023

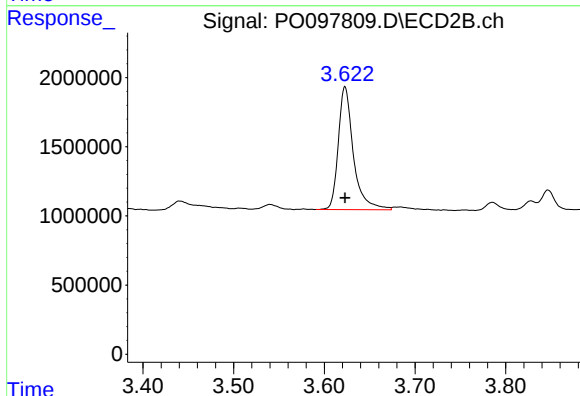


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: 0.000 min
Response: 10280381
Conc: 10.73 ng/ml

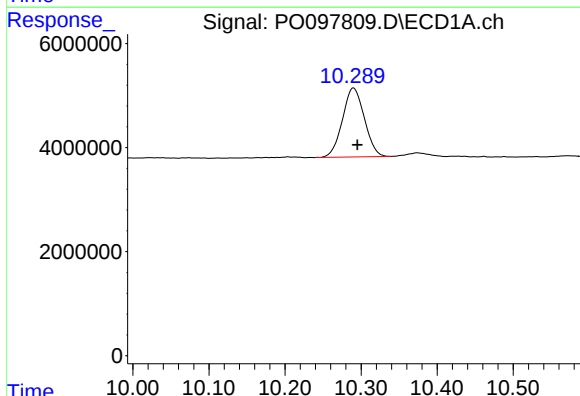


#2 Decachlorobiphenyl

R.T.: 10.290 min
Delta R.T.: -0.005 min
Response: 26493124
Conc: 14.18 ng/ml

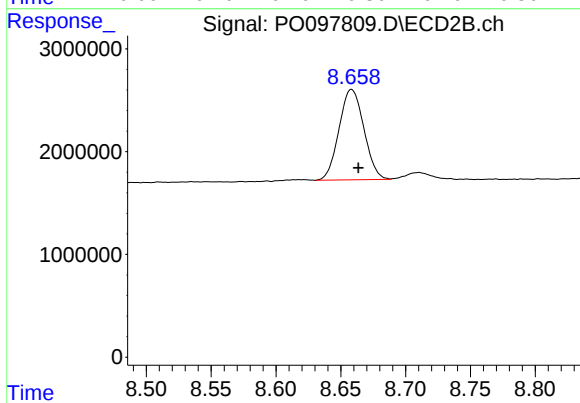

#2 Decachlorobiphenyl

R.T.: 8.658 min
Delta R.T.: -0.005 min
Response: 11757341
Conc: 13.76 ng/ml

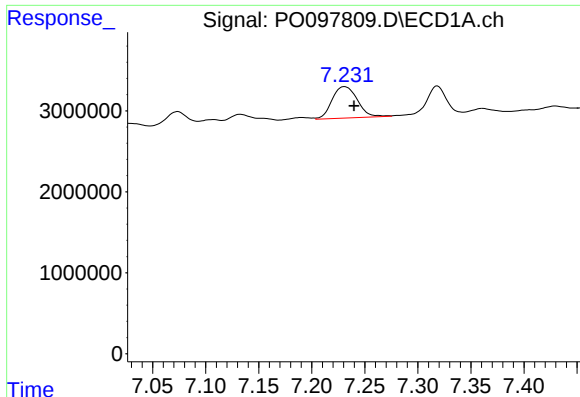


#31 AR-1260-1

R.T.: 7.231 min
Delta R.T.: -0.009 min
Response: 6460960
Conc: 45.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
RT2345


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/08/2023
Supervised By :Ankita Jodhani 09/08/2023

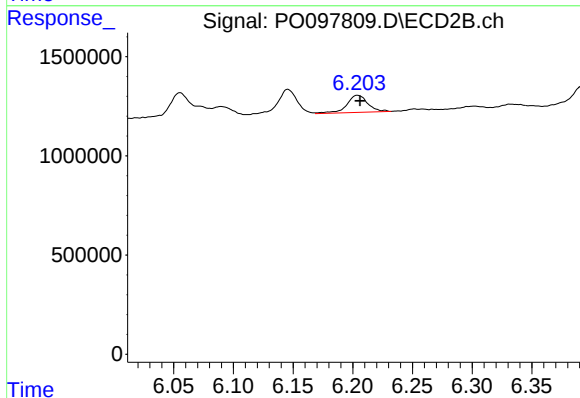


#31 AR-1260-1

R.T.: 6.204 min
Delta R.T.: -0.002 min
Response: 1052701
Conc: 19.79 ng/ml

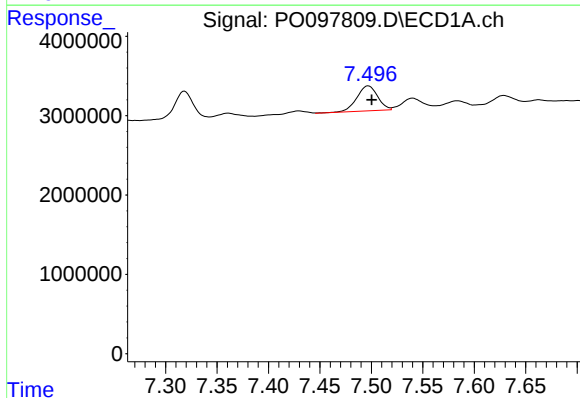


#32 AR-1260-2

R.T.: 7.497 min
Delta R.T.: -0.003 min
Response: 4445651
Conc: 29.41 ng/ml

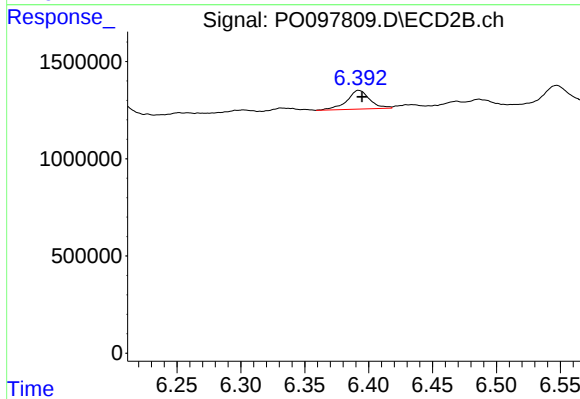

#32 AR-1260-2

R.T.: 6.392 min
Delta R.T.: -0.002 min
Response: 1213426
Conc: 19.38 ng/ml

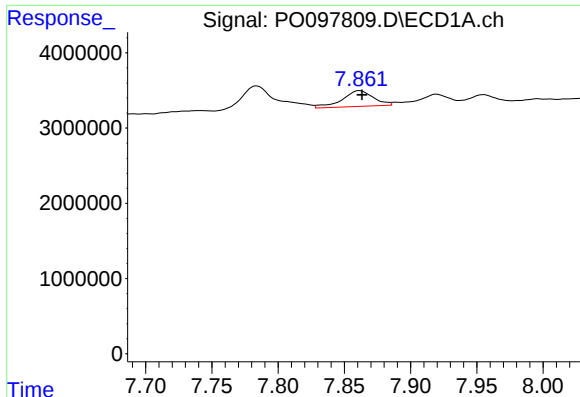


#33 AR-1260-3

R.T.: 7.861 min
Delta R.T.: -0.002 min
Response: 3414757
Conc: 30.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
RT2345


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/08/2023
Supervised By :Ankita Jodhani 09/08/2023

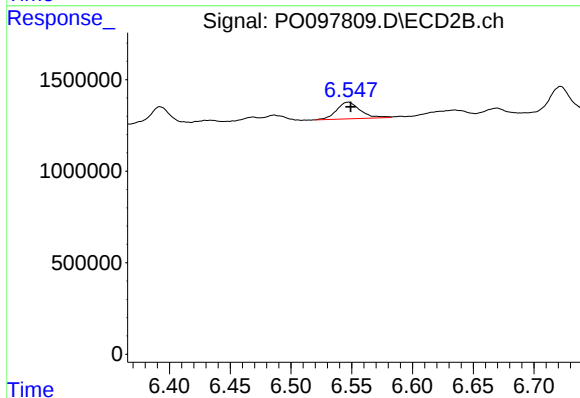


#33 AR-1260-3

R.T.: 6.547 min
Delta R.T.: -0.002 min
Response: 1232050
Conc: 21.37 ng/ml

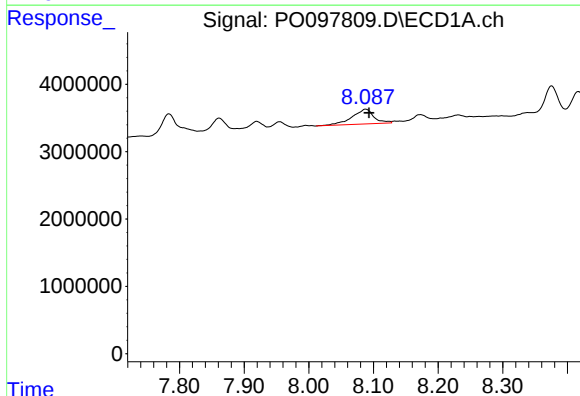


#34 AR-1260-4

R.T.: 8.088 min
Delta R.T.: -0.005 min
Response: 5199239
Conc: 43.74 ng/ml

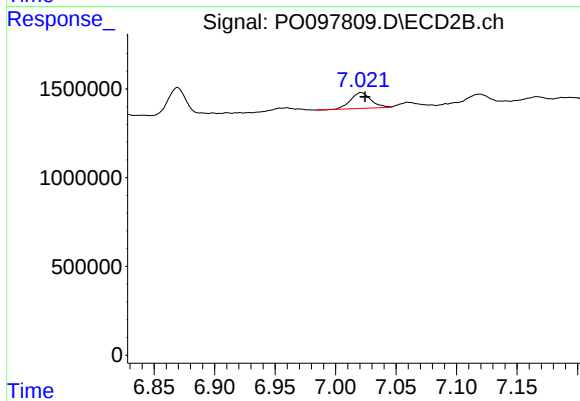

#34 AR-1260-4

R.T.: 7.021 min
Delta R.T.: -0.003 min
Response: 1041837
Conc: 22.21 ng/ml

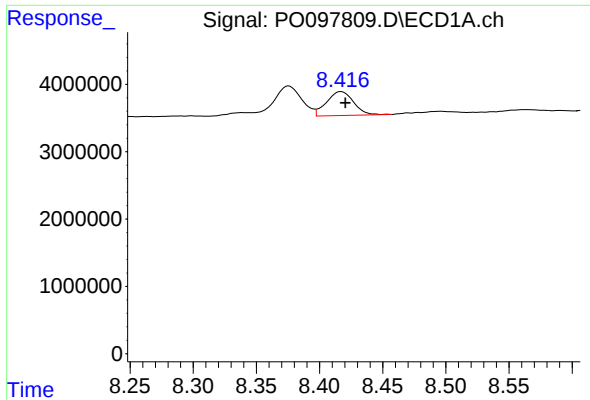


#35 AR-1260-5

R.T.: 8.417 min
Delta R.T.: -0.004 min
Response: 5301533
Conc: 25.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
RT2345

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/08/2023
Supervised By :Ankita Jodhani 09/08/2023

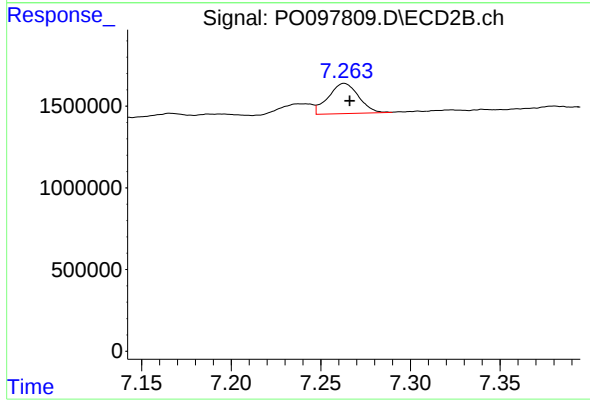

#35 AR-1260-5

R.T.: 7.263 min
Delta R.T.: -0.003 min
Response: 2179188
Conc: 21.98 ng/ml