

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090723\
 Data File : P0097815.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2023 01:23
 Operator : YP/AJ
 Sample : 04299-10
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TWP-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/08/2023
 Supervised By :Ankita Jodhani 09/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 03:13:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 07 02:56:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.440	3.622	66329750	17151282	16.649m	17.909
2) SA Decachlor...	10.289	8.658	19825206	8779079	10.610	10.275

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090723\
Data File : PO097815.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2023 01:23
Operator : YP/AJ
Sample : 04299-10
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TWP-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/08/2023
Supervised By :Ankita Jodhani 09/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 03:13:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090623.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 07 02:56:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

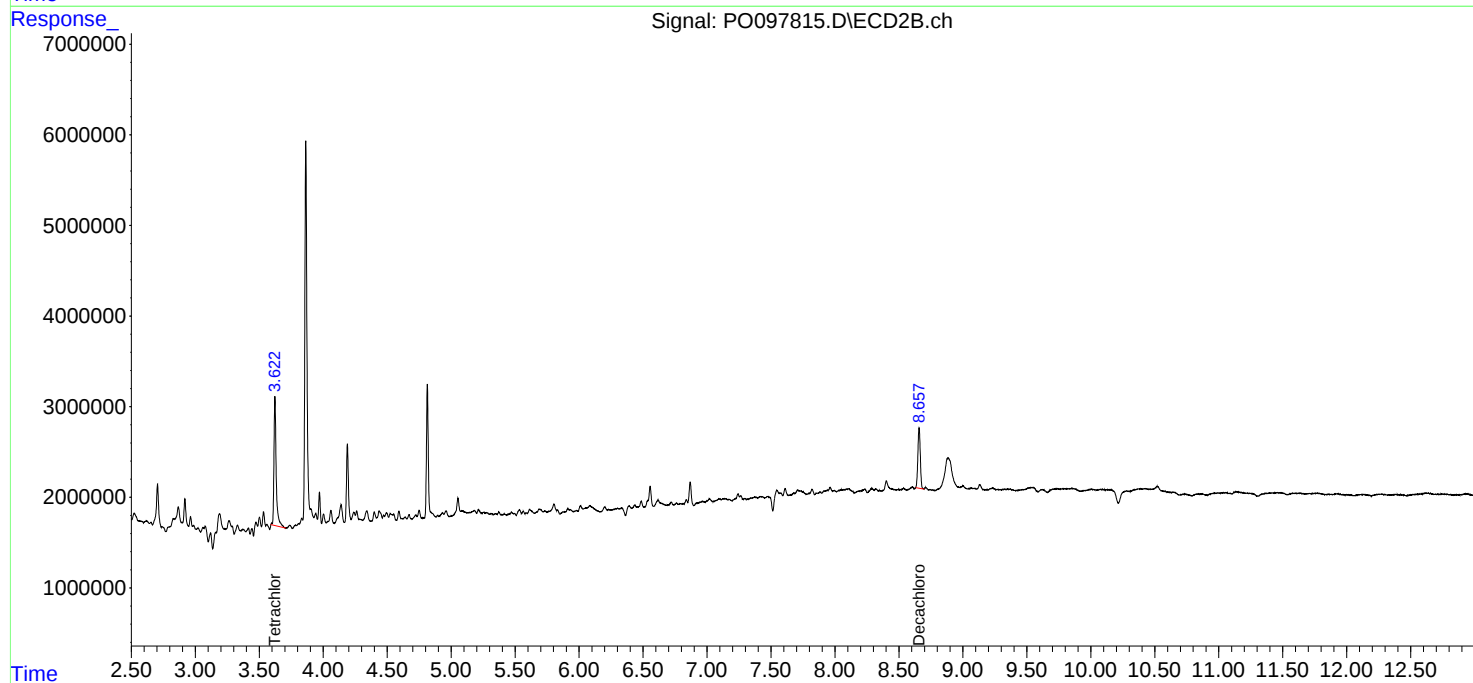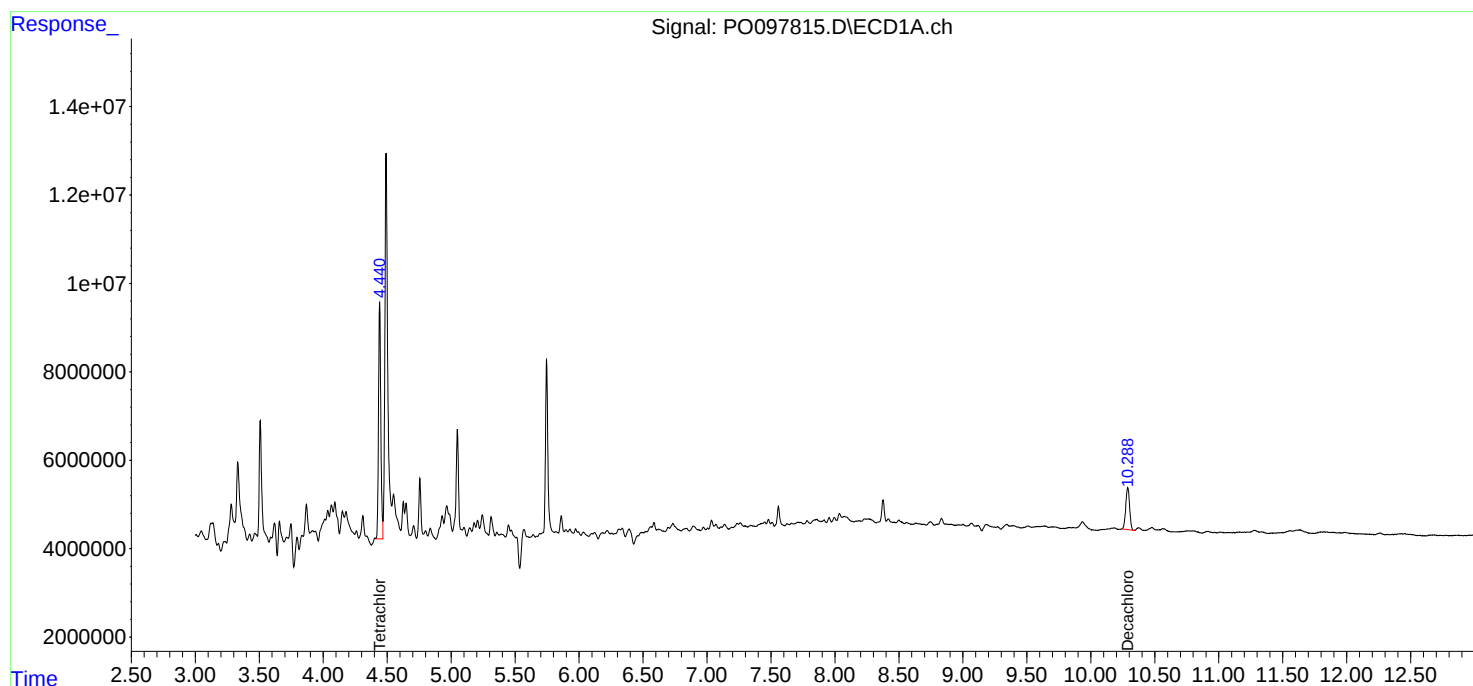

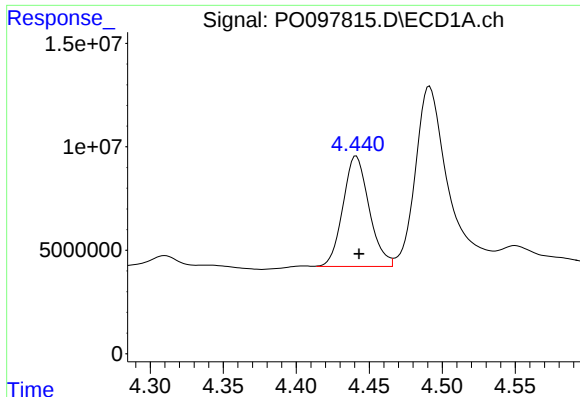


#1 Tetrachloro-m-xylene

R.T.: 4.440 min
Delta R.T.: -0.003 min
Response: 66329750
Conc: 16.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
TWP-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/08/2023
Supervised By :Ankita Jodhani 09/08/2023

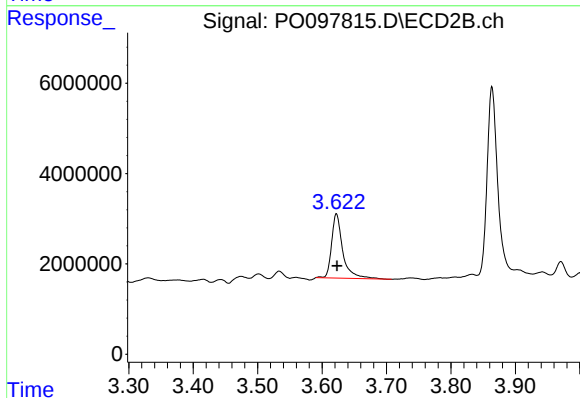


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: 0.000 min
Response: 17151282
Conc: 17.91 ng/ml

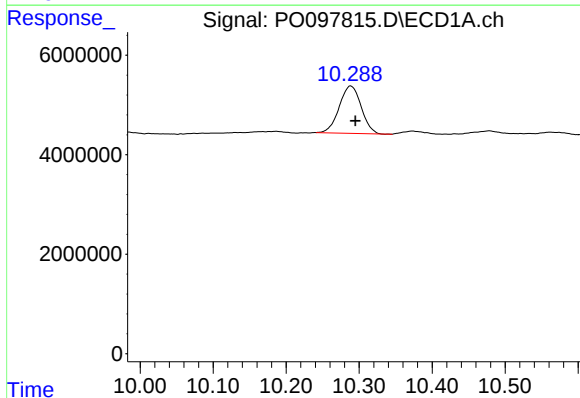

#2 Decachlorobiphenyl

R.T.: 10.289 min
Delta R.T.: -0.007 min
Response: 19825206
Conc: 10.61 ng/ml

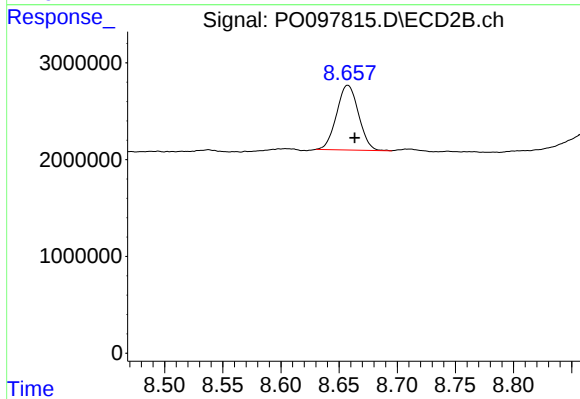

#2 Decachlorobiphenyl

R.T.: 8.658 min
Delta R.T.: -0.006 min
Response: 8779079
Conc: 10.28 ng/ml