

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090820\
 Data File : P0071227.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Sep 2020 12:21
 Operator : DD\AJ
 Sample : L3886-01RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TOTE-31230RE

Manual Integrations
 APPROVED

Ankita
 9/9/2020 10:45:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 14:53:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 28 17:10:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.354	3.541	2355658	1013189	30.503	22.855 #
2) SA Decachlor...	9.996f	8.740f	3645148	1522863	39.836m	26.513m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090820\
Data File : P0071227.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Sep 2020 12:21
Operator : DD\AJ
Sample : L3886-01RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TOTE-31230RE


Manual Integrations
APPROVED

Ankita
9/9/2020 10:45:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 14:53:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:10:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

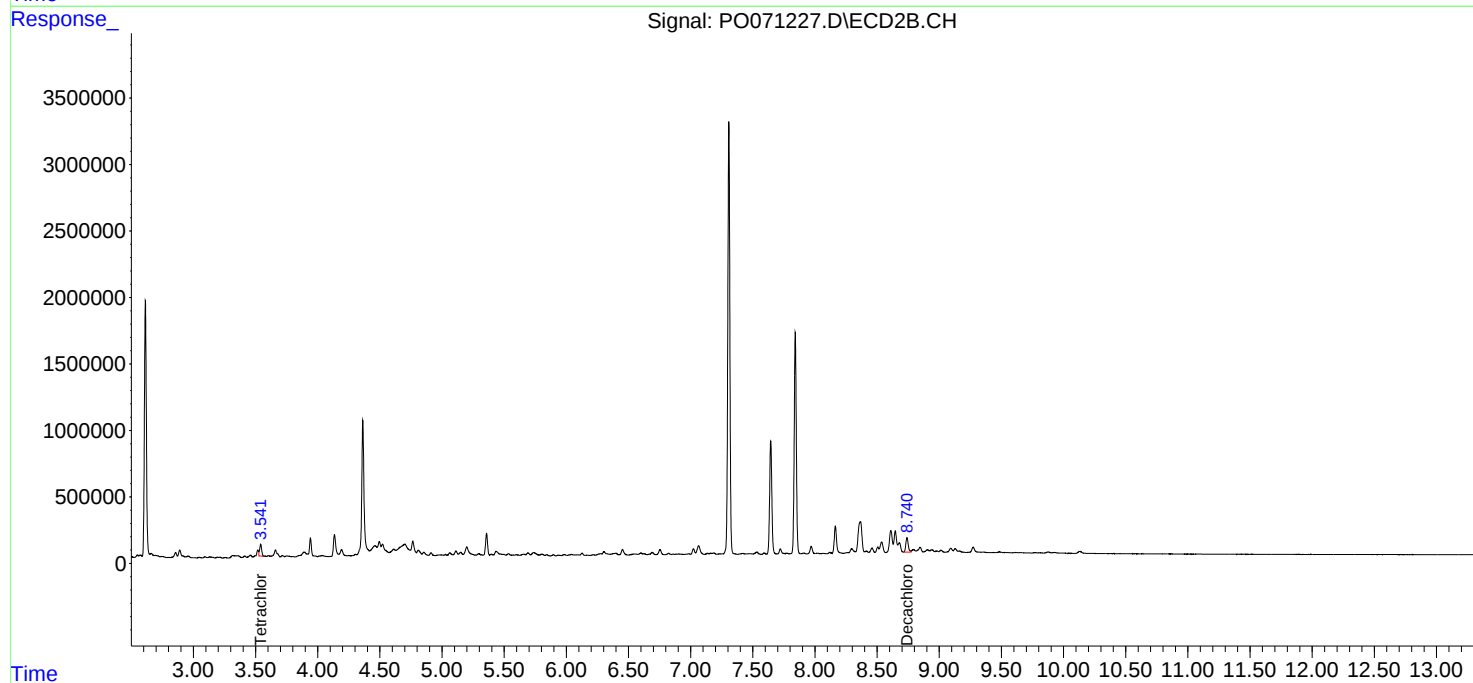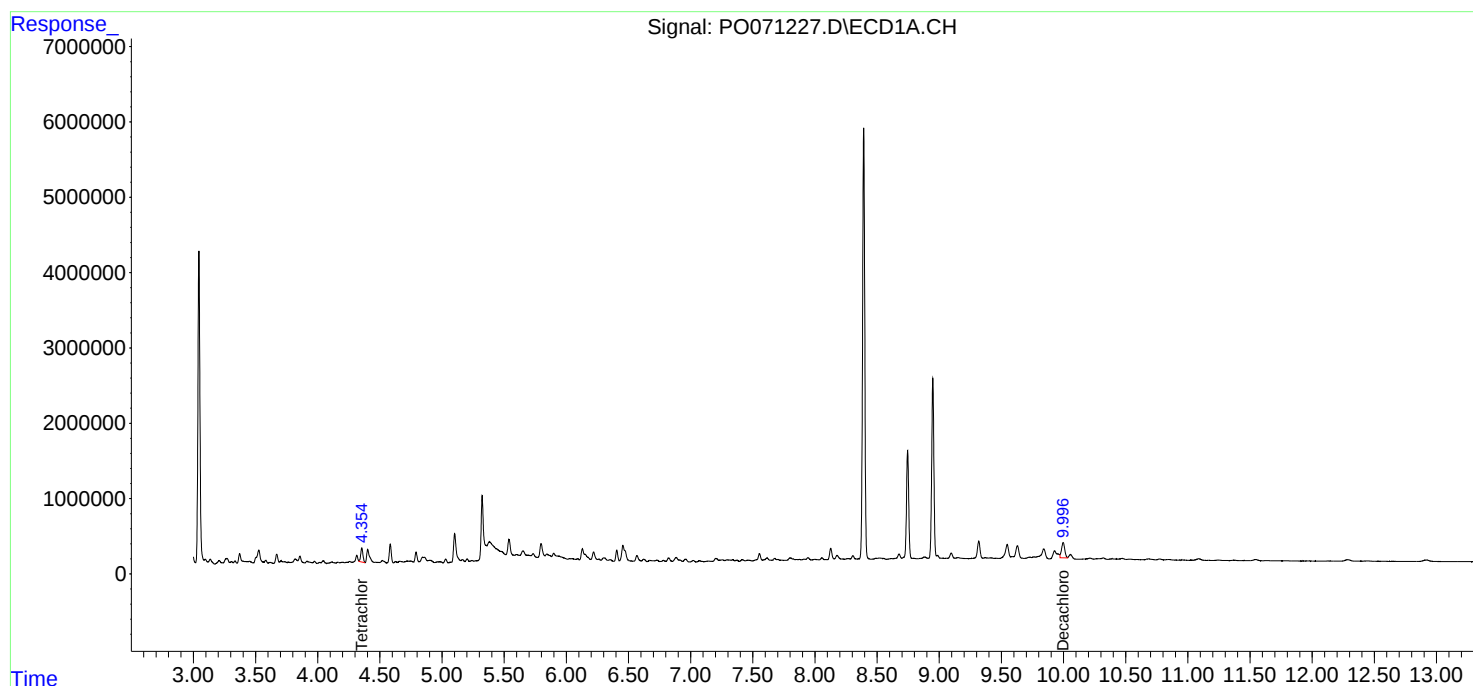

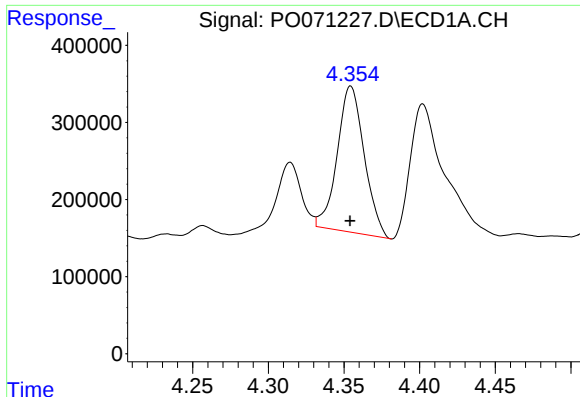


#1 Tetrachloro-m-xylene

R.T.: 4.354 min
Delta R.T.: 0.000 min
Response: 2355658
Conc: 30.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
TOTE-31230RE


Manual Integrations
APPROVED

Ankita
9/9/2020 10:45:17 AM

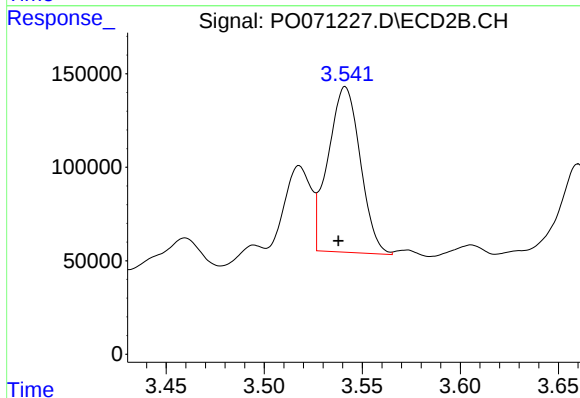


#1 Tetrachloro-m-xylene

R.T.: 3.541 min
Delta R.T.: 0.003 min
Response: 1013189
Conc: 22.86 ng/ml

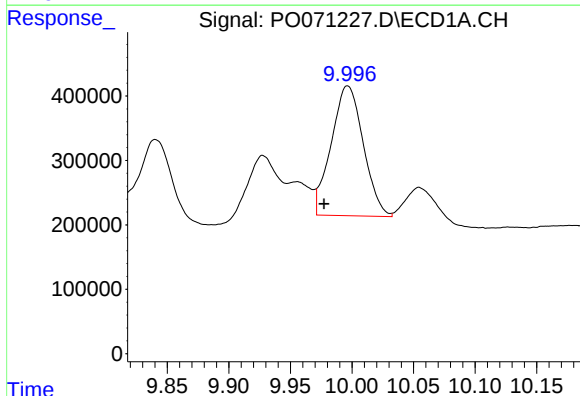

#2 Decachlorobiphenyl

R.T.: 9.996 min
Delta R.T.: 0.019 min
Response: 3645148
Conc: 39.84 ng/ml m

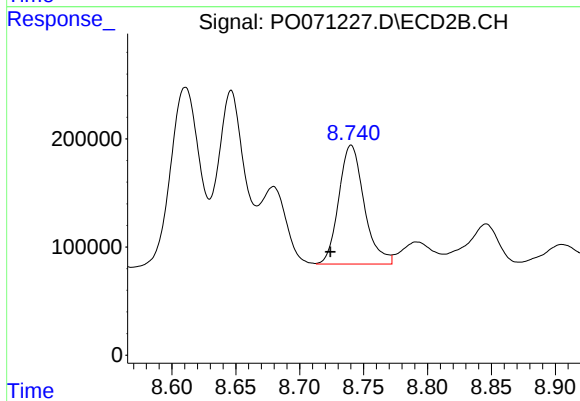

#2 Decachlorobiphenyl

R.T.: 8.740 min
Delta R.T.: 0.016 min
Response: 1522863
Conc: 26.51 ng/ml m