

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090822\
 Data File : P0089412.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2022 17:16
 Operator : YP/AJ
 Sample : N4511-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S1-AQ_DM-IDW-20220902

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 17:47:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 29 17:48:02 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.430	3.587	87108392	26479040	23.231	27.432
2) SA Decachlor...	10.261	8.569	35292269	18303598	15.329	20.699 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090822\
Data File : PO089412.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2022 17:16
Operator : YP/AJ
Sample : N4511-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S1-AQ_DM-IDW-20220902

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 17:47:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082922.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 29 17:48:02 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

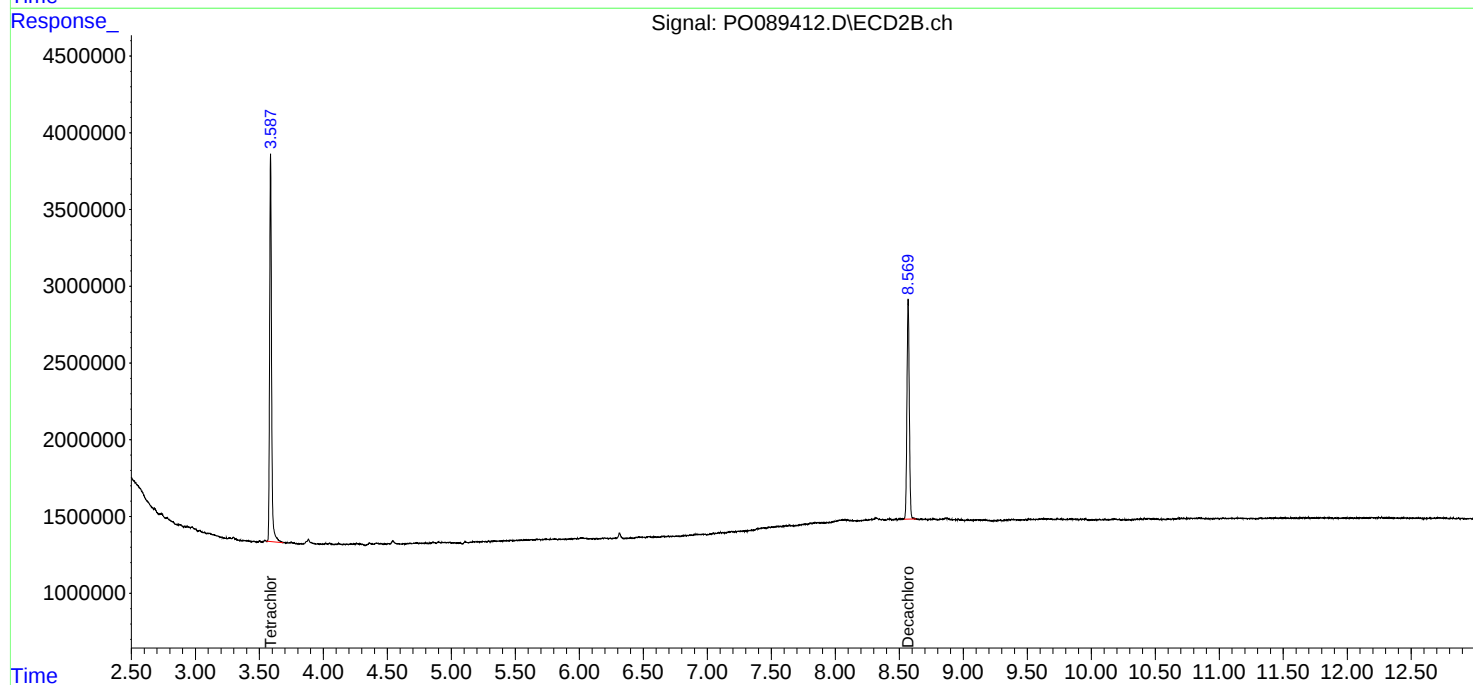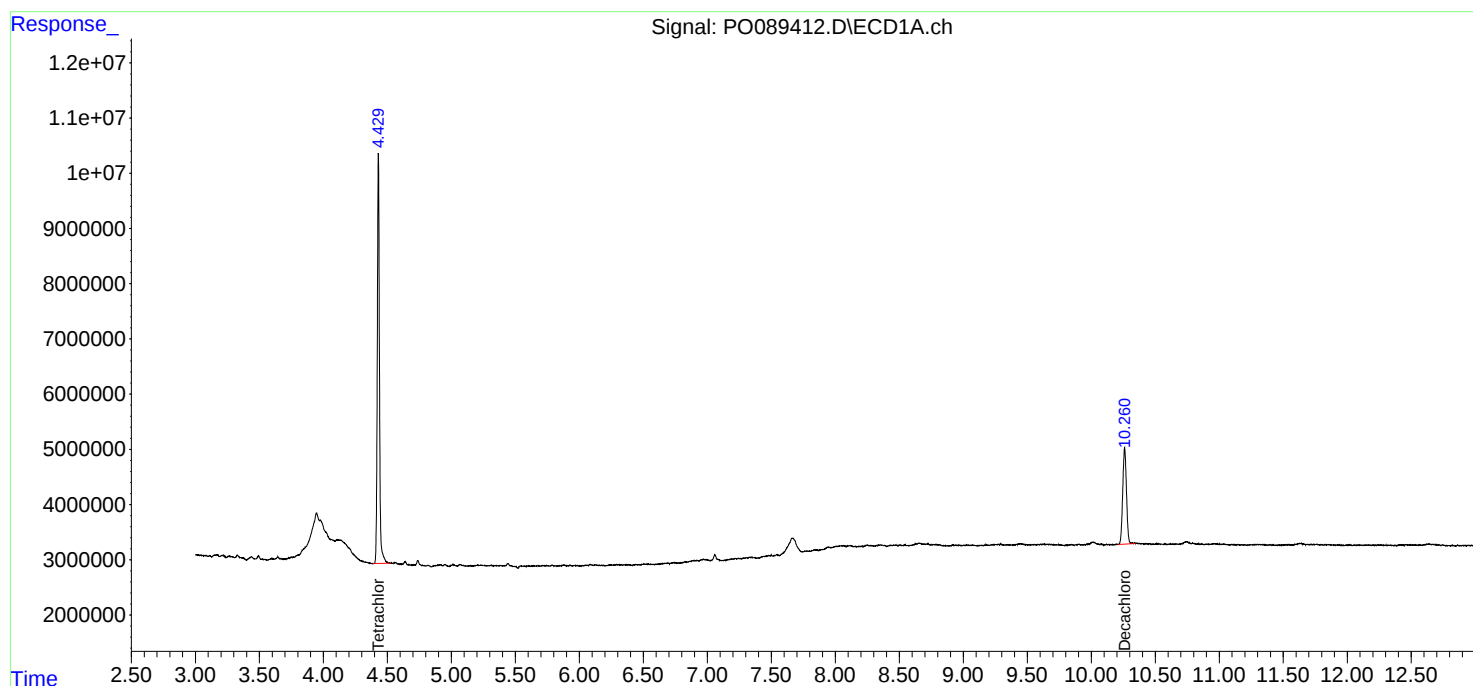


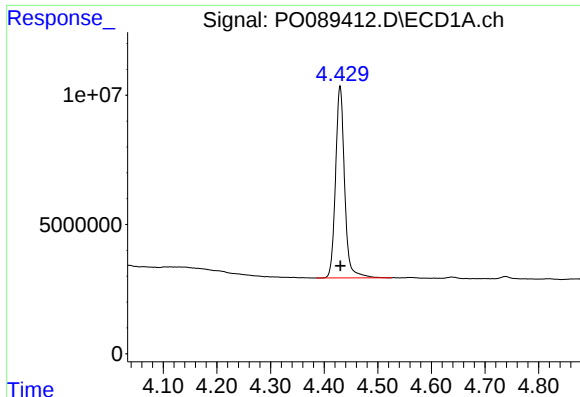

#1 Tetrachloro-m-xylene


R.T.: 4.430 min
Delta R.T.: 0.000 min
Response: 87108392
Conc: 23.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-AQ_DM-IDW-20220902

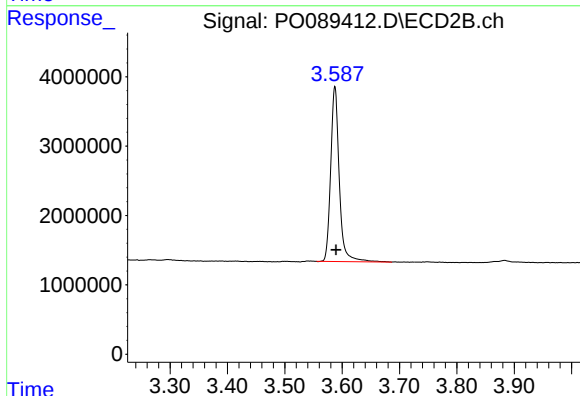


#1 Tetrachloro-m-xylene

R.T.: 3.587 min
Delta R.T.: -0.002 min
Response: 26479040
Conc: 27.43 ng/ml

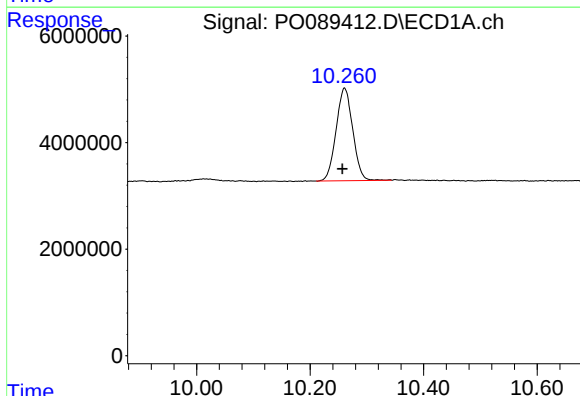

#2 Decachlorobiphenyl

R.T.: 10.261 min
Delta R.T.: 0.004 min
Response: 35292269
Conc: 15.33 ng/ml

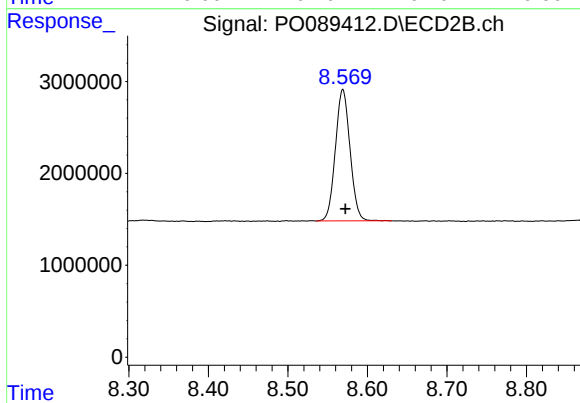

#2 Decachlorobiphenyl

R.T.: 8.569 min
Delta R.T.: -0.003 min
Response: 18303598
Conc: 20.70 ng/ml