

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090823\
 Data File : P0097827.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2023 10:28
 Operator : YP/AJ
 Sample : 04299-10RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TWP-01RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/11/2023
 Supervised By :Ankita Jodhani 09/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 15:51:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 07 02:56:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.442	3.623	63742011	15987716	15.999m	16.694m
2) SA Decachlor...	10.292	8.659	19801995	9097233	10.598	10.648

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090823\
Data File : PO097827.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2023 10:28
Operator : YP/AJ
Sample : 04299-10RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TWP-01RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/11/2023
Supervised By :Ankita Jodhani 09/11/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 15:51:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090623.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 07 02:56:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

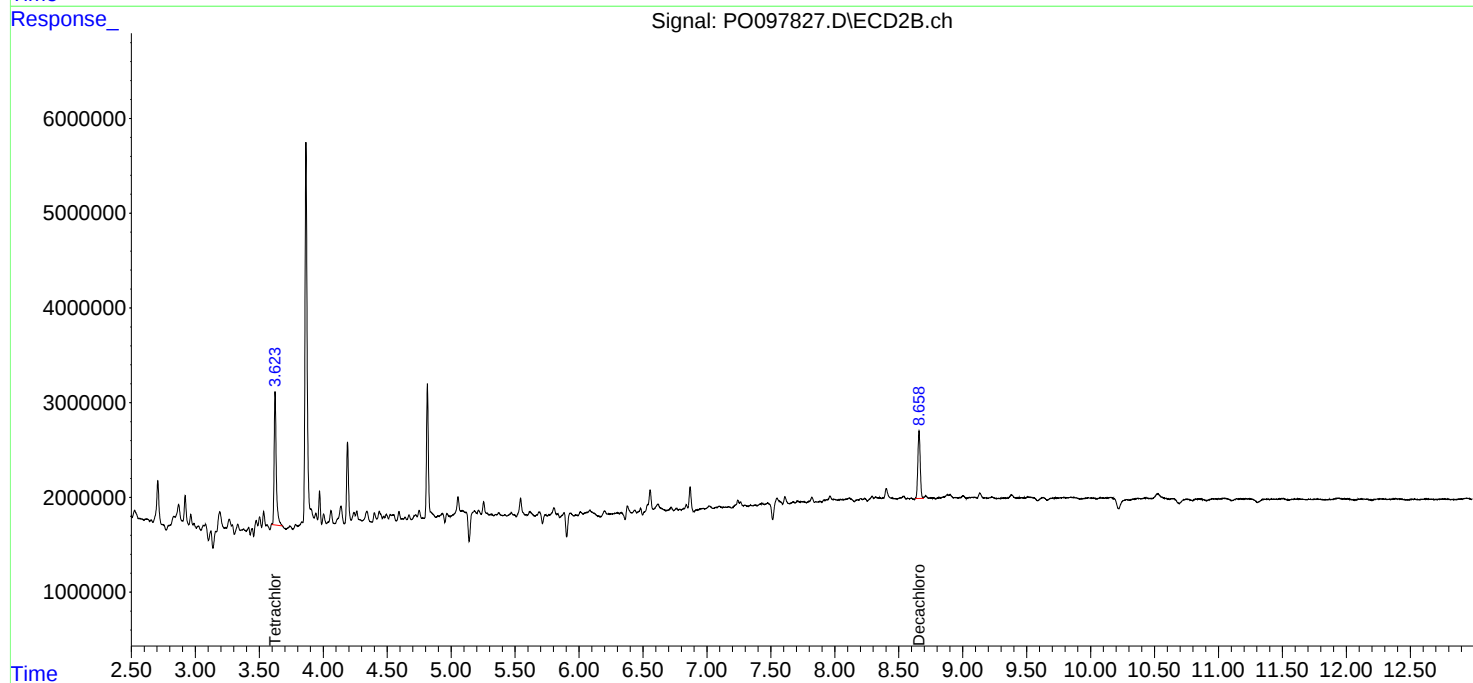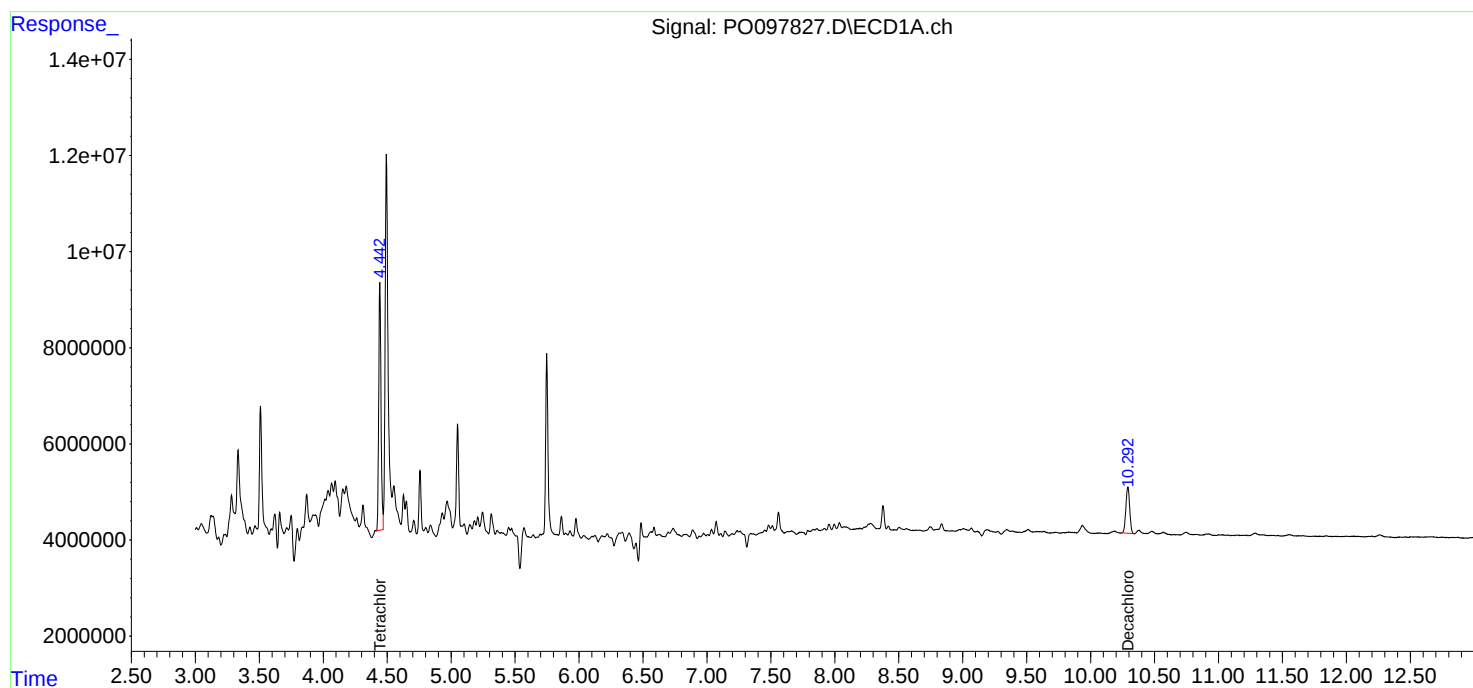

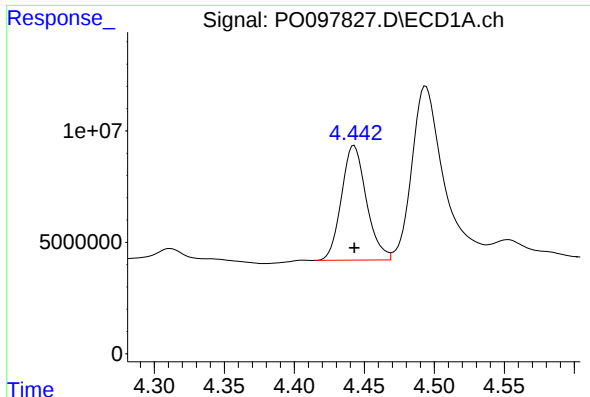


#1 Tetrachloro-m-xylene

R.T.: 4.442 min
Delta R.T.: -0.001 min
Response: 63742011
Conc: 16.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
TWP-01RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/11/2023
Supervised By :Ankita Jodhani 09/11/2023

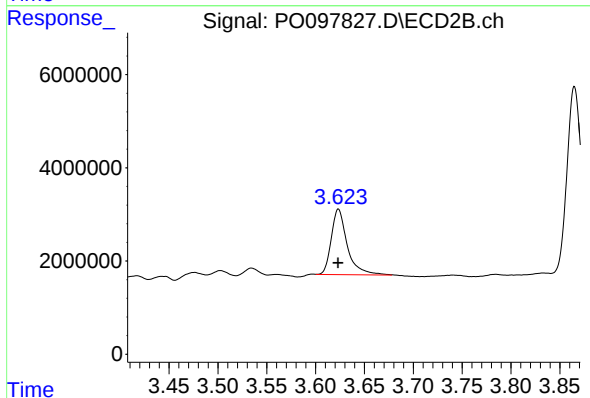


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: 0.000 min
Response: 15987716
Conc: 16.69 ng/ml m

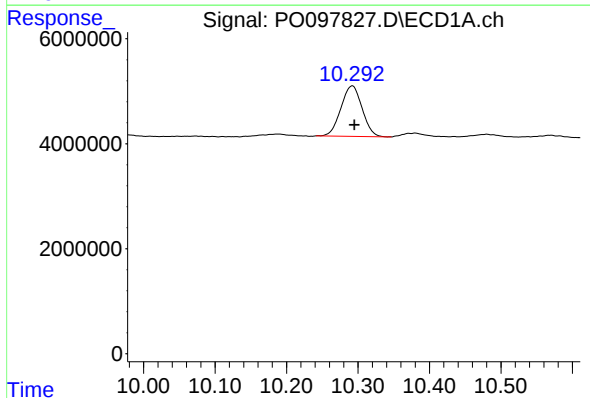

#2 Decachlorobiphenyl

R.T.: 10.292 min
Delta R.T.: -0.003 min
Response: 19801995
Conc: 10.60 ng/ml

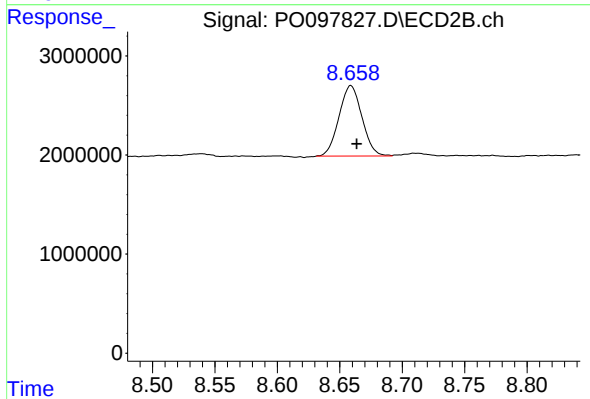

#2 Decachlorobiphenyl

R.T.: 8.659 min
Delta R.T.: -0.005 min
Response: 9097233
Conc: 10.65 ng/ml