

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090823\
 Data File : P0097847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2023 16:07
 Operator : YP/AJ
 Sample : 04336-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TRENCH-B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/11/2023
 Supervised By :Ankita Jodhani 09/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 16:39:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 07 02:56:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.441	3.621	76978481	19747844	19.322	20.620
2) SA Decachlor...	10.287	8.655	26209555	12150929	14.027	14.222m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090823\
Data File : PO097847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2023 16:07
Operator : YP/AJ
Sample : 04336-03
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TRENCH-B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/11/2023
Supervised By :Ankita Jodhani 09/11/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 16:39:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090623.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 07 02:56:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

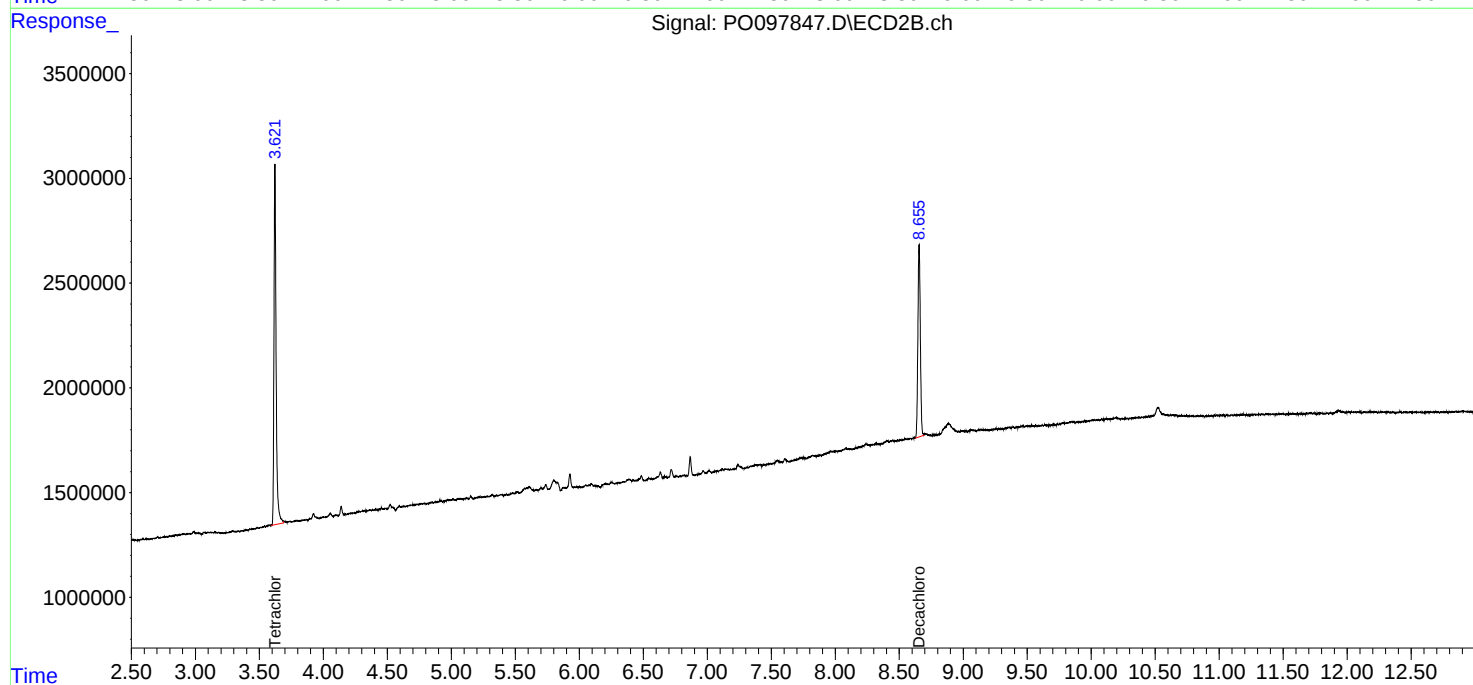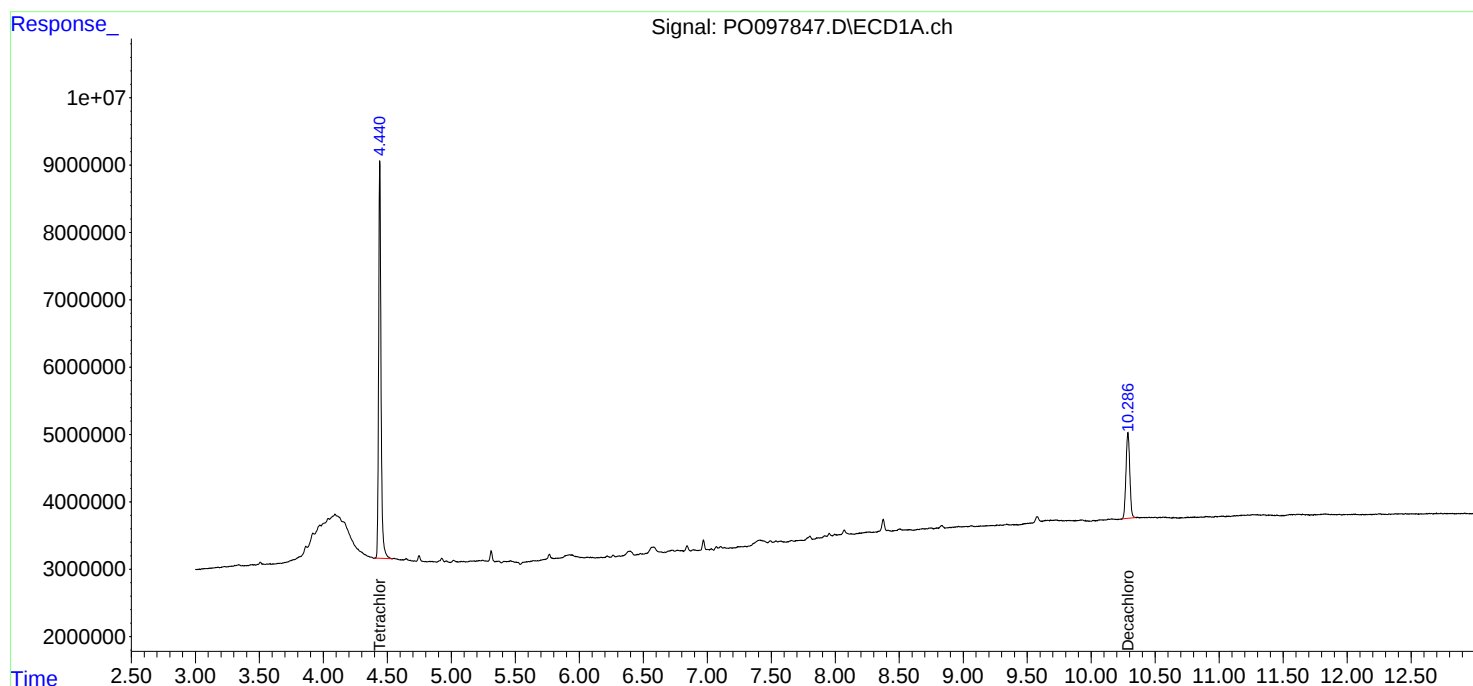

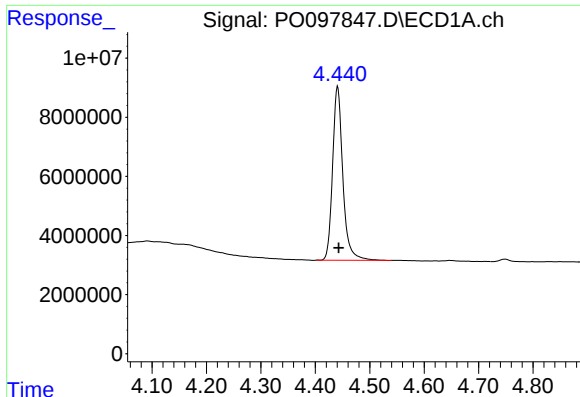


#1 Tetrachloro-m-xylene

R.T.: 4.441 min
Delta R.T.: -0.002 min
Response: 76978481
Conc: 19.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRENCH-B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/11/2023
Supervised By :Ankita Jodhani 09/11/2023

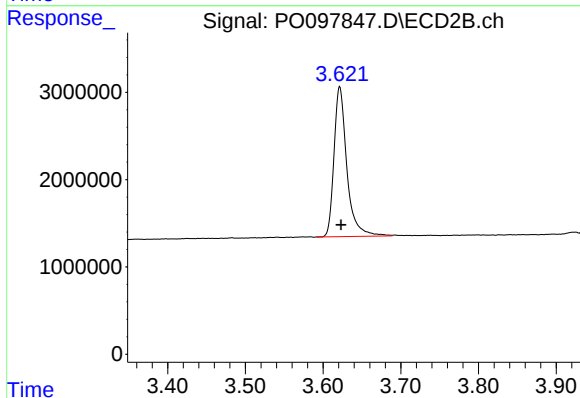


#1 Tetrachloro-m-xylene

R.T.: 3.621 min
Delta R.T.: -0.002 min
Response: 19747844
Conc: 20.62 ng/ml

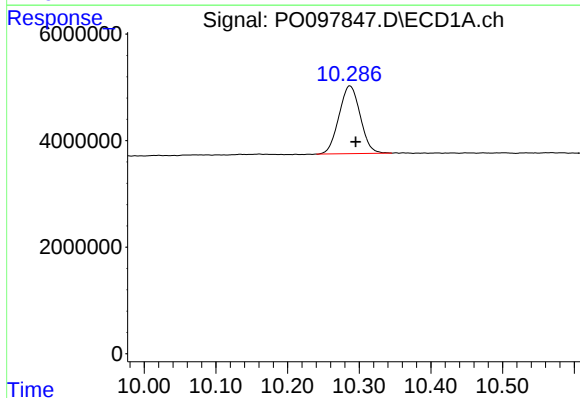

#2 Decachlorobiphenyl

R.T.: 10.287 min
Delta R.T.: -0.008 min
Response: 26209555
Conc: 14.03 ng/ml

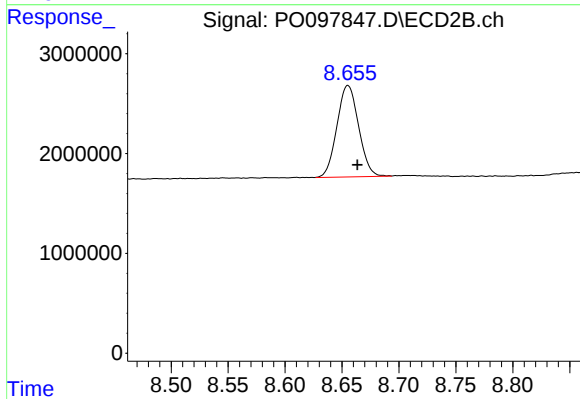

#2 Decachlorobiphenyl

R.T.: 8.655 min
Delta R.T.: -0.009 min
Response: 12150929
Conc: 14.22 ng/ml m