

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090919\
 Data File : P0060540.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Sep 2019 9:33
 Operator : SM/AJ
 Sample : K4761-01 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ADLER-BOX-090619

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 12:07:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Sep 08 02:12:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.378	3.535	117912	116771	2.842	3.802 #
2)	SA Decachlor...	10.042	8.428	209006	165127	3.962	4.461

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090919\
Data File : PO060540.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Sep 2019 9:33
Operator : SM/AJ
Sample : K4761-01 5X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ADLER-BOX-090619

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 12:07:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Sep 08 02:12:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

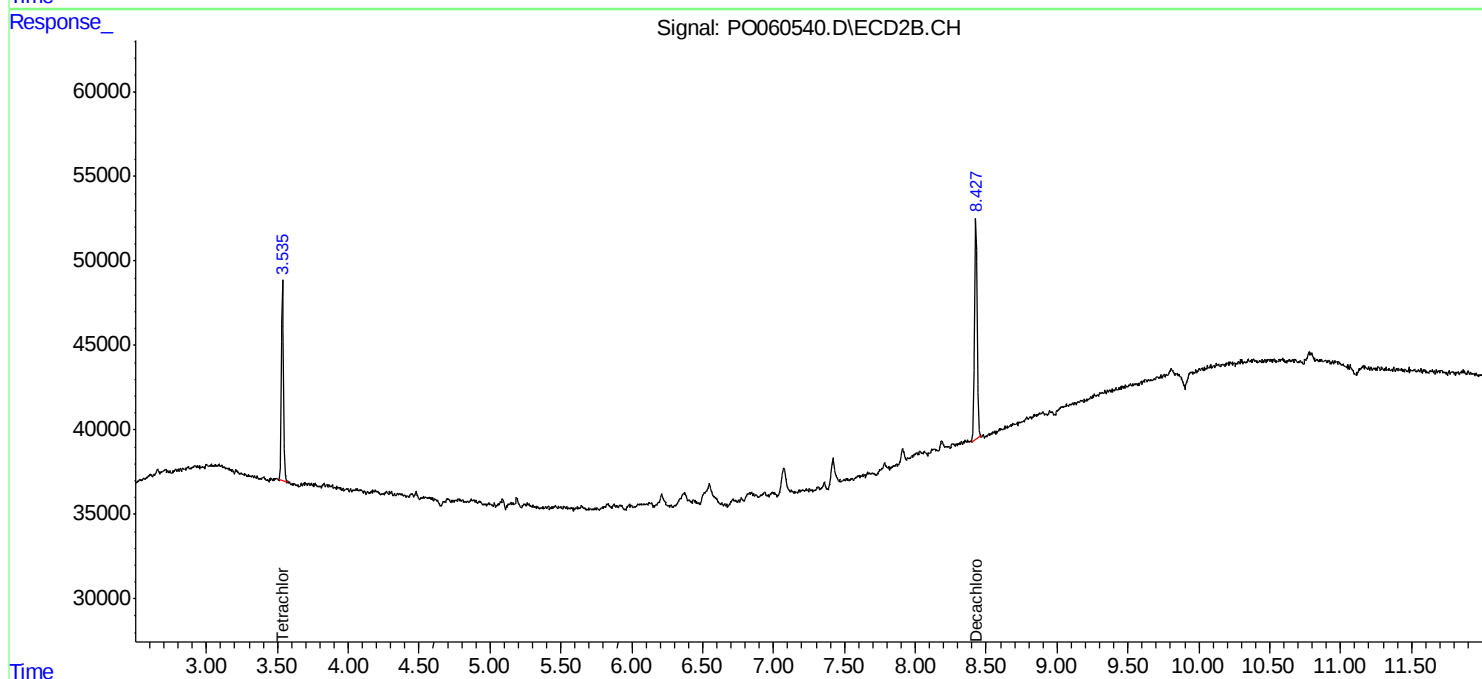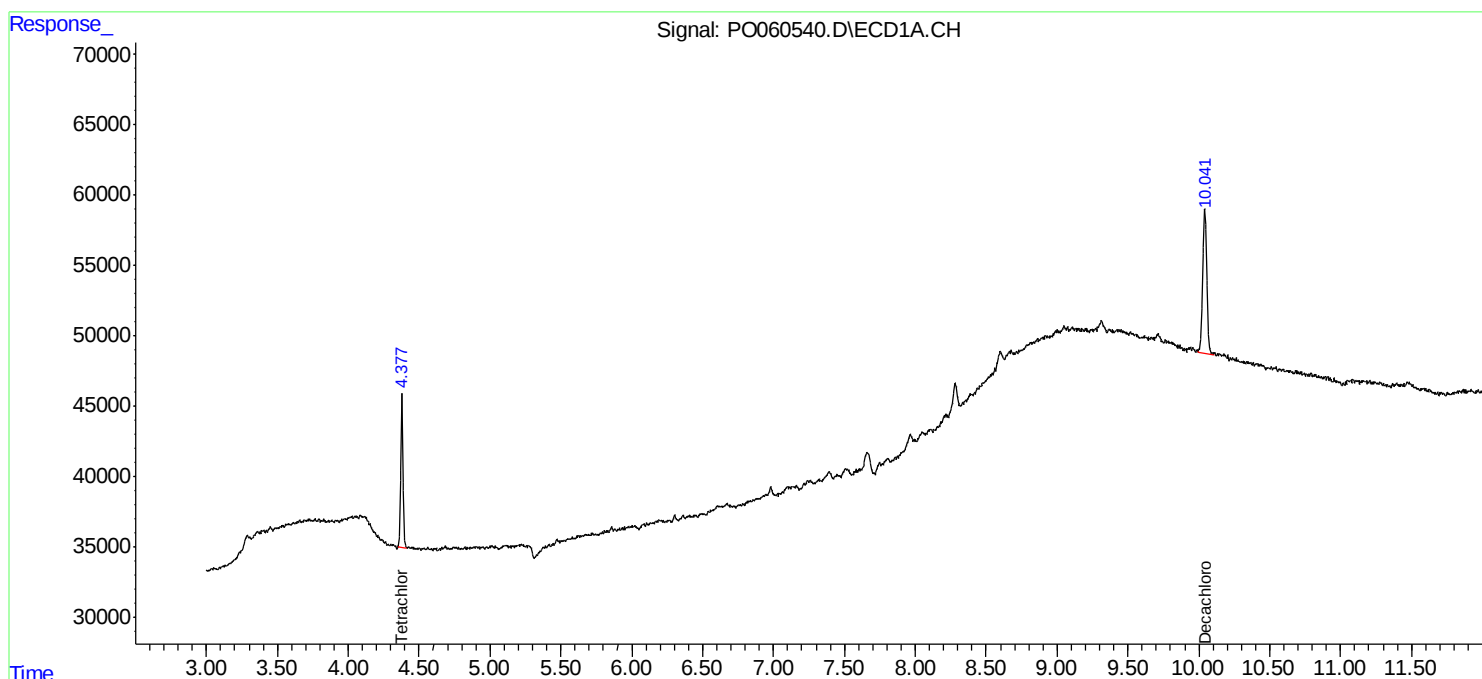


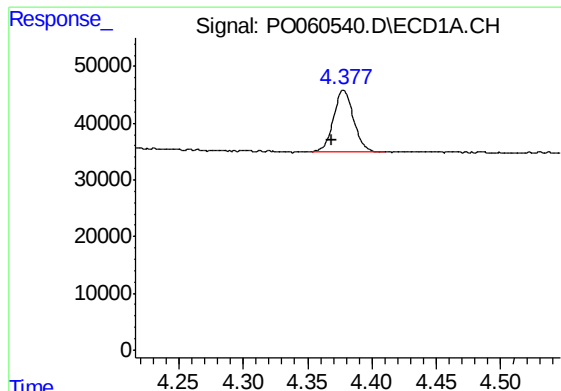

#1 Tetrachloro-m-xylene


R.T.: 4.378 min
Delta R.T.: 0.009 min
Response: 117912
Conc: 2.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
ADLER-BOX-090619

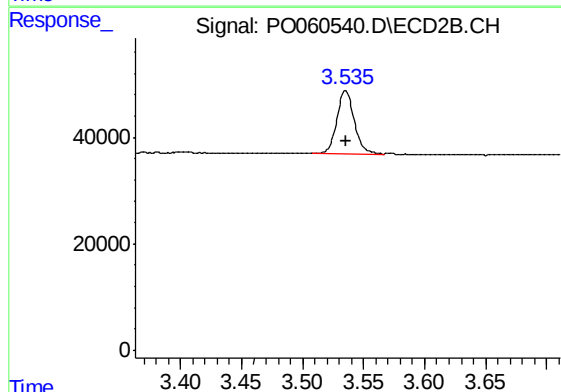


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 116771
Conc: 3.80 ng/ml

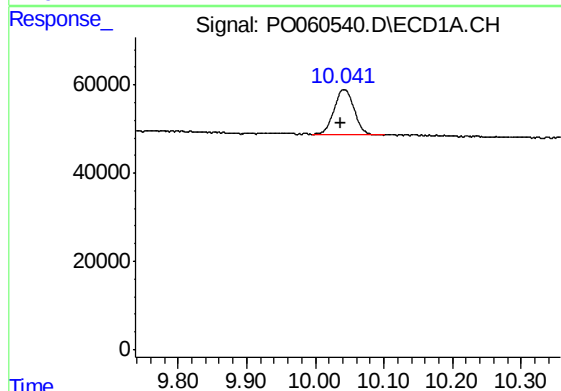

#2 Decachlorobiphenyl

R.T.: 10.042 min
Delta R.T.: 0.005 min
Response: 209006
Conc: 3.96 ng/ml

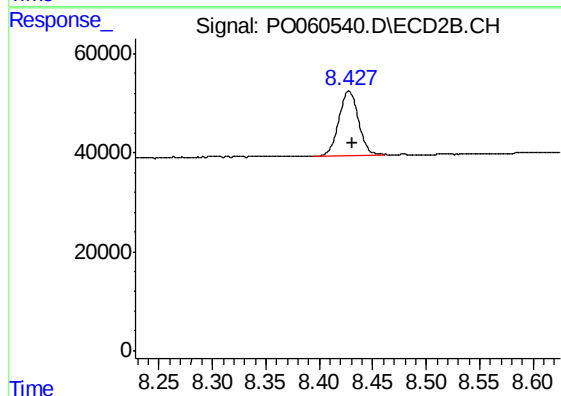

#2 Decachlorobiphenyl

R.T.: 8.428 min
Delta R.T.: -0.003 min
Response: 165127
Conc: 4.46 ng/ml