

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090919\
 Data File : P0060541.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Sep 2019 9:49
 Operator : SM/AJ
 Sample : K4763-01 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FDS-1

Manual Integrations
 APPROVED

Ankita
 9/10/2019 1:52:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 14:13:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Sep 08 02:12:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.366	3.534	116256	70401	2.802	2.292
2) SA Decachlor...	10.031	8.423	86672	76427	1.643	2.065 #
Target Compounds						
26) L6 AR-1254-1	6.382	5.376	95391	75127	52.306m	39.596m
27) L6 AR-1254-2	6.602	5.518	141903	68711	48.963m	40.206m
28) L6 AR-1254-3	6.969	5.914	146596	121093	45.967m	43.177m
29) L6 AR-1254-4	7.251	6.140	122769	63057	51.125m	35.295 #
30) L6 AR-1254-5	7.668	6.550	198200	142094	72.860m	54.152 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090919\
Data File : PO060541.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Sep 2019 9:49
Operator : SM/AJ
Sample : K4763-01 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FDS-1


Manual Integrations
APPROVED

Ankita
9/10/2019 1:52:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 14:13:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Sep 08 02:12:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

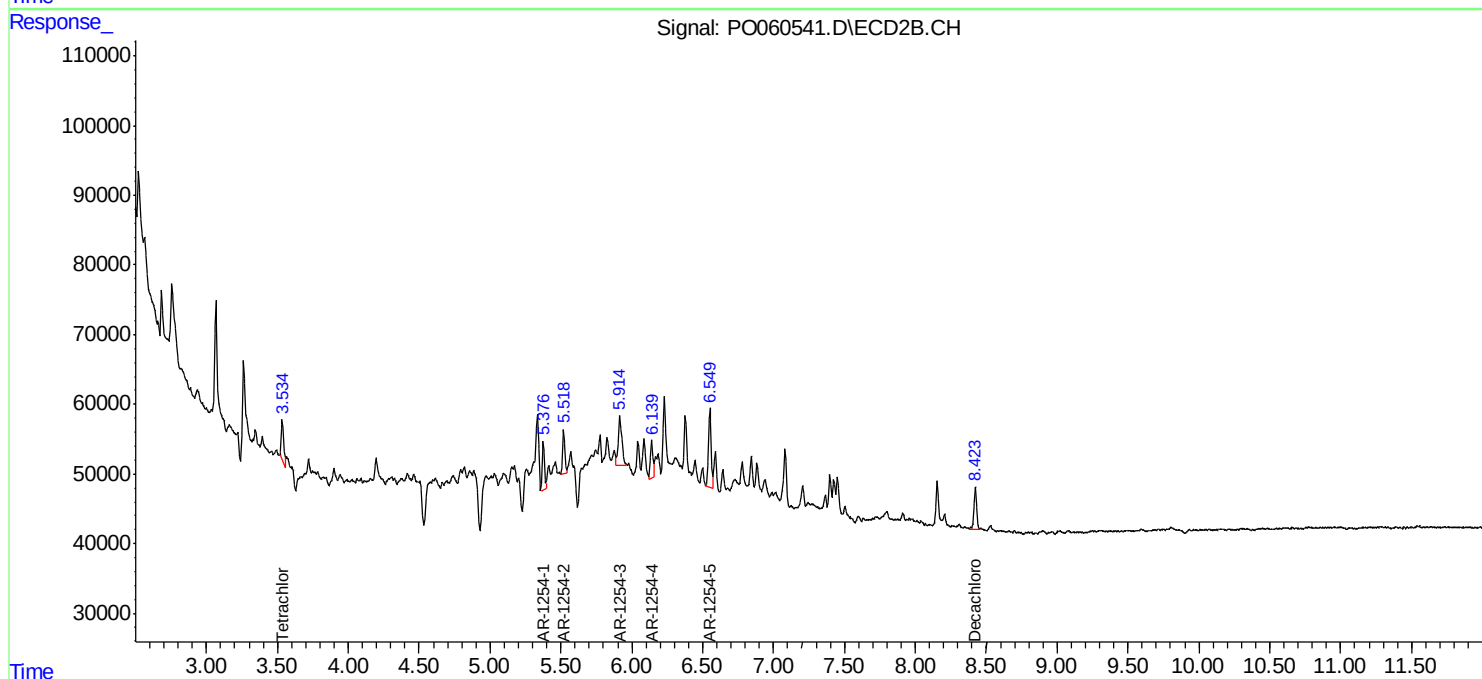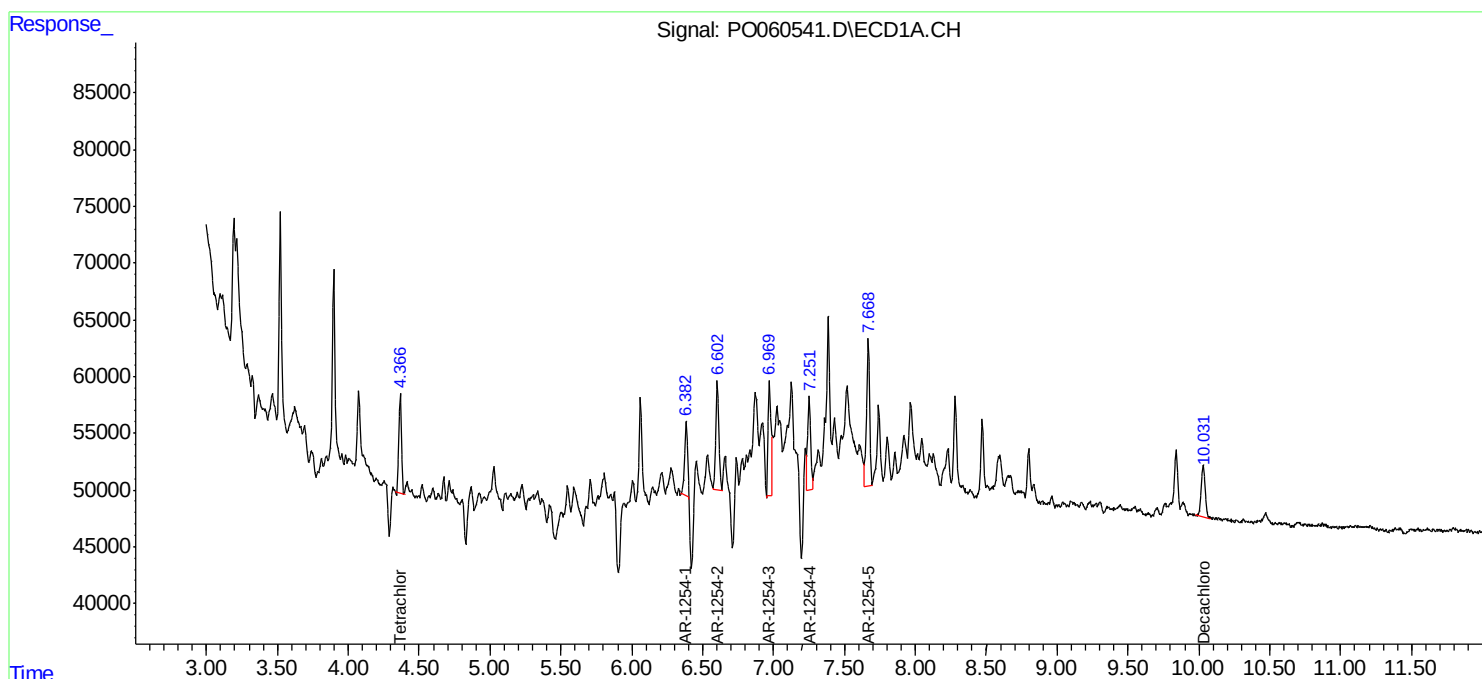

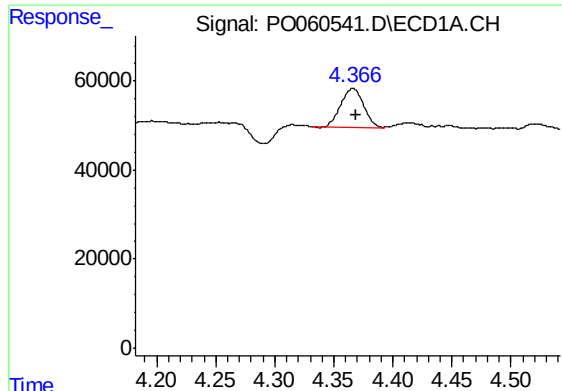


#1 Tetrachloro-m-xylene

R.T.: 4.366 min
Delta R.T.: -0.003 min
Response: 116256
Conc: 2.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
FDS-1


Manual Integrations
APPROVED

Ankita
9/10/2019 1:52:20 PM

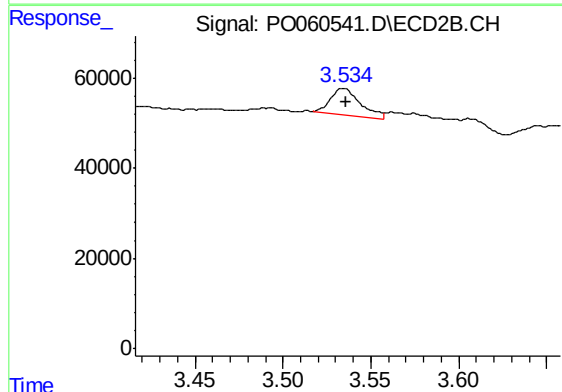


#1 Tetrachloro-m-xylene

R.T.: 3.534 min
Delta R.T.: -0.002 min
Response: 70401
Conc: 2.29 ng/ml

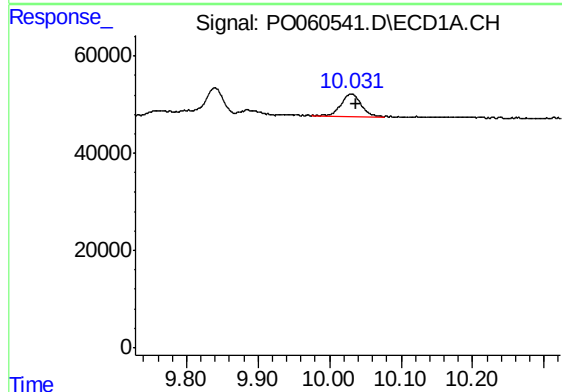


#2 Decachlorobiphenyl

R.T.: 10.031 min
Delta R.T.: -0.006 min
Response: 86672
Conc: 1.64 ng/ml

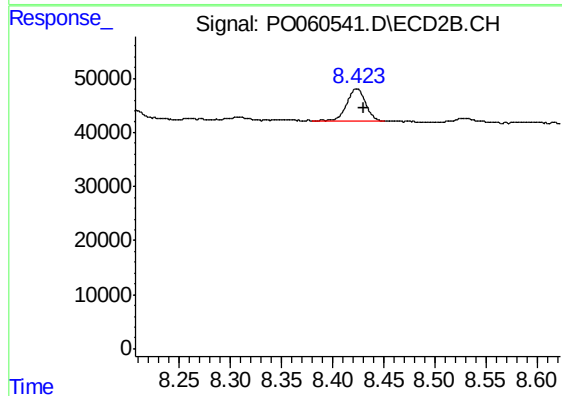

#2 Decachlorobiphenyl

R.T.: 8.423 min
Delta R.T.: -0.008 min
Response: 76427
Conc: 2.06 ng/ml

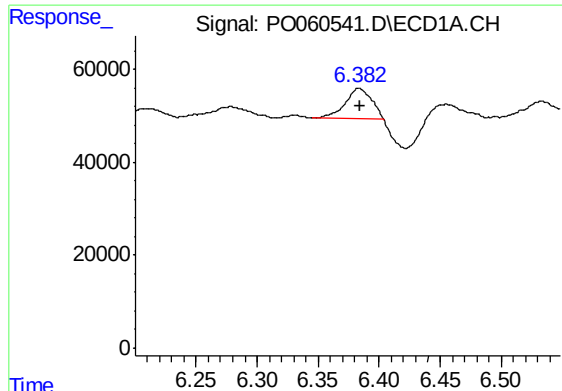


#26 AR-1254-1

R.T.: 6.382 min
Delta R.T.: -0.002 min
Response: 95391
Conc: 52.31 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FDS-1


Manual Integrations
APPROVED

Ankita
9/10/2019 1:52:20 PM

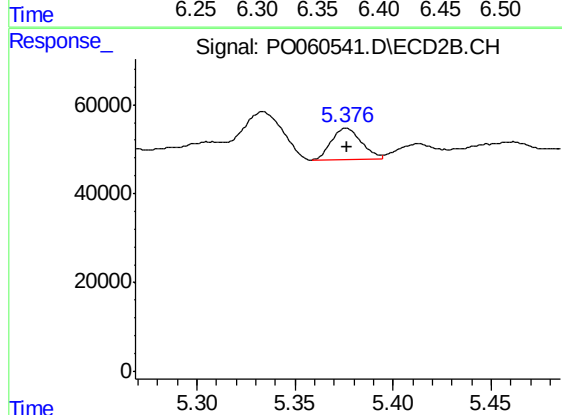


#26 AR-1254-1

R.T.: 5.376 min
Delta R.T.: -0.001 min
Response: 75127
Conc: 39.60 ng/ml m

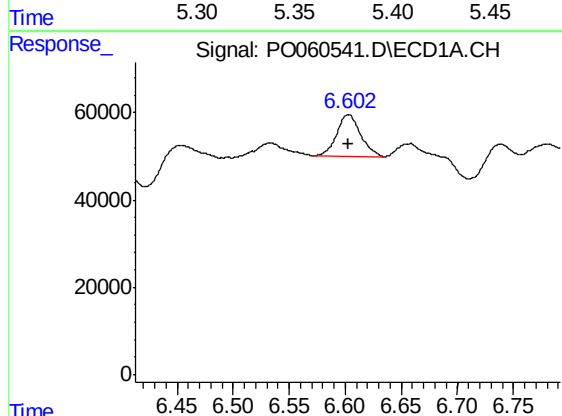


#27 AR-1254-2

R.T.: 6.602 min
Delta R.T.: 0.000 min
Response: 141903
Conc: 48.96 ng/ml m

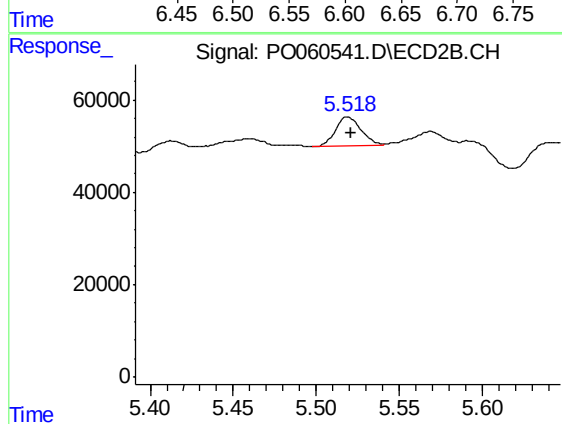

#27 AR-1254-2

R.T.: 5.518 min
Delta R.T.: -0.003 min
Response: 68711
Conc: 40.21 ng/ml m

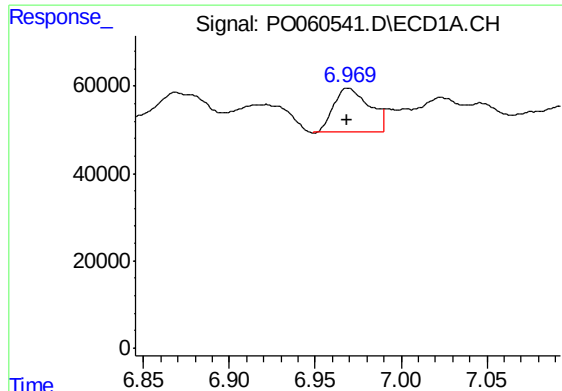


#28 AR-1254-3

R.T.: 6.969 min
Delta R.T.: 0.000 min
Response: 146596
Conc: 45.97 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FDS-1


Manual Integrations
APPROVED

Ankita
9/10/2019 1:52:20 PM

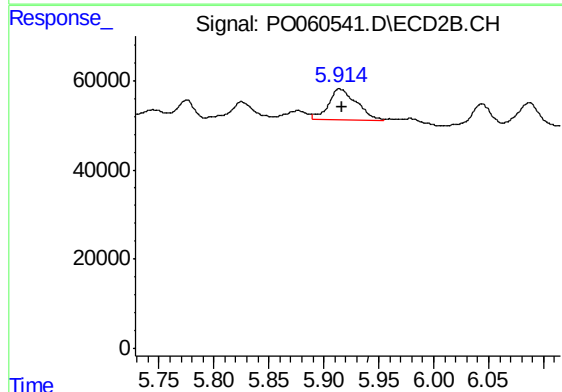


#28 AR-1254-3

R.T.: 5.914 min
Delta R.T.: -0.003 min
Response: 121093
Conc: 43.18 ng/ml m

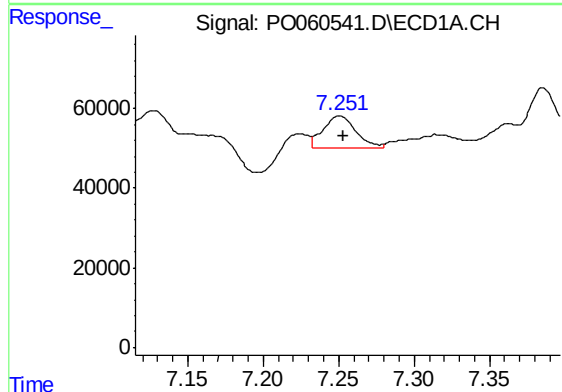


#29 AR-1254-4

R.T.: 7.251 min
Delta R.T.: -0.002 min
Response: 122769
Conc: 51.13 ng/ml m

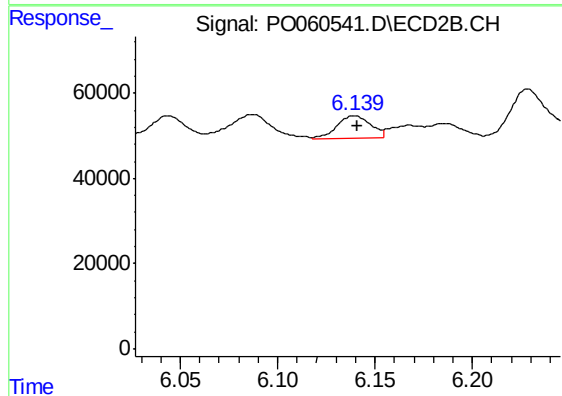

#29 AR-1254-4

R.T.: 6.140 min
Delta R.T.: 0.000 min
Response: 63057
Conc: 35.30 ng/ml

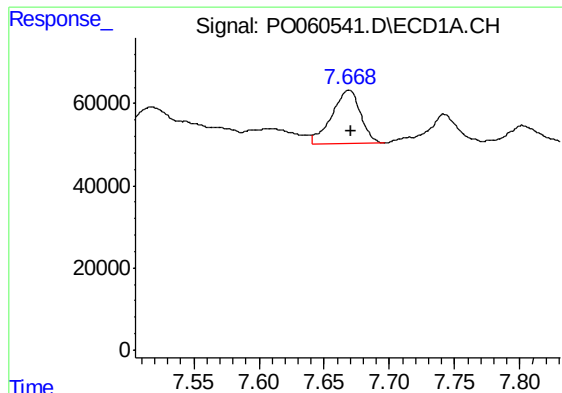


#30 AR-1254-5

R.T.: 7.668 min
Delta R.T.: -0.003 min
Response: 198200
Conc: 72.86 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FDS-1

Manual Integrations
APPROVED

Ankita
9/10/2019 1:52:20 PM

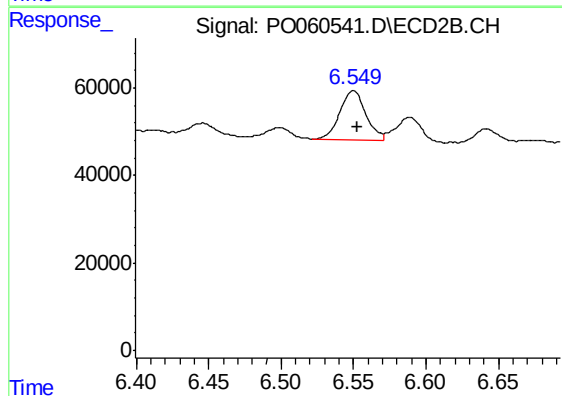

#30 AR-1254-5

R.T.: 6.550 min
Delta R.T.: -0.003 min
Response: 142094
Conc: 54.15 ng/ml