

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090919\
 Data File : P0060542.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Sep 2019 10:06
 Operator : SM/AJ
 Sample : K4763-02 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DSC-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 12:09:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Sep 08 02:12:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.535	55139	57134	1.329	1.860 #
2) SA Decachlor...	10.033	8.426	59264	43622	1.123	1.178

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090919\
Data File : PO060542.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Sep 2019 10:06
Operator : SM/AJ
Sample : K4763-02 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DSC-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 12:09:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Sep 08 02:12:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

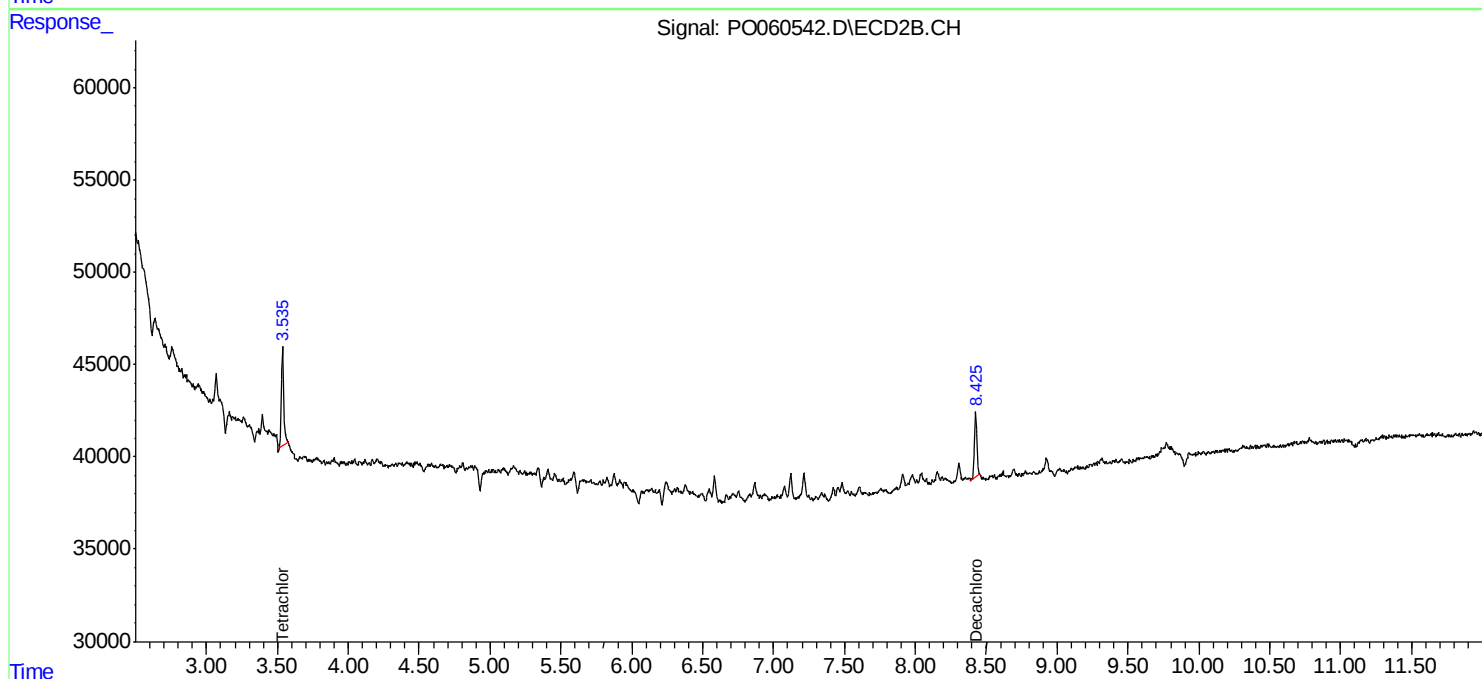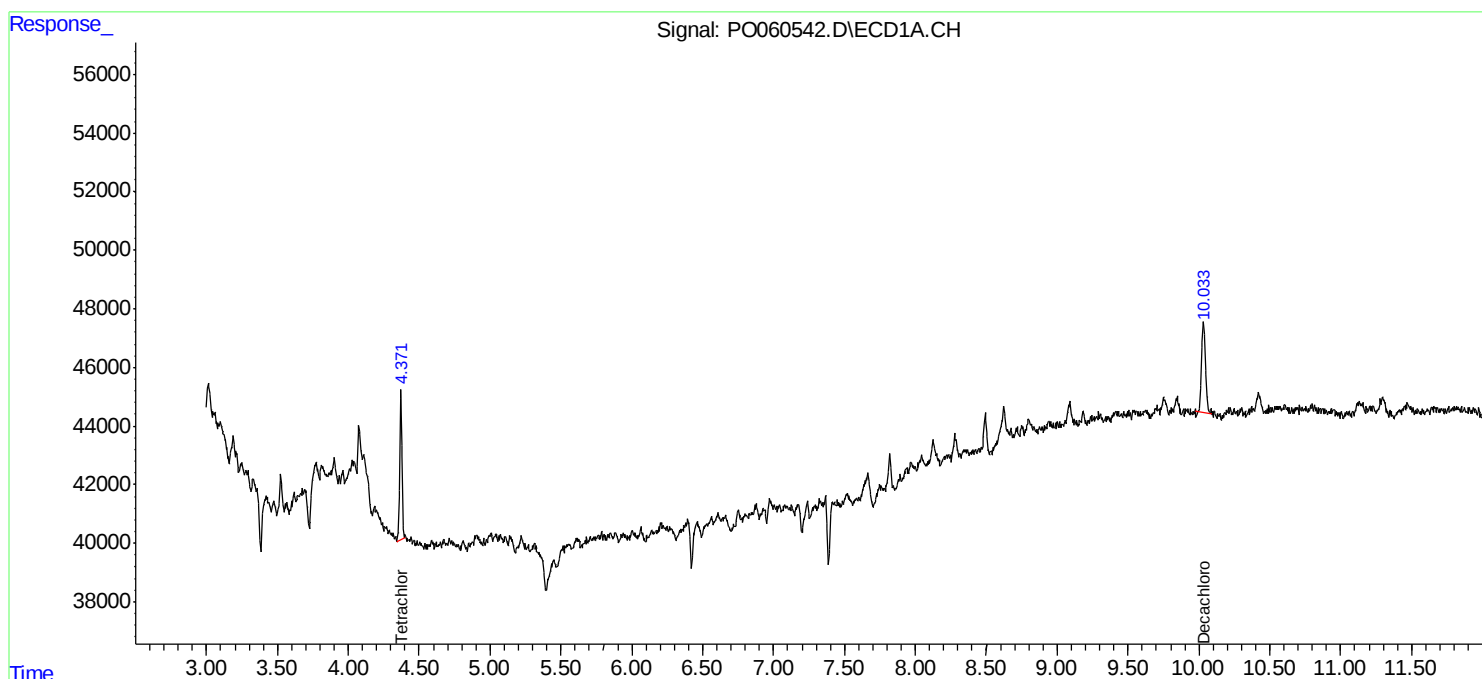


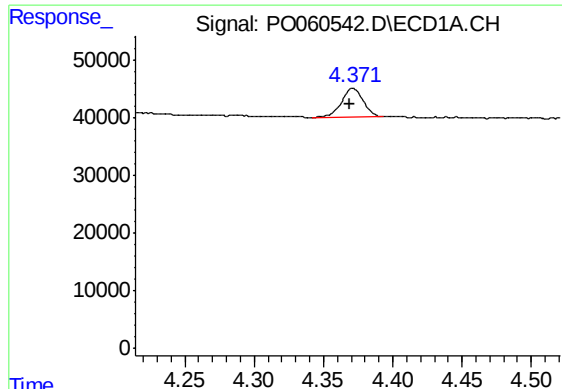

#1 Tetrachloro-m-xylene


R.T.: 4.371 min
Delta R.T.: 0.002 min
Response: 55139
Conc: 1.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
DSC-1

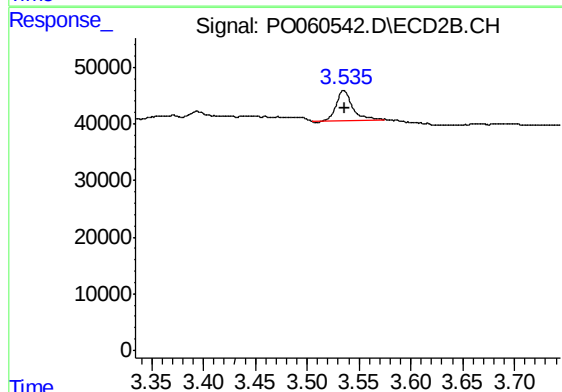


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 57134
Conc: 1.86 ng/ml

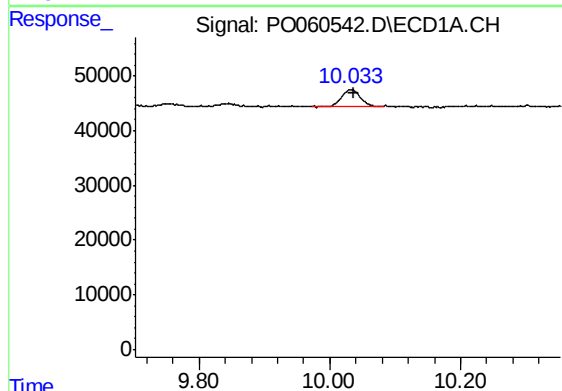

#2 Decachlorobiphenyl

R.T.: 10.033 min
Delta R.T.: -0.004 min
Response: 59264
Conc: 1.12 ng/ml

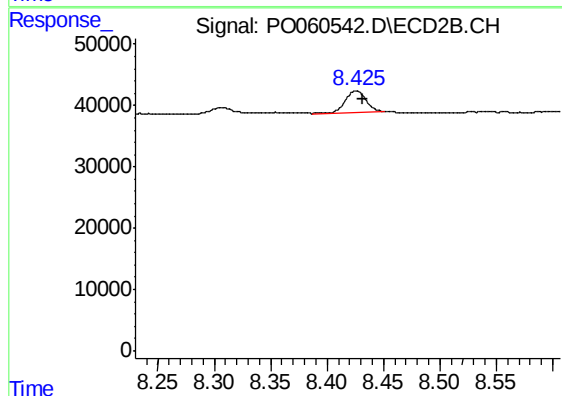

#2 Decachlorobiphenyl

R.T.: 8.426 min
Delta R.T.: -0.005 min
Response: 43622
Conc: 1.18 ng/ml