

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090919\
 Data File : P0060548.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Sep 2019 11:48
 Operator : SM/AJ
 Sample : K4650-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-2

Manual Integrations
 APPROVED

Ankita
 9/10/2019 1:52:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 12:12:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Sep 08 02:12:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.372	3.535	707581	632153	17.053	20.581
2)	SA Decachlor...	10.033	8.425	736816	574007	13.968	15.506
Target Compounds							
26)	L6 AR-1254-1	6.386	5.374	20476	30003	11.228	15.813 #
27)	L6 AR-1254-2	6.602	5.518	187776	58325	64.792m	34.129 #
28)	L6 AR-1254-3	6.969	5.912	124294	113055	38.974	40.311m
29)	L6 AR-1254-4	7.253	6.137	115383	64865	48.049	36.308m
30)	L6 AR-1254-5	7.669	6.548	270486	242584	99.433	92.448m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090919\
Data File : PO060548.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Sep 2019 11:48
Operator : SM/AJ
Sample : K4650-03
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-2


Manual Integrations
APPROVED

Ankita
9/10/2019 1:52:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 12:12:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Sep 08 02:12:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

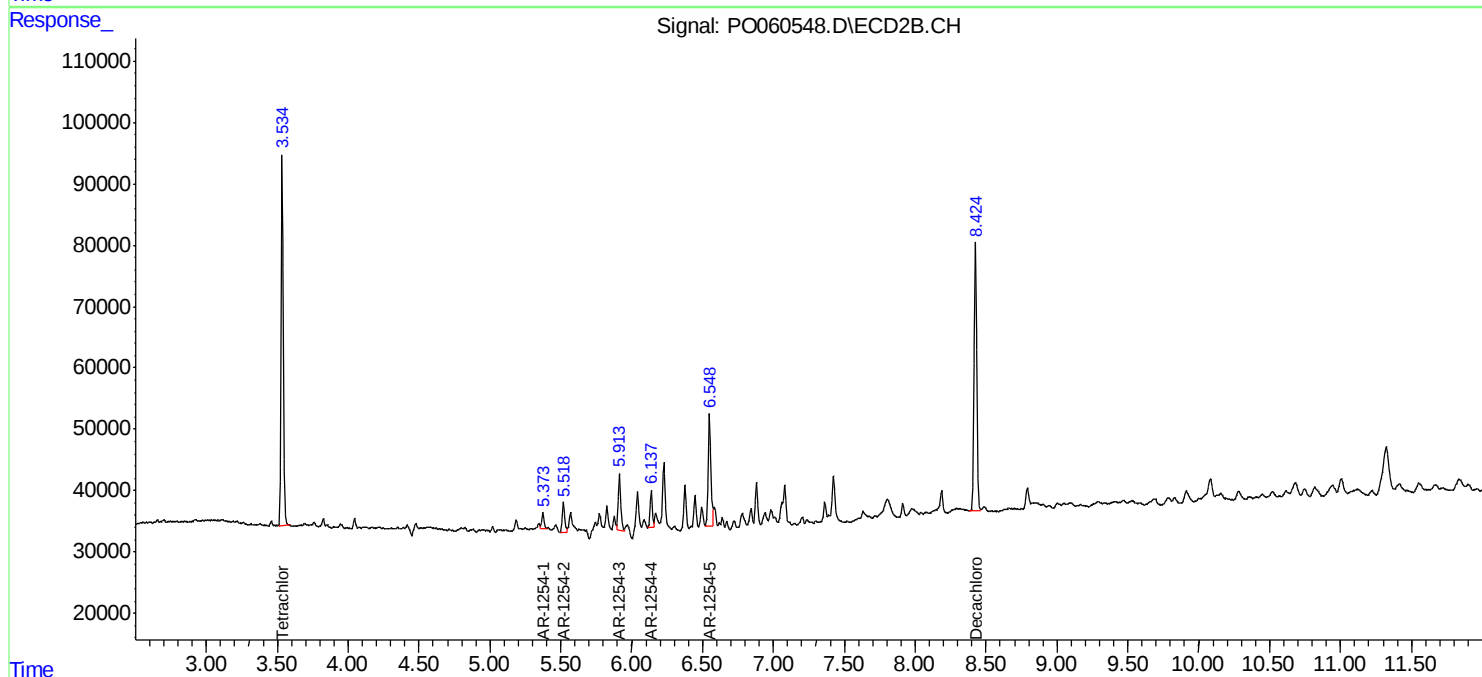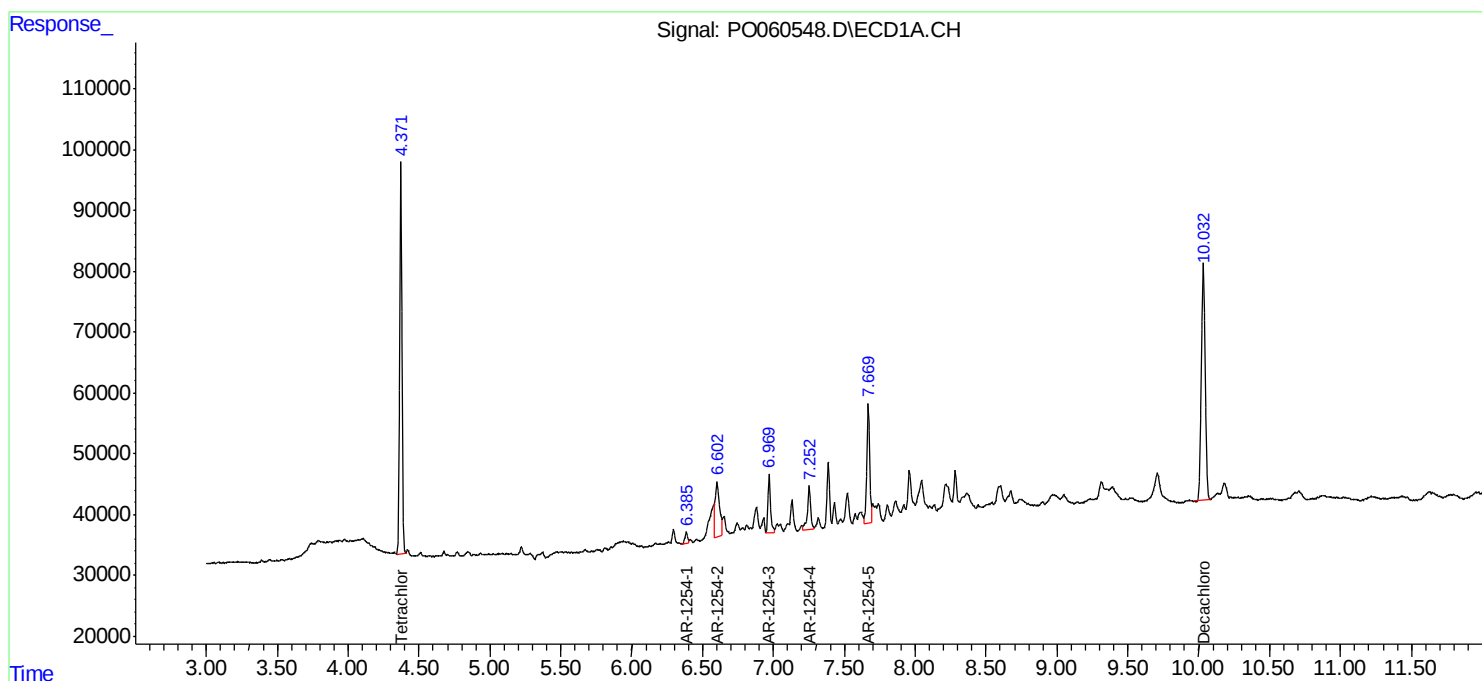

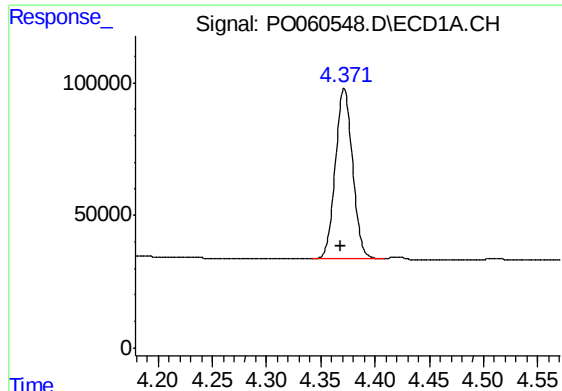


#1 Tetrachloro-m-xylene

R.T.: 4.372 min
Delta R.T.: 0.003 min
Response: 707581
Conc: 17.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
9/10/2019 1:52:23 PM

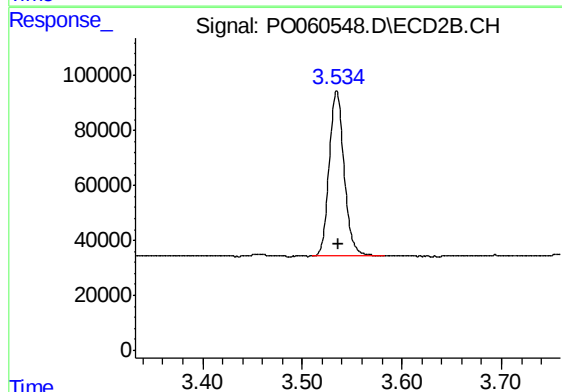


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: -0.001 min
Response: 632153
Conc: 20.58 ng/ml

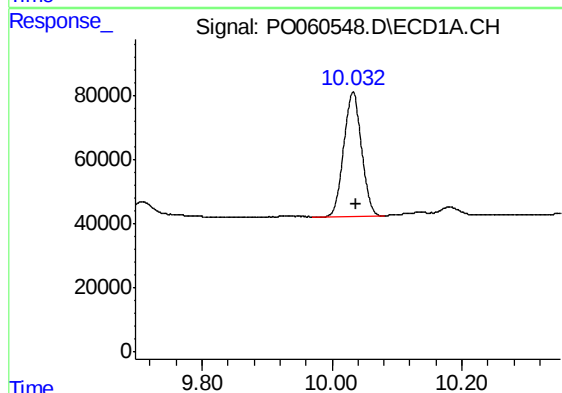


#2 Decachlorobiphenyl

R.T.: 10.033 min
Delta R.T.: -0.004 min
Response: 736816
Conc: 13.97 ng/ml

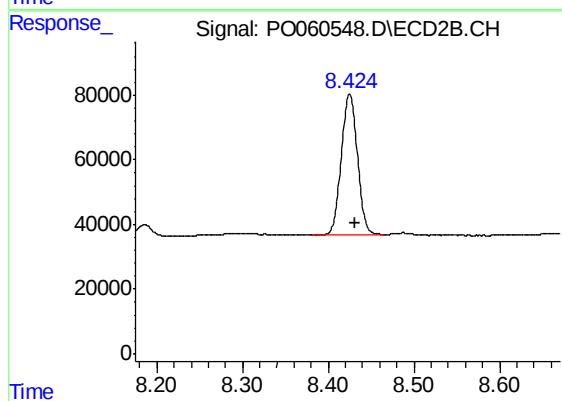

#2 Decachlorobiphenyl

R.T.: 8.425 min
Delta R.T.: -0.006 min
Response: 574007
Conc: 15.51 ng/ml

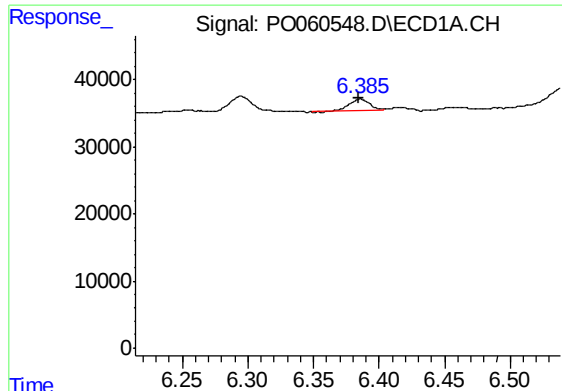


#26 AR-1254-1

R.T.: 6.386 min
Delta R.T.: 0.001 min
Response: 20476
Conc: 11.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
9/10/2019 1:52:23 PM

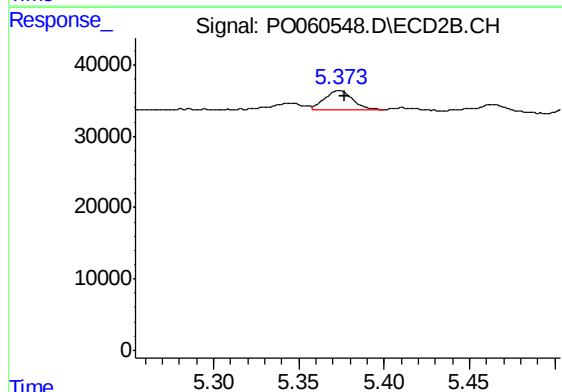


#26 AR-1254-1

R.T.: 5.374 min
Delta R.T.: -0.003 min
Response: 30003
Conc: 15.81 ng/ml

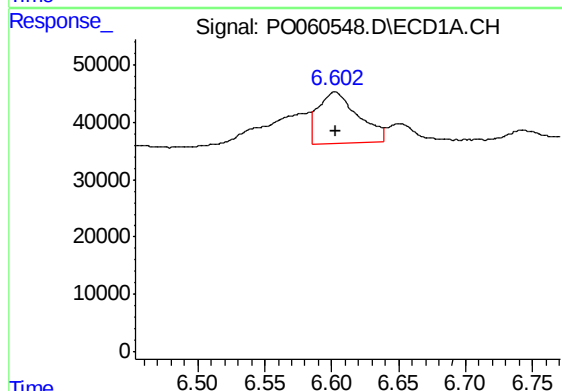


#27 AR-1254-2

R.T.: 6.602 min
Delta R.T.: 0.000 min
Response: 187776
Conc: 64.79 ng/ml m

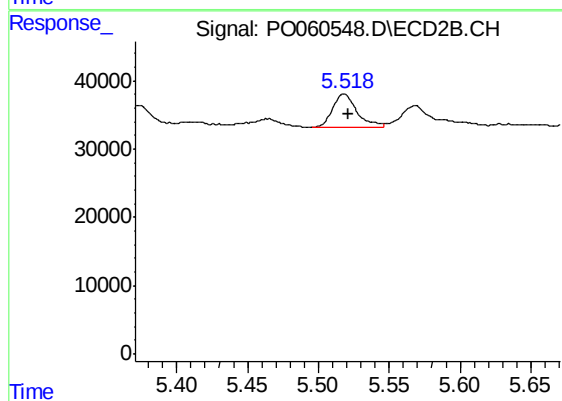

#27 AR-1254-2

R.T.: 5.518 min
Delta R.T.: -0.003 min
Response: 58325
Conc: 34.13 ng/ml

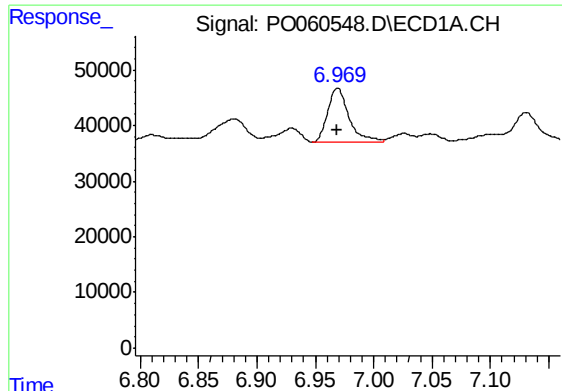


#28 AR-1254-3

R.T.: 6.969 min
Delta R.T.: 0.000 min
Response: 124294
Conc: 38.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
9/10/2019 1:52:23 PM

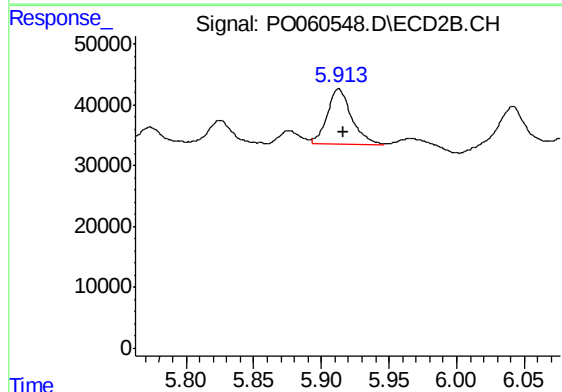


#28 AR-1254-3

R.T.: 5.912 min
Delta R.T.: -0.004 min
Response: 113055
Conc: 40.31 ng/ml m

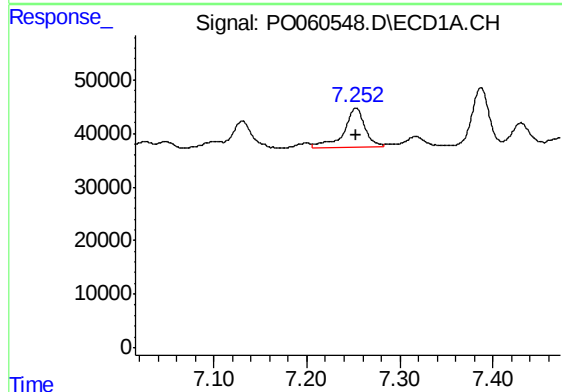


#29 AR-1254-4

R.T.: 7.253 min
Delta R.T.: 0.000 min
Response: 115383
Conc: 48.05 ng/ml

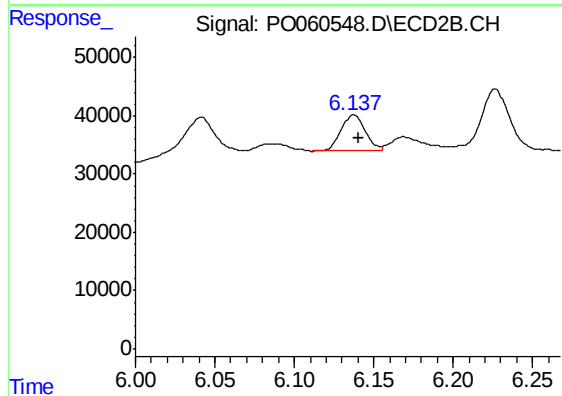

#29 AR-1254-4

R.T.: 6.137 min
Delta R.T.: -0.004 min
Response: 64865
Conc: 36.31 ng/ml m

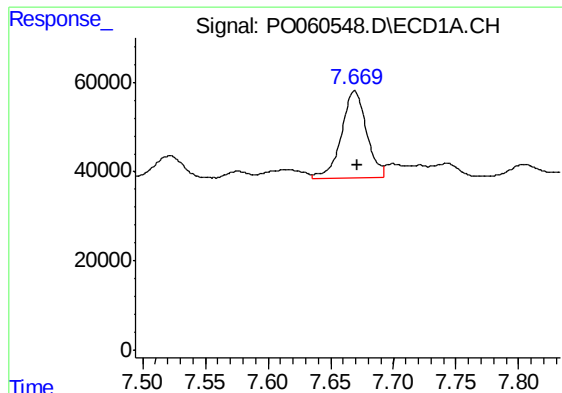


#30 AR-1254-5

R.T.: 7.669 min
Delta R.T.: -0.002 min
Response: 270486
Conc: 99.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2

Manual Integrations
APPROVED

Ankita
9/10/2019 1:52:23 PM

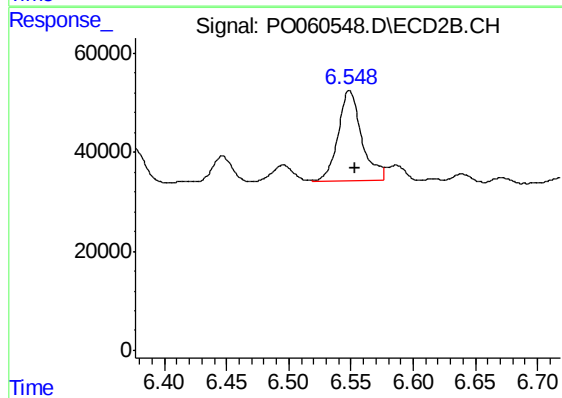

#30 AR-1254-5

R.T.: 6.548 min
Delta R.T.: -0.004 min
Response: 242584
Conc: 92.45 ng/ml m