

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090919\
 Data File : P0060590.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Sep 2019 1:39
 Operator : SM/AJ
 Sample : K4636-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-20-COMP

Manual Integrations
 APPROVED

Ankita
 9/10/2019 1:53:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 07:36:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Sep 08 02:12:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.367	3.534	876251	674017	21.118	21.944
2)	SA Decachlor...	10.027	8.421	1334029	1001752	25.290	27.061
Target Compounds							
31)	L7 AR-1260-1	7.125	6.037	279622	276071	111.862m	134.249
32)	L7 AR-1260-2	7.376	6.225	616282	245556	198.326	98.074m#
33)	L7 AR-1260-3	7.739	6.375	194540	176690	77.772	76.051
34)	L7 AR-1260-4	7.962	6.839	272426	140896	92.012	69.371
35)	L7 AR-1260-5	8.278	7.077	329492	333869	58.662	72.884m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090919\
Data File : PO060590.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Sep 2019 1:39
Operator : SM/AJ
Sample : K4636-04
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-20-COMP


Manual Integrations
APPROVED

Ankita
9/10/2019 1:53:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 07:36:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Sep 08 02:12:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

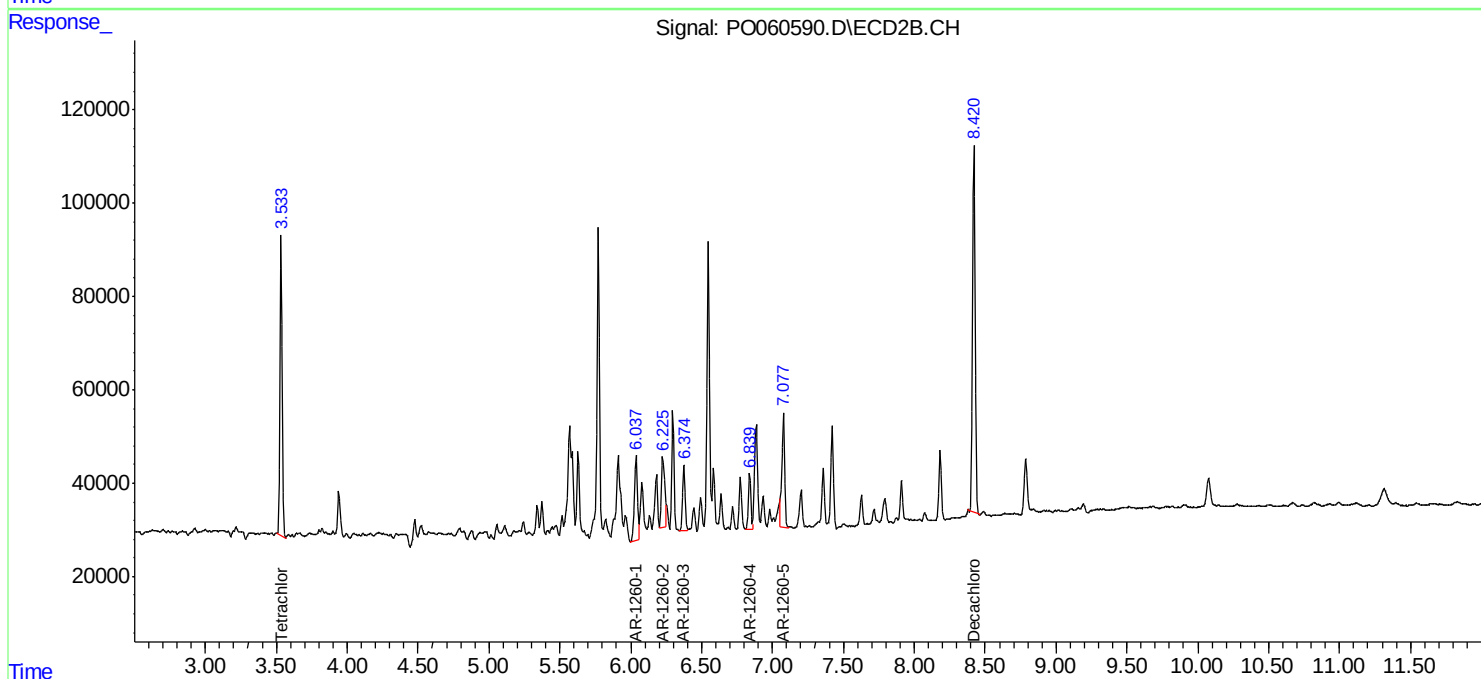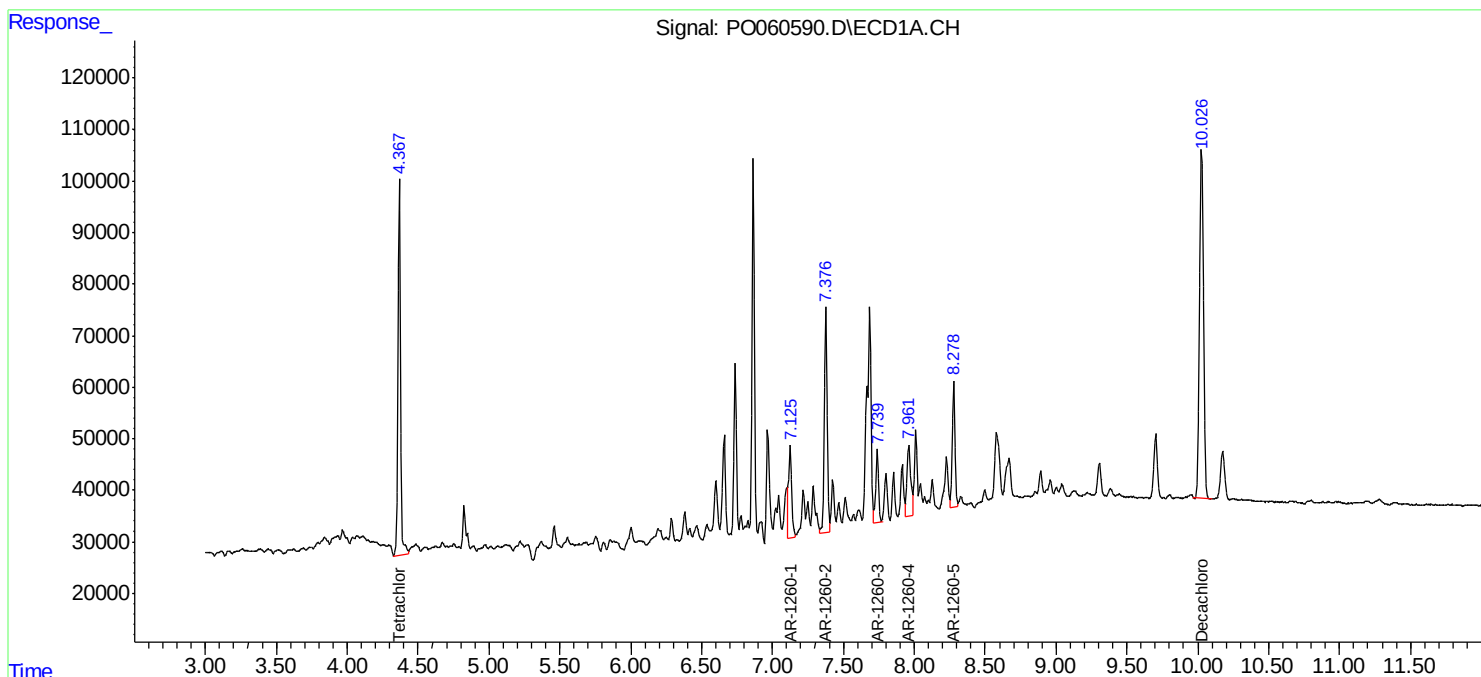

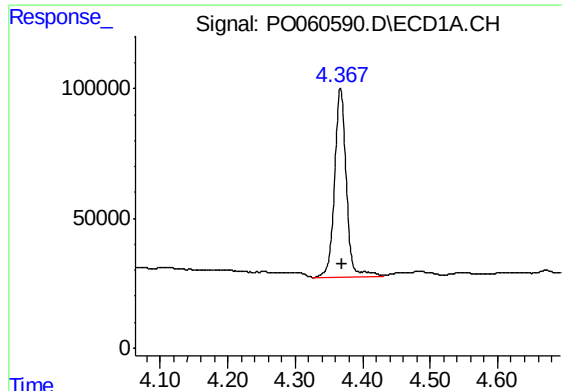


#1 Tetrachloro-m-xylene

R.T.: 4.367 min
Delta R.T.: -0.002 min
Response: 876251
Conc: 21.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-20-COMP


Manual Integrations
APPROVED

Ankita
9/10/2019 1:53:11 PM

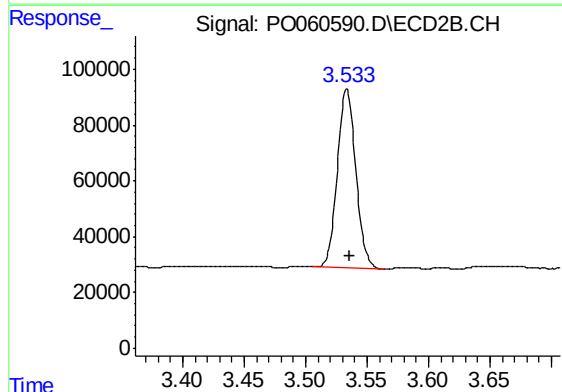


#1 Tetrachloro-m-xylene

R.T.: 3.534 min
Delta R.T.: -0.003 min
Response: 674017
Conc: 21.94 ng/ml

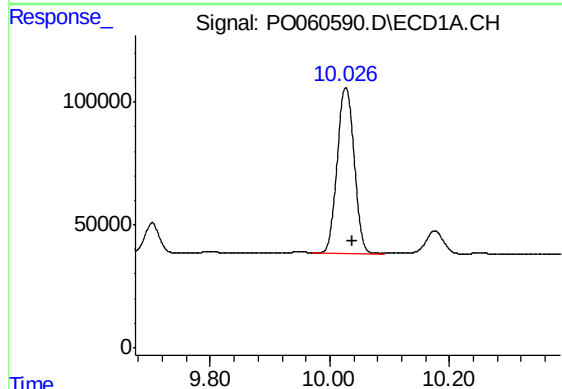


#2 Decachlorobiphenyl

R.T.: 10.027 min
Delta R.T.: -0.011 min
Response: 1334029
Conc: 25.29 ng/ml

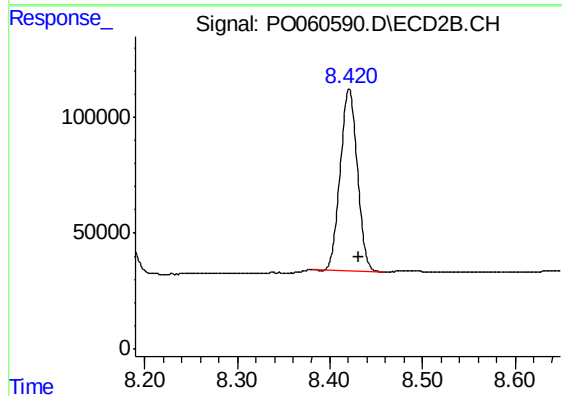

#2 Decachlorobiphenyl

R.T.: 8.421 min
Delta R.T.: -0.010 min
Response: 1001752
Conc: 27.06 ng/ml

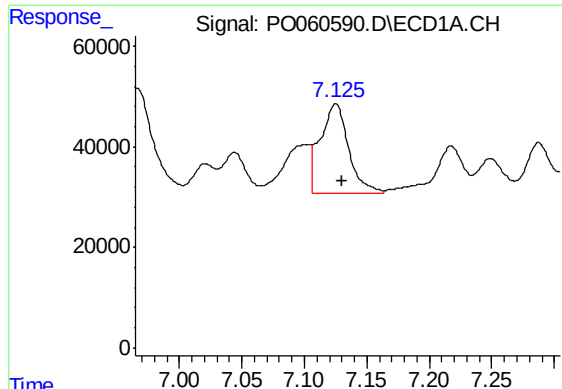


#31 AR-1260-1

R.T.: 7.125 min
Delta R.T.: -0.005 min
Response: 279622
Conc: 111.86 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-20-COMP


Manual Integrations
APPROVED

Ankita
9/10/2019 1:53:11 PM

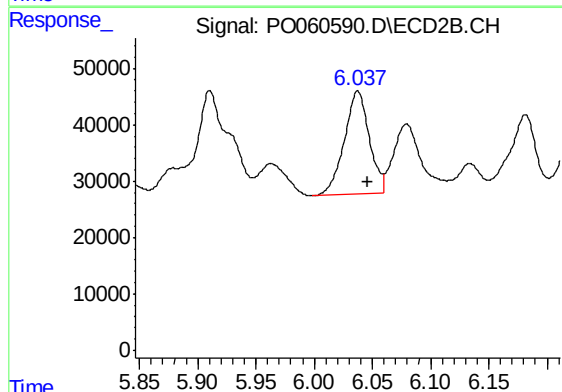


#31 AR-1260-1

R.T.: 6.037 min
Delta R.T.: -0.009 min
Response: 276071
Conc: 134.25 ng/ml

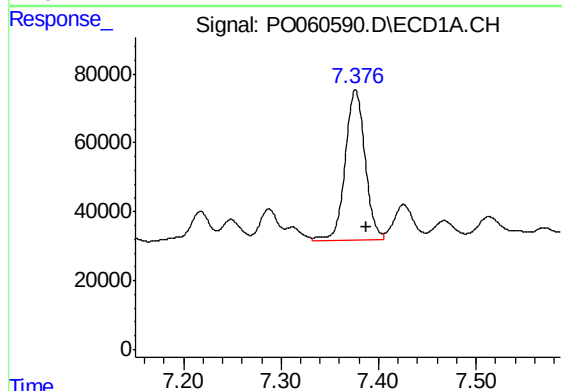


#32 AR-1260-2

R.T.: 7.376 min
Delta R.T.: -0.012 min
Response: 616282
Conc: 198.33 ng/ml

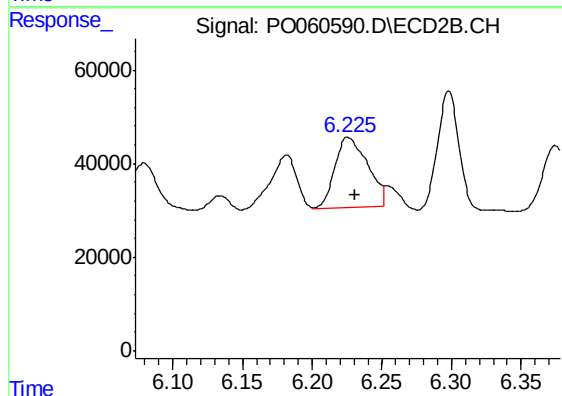

#32 AR-1260-2

R.T.: 6.225 min
Delta R.T.: -0.006 min
Response: 245556
Conc: 98.07 ng/ml m

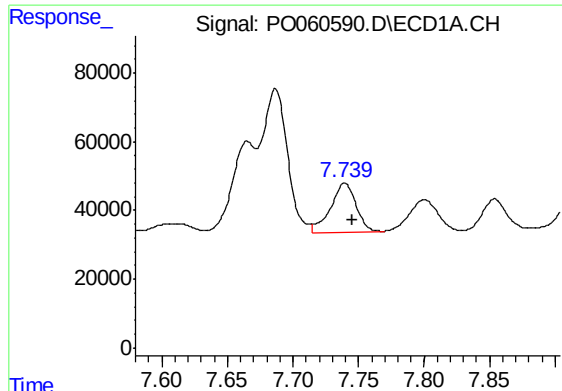


#33 AR-1260-3

R.T.: 7.739 min
Delta R.T.: -0.006 min
Response: 194540
Conc: 77.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-20-COMP


Manual Integrations
APPROVED

Ankita
9/10/2019 1:53:11 PM

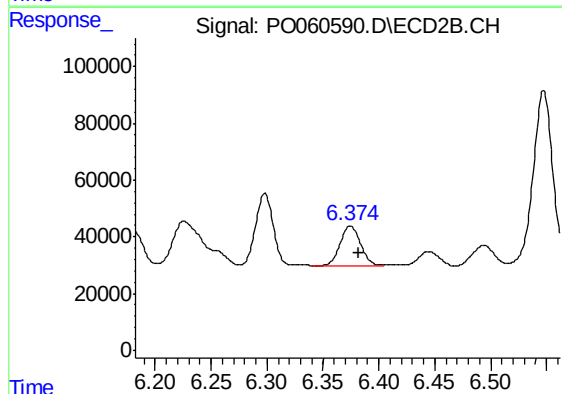


#33 AR-1260-3

R.T.: 6.375 min
Delta R.T.: -0.007 min
Response: 176690
Conc: 76.05 ng/ml

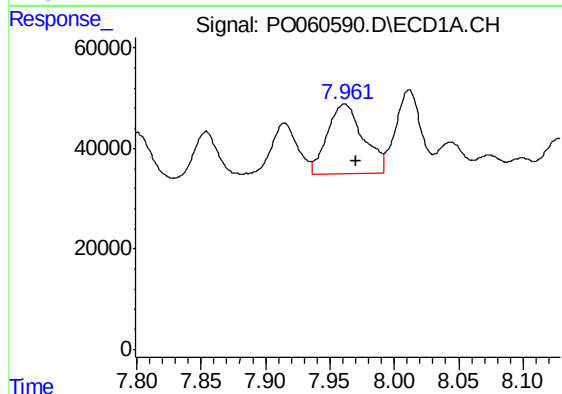


#34 AR-1260-4

R.T.: 7.962 min
Delta R.T.: -0.009 min
Response: 272426
Conc: 92.01 ng/ml

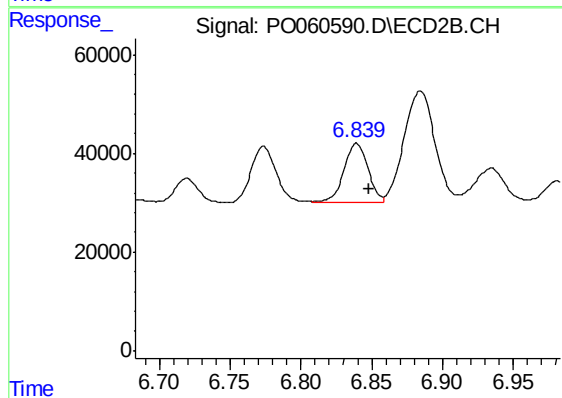

#34 AR-1260-4

R.T.: 6.839 min
Delta R.T.: -0.009 min
Response: 140896
Conc: 69.37 ng/ml

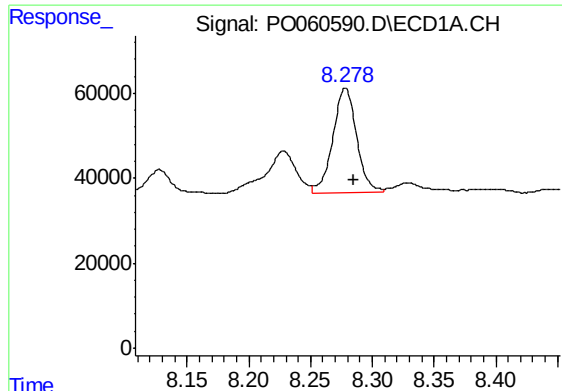


#35 AR-1260-5

R.T.: 8.278 min
Delta R.T.: -0.006 min
Response: 329492
Conc: 58.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-20-COMP

Manual Integrations
APPROVED

Ankita
9/10/2019 1:53:11 PM

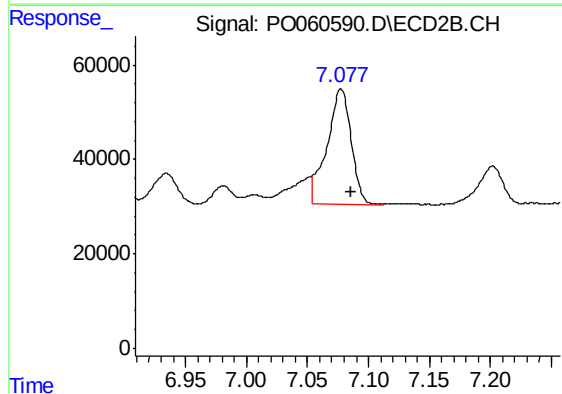

#35 AR-1260-5

R.T.: 7.077 min
Delta R.T.: -0.009 min
Response: 333869
Conc: 72.88 ng/ml m