

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090919\
 Data File : P0060591.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Sep 2019 1:55
 Operator : SM/AJ
 Sample : K4636-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-21-COMP

Manual Integrations
 APPROVED

Ankita
 9/10/2019 1:53:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 07:37:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Sep 08 02:12:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.368	3.534	867475	672683	20.907	21.901
2)	SA Decachlor...	10.026	8.420	1031828	759955	19.561	20.529m
Target Compounds							
31)	L7 AR-1260-1	7.126	6.039	550641	474094	220.282m	230.544
32)	L7 AR-1260-2	7.376	6.225	1307522	479405	420.773	191.473 #
33)	L7 AR-1260-3	7.740	6.374	287220	355704	114.823	153.103 #
34)	L7 AR-1260-4	7.958	6.840	407982	203201	137.796m	100.047 #
35)	L7 AR-1260-5	8.279	7.078	500479	454535	89.104	99.226

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090919\
Data File : PO060591.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Sep 2019 1:55
Operator : SM/AJ
Sample : K4636-06
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SB-21-COMP


Manual Integrations
APPROVED

Ankita
9/10/2019 1:53:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 07:37:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Sep 08 02:12:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

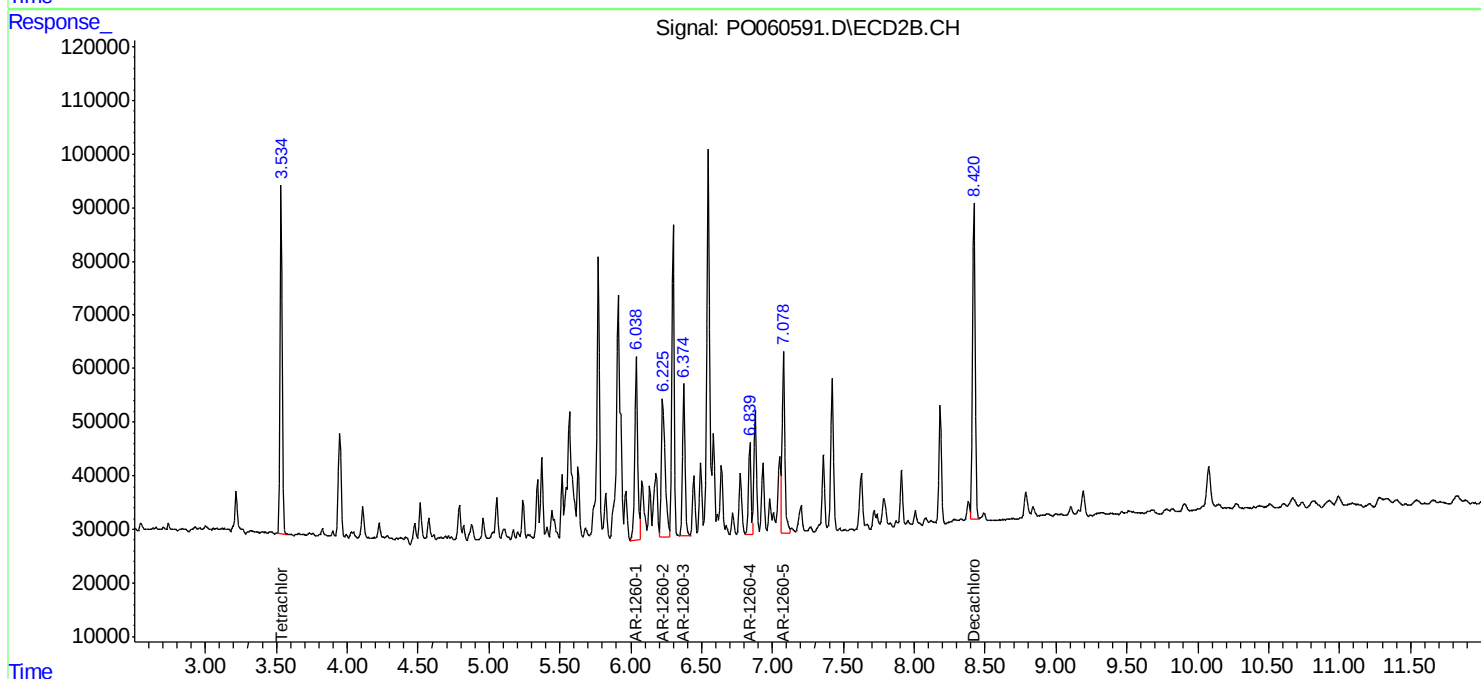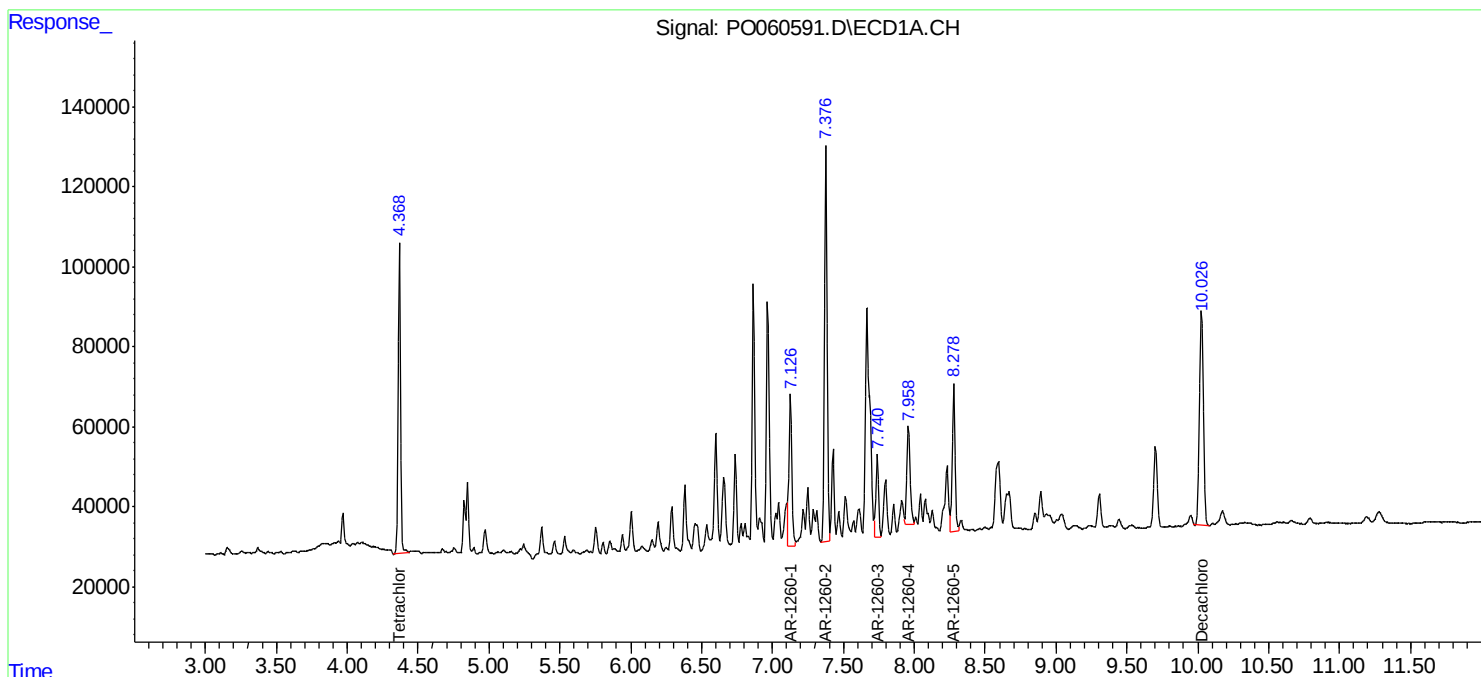

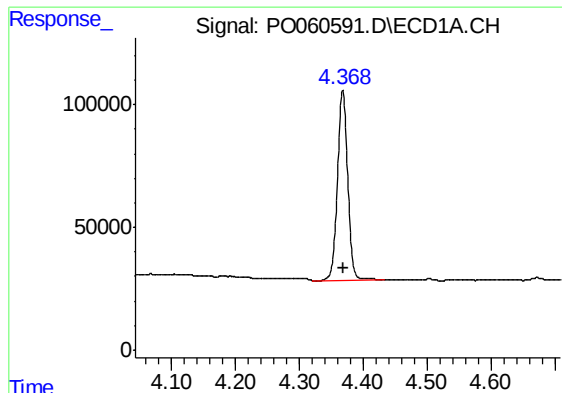


#1 Tetrachloro-m-xylene

R.T.: 4.368 min
Delta R.T.: -0.001 min
Response: 867475
Conc: 20.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-21-COMP


Manual Integrations
APPROVED

Ankita
9/10/2019 1:53:14 PM

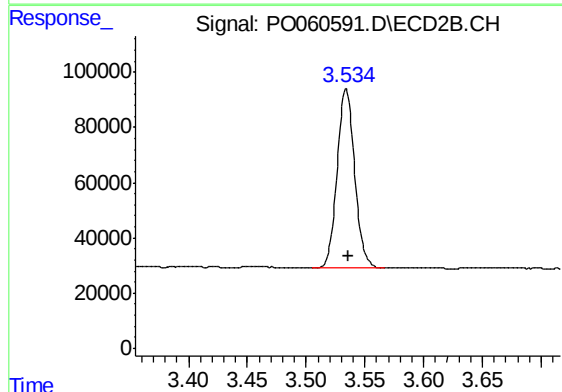


#1 Tetrachloro-m-xylene

R.T.: 3.534 min
Delta R.T.: -0.002 min
Response: 672683
Conc: 21.90 ng/ml

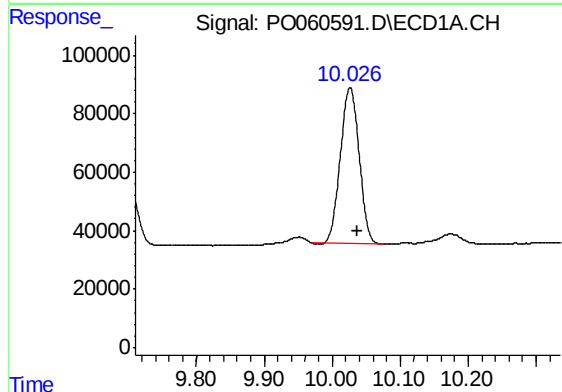


#2 Decachlorobiphenyl

R.T.: 10.026 min
Delta R.T.: -0.011 min
Response: 1031828
Conc: 19.56 ng/ml

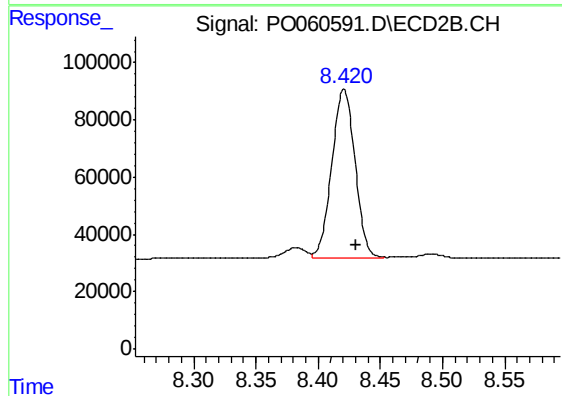

#2 Decachlorobiphenyl

R.T.: 8.420 min
Delta R.T.: -0.011 min
Response: 759955
Conc: 20.53 ng/ml m

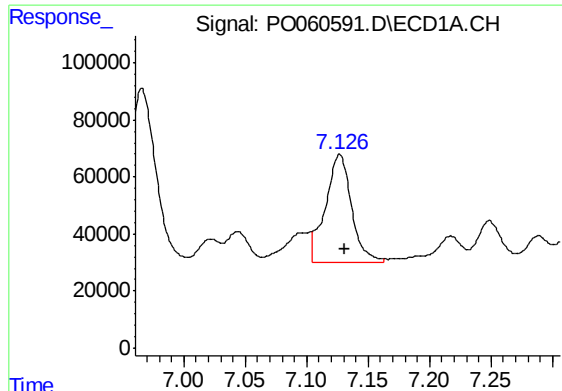


#31 AR-1260-1

R.T.: 7.126 min
Delta R.T.: -0.004 min
Response: 550641
Conc: 220.28 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-21-COMP


Manual Integrations
APPROVED

Ankita
9/10/2019 1:53:14 PM

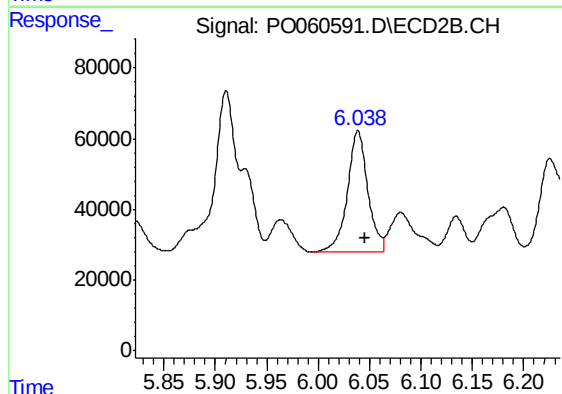


#31 AR-1260-1

R.T.: 6.039 min
Delta R.T.: -0.007 min
Response: 474094
Conc: 230.54 ng/ml

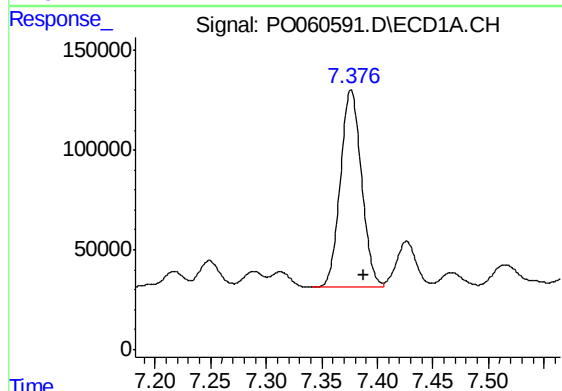


#32 AR-1260-2

R.T.: 7.376 min
Delta R.T.: -0.011 min
Response: 1307522
Conc: 420.77 ng/ml

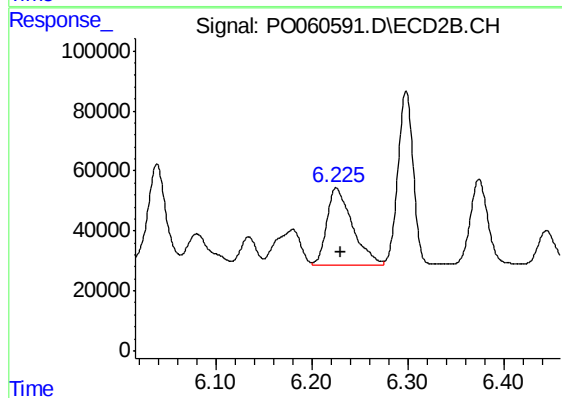

#32 AR-1260-2

R.T.: 6.225 min
Delta R.T.: -0.005 min
Response: 479405
Conc: 191.47 ng/ml

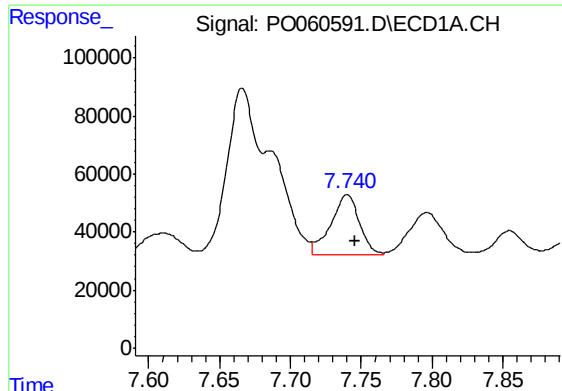


#33 AR-1260-3

R.T.: 7.740 min
Delta R.T.: -0.005 min
Response: 287220
Conc: 114.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-21-COMP


Manual Integrations
APPROVED

Ankita
9/10/2019 1:53:14 PM

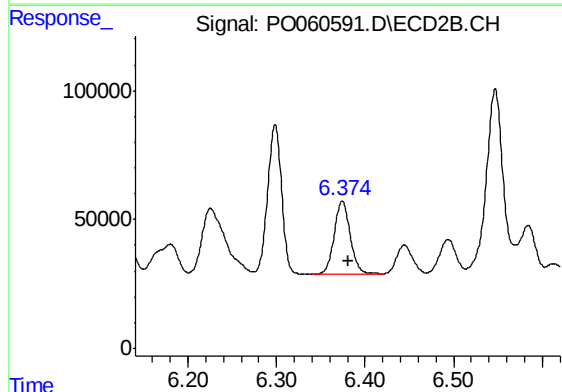


#33 AR-1260-3

R.T.: 6.374 min
Delta R.T.: -0.007 min
Response: 355704
Conc: 153.10 ng/ml

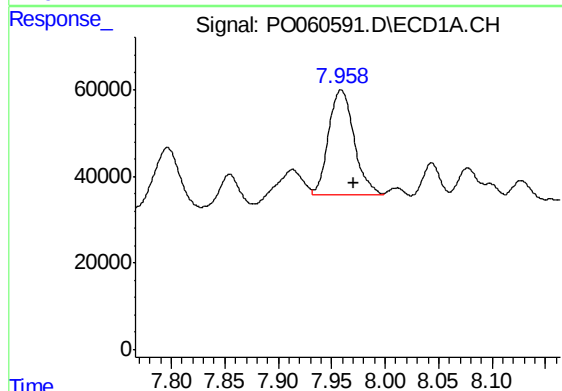


#34 AR-1260-4

R.T.: 7.958 min
Delta R.T.: -0.013 min
Response: 407982
Conc: 137.80 ng/ml m

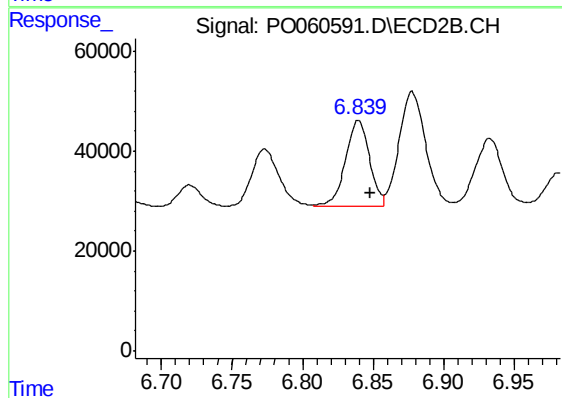

#34 AR-1260-4

R.T.: 6.840 min
Delta R.T.: -0.008 min
Response: 203201
Conc: 100.05 ng/ml

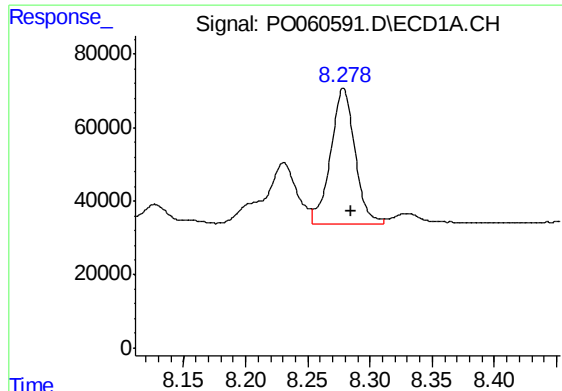


#35 AR-1260-5

R.T.: 8.279 min
Delta R.T.: -0.006 min
Response: 500479
Conc: 89.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-21-COMP

Manual Integrations
APPROVED

Ankita
9/10/2019 1:53:14 PM

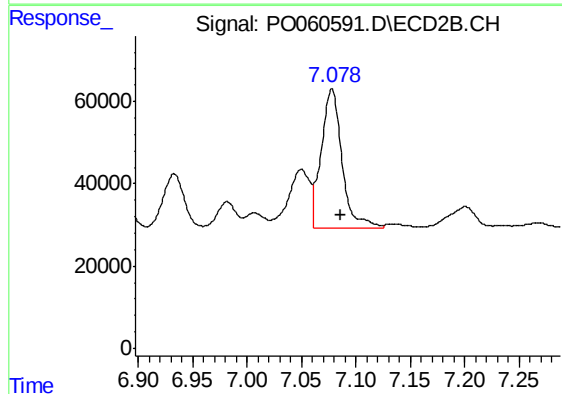

#35 AR-1260-5

R.T.: 7.078 min
Delta R.T.: -0.008 min
Response: 454535
Conc: 99.23 ng/ml