

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090919\
 Data File : P0060611.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Sep 2019 7:49
 Operator : SM/AJ
 Sample : K4745-01
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-058

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 08:31:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Sep 08 02:12:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.367	3.533	885307	702812	21.337	22.882
2)	SA Decachlor...	10.023	8.418	614193	481825	11.643	13.016

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090919\
Data File : P0060611.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Sep 2019 7:49
Operator : SM/AJ
Sample : K4745-01
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-058

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 08:31:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Sep 08 02:12:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

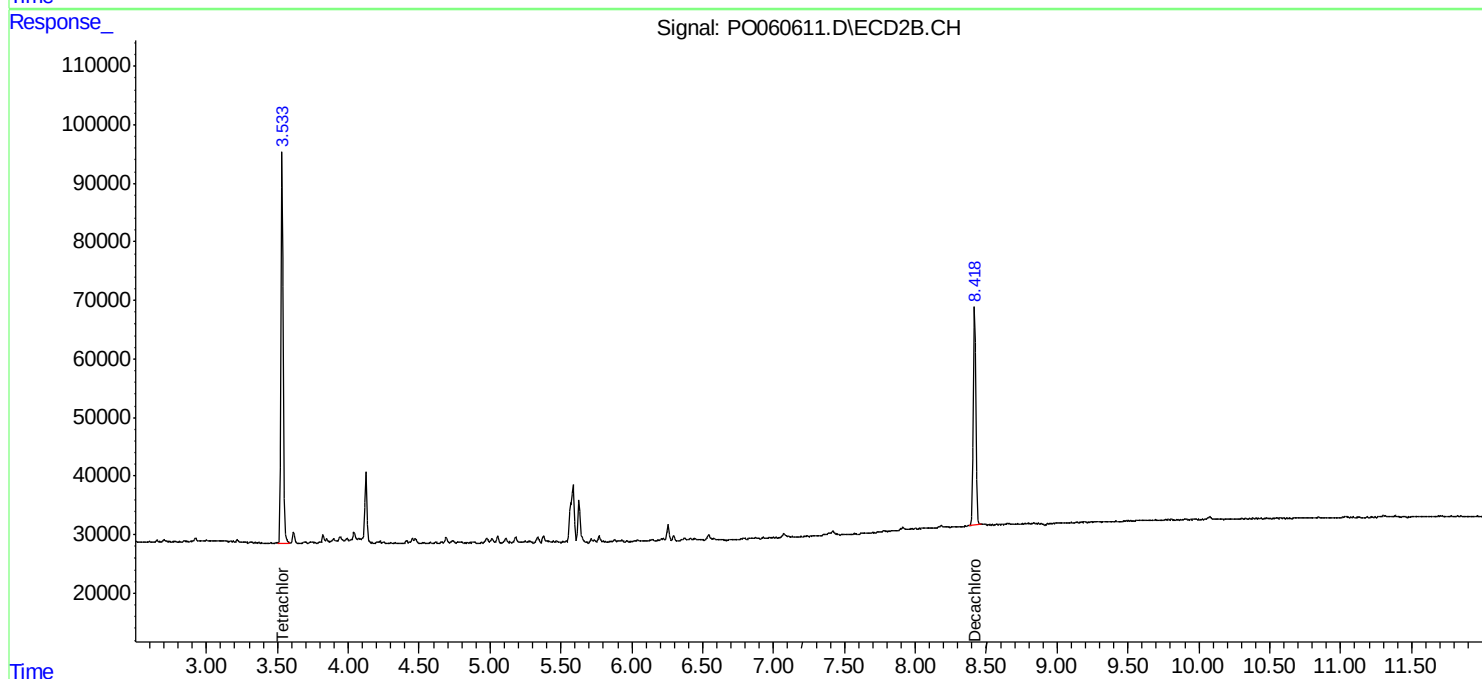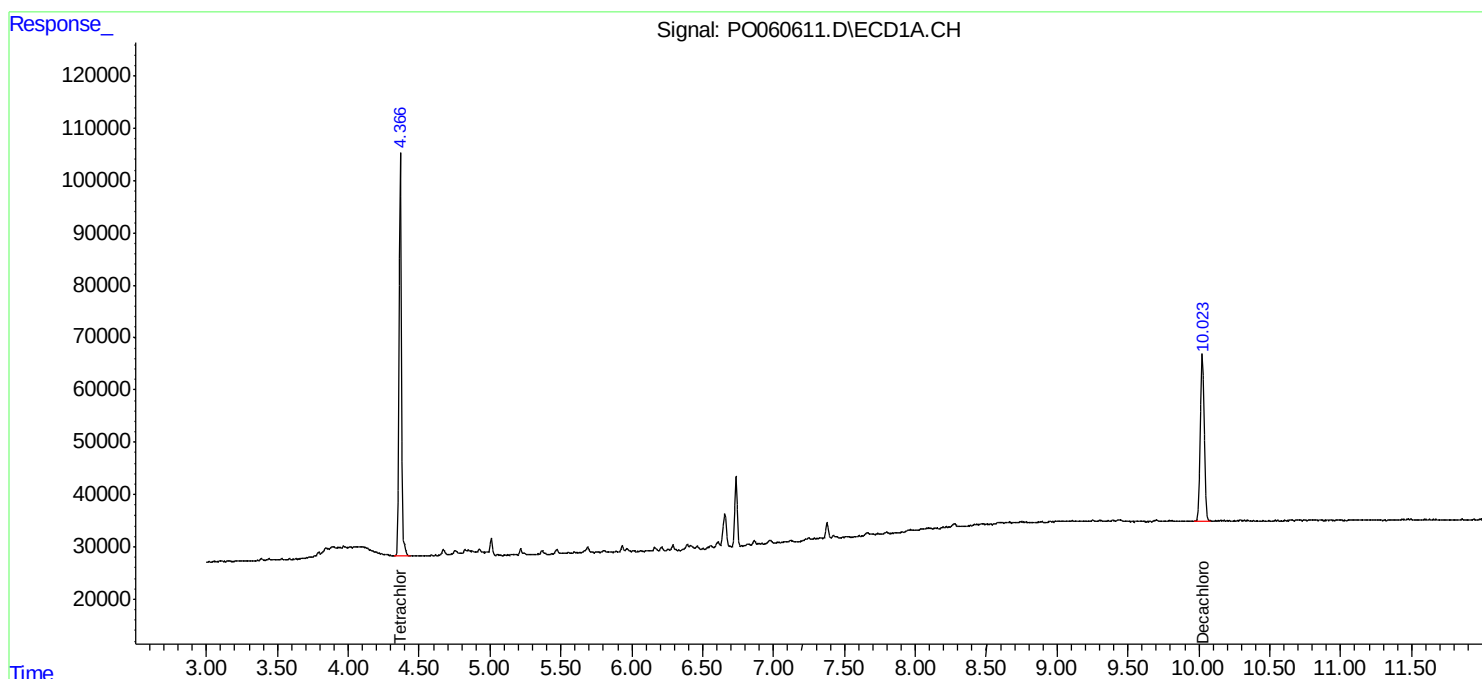


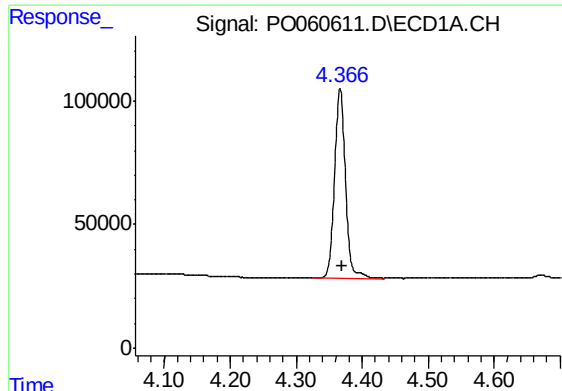

#1 Tetrachloro-m-xylene


R.T.: 4.367 min
Delta R.T.: -0.002 min
Response: 885307
Conc: 21.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-058

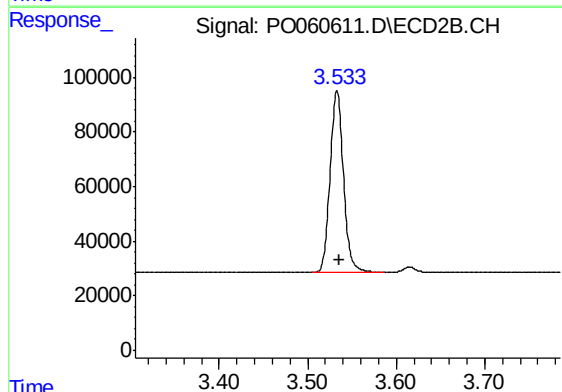


#1 Tetrachloro-m-xylene

R.T.: 3.533 min
Delta R.T.: -0.003 min
Response: 702812
Conc: 22.88 ng/ml

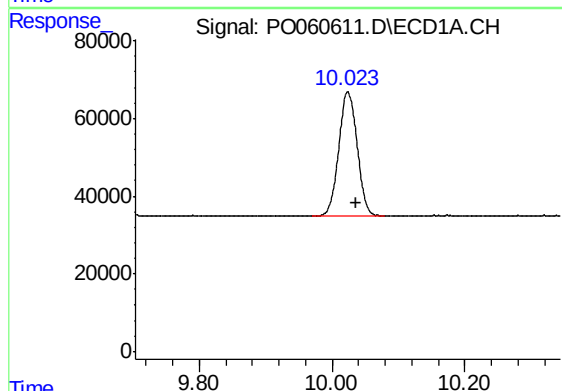

#2 Decachlorobiphenyl

R.T.: 10.023 min
Delta R.T.: -0.014 min
Response: 614193
Conc: 11.64 ng/ml

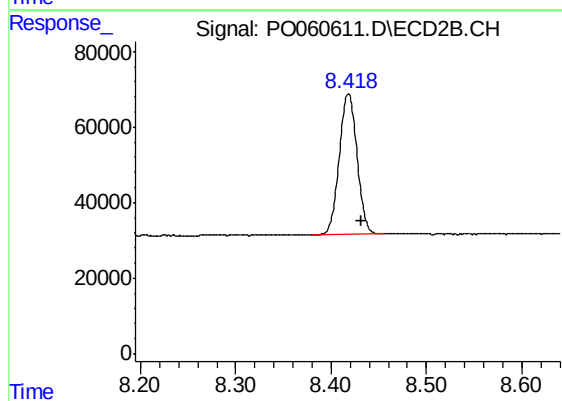

#2 Decachlorobiphenyl

R.T.: 8.418 min
Delta R.T.: -0.013 min
Response: 481825
Conc: 13.02 ng/ml