

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090920\
 Data File : P0071236.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Sep 2020 11:50
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 16:05:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.344	3.529	1416278	784162	19.985	20.086
2)	SA Decachlor...	9.959	8.710	1849443	1083251	19.832	19.665
Target Compounds							
9)	L2 AR-1221-2	4.688	0.000	47002	0	85.188	N.D. #
16)	L4 AR-1242-1	5.607f	0.000	43145	0	18.435	N.D. #
24)	L5 AR-1248-4	6.553f	0.000	598851	0	164.794	N.D. #
26)	L6 AR-1254-1	6.553f	0.000	598851	0	170.690	N.D. #
35)	L7 AR-1260-5	8.474	0.000	217072	0	17.119	N.D. #
37)	L8 AR-1262-2	8.474	0.000	217072	0	15.037	N.D. #
39)	L8 AR-1262-4	8.809	0.000	13590	0	2.137	N.D. #
42)	L9 AR-1268-2	8.809	0.000	13590	0	0.972	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090920\
Data File : PO071236.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Sep 2020 11:50
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 16:05:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

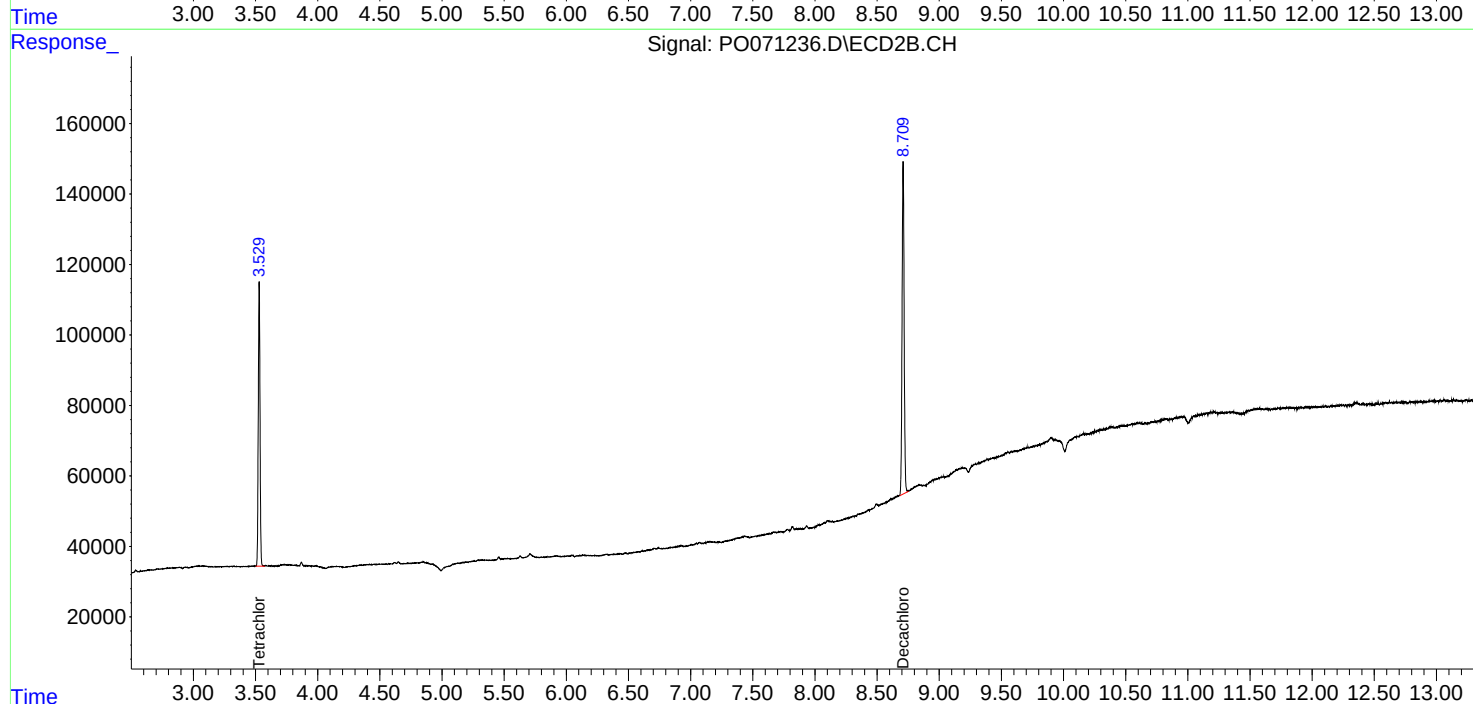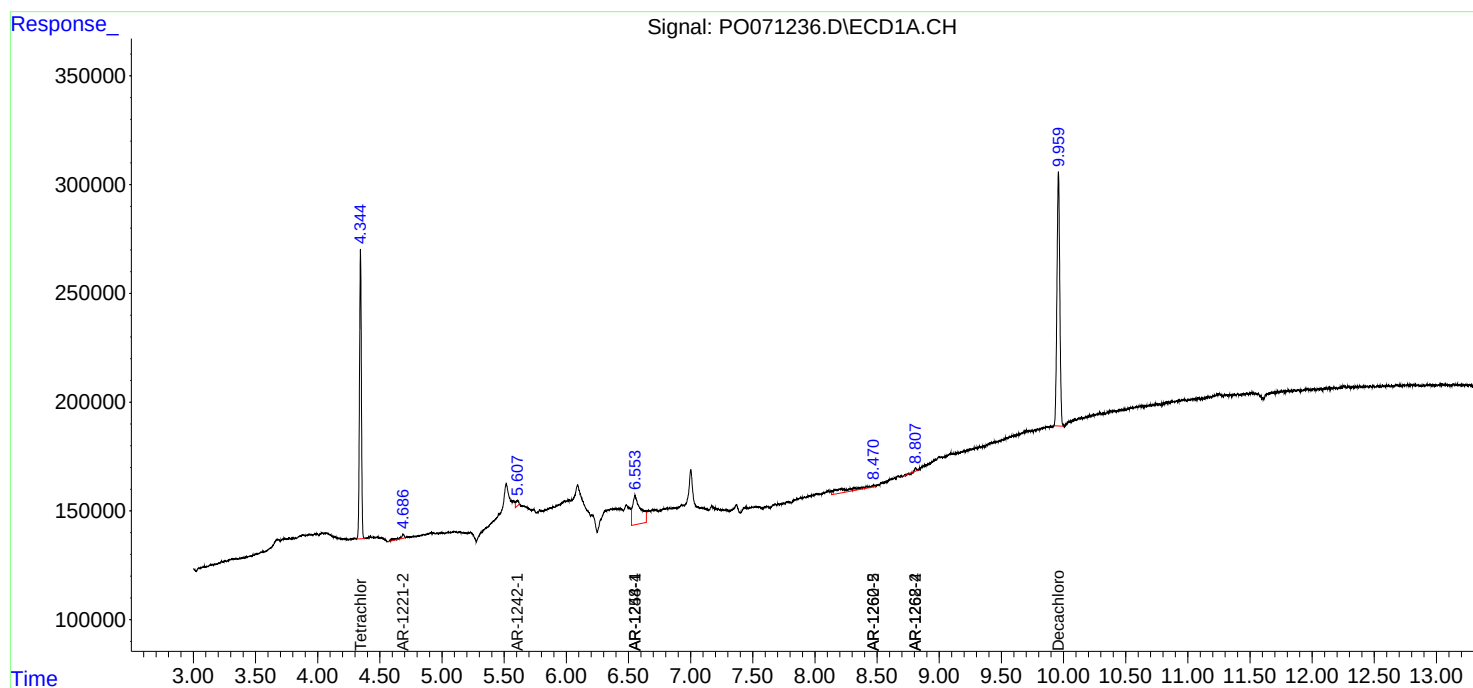


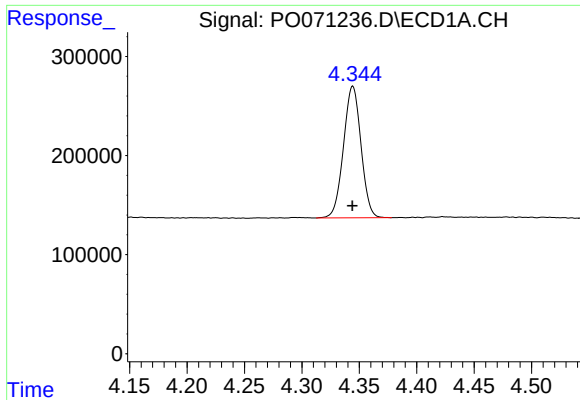

#1 Tetrachloro-m-xylene


R.T.: 4.344 min
Delta R.T.: 0.000 min
Response: 1416278
Conc: 19.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

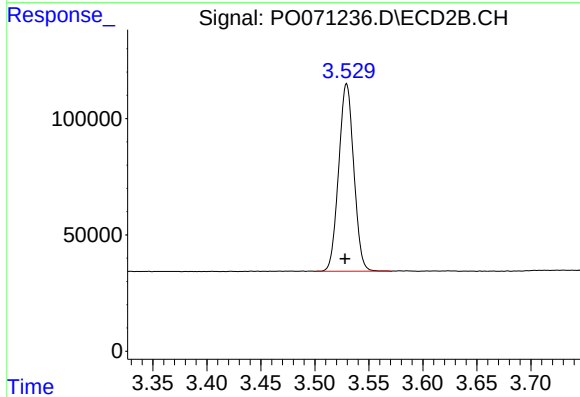


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: 0.001 min
Response: 784162
Conc: 20.09 ng/ml

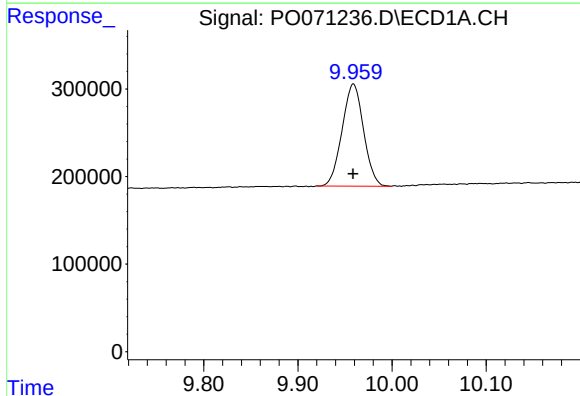


#2 Decachlorobiphenyl

R.T.: 9.959 min
Delta R.T.: 0.000 min
Response: 1849443
Conc: 19.83 ng/ml

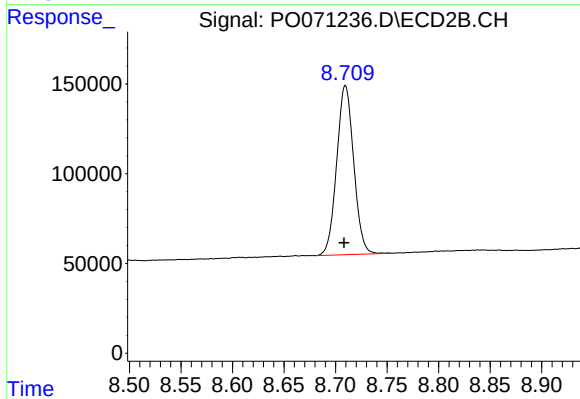

#2 Decachlorobiphenyl


R.T.: 8.710 min
Delta R.T.: 0.001 min
Response: 1083251
Conc: 19.67 ng/ml

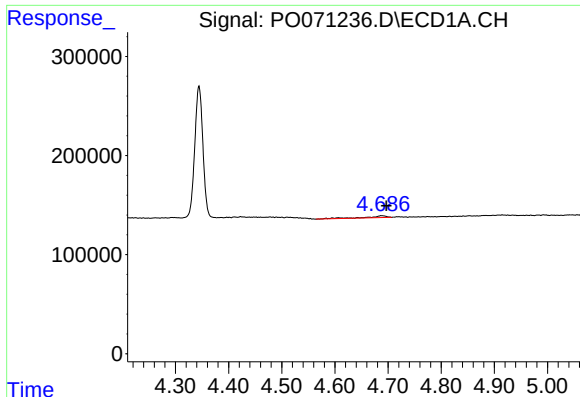

#9 AR-1221-2


R.T.: 4.688 min
Delta R.T.: -0.009 min
Response: 47002
Conc: 85.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

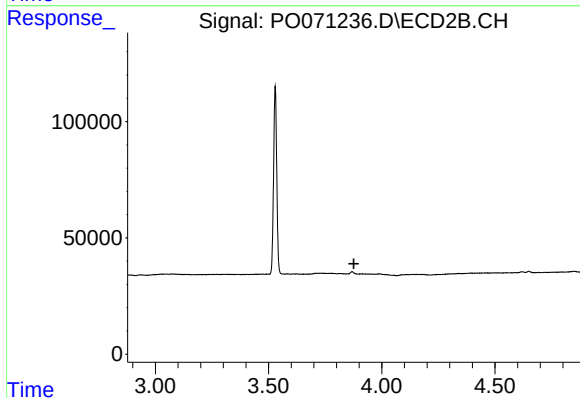


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.877 min
Response: 0
Conc: N.D.

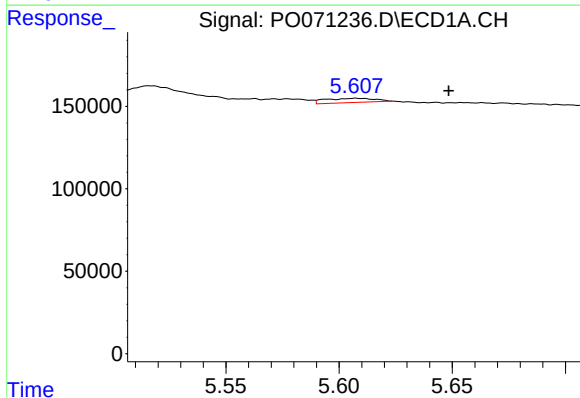


#16 AR-1242-1

R.T.: 5.607 min
Delta R.T.: -0.041 min
Response: 43145
Conc: 18.44 ng/ml

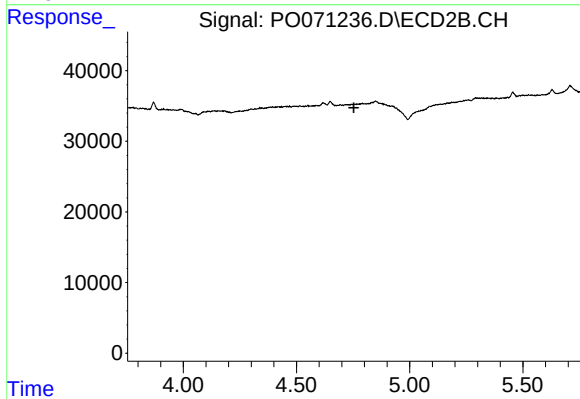

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.754 min
Response: 0
Conc: N.D.

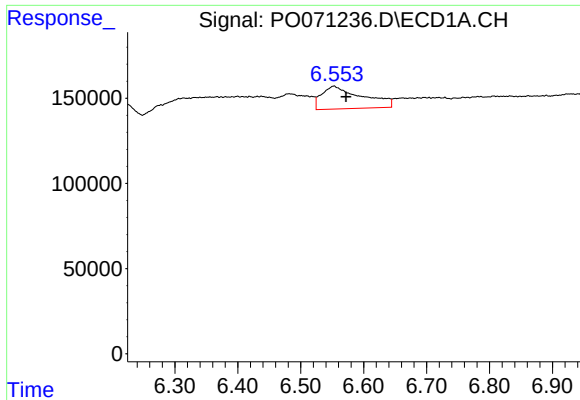

#24 AR-1248-4


R.T.: 6.553 min
Delta R.T.: -0.019 min
Response: 598851
Conc: 164.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

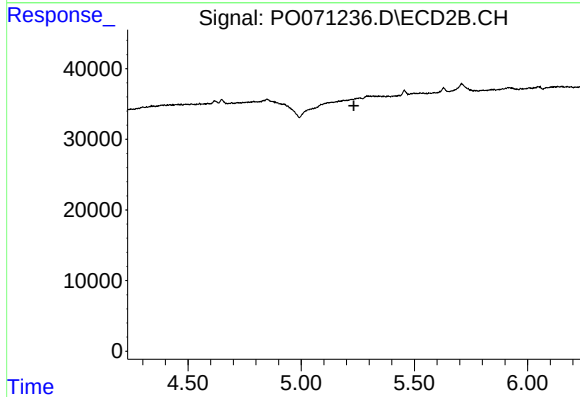


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.233 min
Response: 0
Conc: N.D.

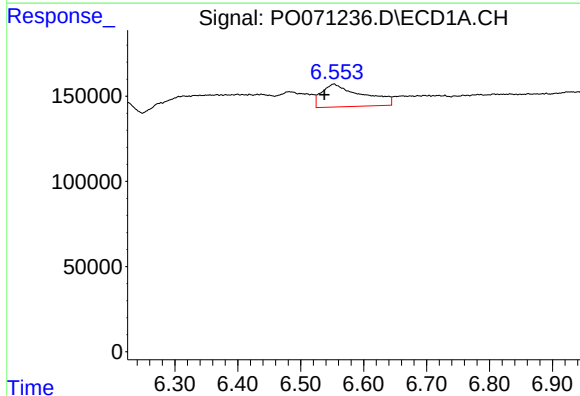


#26 AR-1254-1

R.T.: 6.553 min
Delta R.T.: 0.015 min
Response: 598851
Conc: 170.69 ng/ml

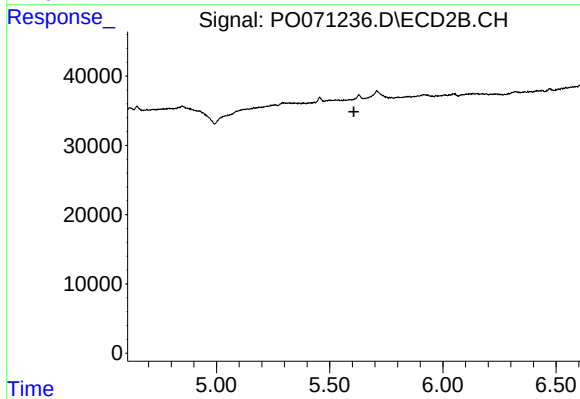

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.607 min
Response: 0
Conc: N.D.

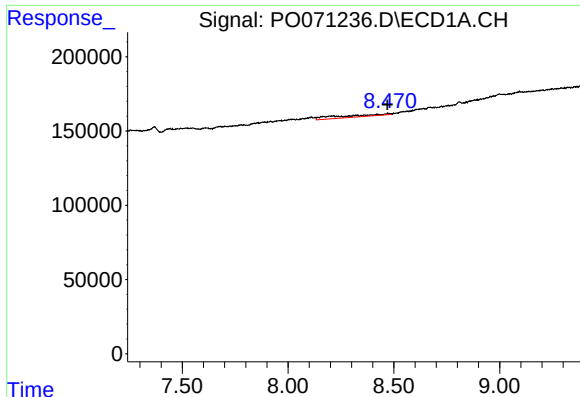

#35 AR-1260-5


R.T.: 8.474 min
Delta R.T.: 0.004 min
Response: 217072
Conc: 17.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

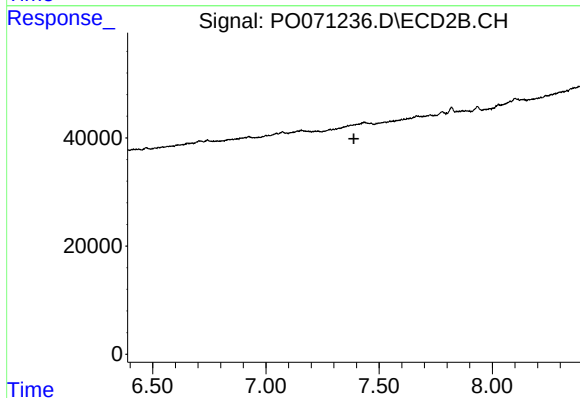


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.388 min
Response: 0
Conc: N.D.

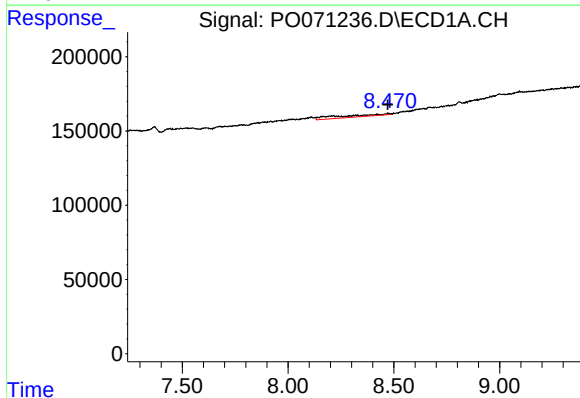


#37 AR-1262-2

R.T.: 8.474 min
Delta R.T.: 0.003 min
Response: 217072
Conc: 15.04 ng/ml

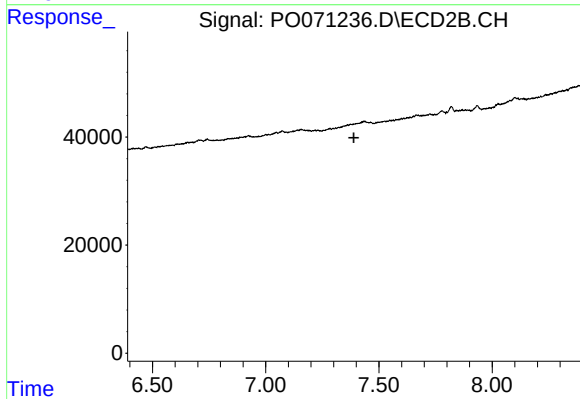

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.

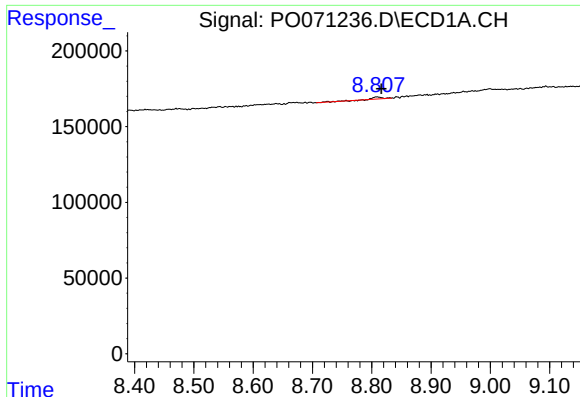

#39 AR-1262-4


R.T.: 8.809 min
Delta R.T.: -0.008 min
Response: 13590
Conc: 2.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

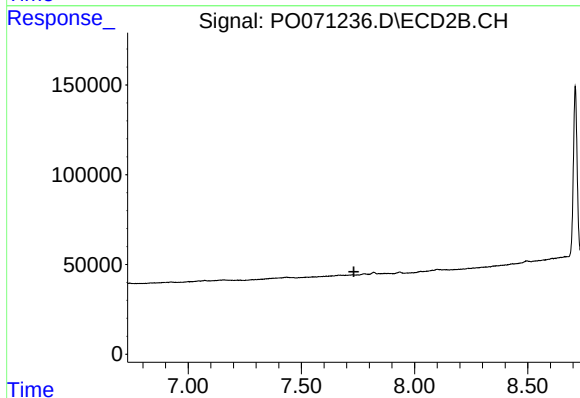


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.732 min
Response: 0
Conc: N.D.

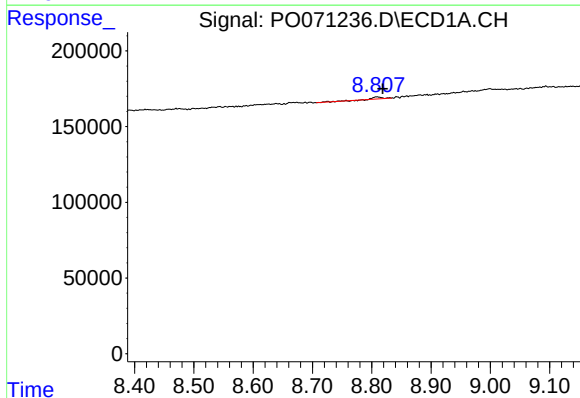

#42 AR-1268-2

R.T.: 8.809 min
Delta R.T.: -0.010 min
Response: 13590
Conc: 0.97 ng/ml

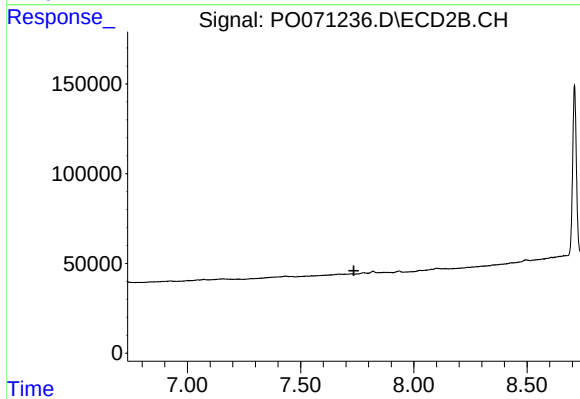

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.735 min
Response: 0
Conc: N.D.