

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091018\
 Data File : P0048902.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Sep 2018 21:58
 Operator : SM/SJ
 Sample : J4833-03 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 00:56:38 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 06 03:44:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.400	3.530	297467	570650	2.465	3.651 #
2)	SA Decachlor...	10.117	8.469	161987	265203	1.161	1.794 #
Target Compounds							
4)	L1 AR-1016-2	0.000	4.657	0	219429	N.D.	34.077 #
5)	L1 AR-1016-3	5.635	4.657	268171	219429	53.112	25.987 #
6)	L1 AR-1016-4	5.635	4.657	268171	219429	58.264	37.352 #
8)	L2 AR-1221-1	4.646	3.680	542595	181175	349.450	84.631 #
11)	L3 AR-1232-1	5.635	0.000	268171	0	96.670	N.D. #
14)	L3 AR-1232-4	6.326	0.000	85711	0	216.356	N.D. #
45)	L9 AR-1268-5	9.852	0.000	104729	0	2.020	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091018\
Data File : PO048902.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Sep 2018 21:58
Operator : SM/SJ
Sample : J4833-03 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 00:56:38 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090418.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 06 03:44:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

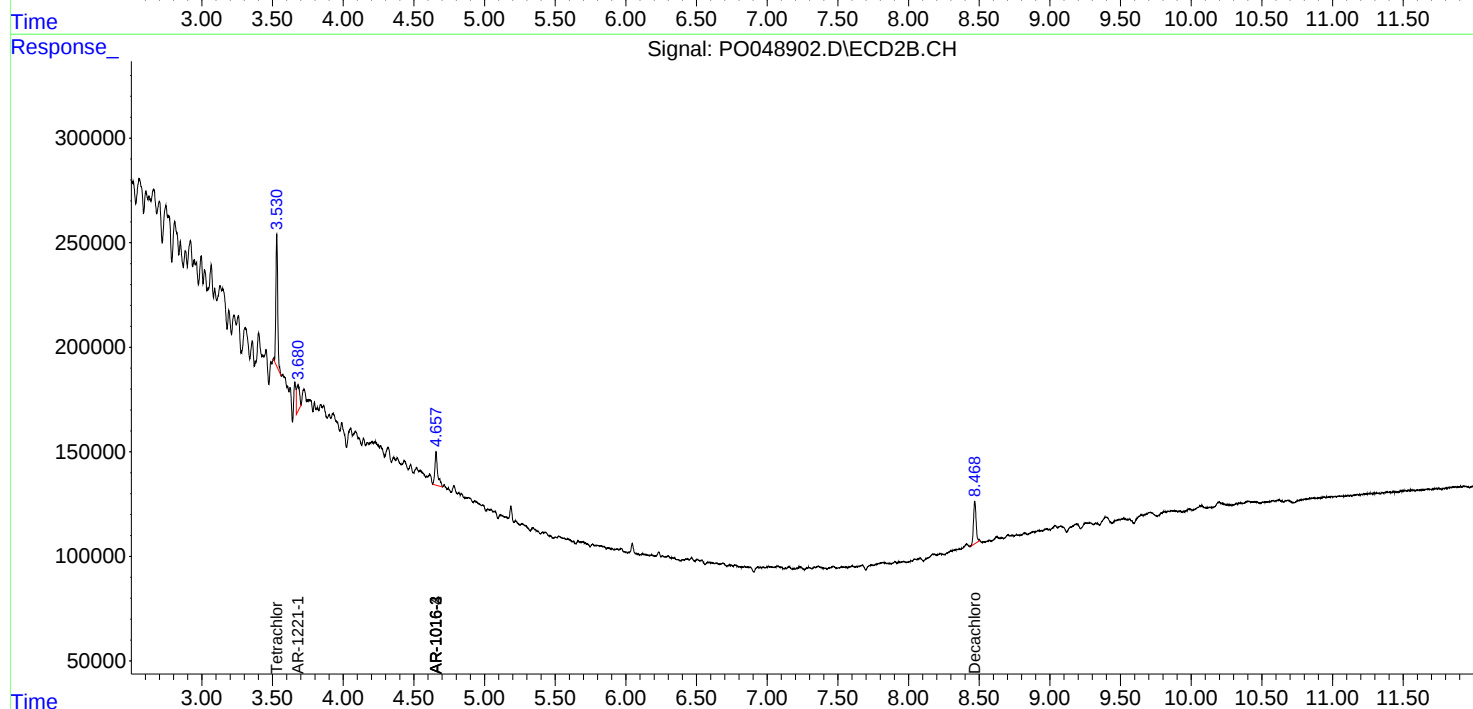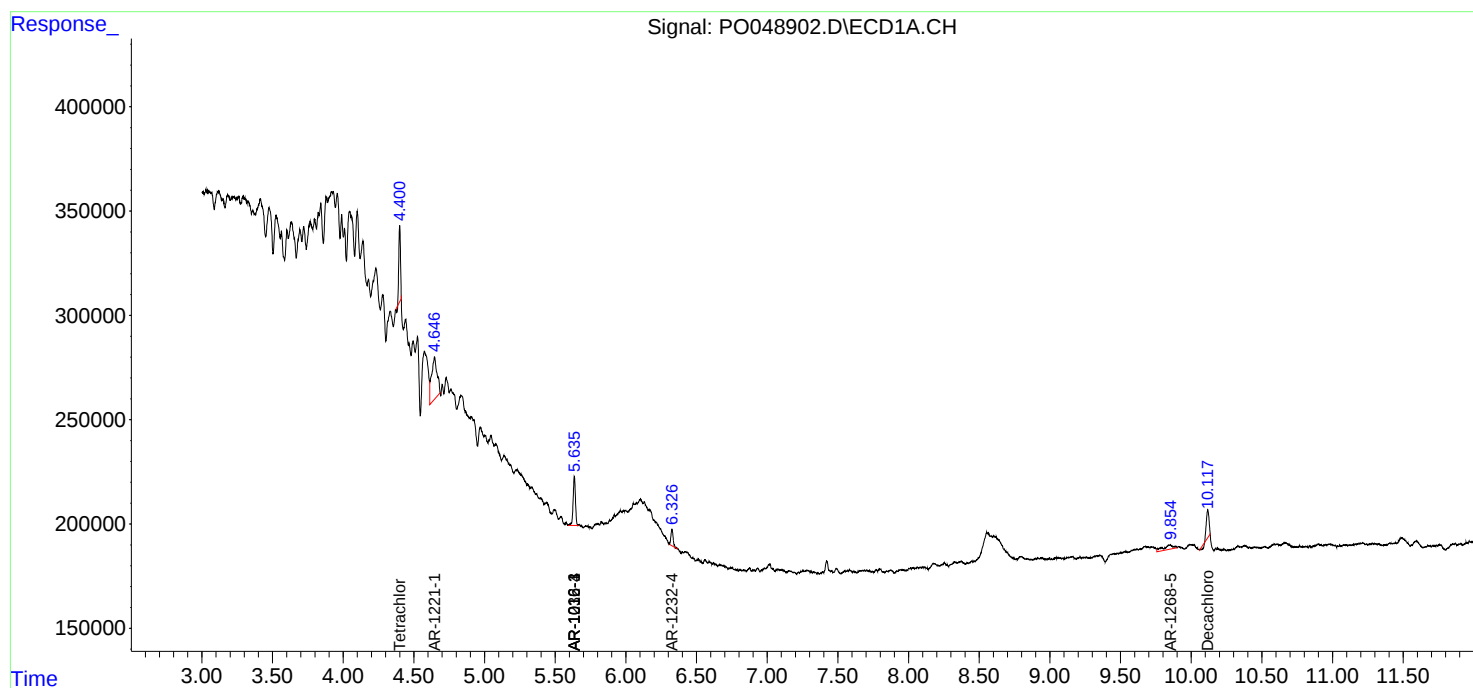


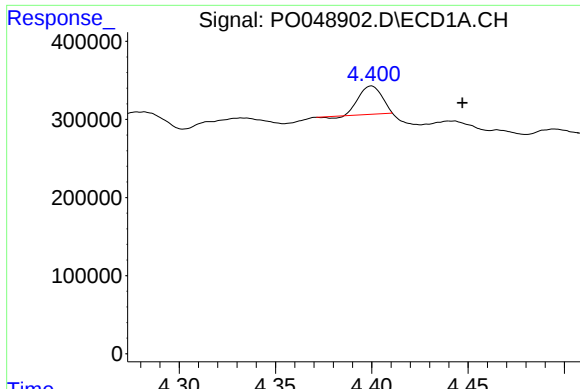

#1 Tetrachloro-m-xylene


R.T.: 4.400 min
Delta R.T.: -0.047 min
Response: 297467
Conc: 2.47 ng/ml

Instrument :
ECD_O
ClientSampleId :

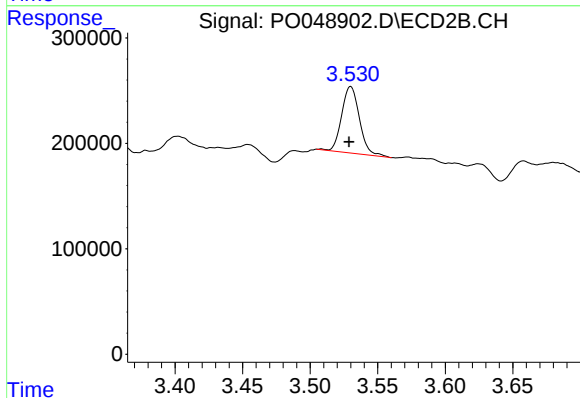


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: 0.001 min
Response: 570650
Conc: 3.65 ng/ml

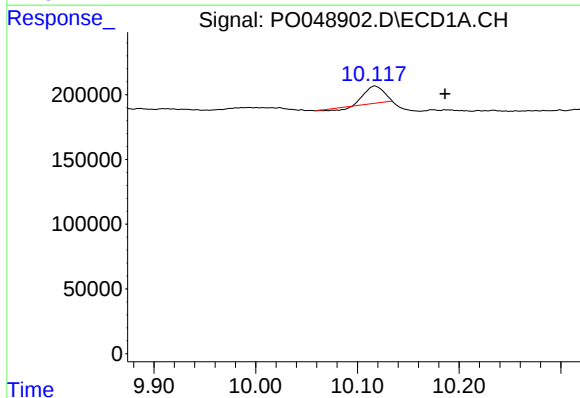


#2 Decachlorobiphenyl

R.T.: 10.117 min
Delta R.T.: -0.069 min
Response: 161987
Conc: 1.16 ng/ml

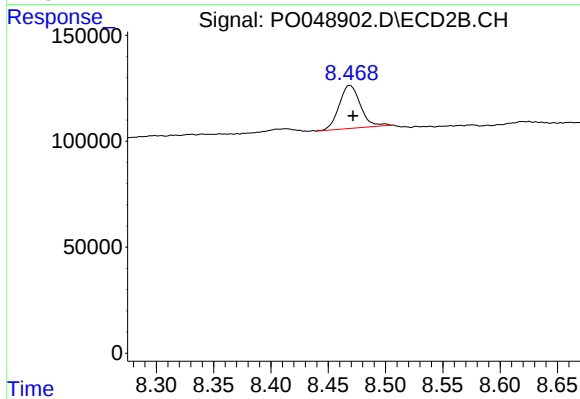

#2 Decachlorobiphenyl


R.T.: 8.469 min
Delta R.T.: -0.003 min
Response: 265203
Conc: 1.79 ng/ml

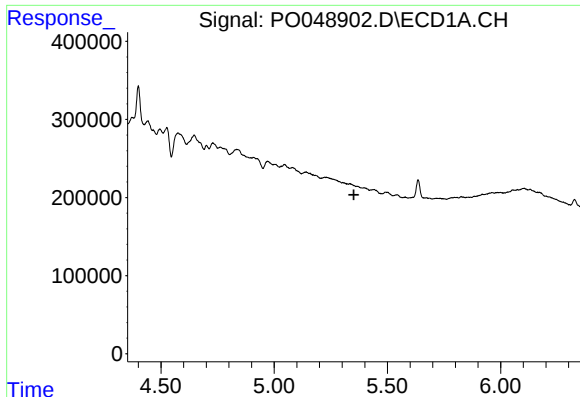

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T.: 5.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

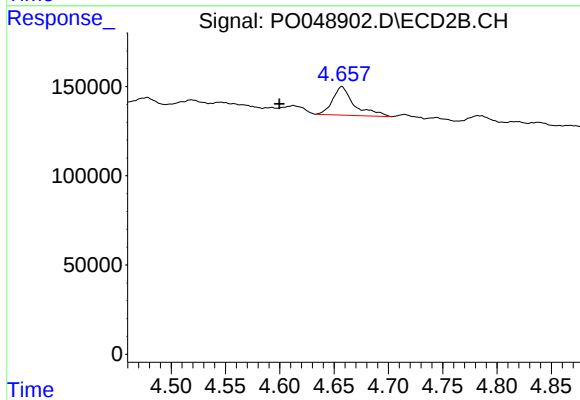


#4 AR-1016-2

R.T.: 4.657 min
Delta R.T.: 0.057 min
Response: 219429
Conc: 34.08 ng/ml

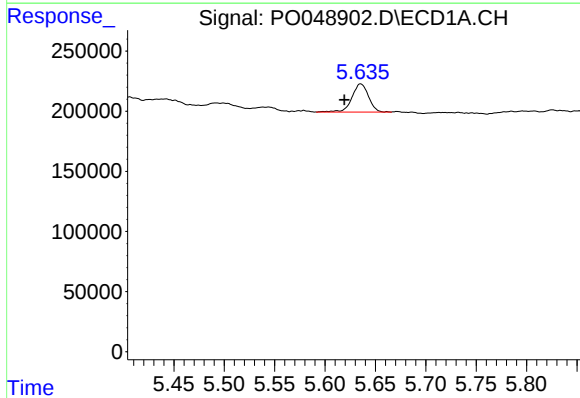


#5 AR-1016-3

R.T.: 5.635 min
Delta R.T.: 0.016 min
Response: 268171
Conc: 53.11 ng/ml

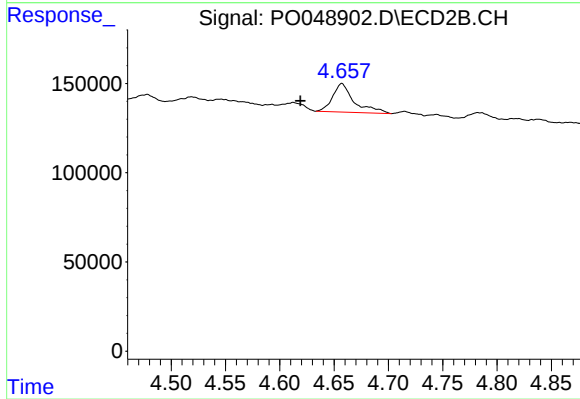

#5 AR-1016-3


R.T.: 4.657 min
Delta R.T.: 0.038 min
Response: 219429
Conc: 25.99 ng/ml

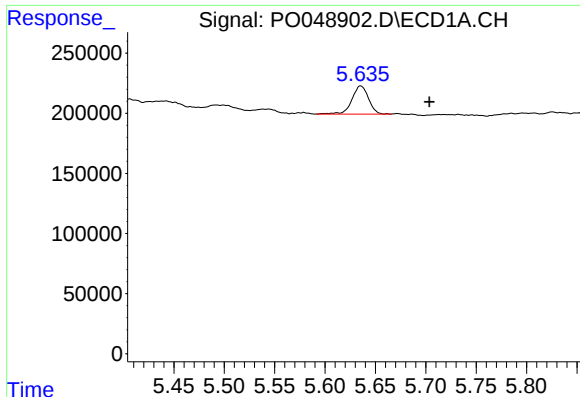

#6 AR-1016-4


R.T.: 5.635 min
Delta R.T.: -0.068 min
Response: 268171
Conc: 58.26 ng/ml

Instrument :
ECD_O
ClientSampleId :

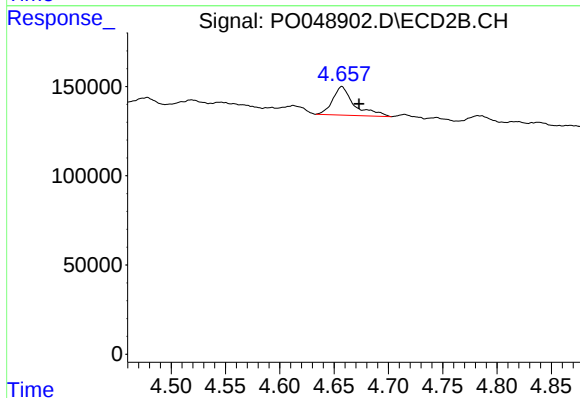


#6 AR-1016-4

R.T.: 4.657 min
Delta R.T.: -0.016 min
Response: 219429
Conc: 37.35 ng/ml

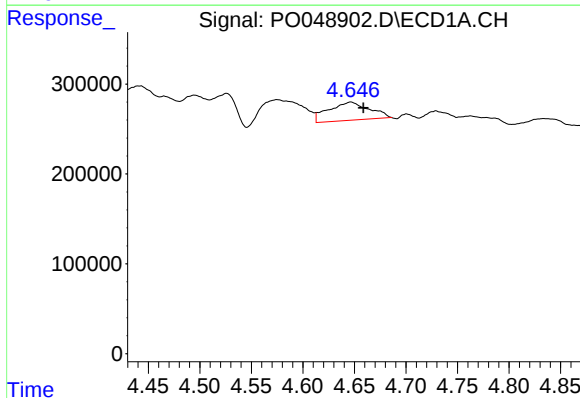


#8 AR-1221-1

R.T.: 4.646 min
Delta R.T.: -0.012 min
Response: 542595
Conc: 349.45 ng/ml

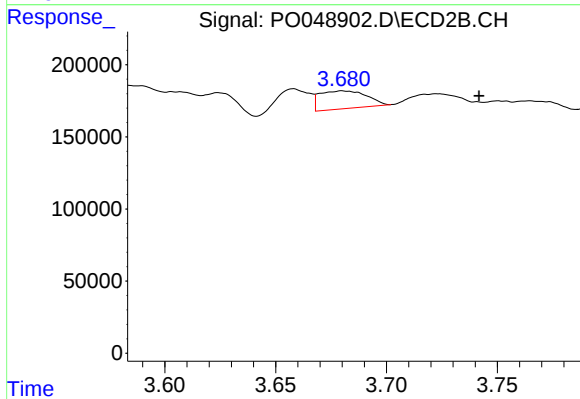

#8 AR-1221-1


R.T.: 3.680 min
Delta R.T.: -0.061 min
Response: 181175
Conc: 84.63 ng/ml

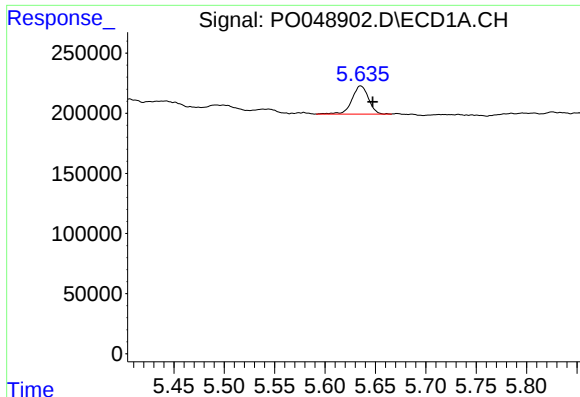

#11 AR-1232-1


R.T.: 5.635 min
Delta R.T.: -0.012 min
Response: 268171
Conc: 96.67 ng/ml

Instrument :
ECD_O
ClientSampleId :

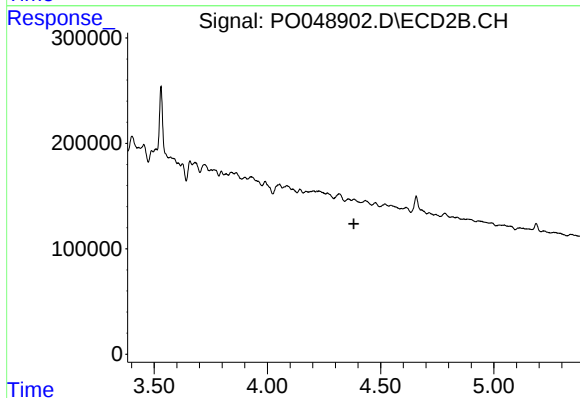


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.382 min
Response: 0
Conc: N.D.

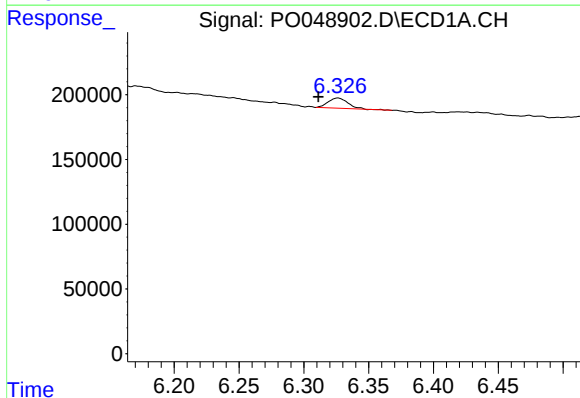


#14 AR-1232-4

R.T.: 6.326 min
Delta R.T.: 0.015 min
Response: 85711
Conc: 216.36 ng/ml

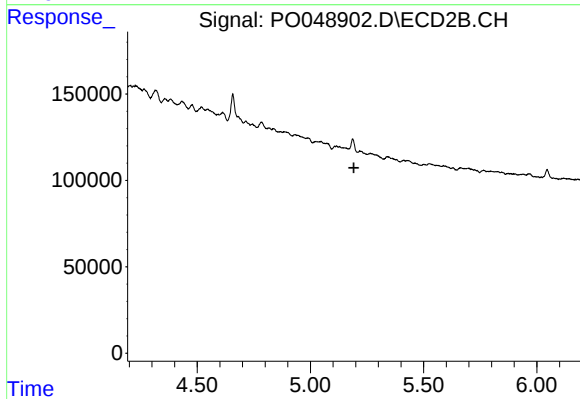

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 5.192 min
Response: 0
Conc: N.D.

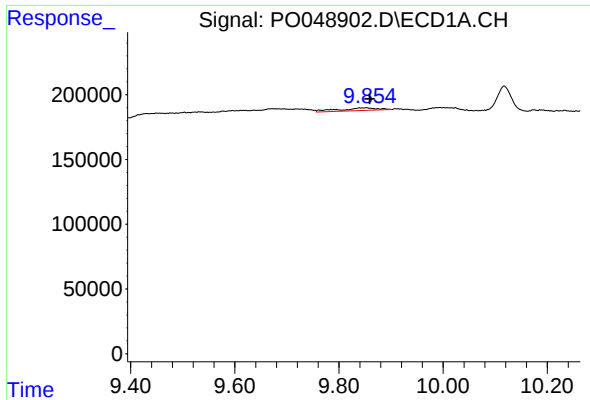

#45 AR-1268-5

R.T.: 9.852 min
Delta R.T.: -0.007 min
Response: 104729
Conc: 2.02 ng/ml

Instrument :
ECD_O
ClientSampleId :

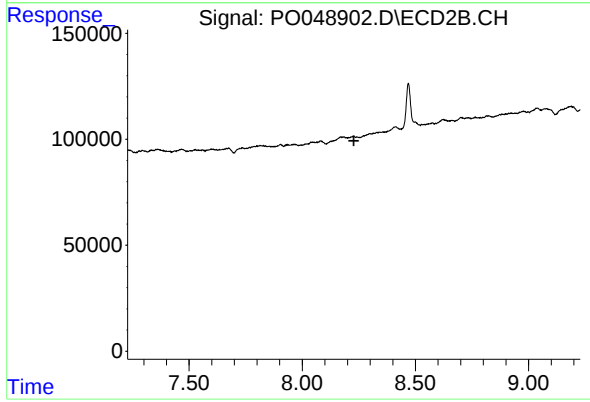

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.228 min
Response: 0
Conc: N.D.