

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091019\
 Data File : P0060617.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Sep 2019 10:14
 Operator : SM/AJ
 Sample : K4636-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-20-COMP

Manual Integrations
 APPROVED

Ankita
 9/11/2019 9:09:34 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 04:28:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Sep 08 02:12:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.368	3.532	762297	628259	18.372	20.455
2)	SA Decachlor...	10.024	8.417	1293407	933944	24.520	25.229
Target Compounds							
31)	L7 AR-1260-1	7.124	6.035	195848	262117	78.348m	127.464 #
32)	L7 AR-1260-2	7.376	6.223	603068	274401	194.073	109.595m#
33)	L7 AR-1260-3	7.739	6.371	200145	166657	80.013	71.733
34)	L7 AR-1260-4	7.961	6.836	290850	133247	98.235	65.605 #
35)	L7 AR-1260-5	8.277	7.075	329496	407892	58.662	89.044 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091019\
Data File : PO060617.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Sep 2019 10:14
Operator : SM/AJ
Sample : K4636-04
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-20-COMP


Manual Integrations
APPROVED

Ankita
9/11/2019 9:09:34 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 04:28:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Sep 08 02:12:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

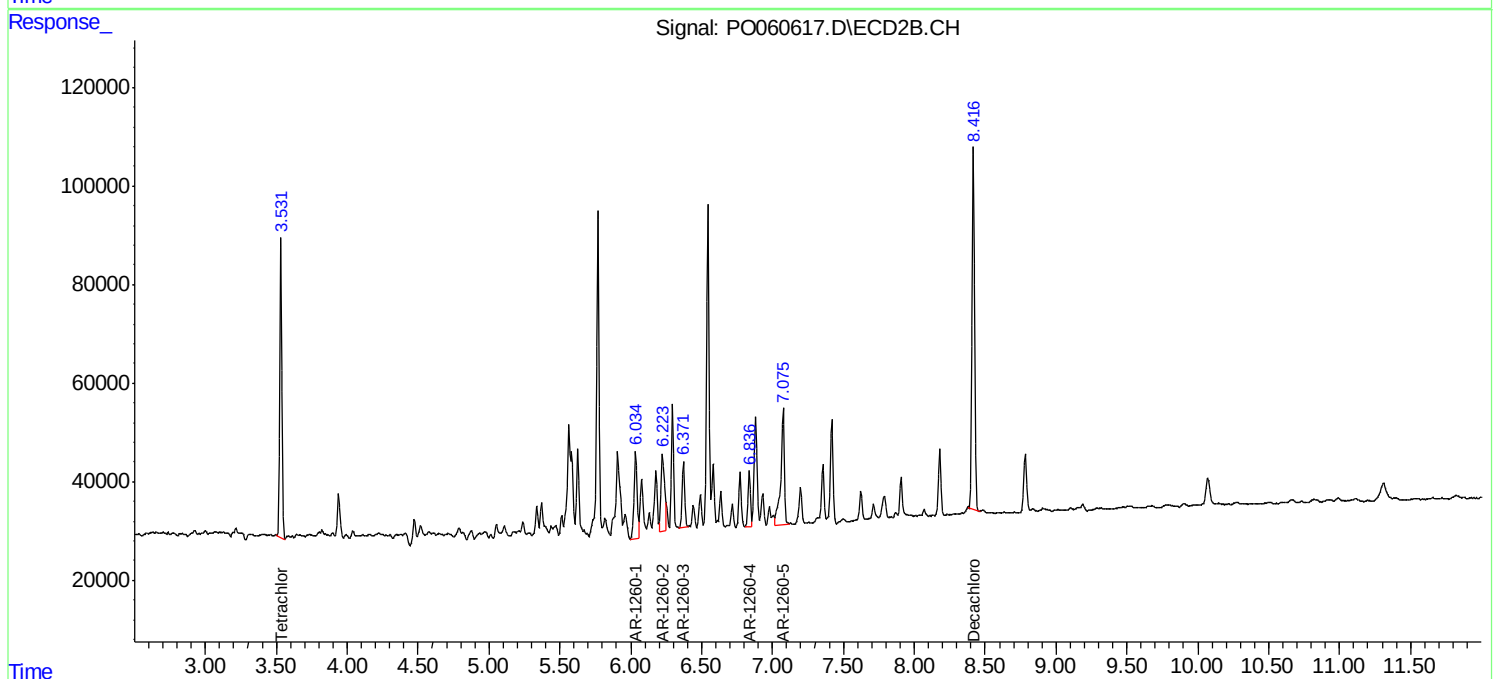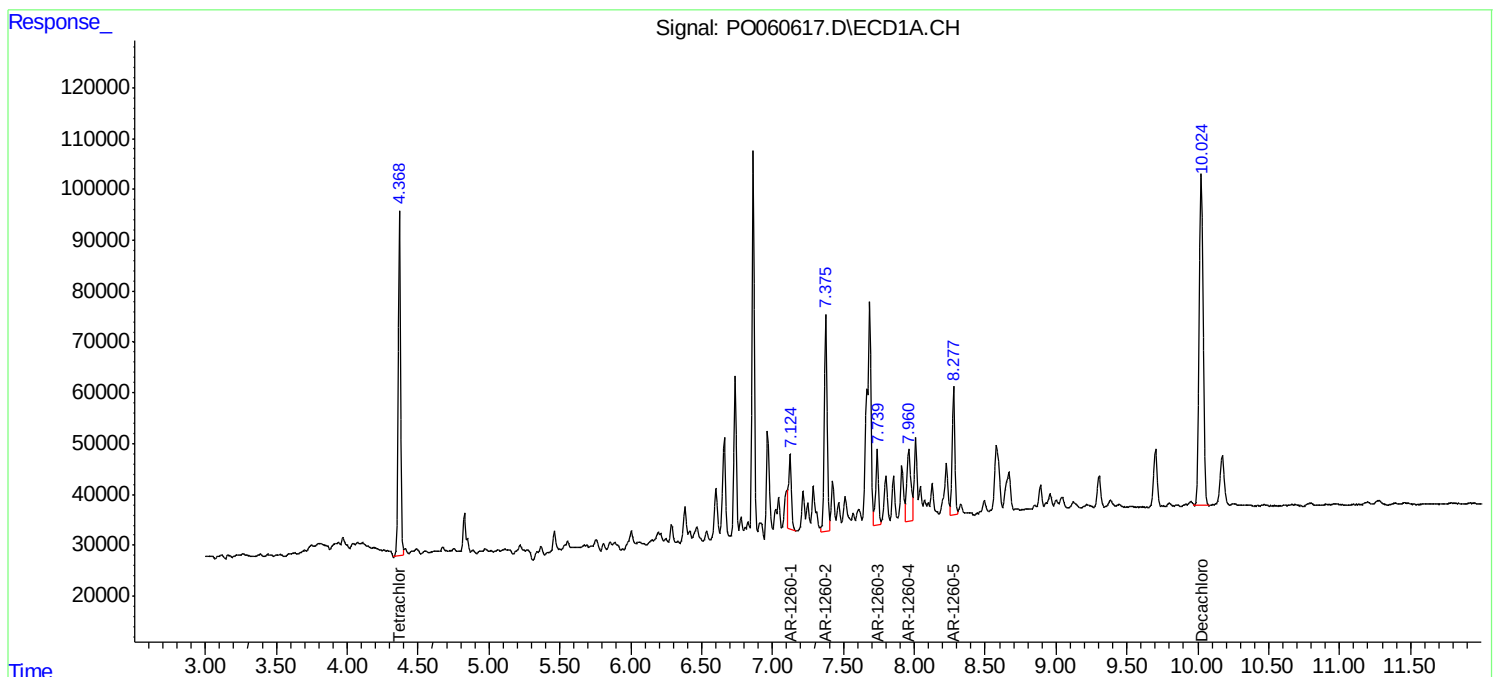

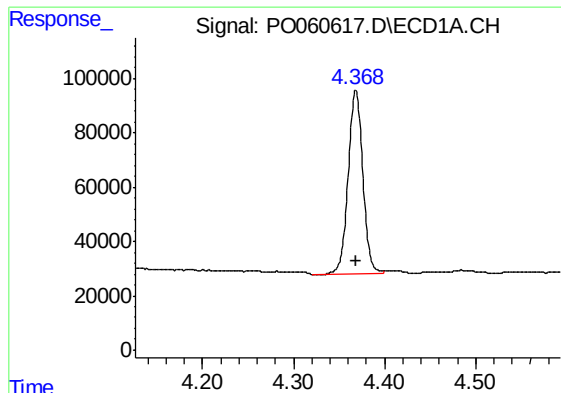


#1 Tetrachloro-m-xylene

R.T.: 4.368 min
Delta R.T.: 0.000 min
Response: 762297
Conc: 18.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-20-COMP


Manual Integrations
APPROVED

Ankita
9/11/2019 9:09:34 AM

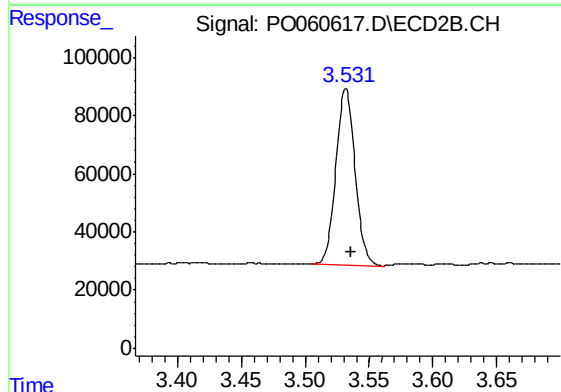


#1 Tetrachloro-m-xylene

R.T.: 3.532 min
Delta R.T.: -0.004 min
Response: 628259
Conc: 20.45 ng/ml

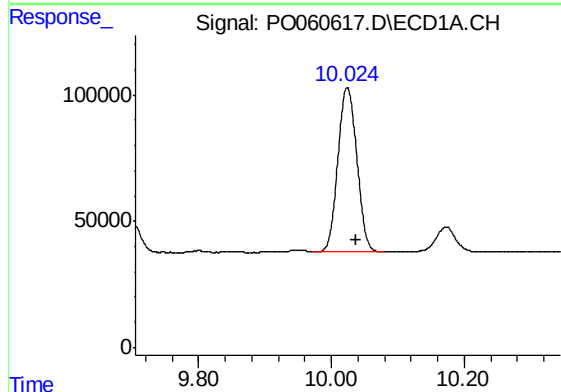


#2 Decachlorobiphenyl

R.T.: 10.024 min
Delta R.T.: -0.013 min
Response: 1293407
Conc: 24.52 ng/ml

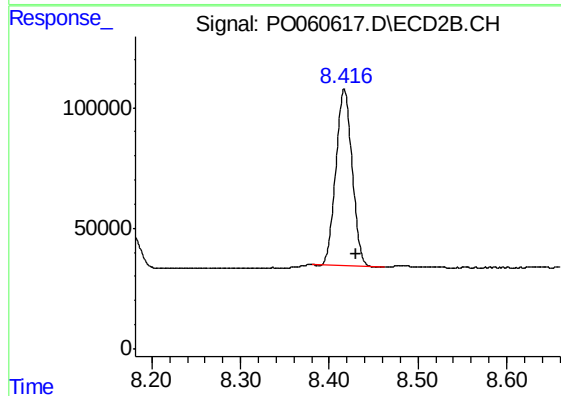

#2 Decachlorobiphenyl

R.T.: 8.417 min
Delta R.T.: -0.014 min
Response: 933944
Conc: 25.23 ng/ml

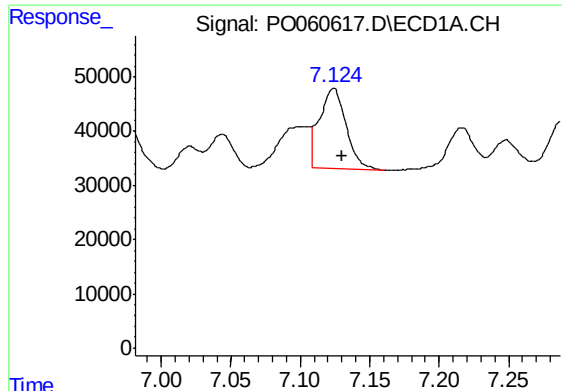


#31 AR-1260-1

R.T.: 7.124 min
Delta R.T.: -0.007 min
Response: 195848
Conc: 78.35 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-20-COMP


Manual Integrations
APPROVED

Ankita
9/11/2019 9:09:34 AM

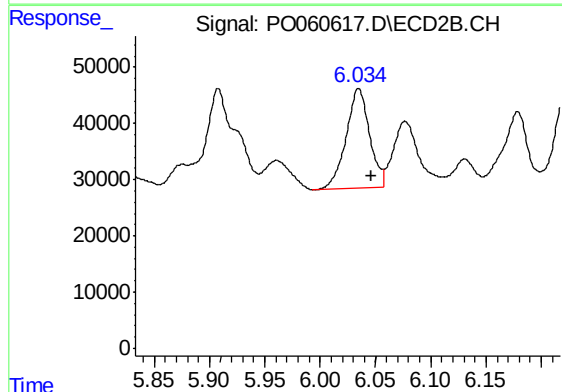


#31 AR-1260-1

R.T.: 6.035 min
Delta R.T.: -0.011 min
Response: 262117
Conc: 127.46 ng/ml

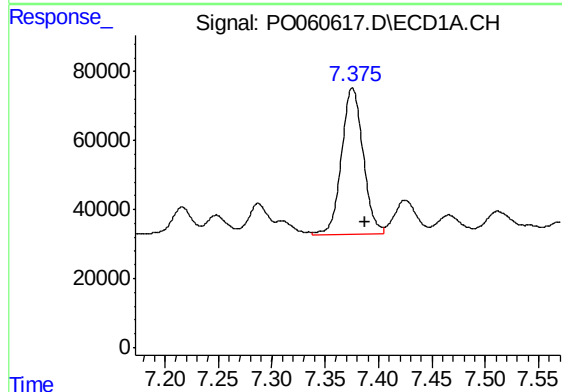


#32 AR-1260-2

R.T.: 7.376 min
Delta R.T.: -0.012 min
Response: 603068
Conc: 194.07 ng/ml

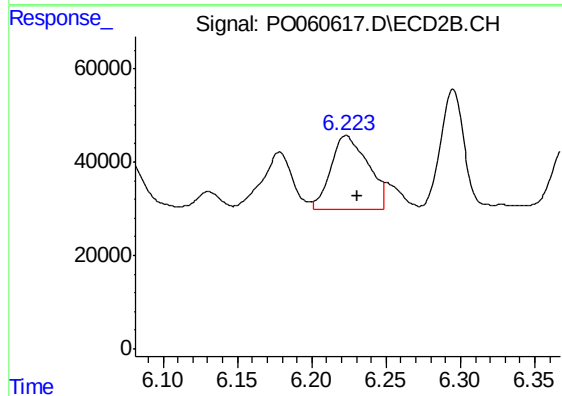

#32 AR-1260-2

R.T.: 6.223 min
Delta R.T.: -0.008 min
Response: 274401
Conc: 109.59 ng/ml m

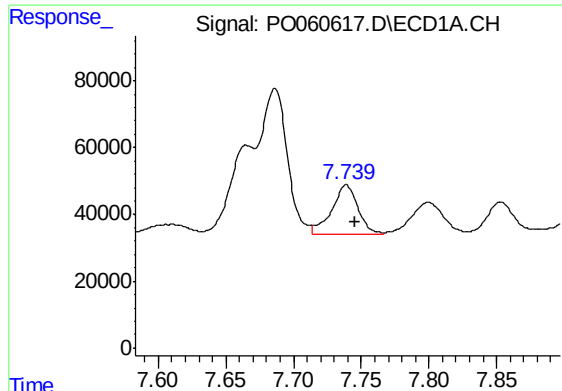


#33 AR-1260-3

R.T.: 7.739 min
Delta R.T.: -0.006 min
Response: 200145
Conc: 80.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-20-COMP


Manual Integrations
APPROVED

Ankita
9/11/2019 9:09:34 AM

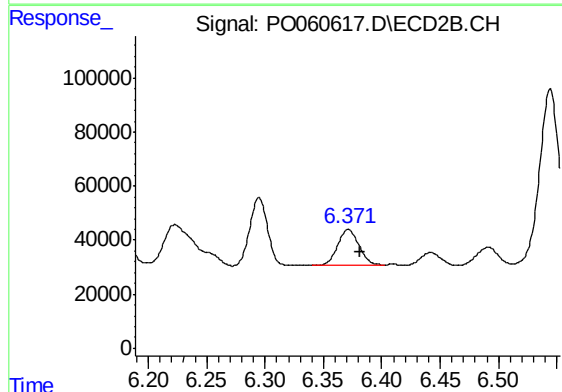


#33 AR-1260-3

R.T.: 6.371 min
Delta R.T.: -0.010 min
Response: 166657
Conc: 71.73 ng/ml

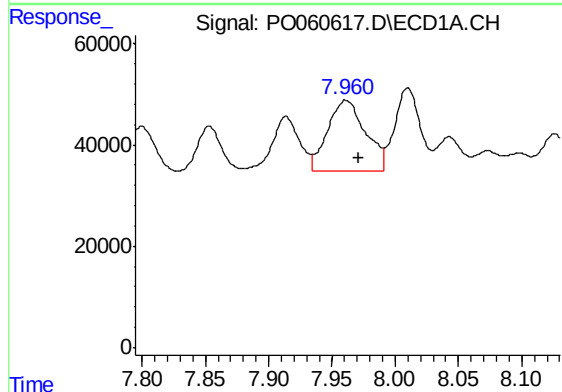


#34 AR-1260-4

R.T.: 7.961 min
Delta R.T.: -0.010 min
Response: 290850
Conc: 98.23 ng/ml

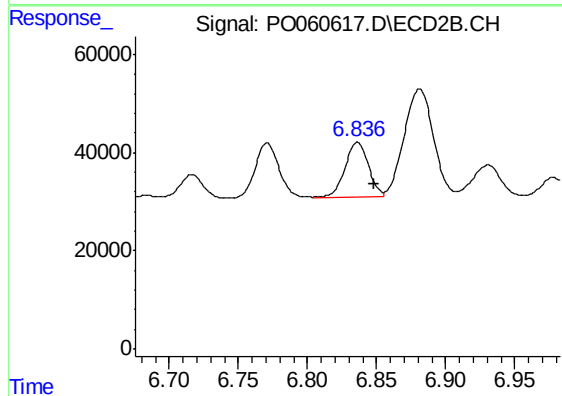

#34 AR-1260-4

R.T.: 6.836 min
Delta R.T.: -0.012 min
Response: 133247
Conc: 65.60 ng/ml

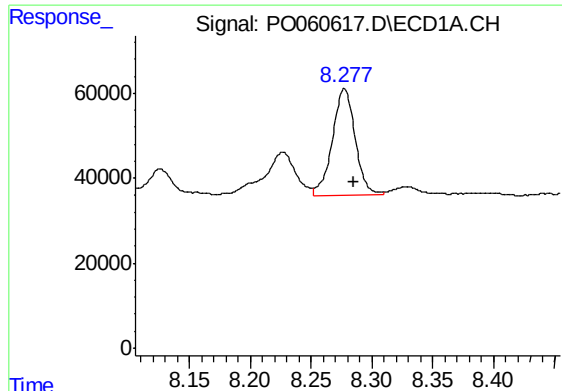


#35 AR-1260-5

R.T.: 8.277 min
Delta R.T.: -0.007 min
Response: 329496
Conc: 58.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-20-COMP

Manual Integrations
APPROVED

Ankita
9/11/2019 9:09:34 AM

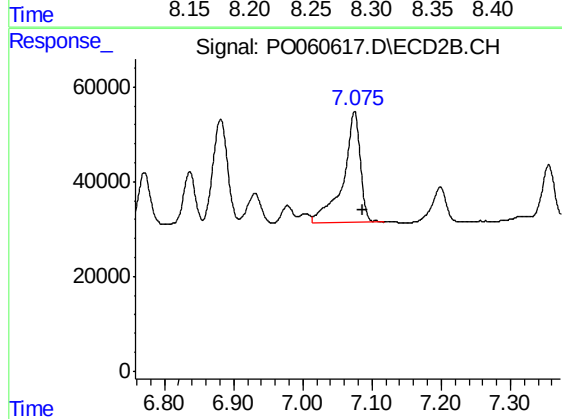

#35 AR-1260-5

R.T.: 7.075 min
Delta R.T.: -0.011 min
Response: 407892
Conc: 89.04 ng/ml