

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091019\
Data File : P0060641.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Sep 2019 17:59
Operator : SM/AJ
Sample : K4786-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 03:00:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Sep 08 02:12:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.367	3.531	890586	720079	21.464	23.444
2)	SA Decachlor...	10.026	8.416	913499	707313	17.317	19.107

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091019\
Data File : PO060641.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Sep 2019 17:59
Operator : SM/AJ
Sample : K4786-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 03:00:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Sep 08 02:12:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

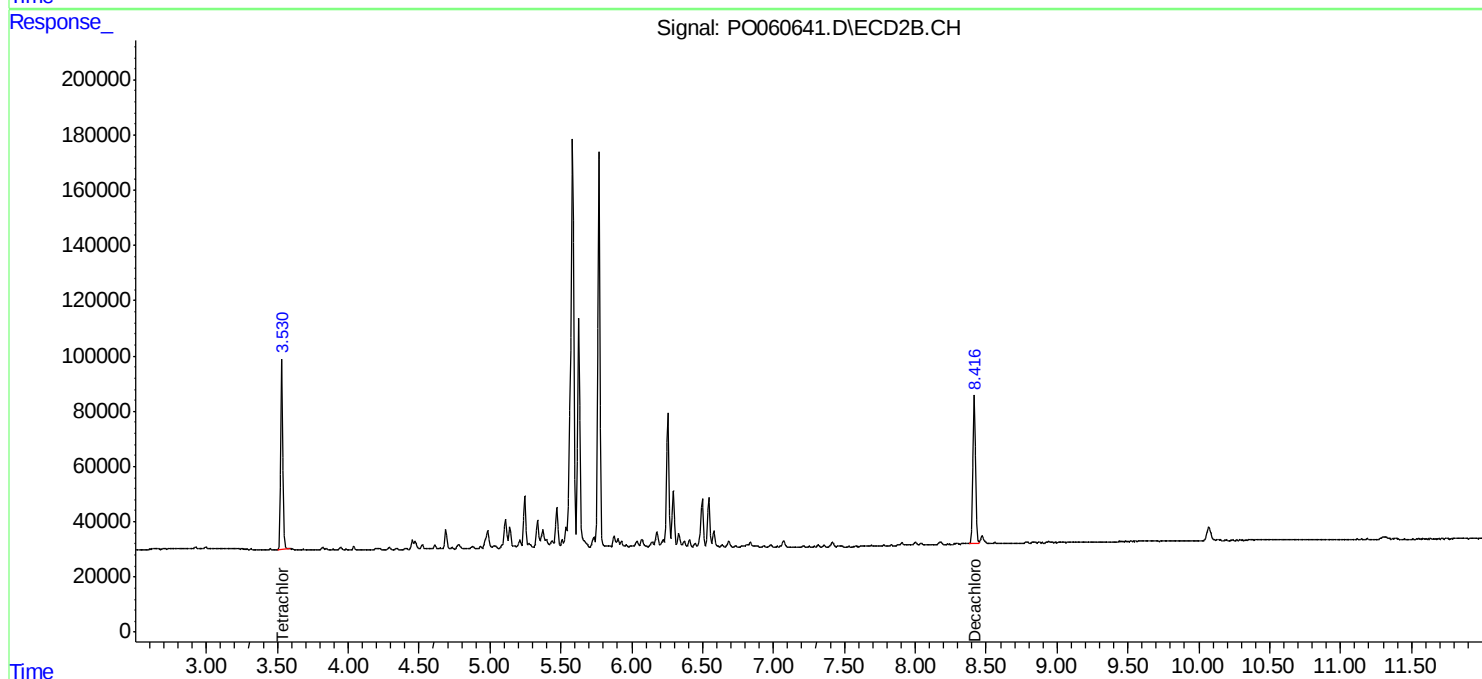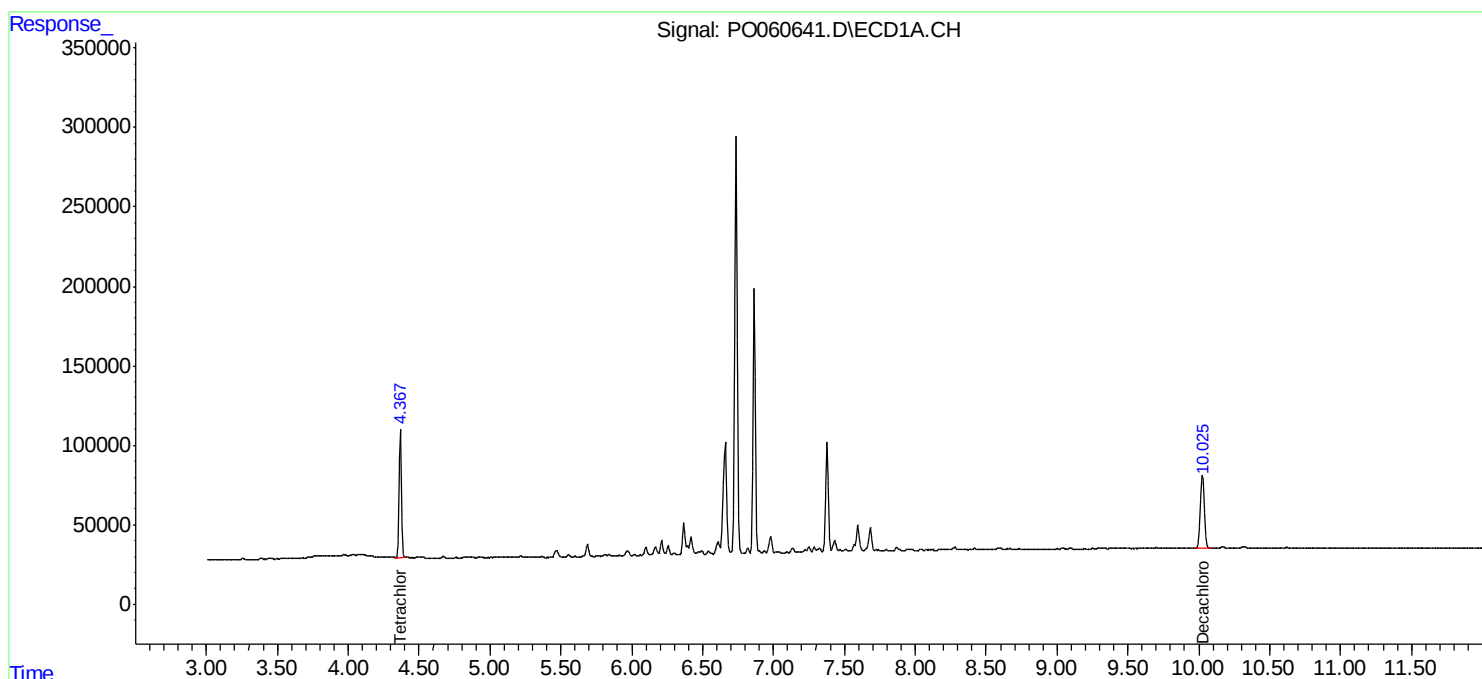


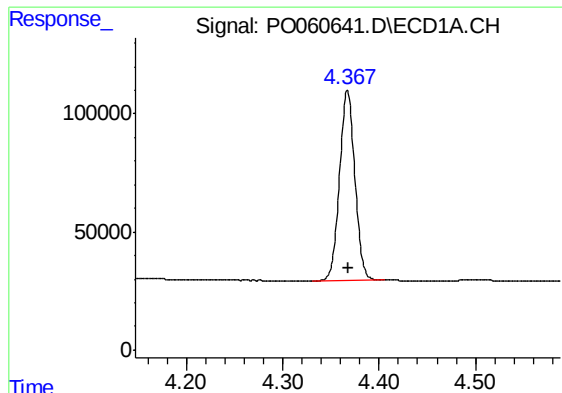

#1 Tetrachloro-m-xylene


R.T.: 4.367 min
Delta R.T.: -0.002 min
Response: 890586
Conc: 21.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP2

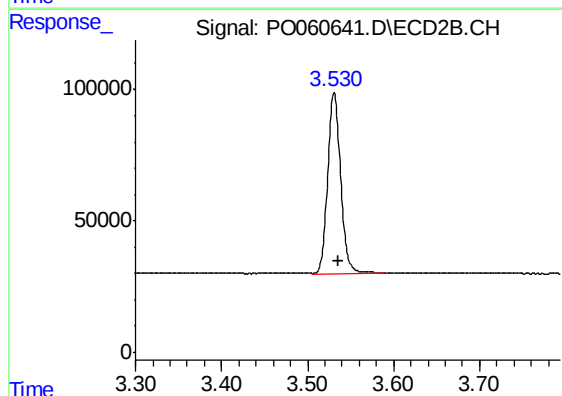


#1 Tetrachloro-m-xylene

R.T.: 3.531 min
Delta R.T.: -0.005 min
Response: 720079
Conc: 23.44 ng/ml

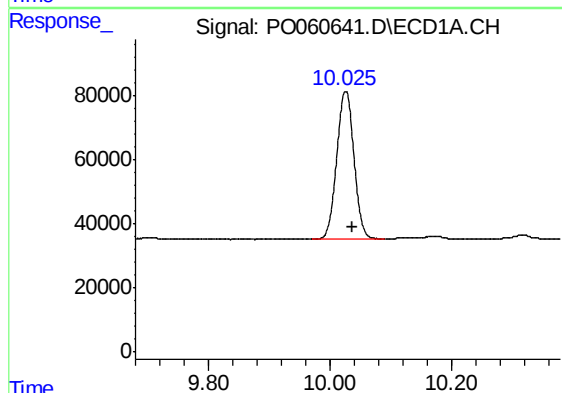

#2 Decachlorobiphenyl

R.T.: 10.026 min
Delta R.T.: -0.012 min
Response: 913499
Conc: 17.32 ng/ml

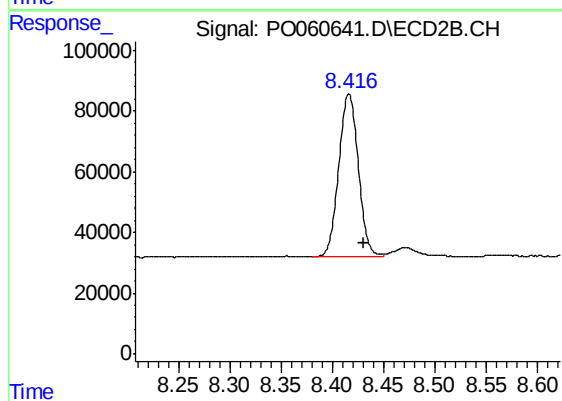

#2 Decachlorobiphenyl

R.T.: 8.416 min
Delta R.T.: -0.015 min
Response: 707313
Conc: 19.11 ng/ml