

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091020\
 Data File : P0071258.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Sep 2020 11:07
 Operator : DD\AJ
 Sample : L3939-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 15:37:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.345	3.530	1581520	885513	22.317	22.682
2)	SA Decachlor...	9.959	8.710	1922780	1080686	20.619	19.619
Target Compounds							
10)	L2 AR-1221-3	4.798f	0.000	63019	0	34.669	N.D. #
11)	L3 AR-1232-1	4.798f	0.000	63019	0	42.102	N.D. #
24)	L5 AR-1248-4	6.552f	0.000	155695	0	42.845	N.D. #
26)	L6 AR-1254-1	6.552	0.000	155695	0	44.378	N.D. #
28)	L6 AR-1254-3	7.171f	0.000	144923	0	24.368	N.D. #
29)	L6 AR-1254-4	7.460f	0.000	68921	0	11.864	N.D. #
30)	L6 AR-1254-5	7.851	0.000	64521	0	11.566	N.D. #
42)	L9 AR-1268-2	8.848f	0.000	183719	0	13.142	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091020\
Data File : PO071258.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Sep 2020 11:07
Operator : DD\AJ
Sample : L3939-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 15:37:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

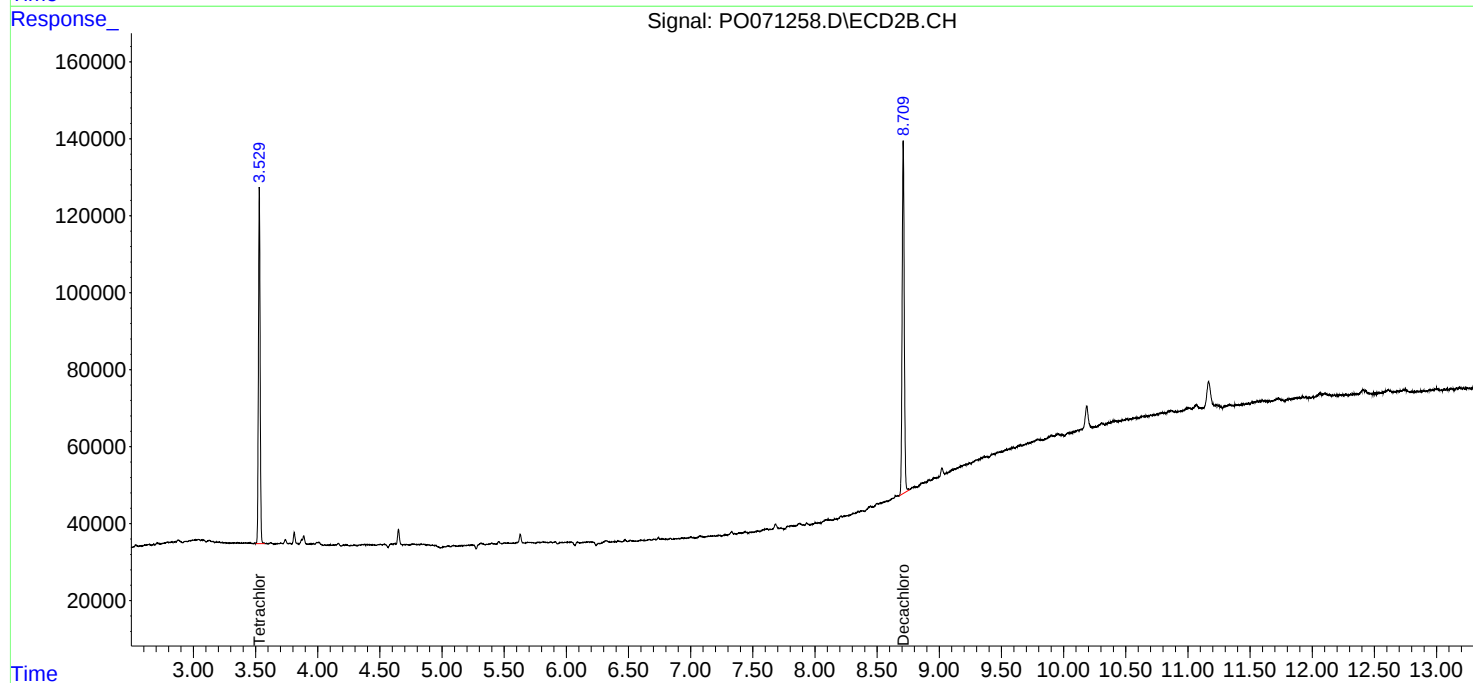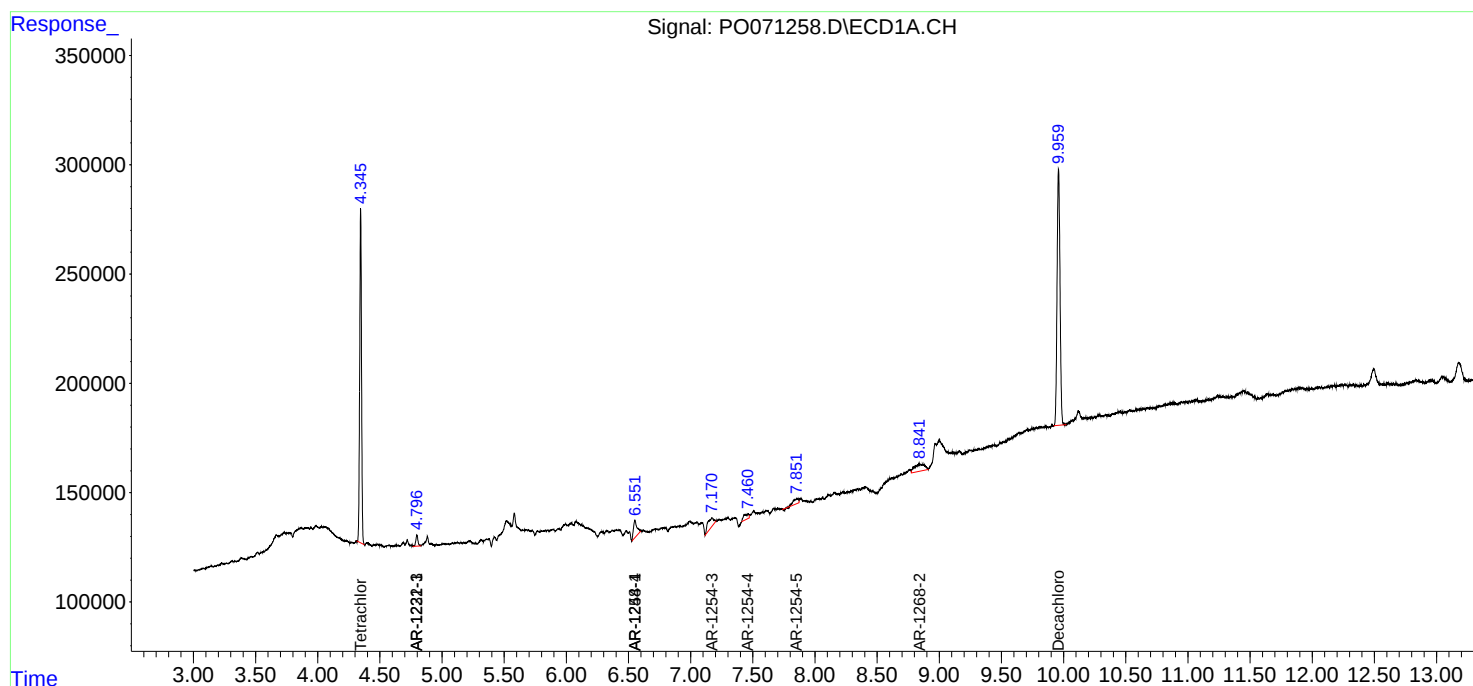


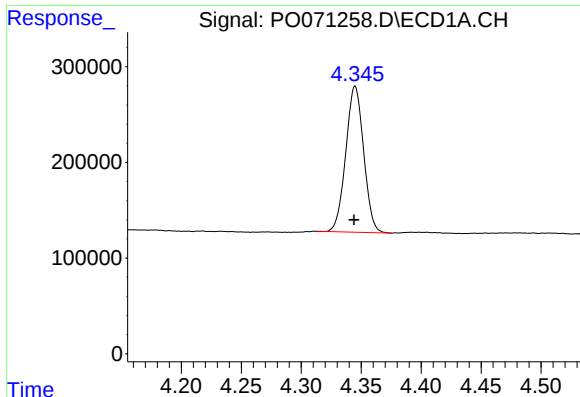

#1 Tetrachloro-m-xylene


R.T.: 4.345 min
Delta R.T.: 0.000 min
Response: 1581520
Conc: 22.32 ng/ml

Instrument :
ECD_O
ClientSampleId :

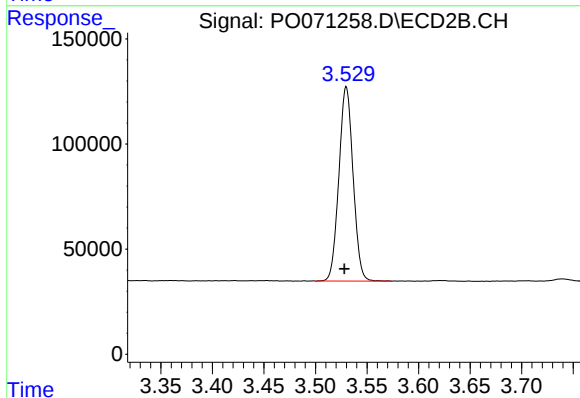


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: 0.002 min
Response: 885513
Conc: 22.68 ng/ml

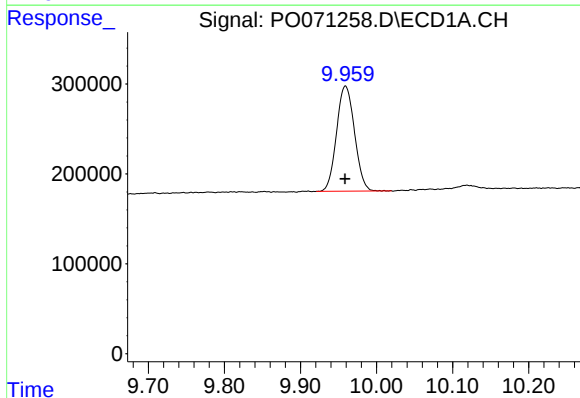


#2 Decachlorobiphenyl

R.T.: 9.959 min
Delta R.T.: 0.000 min
Response: 1922780
Conc: 20.62 ng/ml

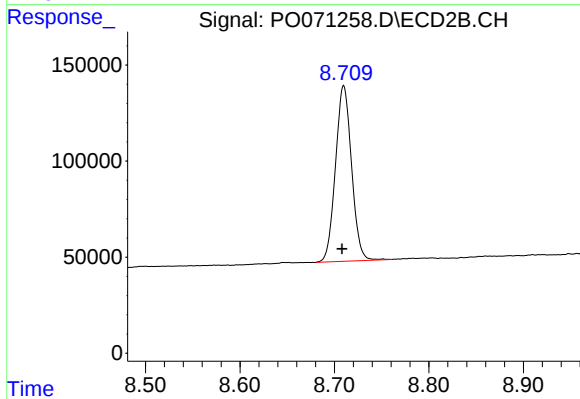

#2 Decachlorobiphenyl


R.T.: 8.710 min
Delta R.T.: 0.002 min
Response: 1080686
Conc: 19.62 ng/ml

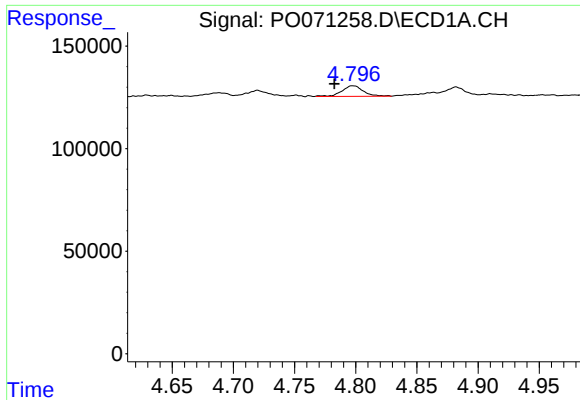

#10 AR-1221-3


R.T.: 4.798 min
Delta R.T.: 0.015 min
Response: 63019
Conc: 34.67 ng/ml

Instrument :
ECD_O
ClientSampleId :

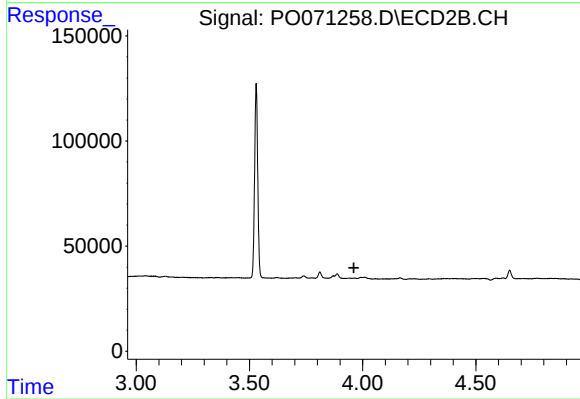


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 3.961 min
Response: 0
Conc: N.D.

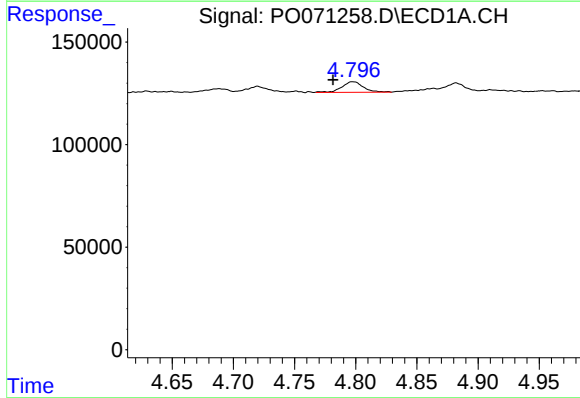


#11 AR-1232-1

R.T.: 4.798 min
Delta R.T.: 0.016 min
Response: 63019
Conc: 42.10 ng/ml

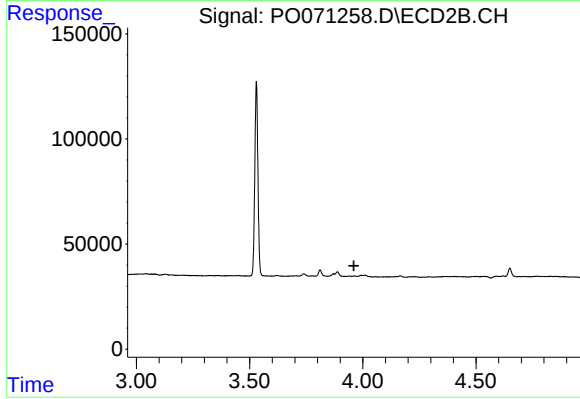

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 3.960 min
Response: 0
Conc: N.D.

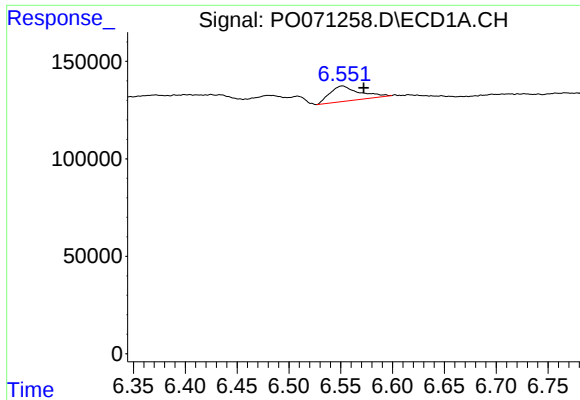

#24 AR-1248-4


R.T.: 6.552 min
Delta R.T.: -0.021 min
Response: 155695
Conc: 42.84 ng/ml

Instrument :
ECD_O
ClientSampleId :

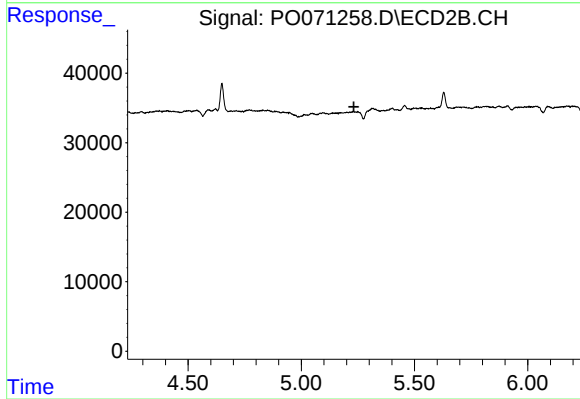


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.233 min
Response: 0
Conc: N.D.

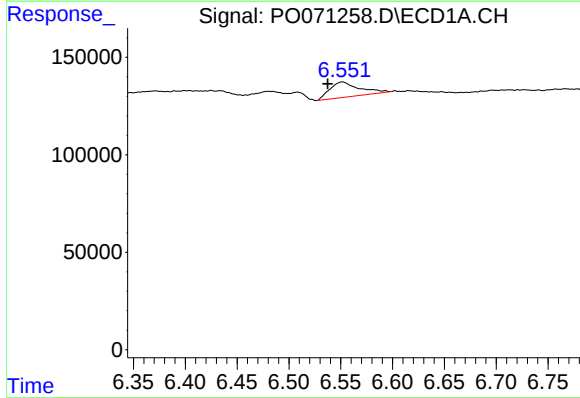


#26 AR-1254-1

R.T.: 6.552 min
Delta R.T.: 0.014 min
Response: 155695
Conc: 44.38 ng/ml

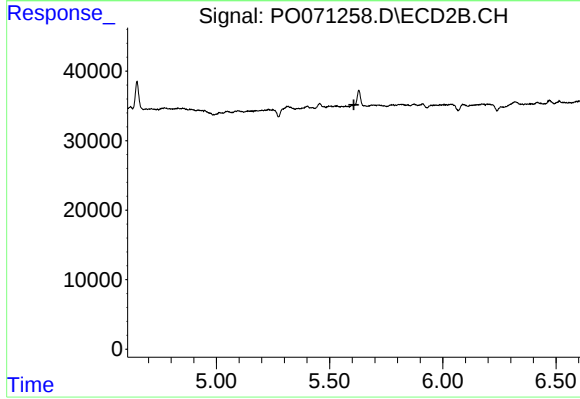

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.607 min
Response: 0
Conc: N.D.

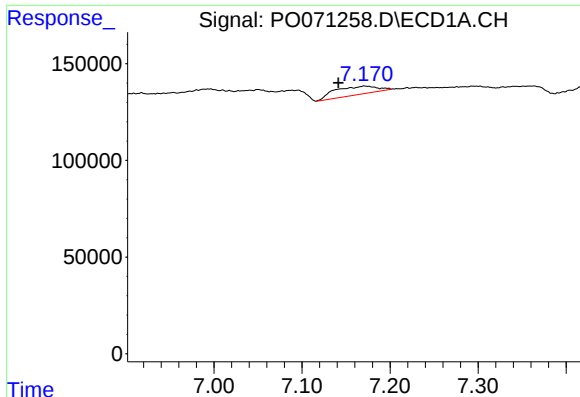

#28 AR-1254-3


R.T.: 7.171 min
Delta R.T.: 0.029 min
Response: 144923
Conc: 24.37 ng/ml

Instrument :
ECD_O
ClientSampleId :

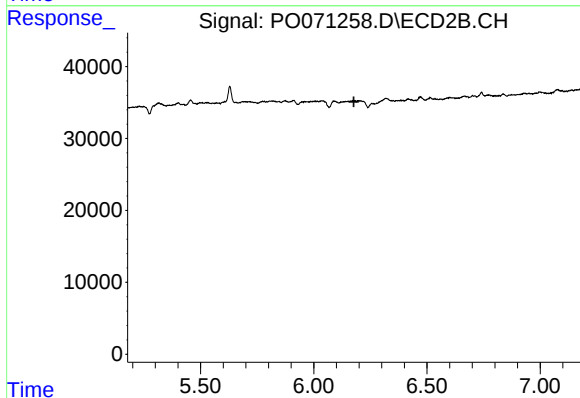


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.177 min
Response: 0
Conc: N.D.

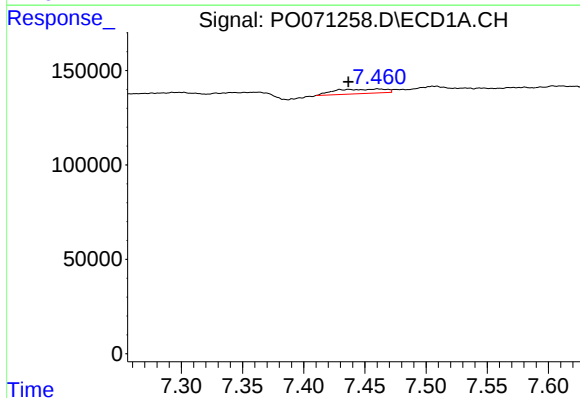


#29 AR-1254-4

R.T.: 7.460 min
Delta R.T.: 0.024 min
Response: 68921
Conc: 11.86 ng/ml

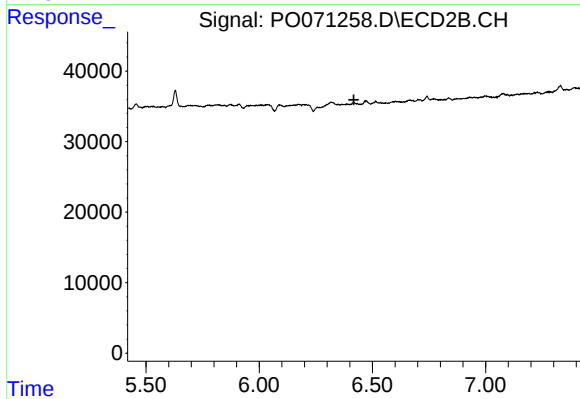

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.418 min
Response: 0
Conc: N.D.

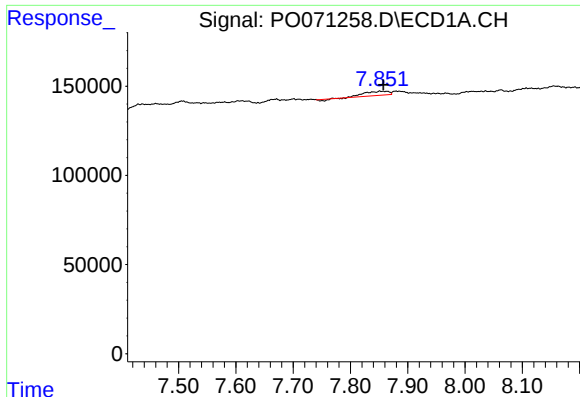

#30 AR-1254-5


R.T.: 7.851 min
Delta R.T.: -0.006 min
Response: 64521
Conc: 11.57 ng/ml

Instrument :
ECD_O
ClientSampleId :

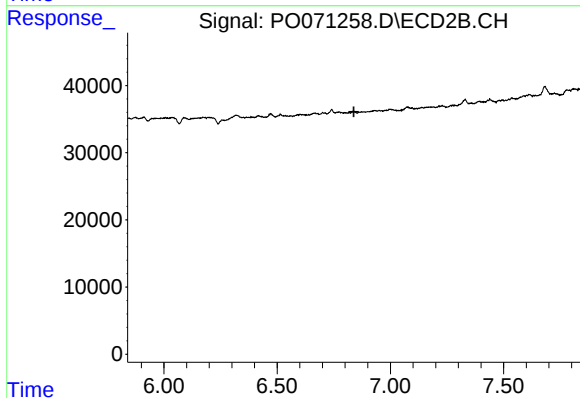


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.839 min
Response: 0
Conc: N.D.

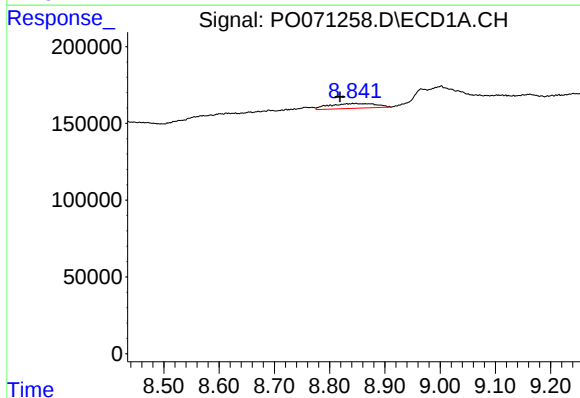

#42 AR-1268-2

R.T.: 8.848 min
Delta R.T.: 0.029 min
Response: 183719
Conc: 13.14 ng/ml

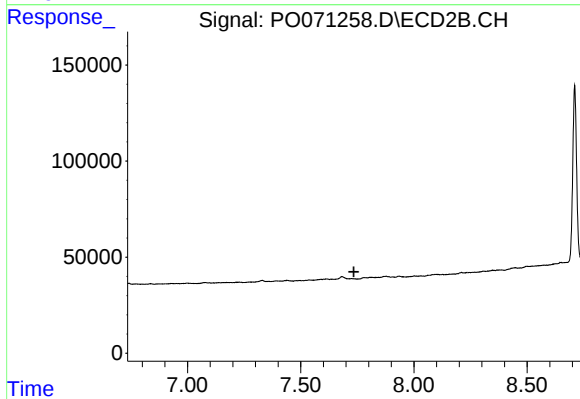

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.735 min
Response: 0
Conc: N.D.