

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091020\
 Data File : P0071258.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Sep 2020 11:07
 Operator : DD\AJ
 Sample : L3939-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PAV-B41-090820-0-10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 15:37:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.345	3.530	1581520	885513	22.317	22.682
2) SA Decachlor...	9.959	8.710	1922780	1080686	20.619	19.619

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091020\
Data File : P0071258.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Sep 2020 11:07
Operator : DD\AJ
Sample : L3939-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PAV-B41-090820-0-10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 15:37:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

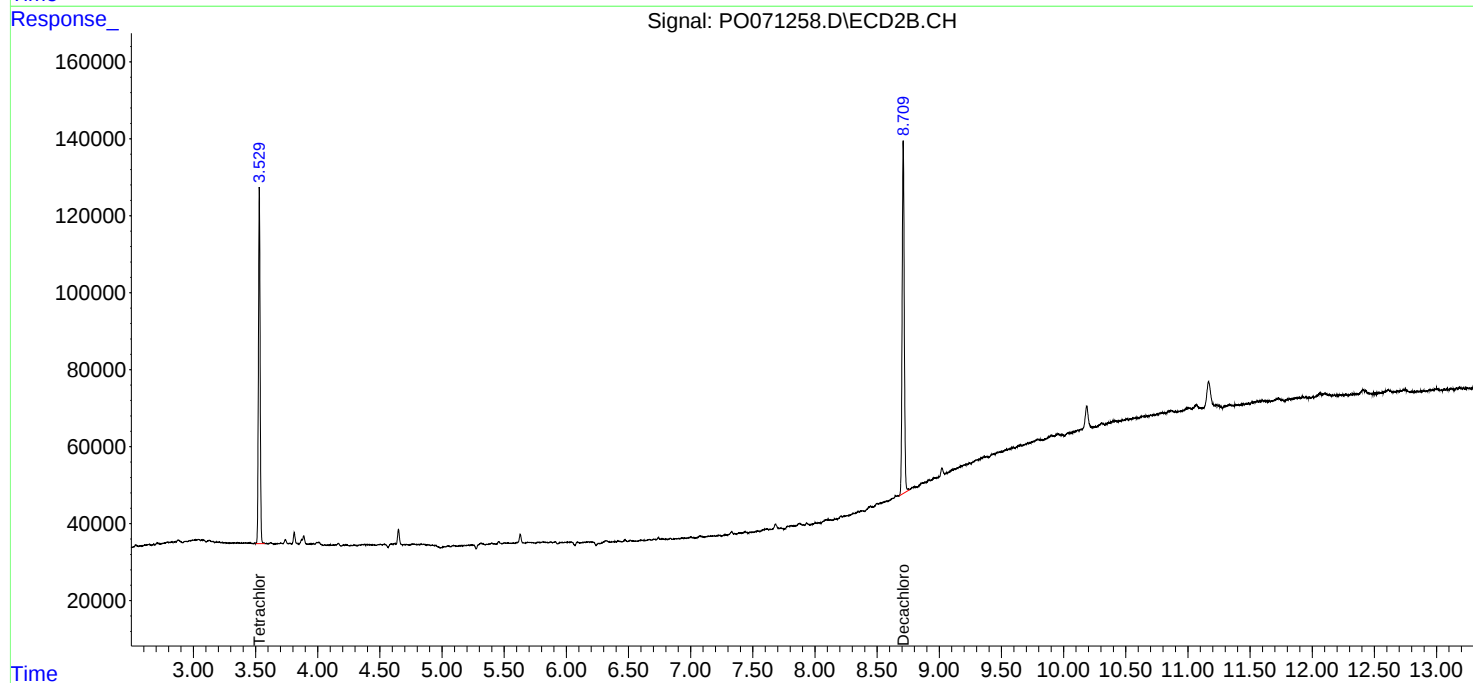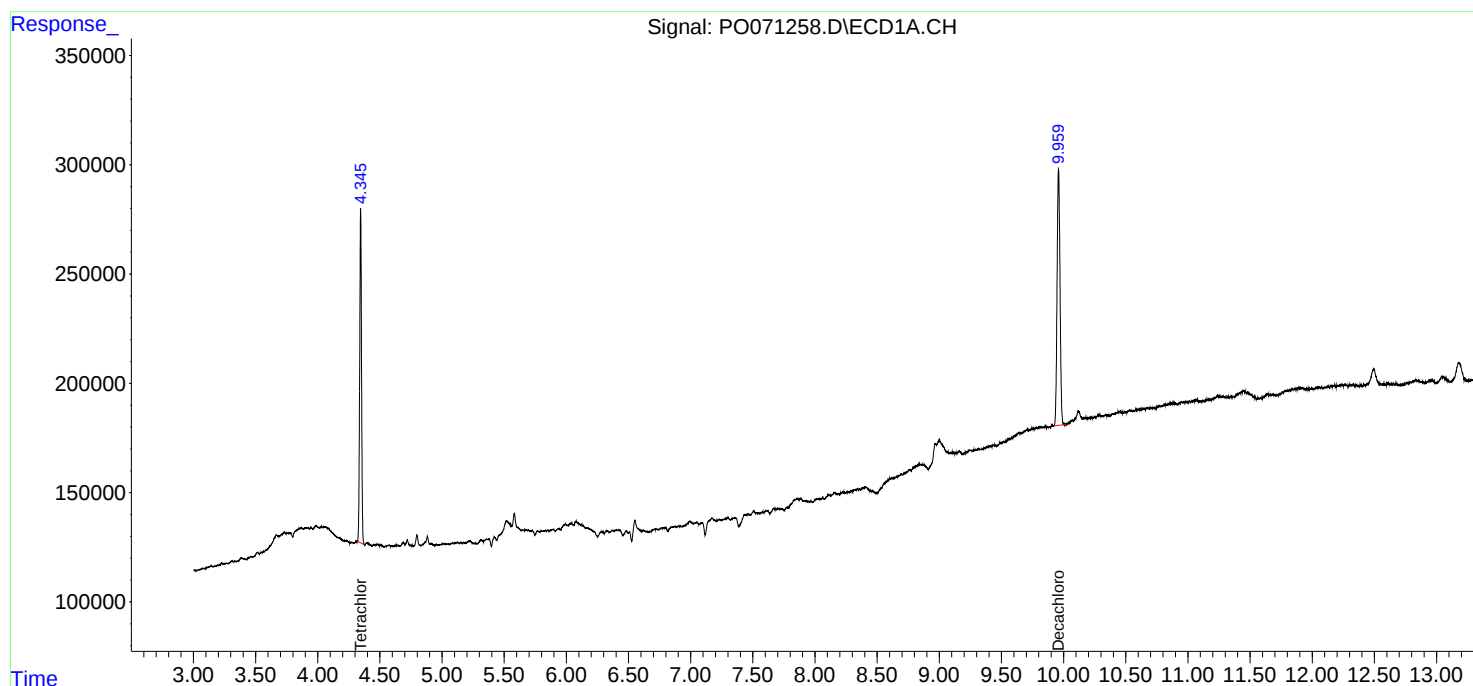


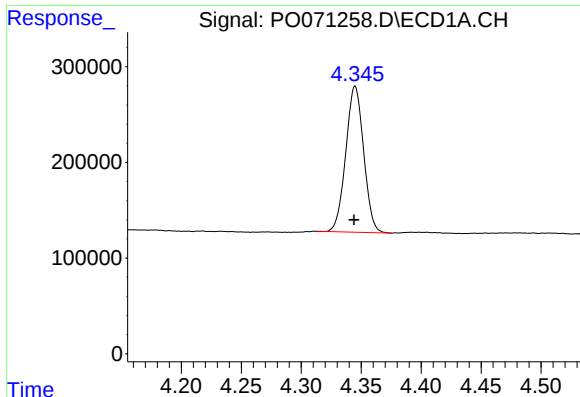

#1 Tetrachloro-m-xylene


R.T.: 4.345 min
Delta R.T.: 0.000 min
Response: 1581520
Conc: 22.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
PAV-B41-090820-0-10

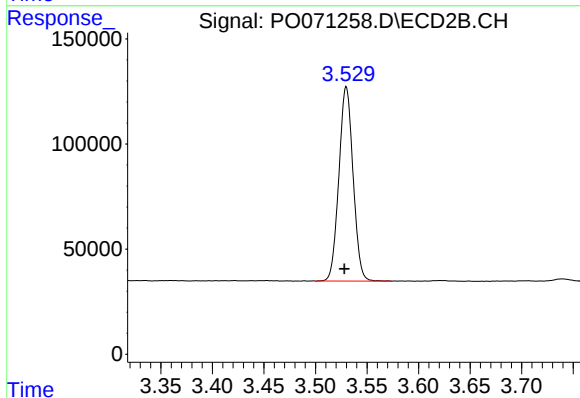


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: 0.002 min
Response: 885513
Conc: 22.68 ng/ml

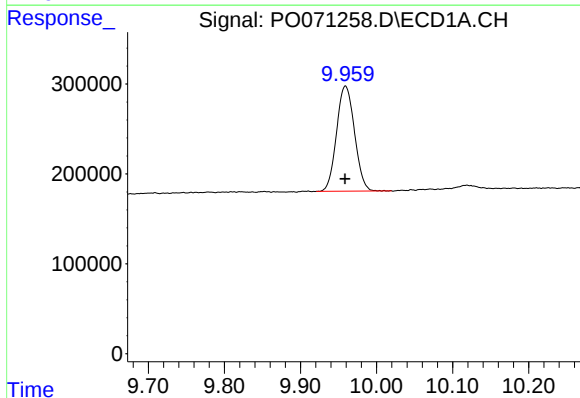

#2 Decachlorobiphenyl

R.T.: 9.959 min
Delta R.T.: 0.000 min
Response: 1922780
Conc: 20.62 ng/ml

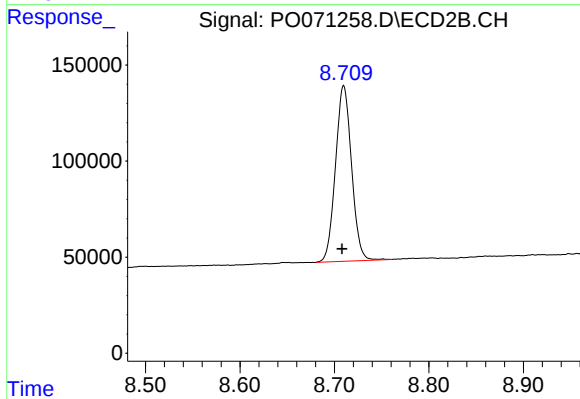

#2 Decachlorobiphenyl

R.T.: 8.710 min
Delta R.T.: 0.002 min
Response: 1080686
Conc: 19.62 ng/ml