

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091020\
 Data File : P0071259.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Sep 2020 11:24
 Operator : DD\AJ
 Sample : L3870-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SU-04-090820

Manual Integrations
 APPROVED

Ankita
 9/11/2020 11:48:13 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 15:37:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.345	3.530	1770854	963223	24.988m	24.672
2) SA Decachlor...	9.960	8.709	2146657	1167226	23.019	21.190

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091020\
Data File : P0071259.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Sep 2020 11:24
Operator : DD\AJ
Sample : L3870-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SU-04-090820


Manual Integrations
APPROVED

Ankita
9/11/2020 11:48:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 15:37:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

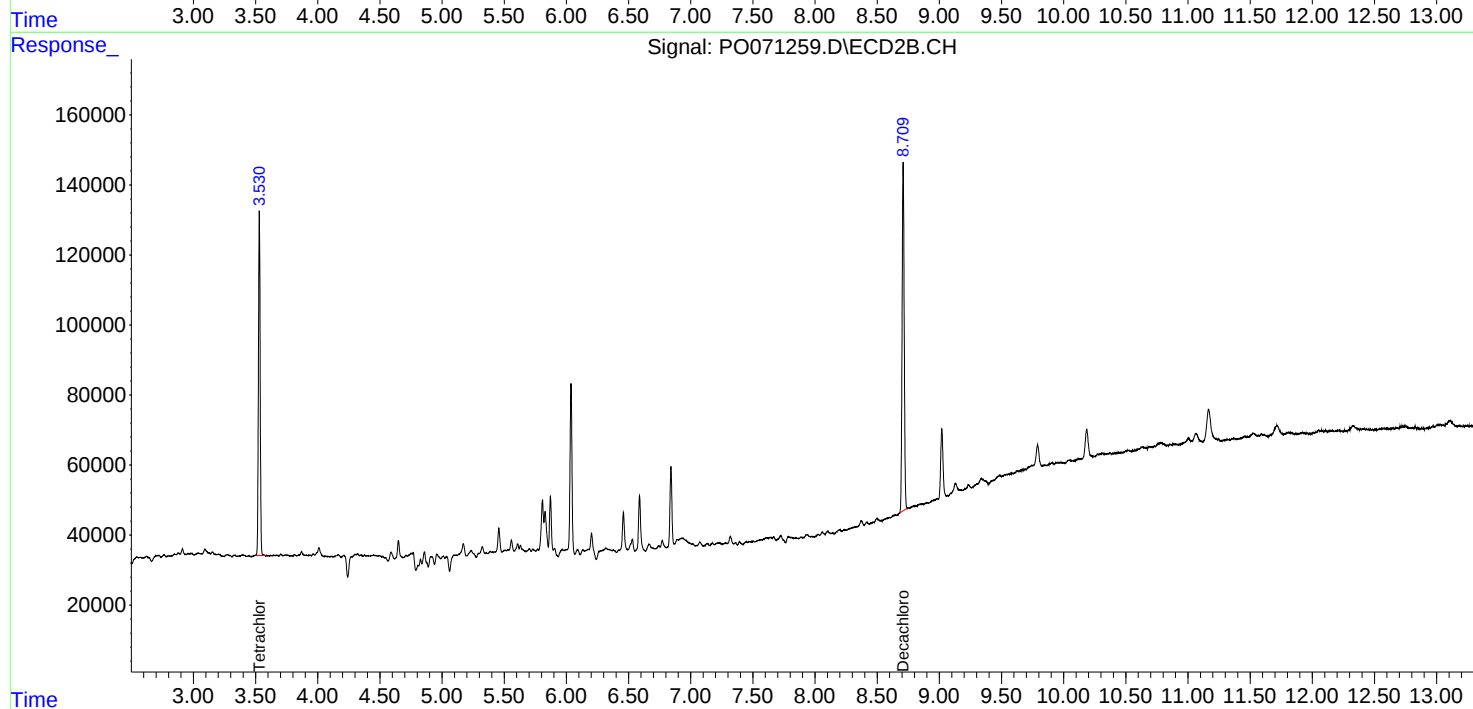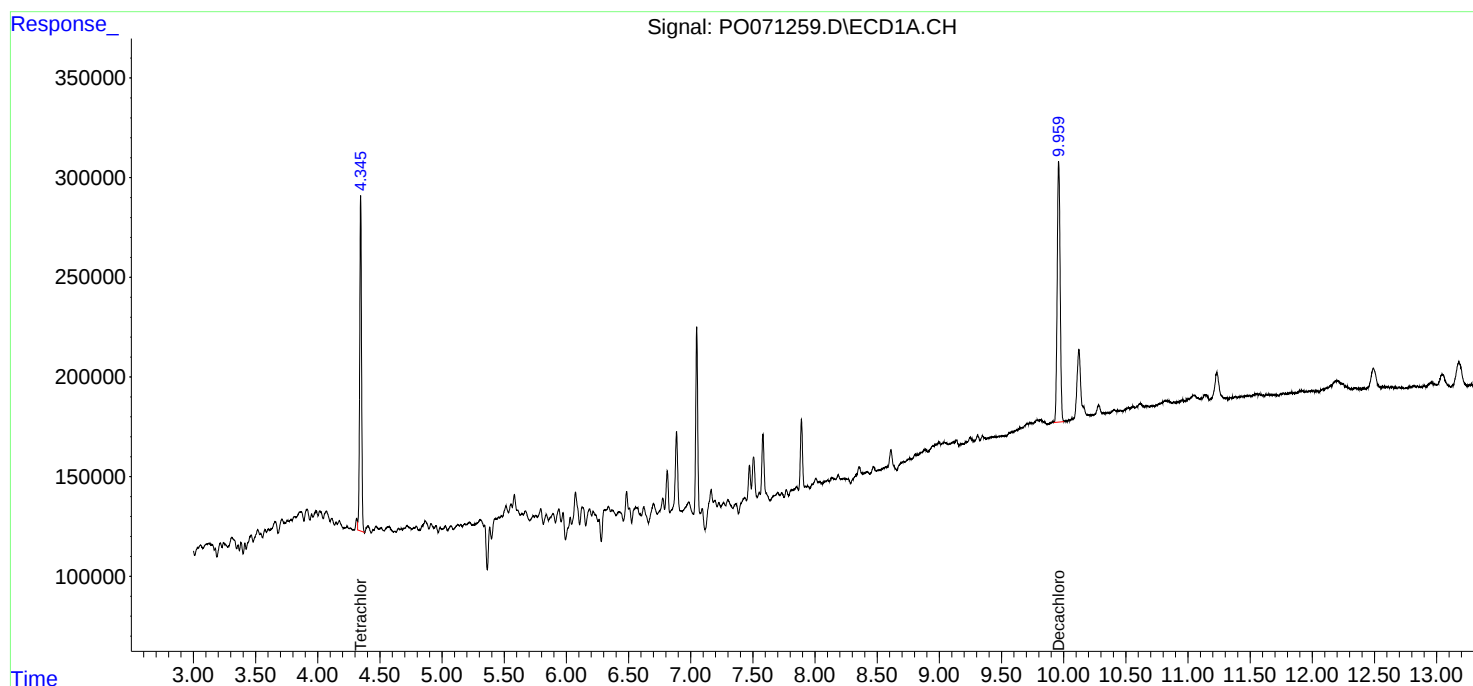

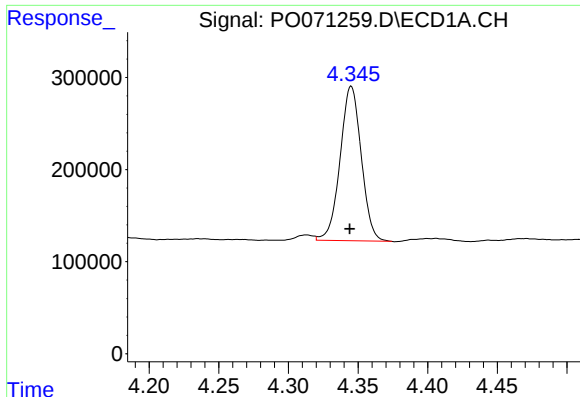


#1 Tetrachloro-m-xylene

R.T.: 4.345 min
Delta R.T.: 0.000 min
Response: 1770854
Conc: 24.99 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SU-04-090820


Manual Integrations
APPROVED

Ankita
9/11/2020 11:48:13 AM

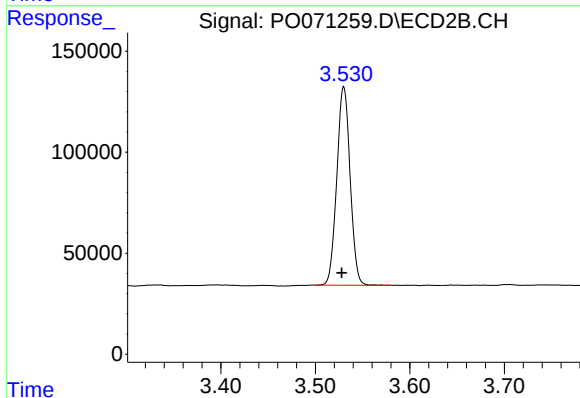


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: 0.002 min
Response: 963223
Conc: 24.67 ng/ml

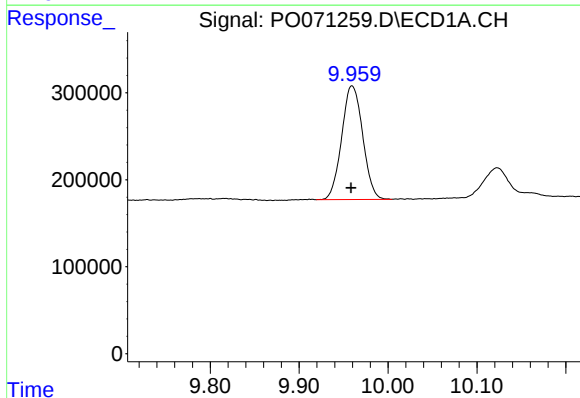

#2 Decachlorobiphenyl

R.T.: 9.960 min
Delta R.T.: 0.000 min
Response: 2146657
Conc: 23.02 ng/ml

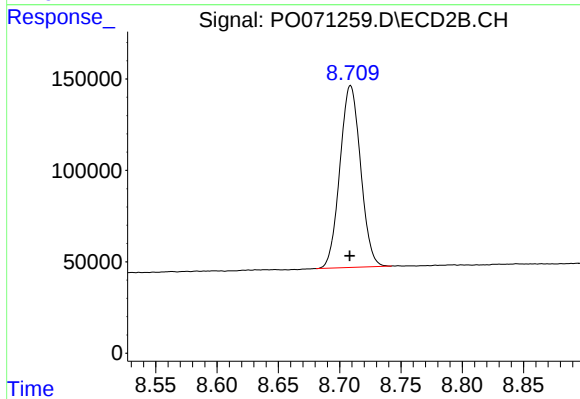

#2 Decachlorobiphenyl

R.T.: 8.709 min
Delta R.T.: 0.000 min
Response: 1167226
Conc: 21.19 ng/ml