

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091021\
 Data File : P0081104.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Sep 2021 7:00
 Operator : DD\AJ
 Sample : M3681-04
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 01:23:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.927	4.053	1487793	472970	18.847	19.139
2)	SA Decachlor...	10.991	9.411	627899	242152	10.575	10.373
Target Compounds							
8)	L2 AR-1221-1	5.181	0.000	59934	0	61.679	N.D. #
9)	L2 AR-1221-2	5.281	0.000	21612	0	29.399	N.D. #
24)	L5 AR-1248-4	7.199	0.000	23236	0	8.068	N.D. #
26)	L6 AR-1254-1	7.183	0.000	11571	0	3.580	N.D. #
27)	L6 AR-1254-2	7.413	0.000	39397	0	7.916	N.D. #
28)	L6 AR-1254-3	7.805	0.000	115701	0	22.882	N.D. #
32)	L7 AR-1260-2	0.000	7.104f	0	33228	N.D.	18.930 #
33)	L7 AR-1260-3	0.000	7.291	0	44050	N.D.	24.062 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091021\
Data File : P0081104.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2021 7:00
Operator : DD\AJ
Sample : M3681-04
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 01:23:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

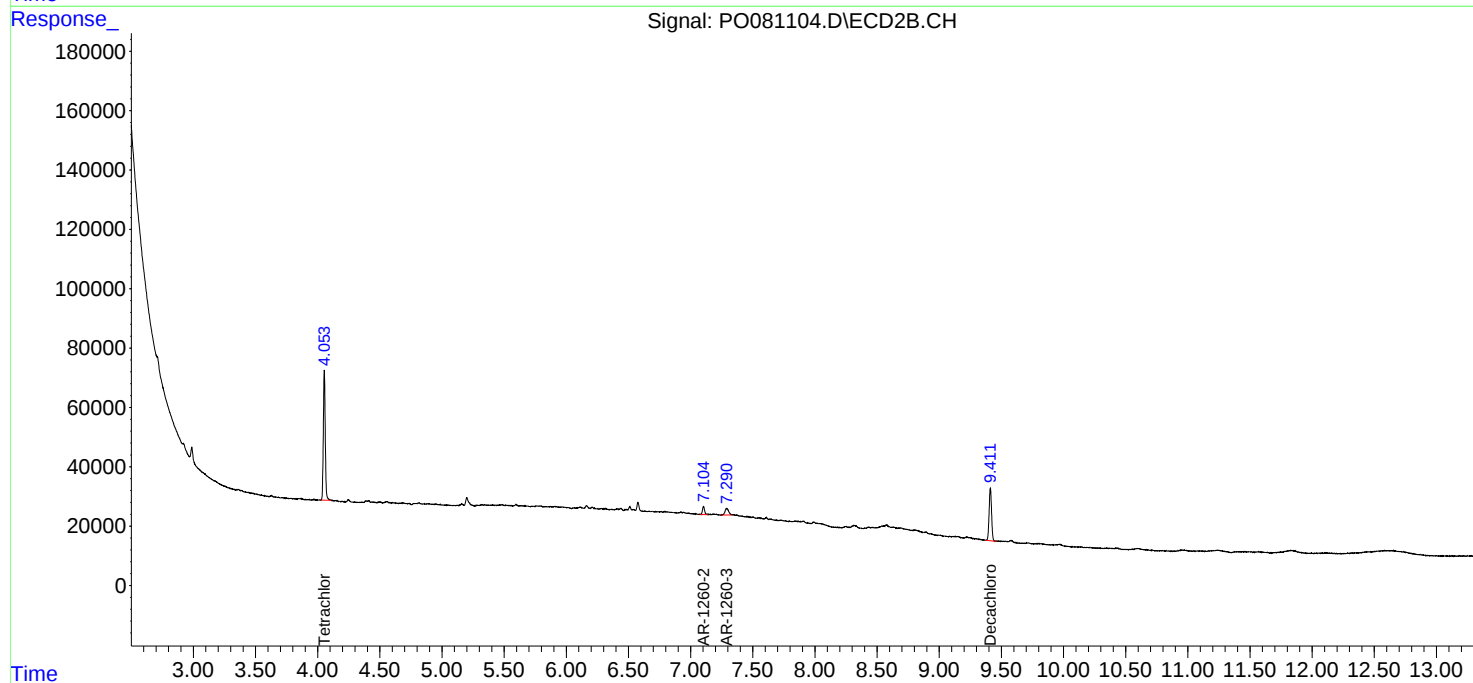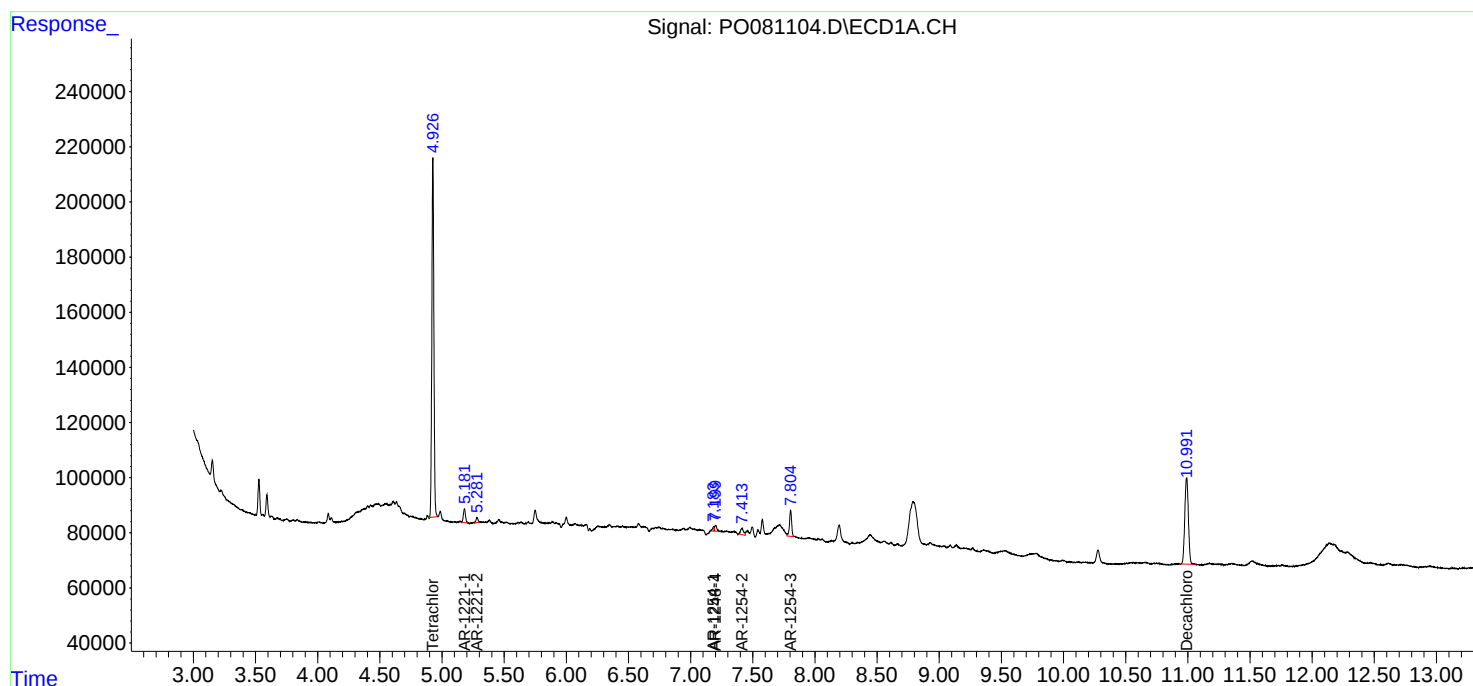


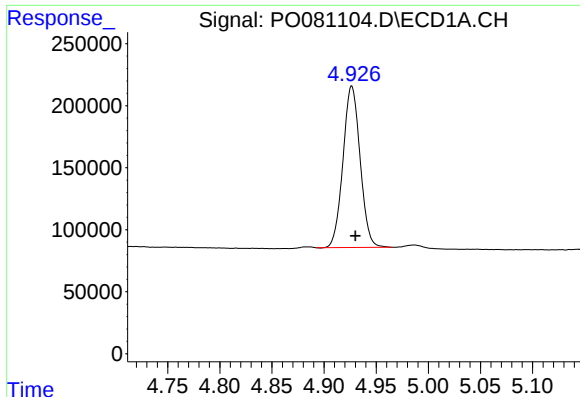

#1 Tetrachloro-m-xylene


R.T.: 4.927 min
Delta R.T.: -0.003 min
Response: 1487793
Conc: 18.85 ng/ml

Instrument :
ECD_O
ClientSampleId :

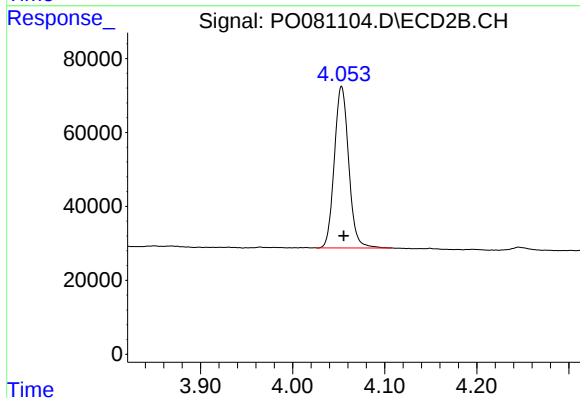


#1 Tetrachloro-m-xylene

R.T.: 4.053 min
Delta R.T.: -0.002 min
Response: 472970
Conc: 19.14 ng/ml

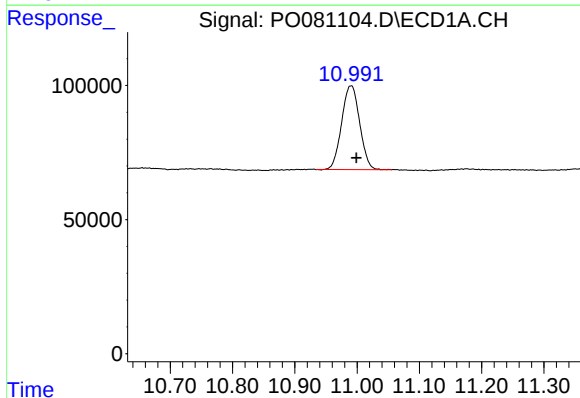


#2 Decachlorobiphenyl

R.T.: 10.991 min
Delta R.T.: -0.008 min
Response: 627899
Conc: 10.58 ng/ml

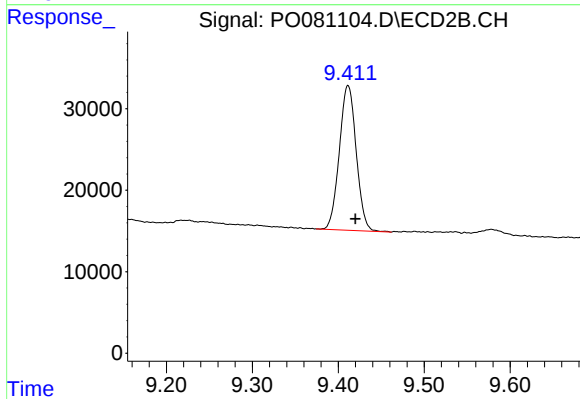

#2 Decachlorobiphenyl


R.T.: 9.411 min
Delta R.T.: -0.009 min
Response: 242152
Conc: 10.37 ng/ml

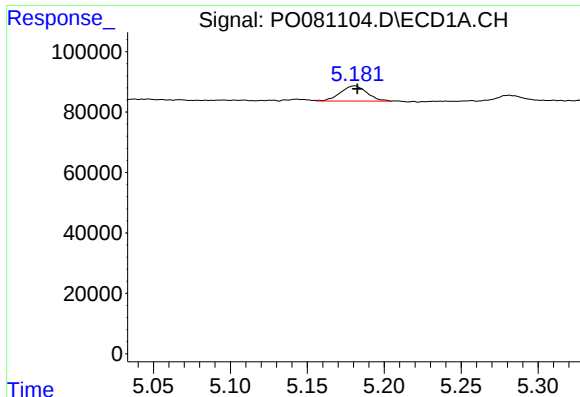

#8 AR-1221-1


R.T.: 5.181 min
Delta R.T.: -0.002 min
Response: 59934
Conc: 61.68 ng/ml

Instrument :
ECD_O
ClientSampleId :

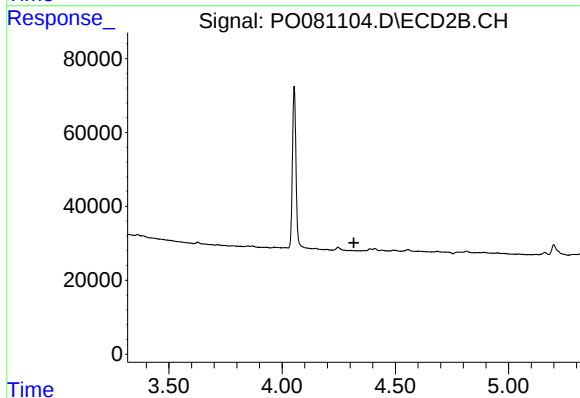


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

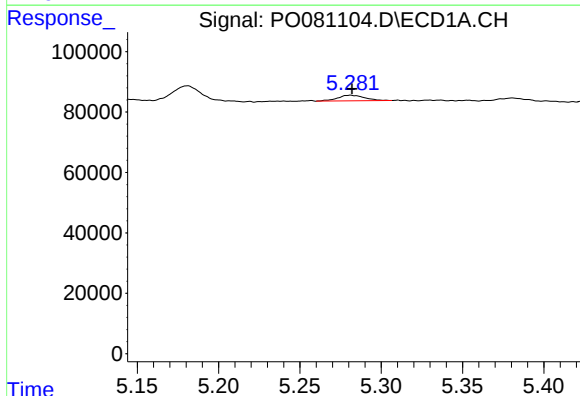


#9 AR-1221-2

R.T.: 5.281 min
Delta R.T.: 0.000 min
Response: 21612
Conc: 29.40 ng/ml

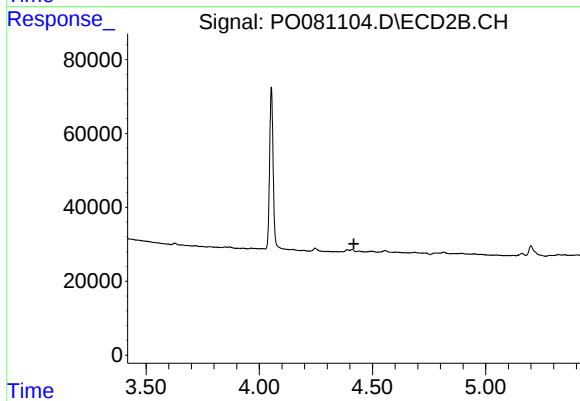

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.418 min
Response: 0
Conc: N.D.

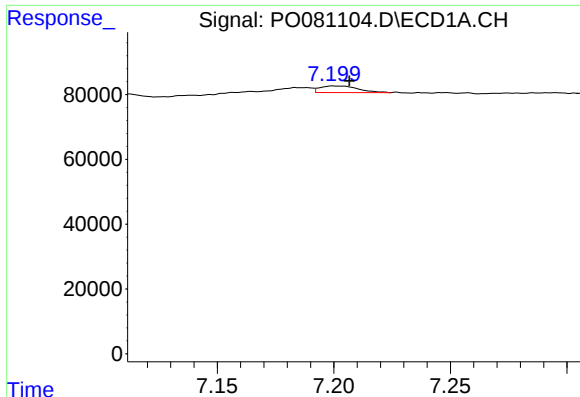

#24 AR-1248-4


R.T.: 7.199 min
Delta R.T.: -0.007 min
Response: 23236
Conc: 8.07 ng/ml

Instrument :
ECD_O
ClientSampleId :

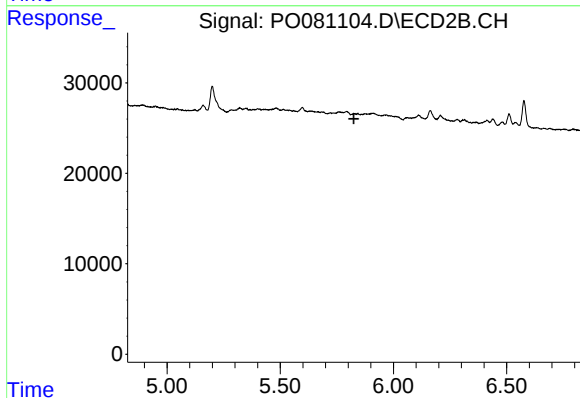


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.825 min
Response: 0
Conc: N.D.

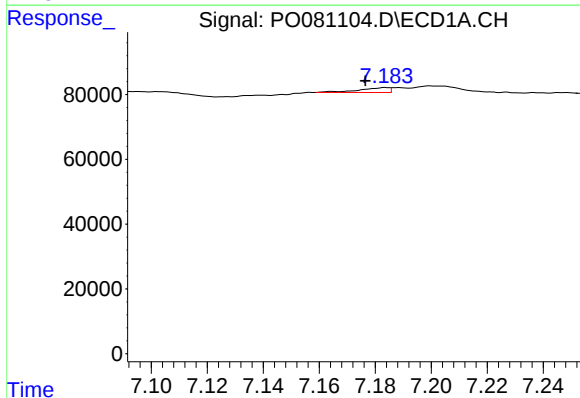


#26 AR-1254-1

R.T.: 7.183 min
Delta R.T.: 0.007 min
Response: 11571
Conc: 3.58 ng/ml

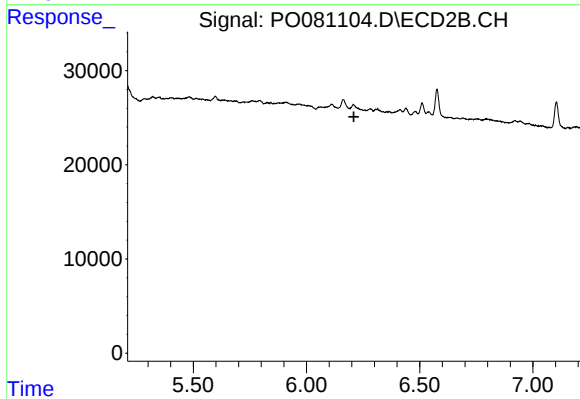

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.209 min
Response: 0
Conc: N.D.

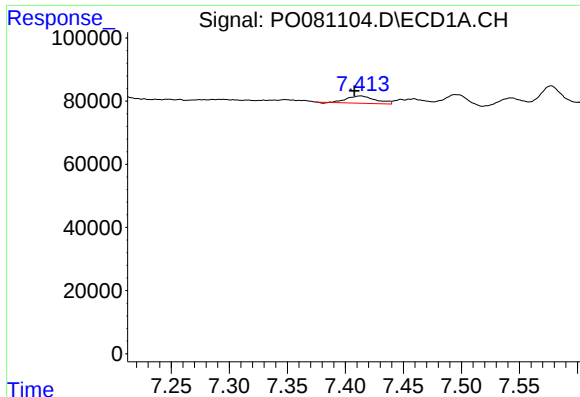

#27 AR-1254-2


R.T.: 7.413 min
Delta R.T.: 0.005 min
Response: 39397
Conc: 7.92 ng/ml

Instrument :
ECD_O
ClientSampleId :

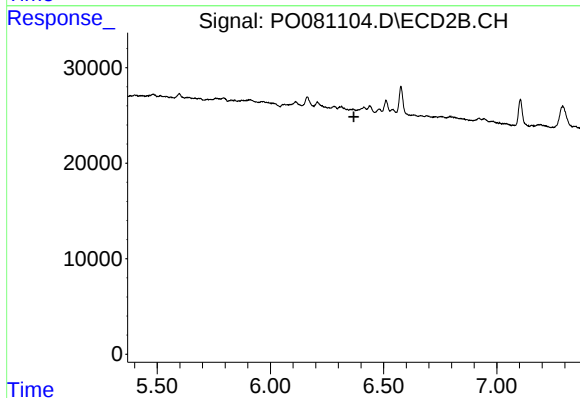


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.369 min
Response: 0
Conc: N.D.

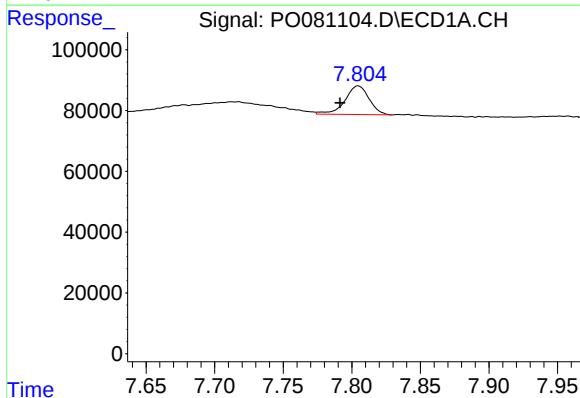


#28 AR-1254-3

R.T.: 7.805 min
Delta R.T.: 0.013 min
Response: 115701
Conc: 22.88 ng/ml

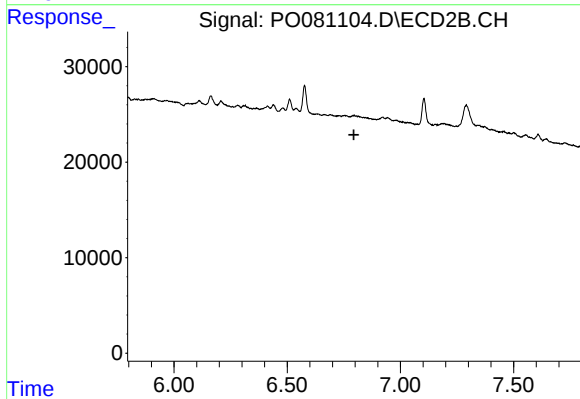

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.795 min
Response: 0
Conc: N.D.

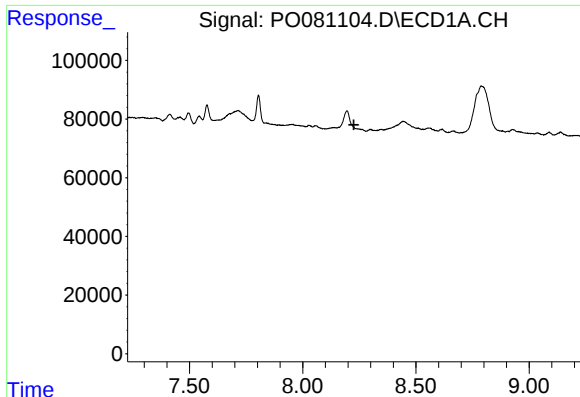

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.226 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

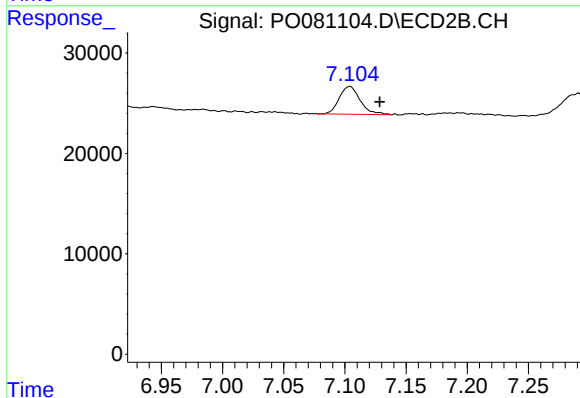


#32 AR-1260-2

R.T.: 7.104 min
Delta R.T.: -0.024 min
Response: 33228
Conc: 18.93 ng/ml

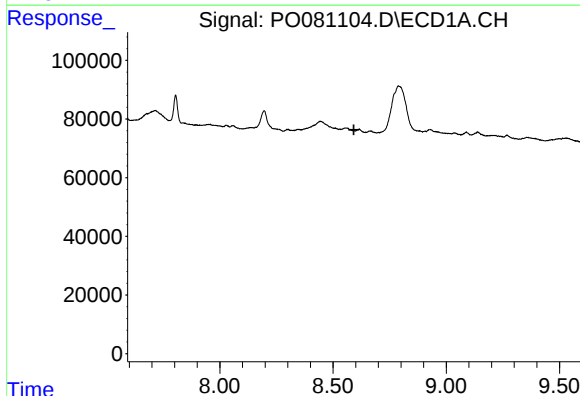

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 8.592 min
Response: 0
Conc: N.D.

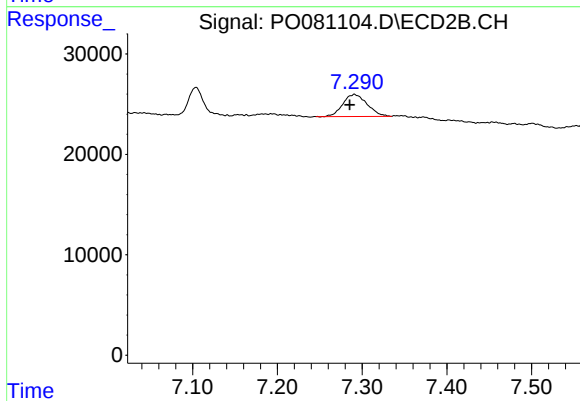

#33 AR-1260-3

R.T.: 7.291 min
Delta R.T.: 0.005 min
Response: 44050
Conc: 24.06 ng/ml