

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091021\
 Data File : P0081105.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Sep 2021 7:17
 Operator : DD\AJ
 Sample : M3688-01
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 01:24:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.927	4.053	1937183	611191	24.539	24.733
2)	SA Decachlor...	10.989	9.412	1146301	438158	19.306	18.769
Target Compounds							
8)	L2 AR-1221-1	5.180	0.000	74987	0	77.171	N.D. #
9)	L2 AR-1221-2	5.282	0.000	21050	0	28.635	N.D. #
20)	L4 AR-1242-5	7.240	0.000	114413	0	71.412	N.D. #
25)	L5 AR-1248-5	7.240	0.000	114413	0	41.603	N.D. #
28)	L6 AR-1254-3	7.804	0.000	46123	0	9.122	N.D. #
30)	L6 AR-1254-5	8.494f	0.000	21746	0	5.257	N.D. #
32)	L7 AR-1260-2	8.196f	7.102f	106210	13616	23.831	7.757 #
33)	L7 AR-1260-3	0.000	7.293	0	48114	N.D.	26.282 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091021\
Data File : PO081105.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2021 7:17
Operator : DD\AJ
Sample : M3688-01
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 01:24:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

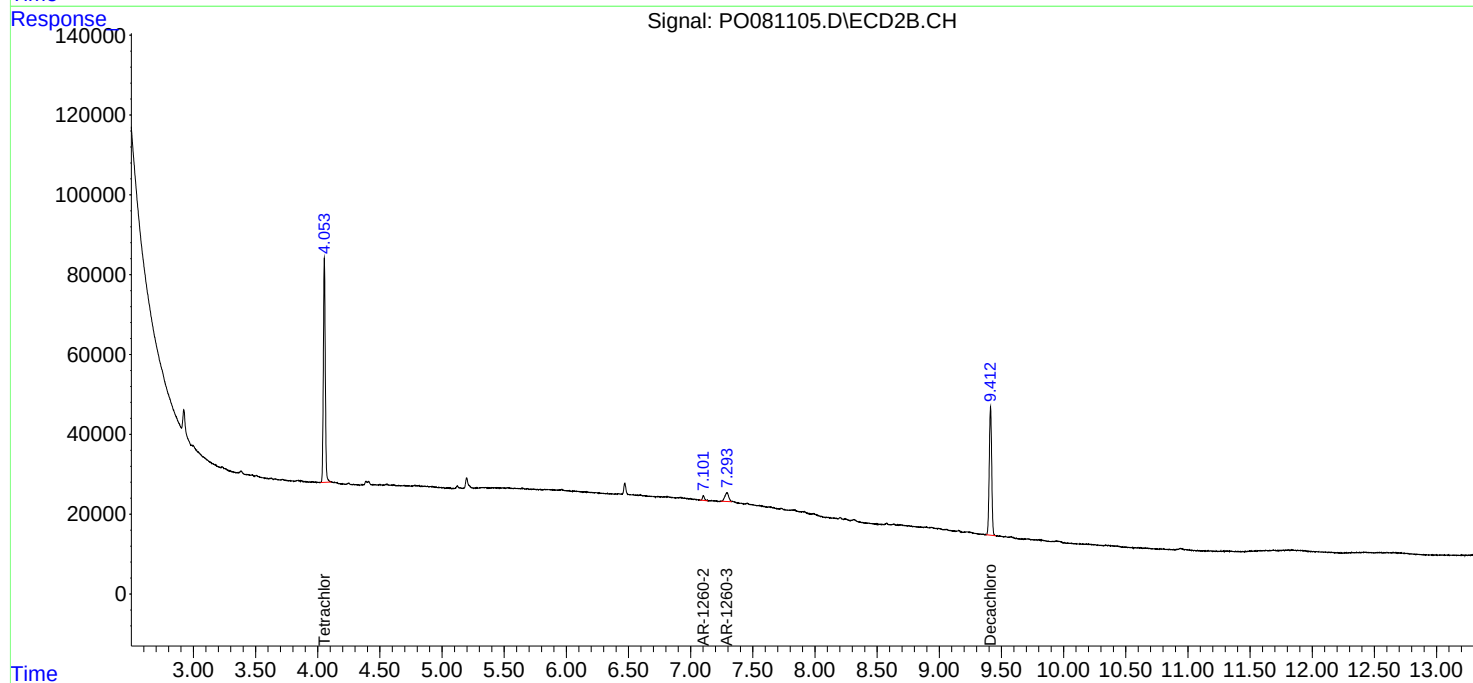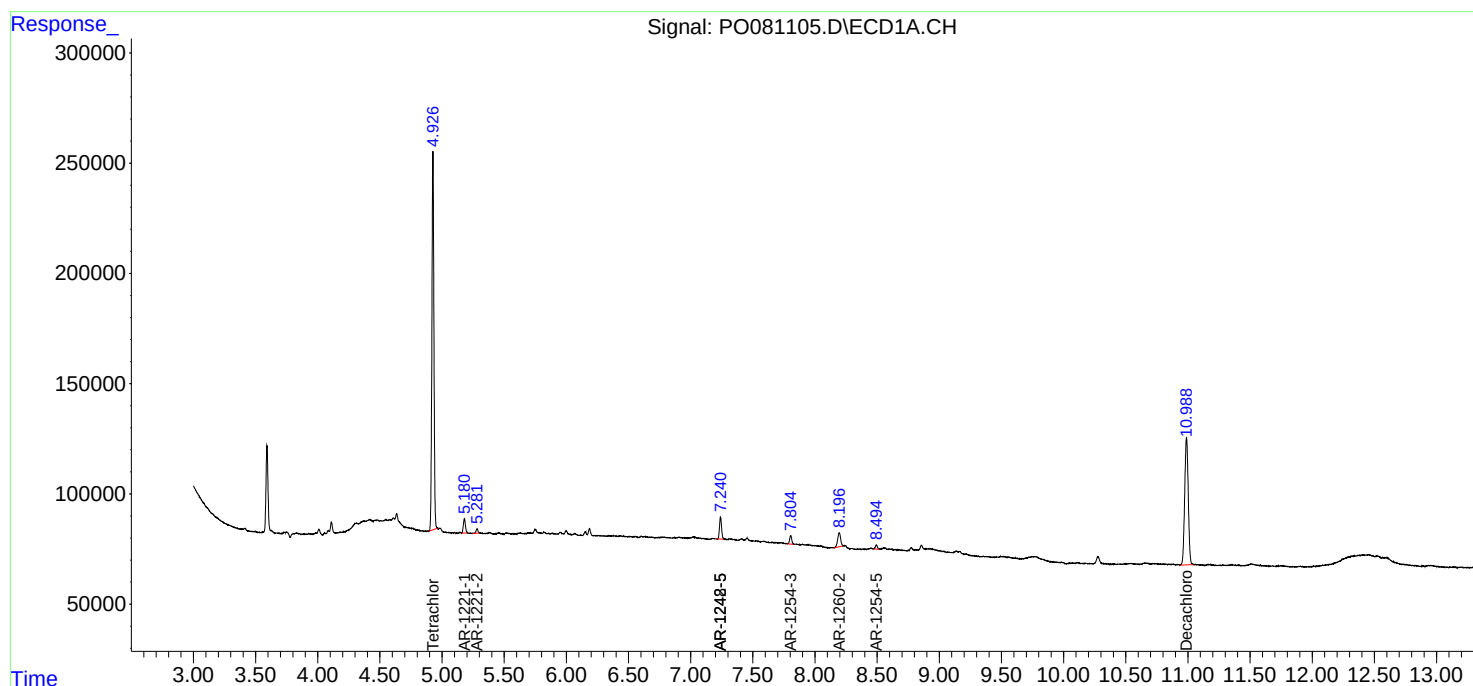


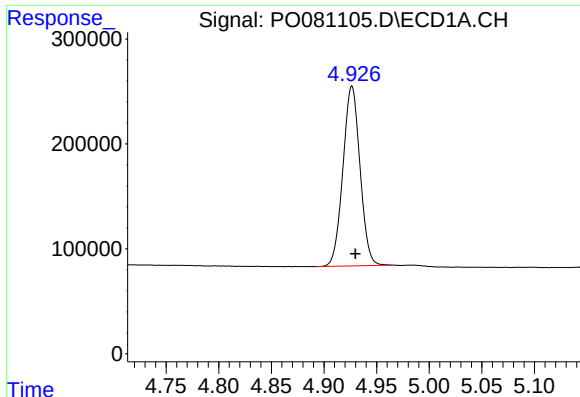

#1 Tetrachloro-m-xylene


R.T.: 4.927 min
Delta R.T.: -0.003 min
Response: 1937183
Conc: 24.54 ng/ml

Instrument :
ECD_O
ClientSampleId :

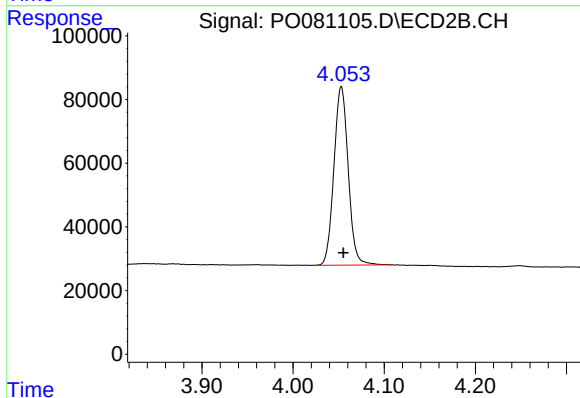


#1 Tetrachloro-m-xylene

R.T.: 4.053 min
Delta R.T.: -0.002 min
Response: 611191
Conc: 24.73 ng/ml

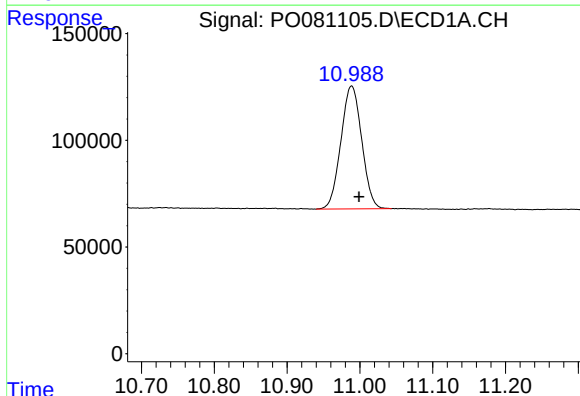


#2 Decachlorobiphenyl

R.T.: 10.989 min
Delta R.T.: -0.010 min
Response: 1146301
Conc: 19.31 ng/ml

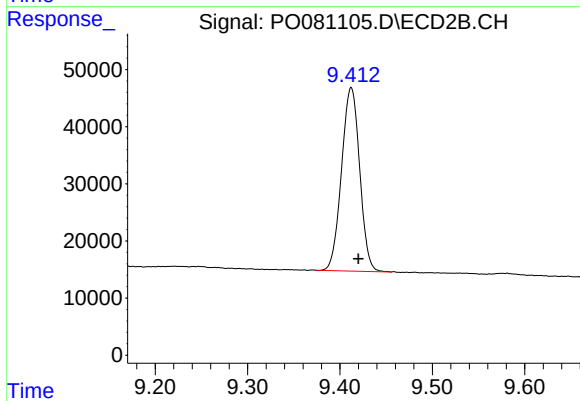

#2 Decachlorobiphenyl


R.T.: 9.412 min
Delta R.T.: -0.008 min
Response: 438158
Conc: 18.77 ng/ml

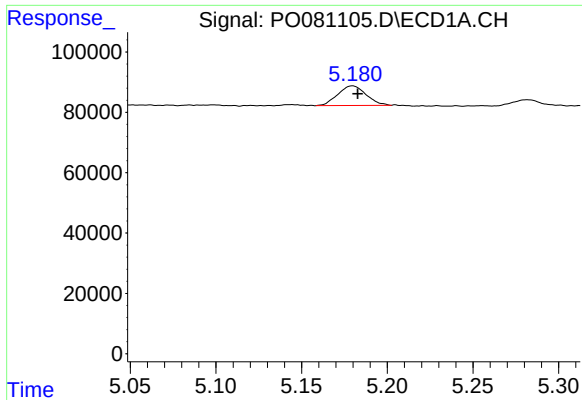

#8 AR-1221-1


R.T.: 5.180 min
Delta R.T.: -0.003 min
Response: 74987
Conc: 77.17 ng/ml

Instrument :
ECD_O
ClientSampleId :

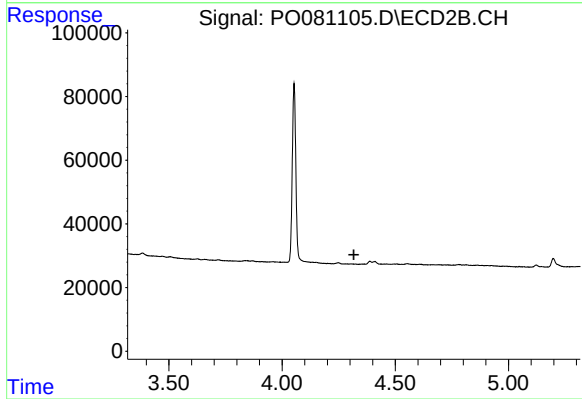


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

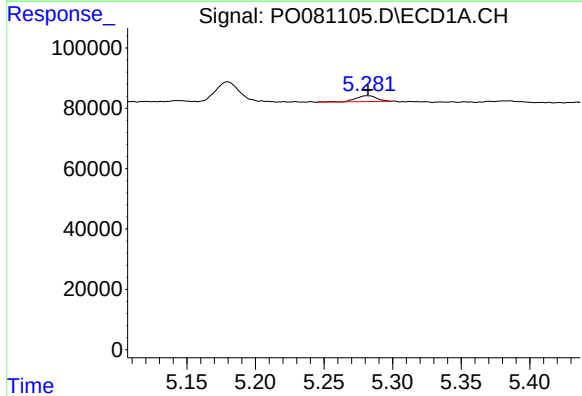


#9 AR-1221-2

R.T.: 5.282 min
Delta R.T.: 0.000 min
Response: 21050
Conc: 28.64 ng/ml

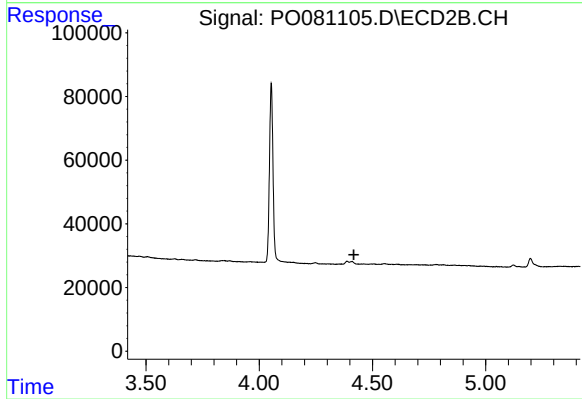

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.418 min
Response: 0
Conc: N.D.

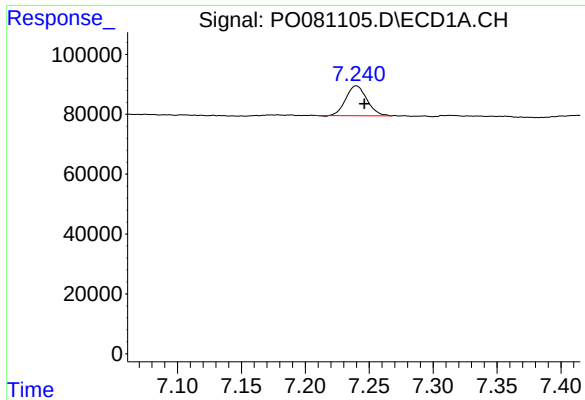

#20 AR-1242-5


R.T.: 7.240 min
Delta R.T.: -0.006 min
Response: 114413
Conc: 71.41 ng/ml

Instrument :
ECD_O
ClientSampleId :

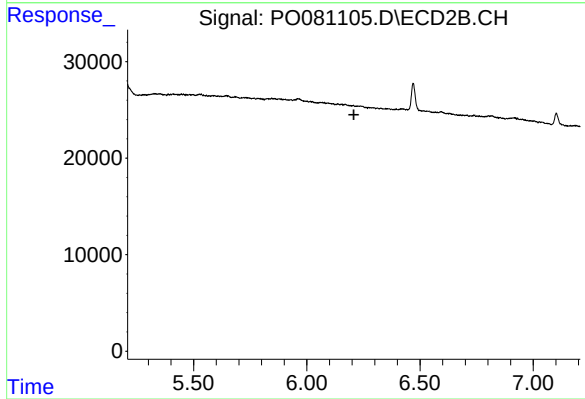


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.208 min
Response: 0
Conc: N.D.

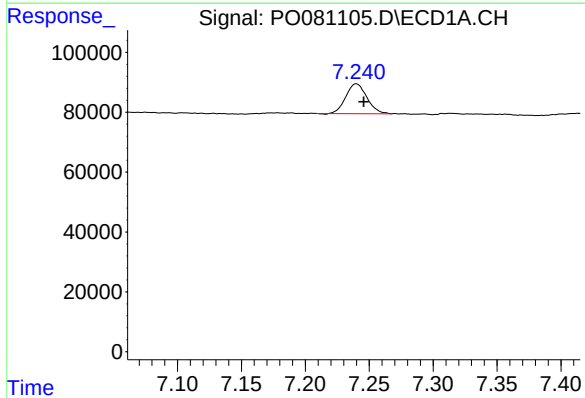


#25 AR-1248-5

R.T.: 7.240 min
Delta R.T.: -0.006 min
Response: 114413
Conc: 41.60 ng/ml

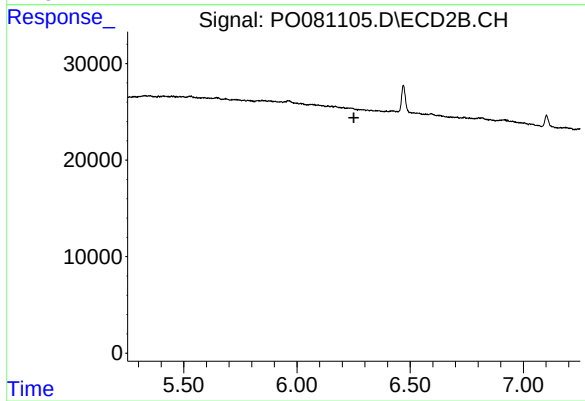

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.251 min
Response: 0
Conc: N.D.

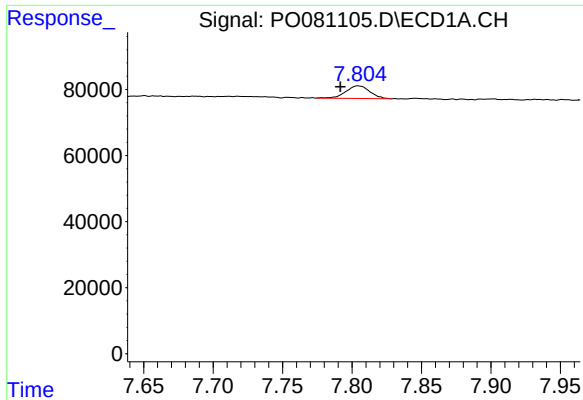

#28 AR-1254-3


R.T.: 7.804 min
Delta R.T.: 0.013 min
Response: 46123
Conc: 9.12 ng/ml

Instrument :
ECD_O
ClientSampleId :

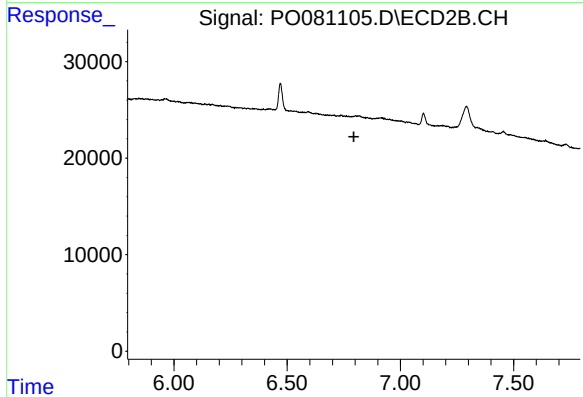


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.795 min
Response: 0
Conc: N.D.

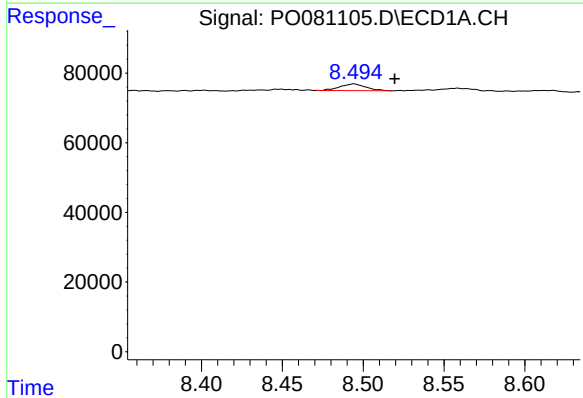


#30 AR-1254-5

R.T.: 8.494 min
Delta R.T.: -0.025 min
Response: 21746
Conc: 5.26 ng/ml

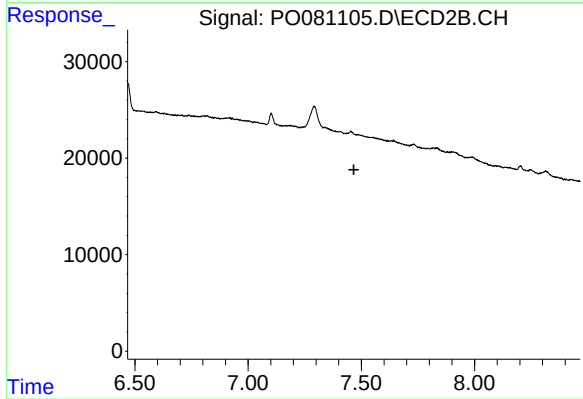

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.467 min
Response: 0
Conc: N.D.

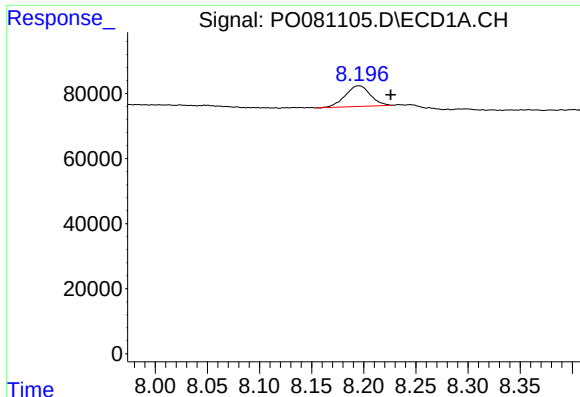

#32 AR-1260-2


R.T.: 8.196 min
Delta R.T.: -0.030 min
Response: 106210
Conc: 23.83 ng/ml

Instrument :
ECD_O
ClientSampleId :

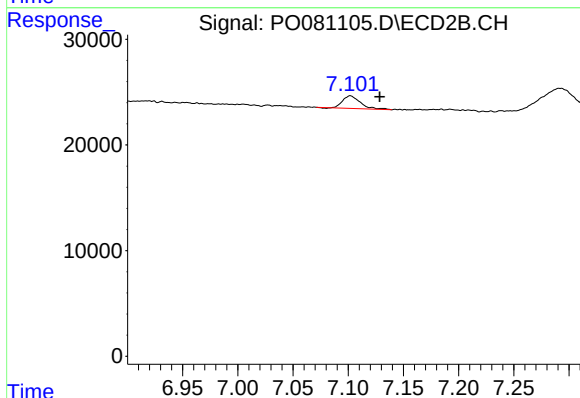


#32 AR-1260-2

R.T.: 7.102 min
Delta R.T.: -0.027 min
Response: 13616
Conc: 7.76 ng/ml

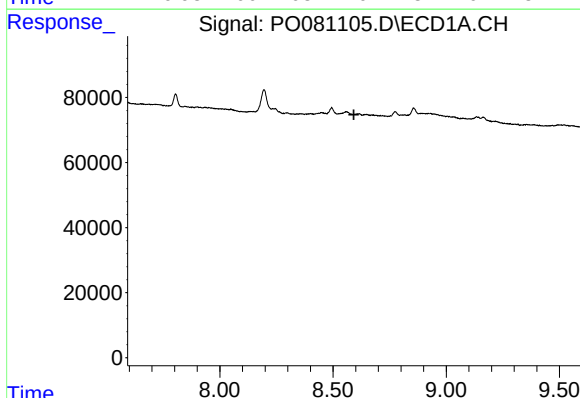

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.592 min
Response: 0
Conc: N.D.

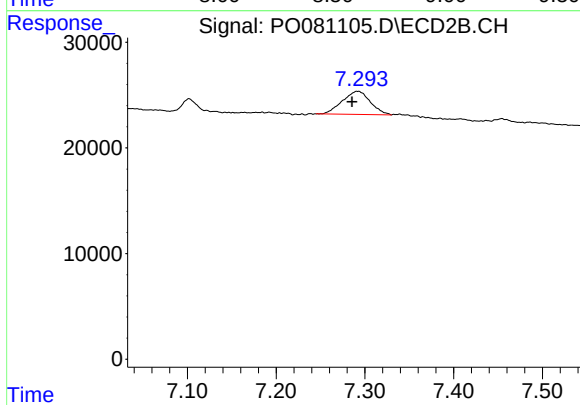

#33 AR-1260-3

R.T.: 7.293 min
Delta R.T.: 0.008 min
Response: 48114
Conc: 26.28 ng/ml