

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091021\
 Data File : P0081106.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Sep 2021 7:35
 Operator : DD\AJ
 Sample : M3689-02
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 01:24:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.926	4.053	790726	256551	10.017	10.382
2)	SA Decachlor...	10.989	9.411	345138	118649	5.813	5.083
Target Compounds							
8)	L2 AR-1221-1	5.180	0.000	814253	0	837.965	N.D. #
9)	L2 AR-1221-2	0.000	4.388f	0	103328	N.D.	419.157 #
20)	L4 AR-1242-5	7.239	0.000	365738	0	228.278	N.D. #
25)	L5 AR-1248-5	7.239	0.000	365738	0	132.990	N.D. #
26)	L6 AR-1254-1	7.176	0.000	6261	0	1.937	N.D. #
28)	L6 AR-1254-3	7.802	0.000	53126	0	10.507	N.D. #
32)	L7 AR-1260-2	0.000	7.102f	0	14378	N.D.	8.191 #
33)	L7 AR-1260-3	0.000	7.294	0	41709	N.D.	22.783 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091021\
Data File : P0081106.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2021 7:35
Operator : DD\AJ
Sample : M3689-02
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 01:24:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

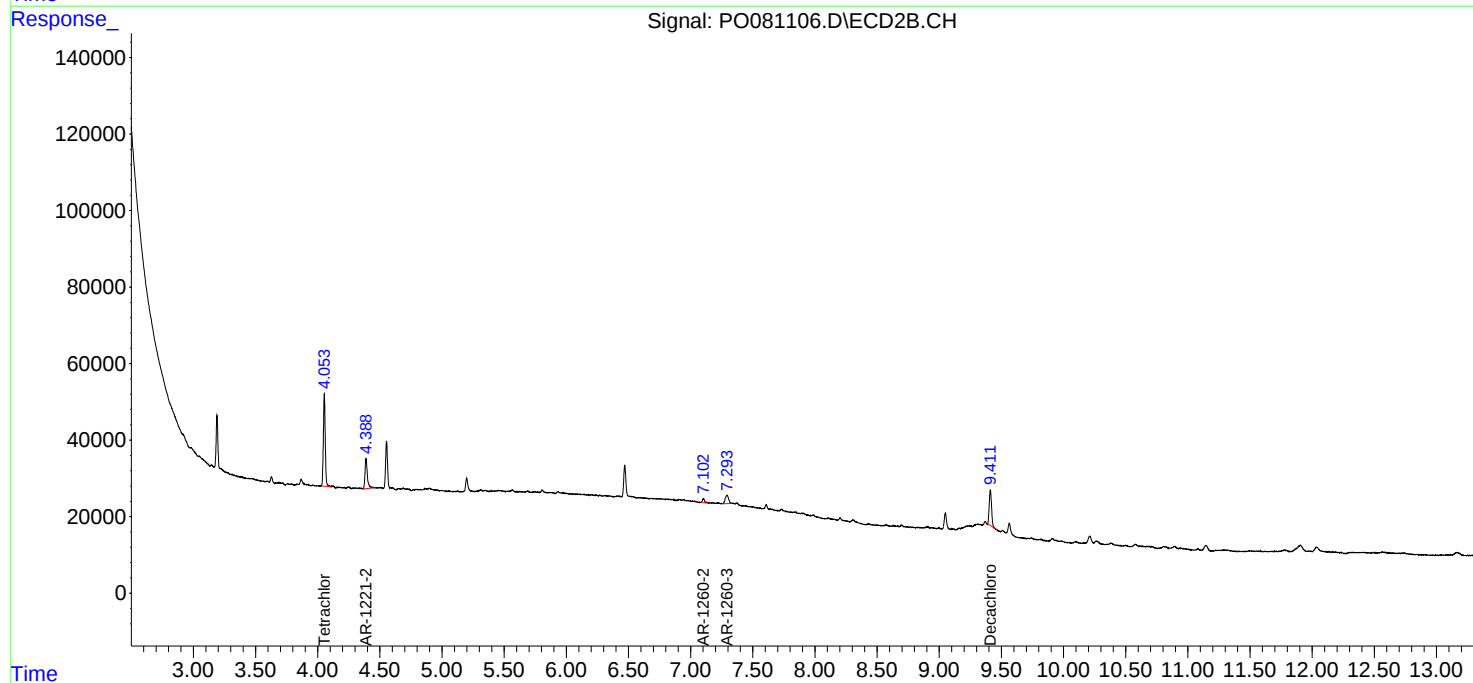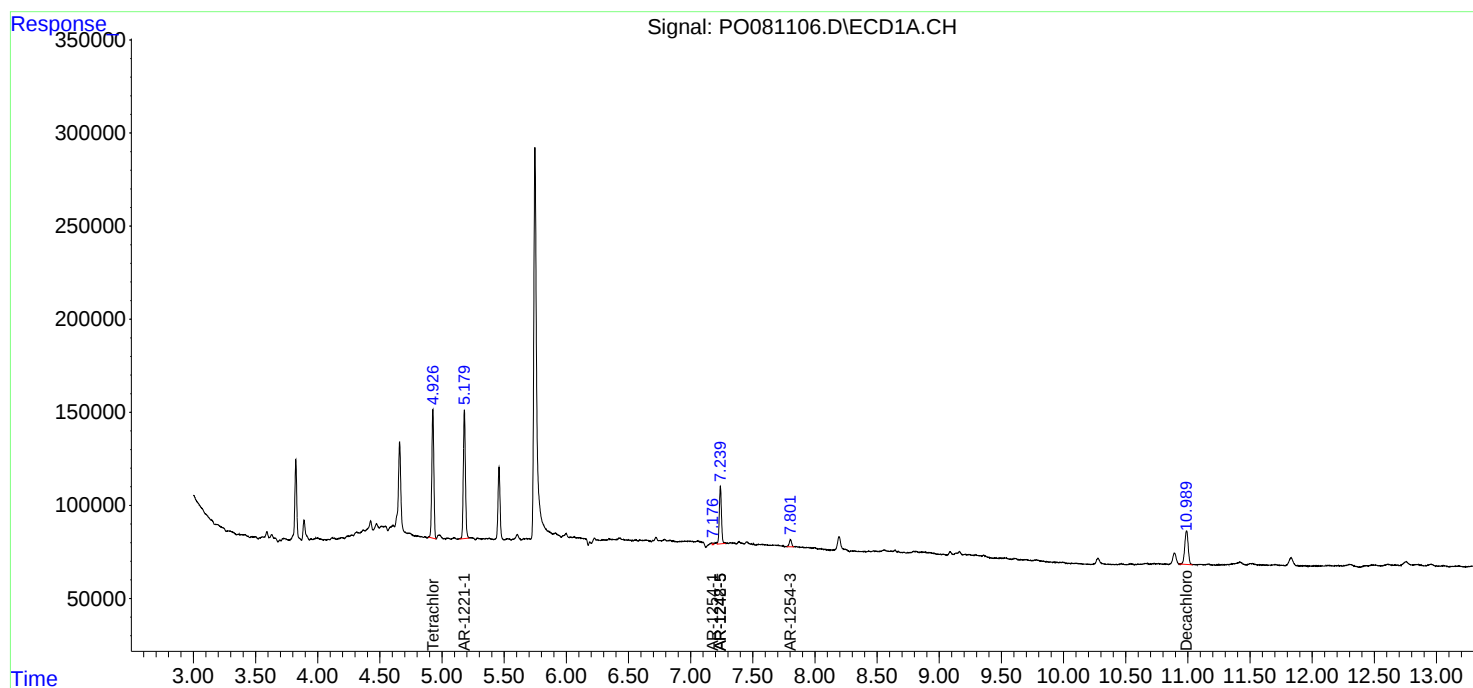


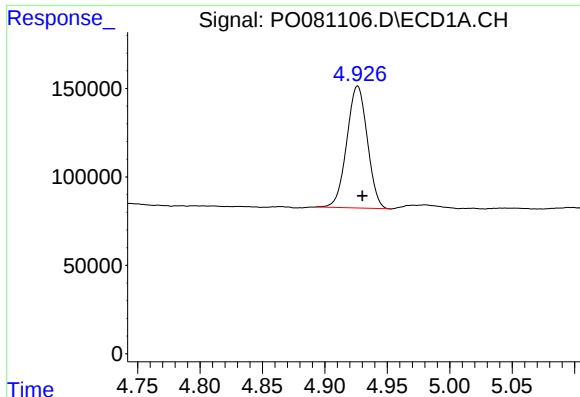

#1 Tetrachloro-m-xylene


R.T.: 4.926 min
Delta R.T.: -0.004 min
Response: 790726
Conc: 10.02 ng/ml

Instrument :
ECD_O
ClientSampleId :

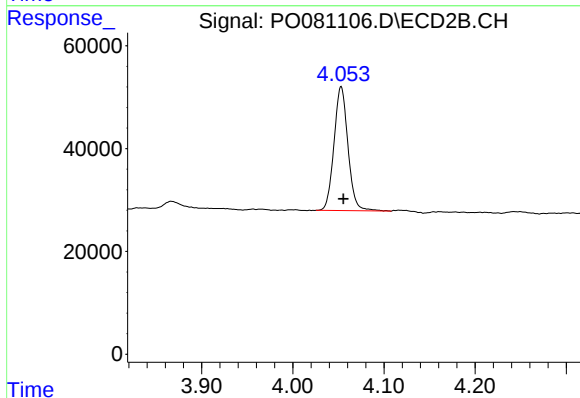


#1 Tetrachloro-m-xylene

R.T.: 4.053 min
Delta R.T.: -0.002 min
Response: 256551
Conc: 10.38 ng/ml

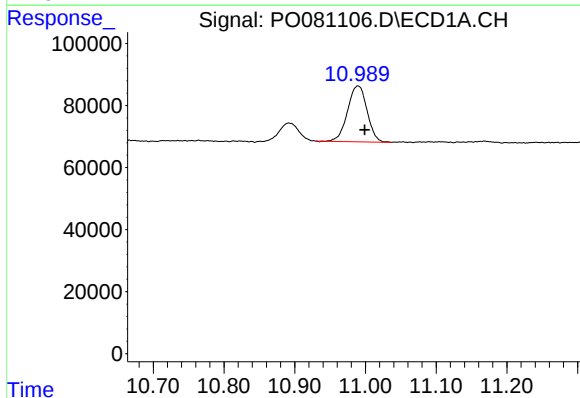


#2 Decachlorobiphenyl

R.T.: 10.989 min
Delta R.T.: -0.010 min
Response: 345138
Conc: 5.81 ng/ml

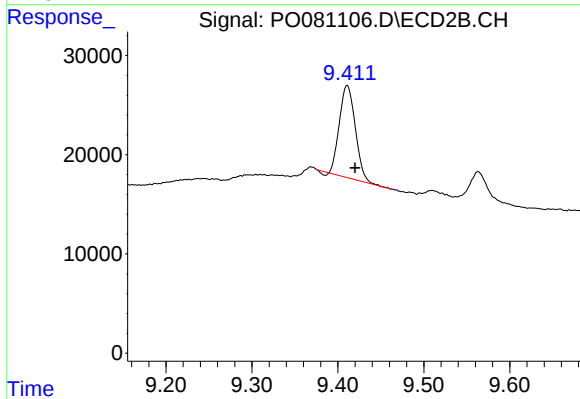

#2 Decachlorobiphenyl


R.T.: 9.411 min
Delta R.T.: -0.009 min
Response: 118649
Conc: 5.08 ng/ml

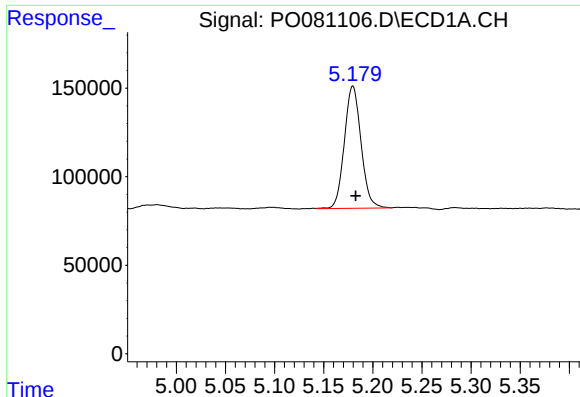

#8 AR-1221-1


R.T.: 5.180 min
Delta R.T.: -0.003 min
Response: 814253
Conc: 837.96 ng/ml

Instrument :
ECD_O
ClientSampleId :

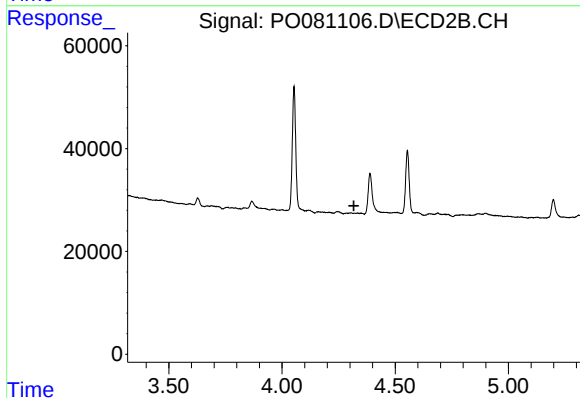


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

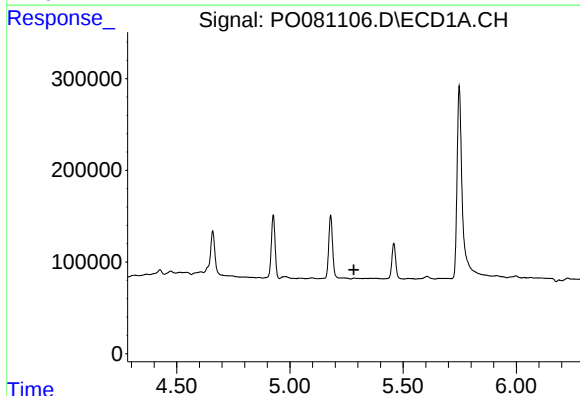


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.282 min
Response: 0
Conc: N.D.

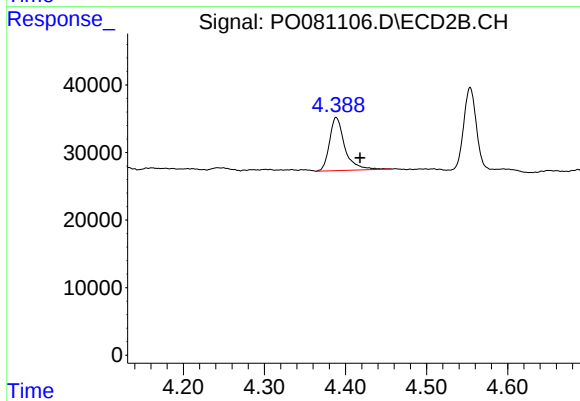

#9 AR-1221-2


R.T.: 4.388 min
Delta R.T.: -0.029 min
Response: 103328
Conc: 419.16 ng/ml

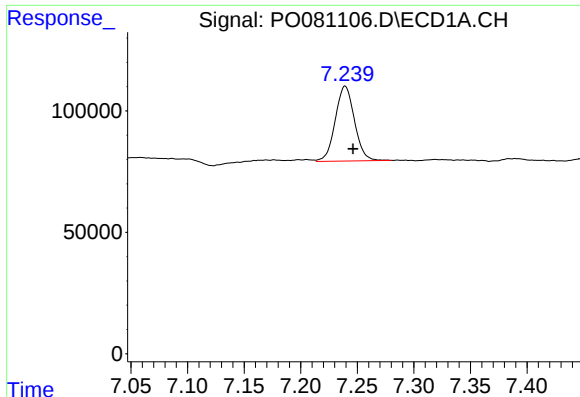

#20 AR-1242-5


R.T.: 7.239 min
Delta R.T.: -0.007 min
Response: 365738
Conc: 228.28 ng/ml

Instrument :
ECD_O
ClientSampleId :

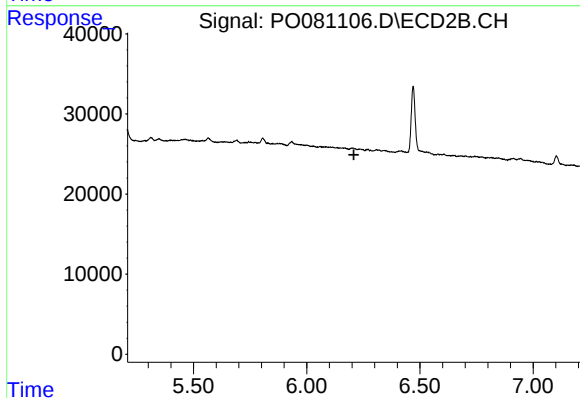


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.208 min
Response: 0
Conc: N.D.

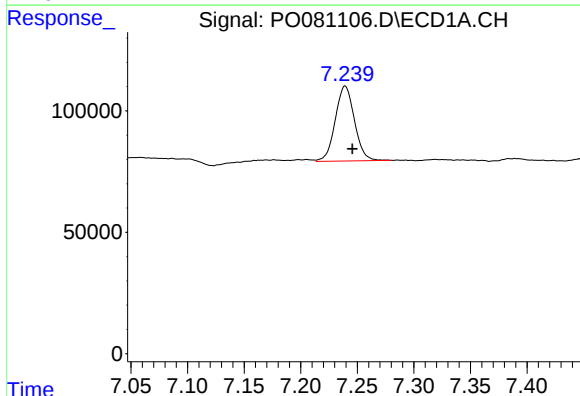


#25 AR-1248-5

R.T.: 7.239 min
Delta R.T.: -0.006 min
Response: 365738
Conc: 132.99 ng/ml

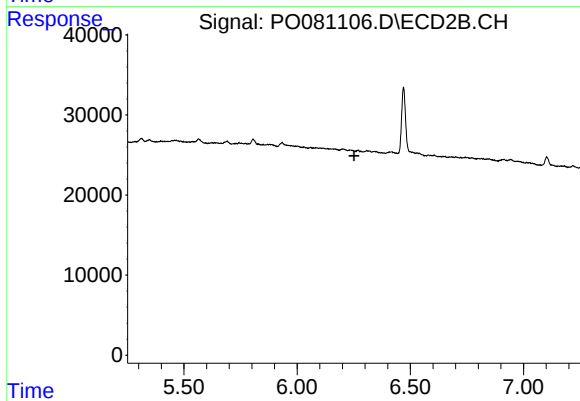

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.251 min
Response: 0
Conc: N.D.

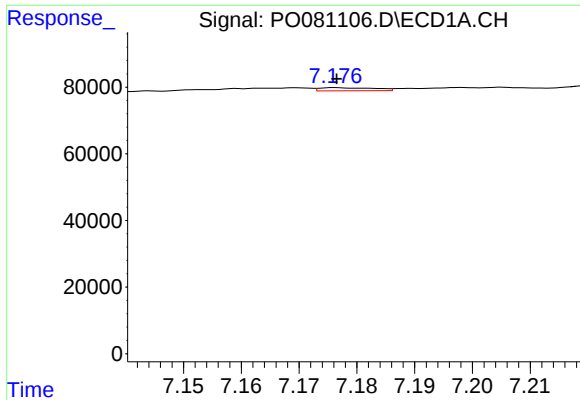

#26 AR-1254-1


R.T.: 7.176 min
Delta R.T.: 0.000 min
Response: 6261
Conc: 1.94 ng/ml

Instrument :
ECD_O
ClientSampleId :

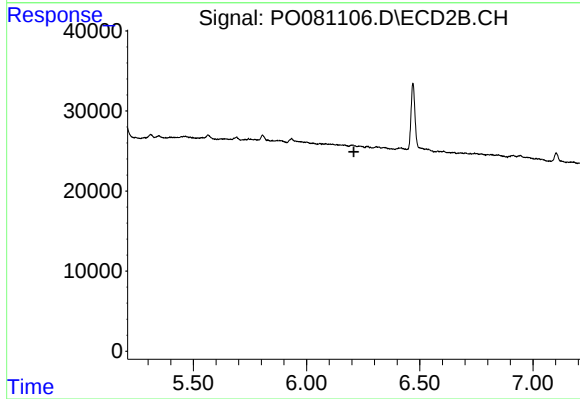


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.209 min
Response: 0
Conc: N.D.

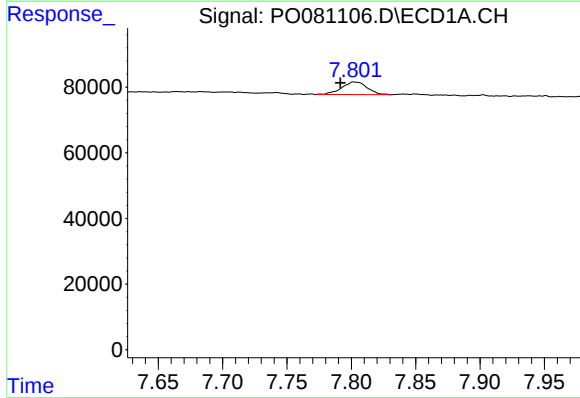


#28 AR-1254-3

R.T.: 7.802 min
Delta R.T.: 0.010 min
Response: 53126
Conc: 10.51 ng/ml

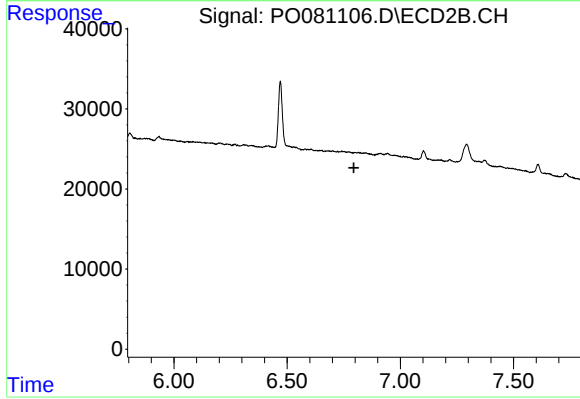

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.795 min
Response: 0
Conc: N.D.

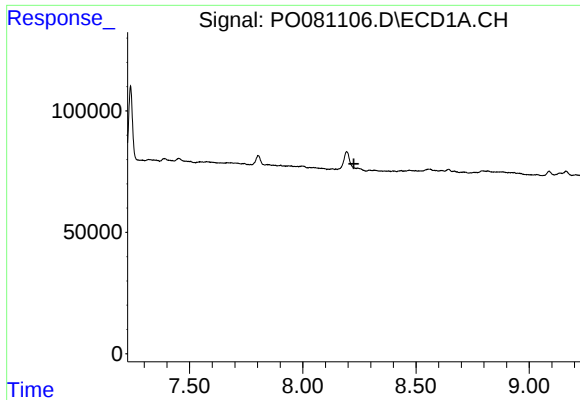

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 8.226 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

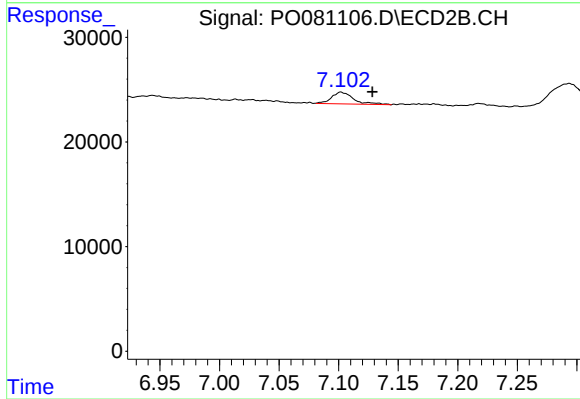


#32 AR-1260-2

R.T.: 7.102 min
Delta R.T.: -0.027 min
Response: 14378
Conc: 8.19 ng/ml

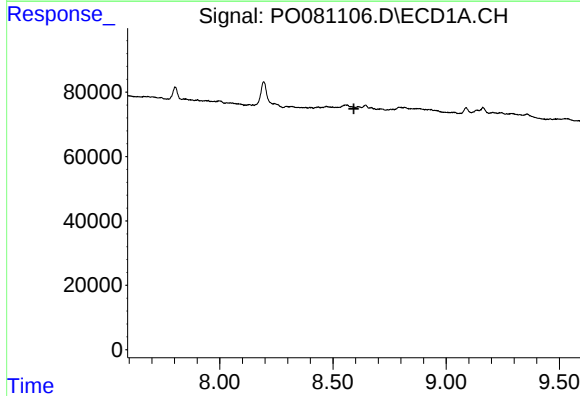

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.592 min
Response: 0
Conc: N.D.

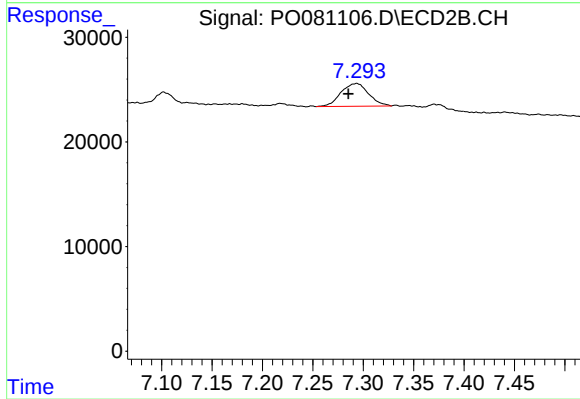

#33 AR-1260-3

R.T.: 7.294 min
Delta R.T.: 0.008 min
Response: 41709
Conc: 22.78 ng/ml