

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091021\
 Data File : P0081100.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Sep 2021 5:51
 Operator : DD\AJ
 Sample : M3689-03
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 257

Manual Integrations
 APPROVED

mohammad
 9/13/2021 4:38:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 01:21:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 07:15:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.927	4.053	920044	408502	11.655	16.530 #
2) SA Decachlor...	10.992	9.412	549338	207104	9.252m	8.872

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091021\
Data File : PO081100.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2021 5:51
Operator : DD\AJ
Sample : M3689-03
Misc :
ALS Vial : 53 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
257


Manual Integrations
APPROVED

mohammad
9/13/2021 4:38:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 01:21:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 07:15:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

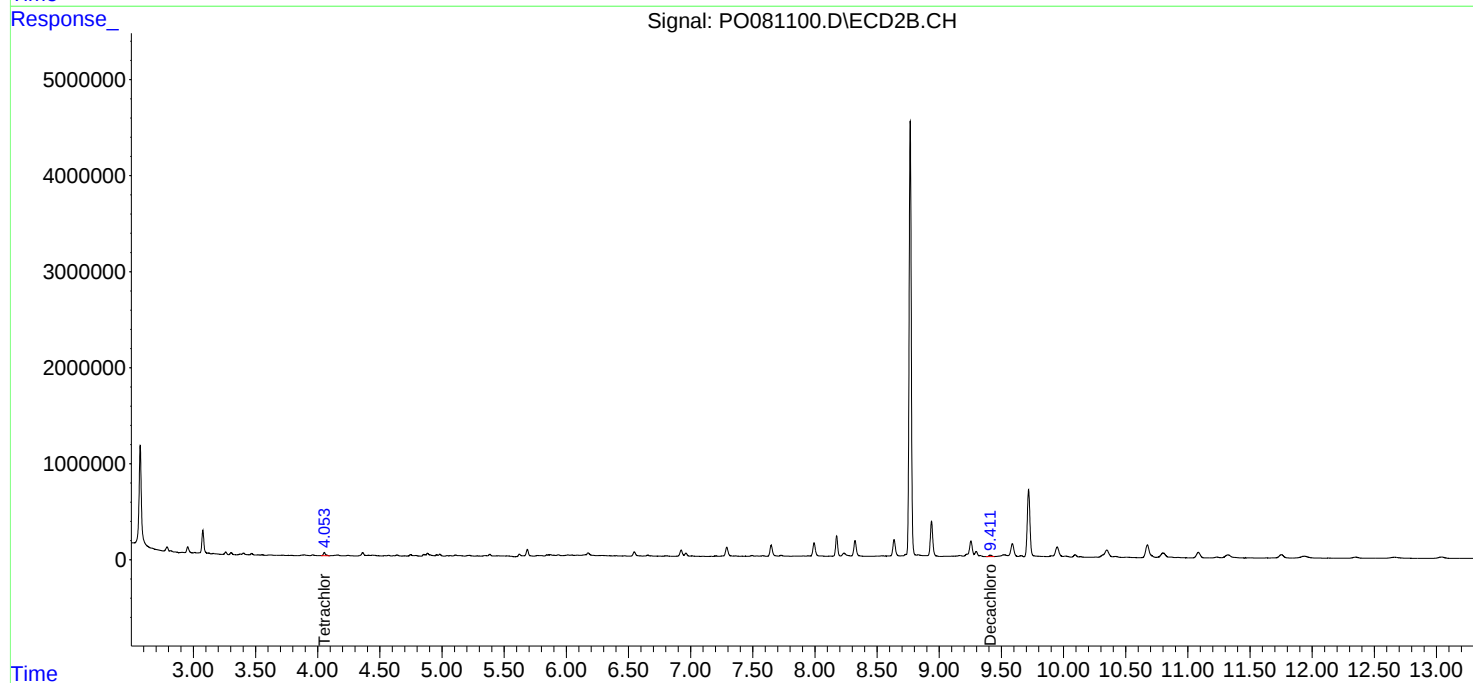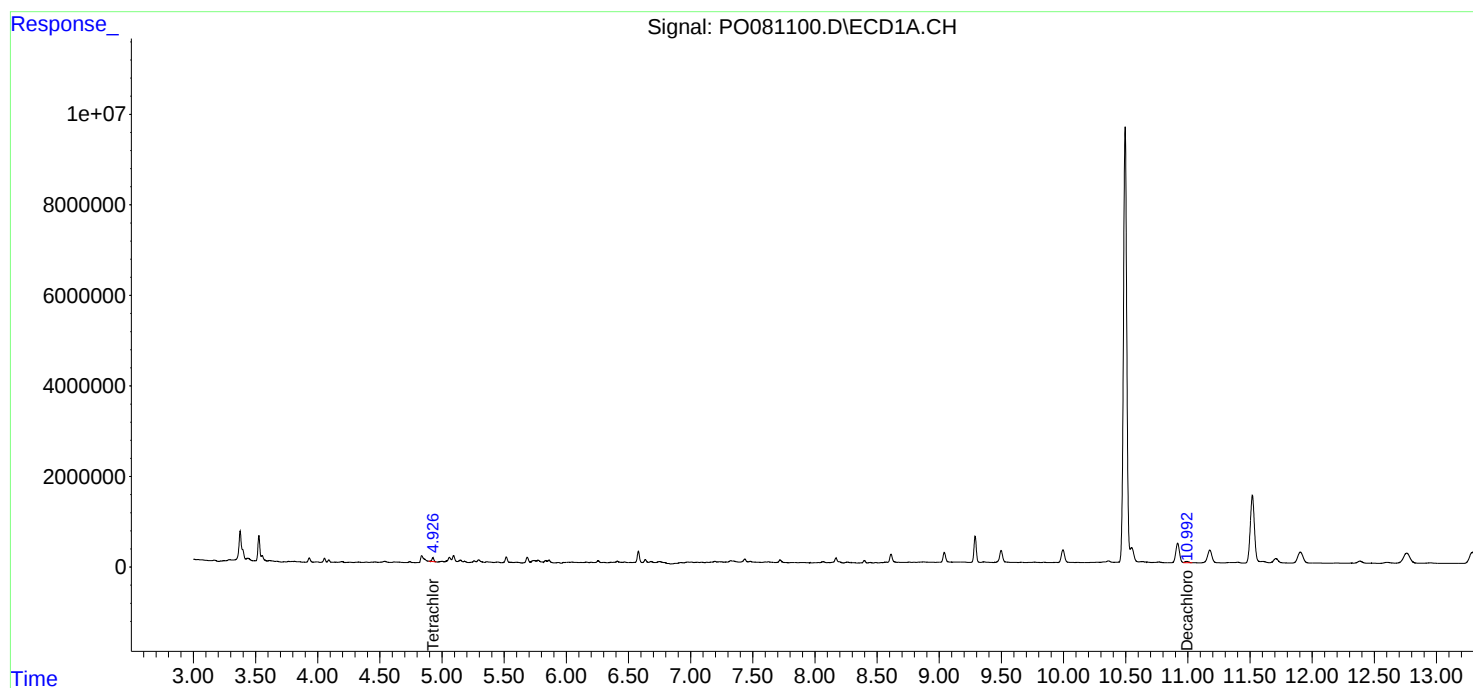

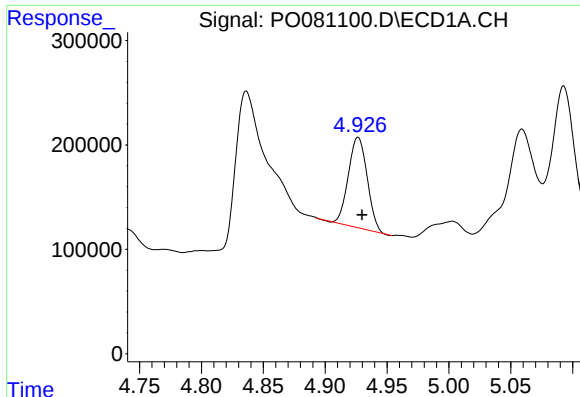


#1 Tetrachloro-m-xylene

R.T.: 4.927 min
Delta R.T.: -0.003 min
Response: 920044
Conc: 11.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
257


Manual Integrations
APPROVED

mohammad
9/13/2021 4:38:58 PM

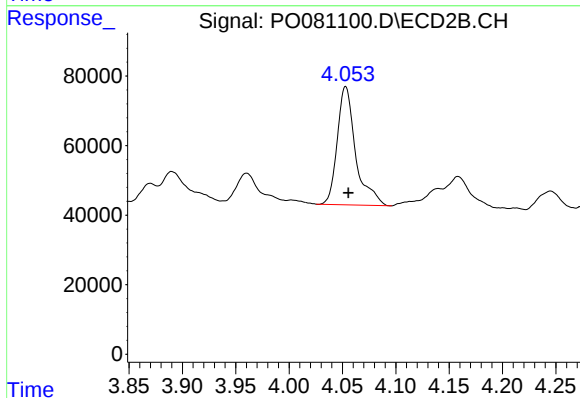


#1 Tetrachloro-m-xylene

R.T.: 4.053 min
Delta R.T.: -0.002 min
Response: 408502
Conc: 16.53 ng/ml

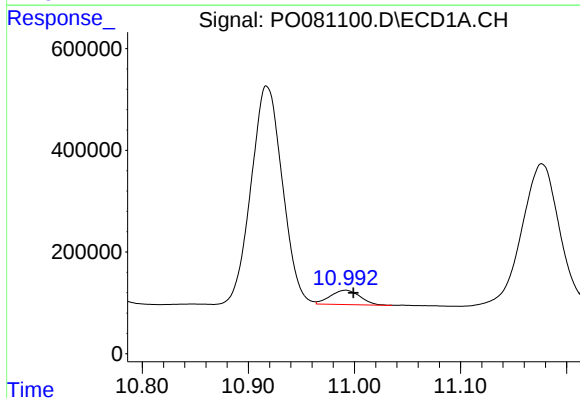

#2 Decachlorobiphenyl

R.T.: 10.992 min
Delta R.T.: -0.007 min
Response: 549338
Conc: 9.25 ng/ml m

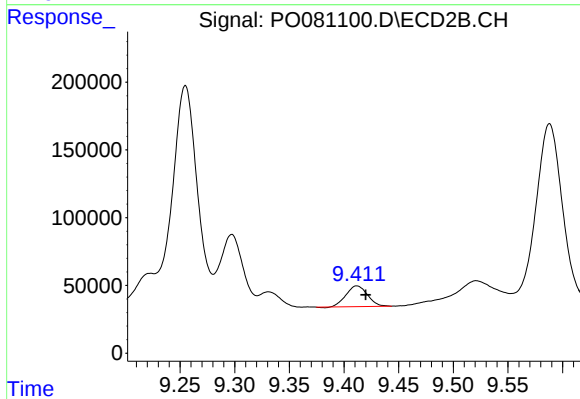

#2 Decachlorobiphenyl

R.T.: 9.412 min
Delta R.T.: -0.008 min
Response: 207104
Conc: 8.87 ng/ml